

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN061825\
 Data File : VN087097.D
 Acq On : 18 Jun 2025 19:21
 Operator : JC\MD
 Sample : VIBLK
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VIBLK

Quant Time: Jun 19 01:34:24 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N060625W.M
 Quant Title : SW846 8260
 QLast Update : Sat Jun 07 02:12:50 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.229	168	151838	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.106	114	305775	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.865	117	276771	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.788	152	126979	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.582	65	112887	55.529	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	111.060%
35) Dibromofluoromethane	8.177	113	94815	52.323	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	104.640%
50) Toluene-d8	10.565	98	376582	52.496	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	105.000%
62) 4-Bromofluorobenzene	12.847	95	130417	48.933	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	=	97.860%
Target Compounds						
					Qvalue	
5) Bromomethane	3.018	94	283	0.251	ug/l	99
15) Acrylonitrile	5.753	53	422	0.327	ug/l #	43
16) Acetone	4.465	43	426	0.395	ug/l #	40
17) Carbon Disulfide	4.736	76	2303	0.493	ug/l #	75
20) Methylene Chloride	5.294	84	1561	0.773	ug/l #	87
21) trans-1,2-Dichloroethene	5.818	96	405	0.215	ug/l #	60
31) Cyclohexane	8.229	56	2801	0.850	ug/l #	1
36) 1,1-Dichloropropene	8.235	75	11376	4.213	ug/l #	48
38) Carbon Tetrachloride	8.229	117	14690	5.541	ug/l #	16
68) m/p-Xylenes	12.070	106	935	0.232	ug/l	84
71) Bromoform	12.847	173	800	0.550	ug/l #	1
73) Isopropylbenzene	12.694	105	1865	0.202	ug/l	78
76) 1,2,3-Trichloropropane	12.847	75	59554	19.731	ug/l #	1
78) n-propylbenzene	13.035	91	2665	0.237	ug/l	89
80) 1,3,5-Trimethylbenzene	13.170	105	1550	0.203	ug/l	94
81) trans-1,4-Dichloro-2-b...	12.847	75	59554	45.419	ug/l #	16
82) 4-Chlorotoluene	13.223	91	1460	0.214	ug/l	86
83) tert-Butylbenzene	13.435	119	1667	0.238	ug/l	97
84) 1,2,4-Trimethylbenzene	13.482	105	1590	0.208	ug/l	92
85) sec-Butylbenzene	13.617	105	2864	0.282	ug/l	99
86) p-Isopropyltoluene	13.729	119	2092	0.249	ug/l	91
87) 1,3-Dichlorobenzene	13.735	146	933	0.224	ug/l	92
88) 1,4-Dichlorobenzene	13.735	146	933	0.219	ug/l	91
89) n-Butylbenzene	14.059	91	2583	0.318	ug/l	88
90) Hexachloroethane	14.335	117	411	0.289	ug/l #	37
91) 1,2-Dichlorobenzene	14.106	146	849	0.212	ug/l	72
93) 1,2,4-Trichlorobenzene	15.394	180	1204	0.470	ug/l	96
94) Hexachlorobutadiene	15.500	225	1075	1.127	ug/l	94
95) Naphthalene	15.641	128	3674	0.385	ug/l #	87
96) 1,2,3-Trichlorobenzene	15.835	180	1346	0.529	ug/l	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN061825\
 Data File : VN087097.D
 Acq On : 18 Jun 2025 19:21
 Operator : JC\MD
 Sample : VIBLK
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VIBLK

Quant Time: Jun 19 01:34:24 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N060625W.M
 Quant Title : SW846 8260
 QLast Update : Sat Jun 07 02:12:50 2025
 Response via : Initial Calibration




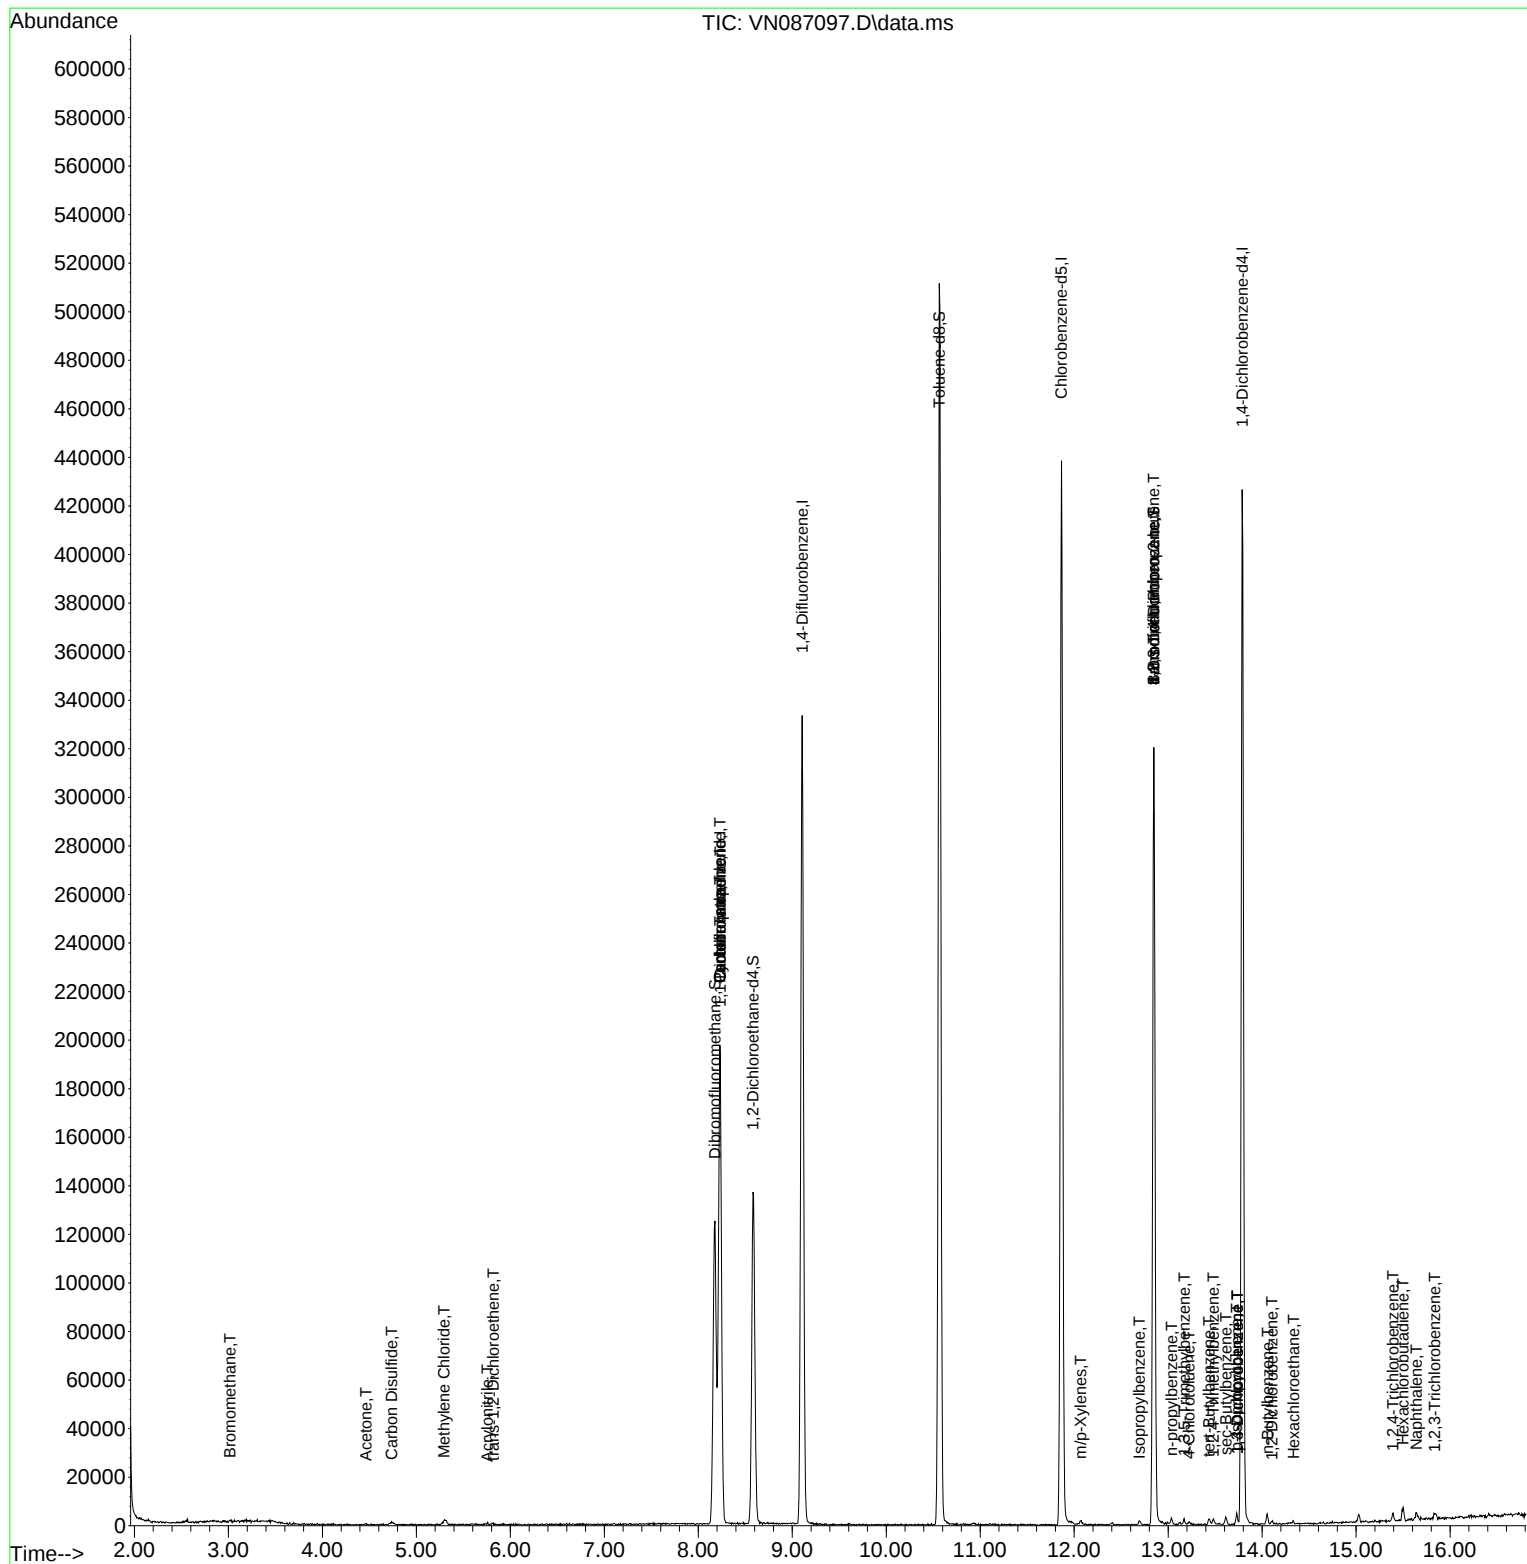


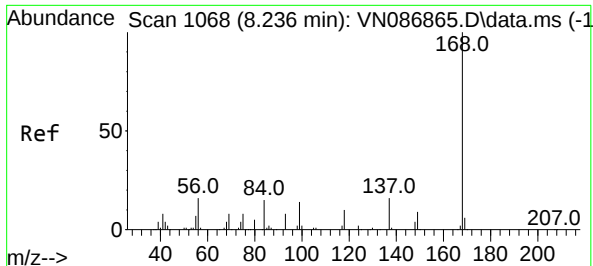

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.229 min Scan# 11
Delta R.T. -0.007 min
Lab File: VN087097.D
Acq: 18 Jun 2025 19:21




Instrument :
MSVOA_N
ClientSampleId :
VIBLK


Tgt Ion:168 Resp: 151838
Ion Ratio Lower Upper
168 100
99 56.8 49.1 73.7

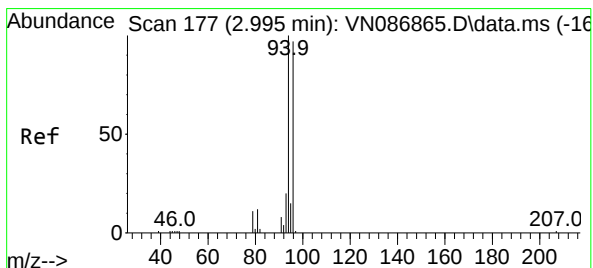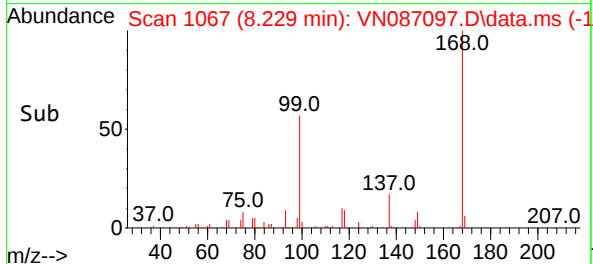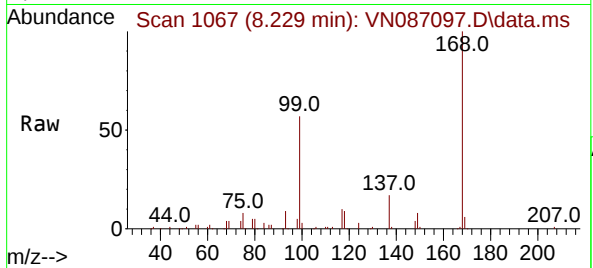

#5
Bromomethane
Concen: 0.251 ug/l
RT: 3.018 min Scan# 181
Delta R.T. 0.023 min
Lab File: VN087097.D
Acq: 18 Jun 2025 19:21

Tgt Ion: 94 Resp: 283
Ion Ratio Lower Upper
94 100
96 98.8 77.9 116.9


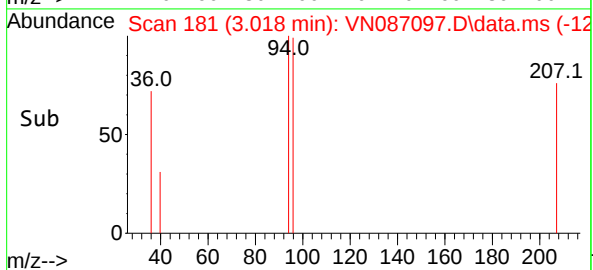

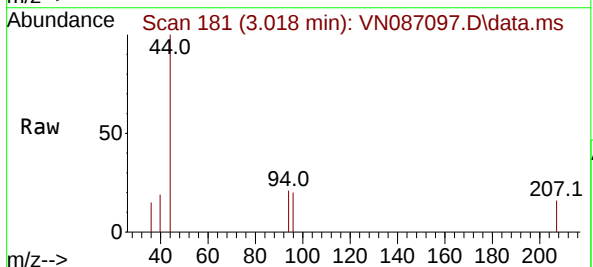




#15
Acrylonitrile
Concen: 0.327 ug/l
RT: 5.753 min Scan# 644
Delta R.T. 0.012 min
Lab File: VN087097.D
Acq: 18 Jun 2025 19:21




Instrument :
MSVOA_N
ClientSampleId :
VIBLK


Tgt Ion: 53 Resp: 422
Ion Ratio Lower Upper
53 100
52 32.0 65.0 97.6#
51 0.0 27.2 40.8#

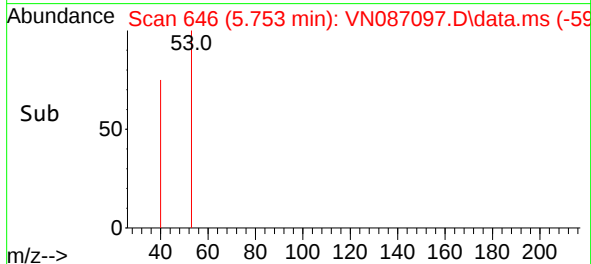

#16
Acetone
Concen: 0.395 ug/l
RT: 4.465 min Scan# 427
Delta R.T. 0.017 min
Lab File: VN087097.D
Acq: 18 Jun 2025 19:21

Tgt Ion: 43 Resp: 426
Ion Ratio Lower Upper
43 100
58 0.0 28.0 42.0#




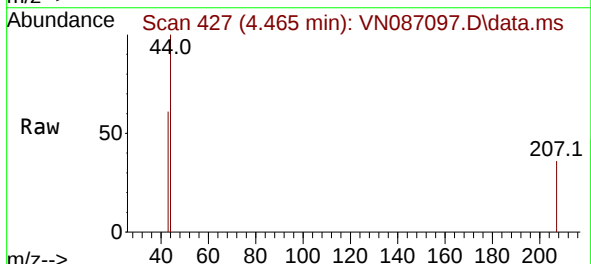




#17
Carbon Disulfide
Concen: 0.493 ug/l
RT: 4.736 min Scan# 472
Delta R.T. 0.006 min
Lab File: VN087097.D
Acq: 18 Jun 2025 19:21




Instrument :
MSVOA_N
ClientSampleId :
VIBLK


Tgt Ion: 76 Resp: 2303
Ion Ratio Lower Upper
76 100
78 0.0 7.3 10.9#

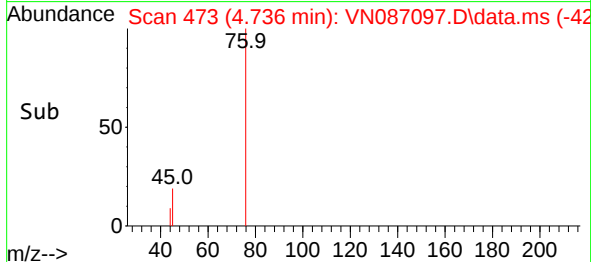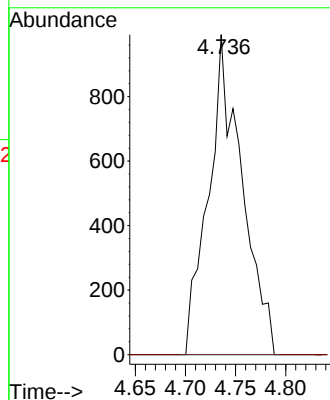

#20
Methylene Chloride
Concen: 0.773 ug/l
RT: 5.294 min Scan# 568
Delta R.T. -0.000 min
Lab File: VN087097.D
Acq: 18 Jun 2025 19:21

Tgt Ion: 84 Resp: 1561
Ion Ratio Lower Upper
84 100
49 136.8 90.5 135.7#
51 35.8 28.5 42.7
86 57.0 48.1 72.1


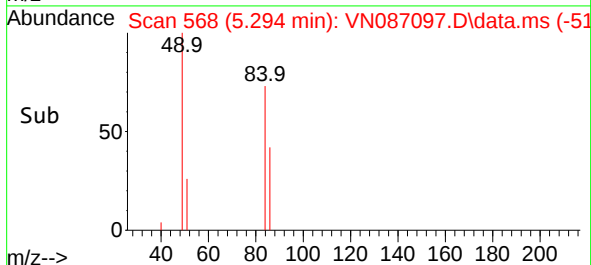
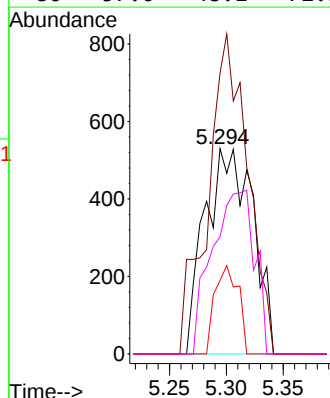
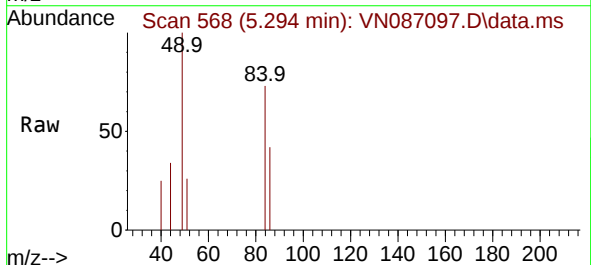




#21
trans-1,2-Dichloroethene
Concen: 0.215 ug/l
RT: 5.818 min Scan# 61
Delta R.T. 0.012 min
Lab File: VN087097.D
Acq: 18 Jun 2025 19:21




Instrument :
MSVOA_N
ClientSampleId :
VIBLK


Tgt Ion: 96 Resp: 405
Ion Ratio Lower Upper
96 100
61 110.8 109.2 163.8
98 0.0 49.8 74.8#

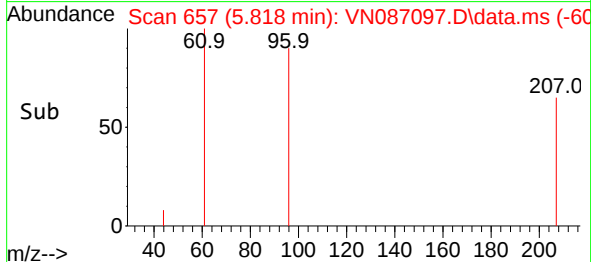

#31
Cyclohexane
Concen: 0.850 ug/l
RT: 8.229 min Scan# 1067
Delta R.T. -0.041 min
Lab File: VN087097.D
Acq: 18 Jun 2025 19:21

Tgt Ion: 56 Resp: 2801
Ion Ratio Lower Upper
56 100
69 219.1 25.4 38.0#
84 181.6 68.8 103.2#

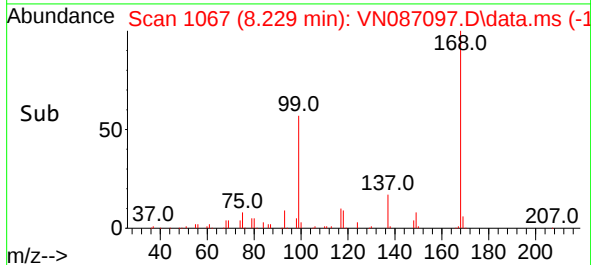

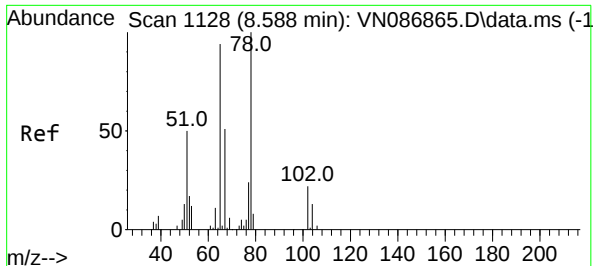

#33

1,2-Dichloroethane-d4

Concen: 55.529 ug/l

RT: 8.582 min Scan# 1128

Delta R.T. -0.006 min

Lab File: VN087097.D

Acq: 18 Jun 2025 19:21

Instrument :

MSVOA_N

ClientSampleId :





VIBLK

Tgt Ion: 65 Resp: 112887

Ion Ratio Lower Upper

65 100

67 56.1 0.0 105.6

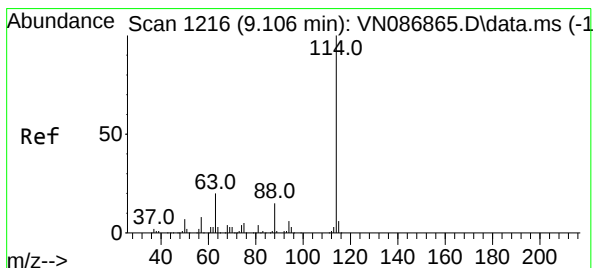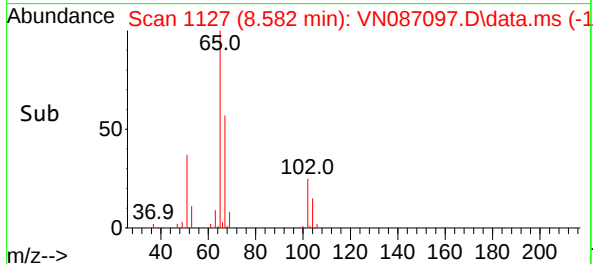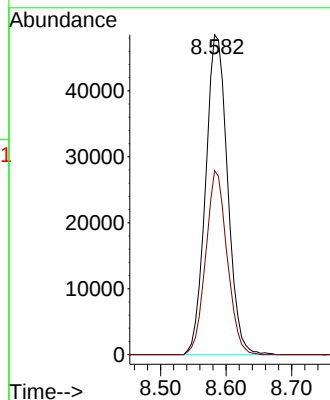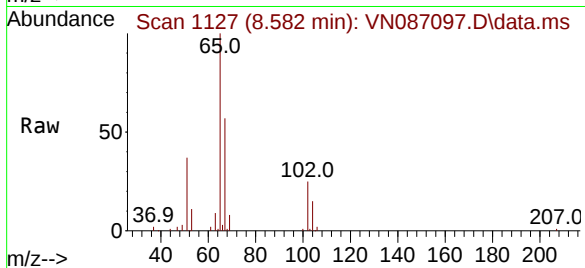

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.106 min Scan# 1216

Delta R.T. -0.000 min

Lab File: VN087097.D

Acq: 18 Jun 2025 19:21




Tgt Ion: 114 Resp: 305775


Ion Ratio Lower Upper

114 100

63 19.3 0.0 39.6

88 16.0 0.0 30.2


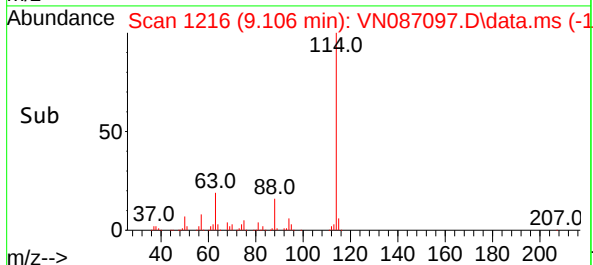
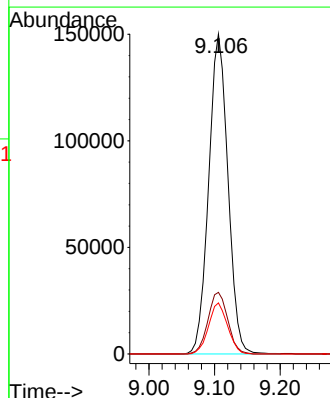
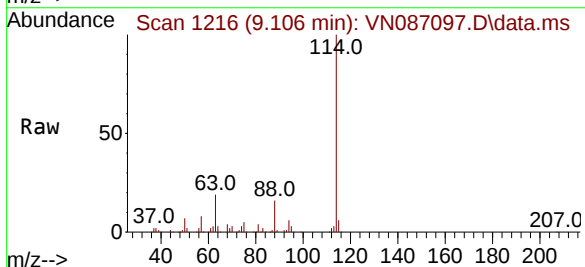


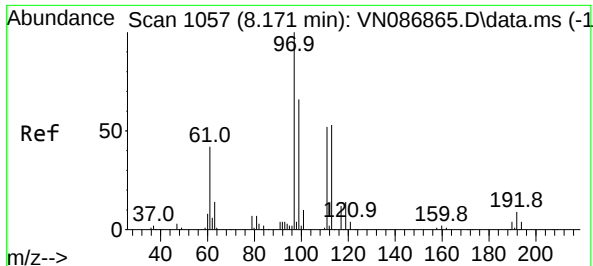

#35
Dibromofluoromethane
Concen: 52.323 ug/l
RT: 8.177 min Scan# 1057
Delta R.T. 0.006 min
Lab File: VN087097.D
Acq: 18 Jun 2025 19:21




Instrument :
MSVOA_N
ClientSampleId :
VIBLK


Tgt Ion:113 Resp: 94815
Ion Ratio Lower Upper
113 100
111 106.2 84.2 126.2
192 17.7 14.2 21.4

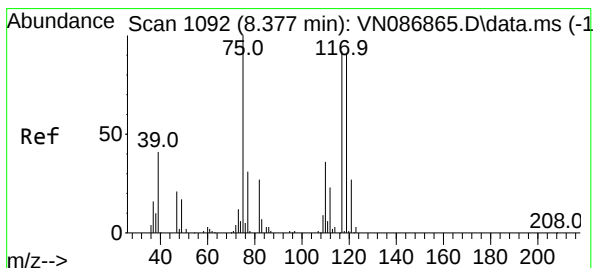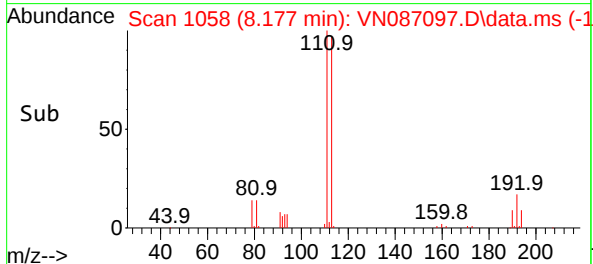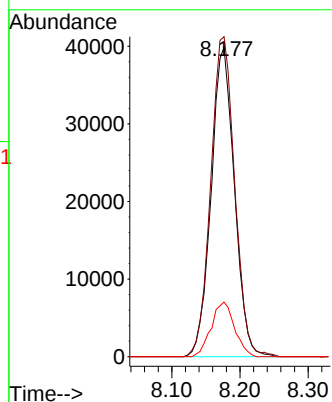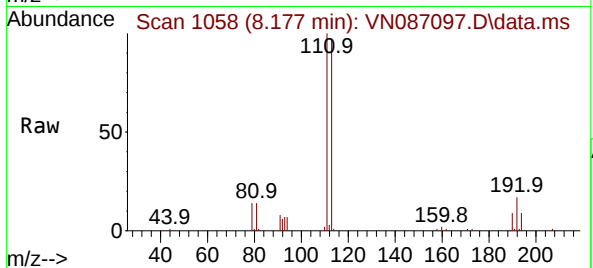

#36
1,1-Dichloropropene
Concen: 4.213 ug/l
RT: 8.235 min Scan# 1068
Delta R.T. -0.141 min
Lab File: VN087097.D
Acq: 18 Jun 2025 19:21

Tgt Ion: 75 Resp: 11376
Ion Ratio Lower Upper
75 100
110 7.1 17.6 52.9#
77 0.0 25.3 37.9#


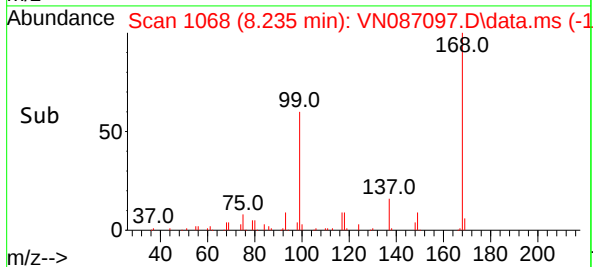

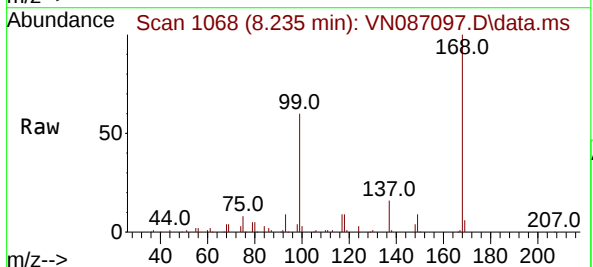


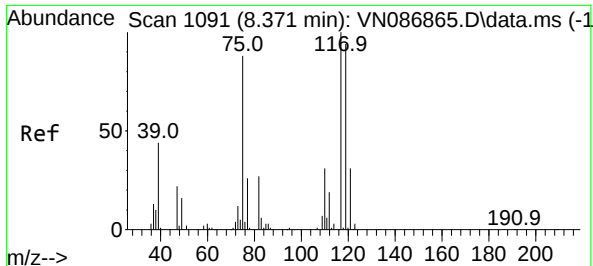

#38
Carbon Tetrachloride
Concen: 5.541 ug/l
RT: 8.229 min Scan# 1091
Delta R.T. -0.141 min
Lab File: VN087097.D
Acq: 18 Jun 2025 19:21




Instrument :
MSVOA_N
ClientSampleId :
VIBLK


Tgt Ion:117 Resp: 14690
Ion Ratio Lower Upper
117 100
119 4.3 75.0 112.6#
121 0.0 24.9 37.3#

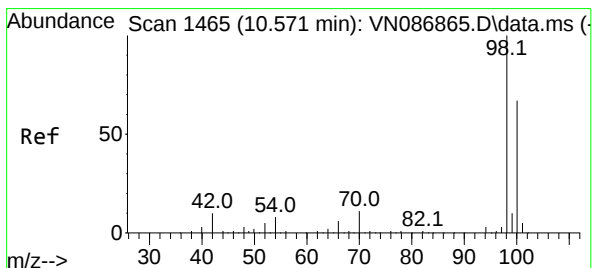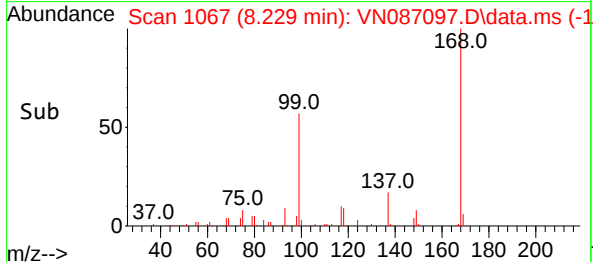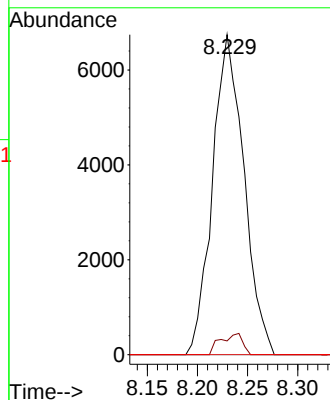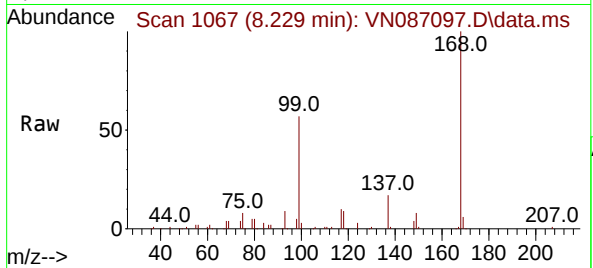

#50
Toluene-d8
Concen: 52.496 ug/l
RT: 10.565 min Scan# 1464
Delta R.T. -0.006 min
Lab File: VN087097.D
Acq: 18 Jun 2025 19:21

Tgt Ion: 98 Resp: 376582
Ion Ratio Lower Upper
98 100
100 66.8 53.4 80.0


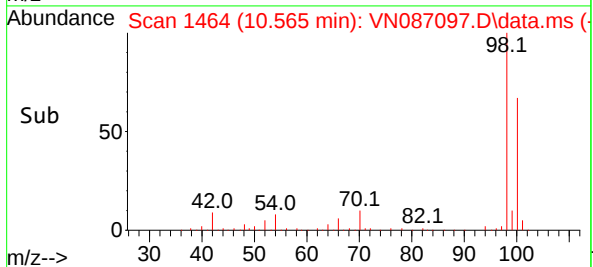
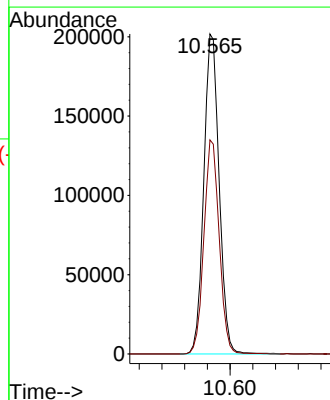
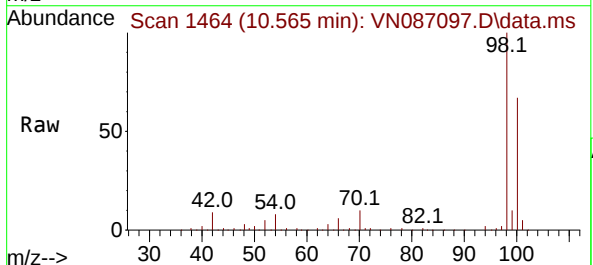




#62
4-Bromofluorobenzene
Concen: 48.933 ug/l
RT: 12.847 min Scan# 1852
Delta R.T. -0.000 min
Lab File: VN087097.D
Acq: 18 Jun 2025 19:21




Instrument :
MSVOA_N
ClientSampleId :
VIBLK


Tgt Ion: 95 Resp: 130417
Ion Ratio Lower Upper
95 100
174 72.5 0.0 141.8
176 67.6 0.0 132.6

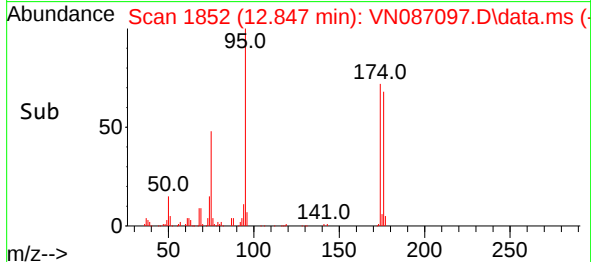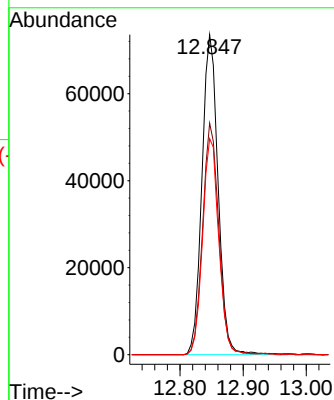

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.865 min Scan# 1685
Delta R.T. -0.000 min
Lab File: VN087097.D
Acq: 18 Jun 2025 19:21

Tgt Ion: 117 Resp: 276771
Ion Ratio Lower Upper
117 100
82 55.8 44.6 67.0
119 31.2 25.5 38.3



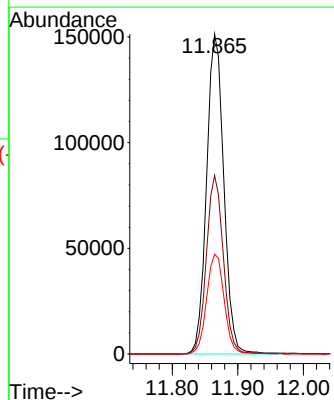
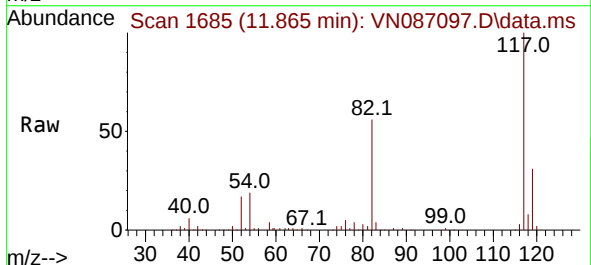




#68
m/p-Xylenes
Concen: 0.232 ug/l
RT: 12.070 min Scan# 11
Delta R.T. -0.000 min
Lab File: VN087097.D
Acq: 18 Jun 2025 19:21




Instrument :
MSVOA_N
ClientSampleId :
VIBLK


Tgt Ion:106 Resp: 935
Ion Ratio Lower Upper
106 100
91 174.7 159.4 239.0

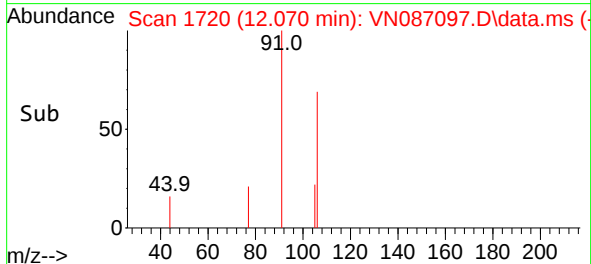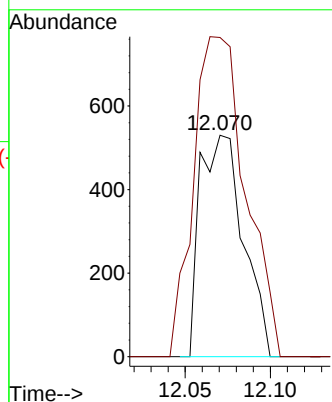

#71
Bromoform
Concen: 0.550 ug/l
RT: 12.847 min Scan# 1852
Delta R.T. 0.264 min
Lab File: VN087097.D
Acq: 18 Jun 2025 19:21

Tgt Ion:173 Resp: 800
Ion Ratio Lower Upper
173 100
175 732.3 24.1 72.4#
254 0.0 0.0 0.0



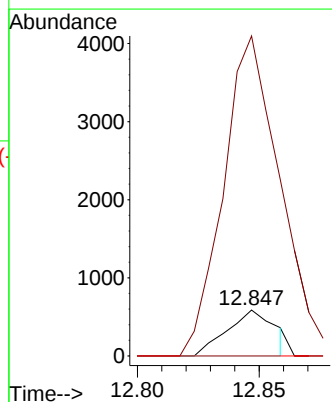
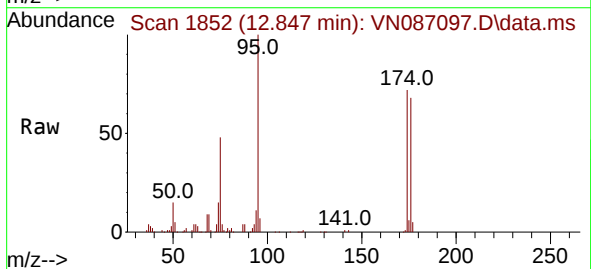




#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.788 min Scan# 2013
Delta R.T. -0.006 min
Lab File: VN087097.D
Acq: 18 Jun 2025 19:21




Instrument :
MSVOA_N
ClientSampleId :
VIBLK


Tgt Ion:152 Resp: 126979
Ion Ratio Lower Upper
152 100
115 60.6 30.1 90.5
150 158.4 0.0 345.0

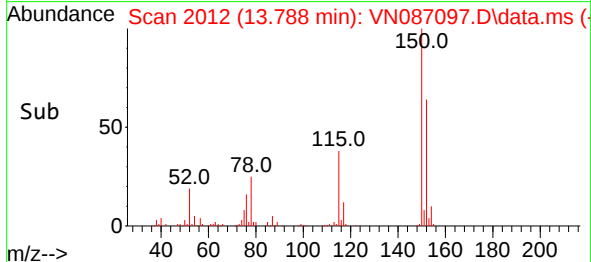

#73
Isopropylbenzene
Concen: 0.202 ug/l
RT: 12.694 min Scan# 1826
Delta R.T. -0.000 min
Lab File: VN087097.D
Acq: 18 Jun 2025 19:21

Tgt Ion:105 Resp: 1865
Ion Ratio Lower Upper
105 100
120 15.7 13.5 40.4

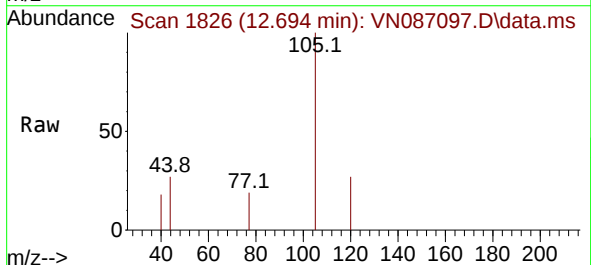



#76

1,2,3-Trichloropropane

Concen: 19.731 ug/l

RT: 12.847 min Scan# 1852

Delta R.T. -0.147 min

Lab File: VN087097.D

Acq: 18 Jun 2025 19:21

Instrument :

MSVOA_N

ClientSampleId :





VIBLK

Tgt Ion: 75 Resp: 59554

Ion Ratio Lower Upper

75 100

77 1.4 79.3 237.9#

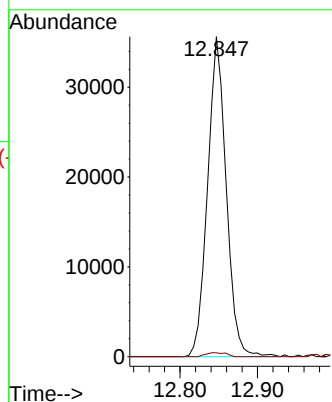

#78

n-propylbenzene

Concen: 0.237 ug/l

RT: 13.035 min Scan# 1884

Delta R.T. -0.000 min

Lab File: VN087097.D




Acq: 18 Jun 2025 19:21


Tgt Ion: 91 Resp: 2665

Ion Ratio Lower Upper

91 100

120 17.3 11.4 34.2





#80

1,3,5-Trimethylbenzene

Concen: 0.203 ug/l

RT: 13.170 min Scan# 1907

Delta R.T. -0.000 min

Lab File: VN087097.D

Acq: 18 Jun 2025 19:21

Instrument :

MSVOA_N

ClientSampleId :





VIBLK

Tgt Ion:105 Resp: 1550

Ion Ratio Lower Upper

105 100

120 53.5 24.9 74.6

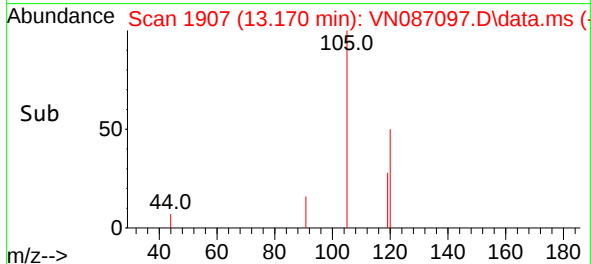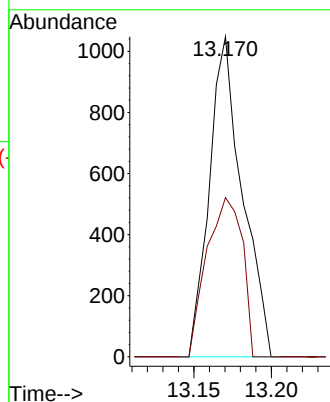

#81

trans-1,4-Dichloro-2-butene

Concen: 45.419 ug/l

RT: 12.847 min Scan# 1852

Delta R.T. 0.112 min

Lab File: VN087097.D

Acq: 18 Jun 2025 19:21




Tgt Ion: 75 Resp: 59554


Ion Ratio Lower Upper

75 100

53 0.0 66.6 99.8#

89 0.0 36.7 55.1#



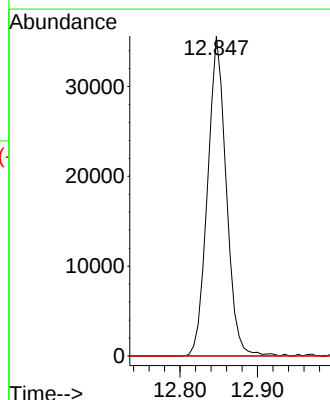





#82
4-Chlorotoluene
Concen: 0.214 ug/l
RT: 13.223 min Scan# 1916
Delta R.T. -0.000 min
Lab File: VN087097.D
Acq: 18 Jun 2025 19:21




Instrument :
MSVOA_N
ClientSampleId :
VIBLK


Tgt Ion: 91 Resp: 1460
Ion Ratio Lower Upper
91 100
126 25.3 16.7 50.1

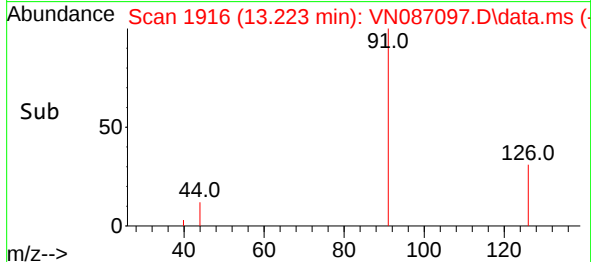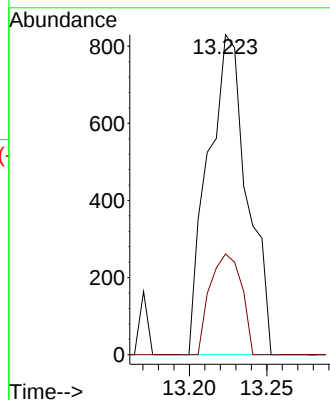

#83
tert-Butylbenzene
Concen: 0.238 ug/l
RT: 13.435 min Scan# 1952
Delta R.T. -0.000 min
Lab File: VN087097.D
Acq: 18 Jun 2025 19:21

Tgt Ion: 119 Resp: 1667
Ion Ratio Lower Upper
119 100
91 65.6 32.1 96.5
134 22.7 13.4 40.1



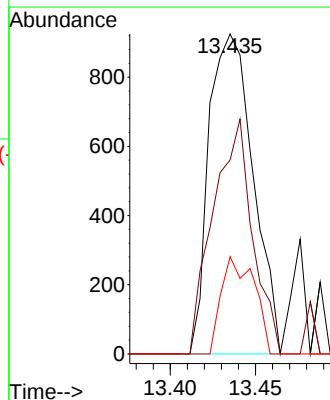
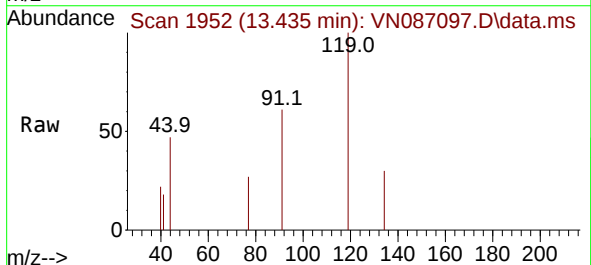




#84
1,2,4-Trimethylbenzene
Concen: 0.208 ug/l
RT: 13.482 min Scan# 1960
Delta R.T. -0.000 min
Lab File: VN087097.D
Acq: 18 Jun 2025 19:21




Instrument :
MSVOA_N
ClientSampleId :
VIBLK


Tgt Ion:105 Resp: 1590
Ion Ratio Lower Upper
105 100
120 51.6 23.2 69.6

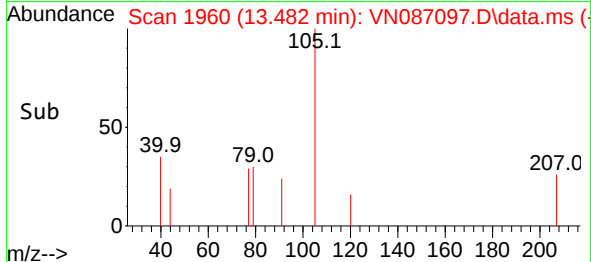

#85
sec-Butylbenzene
Concen: 0.282 ug/l
RT: 13.617 min Scan# 1983
Delta R.T. -0.000 min
Lab File: VN087097.D
Acq: 18 Jun 2025 19:21

Tgt Ion:105 Resp: 2864
Ion Ratio Lower Upper
105 100
134 19.4 10.0 30.0




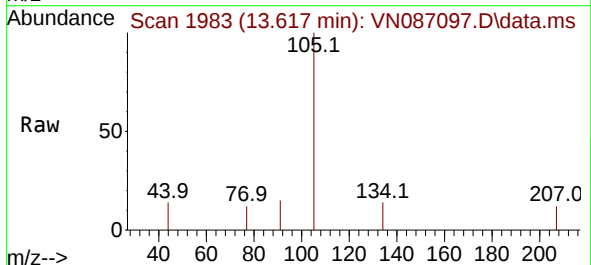




#86
p-Isopropyltoluene
Concen: 0.249 ug/l
RT: 13.729 min Scan# 2002
Delta R.T. -0.000 min
Lab File: VN087097.D
Acq: 18 Jun 2025 19:21




Instrument :
MSVOA_N
ClientSampleId :
VIBLK


Tgt Ion:	119	Resp:	2092
Ion	Ratio	Lower	Upper
119	100		
134	21.0	13.5	40.4
91	20.0	11.5	34.4

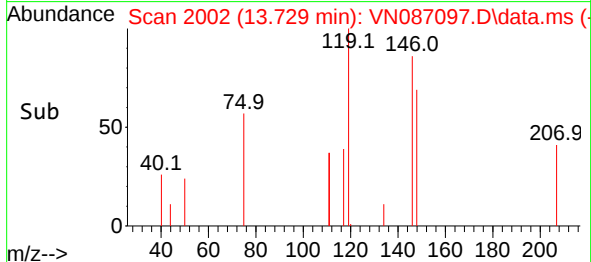

#87
1,3-Dichlorobenzene
Concen: 0.224 ug/l
RT: 13.735 min Scan# 2003
Delta R.T. -0.000 min
Lab File: VN087097.D
Acq: 18 Jun 2025 19:21

Tgt Ion:	146	Resp:	933
Ion	Ratio	Lower	Upper
146	100		
111	43.8	20.9	62.8
148	55.4	32.0	96.2




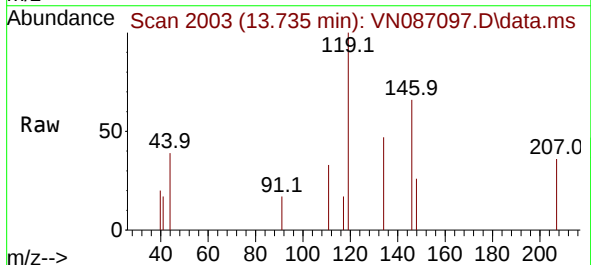




#88
1,4-Dichlorobenzene
Concen: 0.219 ug/l
RT: 13.735 min Scan# 2016
Delta R.T. -0.077 min
Lab File: VN087097.D
Acq: 18 Jun 2025 19:21




Instrument :
MSVOA_N
ClientSampleId :
VIBLK


Tgt Ion:146 Resp: 933
Ion Ratio Lower Upper
146 100
111 43.8 19.9 59.7
148 55.4 31.8 95.4

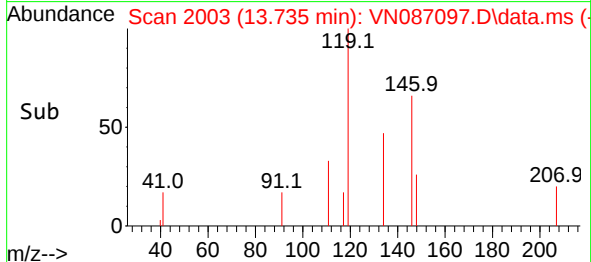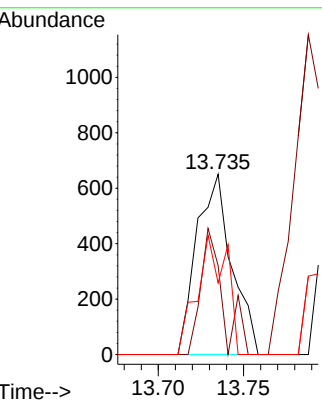

#89
n-Butylbenzene
Concen: 0.318 ug/l
RT: 14.059 min Scan# 2058
Delta R.T. 0.006 min
Lab File: VN087097.D
Acq: 18 Jun 2025 19:21

Tgt Ion: 91 Resp: 2583
Ion Ratio Lower Upper
91 100
92 66.4 27.5 82.4
134 24.8 13.0 39.0



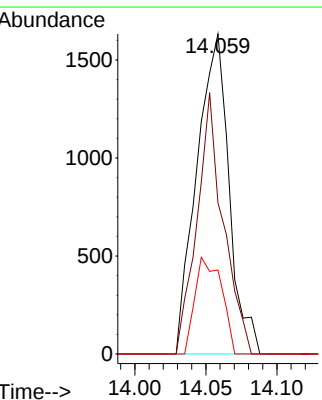
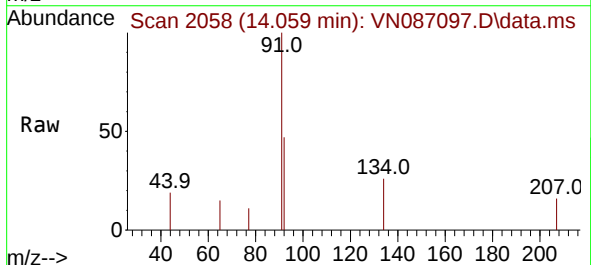


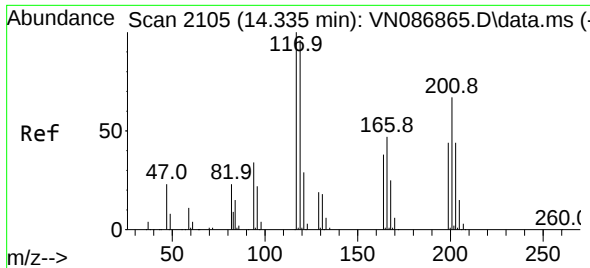

#90
Hexachloroethane
Concen: 0.289 ug/l
RT: 14.335 min Scan# 2105
Delta R.T. -0.000 min
Lab File: VN087097.D
Acq: 18 Jun 2025 19:21




Instrument :
MSVOA_N
ClientSampleId :
VIBLK


Tgt Ion:117 Resp: 411
Ion Ratio Lower Upper
117 100
201 16.1 33.2 99.6#

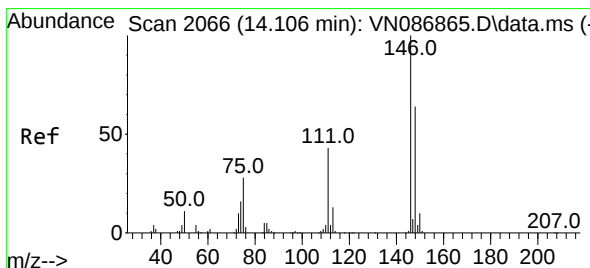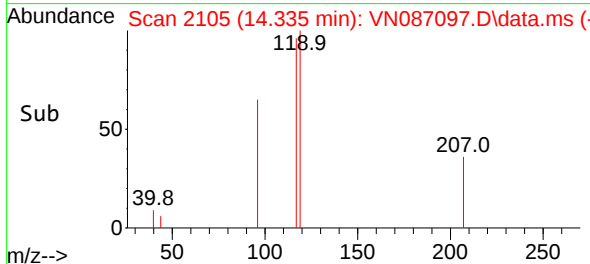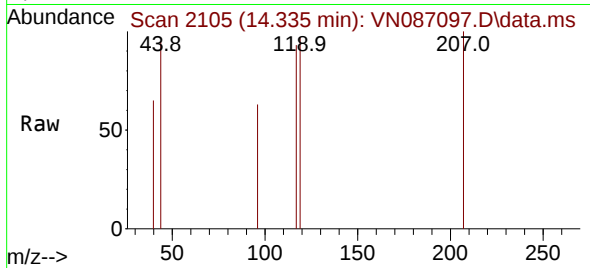

#91
1,2-Dichlorobenzene
Concen: 0.212 ug/l
RT: 14.106 min Scan# 2066
Delta R.T. -0.000 min
Lab File: VN087097.D
Acq: 18 Jun 2025 19:21

Tgt Ion:146 Resp: 849
Ion Ratio Lower Upper
146 100
111 23.9 21.6 64.6
148 42.8 31.7 95.1


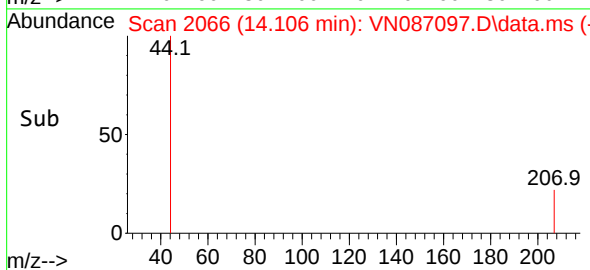

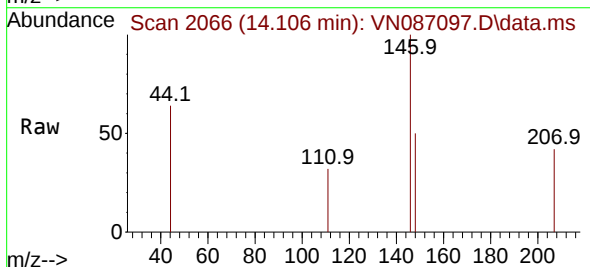




#93
1,2,4-Trichlorobenzene
Concen: 0.470 ug/l
RT: 15.394 min Scan# 21
Delta R.T. 0.006 min
Lab File: VN087097.D
Acq: 18 Jun 2025 19:21




Instrument :
MSVOA_N
ClientSampleId :
VIBLK


Tgt Ion:180 Resp: 1204
Ion Ratio Lower Upper
180 100
182 97.1 46.9 140.7
145 29.0 16.0 47.9

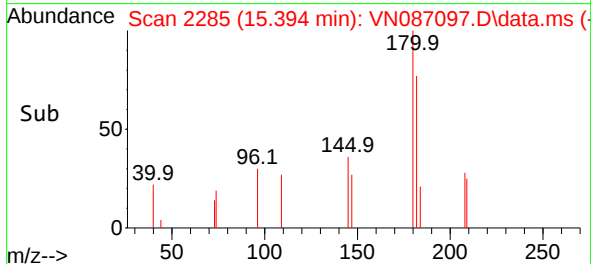

#94
Hexachlorobutadiene
Concen: 1.127 ug/l
RT: 15.500 min Scan# 2303
Delta R.T. -0.000 min
Lab File: VN087097.D
Acq: 18 Jun 2025 19:21

Tgt Ion:225 Resp: 1075
Ion Ratio Lower Upper
225 100
223 73.5 33.5 100.4
227 65.0 31.1 93.5





#95

Naphthalene

Concen: 0.385 ug/l

RT: 15.641 min Scan# 2327

Delta R.T. -0.000 min

Lab File: VN087097.D

Acq: 18 Jun 2025 19:21





Instrument :

MSVOA_N

ClientSampleId :

VIBLK

Tgt Ion:	128	Resp:	3674
Ion	Ratio	Lower	Upper
128	100		
127	8.8	10.2	15.2#
129	4.8	8.8	13.2#

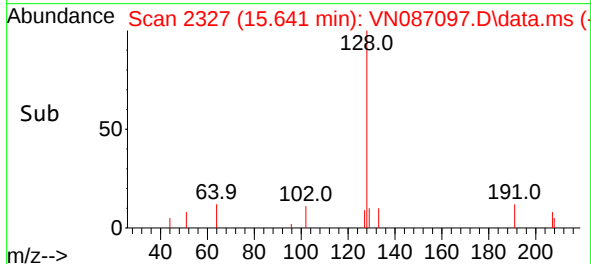

#96

1,2,3-Trichlorobenzene

Concen: 0.529 ug/l

RT: 15.835 min Scan# 2360

Delta R.T. -0.000 min

Lab File: VN087097.D

Acq: 18 Jun 2025 19:21

Tgt Ion:	180	Resp:	1346
Ion	Ratio	Lower	Upper
180	100		
182	85.7	47.0	141.0
145	29.2	16.6	49.8

