


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN061825\
Data File : VN087073.D
Acq On : 18 Jun 2025 08:43
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N060625W.M
Title : SW846 8260
Last Update : Sat Jun 07 02:12:50 2025

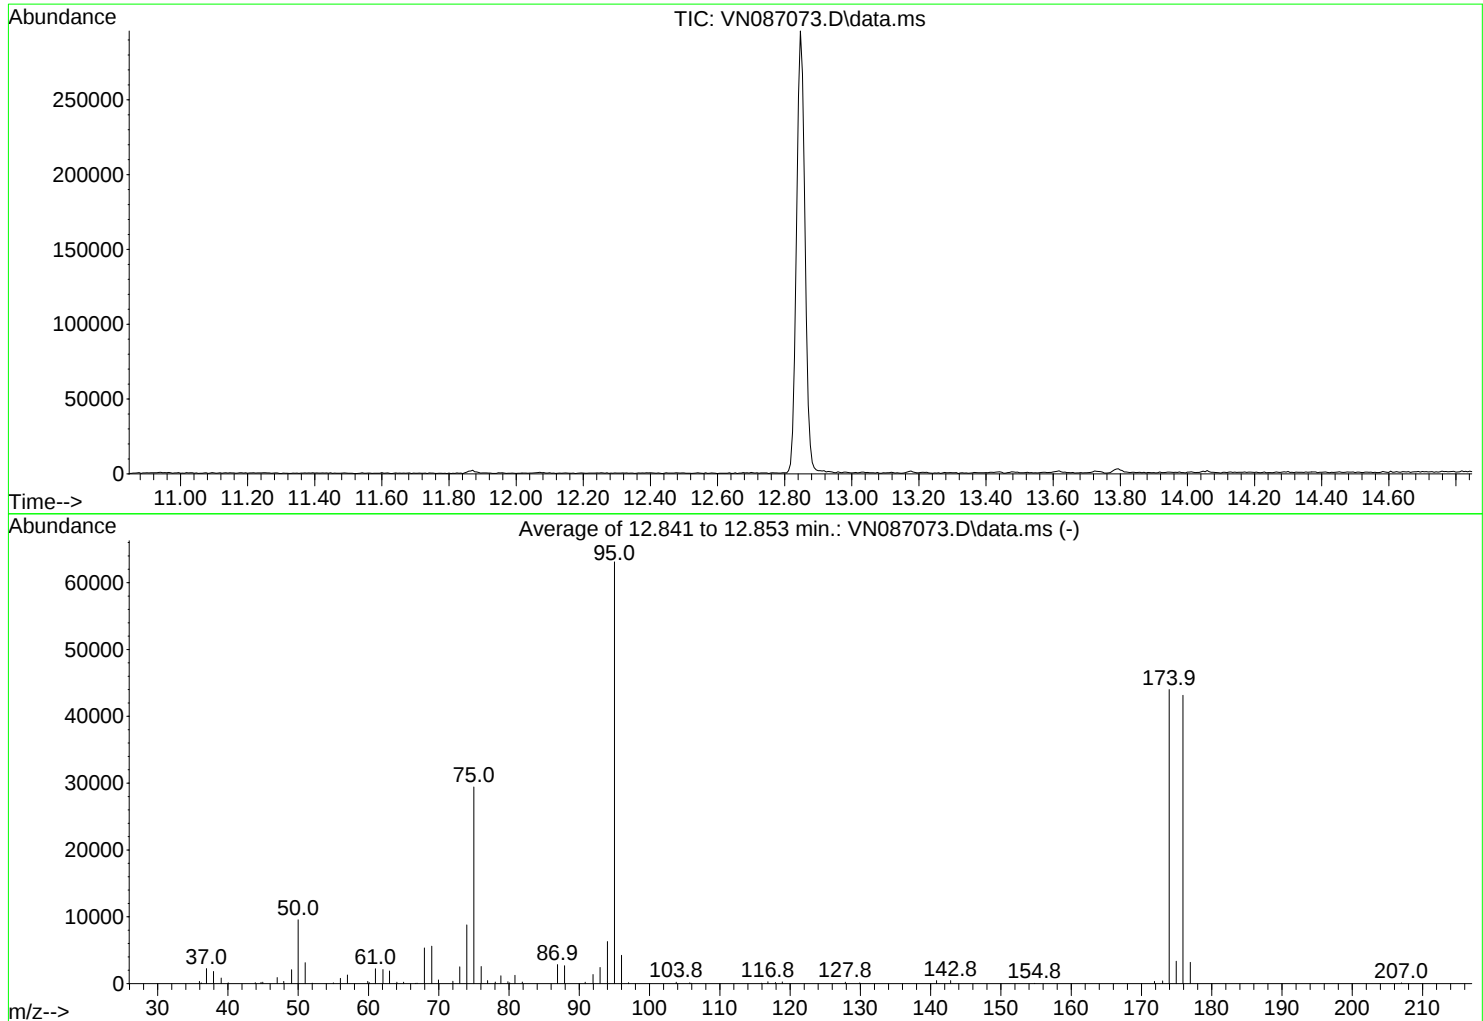

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.1	9552	PASS
75	95	30	60	46.6	29437	PASS
95	95	100	100	100.0	63117	PASS
96	95	5	9	6.7	4230	PASS
173	174	0.00	2	0.9	398	PASS
174	95	50	100	69.7	44019	PASS
175	174	5	9	7.6	3359	PASS
176	174	95	101	98.0	43136	PASS
177	176	5	9	7.4	3181	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	326	49.05	2072	63.00	1887	75.00	2943
36.20	127	50.00	9552	64.05	214	76.05	256
36.95	2245	51.00	3150	65.00	213	76.95	45
37.95	1829	52.00	67	66.70	53	78.05	25
39.05	850	55.00	121	66.90	83	78.85	1181
40.05	131	56.00	802	67.95	5346	79.85	283
43.90	153	57.00	1293	69.00	5613	80.10	112
44.70	199	59.90	330	69.95	547	80.85	1236
44.95	220	60.10	160	72.00	352	81.90	245
47.00	909	61.00	2238	73.00	2520	86.90	2859
47.95	328	62.05	2116	74.00	8779	87.90	2679

Average of 12.841 to 12.853 min.: VN087073.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
90.85	208	116.85	290	174.95	3359		
91.95	1375	117.90	160	175.90	43136		
92.95	2428	118.90	278	176.95	3181		
94.00	6293	127.85	229	207.00	128		
95.00	63117	129.90	119				
96.00	4230	140.85	459				
97.00	146	142.85	461				
103.80	218	154.80	59				
105.70	125	171.85	340				
105.90	65	173.00	398				
115.90	84	173.95	44019				

Instrument :

MSVOA_N

ClientSampleId :

BFB