


Methylene Chloride

Response Ratio

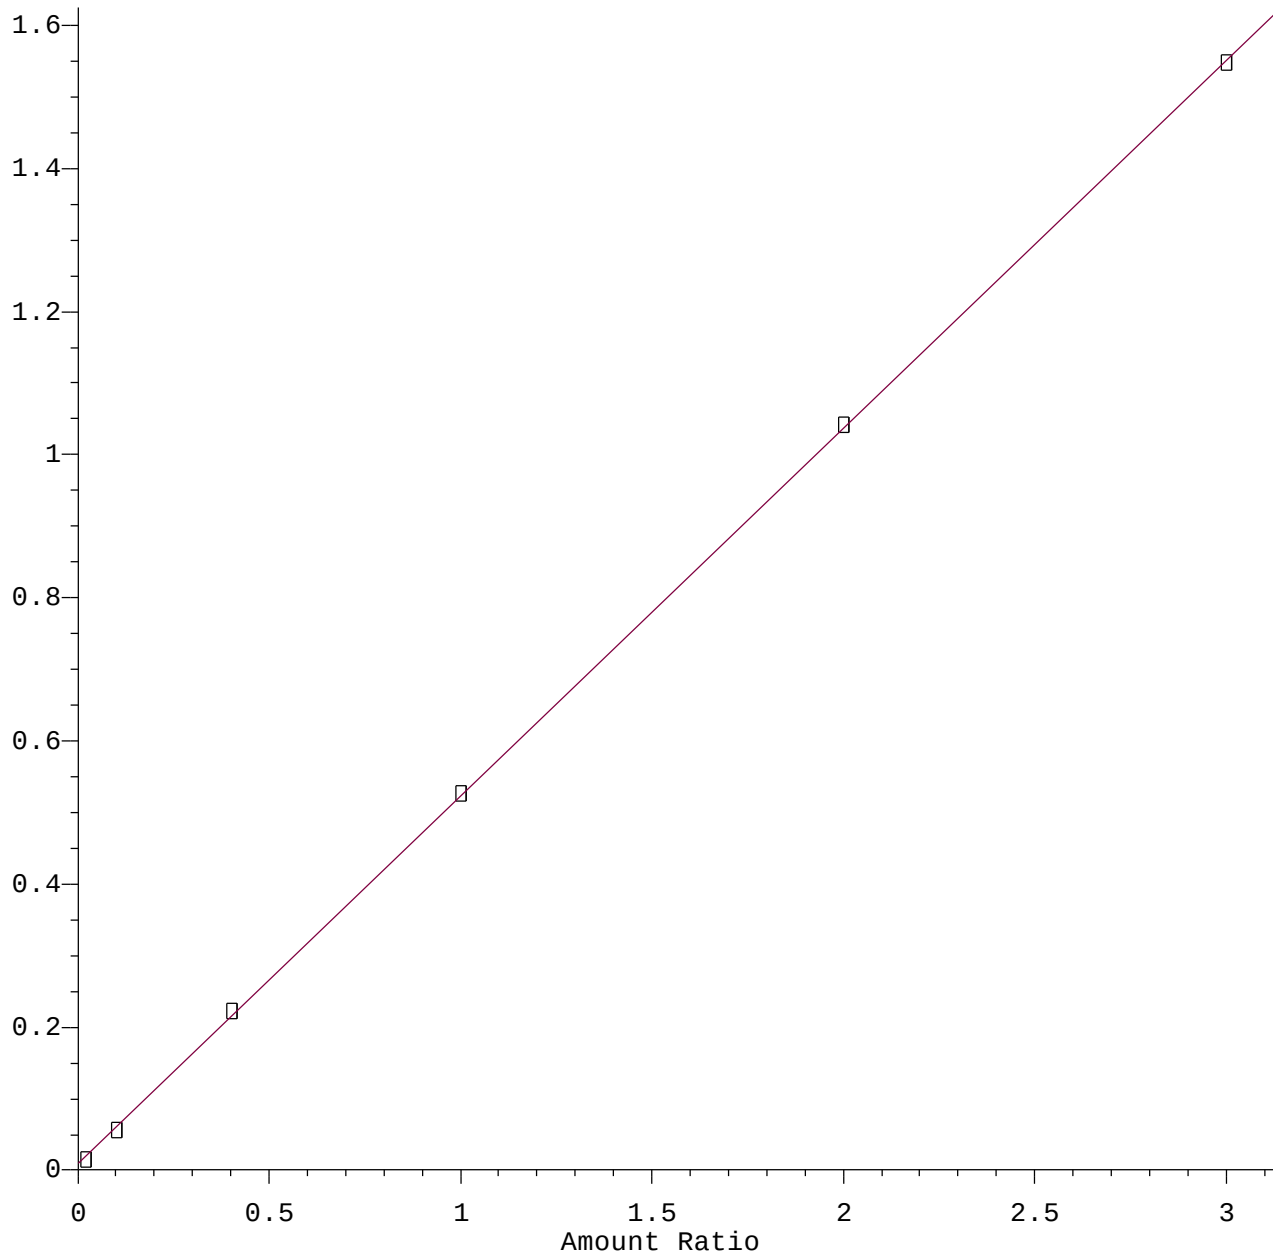


Resp Ratio = 5.14e-001 * Amt + 9.32e-003
Coef of Det (r^2) = 1.000 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N061919W.M
Calibration Table Last Updated: Fri Jun 21 03:45:40 2019


t-1,3-Dichloropropene

Response Ratio

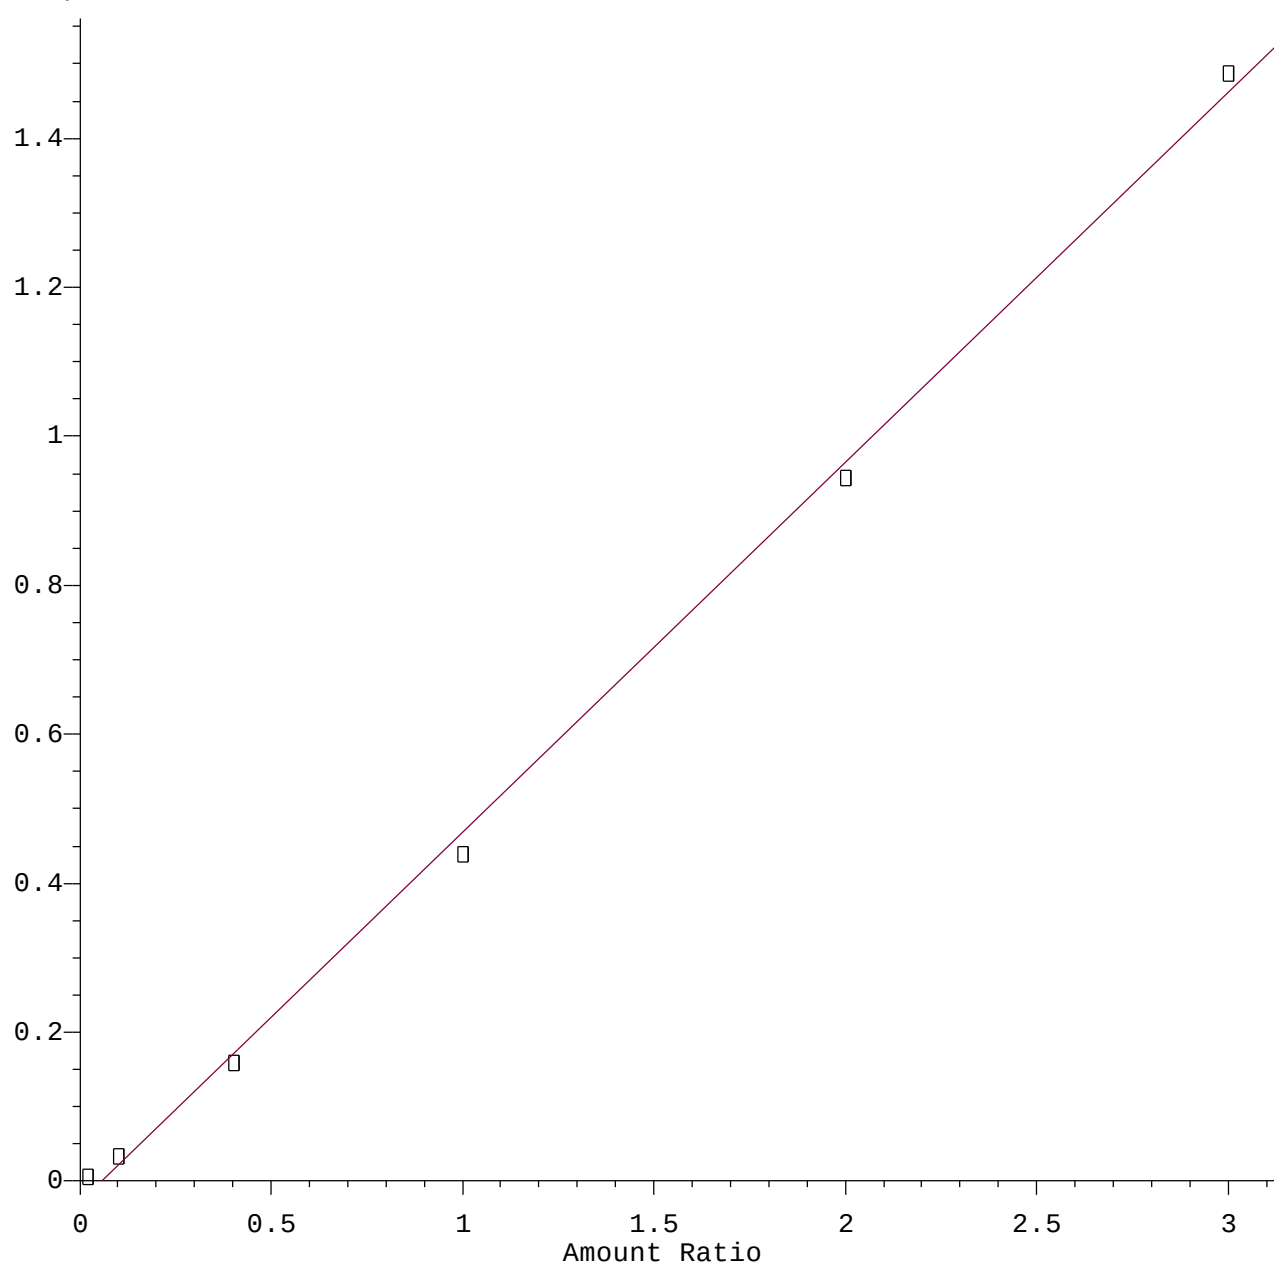


Resp Ratio = $4.97 \times 10^{-1} \times \text{Amt} - 2.87 \times 10^{-2}$
Coef of Det (r^2) = 0.998 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N061919W.M
Calibration Table Last Updated: Fri Jun 21 03:45:40 2019

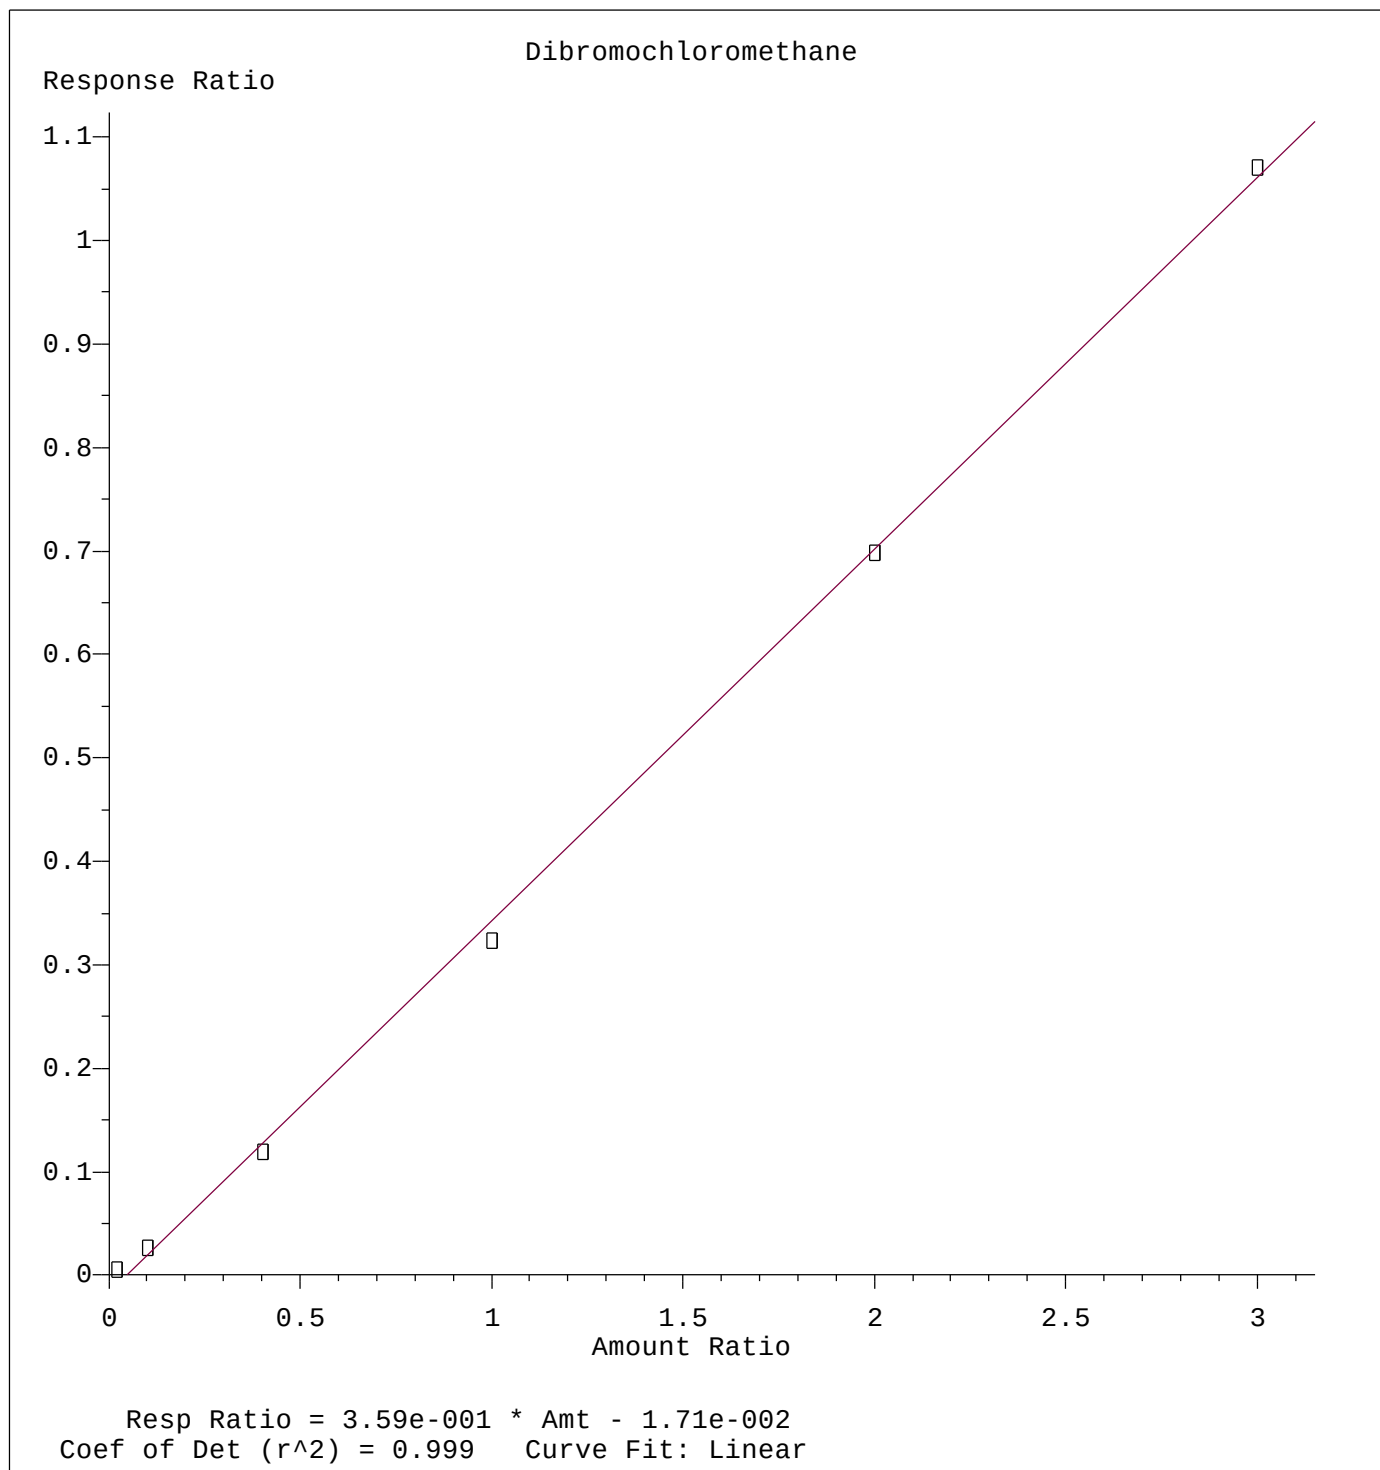


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N061919W.M
Calibration Table Last Updated: Fri Jun 21 03:45:40 2019

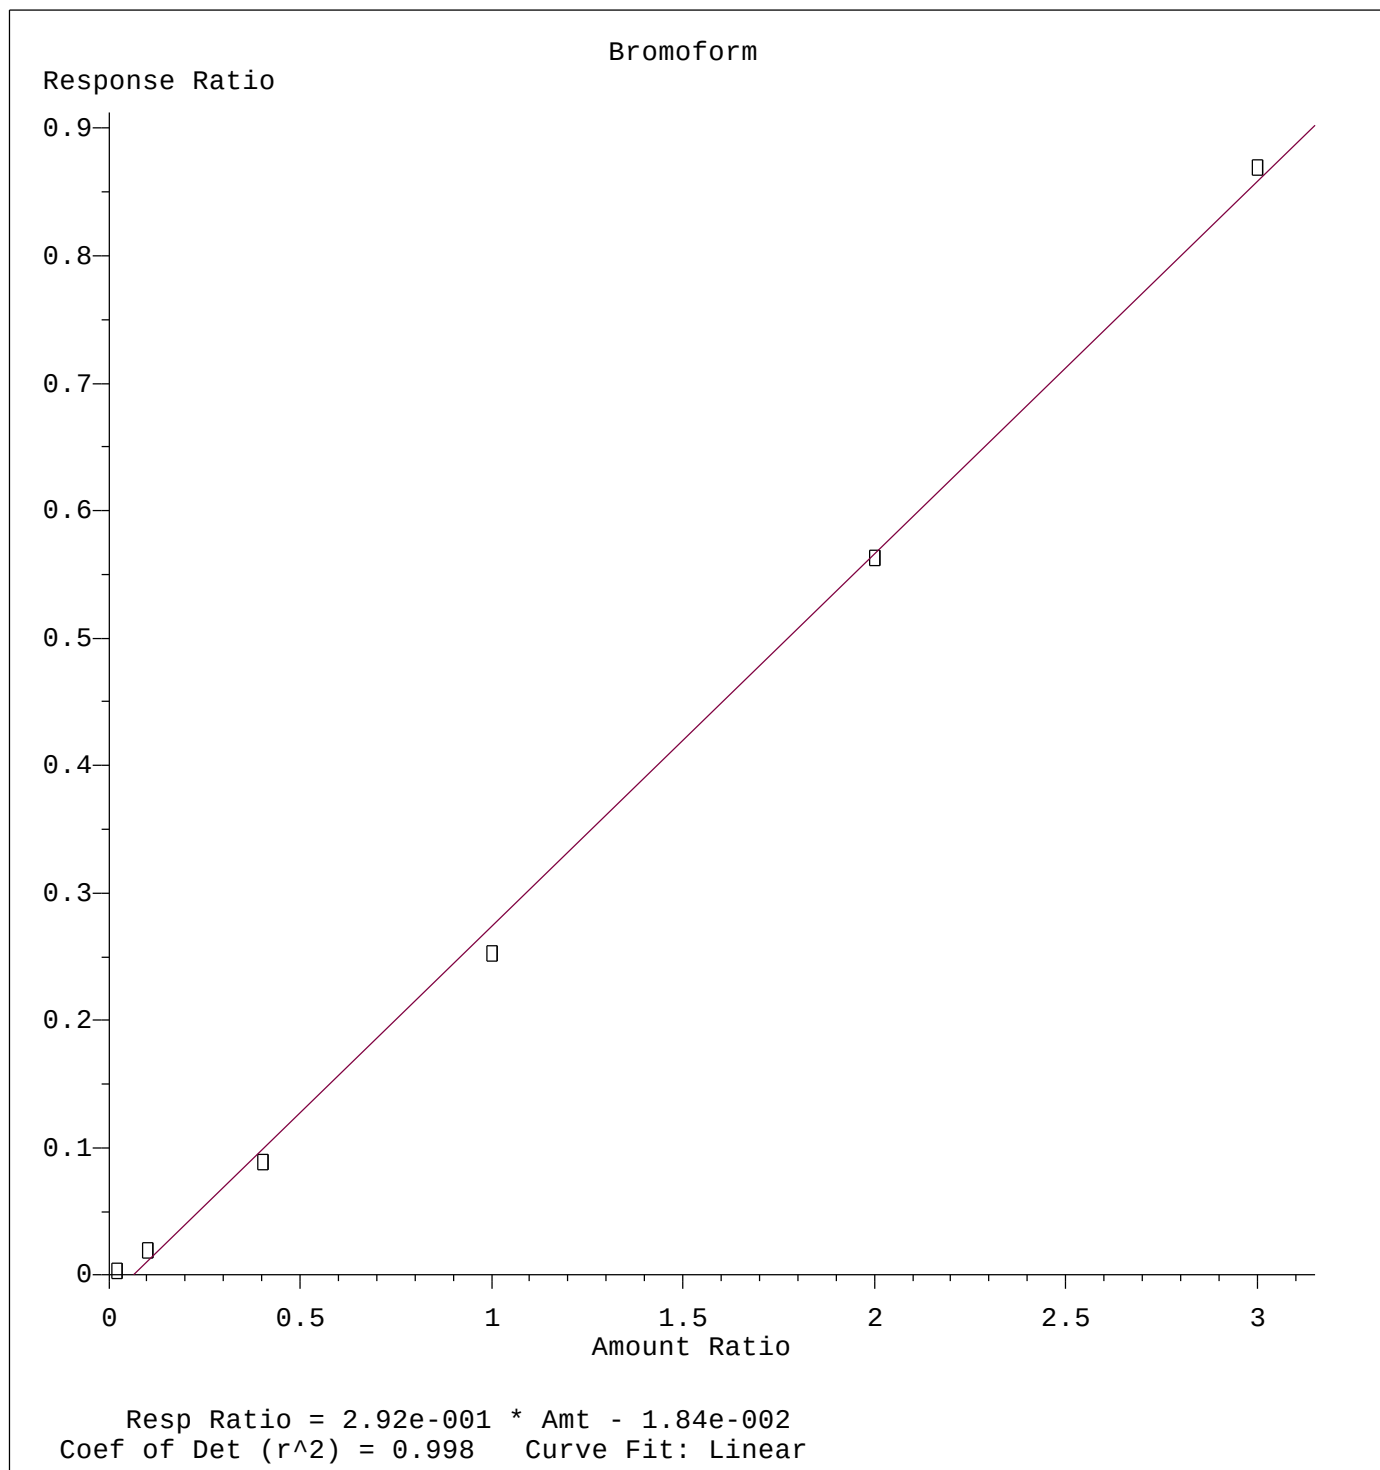

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N061919W.M
Calibration Table Last Updated: Fri Jun 21 03:45:40 2019

Isopropylbenzene

Response Ratio

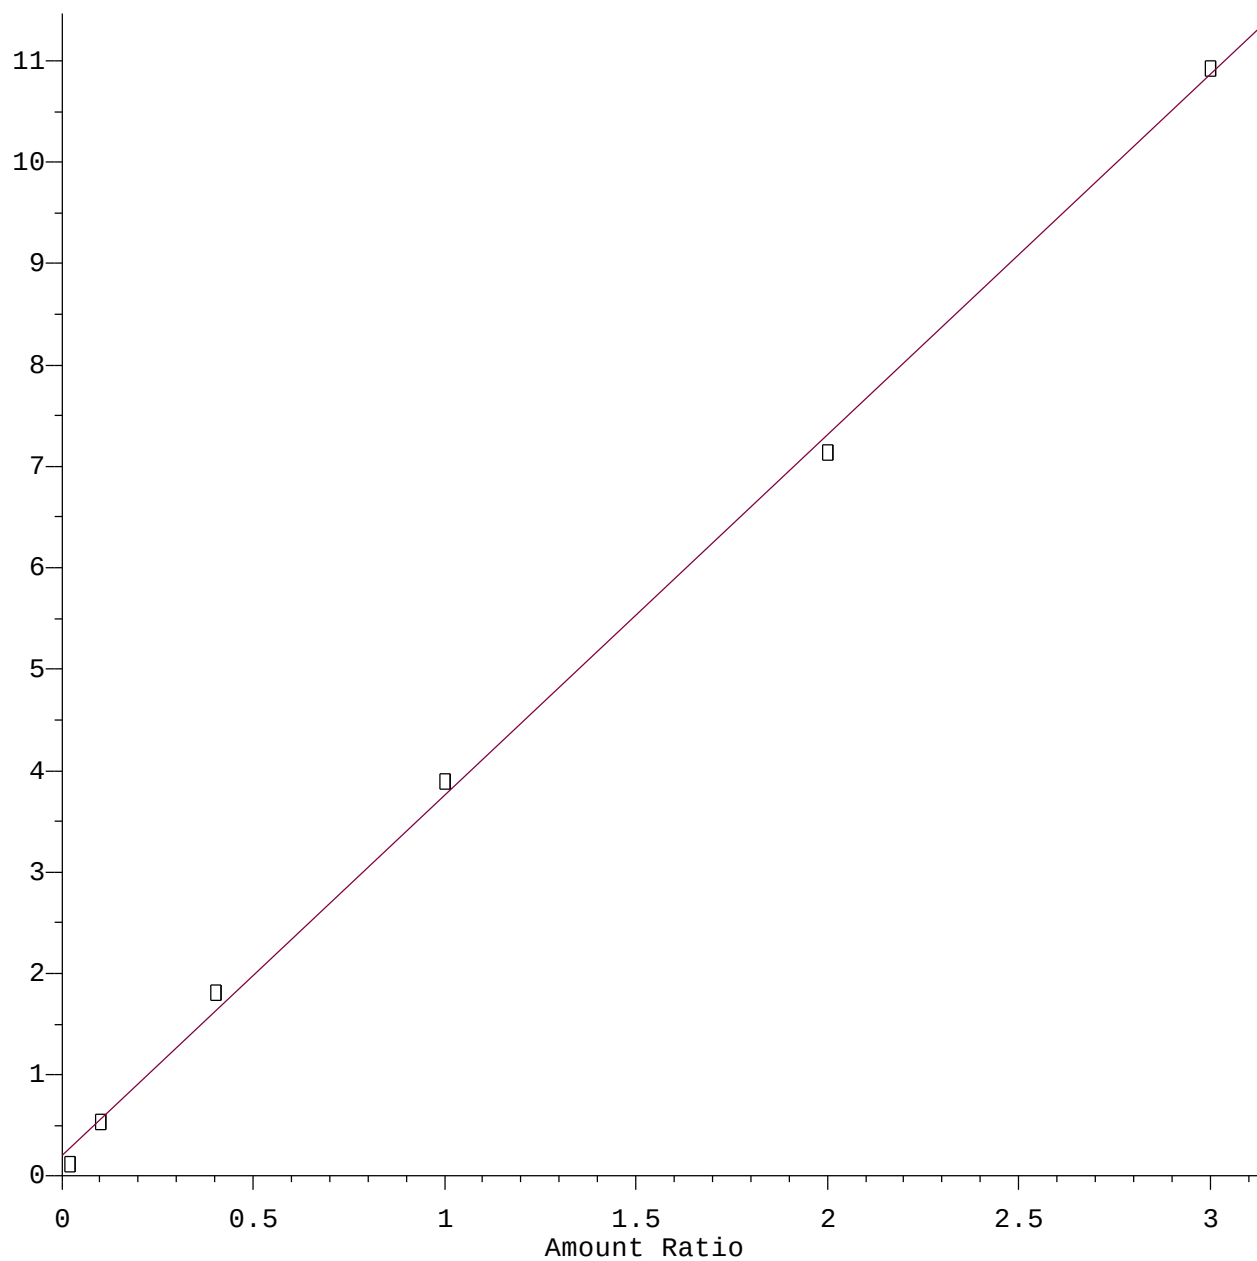


Resp Ratio = 3.55×10^0 * Amt + 2.02×10^{-1}
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N061919W.M
Calibration Table Last Updated: Fri Jun 21 03:45:40 2019

1,1,2,2-Tetrachloroethane

Response Ratio

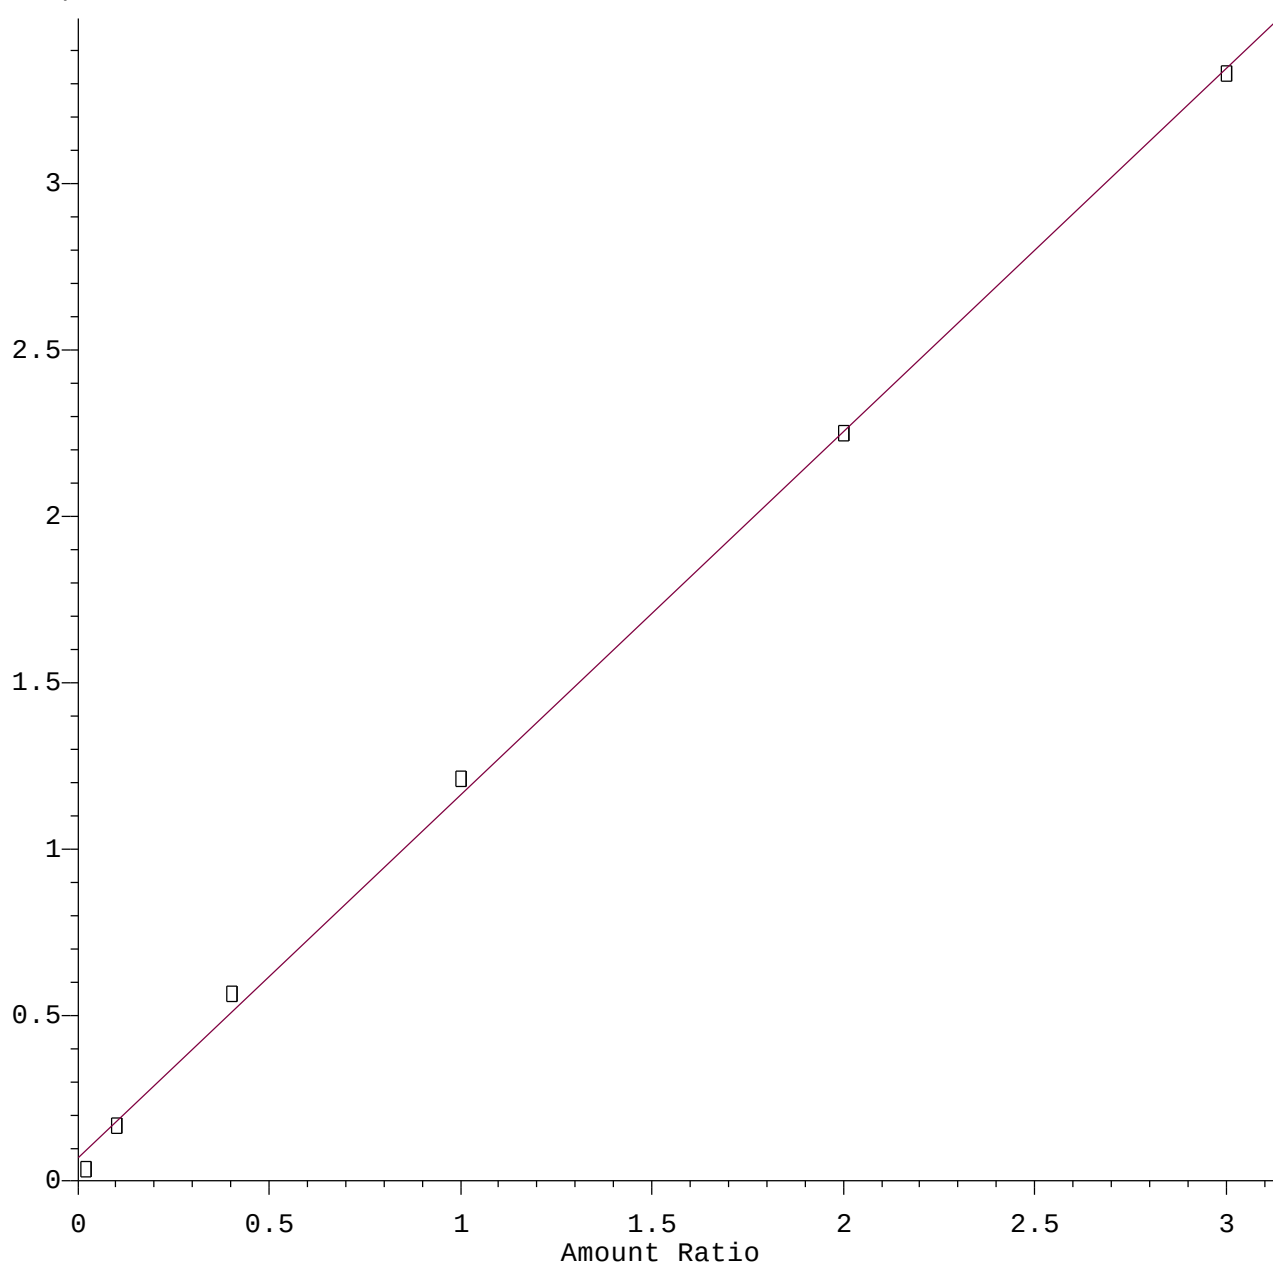


Resp Ratio = 1.09e+000 * Amt + 7.15e-002
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N061919W.M
Calibration Table Last Updated: Fri Jun 21 03:45:40 2019

2-Chlorotoluene

Response Ratio

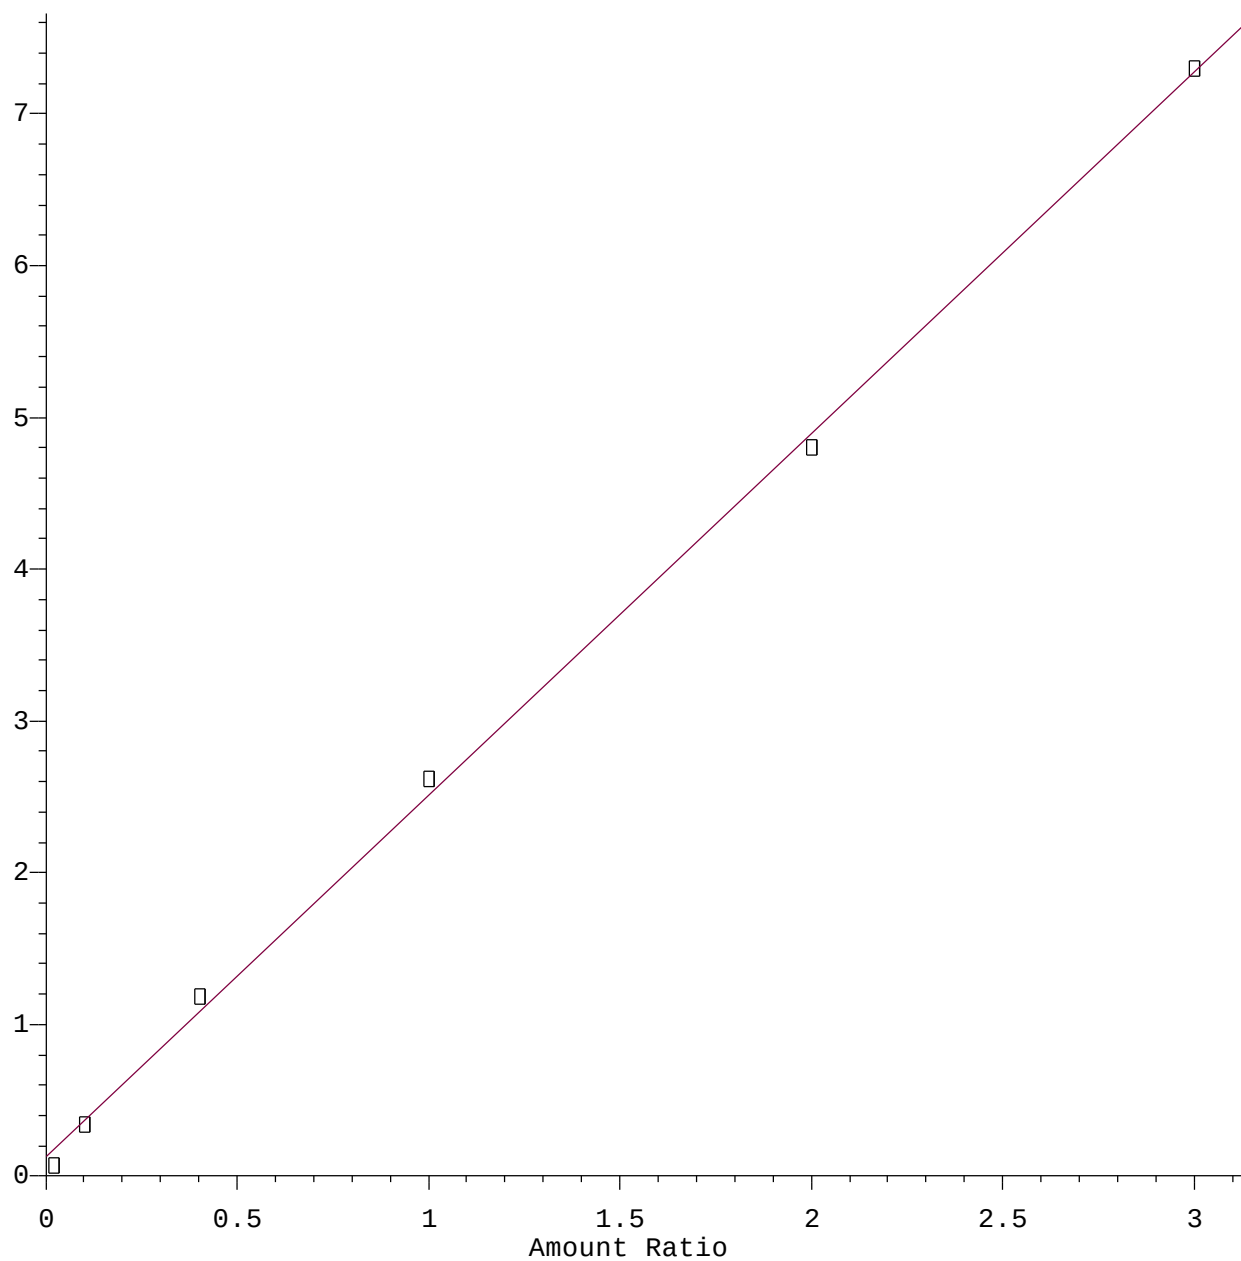


Resp Ratio = 2.38e+000 * Amt + 1.27e-001
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N061919W.M
Calibration Table Last Updated: Fri Jun 21 03:45:40 2019

1,3,5-Trimethylbenzene

Response Ratio

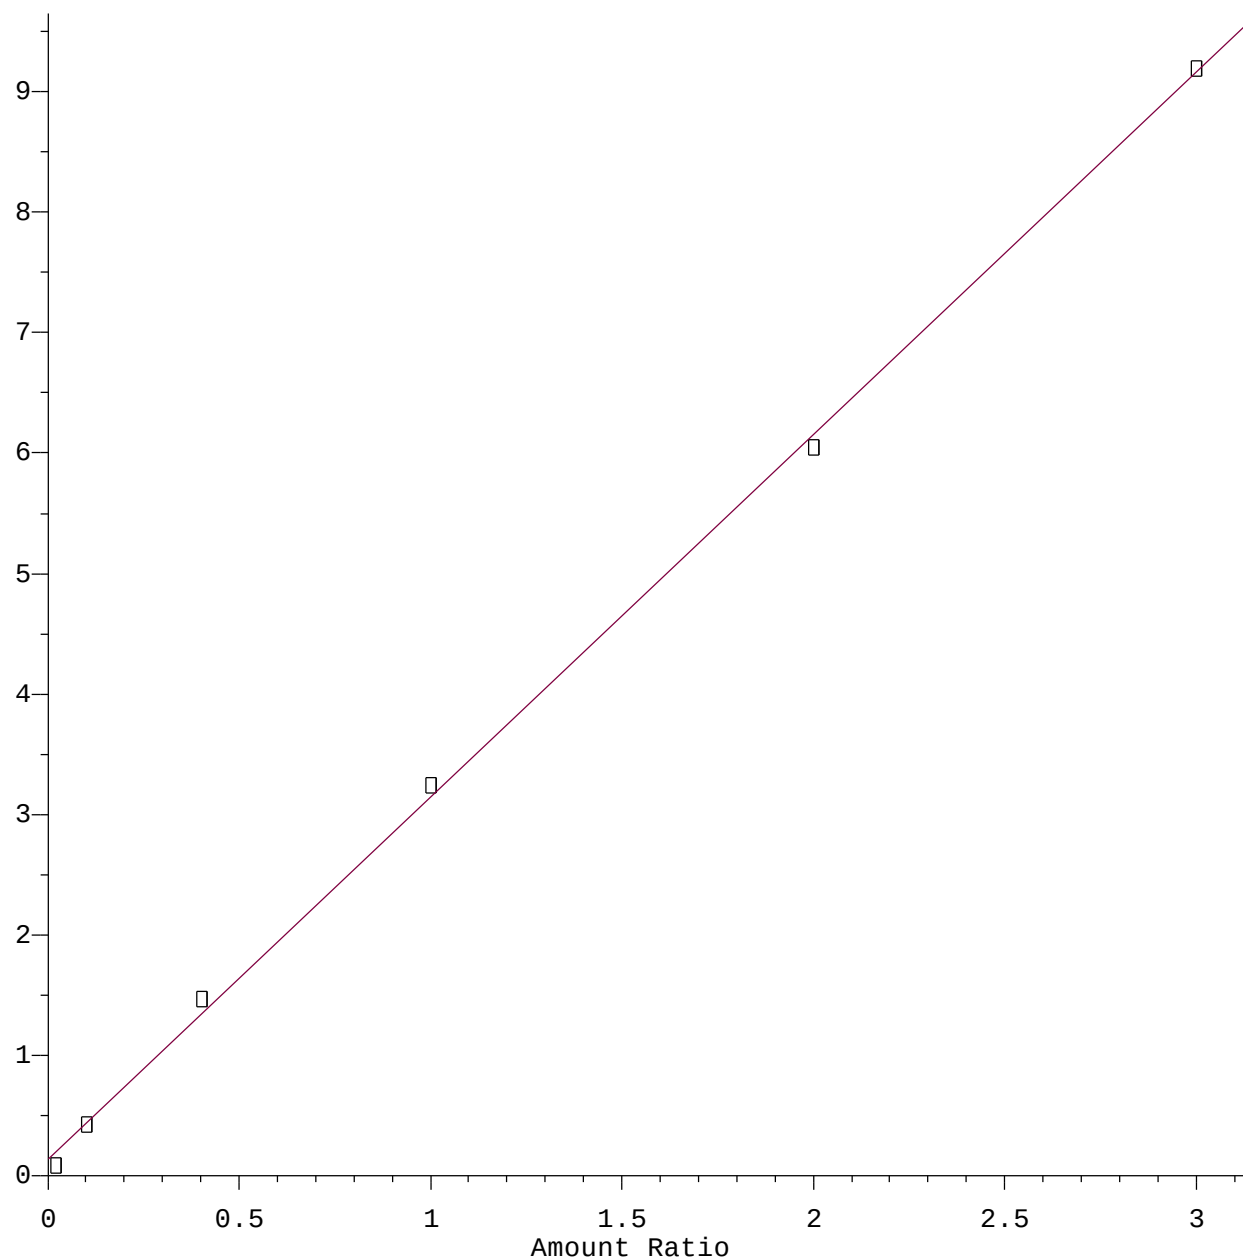


Resp Ratio = 3.00e+000 * Amt + 1.42e-001
Coef of Det (r²) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N061919W.M
Calibration Table Last Updated: Fri Jun 21 03:45:40 2019

tert-Butylbenzene

Response Ratio

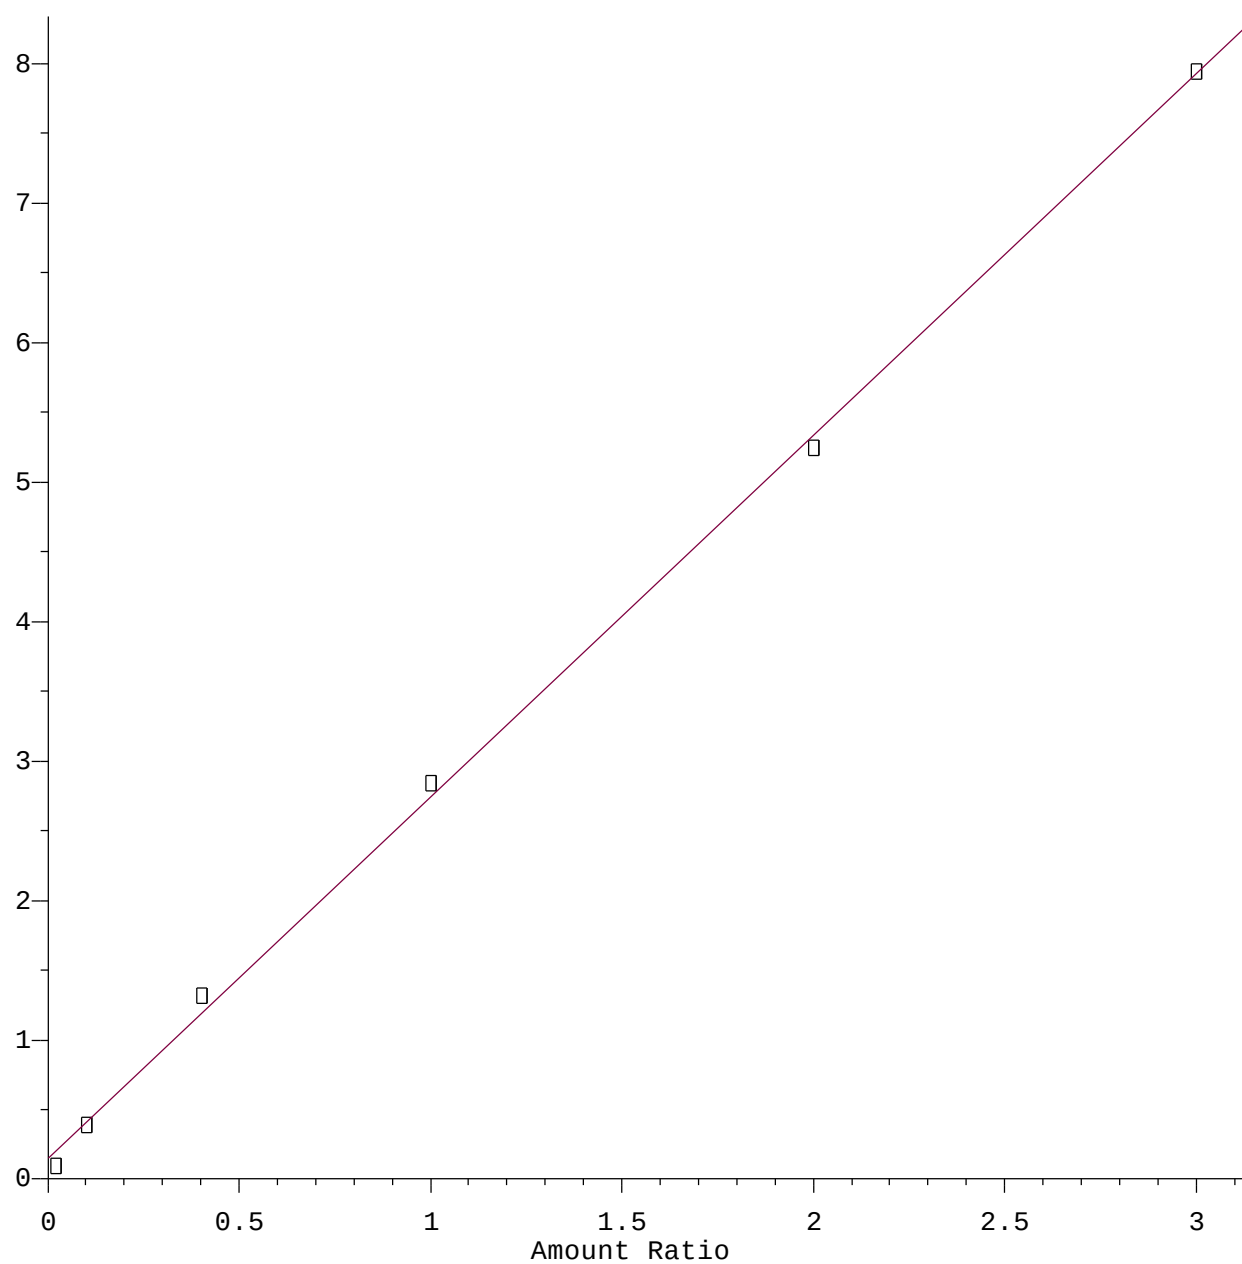


Resp Ratio = 2.59e+000 * Amt + 1.51e-001
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N061919W.M
Calibration Table Last Updated: Fri Jun 21 03:45:40 2019


1,2,4-Trichlorobenzene

Response Ratio

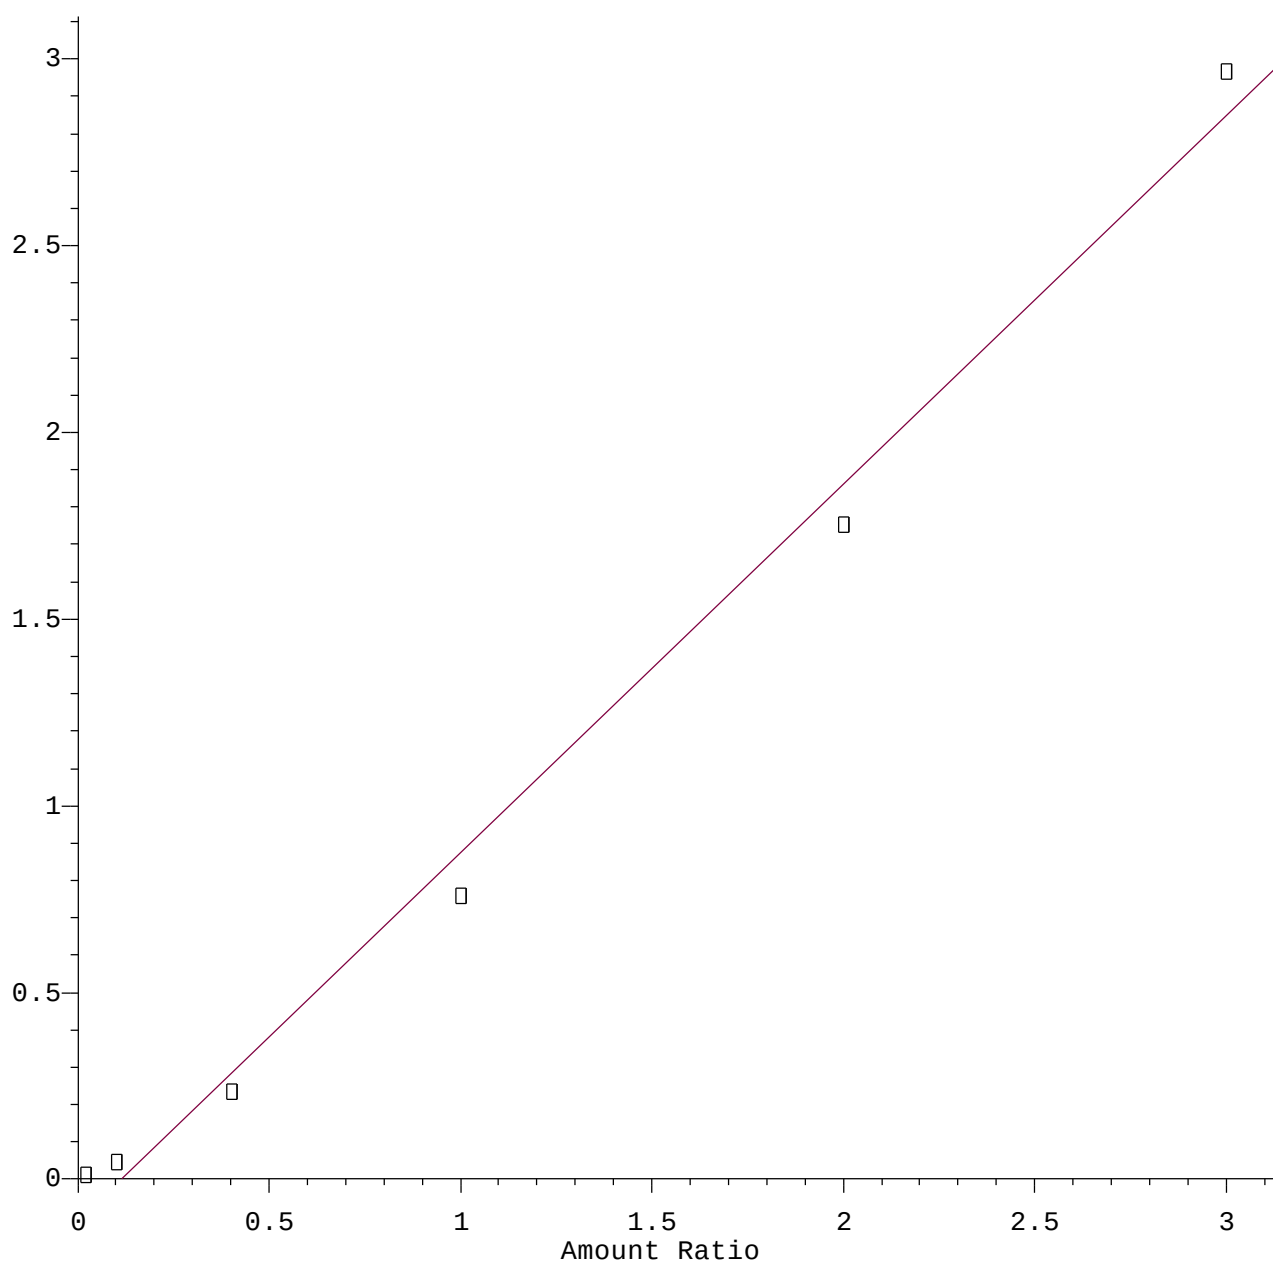

Resp Ratio = $9.86e-001 * \text{Amt} - 1.11e-001$
Coef of Det (r^2) = 0.992 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N061919W.M
Calibration Table Last Updated: Fri Jun 21 03:45:40 2019

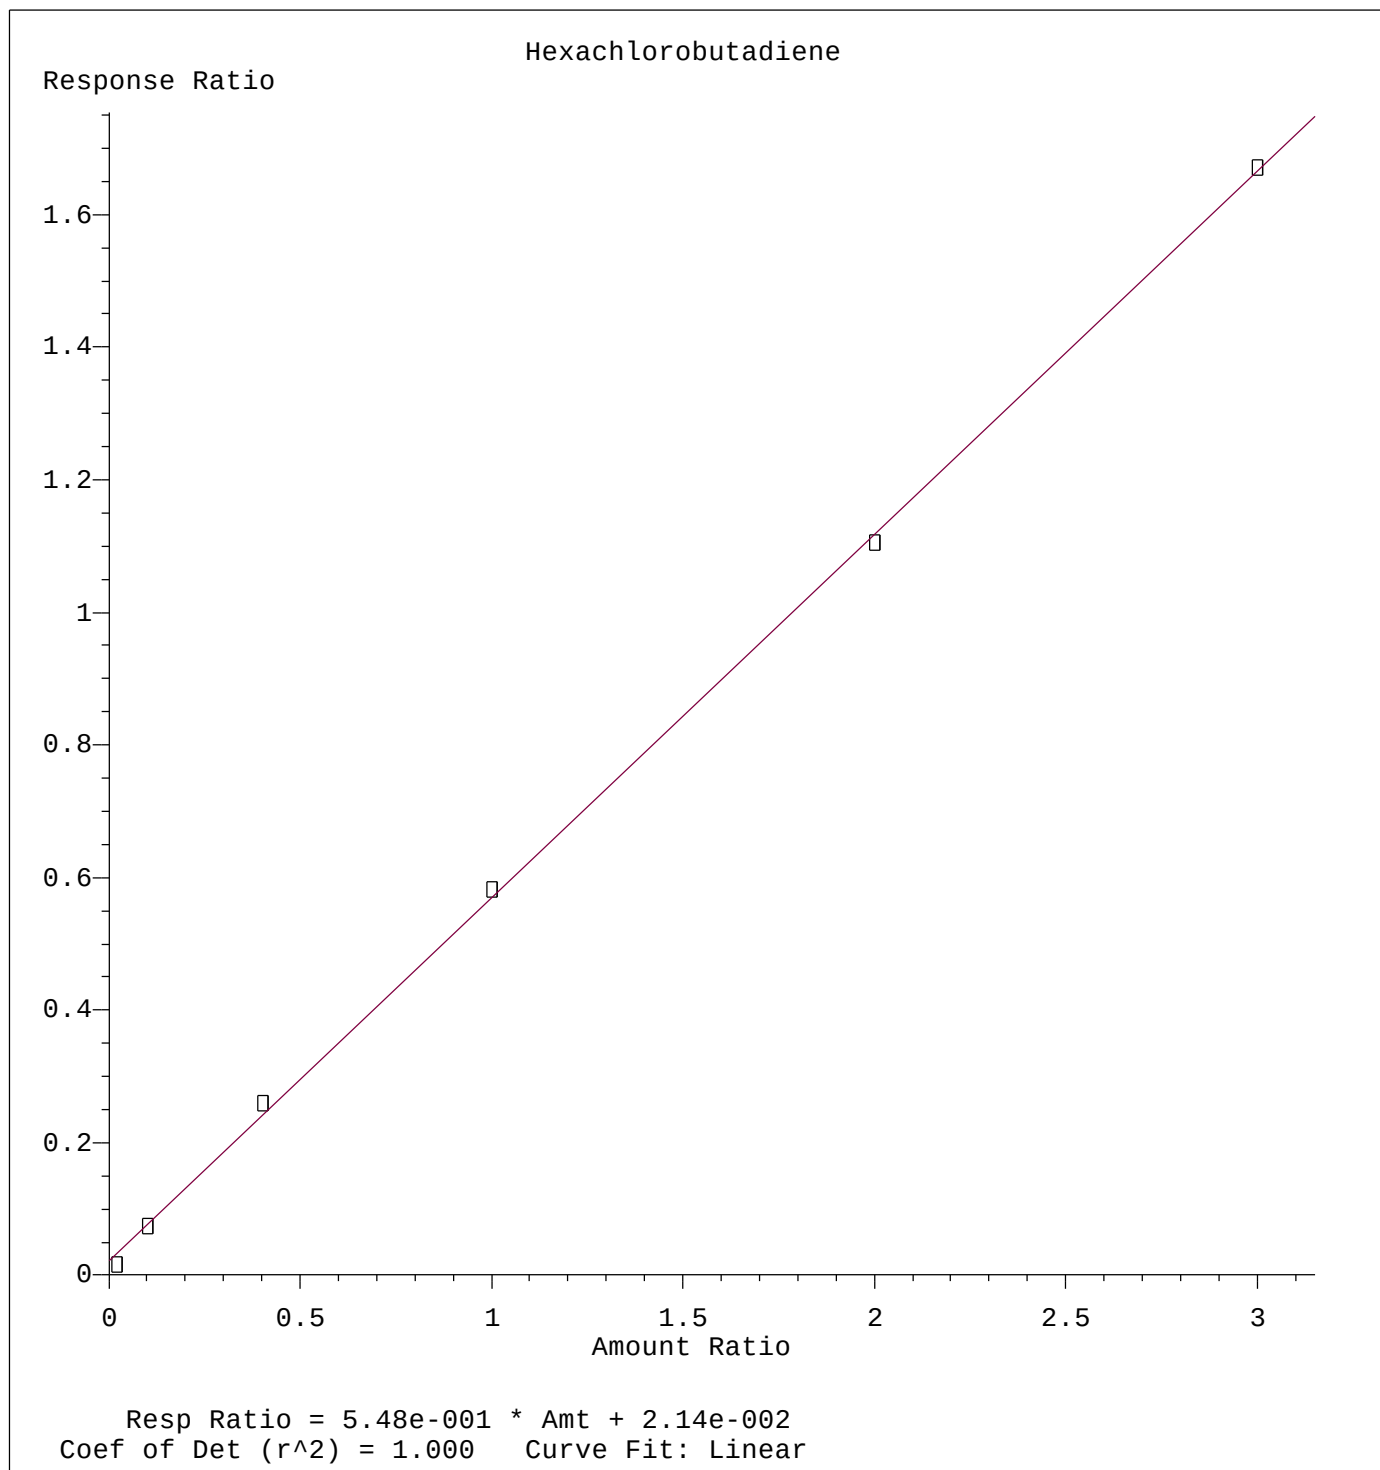

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N061919W.M
Calibration Table Last Updated: Fri Jun 21 03:45:40 2019

Naphthalene

Response Ratio

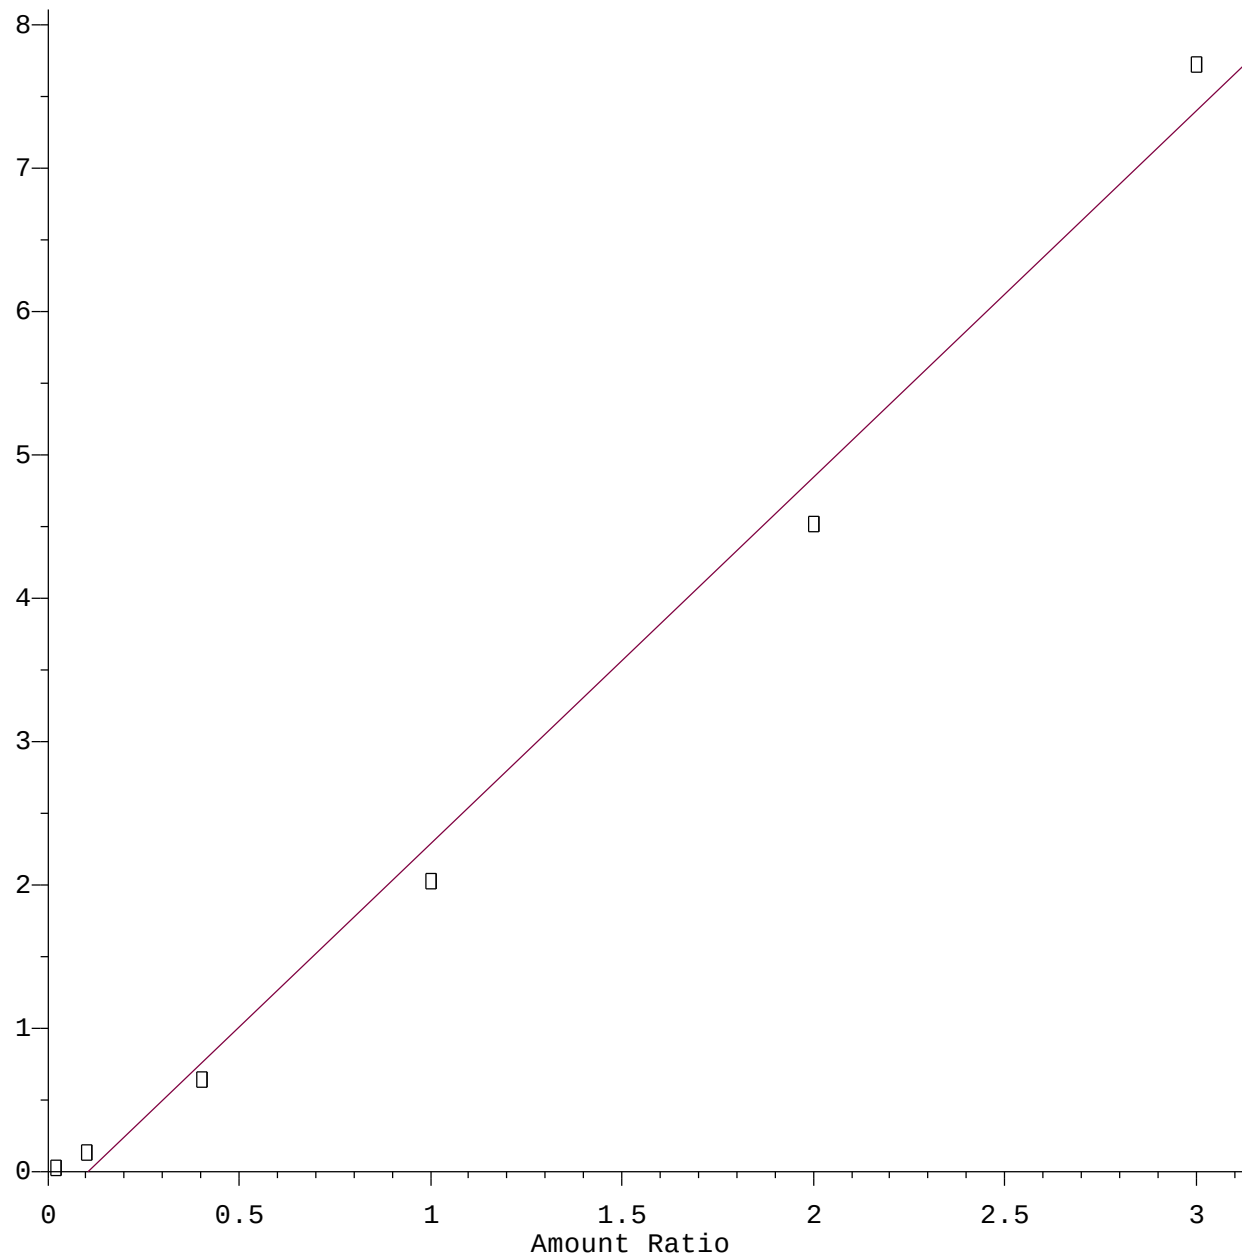


Resp Ratio = 2.56×10^0 * Amt - 2.68×10^{-1}
Coef of Det (r^2) = 0.992 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N061919W.M
Calibration Table Last Updated: Fri Jun 21 03:45:40 2019


1,2,3-Trichlorobenzene

Response Ratio

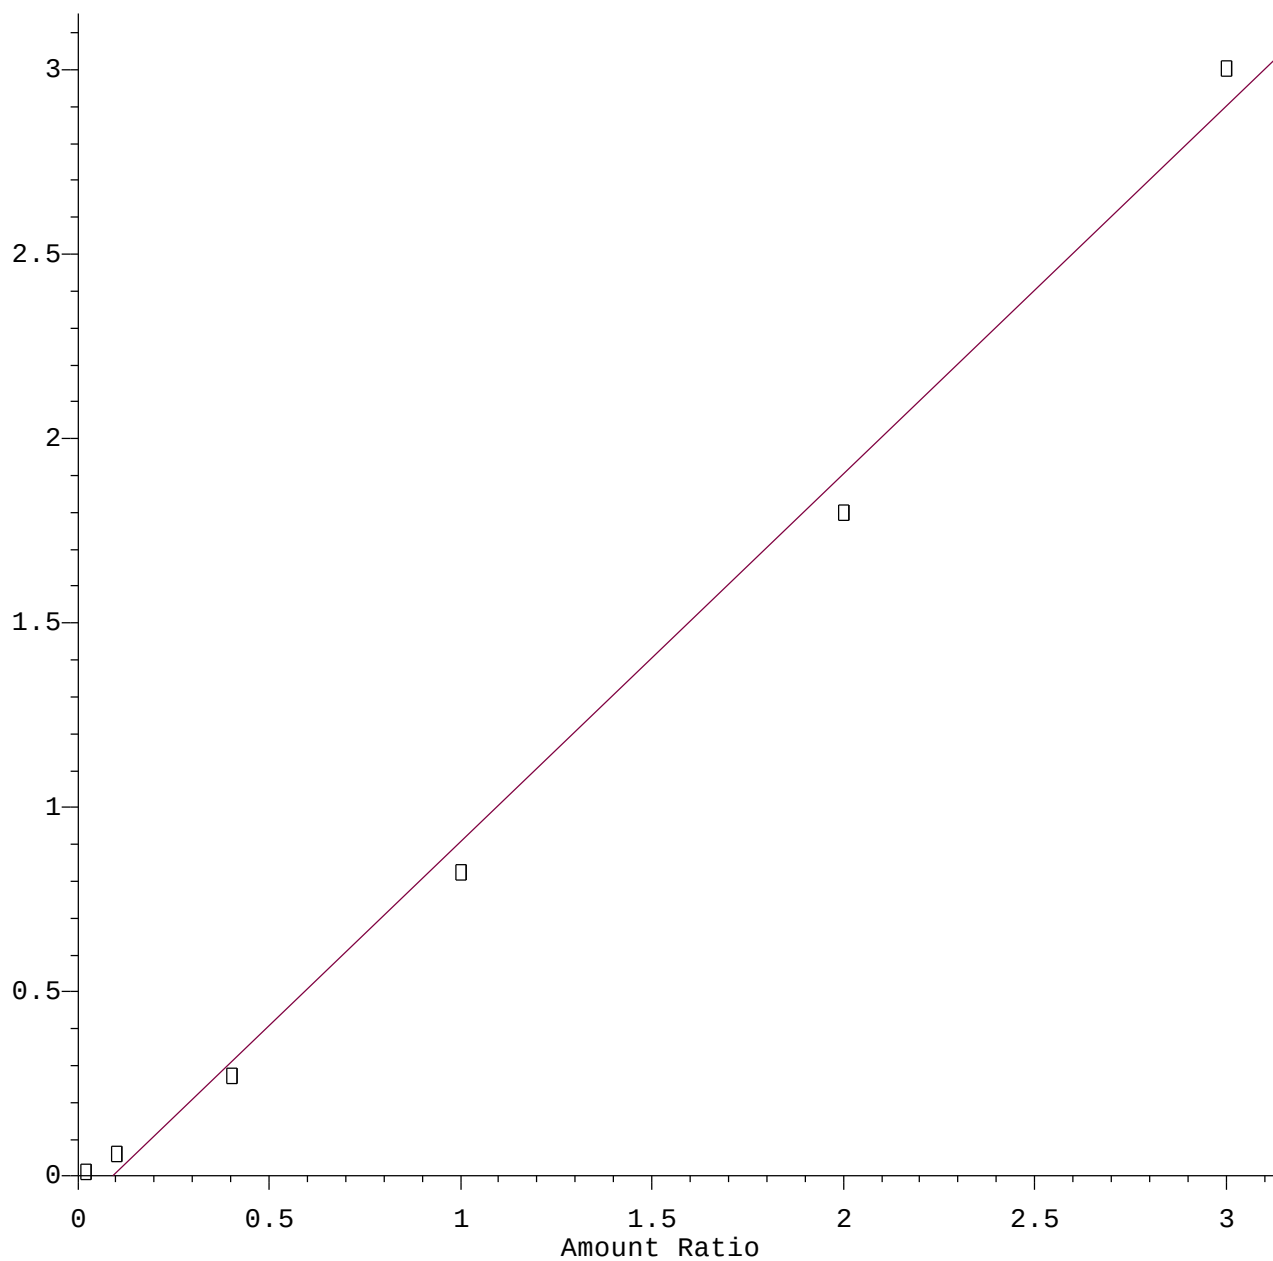

Resp Ratio = $9.96 \times 10^{-1} \times \text{Amt} - 8.93 \times 10^{-2}$
Coef of Det (r^2) = 0.994 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N061919W.M
Calibration Table Last Updated: Fri Jun 21 03:45:40 2019

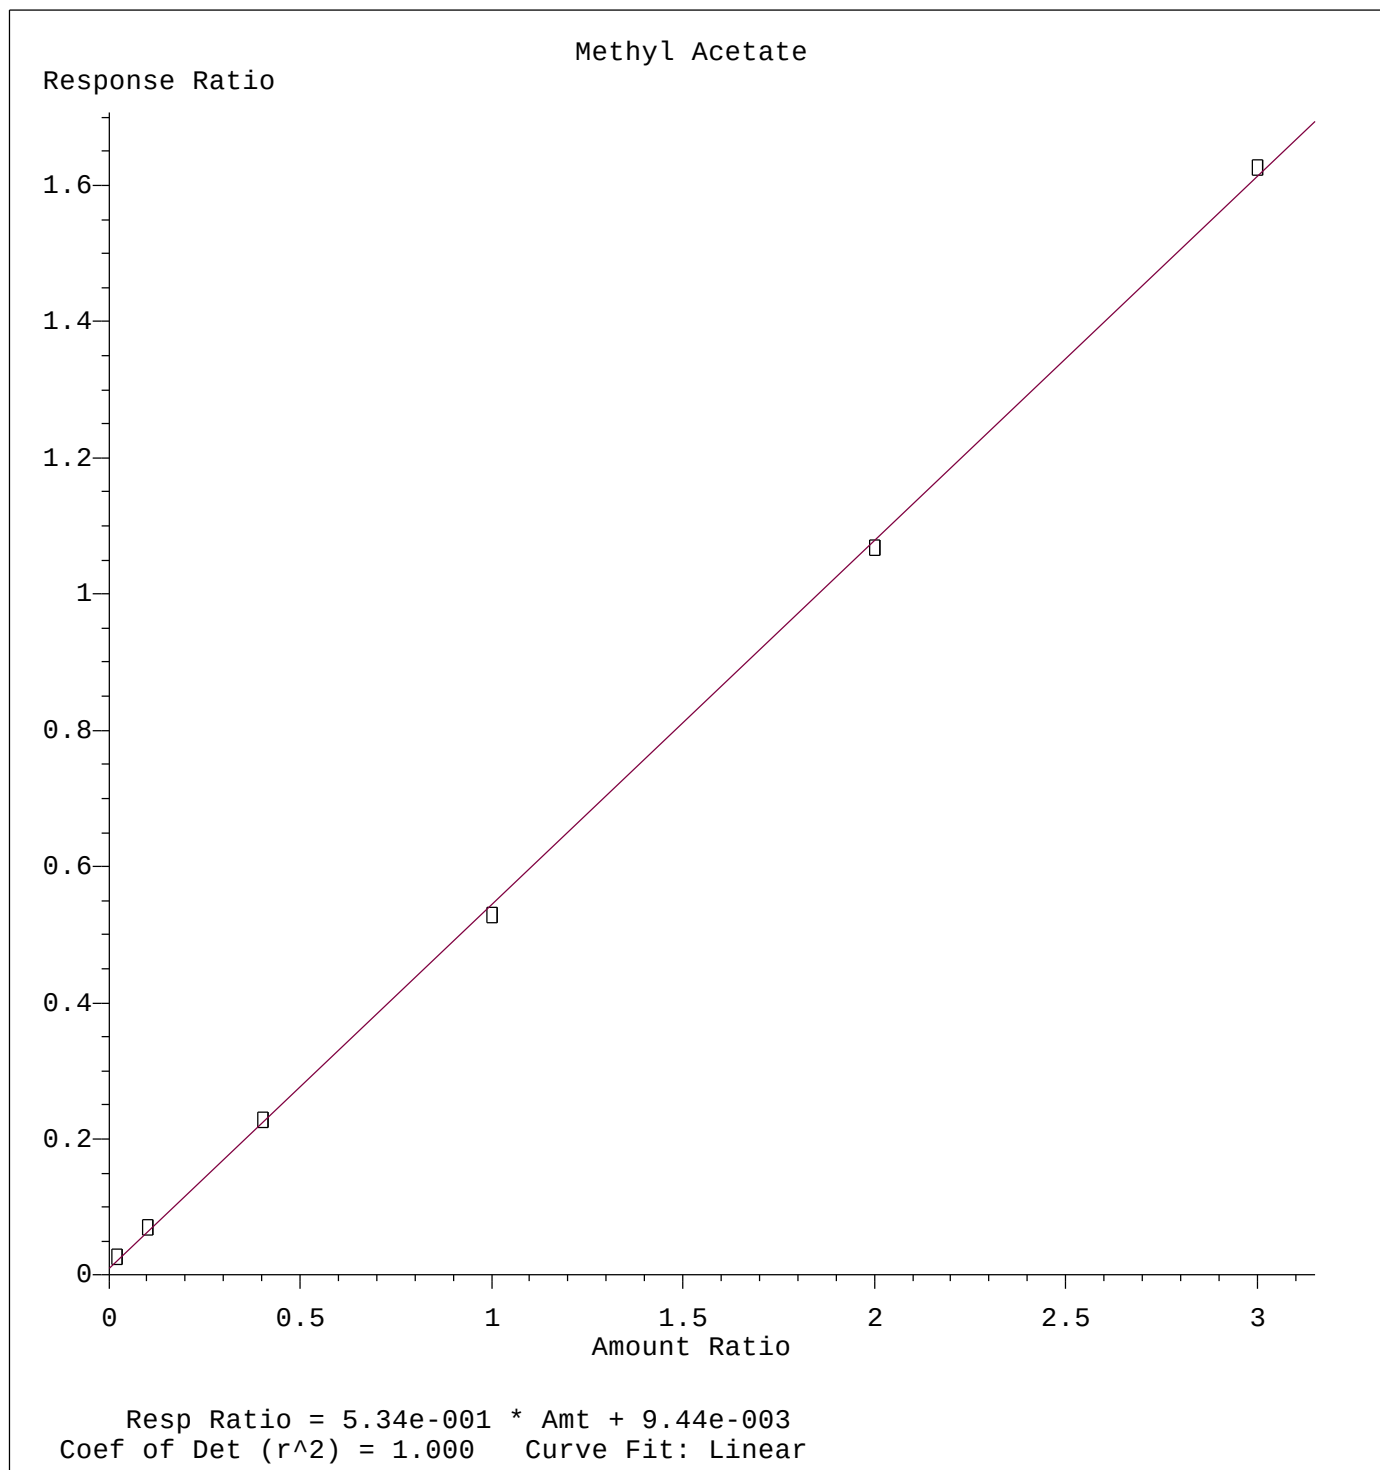

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N061919W.M
Calibration Table Last Updated: Fri Jun 21 03:45:40 2019