

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN061923\
 Data File : VN078271.D
 Acq On : 19 Jun 2023 11:37
 Operator : JC\MD
 Sample : VN0619MBL01
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN0619MBL01

Quant Time: Jun 19 16:02:29 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N060623W.M
 Quant Title : SW846 8260
 QLast Update : Wed Jun 07 05:05:00 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.235	168	427697	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.106	114	782070	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.870	117	696489	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.800	152	217128	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.588	65	304319	53.366	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery = 106.740%			
35) Dibromofluoromethane	8.177	113	275844	55.783	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery = 111.560%			
50) Toluene-d8	10.570	98	908860	47.676	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery = 95.360%			
62) 4-Bromofluorobenzene	12.859	95	283189	47.785	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery = 95.580%			
Target Compounds						
					Qvalue	
3) Chloromethane	2.371	50	970	Below Cal	#	72
5) Bromomethane	2.983	94	2706	0.566	ug/l #	55
10) Methyl Iodide	4.600	142	1717	0.268	ug/l #	71
13) Acrolein	4.206	56	720	0.830	ug/l	93
15) Acrylonitrile	5.747	53	1796	0.885	ug/l #	67
16) Acetone	4.430	43	465	0.283	ug/l #	40
17) Carbon Disulfide	4.718	76	3551	0.295	ug/l #	75
18) Methyl Acetate	5.053	43	2041	0.270	ug/l #	57
31) Cyclohexane	8.235	56	11223	1.534	ug/l #	38
36) 1,1-Dichloropropene	8.229	75	37526	5.291	ug/l #	47
38) Carbon Tetrachloride	8.235	117	46131	6.159	ug/l #	14
43) Isopropyl Acetate	8.735	43	8897	0.840	ug/l #	49
49) 1,4-Dioxane	9.706	88	55	0.588	ug/l #	1
51) 4-Methyl-2-Pentanone	10.459	43	2333	0.418	ug/l #	63
59) 2-Hexanone	11.194	43	3067	0.789	ug/l	83
75) 1,1,2,2-Tetrachloroethane	12.947	83	1265	Below Cal	#	81
76) 1,2,3-Trichloropropane	12.853	75	154969	30.191	ug/l #	1
77) Bromobenzene	12.988	156	1335	0.280	ug/l	72
81) trans-1,4-Dichloro-2-b...	12.853	75	154969	92.756	ug/l #	15
82) 4-Chlorotoluene	13.223	91	3634	0.270	ug/l	99
85) sec-Butylbenzene	13.617	105	4099	0.217	ug/l	90
87) 1,3-Dichlorobenzene	13.741	146	3018	0.374	ug/l	95
88) 1,4-Dichlorobenzene	13.741	146	3018	0.388	ug/l	98
89) n-Butylbenzene	14.059	91	5295	0.437	ug/l	90
91) 1,2-Dichlorobenzene	14.106	146	3085	0.392	ug/l	95
92) 1,2-Dibromo-3-Chloropr...	14.735	75	724	0.712	ug/l #	41
93) 1,2,4-Trichlorobenzene	15.400	180	3027	1.078	ug/l	93
94) Hexachlorobutadiene	15.505	225	2697	Below Cal		92
95) Naphthalene	15.641	128	10435	1.105	ug/l #	90
96) 1,2,3-Trichlorobenzene	15.841	180	3352	1.068	ug/l	80


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN061923\
Data File : VN078271.D
Acq On : 19 Jun 2023 11:37
Operator : JC\MD
Sample : VN0619MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN0619MBL01

Quant Time: Jun 19 16:02:29 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N060623W.M
Quant Title : SW846 8260
QLast Update : Wed Jun 07 05:05:00 2023
Response via : Initial Calibration




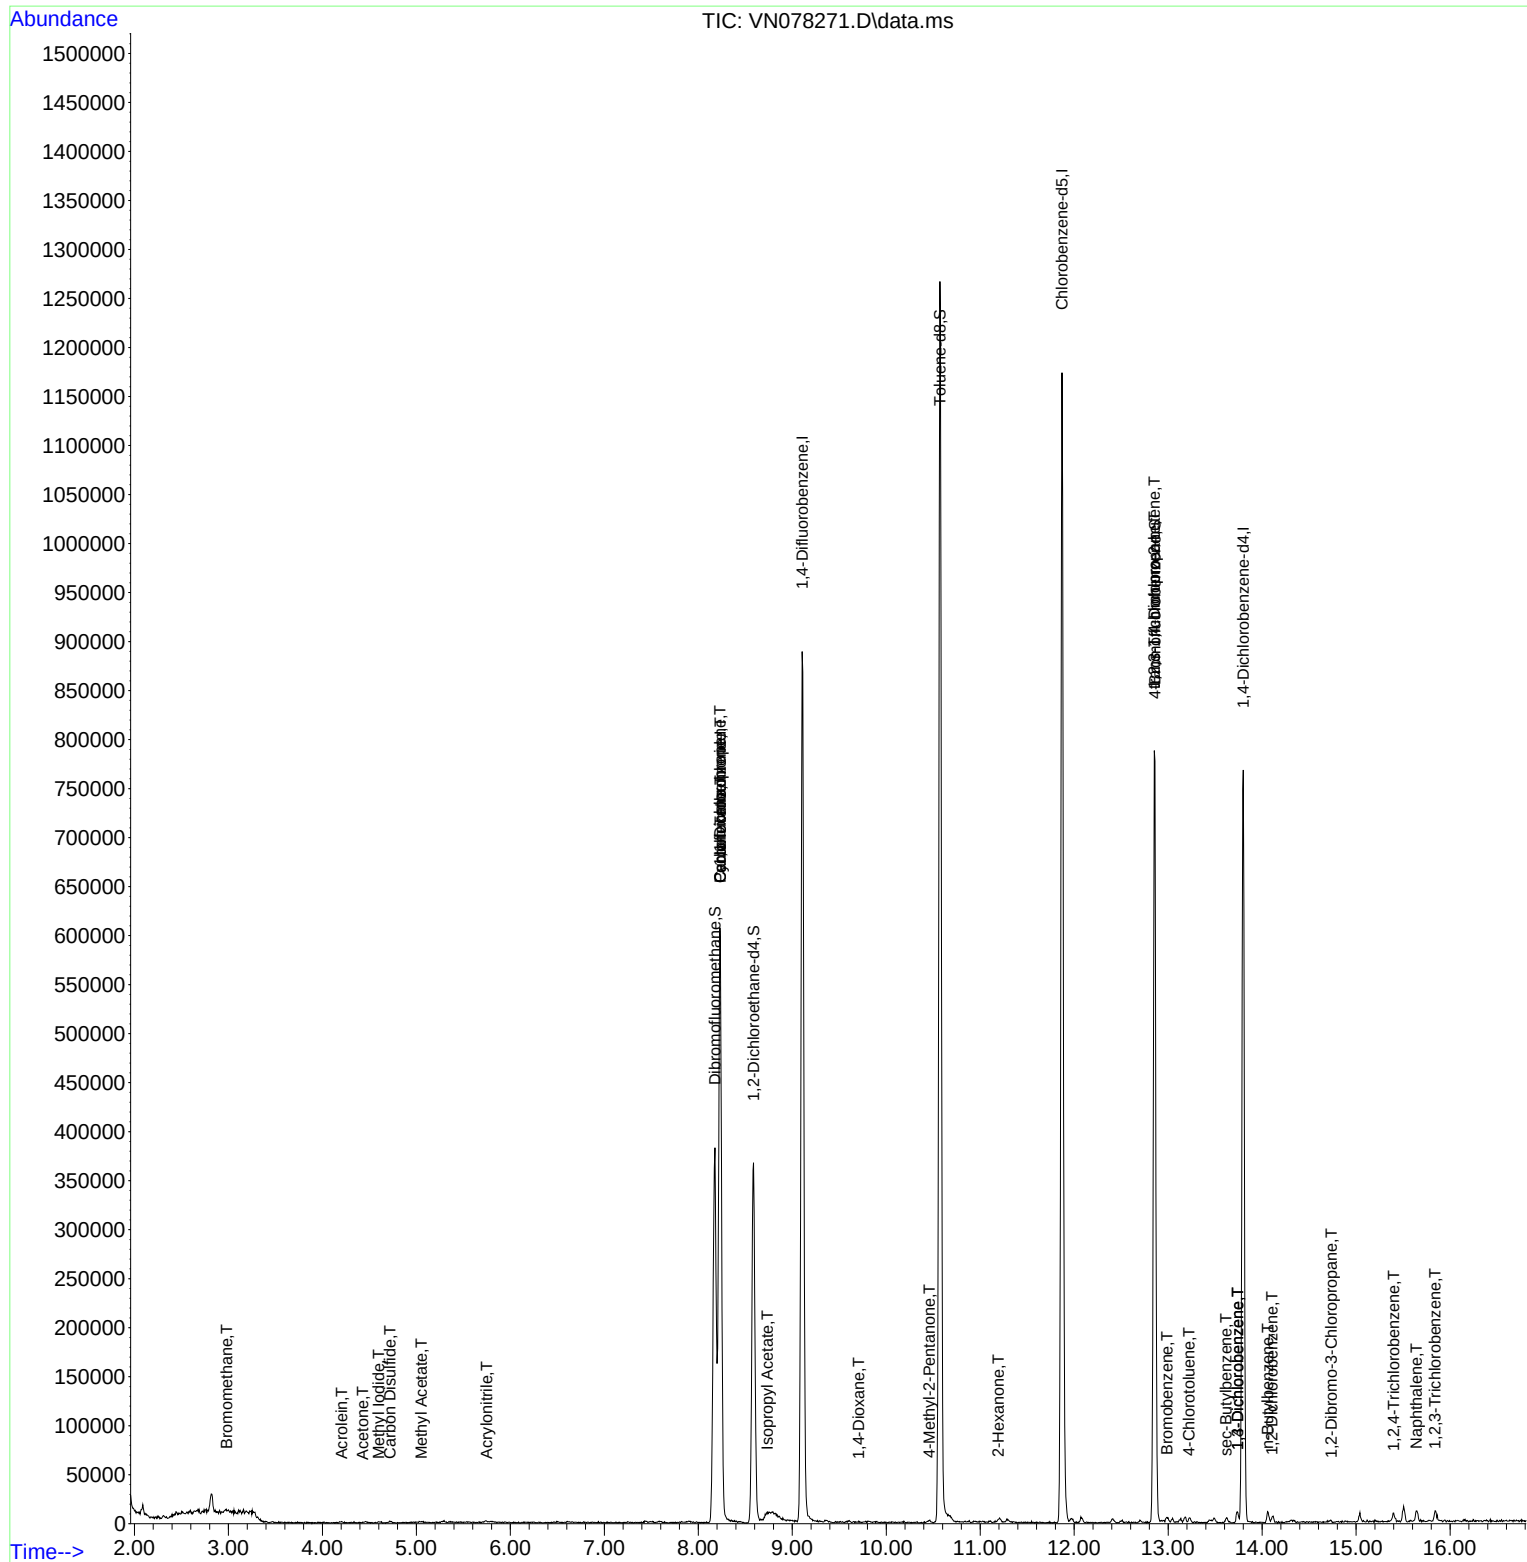




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.235 min Scan# 1068
Delta R.T. 0.000 min
Lab File: VN078271.D
Acq: 19 Jun 2023 11:37




Instrument :
MSVOA_N
ClientSampleId :
VN0619MBL01


Tgt Ion:168 Resp: 427697
Ion Ratio Lower Upper
168 100
99 60.7 53.0 79.6

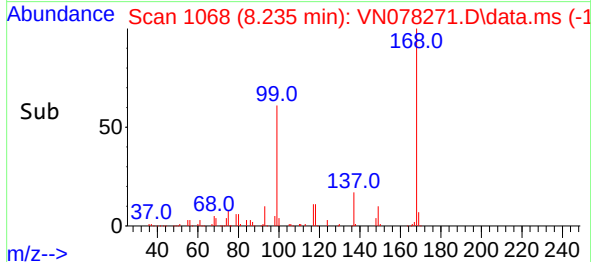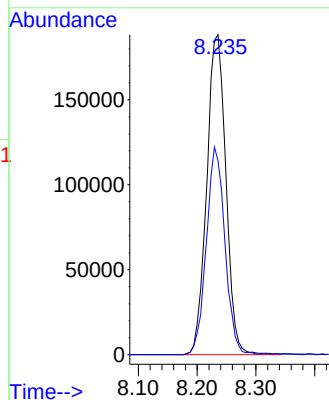

#3
Chloromethane
Concen: Below Cal
RT: 2.371 min Scan# 71
Delta R.T. 0.000 min
Lab File: VN078271.D
Acq: 19 Jun 2023 11:37

Tgt Ion: 50 Resp: 970
Ion Ratio Lower Upper
50 100
52 49.1 26.5 39.7#



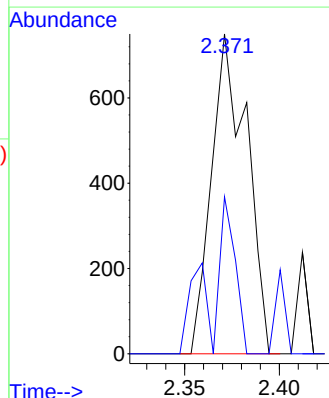





#5
Bromomethane
Concen: 0.566 ug/l
RT: 2.983 min Scan# 11
Delta R.T. 0.029 min
Lab File: VN078271.D
Acq: 19 Jun 2023 11:37




Instrument :
MSVOA_N
ClientSampleId :
VN0619MBL01


Tgt Ion: 94 Resp: 2706
Ion Ratio Lower Upper
94 100
96 48.4 73.1 109.7#

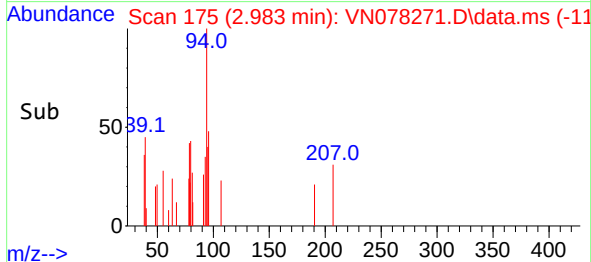

#10
Methyl Iodide
Concen: 0.268 ug/l
RT: 4.600 min Scan# 450
Delta R.T. 0.006 min
Lab File: VN078271.D
Acq: 19 Jun 2023 11:37

Tgt Ion: 142 Resp: 1717
Ion Ratio Lower Upper
142 100
127 65.1 37.6 56.4#
141 0.0 11.4 17.0#


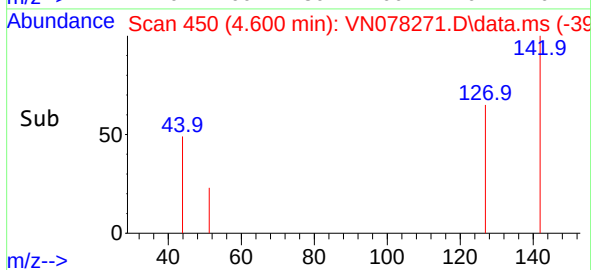






#13
Acrolein
Concen: 0.830 ug/l
RT: 4.206 min Scan# 31
Delta R.T. 0.018 min
Lab File: VN078271.D
Acq: 19 Jun 2023 11:37




Instrument :
MSVOA_N
ClientSampleId :
VN0619MBL01


Tgt Ion: 56 Resp: 720
Ion Ratio Lower Upper
56 100
55 62.4 54.5 81.7

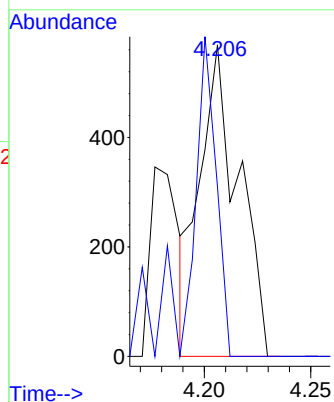

#15
Acrylonitrile
Concen: 0.885 ug/l
RT: 5.747 min Scan# 645
Delta R.T. 0.018 min
Lab File: VN078271.D
Acq: 19 Jun 2023 11:37

Tgt Ion: 53 Resp: 1796
Ion Ratio Lower Upper
53 100
52 45.2 65.3 97.9#
51 27.7 28.9 43.3#


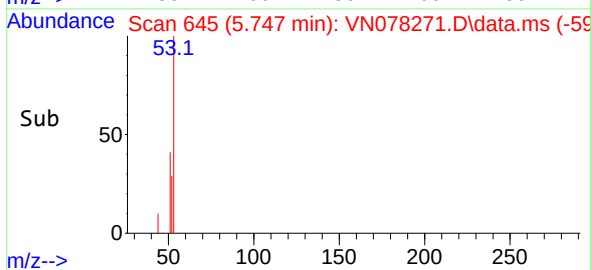
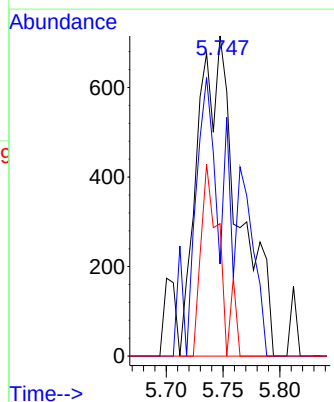





#16
Acetone
Concen: 0.283 ug/l
RT: 4.430 min Scan# 41
Delta R.T. -0.006 min
Lab File: VN078271.D
Acq: 19 Jun 2023 11:37




Instrument :
MSVOA_N
ClientSampleId :
VN0619MBL01


Tgt Ion: 43 Resp: 465
Ion Ratio Lower Upper
43 100
58 0.0 28.0 42.0#

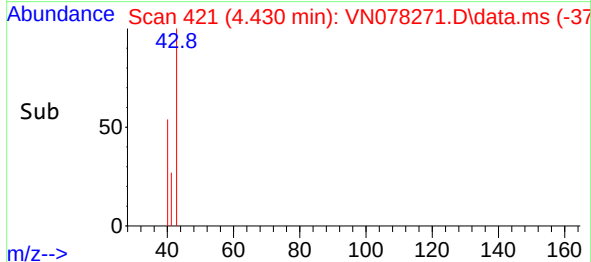

#17
Carbon Disulfide
Concen: 0.295 ug/l
RT: 4.718 min Scan# 470
Delta R.T. -0.000 min
Lab File: VN078271.D
Acq: 19 Jun 2023 11:37

Tgt Ion: 76 Resp: 3551
Ion Ratio Lower Upper
76 100
78 0.0 7.4 11.0#



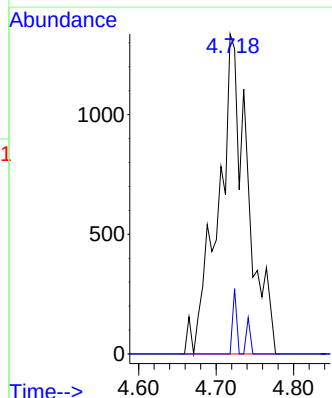



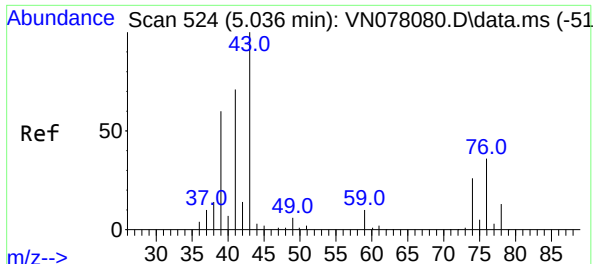

#18
Methyl Acetate
Concen: 0.270 ug/l
RT: 5.053 min Scan# 51
Delta R.T. 0.018 min
Lab File: VN078271.D
Acq: 19 Jun 2023 11:37




Instrument :
MSVOA_N
ClientSampleId :
VN0619MBL01


Tgt Ion: 43 Resp: 2041
Ion Ratio Lower Upper
43 100
74 8.3 26.2 39.4#

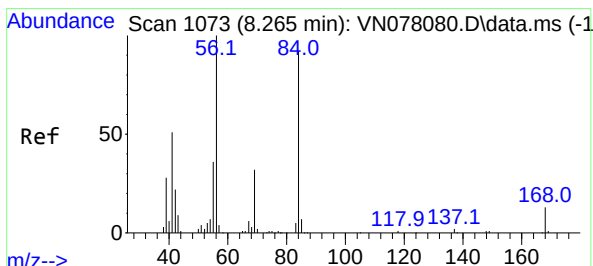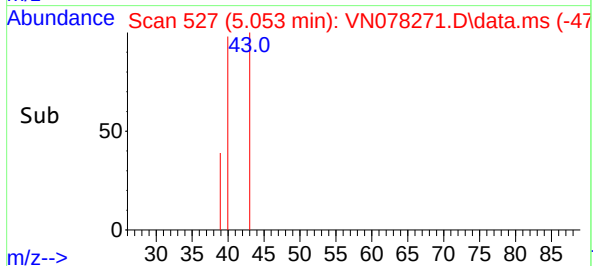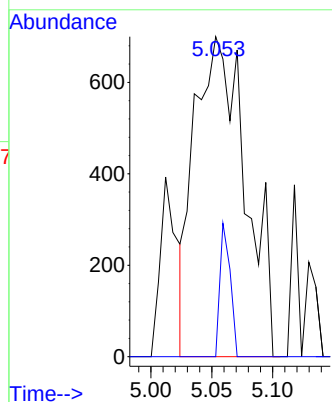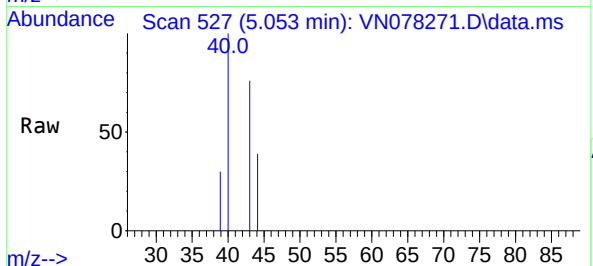

#31
Cyclohexane
Concen: 1.534 ug/l
RT: 8.235 min Scan# 1068
Delta R.T. -0.029 min
Lab File: VN078271.D
Acq: 19 Jun 2023 11:37

Tgt Ion: 56 Resp: 11223
Ion Ratio Lower Upper
56 100
69 140.2 26.8 40.2#
84 123.5 81.8 122.6#

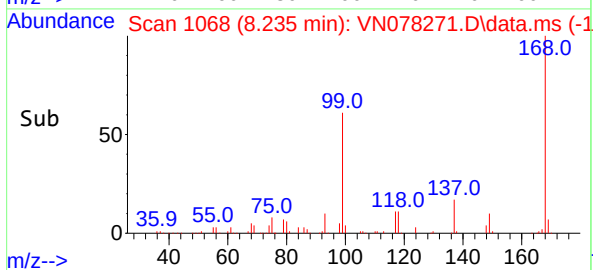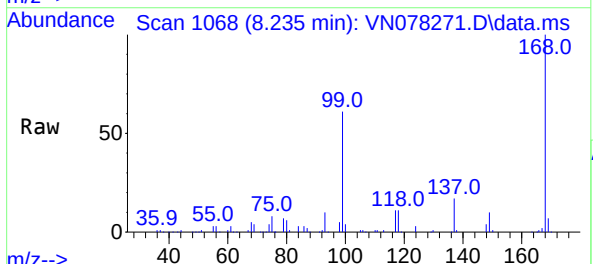

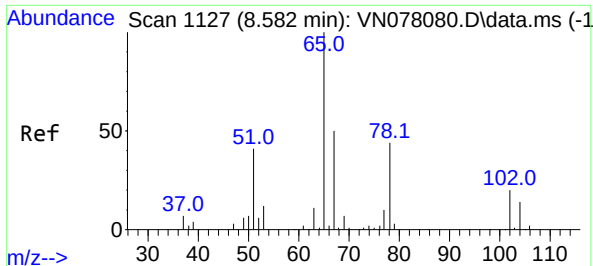

#33

1,2-Dichloroethane-d4

Concen: 53.366 ug/l

RT: 8.588 min Scan# 1127

Delta R.T. 0.006 min

Lab File: VN078271.D

Acq: 19 Jun 2023 11:37

Instrument :

MSVOA_N

ClientSampleId :





VN0619MBL01

Tgt Ion: 65 Resp: 304319

Ion Ratio Lower Upper

65 100

67 52.3 0.0 106.6

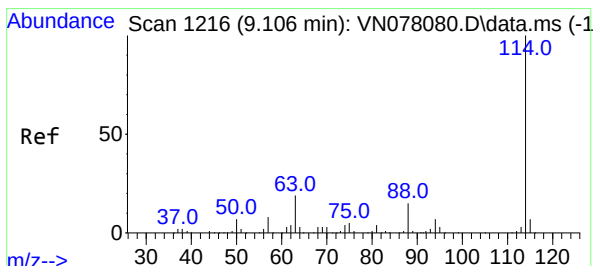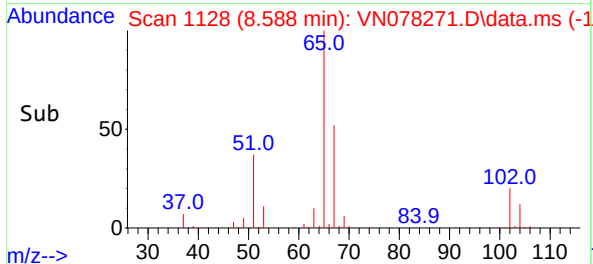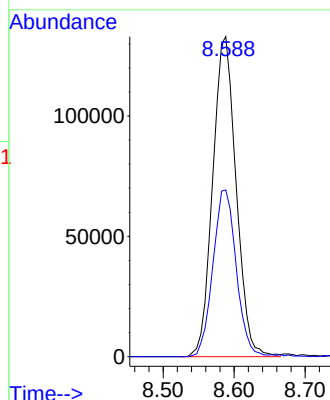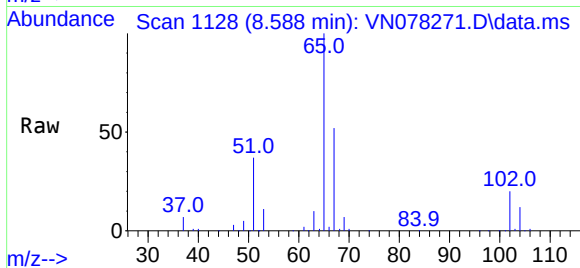

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.106 min Scan# 1216

Delta R.T. -0.000 min

Lab File: VN078271.D

Acq: 19 Jun 2023 11:37




Tgt Ion: 114 Resp: 782070


Ion Ratio Lower Upper

114 100

63 19.0 0.0 36.4

88 14.5 0.0 30.6


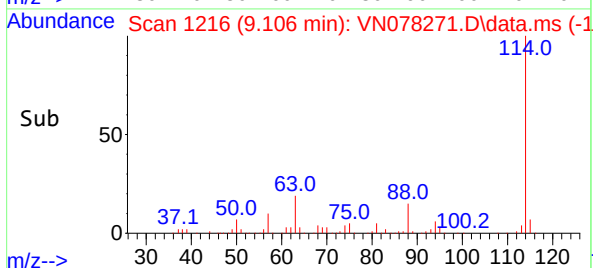
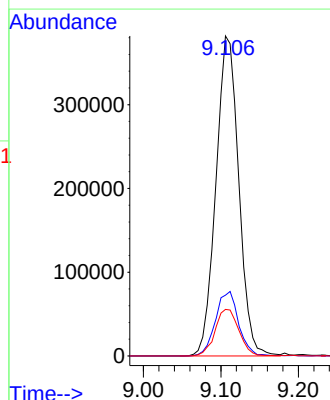
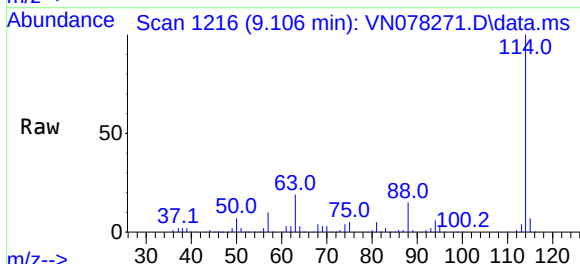


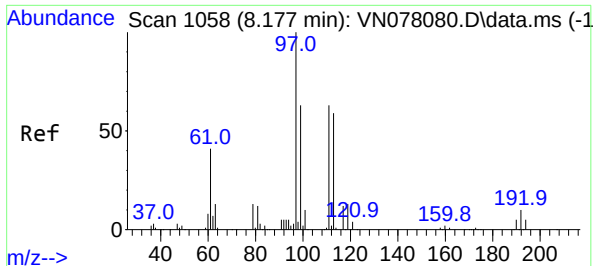

#35
Dibromofluoromethane
Concen: 55.783 ug/l
RT: 8.177 min Scan# 1058
Delta R.T. -0.000 min
Lab File: VN078271.D
Acq: 19 Jun 2023 11:37




Instrument :
MSVOA_N
ClientSampleId :
VN0619MBL01


Tgt Ion:113 Resp: 275844
Ion Ratio Lower Upper
113 100
111 103.6 82.6 123.8
192 16.7 12.7 19.1

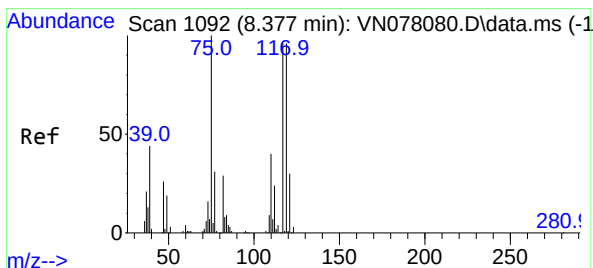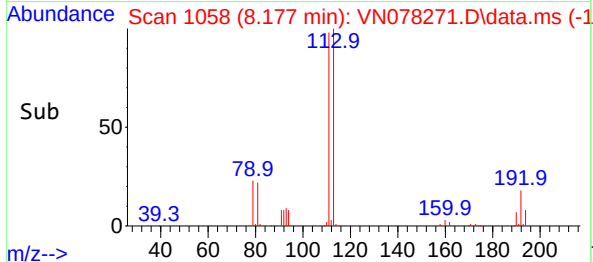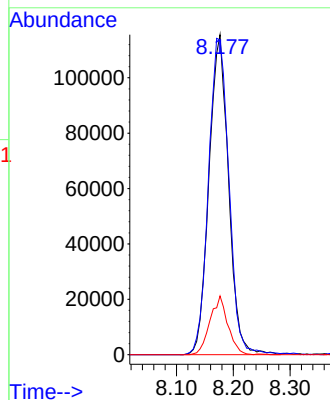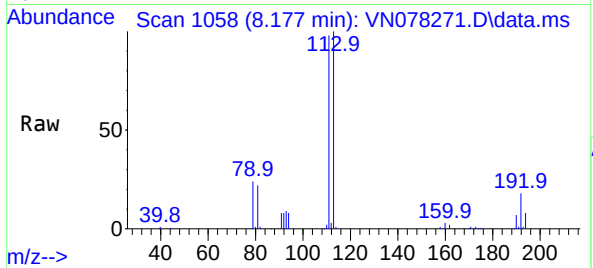

#36
1,1-Dichloropropene
Concen: 5.291 ug/l
RT: 8.229 min Scan# 1067
Delta R.T. -0.147 min
Lab File: VN078271.D
Acq: 19 Jun 2023 11:37


Tgt Ion: 75 Resp: 37526
Ion Ratio Lower Upper
75 100
110 7.6 19.1 57.3#
77 0.0 25.0 37.4#

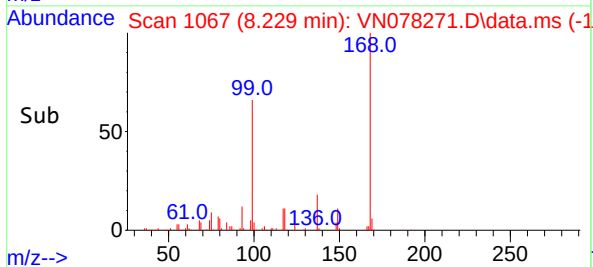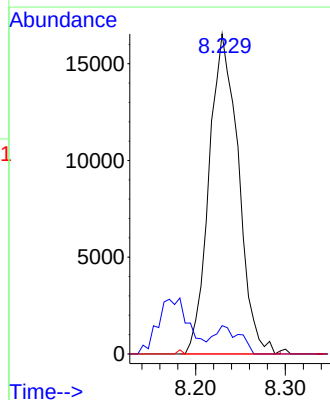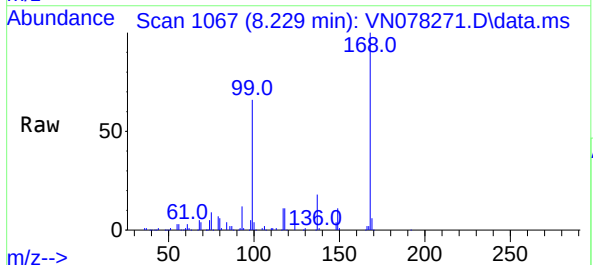



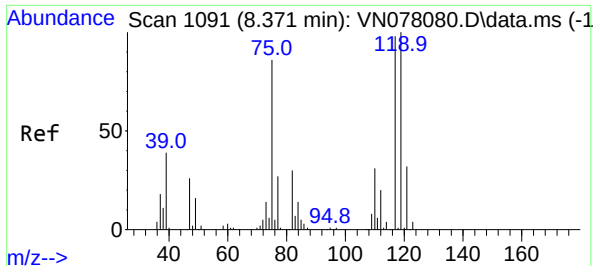


#38
Carbon Tetrachloride
Concen: 6.159 ug/l
RT: 8.235 min Scan# 1107
Delta R.T. -0.135 min
Lab File: VN078271.D
Acq: 19 Jun 2023 11:37

Instrument :
MSVOA_N
ClientSampleId :
VN0619MBL01



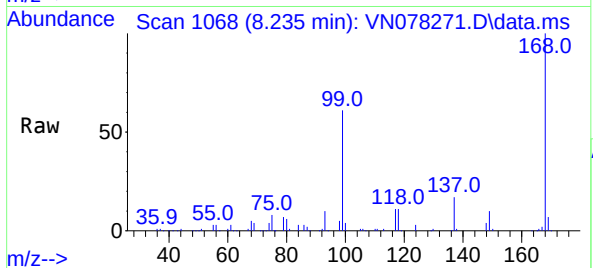



Tgt Ion:117 Resp: 46131
Ion Ratio Lower Upper
117 100
119 2.6 77.3 115.9#
121 0.0 23.3 34.9#

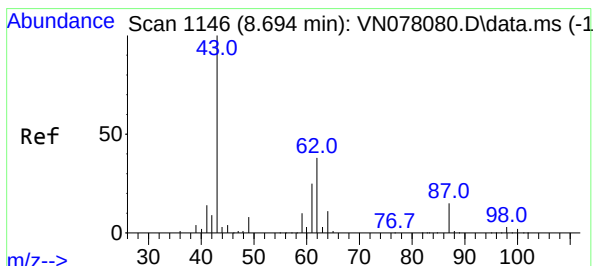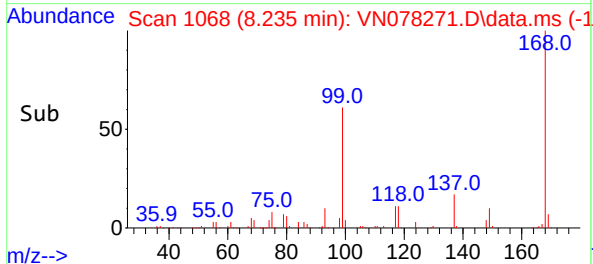

#43
Isopropyl Acetate
Concen: 0.840 ug/l
RT: 8.735 min Scan# 1153
Delta R.T. 0.041 min
Lab File: VN078271.D
Acq: 19 Jun 2023 11:37

Tgt Ion: 43 Resp: 8897
Ion Ratio Lower Upper
43 100
61 0.0 24.7 37.1#
87 0.0 14.6 21.8#


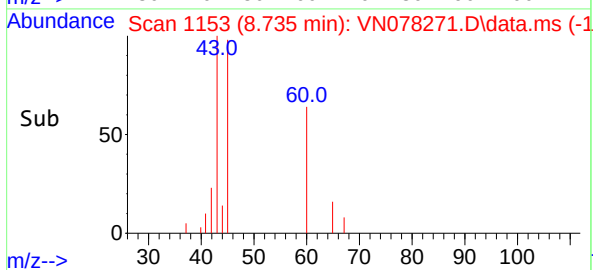

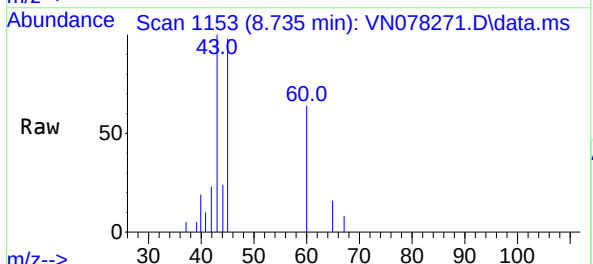


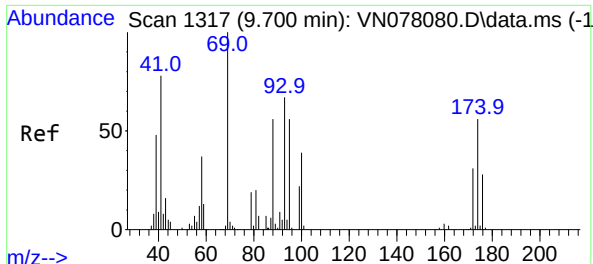

#49
1,4-Dioxane
Concen: 0.588 ug/l
RT: 9.706 min Scan# 11
Delta R.T. 0.006 min
Lab File: VN078271.D
Acq: 19 Jun 2023 11:37




Instrument :
MSVOA_N
ClientSampleId :
VN0619MBL01


Tgt Ion: 88 Resp: 55
Ion Ratio Lower Upper
88 100
43 760.0 17.0 25.6#
58 110.9 47.0 70.4#

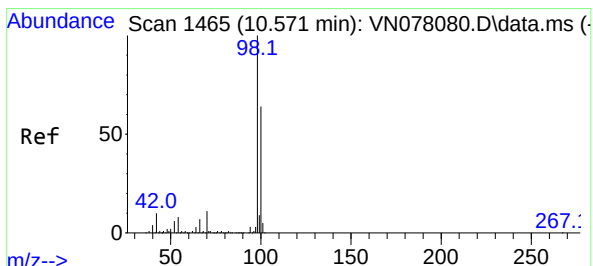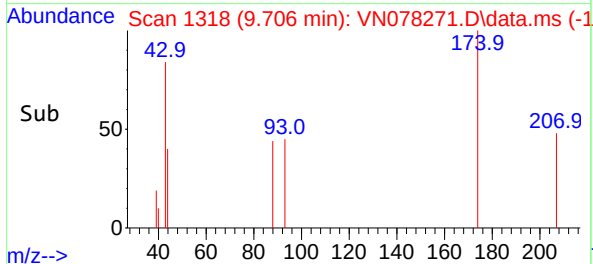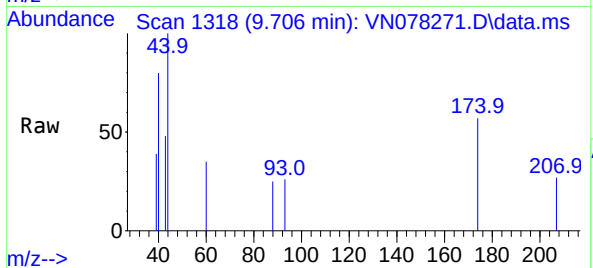

#50
Toluene-d8
Concen: 47.676 ug/l
RT: 10.570 min Scan# 1465
Delta R.T. -0.000 min
Lab File: VN078271.D
Acq: 19 Jun 2023 11:37

Tgt Ion: 98 Resp: 908860
Ion Ratio Lower Upper
98 100
100 62.6 52.0 78.0


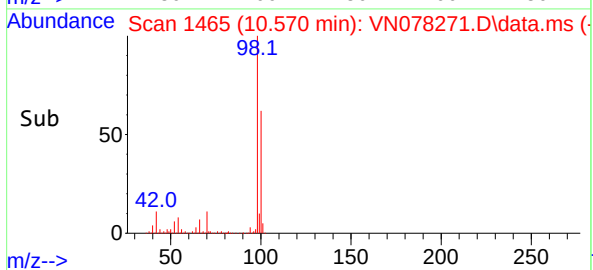

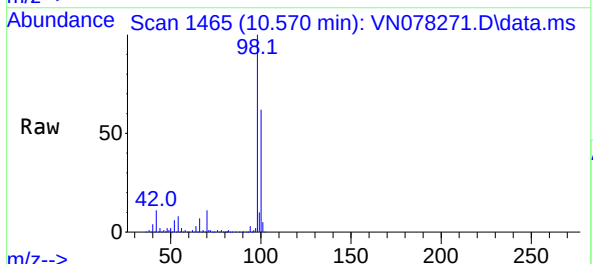




#51
4-Methyl-2-Pentanone
Concen: 0.418 ug/l
RT: 10.459 min Scan# 1445
Delta R.T. 0.006 min
Lab File: VN078271.D
Acq: 19 Jun 2023 11:37




Instrument :
MSVOA_N
ClientSampleId :
VN0619MBL01


Tgt Ion: 43 Resp: 2333
Ion Ratio Lower Upper
43 100
58 21.3 36.6 54.8#



#59
2-Hexanone
Concen: 0.789 ug/l
RT: 11.194 min Scan# 1571
Delta R.T. -0.006 min
Lab File: VN078271.D
Acq: 19 Jun 2023 11:37

Tgt Ion: 43 Resp: 3067
Ion Ratio Lower Upper
43 100
58 50.1 31.7 95.1


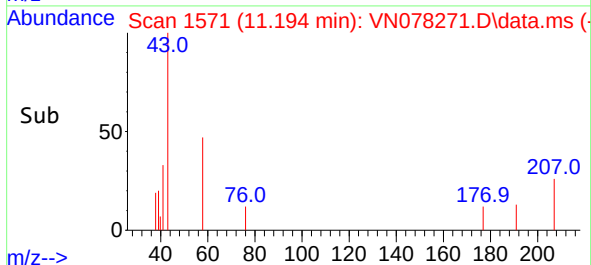
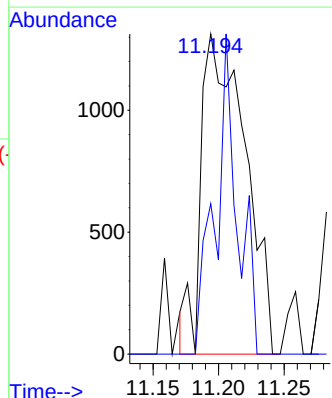
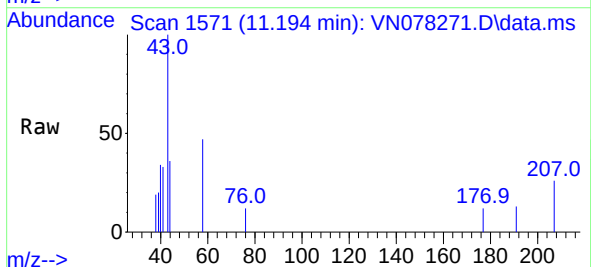




#62
4-Bromofluorobenzene
Concen: 47.785 ug/l
RT: 12.859 min Scan# 11
Delta R.T. 0.006 min
Lab File: VN078271.D
Acq: 19 Jun 2023 11:37




Instrument :
MSVOA_N
ClientSampleId :
VN0619MBL01


Tgt Ion: 95 Resp: 283189
Ion Ratio Lower Upper
95 100
174 75.9 0.0 143.8
176 72.0 0.0 135.8

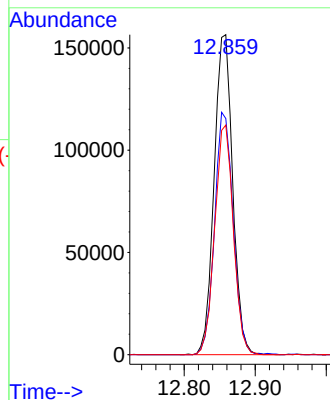

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.870 min Scan# 1686
Delta R.T. -0.000 min
Lab File: VN078271.D
Acq: 19 Jun 2023 11:37

Tgt Ion: 117 Resp: 696489
Ion Ratio Lower Upper
117 100
82 52.9 44.0 66.0
119 32.2 25.6 38.4


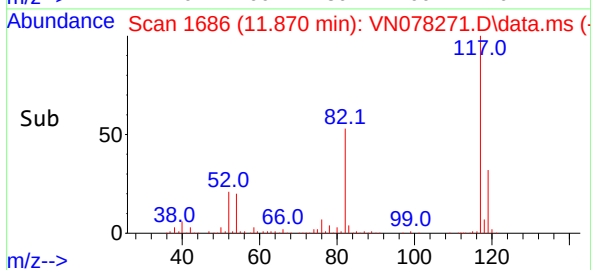
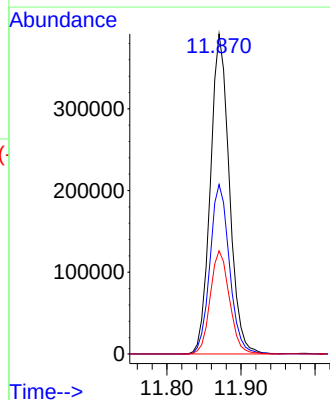





#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.800 min Scan# 20
Delta R.T. -0.000 min
Lab File: VN078271.D
Acq: 19 Jun 2023 11:37




Instrument :
MSVOA_N
ClientSampleId :
VN0619MBL01


Tgt Ion:152 Resp: 217128
Ion Ratio Lower Upper
152 100
115 59.9 32.3 96.8
150 154.3 0.0 355.8

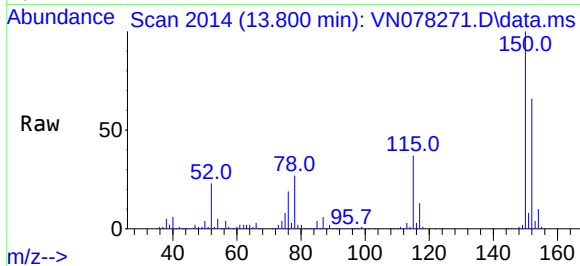

#75
1,1,2,2-Tetrachloroethane
Concen: Below Cal
RT: 12.947 min Scan# 1869
Delta R.T. 0.006 min
Lab File: VN078271.D
Acq: 19 Jun 2023 11:37

Tgt Ion: 83 Resp: 1265
Ion Ratio Lower Upper
83 100
131 0.0 5.0 15.0#
85 50.1 31.9 95.7


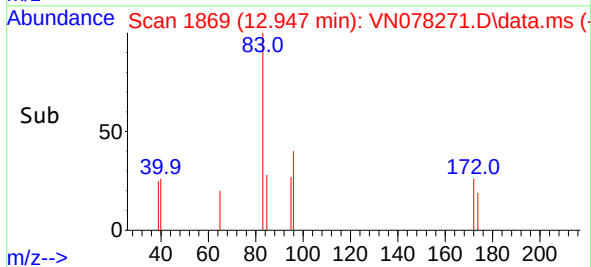

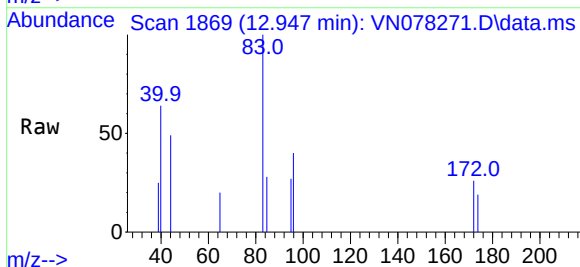




#76
1,2,3-Trichloropropane
Concen: 30.191 ug/l
RT: 12.853 min Scan# 1853
Delta R.T. -0.147 min
Lab File: VN078271.D
Acq: 19 Jun 2023 11:37




Instrument :
MSVOA_N
ClientSampleId :
VN0619MBL01


Tgt Ion: 75 Resp: 154969
Ion Ratio Lower Upper
75 100
77 0.9 84.5 253.5#

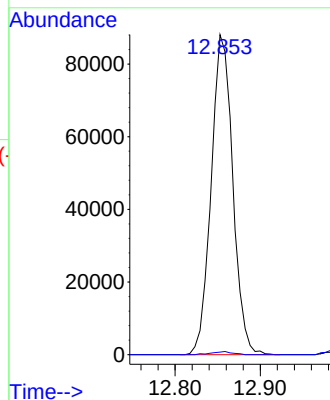

#77
Bromobenzene
Concen: 0.280 ug/l
RT: 12.988 min Scan# 1876
Delta R.T. -0.000 min
Lab File: VN078271.D
Acq: 19 Jun 2023 11:37

Tgt Ion:156 Resp: 1335
Ion Ratio Lower Upper
156 100
77 162.8 107.7 323.3
158 80.9 48.4 145.3


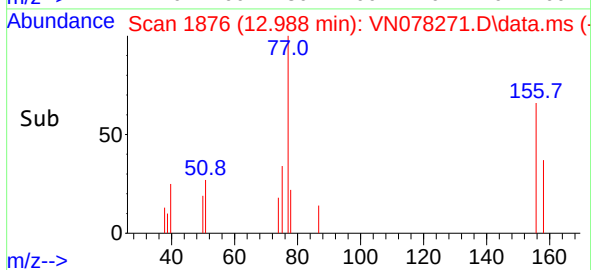
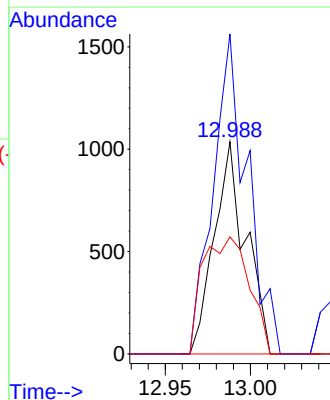





#81
trans-1,4-Dichloro-2-butene
Concen: 92.756 ug/l
RT: 12.853 min Scan# 1853
Delta R.T. 0.112 min
Lab File: VN078271.D
Acq: 19 Jun 2023 11:37




Instrument :
MSVOA_N
ClientSampleId :
VN0619MBL01


Tgt Ion: 75 Resp: 154969
Ion Ratio Lower Upper
75 100
53 0.0 67.4 101.2#
89 0.0 38.8 58.2#



#82
4-Chlorotoluene
Concen: 0.270 ug/l
RT: 13.223 min Scan# 1916
Delta R.T. -0.006 min
Lab File: VN078271.D
Acq: 19 Jun 2023 11:37

Tgt Ion: 91 Resp: 3634
Ion Ratio Lower Upper
91 100
126 34.1 16.7 50.0


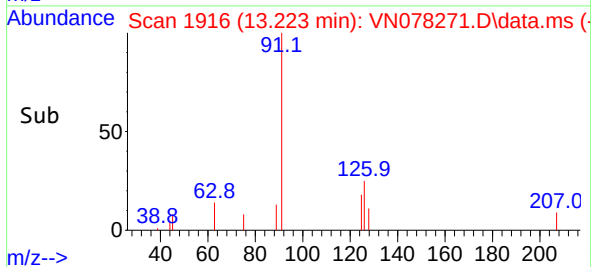

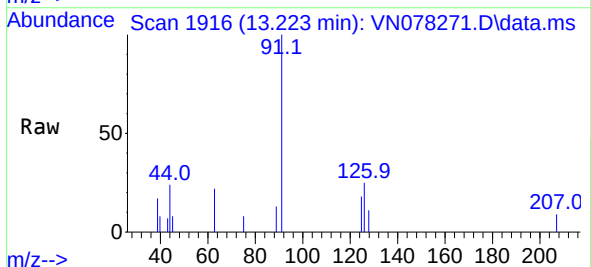




#85
 sec-Butylbenzene
 Concen: 0.217 ug/l
 RT: 13.617 min Scan# 1983
 Delta R.T. -0.006 min
 Lab File: VN078271.D
 Acq: 19 Jun 2023 11:37




Instrument :
 MSVOA_N
 ClientSampleId :
 VN0619MBL01


Tgt Ion:105 Resp: 4099
 Ion Ratio Lower Upper
 105 100
 134 15.1 9.8 29.3

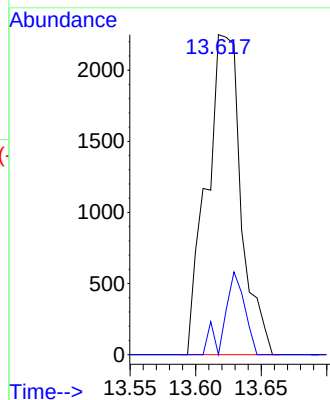

#87
 1,3-Dichlorobenzene
 Concen: 0.374 ug/l
 RT: 13.741 min Scan# 2004
 Delta R.T. -0.000 min
 Lab File: VN078271.D
 Acq: 19 Jun 2023 11:37

Tgt Ion:146 Resp: 3018
 Ion Ratio Lower Upper
 146 100
 111 38.4 22.1 66.3
 148 62.4 32.0 96.0



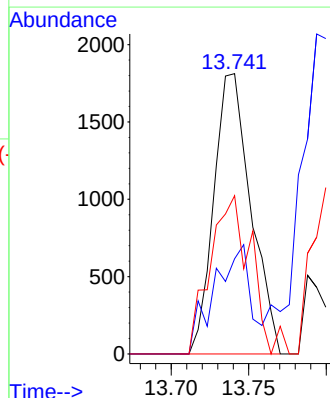





#88
1,4-Dichlorobenzene
Concen: 0.388 ug/l
RT: 13.741 min Scan# 2017
Delta R.T. -0.077 min
Lab File: VN078271.D
Acq: 19 Jun 2023 11:37




Instrument :
MSVOA_N
ClientSampleId :
VN0619MBL01


Tgt Ion:	146	Resp:	3018
Ion	Ratio	Lower	Upper
146	100		
111	38.4	20.6	61.8
148	62.4	31.6	94.8

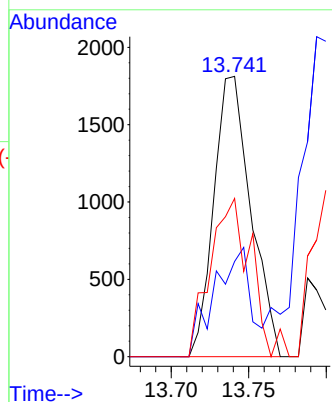

#89
n-Butylbenzene
Concen: 0.437 ug/l
RT: 14.059 min Scan# 2058
Delta R.T. -0.006 min
Lab File: VN078271.D
Acq: 19 Jun 2023 11:37

Tgt Ion:	91	Resp:	5295
Ion	Ratio	Lower	Upper
91	100		
92	62.7	26.4	79.0
134	26.2	12.6	37.6

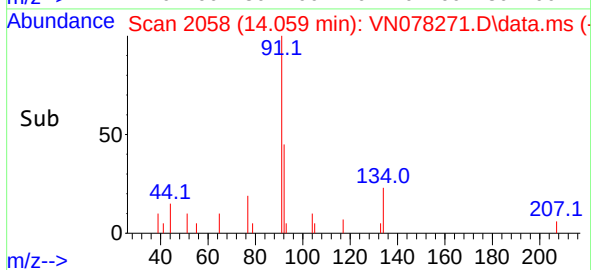



#91

1,2-Dichlorobenzene

Concen: 0.392 ug/l

RT: 14.106 min Scan# 2067

Delta R.T. -0.006 min

Lab File: VN078271.D

Acq: 19 Jun 2023 11:37

Instrument :

MSVOA_N

ClientSampleId :

VN0619MBL01





Tgt Ion:146 Resp: 3085

Ion Ratio Lower Upper

146 100

111 38.3 22.0 66.0

148 61.7 31.8 95.3



#92

1,2-Dibromo-3-Chloropropane

Concen: 0.712 ug/l

RT: 14.735 min Scan# 2173

Delta R.T. 0.012 min

Lab File: VN078271.D

Acq: 19 Jun 2023 11:37




Tgt Ion: 75 Resp: 724


Ion Ratio Lower Upper

75 100

155 33.8 39.1 117.2#

157 35.5 50.3 150.9#


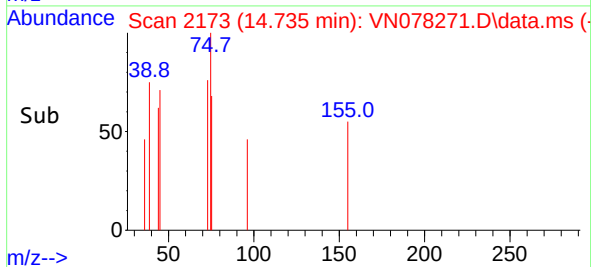

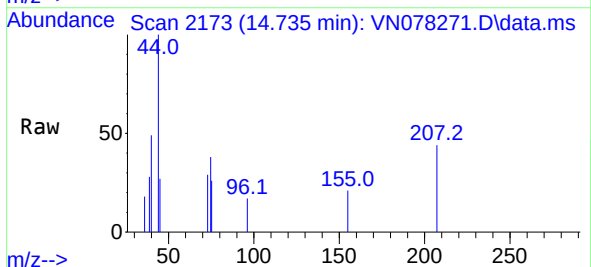




#93
1,2,4-Trichlorobenzene
Concen: 1.078 ug/l
RT: 15.400 min Scan# 21
Delta R.T. -0.000 min
Lab File: VN078271.D
Acq: 19 Jun 2023 11:37




Instrument :
MSVOA_N
ClientSampleId :
VN0619MBL01


Tgt Ion:180 Resp: 3027
Ion Ratio Lower Upper
180 100
182 94.5 46.1 138.2
145 43.7 16.6 49.8

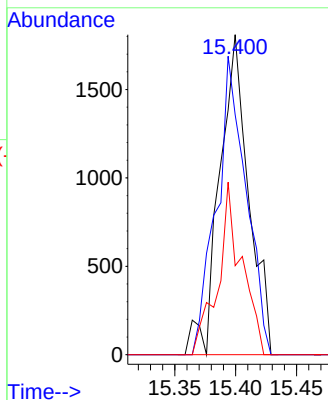

#94
Hexachlorobutadiene
Concen: Below Cal
RT: 15.505 min Scan# 2304
Delta R.T. -0.001 min
Lab File: VN078271.D
Acq: 19 Jun 2023 11:37

Tgt Ion:225 Resp: 2697
Ion Ratio Lower Upper
225 100
223 64.3 31.3 93.8
227 74.3 31.9 95.9



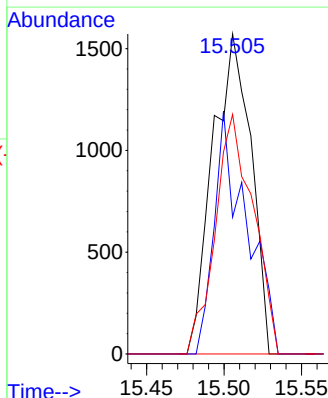





#95
Naphthalene
Concen: 1.105 ug/l
RT: 15.641 min Scan# 21
Delta R.T. -0.006 min
Lab File: VN078271.D
Acq: 19 Jun 2023 11:37

Instrument :
MSVOA_N
ClientSampleId :
VN0619MBL01

Tgt Ion:128 Resp: 10435
Ion Ratio Lower Upper
128 100
127 7.0 10.0 15.0#
129 12.8 8.7 13.1

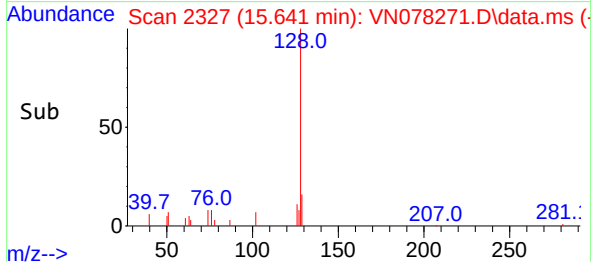

#96
1,2,3-Trichlorobenzene
Concen: 1.068 ug/l
RT: 15.841 min Scan# 2361
Delta R.T. -0.006 min
Lab File: VN078271.D
Acq: 19 Jun 2023 11:37

Tgt Ion:180 Resp: 3352
Ion Ratio Lower Upper
180 100
182 113.1 46.2 138.6
145 43.9 17.5 52.6

