
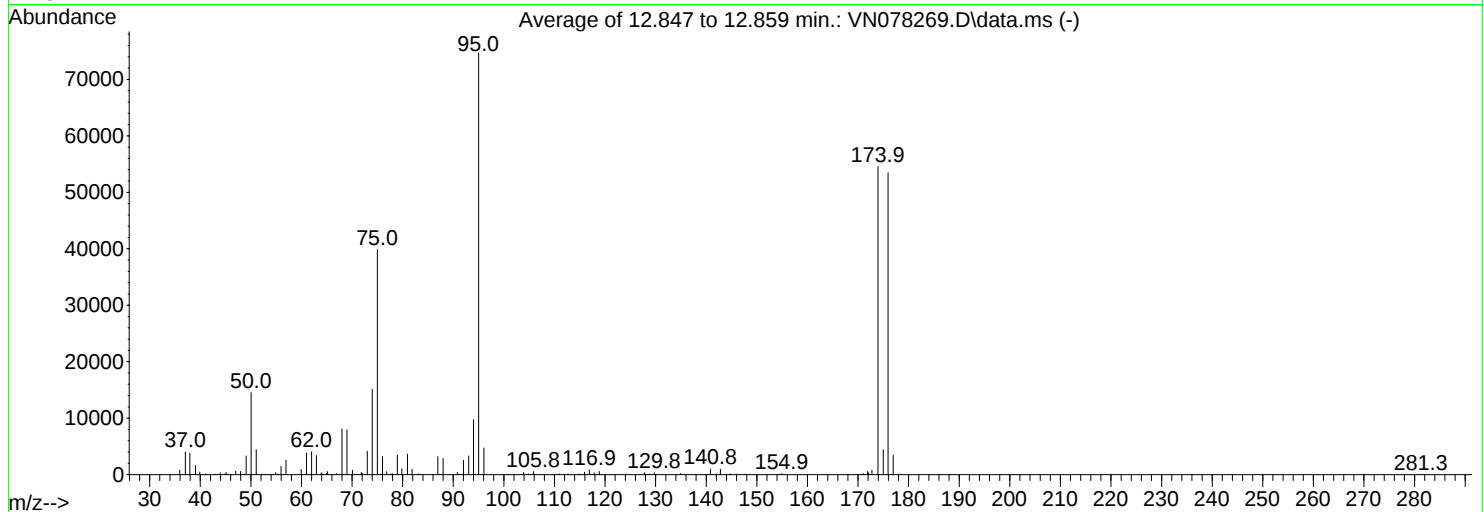


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN061923\
Data File : VN078269.D
Acq On : 19 Jun 2023 10:30
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N060623W.M
Title : SW846 8260
Last Update : Wed Jun 07 05:05:00 2023

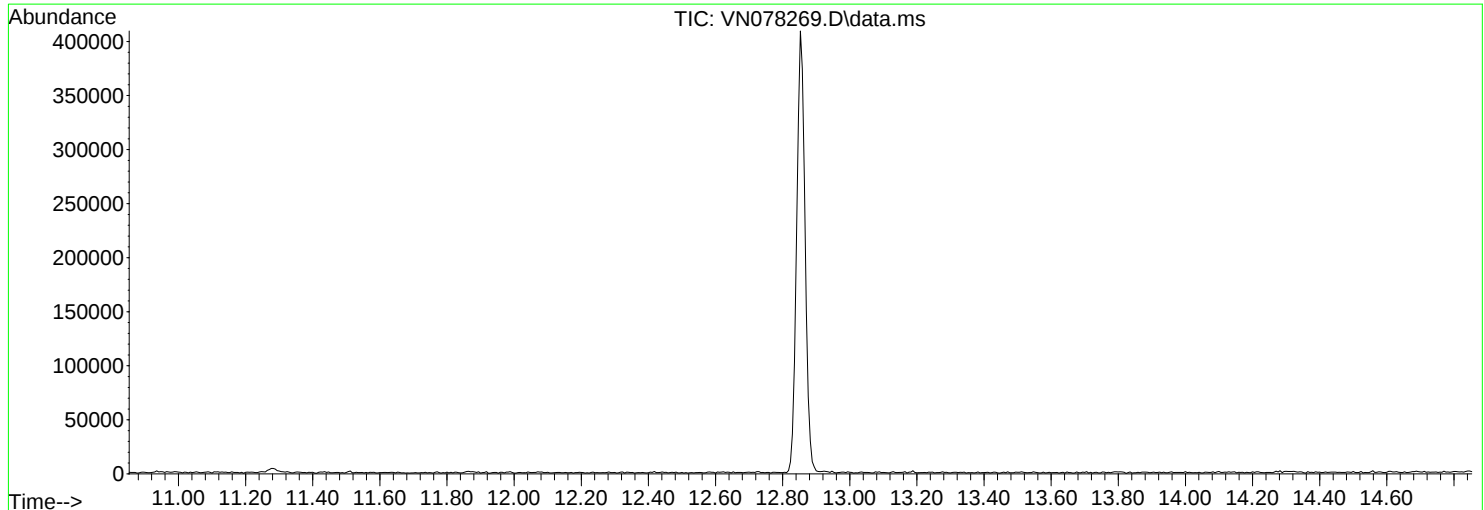

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1844

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.5	14532	PASS
75	95	30	60	53.3	39843	PASS
95	95	100	100	100.0	74704	PASS
96	95	5	9	6.3	4728	PASS
173	174	0.00	2	1.5	802	PASS
174	95	50	100	73.1	54587	PASS
175	174	5	9	8.1	4417	PASS
176	174	95	101	98.0	53480	PASS
177	176	5	9	6.4	3444	PASS

Average of 12.847 to 12.859 min.: VN078269.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	805	47.00	636	59.95	939	70.05	791
37.05	4026	47.95	583	61.00	3835	71.80	381
37.95	3794	49.05	3289	62.00	4059	72.00	281
39.05	1636	50.05	14532	62.95	3371	73.00	412
39.90	450	51.05	4426	63.80	114	74.00	15114
41.05	133	52.10	129	64.00	353	75.00	39843
42.90	94	52.80	81	64.90	218	76.00	3200
43.95	344	54.90	332	65.15	552	76.85	534
44.90	182	55.20	60	66.90	191	77.60	73
45.10	366	55.95	1478	68.00	8070	77.90	200
46.20	63	56.95	2595	69.00	7950	78.95	3446

Average of 12.847 to 12.859 min.: VN078269.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
79.85	1043	96.05	4728	118.85	579	144.80	127
80.95	3660	103.90	379	124.10	80	145.90	92
81.85	931	104.85	125	127.80	330	146.10	71
83.05	142	105.85	528	128.85	124	147.60	68
86.95	3206	110.95	158	129.75	347	147.90	125
88.00	2860	112.65	112	134.90	215	154.95	186
90.80	413	114.70	65	140.85	996	170.90	56
92.00	2532	115.00	85	142.00	119	171.10	176
93.05	3326	115.95	440	142.80	981	171.90	598
94.00	9726	116.90	849	144.00	102	172.10	332
95.00	74704	117.85	311	144.60	72	172.75	802

Average of 12.847 to 12.859 min.: VN078269.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
173.95	54587						
175.00	4417						
175.95	53480						
176.95	3444						
178.10	109						
281.30	50						