

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN061924\  
 Data File : VN082646.D  
 Acq On : 19 Jun 2024 17:14  
 Operator : JC\MD  
 Sample : P2915-03  
 Misc : 5.0mL/MSVOA\_N/WATER  
 ALS Vial : 20 Sample Multiplier: 1

Instrument :  
 MSVOA\_N  
 ClientSampleId :

Quant Time: Jun 20 03:03:37 2024  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N061724W.M  
 Quant Title : SW846 8260  
 QLast Update : Tue Jun 18 04:52:44 2024  
 Response via : Initial Calibration


| Compound                      | R.T.           | QIon | Response            | Conc   | Units  | Dev(Min) |
|-------------------------------|----------------|------|---------------------|--------|--------|----------|
| -----                         |                |      |                     |        |        |          |
| Internal Standards            |                |      |                     |        |        |          |
| 1) Pentafluorobenzene         | 8.230          | 168  | 126453              | 50.000 | ug/l   | 0.00     |
| 34) 1,4-Difluorobenzene       | 9.106          | 114  | 247773              | 50.000 | ug/l   | 0.00     |
| 63) Chlorobenzene-d5          | 11.871         | 117  | 255358              | 50.000 | ug/l   | 0.00     |
| 72) 1,4-Dichlorobenzene-d4    | 13.794         | 152  | 101359              | 50.000 | ug/l   | 0.00     |
|                               |                |      |                     |        |        |          |
| System Monitoring Compounds   |                |      |                     |        |        |          |
| 33) 1,2-Dichloroethane-d4     | 8.583          | 65   | 120396              | 59.371 | ug/l   | 0.00     |
| Spiked Amount 50.000          | Range 74 - 125 |      | Recovery = 118.740% |        |        |          |
| 35) Dibromofluoromethane      | 8.171          | 113  | 87172               | 51.861 | ug/l   | 0.00     |
| Spiked Amount 50.000          | Range 75 - 124 |      | Recovery = 103.720% |        |        |          |
| 50) Toluene-d8                | 10.571         | 98   | 332950              | 52.380 | ug/l   | 0.00     |
| Spiked Amount 50.000          | Range 86 - 113 |      | Recovery = 104.760% |        |        |          |
| 62) 4-Bromofluorobenzene      | 12.853         | 95   | 106003              | 48.371 | ug/l   | 0.00     |
| Spiked Amount 50.000          | Range 64 - 133 |      | Recovery = 96.740%  |        |        |          |
|                               |                |      |                     |        |        |          |
| Target Compounds              |                |      |                     |        | Qvalue |          |
| 3) Chloromethane              | 2.360          | 50   | 598                 | 0.282  | ug/l # | 43       |
| 11) Tert butyl alcohol        | 5.548          | 59   | 1765                | 5.318  | ug/l # | 71       |
| 16) Acetone                   | 4.436          | 43   | 20727               | 22.475 | ug/l   | 90       |
| 18) Methyl Acetate            | 5.030          | 43   | 3885                | 1.722  | ug/l   | 97       |
| 20) Methylene Chloride        | 5.283          | 84   | 10152               | 6.261  | ug/l # | 89       |
| 25) 2-Butanone                | 7.489          | 43   | 11863               | 9.050  | ug/l   | 99       |
| 29) Tetrahydrofuran           | 7.853          | 42   | 408                 | 0.508  | ug/l # | 38       |
| 31) Cyclohexane               | 8.230          | 56   | 3844                | 1.313  | ug/l # | 26       |
| 36) 1,1-Dichloropropene       | 8.224          | 75   | 11598               | 4.616  | ug/l # | 53       |
| 37) Ethyl Acetate             | 7.559          | 43   | 4698                | 1.468  | ug/l # | 79       |
| 38) Carbon Tetrachloride      | 8.236          | 117  | 13801               | 4.874  | ug/l # | 18       |
| 42) 1,2-Dichloroethane        | 8.677          | 62   | 767                 | 0.260  | ug/l # | 78       |
| 43) Isopropyl Acetate         | 8.694          | 43   | 219377              | 36.675 | ug/l # | 84       |
| 45) 1,2-Dichloropropane       | 9.741          | 63   | 1612                | 0.807  | ug/l # | 44       |
| 48) Methyl methacrylate       | 9.671          | 41   | 4550                | 1.845  | ug/l # | 50       |
| 49) 1,4-Dioxane               | 9.747          | 88   | 74                  | 1.919  | ug/l # | 1        |
| 51) 4-Methyl-2-Pentanone      | 10.453         | 43   | 5305                | 1.729  | ug/l   | 98       |
| 53) t-1,3-Dichloropropene     | 10.730         | 75   | 882                 | 0.299  | ug/l   | 93       |
| 54) cis-1,3-Dichloropropene   | 10.359         | 75   | 42615               | 13.958 | ug/l # | 69       |
| 56) Ethyl methacrylate        | 10.982         | 69   | 2065                | 0.732  | ug/l # | 1        |
| 57) 1,3-Dichloropropane       | 11.206         | 76   | 5487                | 1.743  | ug/l # | 44       |
| 59) 2-Hexanone                | 11.171         | 43   | 125563              | 53.847 | ug/l # | 28       |
| 71) Bromoform                 | 12.853         | 173  | 453                 | 0.274  | ug/l # | 1        |
| 74) N-amyl acetate            | 12.494         | 43   | 961                 | 0.234  | ug/l # | 46       |
| 76) 1,2,3-Trichloropropane    | 12.853         | 75   | 61985               | 25.003 | ug/l # | 1        |
| 81) trans-1,4-Dichloro-2-b... | 12.853         | 75   | 61985               | 59.818 | ug/l # | 6        |
| -----                         |                |      |                     |        |        |          |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN061924\  
Data File : VN082646.D  
Acq On : 19 Jun 2024 17:14  
Operator : JC\MD  
Sample : P2915-03  
Misc : 5.0mL/MSVOA\_N/WATER  
ALS Vial : 20 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :

Quant Time: Jun 20 03:03:37 2024  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N061724W.M  
Quant Title : SW846 8260  
QLast Update : Tue Jun 18 04:52:44 2024  
Response via : Initial Calibration

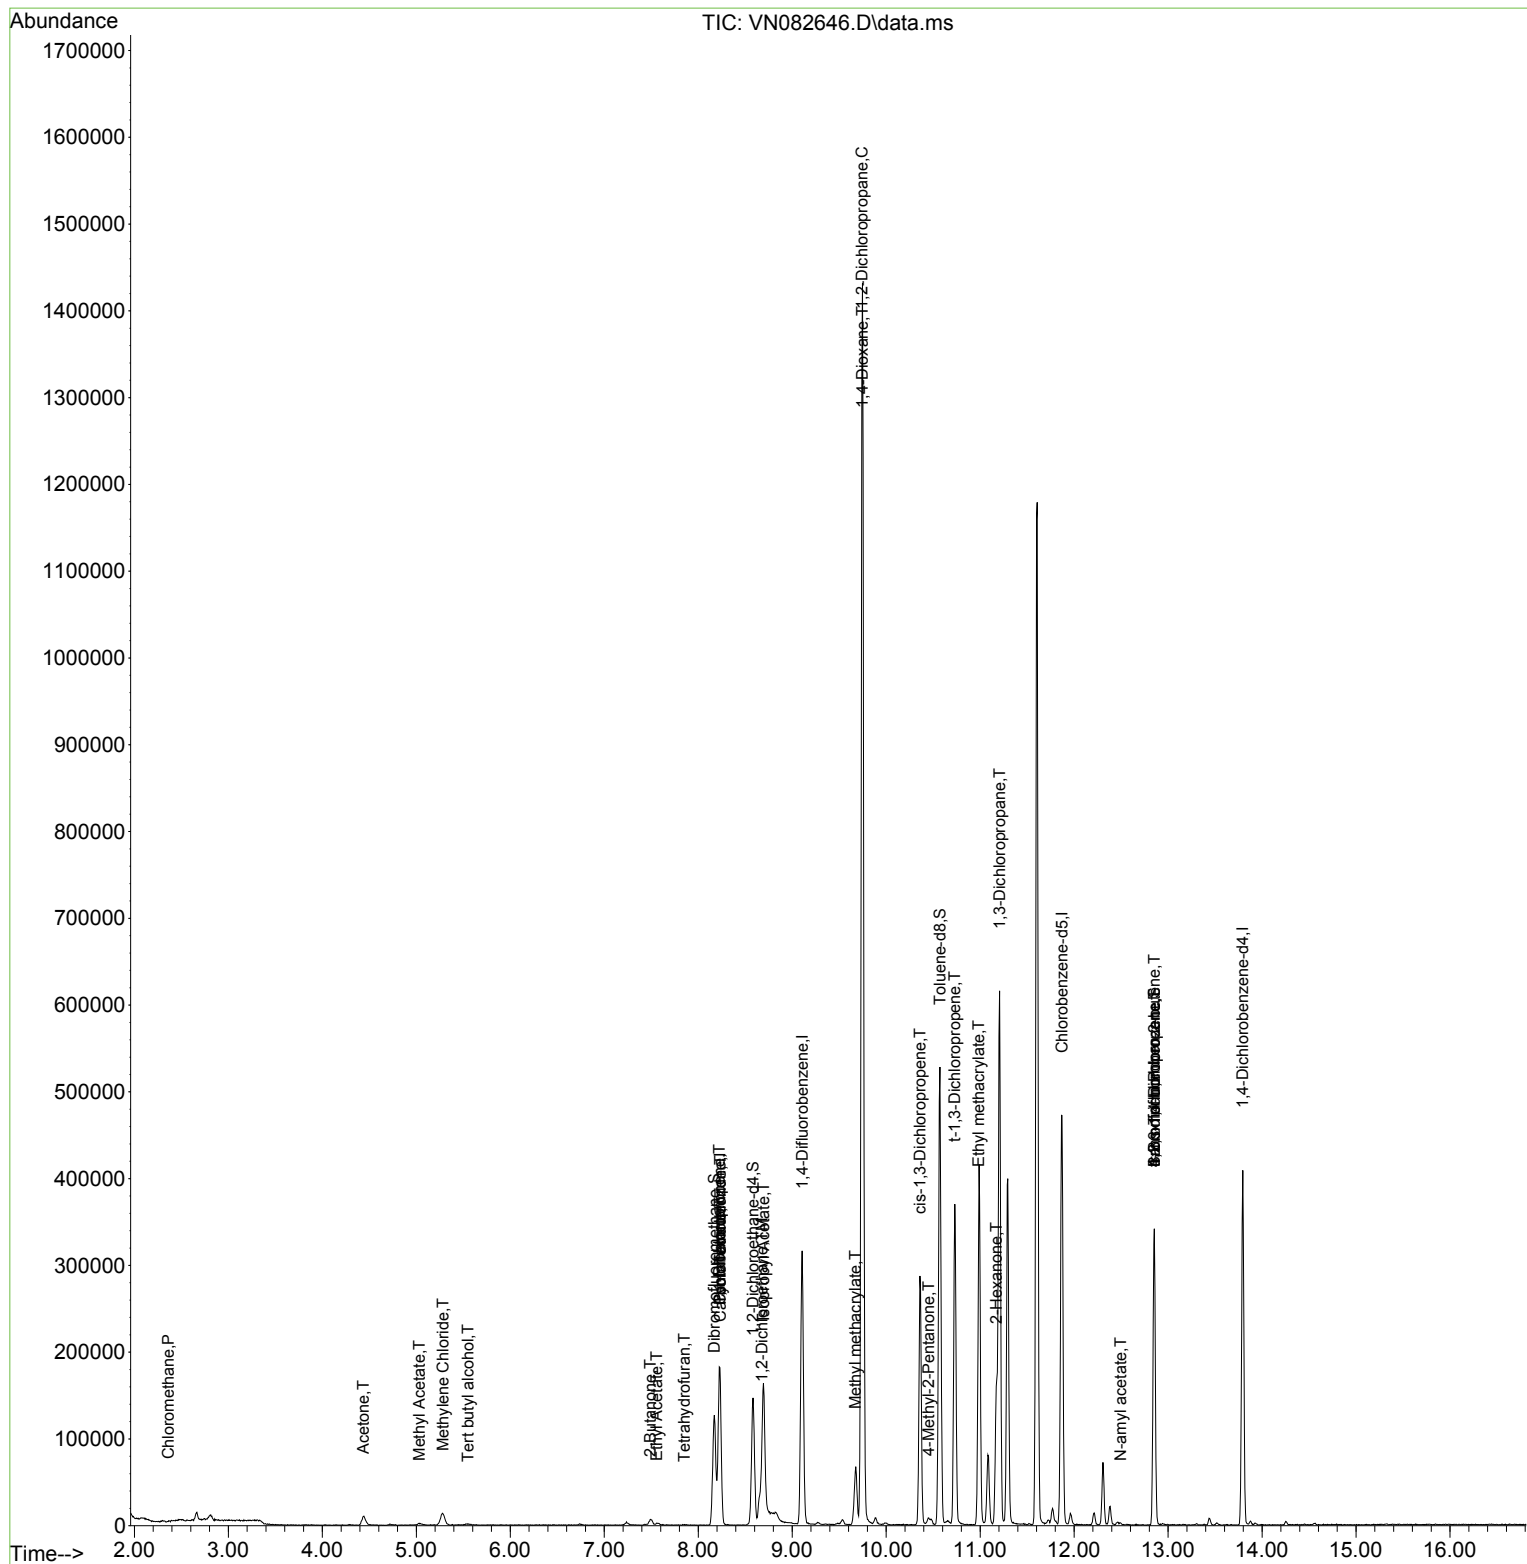



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 8.230 min Scan# 1067

Delta R.T. 0.001 min

Lab File: VN082646.D

Acq: 19 Jun 2024 17:14

Instrument :

MSVOA\_N





ClientSampleId :

Tgt Ion:168 Resp: 126453

Ion Ratio Lower Upper

168 100

99 62.4 48.2 72.4

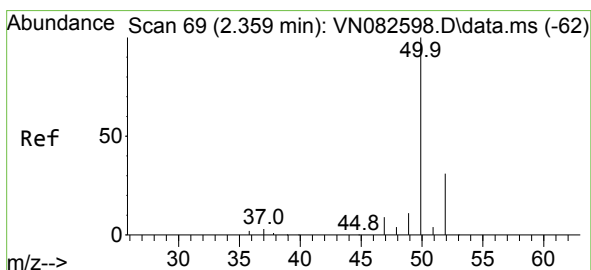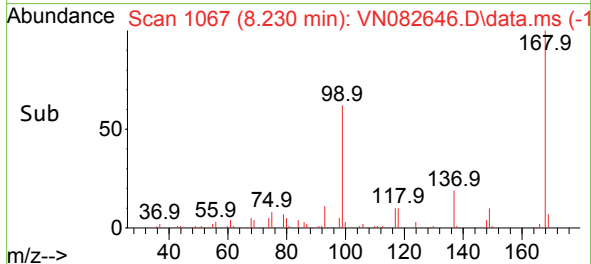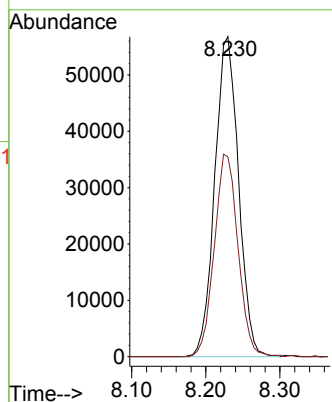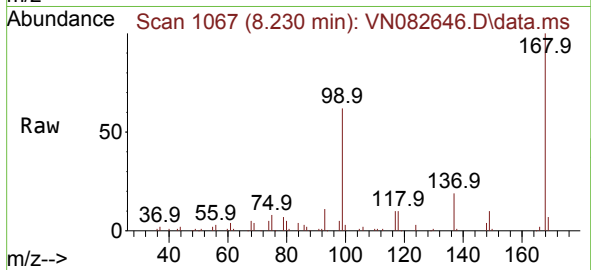

#3

Chloromethane

Concen: 0.282 ug/l

RT: 2.360 min Scan# 69

Delta R.T. 0.000 min

Lab File: VN082646.D




Acq: 19 Jun 2024 17:14


Tgt Ion: 50 Resp: 598

Ion Ratio Lower Upper

50 100


52 0.0 25.0 37.4#

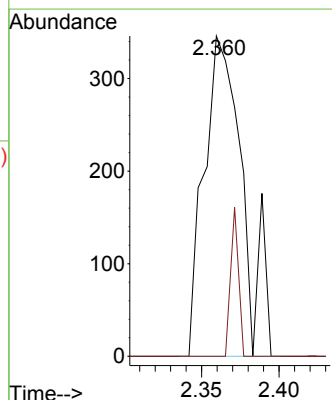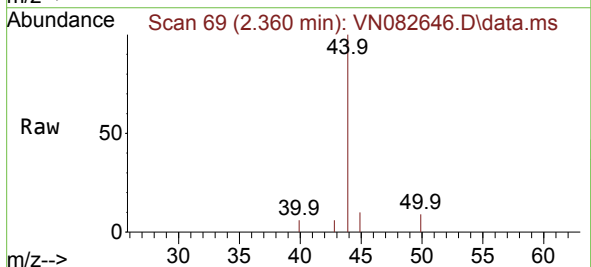






#11  
Tert butyl alcohol  
Concen: 5.318 ug/l  
RT: 5.548 min Scan# 611  
Delta R.T. 0.024 min  
Lab File: VN082646.D  
Acq: 19 Jun 2024 17:14

Instrument :  
MSVOA\_N  
ClientSampleId :



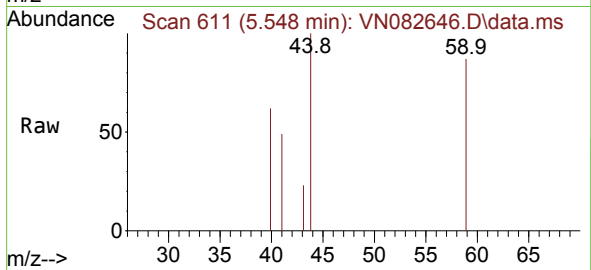



Tgt Ion: 59 Resp: 1765  
Ion Ratio Lower Upper  
59 100  
57 0.0 8.9 13.3#

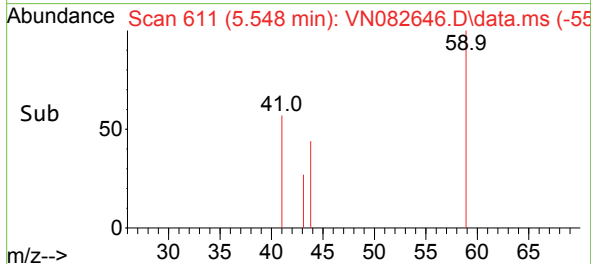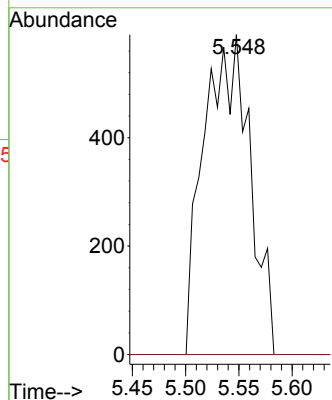

#16  
Acetone  
Concen: 22.475 ug/l  
RT: 4.436 min Scan# 422  
Delta R.T. 0.006 min  
Lab File: VN082646.D  
Acq: 19 Jun 2024 17:14

Tgt Ion: 43 Resp: 20727  
Ion Ratio Lower Upper  
43 100  
58 22.2 21.8 32.6


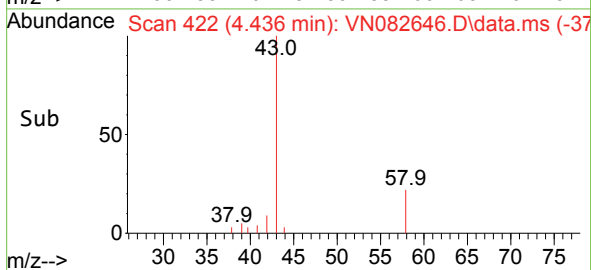
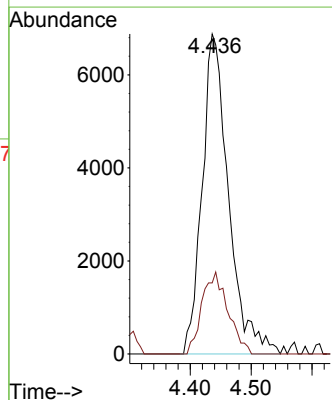
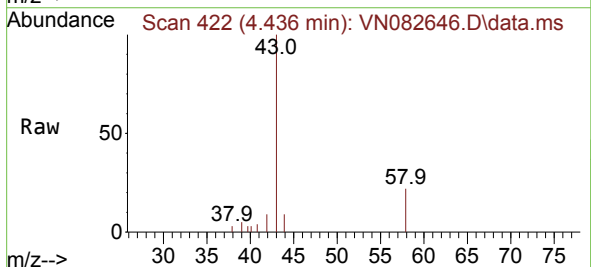




#18  
Methyl Acetate  
Concen: 1.722 ug/l  
RT: 5.030 min Scan# 51  
Delta R.T. 0.000 min  
Lab File: VN082646.D  
Acq: 19 Jun 2024 17:14




Instrument :  
MSVOA\_N  
ClientSampleId :


Tgt Ion: 43 Resp: 3885  
Ion Ratio Lower Upper  
43 100  
74 19.0 16.3 24.5

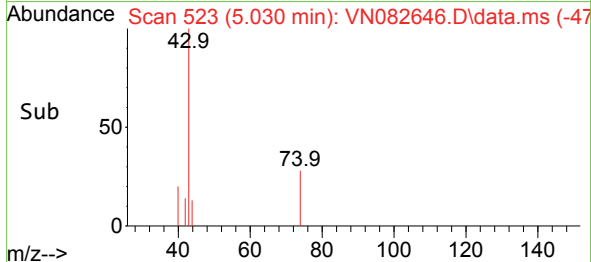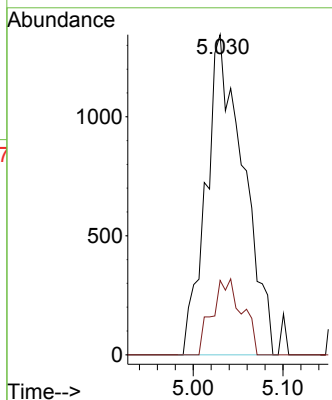

#20  
Methylene Chloride  
Concen: 6.261 ug/l  
RT: 5.283 min Scan# 566  
Delta R.T. 0.006 min  
Lab File: VN082646.D  
Acq: 19 Jun 2024 17:14

Tgt Ion: 84 Resp: 10152  
Ion Ratio Lower Upper  
84 100  
49 138.0 119.6 179.4  
51 32.7 34.8 52.2#  
86 75.4 52.9 79.3


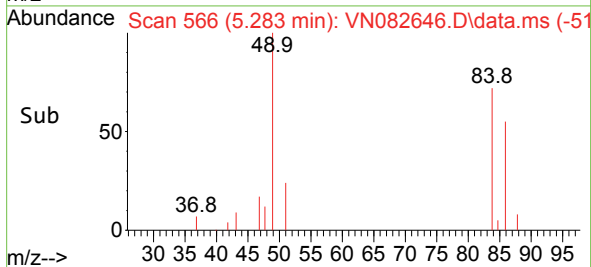
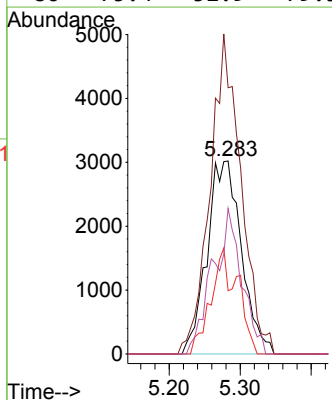
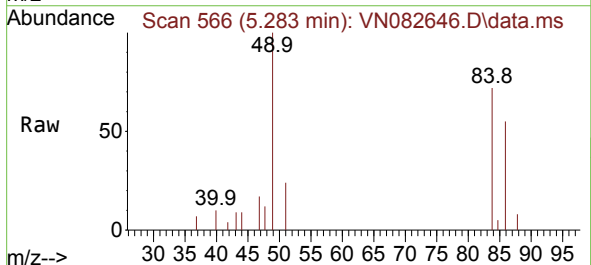


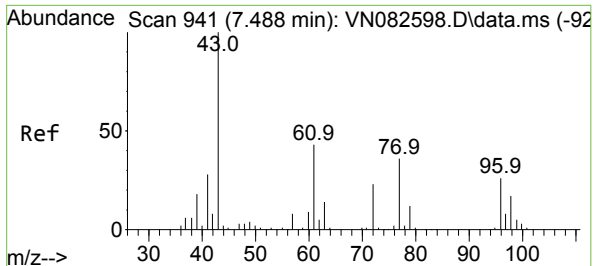

#25  
2-Butanone  
Concen: 9.050 ug/l  
RT: 7.489 min Scan# 941  
Delta R.T. 0.000 min  
Lab File: VN082646.D  
Acq: 19 Jun 2024 17:14




Instrument :  
MSVOA\_N  
ClientSampleId :


Tgt Ion: 43 Resp: 11863  
Ion Ratio Lower Upper  
43 100  
72 23.4 18.2 27.2

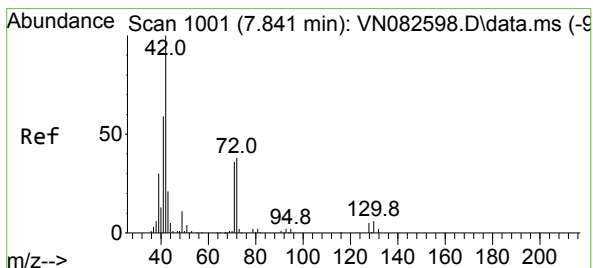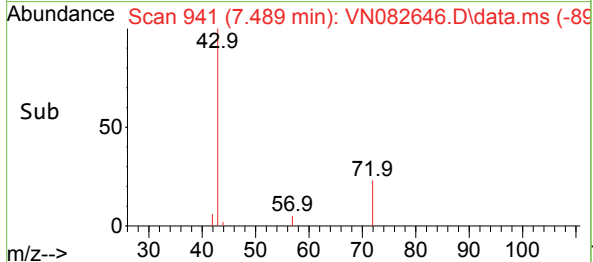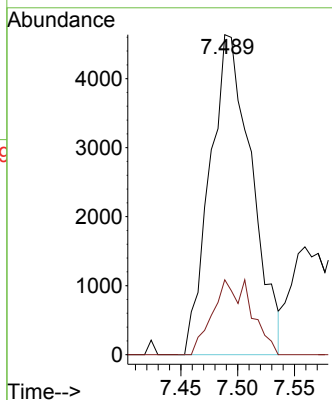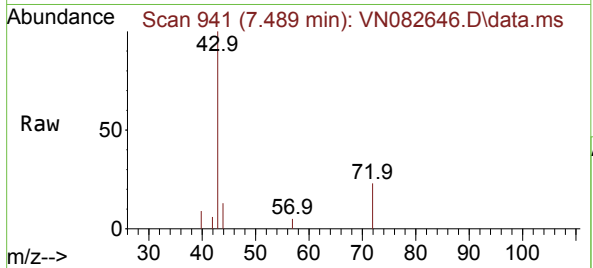

#29  
Tetrahydrofuran  
Concen: 0.508 ug/l  
RT: 7.853 min Scan# 1003  
Delta R.T. 0.012 min  
Lab File: VN082646.D  
Acq: 19 Jun 2024 17:14


Tgt Ion: 42 Resp: 408  
Ion Ratio Lower Upper  
42 100  
72 0.0 30.0 45.0#  
71 0.0 28.3 42.5#

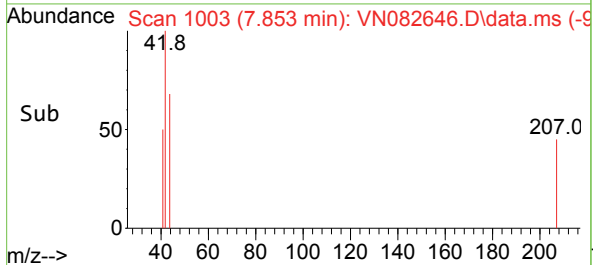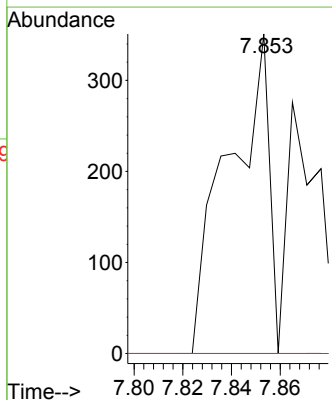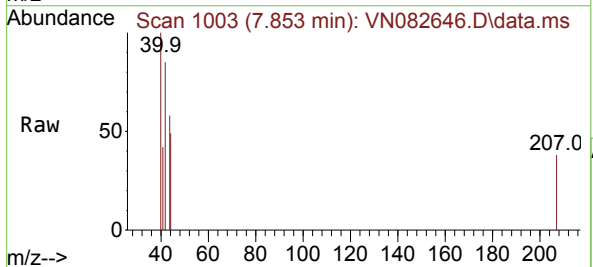






#31  
Cyclohexane  
Concen: 1.313 ug/l  
RT: 8.230 min Scan# 1072  
Delta R.T. -0.029 min  
Lab File: VN082646.D  
Acq: 19 Jun 2024 17:14

Instrument :  
MSVOA\_N  
ClientSampleId :







Tgt Ion: 56 Resp: 3844  
Ion Ratio Lower Upper  
56 100  
69 126.5 24.5 36.7#  
84 115.3 66.0 99.0#

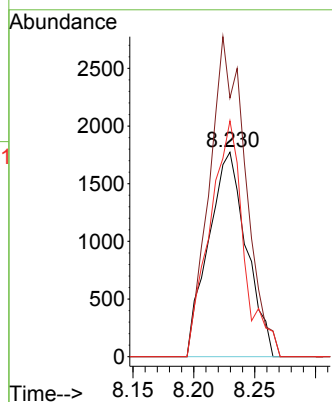

#33  
1,2-Dichloroethane-d4  
Concen: 59.371 ug/l  
RT: 8.583 min Scan# 1127  
Delta R.T. 0.000 min  
Lab File: VN082646.D  
Acq: 19 Jun 2024 17:14


Tgt Ion: 65 Resp: 120396  
Ion Ratio Lower Upper  
65 100  
67 50.3 0.0 104.4

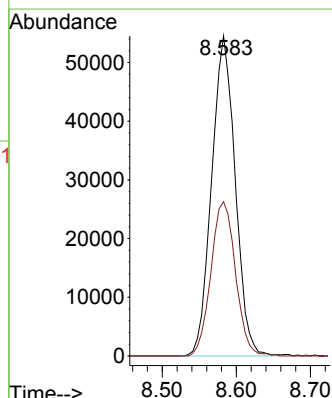






#34  
1,4-Difluorobenzene  
Concen: 50.000 ug/l  
RT: 9.106 min Scan# 11  
Delta R.T. 0.000 min  
Lab File: VN082646.D  
Acq: 19 Jun 2024 17:14

Instrument :  
MSVOA\_N  
ClientSampleId :






Tgt Ion:114 Resp: 247773  
Ion Ratio Lower Upper  
114 100  
63 22.9 0.0 44.6  
88 14.7 0.0 31.4

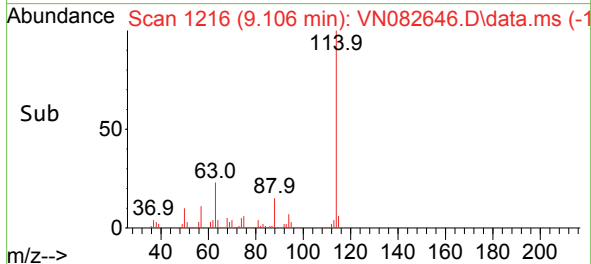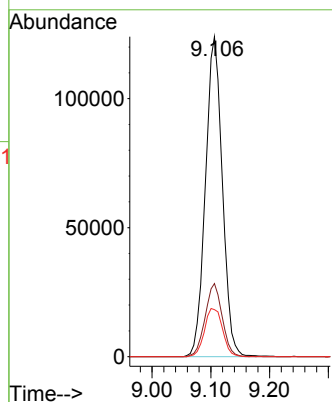


#35  
Dibromofluoromethane  
Concen: 51.861 ug/l  
RT: 8.171 min Scan# 1057  
Delta R.T. 0.006 min  
Lab File: VN082646.D  
Acq: 19 Jun 2024 17:14

Tgt Ion:113 Resp: 87172  
Ion Ratio Lower Upper  
113 100  
111 104.4 82.4 123.6  
192 18.9 14.9 22.3

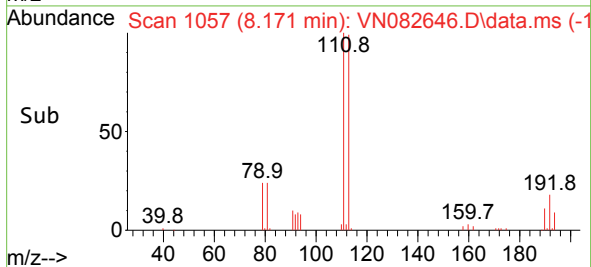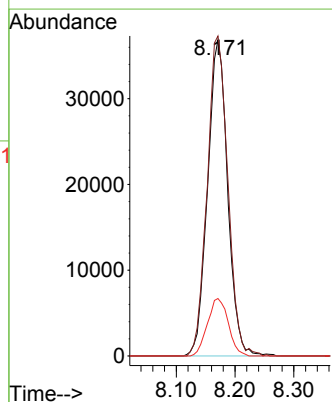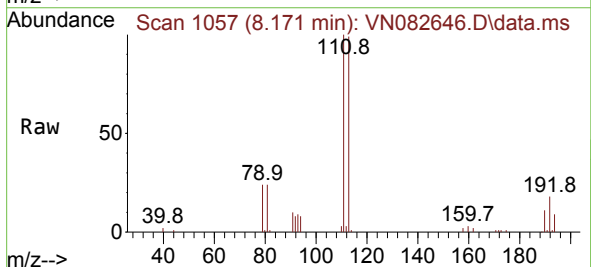









#36  
1,1-Dichloropropene  
Concen: 4.616 ug/l  
RT: 8.224 min Scan# 1066  
Delta R.T. -0.147 min  
Lab File: VN082646.D  
Acq: 19 Jun 2024 17:14

Instrument :  
MSVOA\_N  
ClientSampleId :



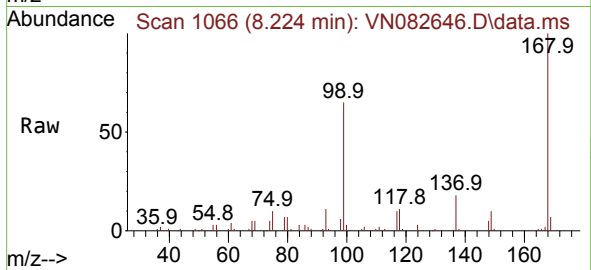



Tgt Ion: 75 Resp: 11598  
Ion Ratio Lower Upper  
75 100  
110 10.8 16.3 48.9#  
77 0.0 24.6 37.0#

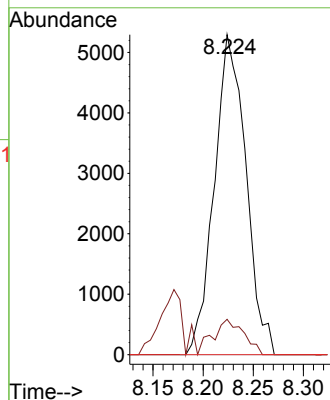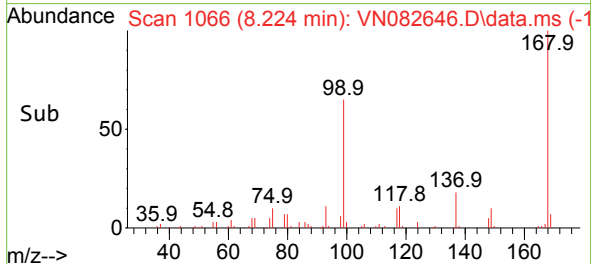

#37  
Ethyl Acetate  
Concen: 1.468 ug/l  
RT: 7.559 min Scan# 953  
Delta R.T. -0.006 min  
Lab File: VN082646.D  
Acq: 19 Jun 2024 17:14

Tgt Ion: 43 Resp: 4698  
Ion Ratio Lower Upper  
43 100  
61 1.5 9.3 13.9#  
70 4.0 7.0 10.6#

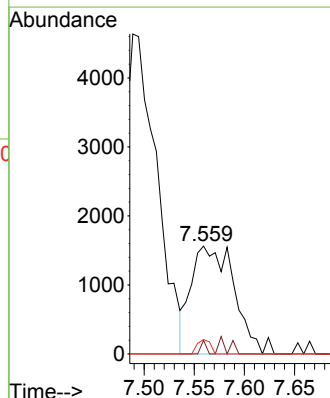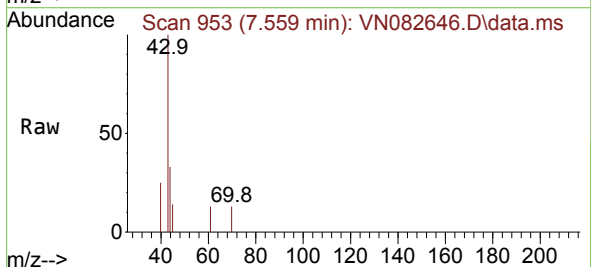

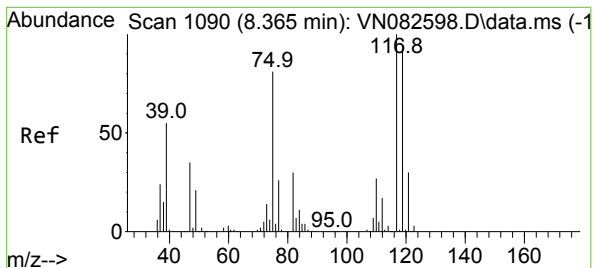

#38

Carbon Tetrachloride

Concen: 4.874 ug/l

RT: 8.236 min Scan# 110

Delta R.T. -0.129 min


Lab File: VN082646.D

Acq: 19 Jun 2024 17:14

Instrument :




MSVOA\_N

ClientSampleId :

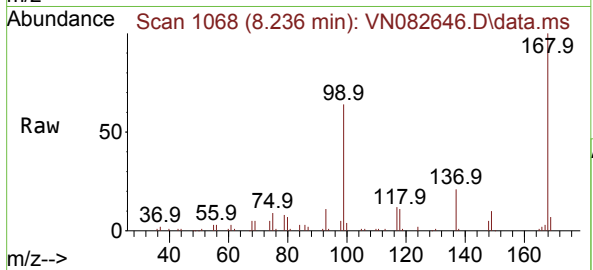

Tgt Ion:117 Resp: 13801

| Ion | Ratio | Lower | Upper  |
|-----|-------|-------|--------|
| 117 | 100   |       |        |
| 119 | 6.5   | 74.9  | 112.3# |
| 121 | 0.0   | 24.3  | 36.5#  |

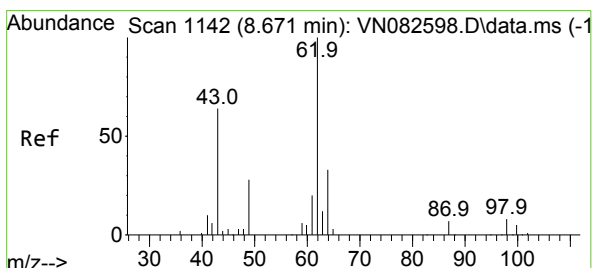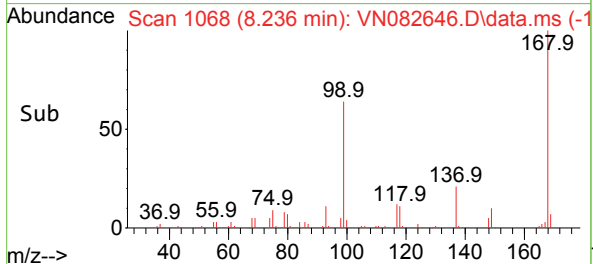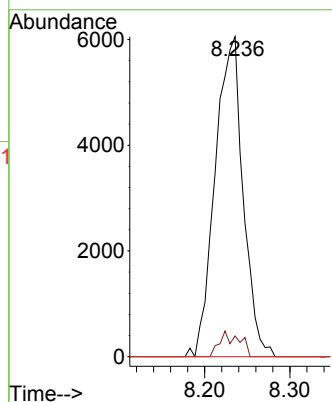

#42

1,2-Dichloroethane

Concen: 0.260 ug/l

RT: 8.677 min Scan# 1143




Delta R.T. 0.006 min


Lab File: VN082646.D

Acq: 19 Jun 2024 17:14

Tgt Ion: 62 Resp: 767


| Ion | Ratio | Lower | Upper |
|-----|-------|-------|-------|
| 62  | 100   |       |       |
| 98  | 0.0   | 0.0   | 15.8  |

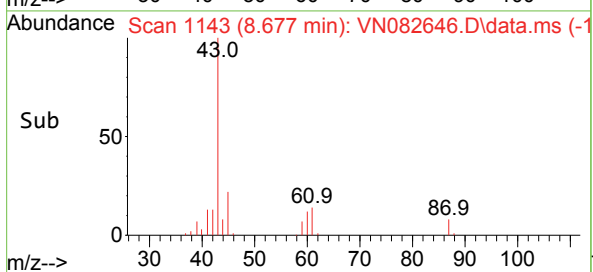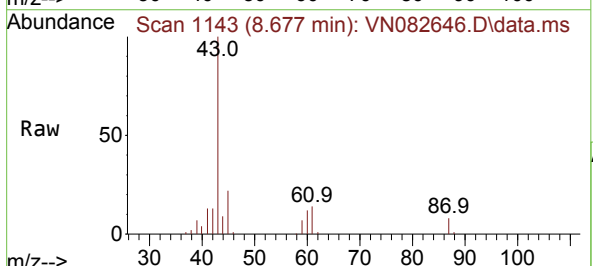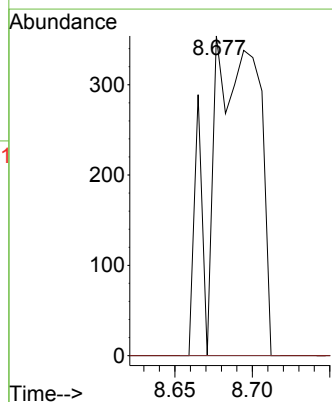






#43  
Isopropyl Acetate  
Concen: 36.675 ug/l  
RT: 8.694 min Scan# 1146  
Delta R.T. 0.000 min  
Lab File: VN082646.D  
Acq: 19 Jun 2024 17:14


Instrument :  
MSVOA\_N  
ClientSampleId :





Tgt Ion: 43 Resp: 219377  
Ion Ratio Lower Upper  
43 100  
61 12.4 17.8 26.6#  
87 7.6 8.2 12.2#

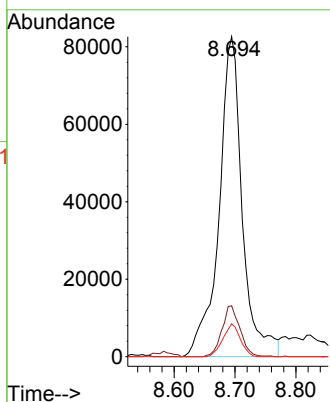


#45  
1,2-Dichloropropane  
Concen: 0.807 ug/l  
RT: 9.741 min Scan# 1324  
Delta R.T. 0.118 min  
Lab File: VN082646.D  
Acq: 19 Jun 2024 17:14

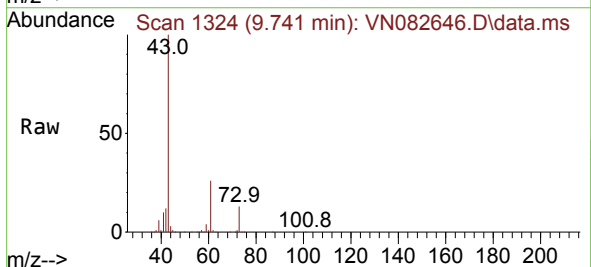

Tgt Ion: 63 Resp: 1612  
Ion Ratio Lower Upper  
63 100  
65 0.0 24.4 36.6#



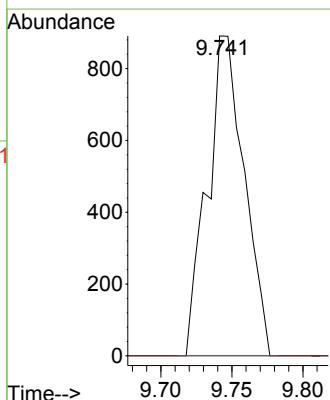





#48  
Methyl methacrylate  
Concen: 1.845 ug/l  
RT: 9.671 min Scan# 11  
Delta R.T. -0.011 min  
Lab File: VN082646.D  
Acq: 19 Jun 2024 17:14




Instrument :  
MSVOA\_N  
ClientSampleId :


Tgt Ion: 41 Resp: 4550  
Ion Ratio Lower Upper  
41 100  
69 0.0 56.3 84.5#  
39 71.3 50.3 75.5

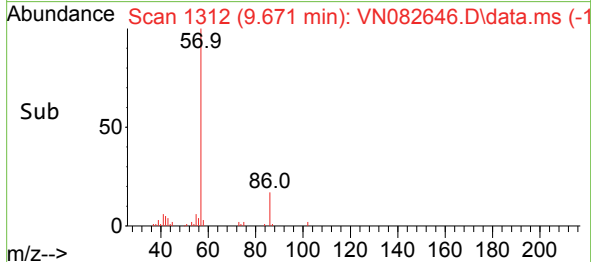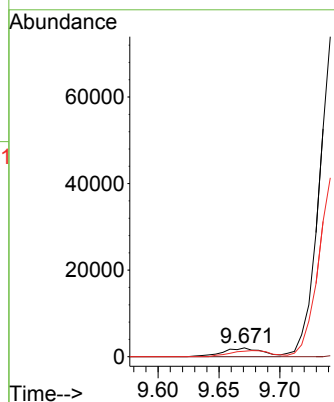

#49  
1,4-Dioxane  
Concen: 1.919 ug/l  
RT: 9.747 min Scan# 1325  
Delta R.T. 0.053 min  
Lab File: VN082646.D  
Acq: 19 Jun 2024 17:14

Tgt Ion: 88 Resp: 74  
Ion Ratio Lower Upper  
88 100  
43 1867474.3 27.8 41.8#  
58 9194.6 59.4 89.0#


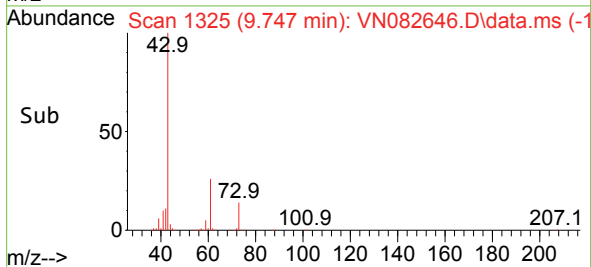
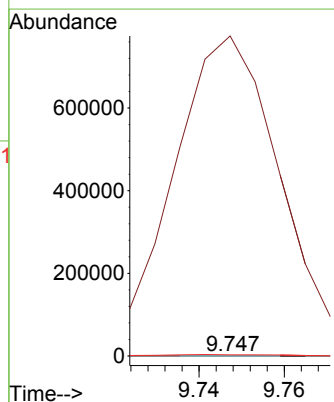
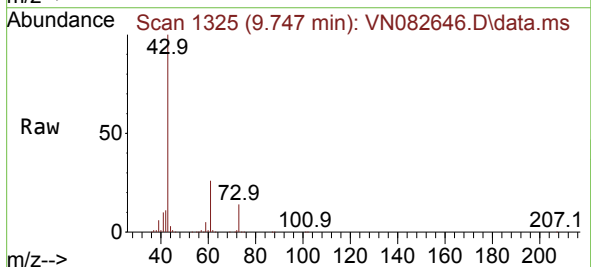


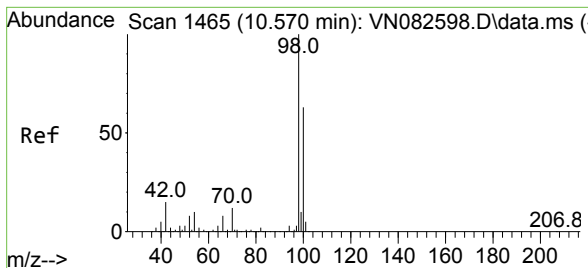

#50  
Toluene-d8  
Concen: 52.380 ug/l  
RT: 10.571 min Scan# 1465  
Delta R.T. 0.000 min  
Lab File: VN082646.D  
Acq: 19 Jun 2024 17:14




Instrument :  
MSVOA\_N  
ClientSampleId :


Tgt Ion: 98 Resp: 332950  
Ion Ratio Lower Upper  
98 100  
100 64.4 51.5 77.3

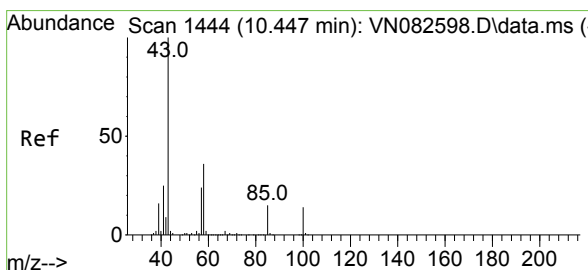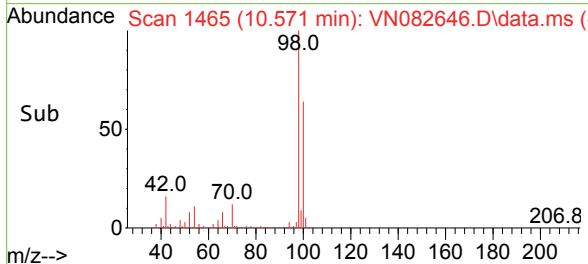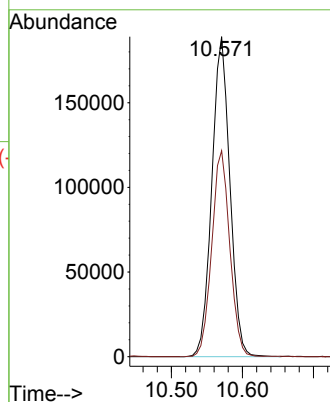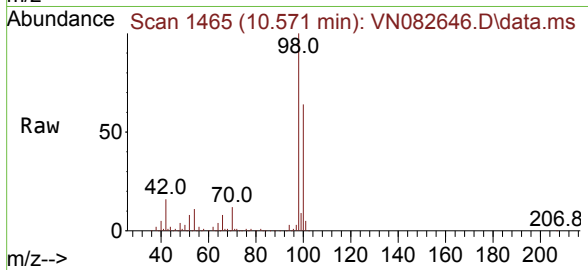

#51  
4-Methyl-2-Pentanone  
Concen: 1.729 ug/l  
RT: 10.453 min Scan# 1445  
Delta R.T. 0.006 min  
Lab File: VN082646.D  
Acq: 19 Jun 2024 17:14


Tgt Ion: 43 Resp: 5305  
Ion Ratio Lower Upper  
43 100  
58 34.0 28.2 42.4

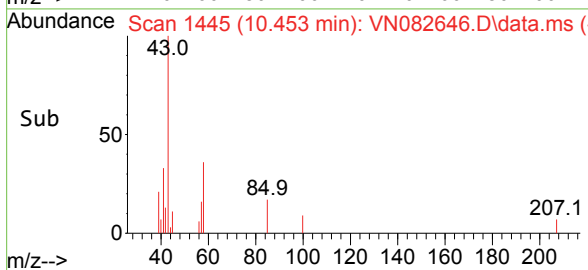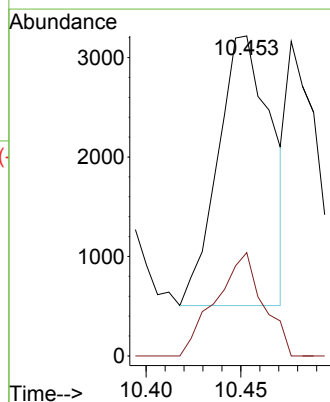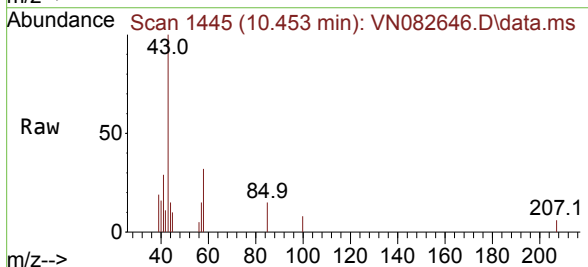



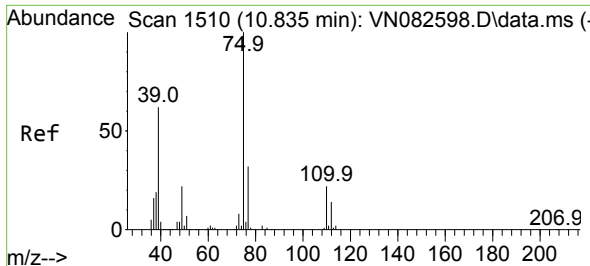


#53  
t-1,3-Dichloropropene  
Concen: 0.299 ug/l  
RT: 10.730 min Scan# 1492  
Delta R.T. -0.106 min  
Lab File: VN082646.D  
Acq: 19 Jun 2024 17:14

Instrument :  
MSVOA\_N  
ClientSampleId :



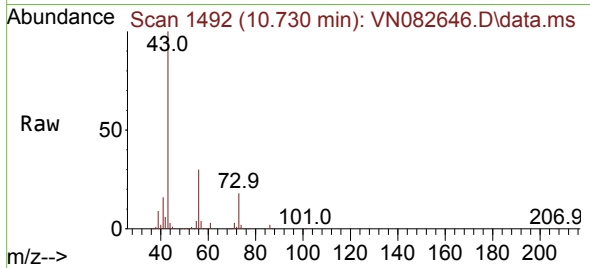



Tgt Ion: 75 Resp: 882  
Ion Ratio Lower Upper  
75 100  
77 27.9 25.7 38.5

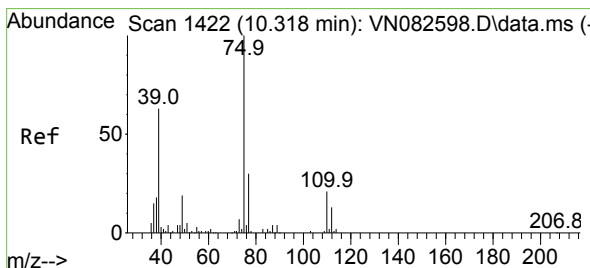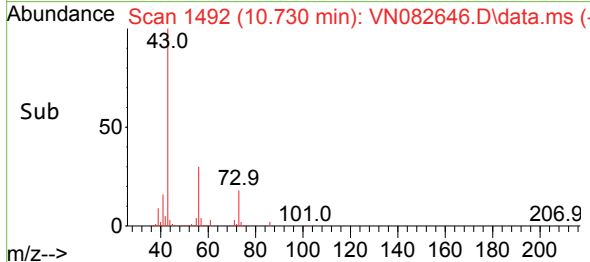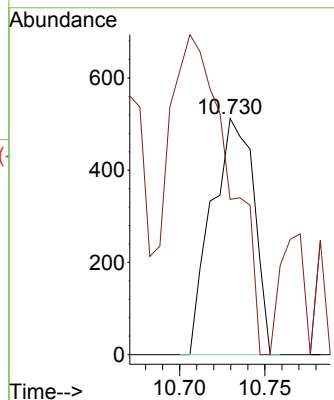

#54  
cis-1,3-Dichloropropene  
Concen: 13.958 ug/l  
RT: 10.359 min Scan# 1429  
Delta R.T. 0.041 min  
Lab File: VN082646.D  
Acq: 19 Jun 2024 17:14

Tgt Ion: 75 Resp: 42615  
Ion Ratio Lower Upper  
75 100  
77 0.0 24.3 36.5#  
39 48.6 50.5 75.7#


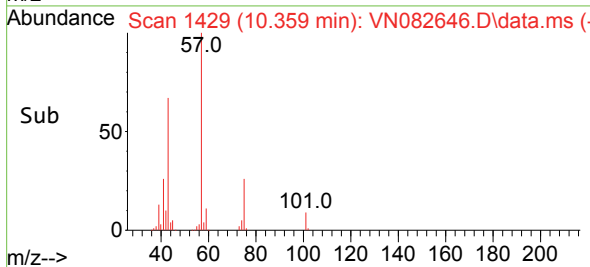
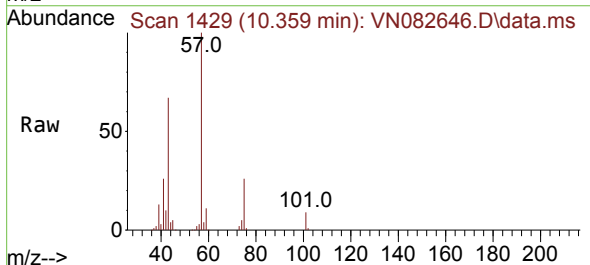
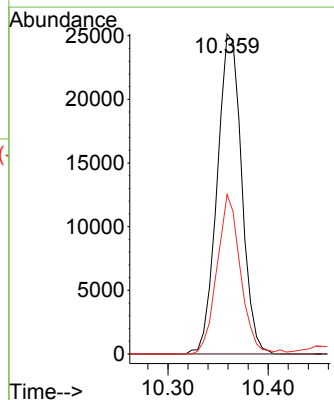


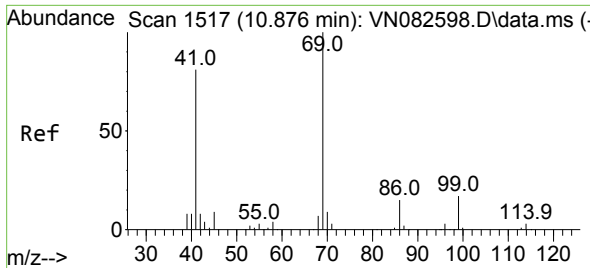

#56  
 Ethyl methacrylate  
 Concen: 0.732 ug/l  
 RT: 10.982 min Scan# 1535  
 Delta R.T. 0.106 min  
 Lab File: VN082646.D  
 Acq: 19 Jun 2024 17:14




Instrument :  
 MSVOA\_N  
 ClientSampleId :


Tgt Ion: 69 Resp: 2065  
 Ion Ratio Lower Upper  
 69 100  
 41 4072.9 63.4 95.2#  
 39 1927.0 37.4 56.0#

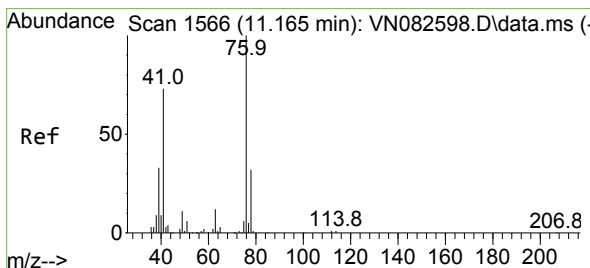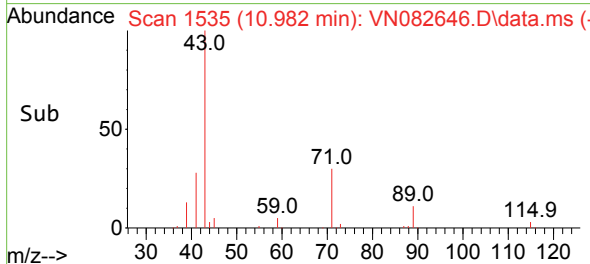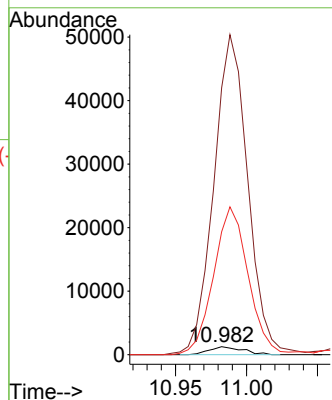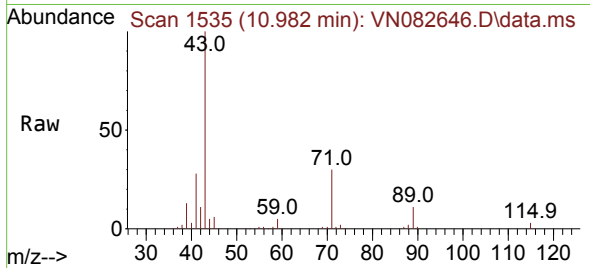

#57  
 1,3-Dichloropropane  
 Concen: 1.743 ug/l  
 RT: 11.206 min Scan# 1573  
 Delta R.T. 0.041 min  
 Lab File: VN082646.D  
 Acq: 19 Jun 2024 17:14

Tgt Ion: 76 Resp: 5487  
 Ion Ratio Lower Upper  
 76 100  
 78 1.0 25.6 38.4#


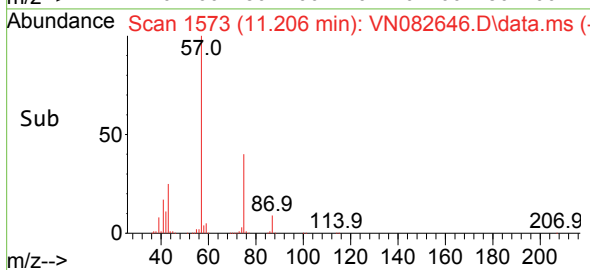
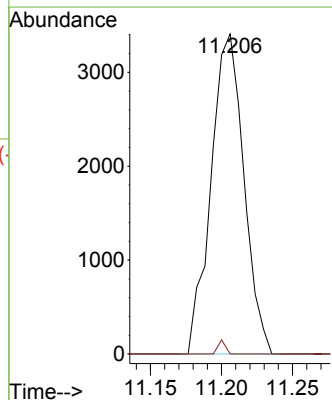
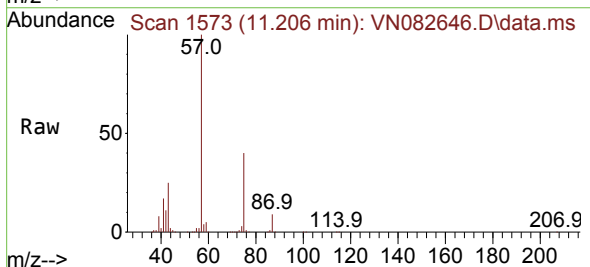




#59  
2-Hexanone  
Concen: 53.847 ug/l  
RT: 11.171 min Scan# 11  
Delta R.T. -0.029 min  
Lab File: VN082646.D  
Acq: 19 Jun 2024 17:14




Instrument :  
MSVOA\_N  
ClientSampleId :

Tgt Ion: 43 Resp: 125563  
Ion Ratio Lower Upper  
43 100  
58 0.0 24.6 73.8#

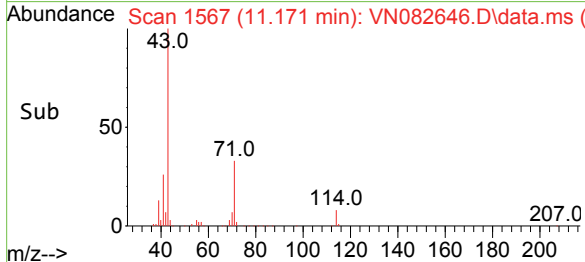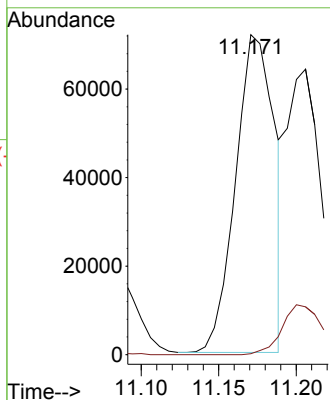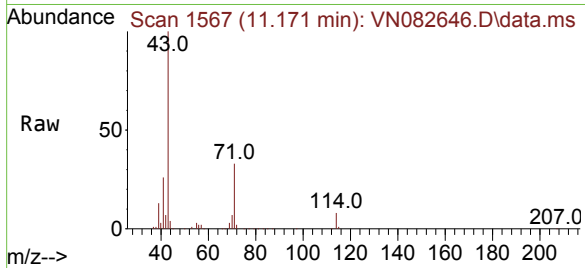


#62  
4-Bromofluorobenzene  
Concen: 48.371 ug/l  
RT: 12.853 min Scan# 1853  
Delta R.T. 0.006 min  
Lab File: VN082646.D  
Acq: 19 Jun 2024 17:14

Tgt Ion: 95 Resp: 106003  
Ion Ratio Lower Upper  
95 100  
174 79.8 0.0 159.2  
176 76.4 0.0 147.6

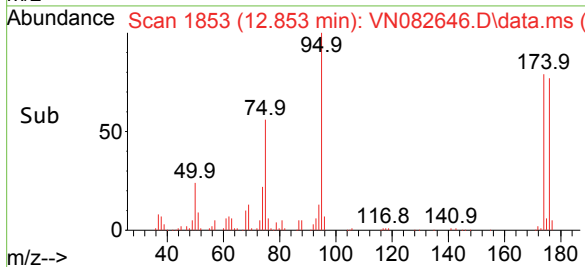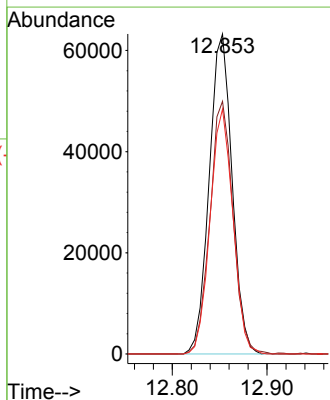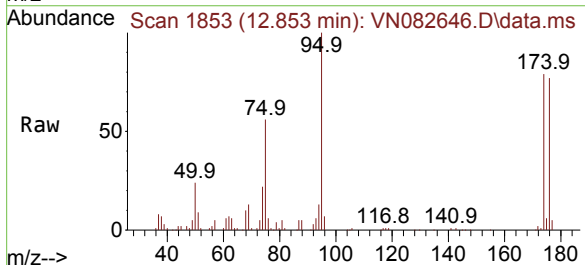









#63  
Chlorobenzene-d5  
Concen: 50.000 ug/l  
RT: 11.871 min Scan# 11  
Delta R.T. 0.000 min  
Lab File: VN082646.D  
Acq: 19 Jun 2024 17:14

Instrument :  
MSVOA\_N  
ClientSampleId :







Tgt Ion:117 Resp: 255358  
Ion Ratio Lower Upper  
117 100  
82 58.4 47.5 71.3  
119 31.2 25.6 38.4

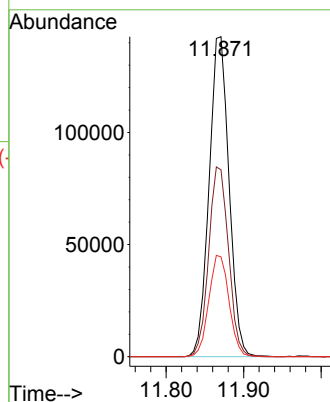

#71  
Bromoform  
Concen: 0.274 ug/l  
RT: 12.853 min Scan# 1853  
Delta R.T. 0.271 min  
Lab File: VN082646.D  
Acq: 19 Jun 2024 17:14

Tgt Ion:173 Resp: 453  
Ion Ratio Lower Upper  
173 100  
175 1207.3 24.0 72.0#  
254 0.0 0.0 0.0


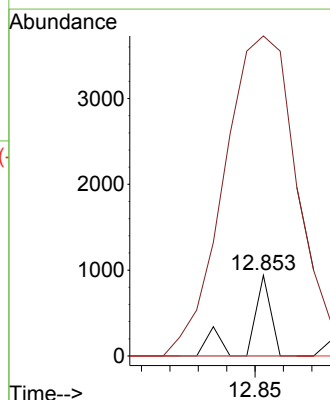
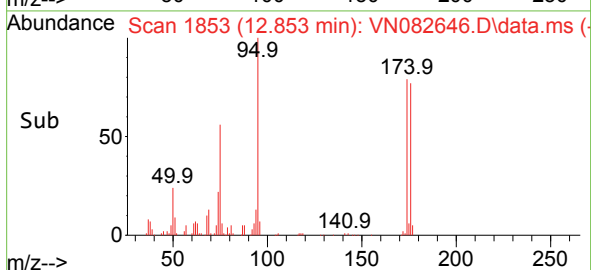



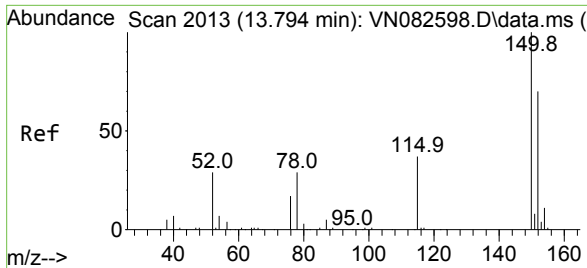

#72  
 1,4-Dichlorobenzene-d4  
 Concen: 50.000 ug/l  
 RT: 13.794 min Scan# 2013  
 Delta R.T. 0.000 min  
 Lab File: VN082646.D  
 Acq: 19 Jun 2024 17:14




Instrument :  
 MSVOA\_N  
 ClientSampleId :


Tgt Ion:152 Resp: 101359  
 Ion Ratio Lower Upper  
 152 100  
 115 59.9 30.6 91.6  
 150 155.8 0.0 348.6

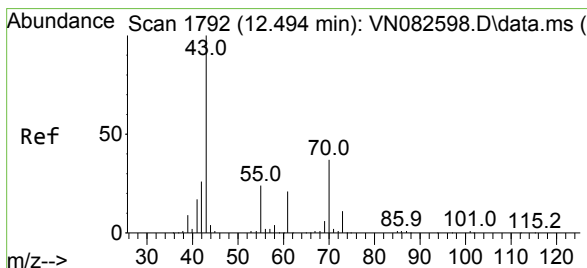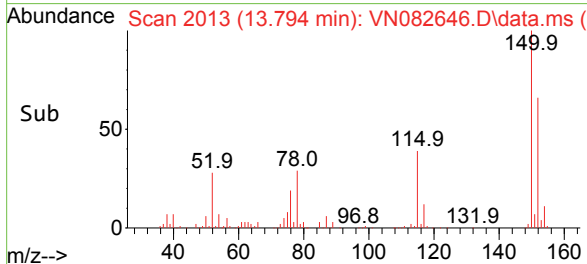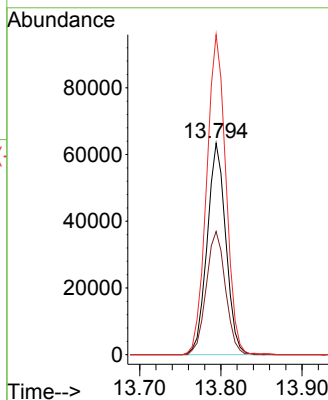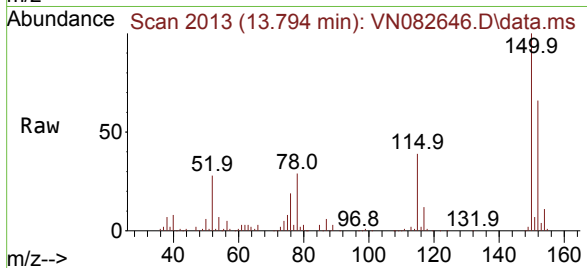

#74  
 N-ethyl acetate  
 Concen: 0.234 ug/l  
 RT: 12.494 min Scan# 1792  
 Delta R.T. 0.000 min  
 Lab File: VN082646.D  
 Acq: 19 Jun 2024 17:14

Tgt Ion: 43 Resp: 961  
 Ion Ratio Lower Upper  
 43 100  
 70 0.0 29.8 44.6#  
 55 0.0 18.7 28.1#  
 61 0.0 17.4 26.0#

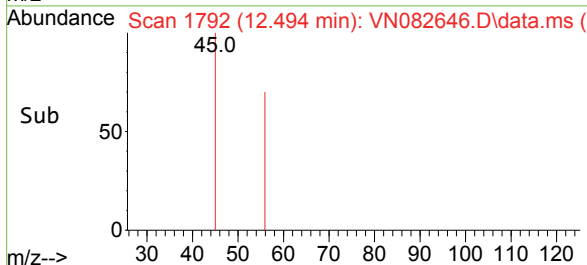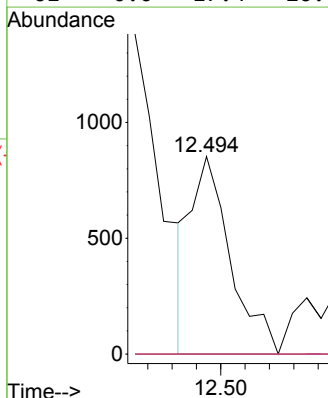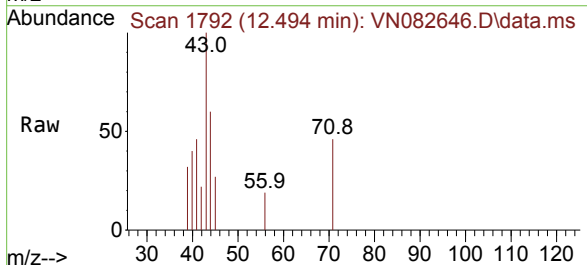



#76

1,2,3-Trichloropropane

Concen: 25.003 ug/l

RT: 12.853 min Scan# 1853

Delta R.T. -0.141 min

Lab File: VN082646.D

Acq: 19 Jun 2024 17:14

Instrument :

MSVOA\_N





ClientSampleId :

Tgt Ion: 75 Resp: 61985

Ion Ratio Lower Upper

75 100

77 1.3 110.9 332.6#

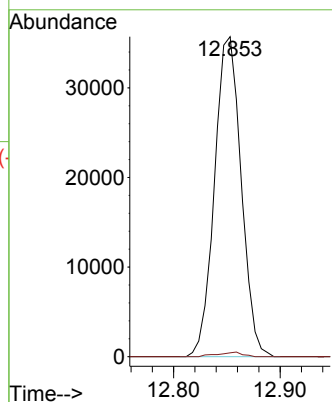

#81

trans-1,4-Dichloro-2-butene

Concen: 59.818 ug/l

RT: 12.853 min Scan# 1853

Delta R.T. 0.112 min

Lab File: VN082646.D

Acq: 19 Jun 2024 17:14

Tgt Ion: 75 Resp: 61985

Ion Ratio Lower Upper

75 100

53 0.0 88.4 132.6#

89 0.0 36.3 54.5#

