


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN061924\
Data File : VN082628.D
Acq On : 19 Jun 2024 09:18
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N061724W.M
Title : SW846 8260
Last Update : Tue Jun 18 04:52:44 2024

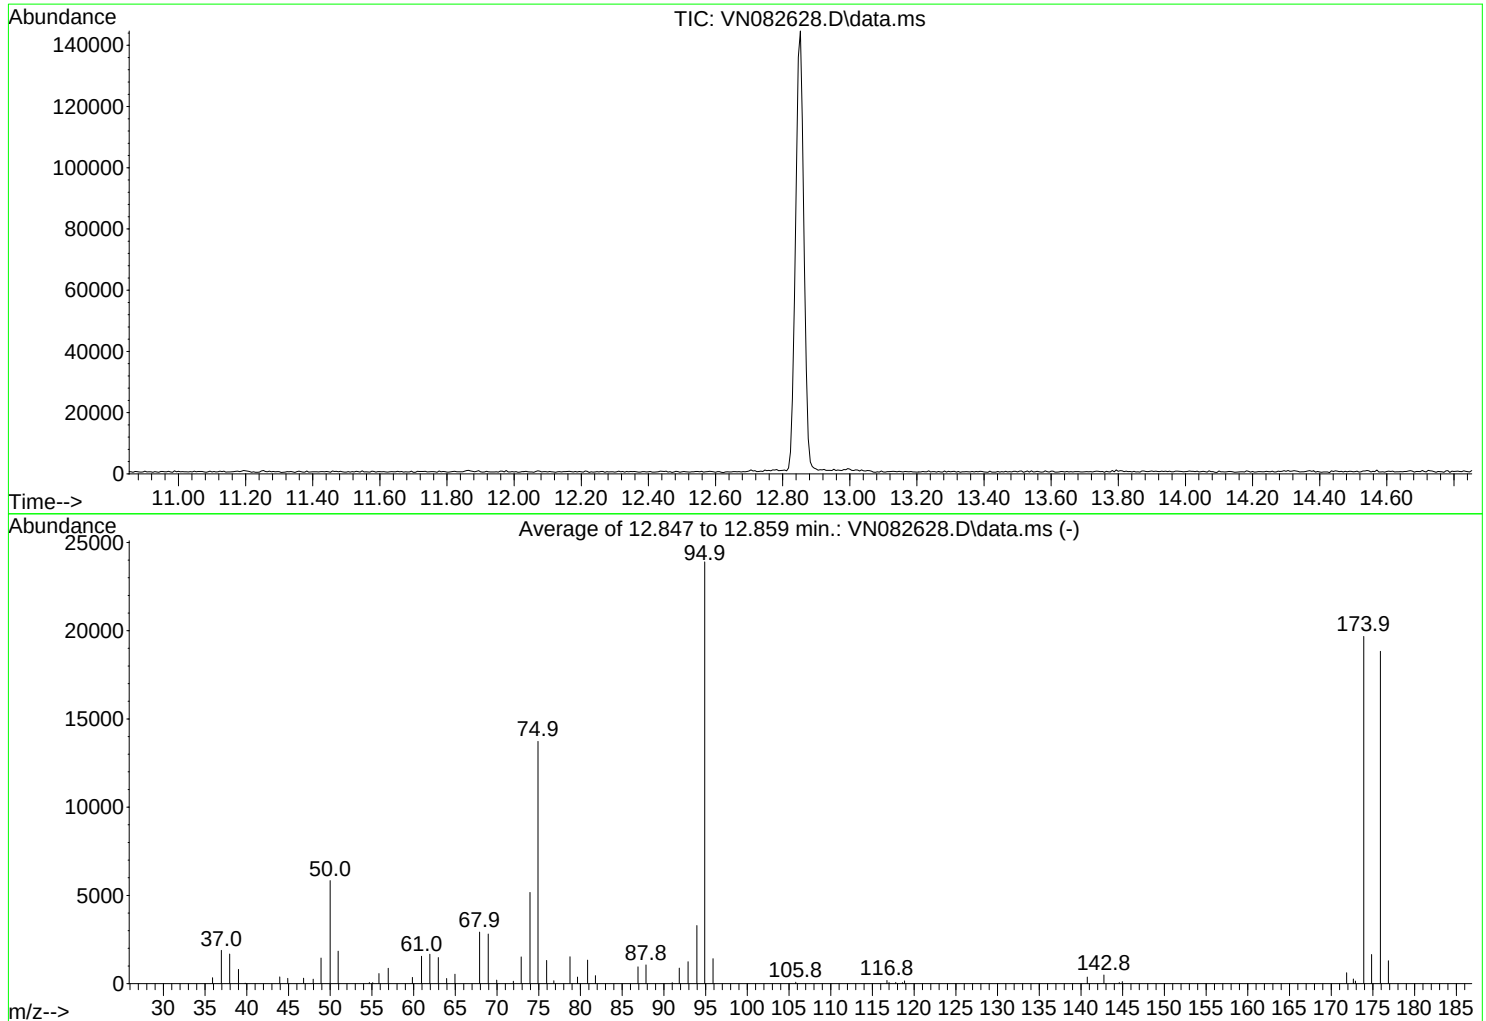

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1844

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	24.4	5837	PASS
75	95	30	60	57.4	13729	PASS
95	95	100	100	100.0	23901	PASS
96	95	5	9	5.9	1417	PASS
173	174	0.00	2	0.7	145	PASS
174	95	50	100	82.3	19675	PASS
175	174	5	9	8.4	1652	PASS
176	174	95	101	95.7	18827	PASS
177	176	5	9	6.9	1298	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.90	336	50.95	1840	67.90	2919	80.85	1331
36.95	1884	54.70	64	68.95	2808	81.80	45
37.95	1682	55.10	53	69.95	199	86.90	95
39.00	805	55.85	572	71.95	135	87.85	106
39.80	28	56.95	872	72.90	1518	91.00	57
43.95	383	59.85	350	73.95	5165	91.85	882
44.90	296	60.95	1550	74.90	13729	92.90	1242
46.80	305	61.95	1670	75.95	1319	93.95	3288
47.95	251	62.95	1474	76.80	161	94.90	23901
48.90	1453	63.95	286	78.75	1523	95.90	1417
50.00	5837	64.95	537	79.65	375	105.80	81

Average of 12.847 to 12.859 min.: VN082628.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
116.75	184	172.90	145				
117.00	62	173.90	19675				
117.80	70	174.85	1652				
118.60	54	175.90	18827				
118.85	151	176.85	1298				
140.75	376						
142.75	486						
144.60	63						
144.95	118						
171.85	616						
172.65	264						

Instrument :

MSVOA_N

ClientSampleId :

BFB