

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN061925\
 Data File : VN087114.D
 Acq On : 19 Jun 2025 16:07
 Operator : JC\MD
 Sample : Q2333-02DL 20X
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 MW-08DL

Quant Time: Jun 20 01:27:23 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N060625W.M
 Quant Title : SW846 8260
 QLast Update : Sat Jun 07 02:12:50 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.229	168	183164	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.106	114	368444	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.865	117	333195	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.788	152	162105	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.582	65	132607	54.073	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery = 108.140%			
35) Dibromofluoromethane	8.177	113	113205	51.846	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery = 103.700%			
50) Toluene-d8	10.570	98	452751	52.378	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery = 104.760%			
62) 4-Bromofluorobenzene	12.847	95	159857	49.777	ug/l	0.00
Spiked Amount 50.000	Range 77 - 121		Recovery = 99.560%			
Target Compounds						Qvalue
11) Tert butyl alcohol	5.553	59	136	0.204	ug/l #	73
13) Acrolein	4.447	56	67	0.318	ug/l #	15
16) Acetone	4.453	43	1307	1.005	ug/l #	40
18) Methyl Acetate	5.294	43	2458	0.649	ug/l #	49
19) Methyl tert-butyl Ether	5.824	73	6454	0.874	ug/l #	1
20) Methylene Chloride	5.300	84	615	0.253	ug/l #	53
31) Cyclohexane	8.271	56	11907	2.994	ug/l #	84
36) 1,1-Dichloropropene	8.235	75	13805	4.243	ug/l #	49
38) Carbon Tetrachloride	8.229	117	18371	5.751	ug/l #	16
39) Methylcyclohexane	9.600	83	5968	1.339	ug/l	89
40) Benzene	8.612	78	65863	6.190	ug/l	99
48) Methyl methacrylate	9.606	41	3065	1.002	ug/l #	77
52) Toluene	10.629	92	8768	1.349	ug/l	97
67) Ethyl Benzene	11.965	91	400804	31.664	ug/l	99
68) m/p-Xylenes	12.076	106	360555	74.410	ug/l	98
69) o-Xylene	12.394	106	155804	33.573	ug/l	96
70) Styrene	12.400	104	7626	0.960	ug/l #	1
71) Bromoform	12.847	173	408	0.233	ug/l #	1
73) Isopropylbenzene	12.694	105	26160	2.215	ug/l	100
76) 1,2,3-Trichloropropane	12.847	75	75683	19.641	ug/l #	1
78) n-propylbenzene	13.035	91	66168	4.610	ug/l	100
79) 2-Chlorotoluene	13.129	91	15391	1.788	ug/l #	42
80) 1,3,5-Trimethylbenzene	13.170	105	24397	2.502	ug/l	84
81) trans-1,4-Dichloro-2-b...	12.847	75	75683	45.213	ug/l #	16
82) 4-Chlorotoluene	13.170	91	2455	0.282	ug/l #	41
83) tert-Butylbenzene	13.482	119	68952	7.726	ug/l #	70
84) 1,2,4-Trimethylbenzene	13.482	105	559574	57.233	ug/l	99
85) sec-Butylbenzene	13.482	105	559075	43.135	ug/l #	56
86) p-Isopropyltoluene	13.676	119	4801	0.448	ug/l #	77
90) Hexachloroethane	14.323	117	5827	3.209	ug/l #	17
95) Naphthalene	15.635	128	244209	20.070	ug/l	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN061925\
Data File : VN087114.D
Acq On : 19 Jun 2025 16:07
Operator : JC\MD
Sample : Q2333-02DL 20X
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
MW-08DL

Quant Time: Jun 20 01:27:23 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N060625W.M
Quant Title : SW846 8260
QLast Update : Sat Jun 07 02:12:50 2025
Response via : Initial Calibration




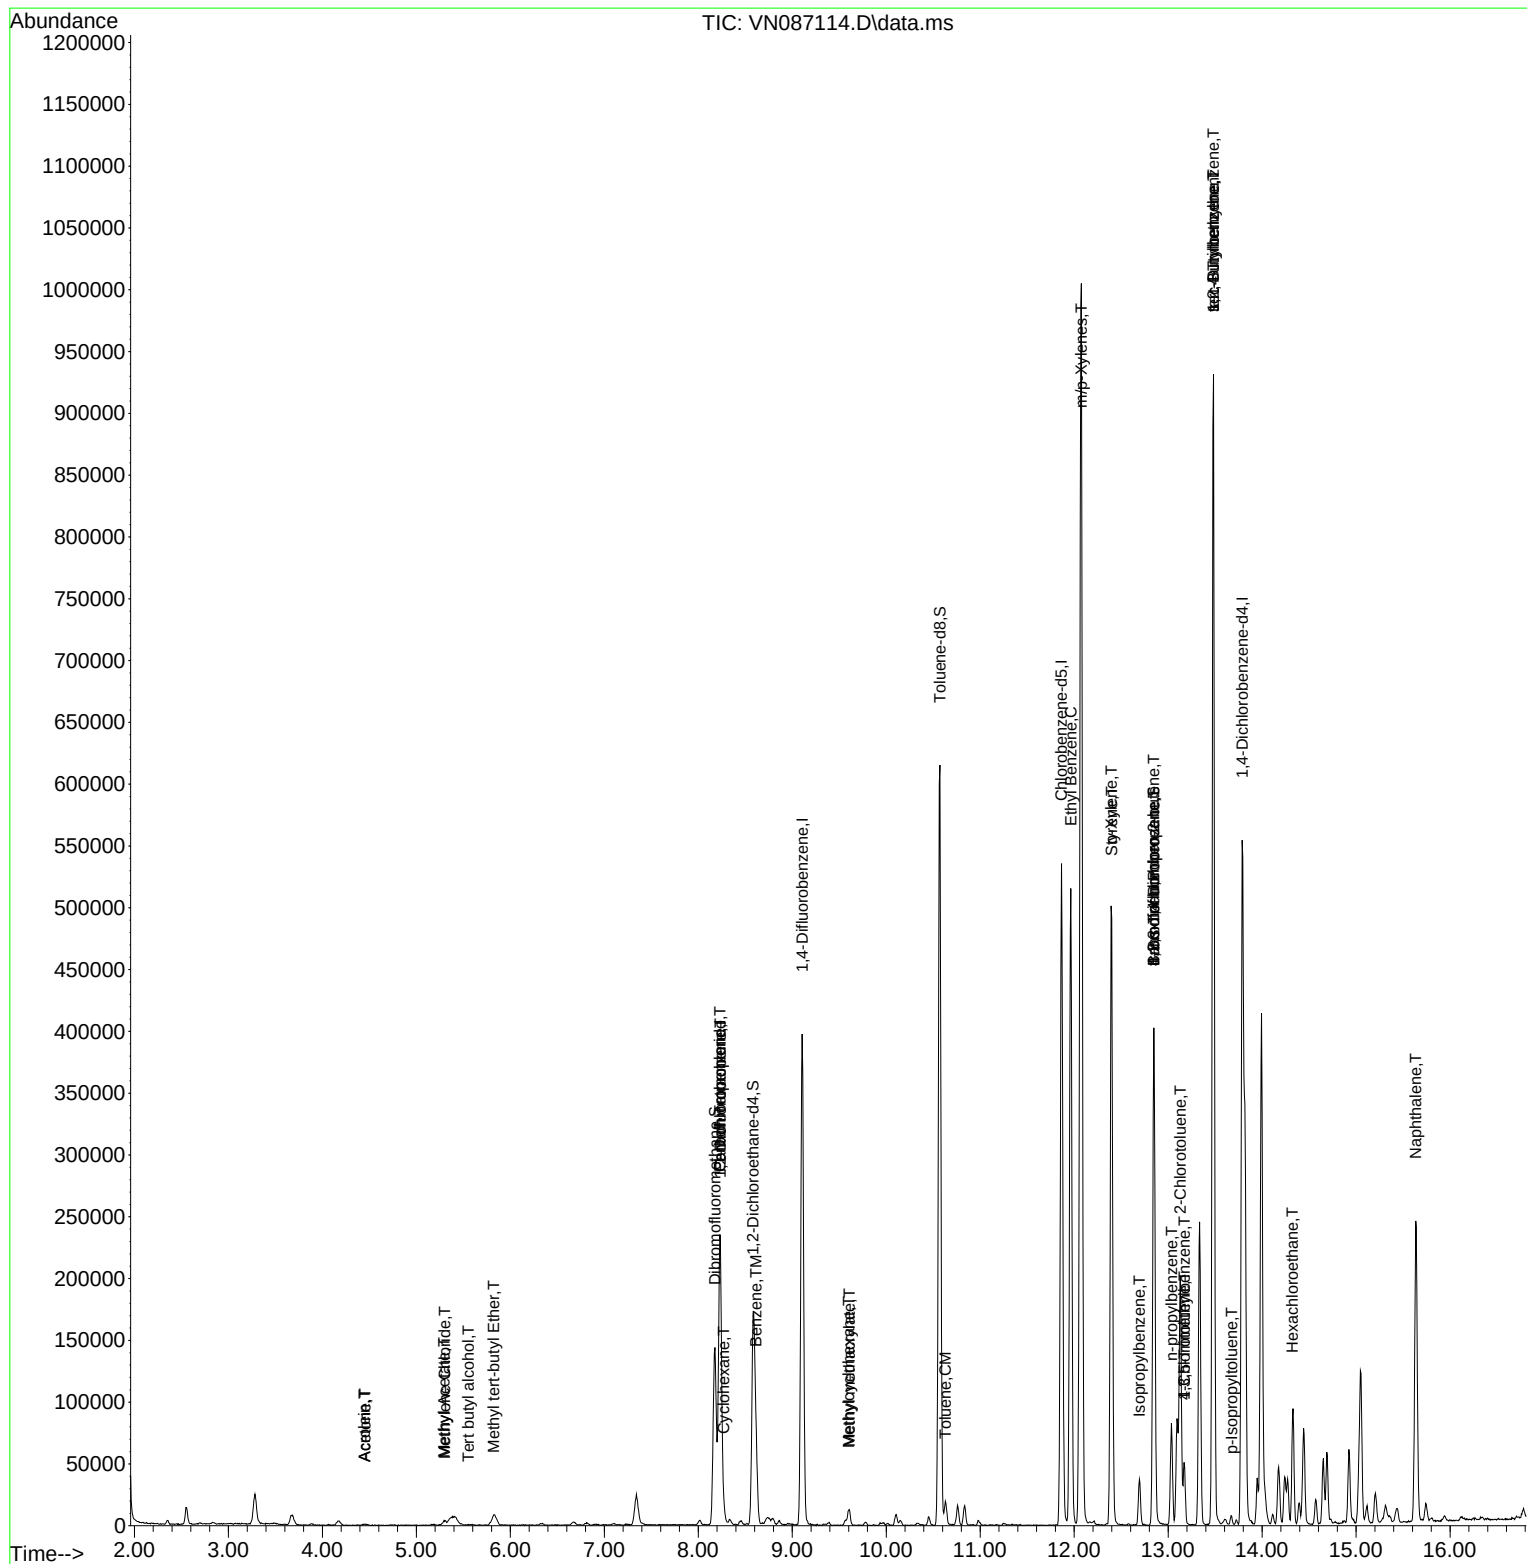


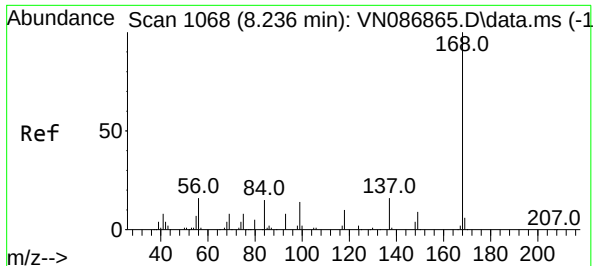

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.229 min Scan# 1067
Delta R.T. -0.007 min
Lab File: VN087114.D
Acq: 19 Jun 2025 16:07




Instrument :
MSVOA_N
ClientSampleId :
MW-08DL


Tgt Ion:168 Resp: 183164
Ion Ratio Lower Upper
168 100
99 57.7 49.1 73.7

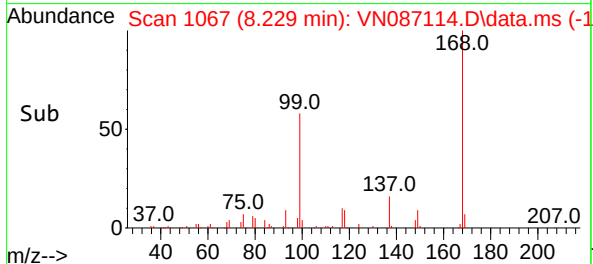

#11
Tert butyl alcohol
Concen: 0.204 ug/l
RT: 5.553 min Scan# 612
Delta R.T. 0.006 min
Lab File: VN087114.D
Acq: 19 Jun 2025 16:07

Tgt Ion: 59 Resp: 136
Ion Ratio Lower Upper
59 100
57 0.0 8.1 12.1#

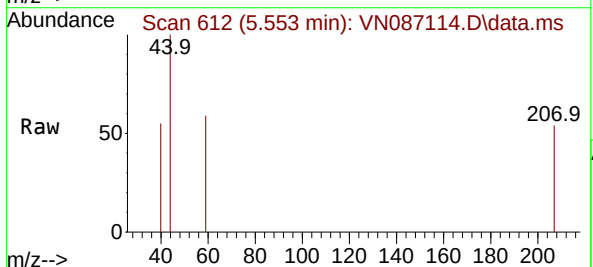



#13

Acrolein

Concen: 0.318 ug/l

RT: 4.447 min Scan# 41

Delta R.T. 0.247 min

Lab File: VN087114.D

Acq: 19 Jun 2025 16:07

Instrument :

MSVOA_N

ClientSampleId :





MW-08DL

Tgt Ion: 56 Resp: 67

Ion Ratio Lower Upper

56 100

55 0.0 55.6 83.4#

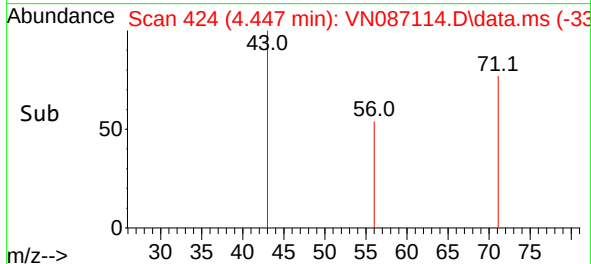

#16

Acetone

Concen: 1.005 ug/l

RT: 4.453 min Scan# 425

Delta R.T. 0.006 min

Lab File: VN087114.D




Acq: 19 Jun 2025 16:07


Tgt Ion: 43 Resp: 1307

Ion Ratio Lower Upper

43 100

58 0.0 28.0 42.0#


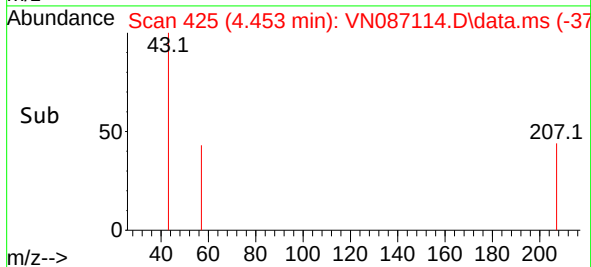

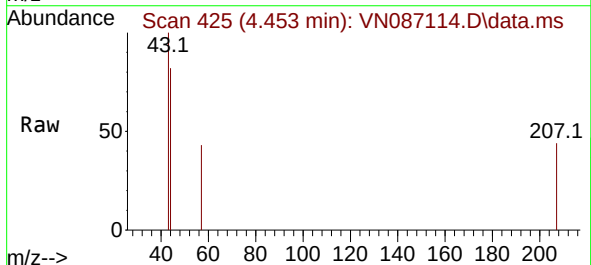




#18
Methyl Acetate
Concen: 0.649 ug/l
RT: 5.294 min Scan# 518
Delta R.T. 0.253 min
Lab File: VN087114.D
Acq: 19 Jun 2025 16:07




Instrument :
MSVOA_N
ClientSampleId :
MW-08DL


Tgt Ion: 43 Resp: 2458
Ion Ratio Lower Upper
43 100
74 0.0 20.7 31.1#

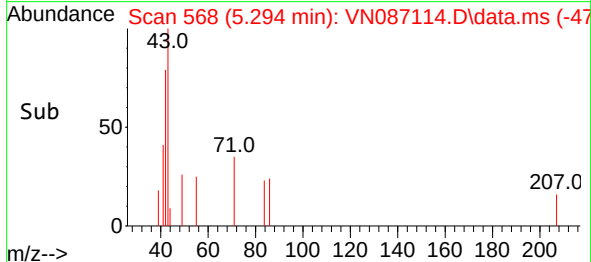

#19
Methyl tert-butyl Ether
Concen: 0.874 ug/l
RT: 5.824 min Scan# 658
Delta R.T. 0.012 min
Lab File: VN087114.D
Acq: 19 Jun 2025 16:07

Tgt Ion: 73 Resp: 6454
Ion Ratio Lower Upper
73 100
57 111.7 17.4 26.2#


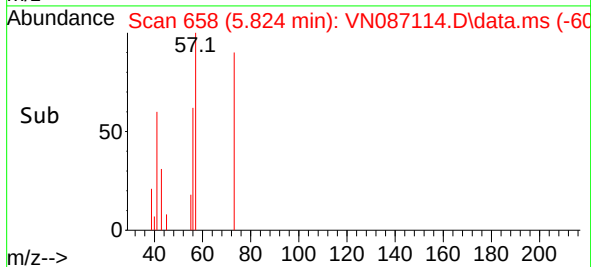

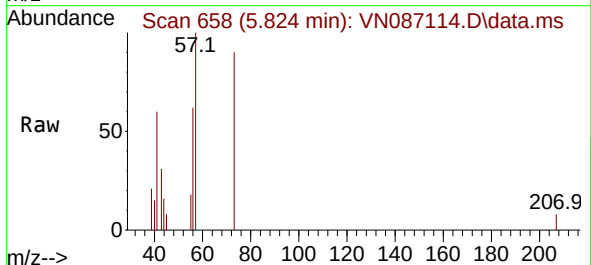




#20
Methylene Chloride
Concen: 0.253 ug/l
RT: 5.300 min Scan# 51
Delta R.T. 0.006 min
Lab File: VN087114.D
Acq: 19 Jun 2025 16:07




Instrument :
MSVOA_N
ClientSampleId :
MW-08DL


Tgt Ion:	84	Resp:	615
Ion	Ratio	Lower	Upper
84	100		
49	85.9	90.5	135.7#
51	0.0	28.5	42.7#
86	0.0	48.1	72.1#

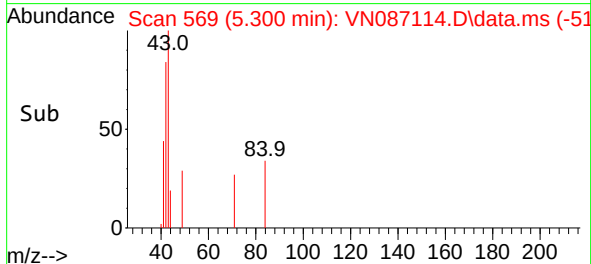

#31
Cyclohexane
Concen: 2.994 ug/l
RT: 8.271 min Scan# 1074
Delta R.T. -0.000 min
Lab File: VN087114.D
Acq: 19 Jun 2025 16:07

Tgt Ion:	56	Resp:	11907
Ion	Ratio	Lower	Upper
56	100		
69	50.2	25.4	38.0#
84	94.8	68.8	103.2

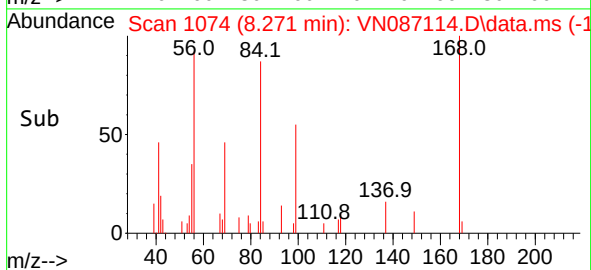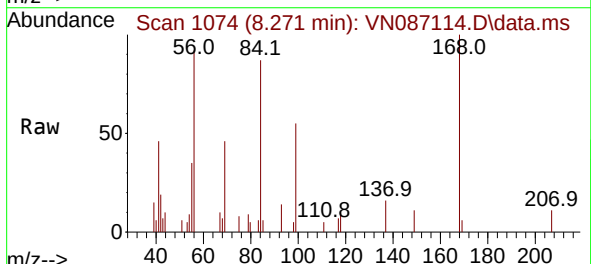

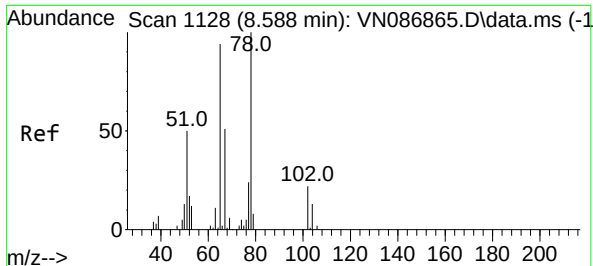

#33

1,2-Dichloroethane-d4

Concen: 54.073 ug/l

RT: 8.582 min Scan# 1128

Delta R.T. -0.006 min

Lab File: VN087114.D

Acq: 19 Jun 2025 16:07

Instrument :

MSVOA_N

ClientSampleId :





MW-08DL

Tgt Ion: 65 Resp: 132607

Ion Ratio Lower Upper

65 100

67 54.5 0.0 105.6

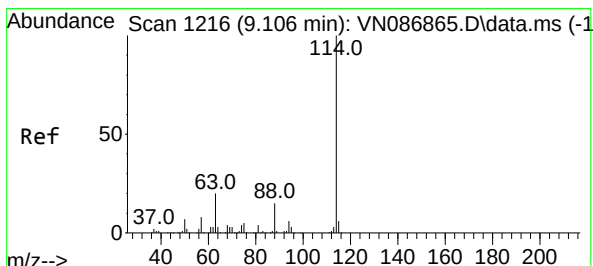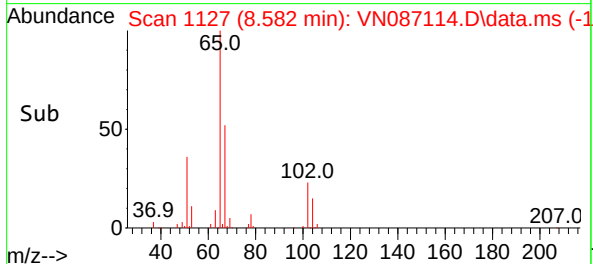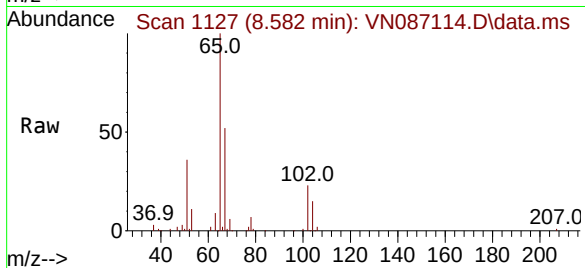

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.106 min Scan# 1216

Delta R.T. -0.000 min

Lab File: VN087114.D

Acq: 19 Jun 2025 16:07




Tgt Ion: 114 Resp: 368444


Ion Ratio Lower Upper

114 100

63 19.1 0.0 39.6

88 16.0 0.0 30.2



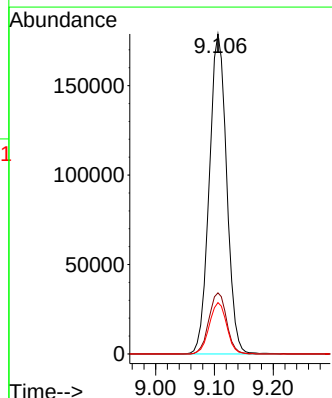
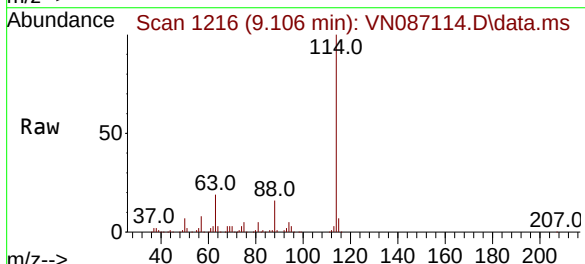


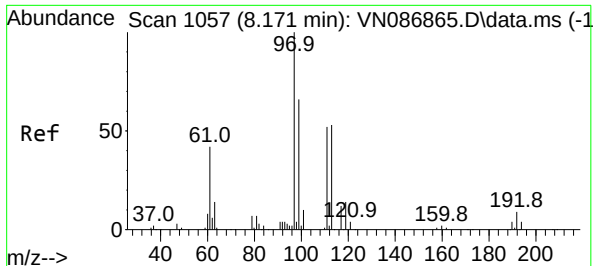

#35
Dibromofluoromethane
Concen: 51.846 ug/l
RT: 8.177 min Scan# 1057
Delta R.T. 0.006 min
Lab File: VN087114.D
Acq: 19 Jun 2025 16:07




Instrument :
MSVOA_N
ClientSampleId :
MW-08DL


Tgt Ion:113 Resp: 113205
Ion Ratio Lower Upper
113 100
111 101.8 84.2 126.2
192 18.2 14.2 21.4

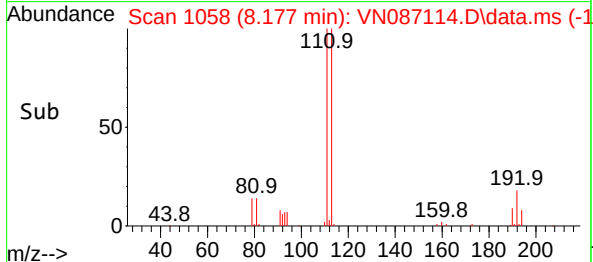

#36
1,1-Dichloropropene
Concen: 4.243 ug/l
RT: 8.235 min Scan# 1068
Delta R.T. -0.141 min
Lab File: VN087114.D
Acq: 19 Jun 2025 16:07

Tgt Ion: 75 Resp: 13805
Ion Ratio Lower Upper
75 100
110 8.2 17.6 52.9#
77 0.0 25.3 37.9#


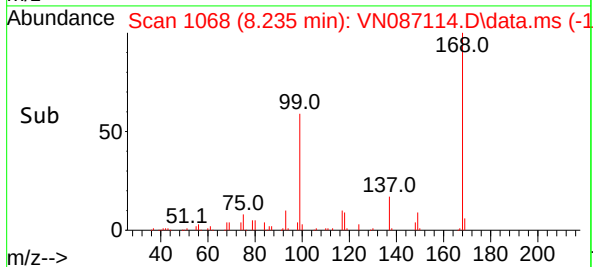

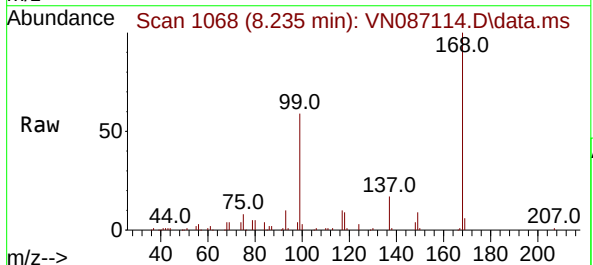


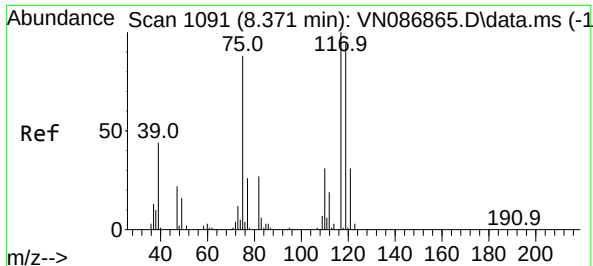

#38
Carbon Tetrachloride
Concen: 5.751 ug/l
RT: 8.229 min Scan# 1067
Delta R.T. -0.141 min
Lab File: VN087114.D
Acq: 19 Jun 2025 16:07




Instrument :
MSVOA_N
ClientSampleId :
MW-08DL


Tgt Ion:117 Resp: 18371
Ion Ratio Lower Upper
117 100
119 3.8 75.0 112.6#
121 0.0 24.9 37.3#

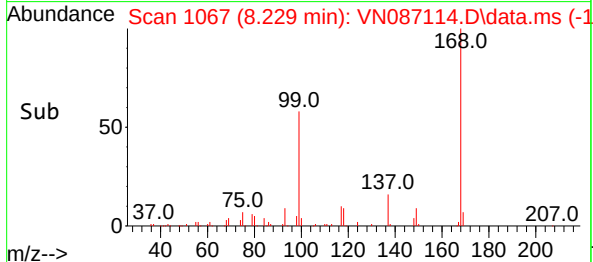

#39
Methylcyclohexane
Concen: 1.339 ug/l
RT: 9.600 min Scan# 1300
Delta R.T. -0.006 min
Lab File: VN087114.D
Acq: 19 Jun 2025 16:07

Tgt Ion: 83 Resp: 5968
Ion Ratio Lower Upper
83 100
55 63.6 61.0 91.6
98 45.7 38.9 58.3


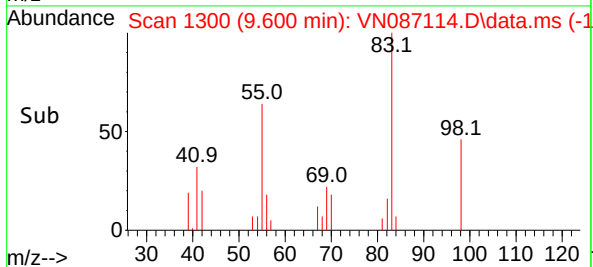

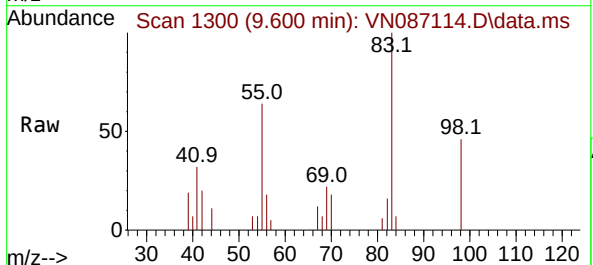


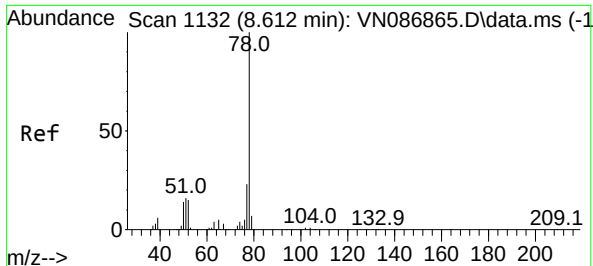

#40
Benzene
Concen: 6.190 ug/l
RT: 8.612 min Scan# 1132
Delta R.T. -0.000 min
Lab File: VN087114.D
Acq: 19 Jun 2025 16:07




Instrument :
MSVOA_N
ClientSampleId :
MW-08DL


Tgt Ion: 78 Resp: 65863
Ion Ratio Lower Upper
78 100
77 23.8 18.7 28.1

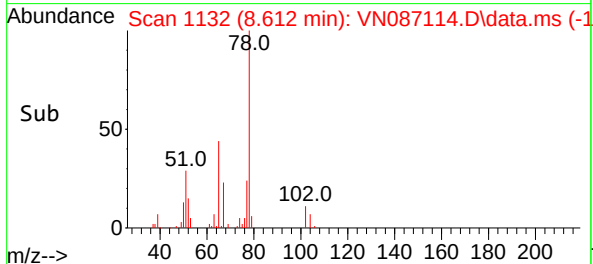

#48
Methyl methacrylate
Concen: 1.002 ug/l
RT: 9.606 min Scan# 1301
Delta R.T. -0.077 min
Lab File: VN087114.D
Acq: 19 Jun 2025 16:07

Tgt Ion: 41 Resp: 3065
Ion Ratio Lower Upper
41 100
69 60.0 74.6 112.0#
39 49.9 40.2 60.4


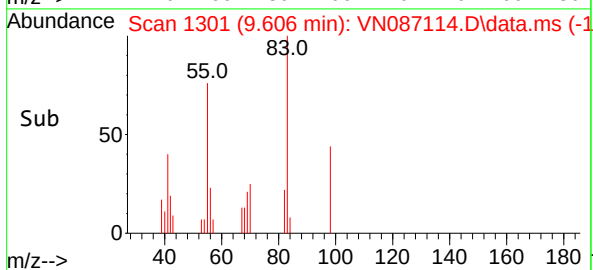

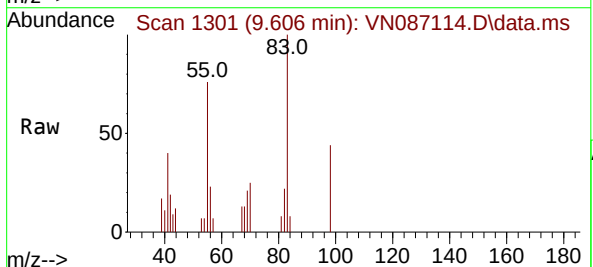




#50
Toluene-d8
Concen: 52.378 ug/l
RT: 10.570 min Scan# 1465
Delta R.T. -0.000 min
Lab File: VN087114.D
Acq: 19 Jun 2025 16:07




Instrument :
MSVOA_N
ClientSampleId :
MW-08DL


Tgt Ion: 98 Resp: 452751
Ion Ratio Lower Upper
98 100
100 66.4 53.4 80.0

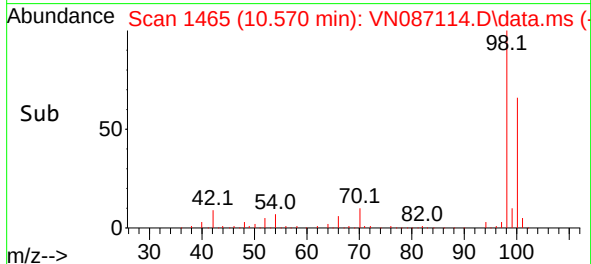

#52
Toluene
Concen: 1.349 ug/l
RT: 10.629 min Scan# 1475
Delta R.T. -0.006 min
Lab File: VN087114.D
Acq: 19 Jun 2025 16:07

Tgt Ion: 92 Resp: 8768
Ion Ratio Lower Upper
92 100
91 174.9 136.5 204.7


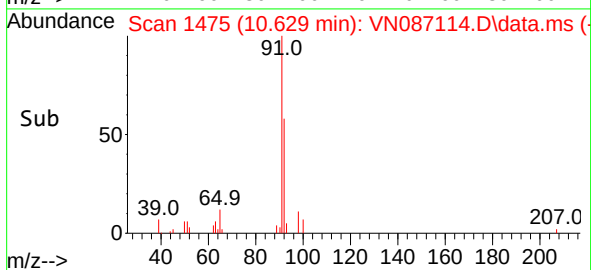

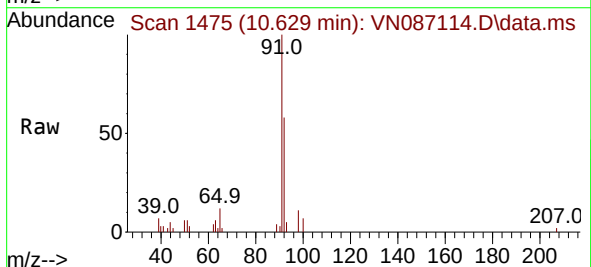




#62
4-Bromofluorobenzene
Concen: 49.777 ug/l
RT: 12.847 min Scan# 1852
Delta R.T. -0.000 min
Lab File: VN087114.D
Acq: 19 Jun 2025 16:07




Instrument :
MSVOA_N
ClientSampleId :
MW-08DL


Tgt Ion: 95 Resp: 159857
Ion Ratio Lower Upper
95 100
174 73.0 0.0 141.8
176 70.4 0.0 132.6

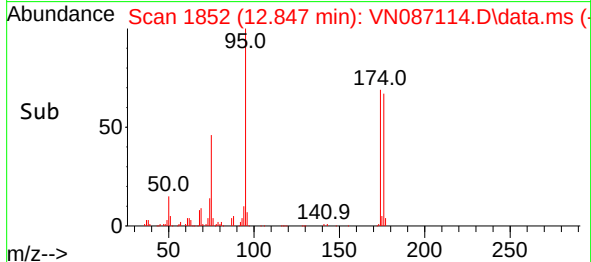

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.865 min Scan# 1685
Delta R.T. -0.000 min
Lab File: VN087114.D
Acq: 19 Jun 2025 16:07

Tgt Ion: 117 Resp: 333195
Ion Ratio Lower Upper
117 100
82 55.0 44.6 67.0
119 32.5 25.5 38.3

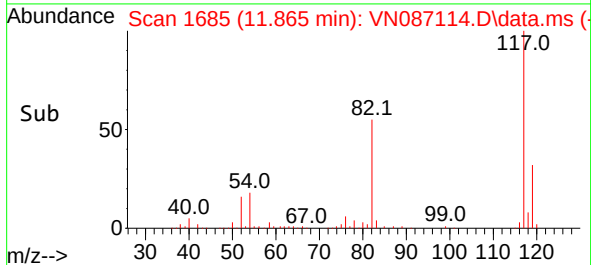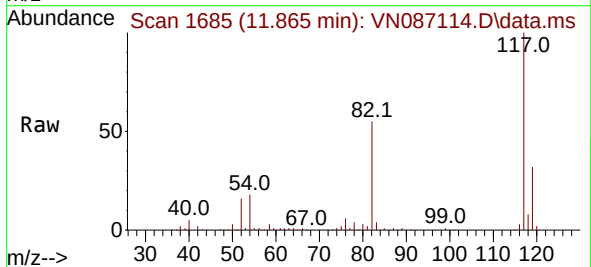



#67

Ethyl Benzene

Concen: 31.664 ug/l

RT: 11.965 min Scan# 1702

Delta R.T. -0.000 min

Lab File: VN087114.D

Acq: 19 Jun 2025 16:07

Instrument :

MSVOA_N

ClientSampleId :





MW-08DL

Tgt Ion: 91 Resp: 400804

Ion Ratio Lower Upper

91 100

106 31.3 25.4 38.2

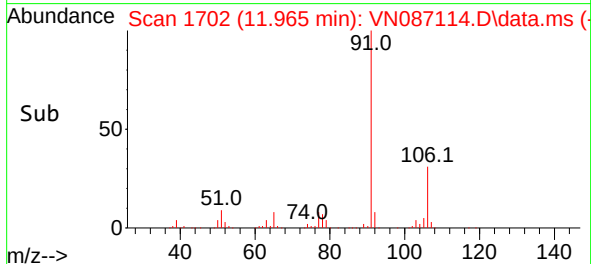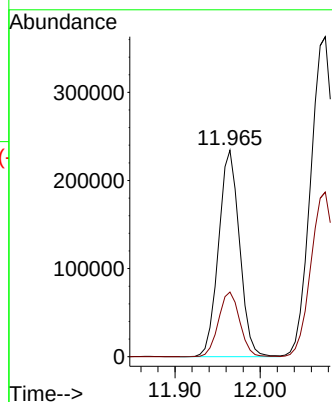

#68

m/p-Xylenes

Concen: 74.410 ug/l

RT: 12.076 min Scan# 1721

Delta R.T. 0.006 min

Lab File: VN087114.D




Acq: 19 Jun 2025 16:07


Tgt Ion:106 Resp: 360555

Ion Ratio Lower Upper

106 100

91 195.8 159.4 239.0

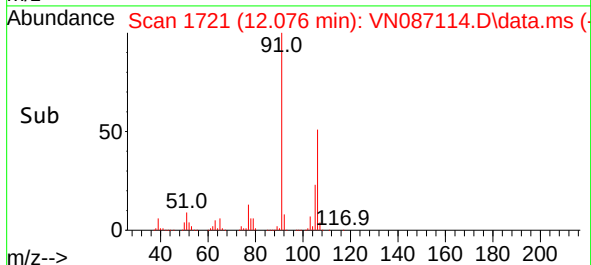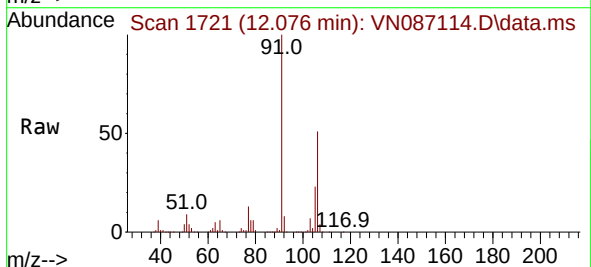



#69

o-Xylene

Concen: 33.573 ug/l

RT: 12.394 min Scan# 1775

Delta R.T. -0.006 min

Lab File: VN087114.D

Acq: 19 Jun 2025 16:07

Instrument :

MSVOA_N

ClientSampleId :





MW-08DL

Tgt Ion:106 Resp: 155804

Ion Ratio Lower Upper

106 100

91 205.7 106.1 318.1

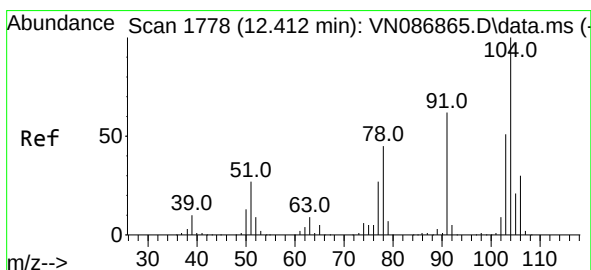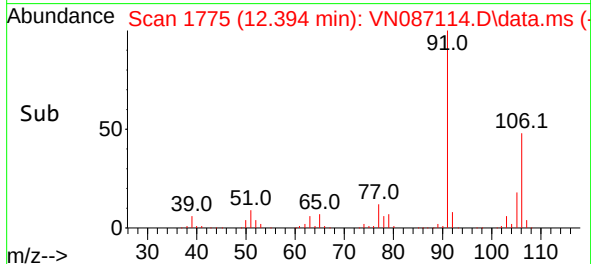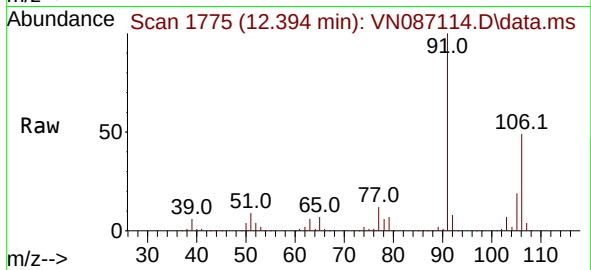

#70

Styrene

Concen: 0.960 ug/l

RT: 12.400 min Scan# 1776

Delta R.T. -0.012 min

Lab File: VN087114.D

Acq: 19 Jun 2025 16:07




Tgt Ion:104 Resp: 7626


Ion Ratio Lower Upper

104 100

78 268.9 38.5 57.7#

103 271.6 43.1 64.7#


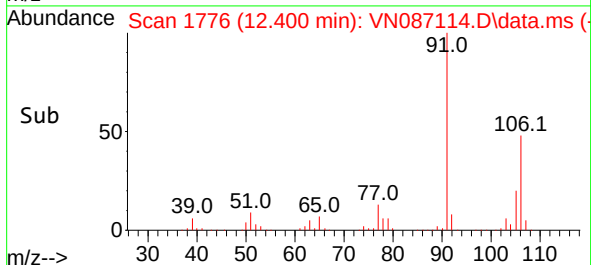
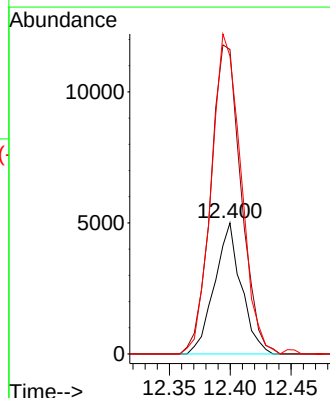
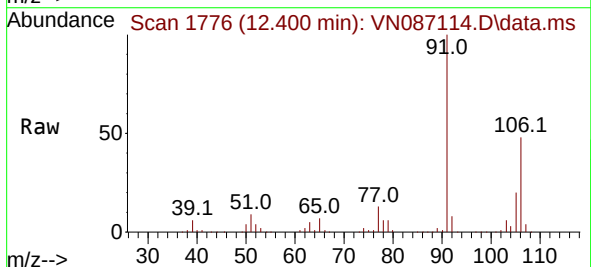




#71
Bromoform
Concen: 0.233 ug/l
RT: 12.847 min Scan# 11
Delta R.T. 0.264 min
Lab File: VN087114.D
Acq: 19 Jun 2025 16:07




Instrument :
MSVOA_N
ClientSampleId :
MW-08DL


Tgt Ion:173 Resp: 408
Ion Ratio Lower Upper
173 100
175 1837.5 24.1 72.4#
254 0.0 0.0 0.0

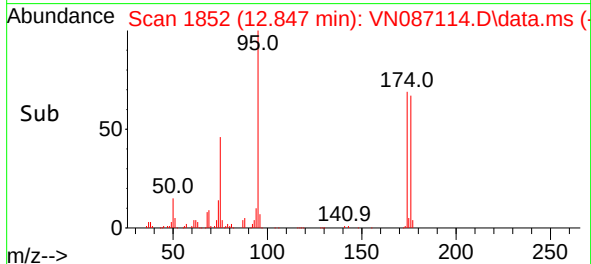

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.788 min Scan# 2012
Delta R.T. -0.006 min
Lab File: VN087114.D
Acq: 19 Jun 2025 16:07

Tgt Ion:152 Resp: 162105
Ion Ratio Lower Upper
152 100
115 64.6 30.1 90.5
150 157.3 0.0 345.0

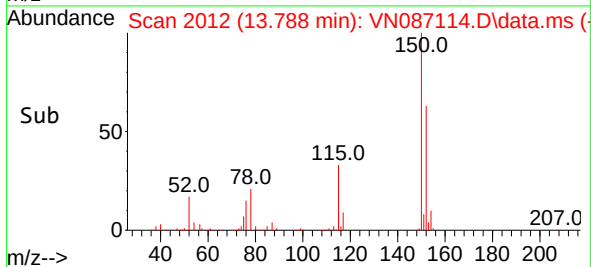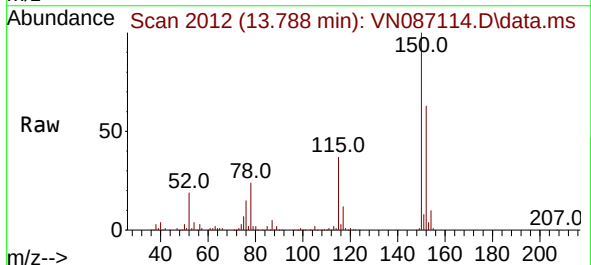

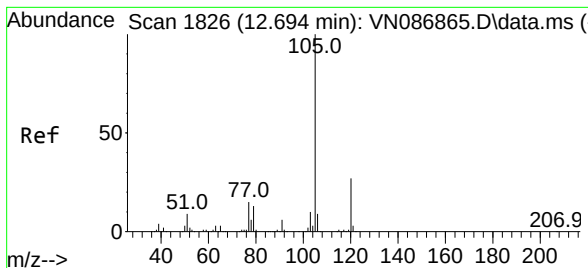

#73

Isopropylbenzene

Concen: 2.215 ug/l

RT: 12.694 min Scan# 1826

Delta R.T. -0.000 min

Lab File: VN087114.D

Acq: 19 Jun 2025 16:07

Instrument :

MSVOA_N

ClientSampleId :





MW-08DL

Tgt Ion:105 Resp: 26160

Ion Ratio Lower Upper

105 100

120 27.0 13.5 40.4

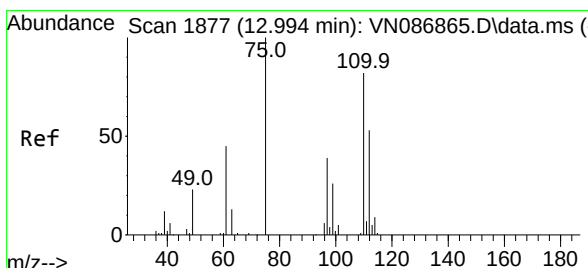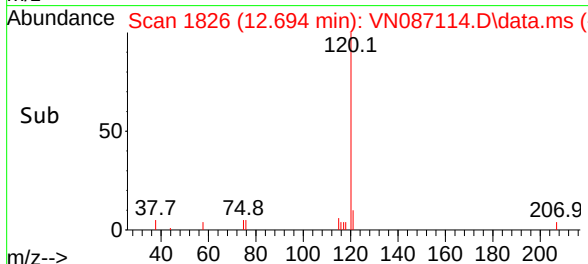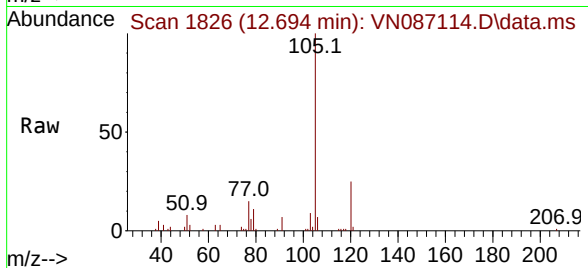

#76

1,2,3-Trichloropropane

Concen: 19.641 ug/l

RT: 12.847 min Scan# 1852

Delta R.T. -0.147 min

Lab File: VN087114.D




Acq: 19 Jun 2025 16:07


Tgt Ion: 75 Resp: 75683

Ion Ratio Lower Upper

75 100

77 1.5 79.3 237.9#


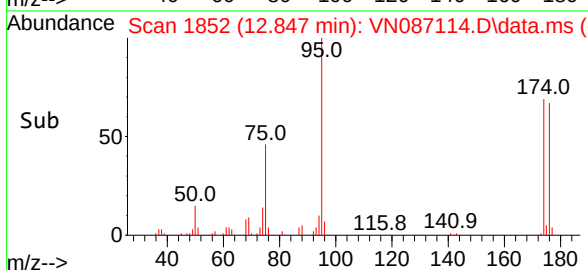

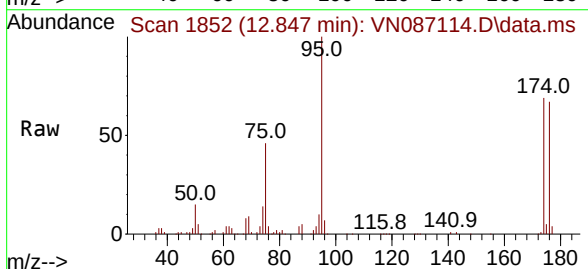


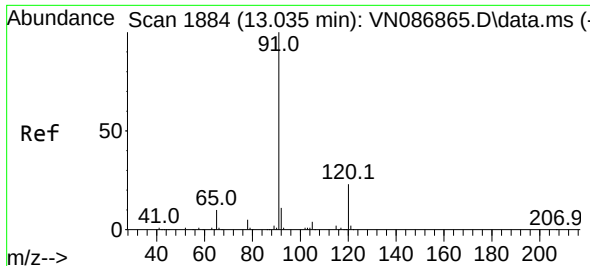

#78
n-propylbenzene
Concen: 4.610 ug/l
RT: 13.035 min Scan# 11
Delta R.T. -0.000 min
Lab File: VN087114.D
Acq: 19 Jun 2025 16:07




Instrument :
MSVOA_N
ClientSampleId :
MW-08DL


Tgt Ion: 91 Resp: 66168
Ion Ratio Lower Upper
91 100
120 22.7 11.4 34.2

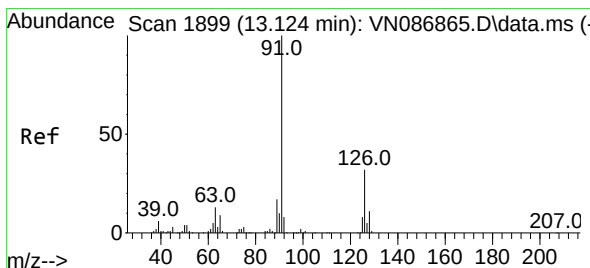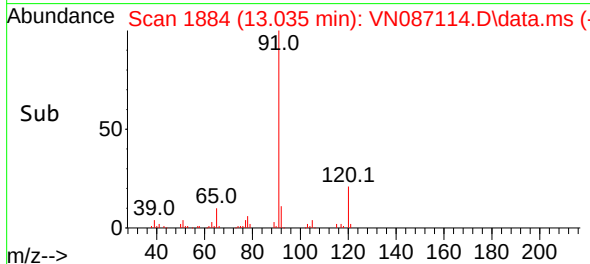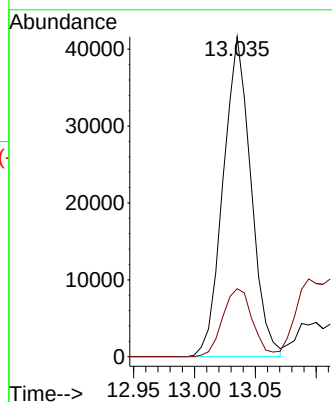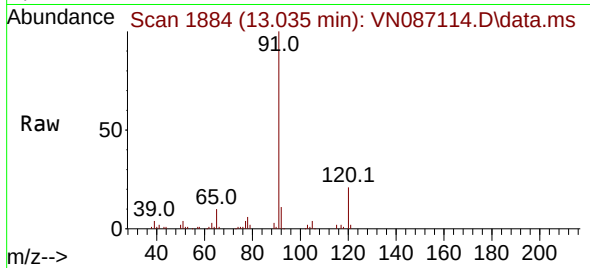

#79
2-Chlorotoluene
Concen: 1.788 ug/l
RT: 13.129 min Scan# 1900
Delta R.T. 0.006 min
Lab File: VN087114.D
Acq: 19 Jun 2025 16:07

Tgt Ion: 91 Resp: 15391
Ion Ratio Lower Upper
91 100
126 0.0 16.2 48.5#


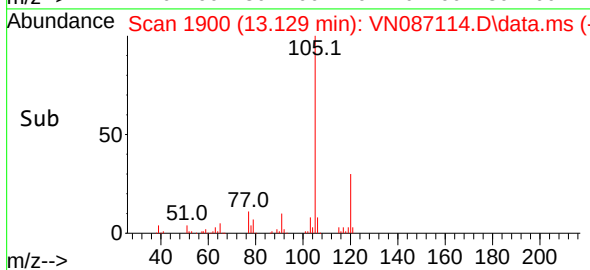
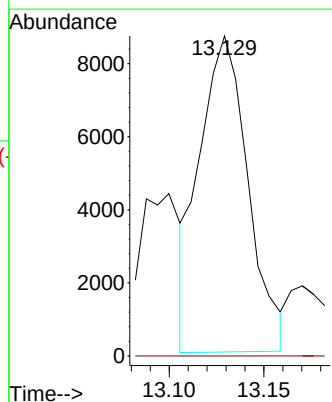
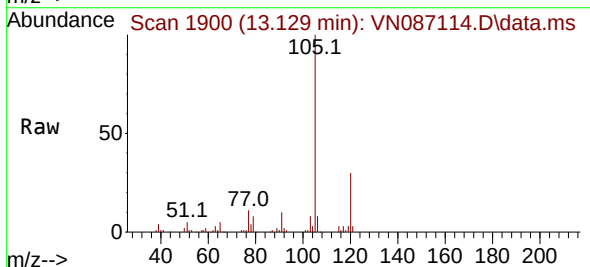




#80
1,3,5-Trimethylbenzene
Concen: 2.502 ug/l
RT: 13.170 min Scan# 1907
Delta R.T. -0.000 min
Lab File: VN087114.D
Acq: 19 Jun 2025 16:07




Instrument :
MSVOA_N
ClientSampleId :
MW-08DL


Tgt Ion:105 Resp: 24397
Ion Ratio Lower Upper
105 100
120 60.6 24.9 74.6

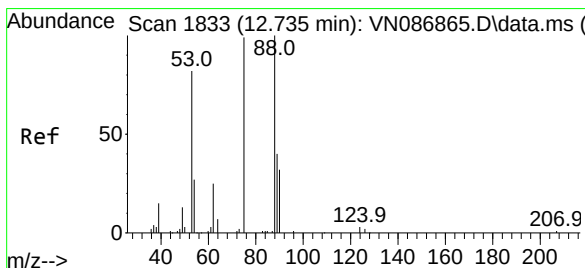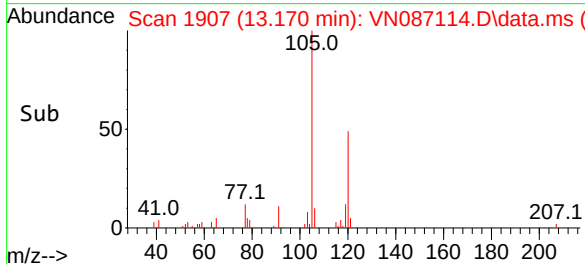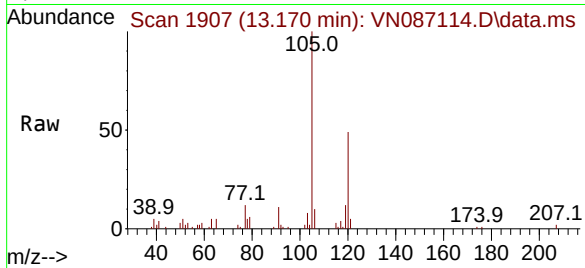

#81
trans-1,4-Dichloro-2-butene
Concen: 45.213 ug/l
RT: 12.847 min Scan# 1852
Delta R.T. 0.112 min
Lab File: VN087114.D
Acq: 19 Jun 2025 16:07

Tgt Ion: 75 Resp: 75683
Ion Ratio Lower Upper
75 100
53 0.0 66.6 99.8#
89 0.0 36.7 55.1#


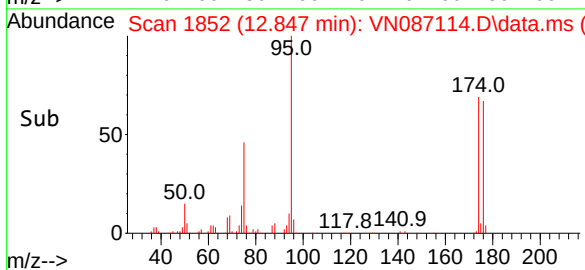

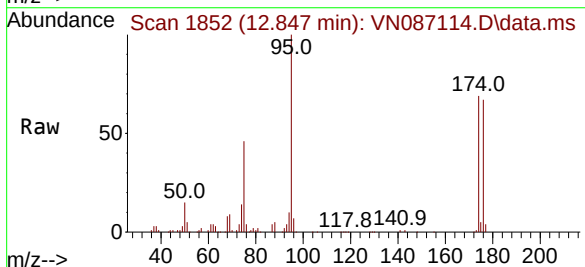




#82
4-Chlorotoluene
Concen: 0.282 ug/l
RT: 13.170 min Scan# 1916
Delta R.T. -0.053 min
Lab File: VN087114.D
Acq: 19 Jun 2025 16:07




Instrument :
MSVOA_N
ClientSampleId :
MW-08DL


Tgt Ion: 91 Resp: 2455
Ion Ratio Lower Upper
91 100
126 0.0 16.7 50.1#

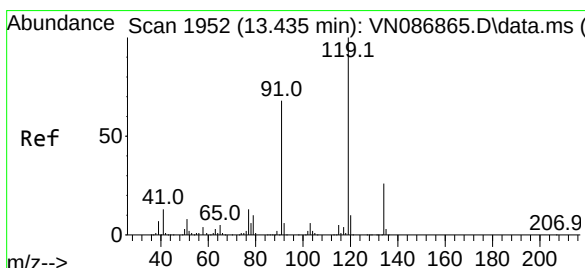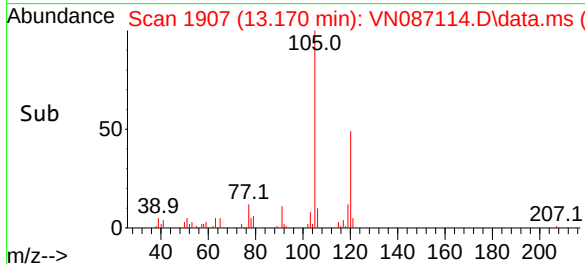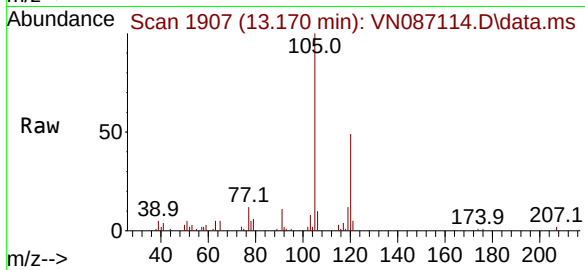

#83
tert-Butylbenzene
Concen: 7.726 ug/l
RT: 13.482 min Scan# 1960
Delta R.T. 0.047 min
Lab File: VN087114.D
Acq: 19 Jun 2025 16:07

Tgt Ion: 119 Resp: 68952
Ion Ratio Lower Upper
119 100
91 80.5 32.1 96.5
134 0.0 13.4 40.1#


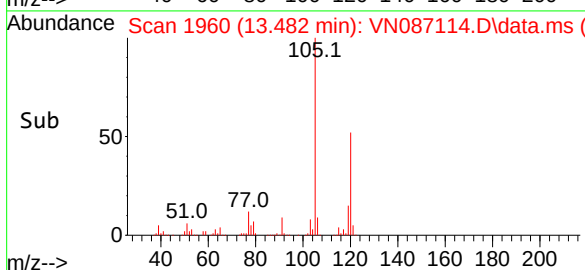

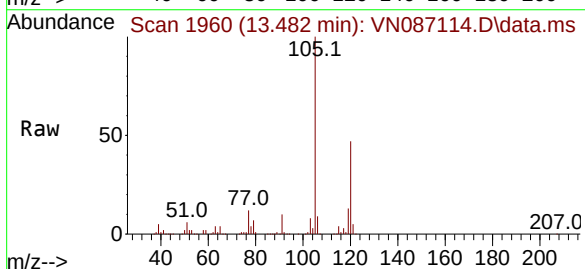




#84
 1,2,4-Trimethylbenzene
 Concen: 57.233 ug/l
 RT: 13.482 min Scan# 1960
 Delta R.T. -0.000 min
 Lab File: VN087114.D
 Acq: 19 Jun 2025 16:07




Instrument :
 MSVOA_N
 ClientSampleId :
 MW-08DL


Tgt Ion:105 Resp: 559574
 Ion Ratio Lower Upper
 105 100
 120 46.9 23.2 69.6

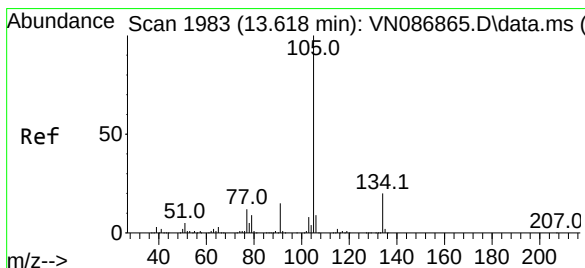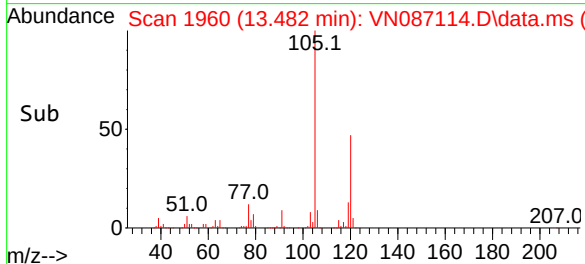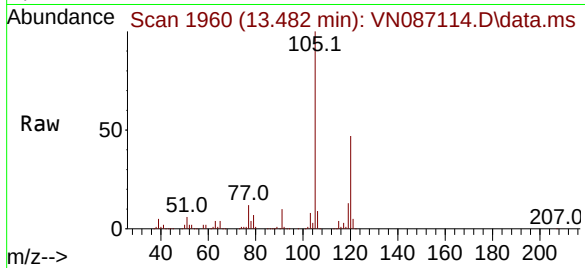

#85
 sec-Butylbenzene
 Concen: 43.135 ug/l
 RT: 13.482 min Scan# 1960
 Delta R.T. -0.136 min
 Lab File: VN087114.D
 Acq: 19 Jun 2025 16:07

Tgt Ion:105 Resp: 559075
 Ion Ratio Lower Upper
 105 100
 134 0.0 10.0 30.0#


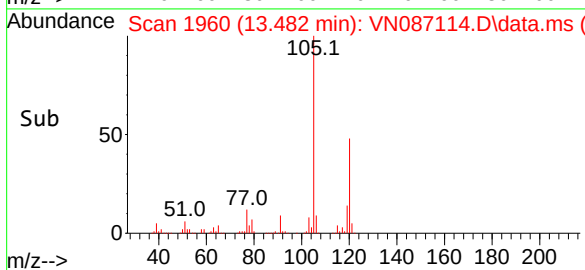

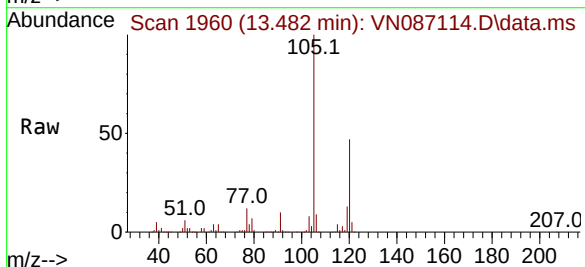




#86
p-Isopropyltoluene
Concen: 0.448 ug/l
RT: 13.676 min Scan# 1993
Delta R.T. -0.053 min
Lab File: VN087114.D
Acq: 19 Jun 2025 16:07




Instrument :
MSVOA_N
ClientSampleId :
MW-08DL


Tgt Ion:119 Resp: 4801
Ion Ratio Lower Upper
119 100
134 25.8 13.5 40.4
91 0.0 11.5 34.4#

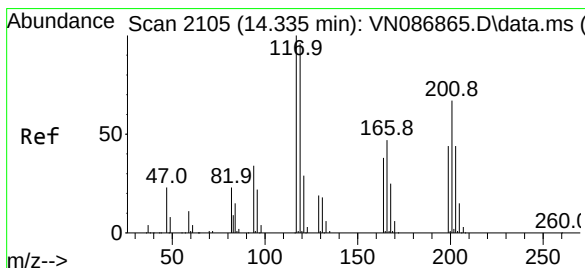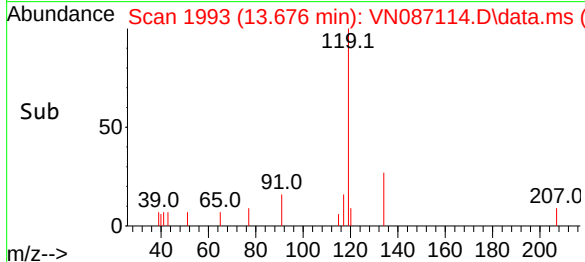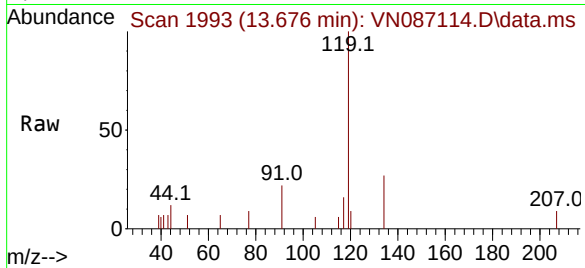

#90
Hexachloroethane
Concen: 3.209 ug/l
RT: 14.323 min Scan# 2103
Delta R.T. -0.012 min
Lab File: VN087114.D
Acq: 19 Jun 2025 16:07


Tgt Ion:117 Resp: 5827
Ion Ratio Lower Upper
117 100
201 0.0 33.2 99.6#

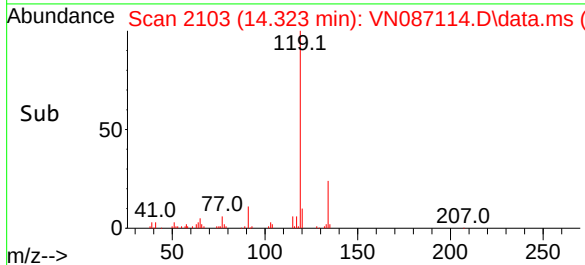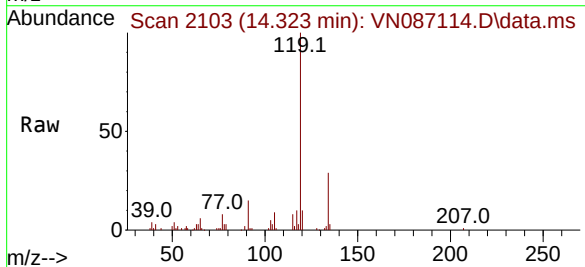

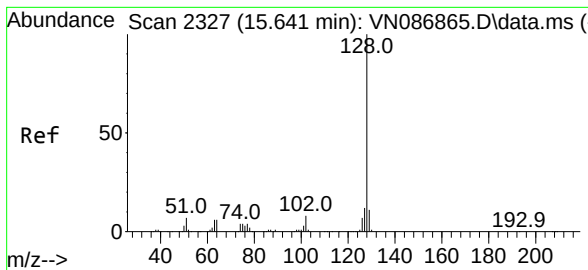

#95
Naphthalene
Concen: 20.070 ug/l
RT: 15.635 min Scan# 21
Delta R.T. -0.006 min
Lab File: VN087114.D
Acq: 19 Jun 2025 16:07

Instrument :
MSVOA_N
ClientSampleId :
MW-08DL

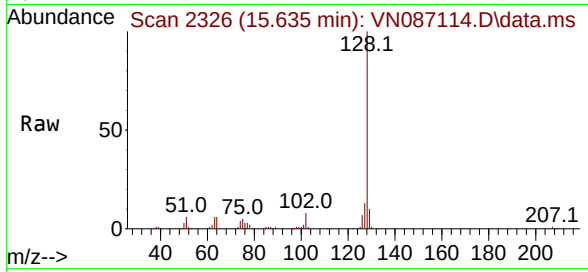

Tgt Ion:128 Resp: 244209
Ion Ratio Lower Upper
128 100
127 12.5 10.2 15.2
129 10.6 8.8 13.2

