
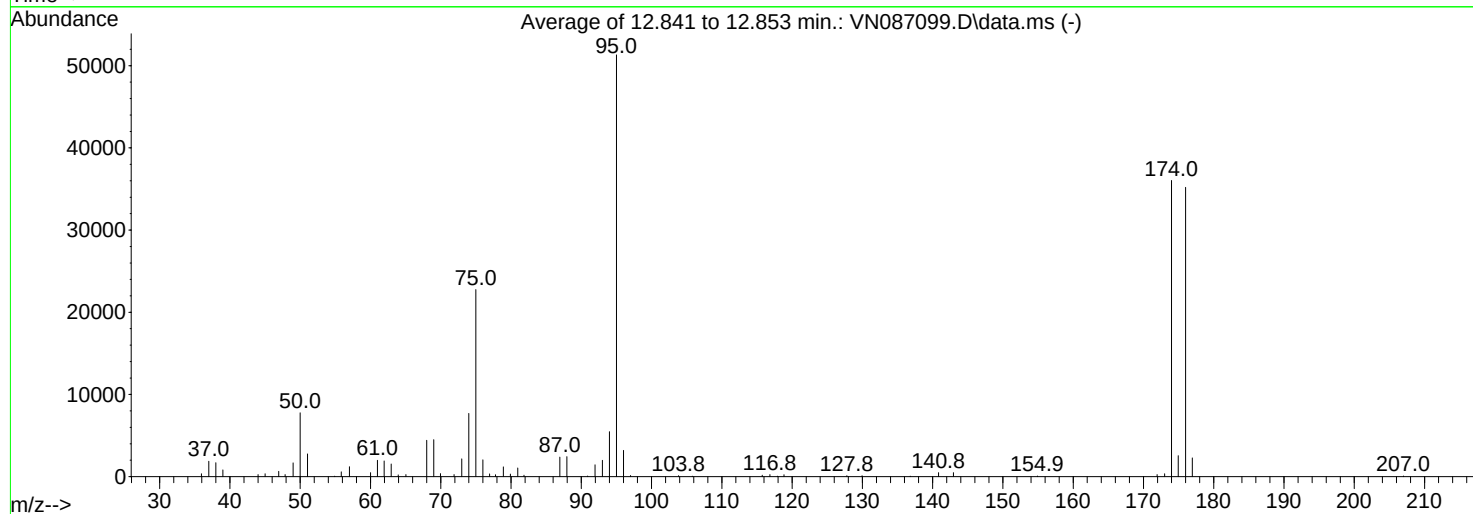


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN061925\
Data File : VN087099.D
Acq On : 19 Jun 2025 08:58
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N060625W.M
Title : SW846 8260
Last Update : Sat Jun 07 02:12:50 2025

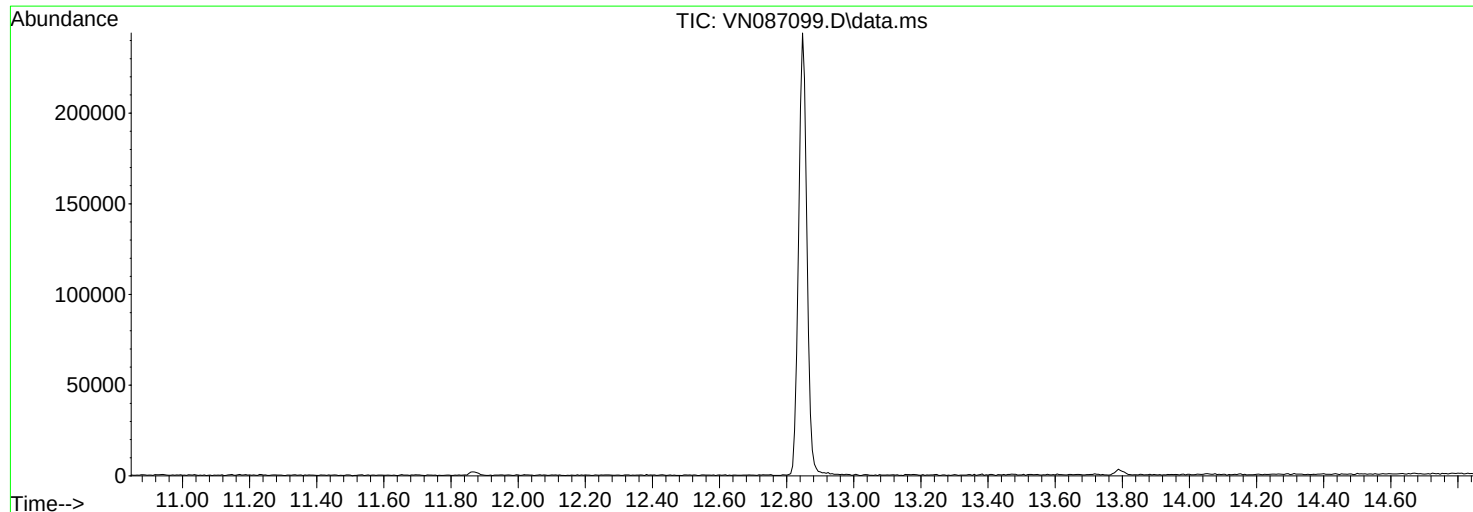

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.1	7775	PASS
75	95	30	60	44.3	22760	PASS
95	95	100	100	100.0	51323	PASS
96	95	5	9	6.2	3191	PASS
173	174	0.00	2	1.0	343	PASS
174	95	50	100	70.2	36029	PASS
175	174	5	9	7.1	2561	PASS
176	174	95	101	97.7	35200	PASS
177	176	5	9	6.5	2289	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	349	54.90	69	69.95	380	81.85	181
37.00	1862	55.85	580	71.90	252	86.95	238
38.00	1689	57.00	1210	73.00	2167	87.95	243
39.00	812	60.00	479	74.00	7682	90.90	81
44.00	253	61.00	1993	75.00	22760	91.95	1434
45.00	344	61.95	1906	76.00	2052	93.00	1982
46.95	634	62.95	1533	76.95	336	94.00	5471
47.85	248	63.95	210	77.80	234	95.00	51323
49.00	1670	65.05	263	78.90	1196	96.00	3191
50.00	7775	68.00	4412	79.90	310	97.00	142
51.05	2762	69.00	4501	80.95	1054	103.85	119

Average of 12.841 to 12.853 min.: VN087099.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
105.80	57	171.95	252				
115.75	182	173.00	343				
116.85	260	174.00	36029				
117.90	56	174.95	2561				
118.85	240	176.00	35200				
127.80	126	176.95	2289				
129.95	111	207.00	81				
136.80	52						
140.85	492						
142.95	481						
154.90	75						

Instrument :

MSVOA_N

ClientSampleId :

BFB