

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN062022\
 Data File : VN072955.D
 Acq On : 20 Jun 2022 12:39
 Operator : JC\MD
 Sample : N3357-03
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 MW-1MS

Quant Time: Jun 21 05:54:32 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N061722W.M
 Quant Title : SW846 8260
 QLast Update : Sat Jun 18 06:22:45 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.016	168	350492	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.898	114	555026	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.680	117	497874	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.610	152	243748	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.369	65	203144	42.870	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	85.740%
35) Dibromofluoromethane	7.951	113	177217	51.658	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	103.320%
50) Toluene-d8	10.374	98	572270	44.830	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	89.660%
62) 4-Bromofluorobenzene	12.668	95	254839	55.518	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	111.040%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN062022\
Data File : VN072955.D
Acq On : 20 Jun 2022 12:39
Operator : JC\MD
Sample : N3357-03
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
MW-1MS

Quant Time: Jun 21 05:54:32 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N061722W.M
Quant Title : SW846 8260
QLast Update : Sat Jun 18 06:22:45 2022
Response via : Initial Calibration




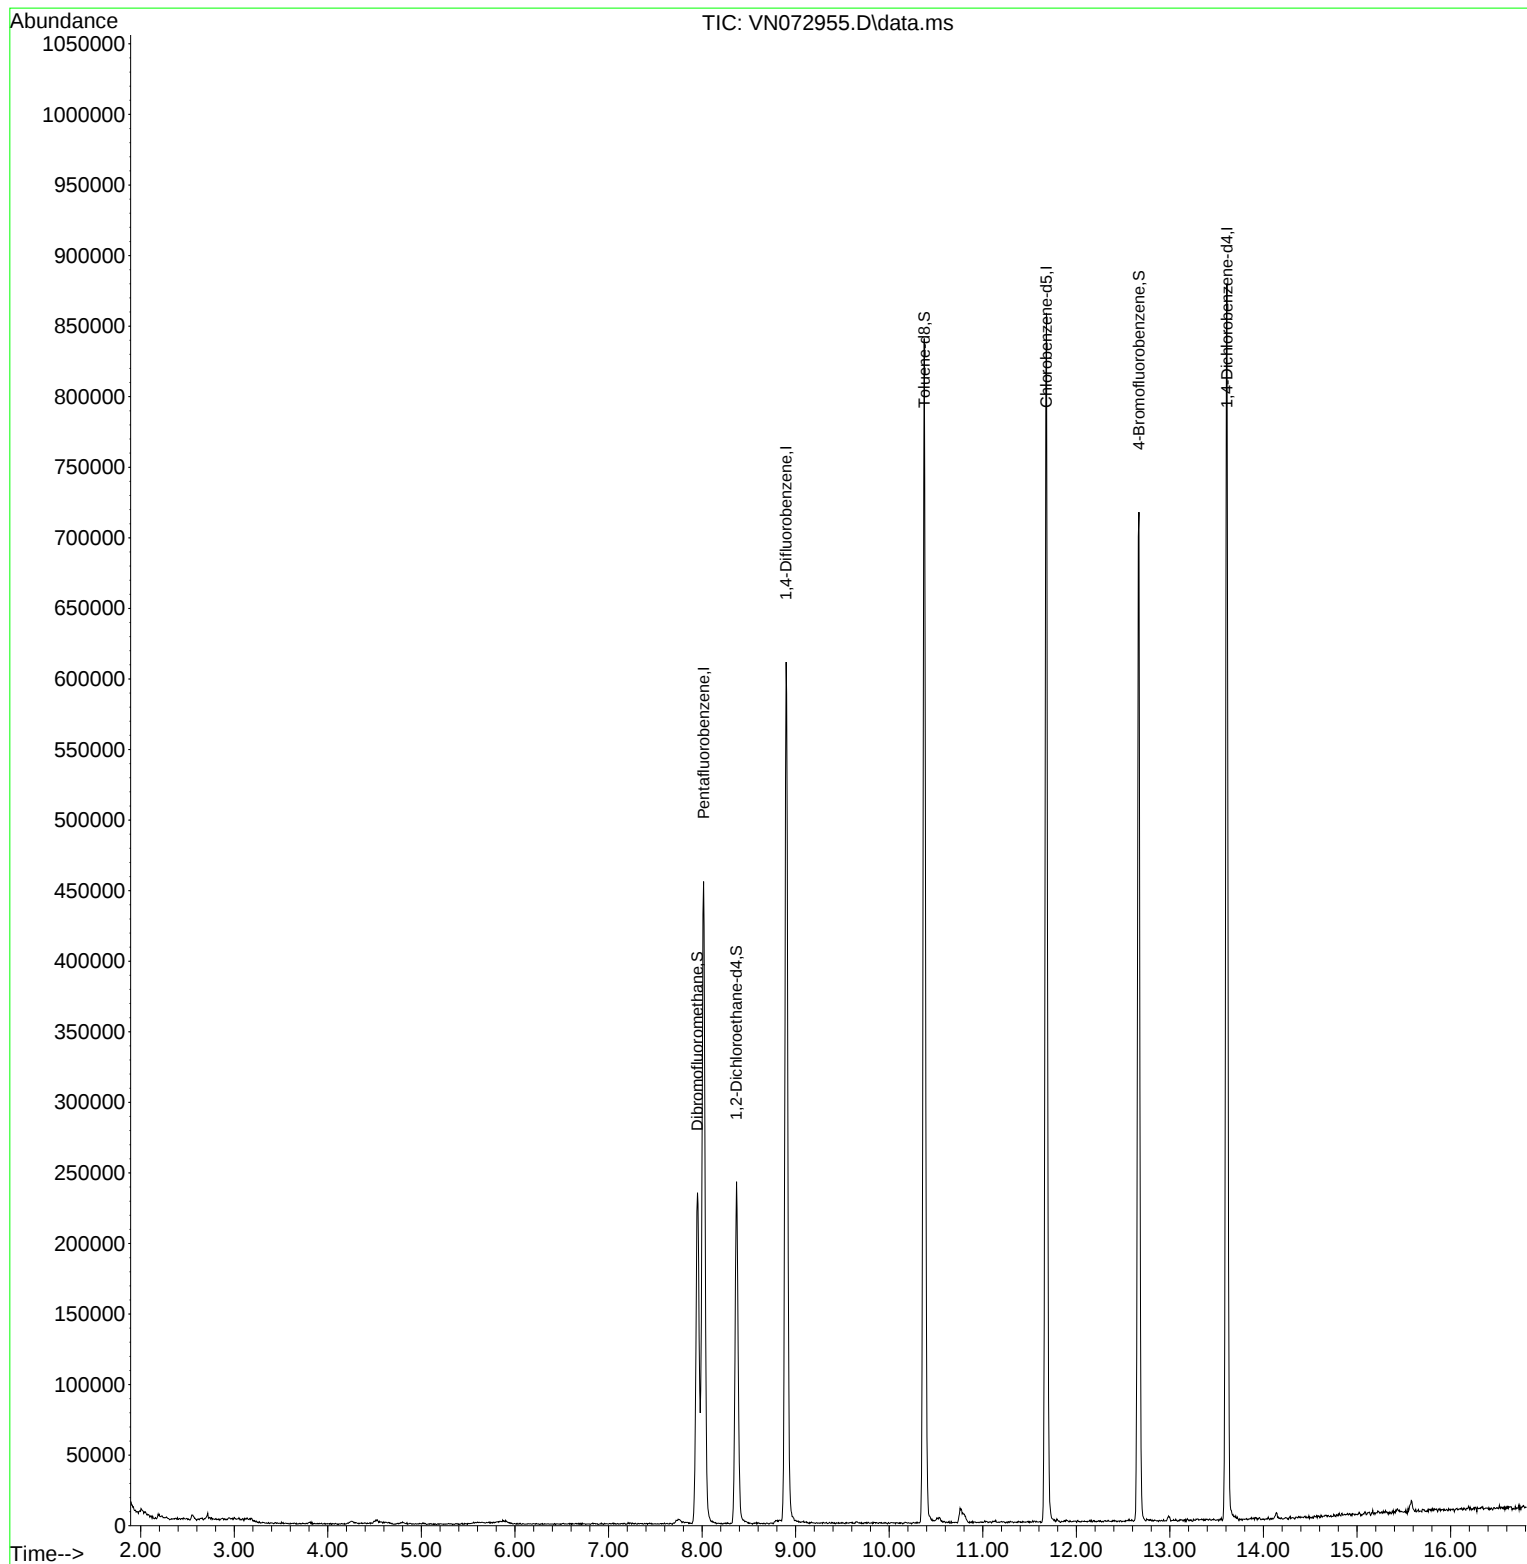


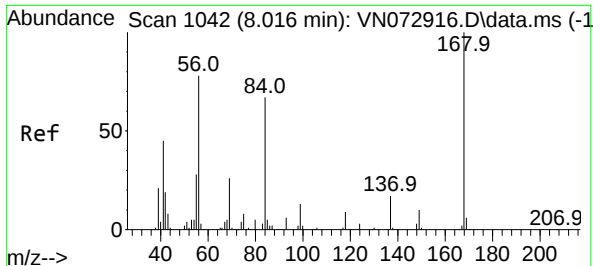

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.016 min Scan# 1042
Delta R.T. -0.000 min
Lab File: VN072955.D
Acq: 20 Jun 2022 12:39




Instrument :
MSVOA_N
ClientSampleId :
MW-1MS


Tgt Ion:168 Resp: 350492
Ion Ratio Lower Upper
168 100
99 60.4 42.3 63.5

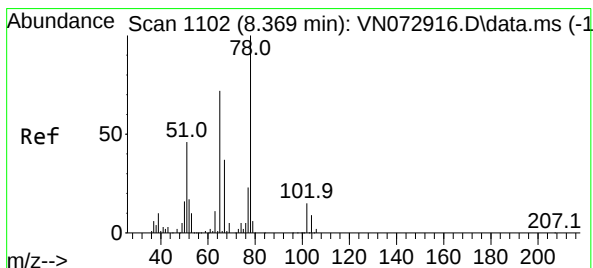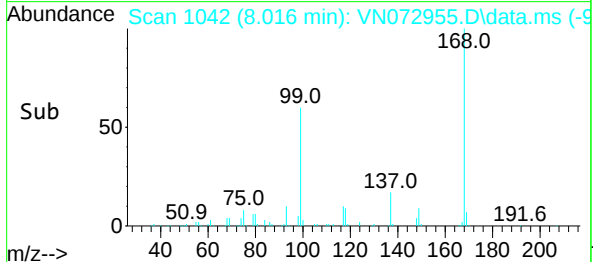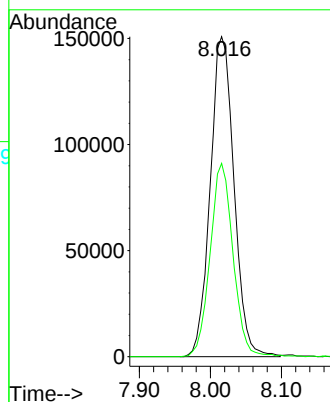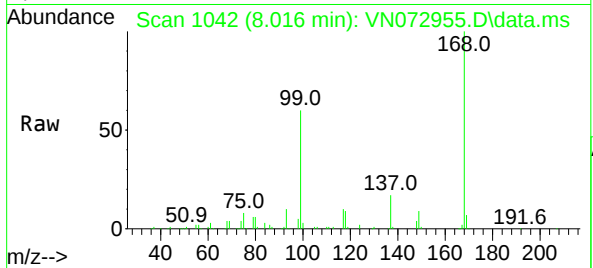

#33
1,2-Dichloroethane-d4
Concen: 42.870 ug/l
RT: 8.369 min Scan# 1102
Delta R.T. 0.000 min
Lab File: VN072955.D
Acq: 20 Jun 2022 12:39

Tgt Ion: 65 Resp: 203144
Ion Ratio Lower Upper
65 100
67 51.1 0.0 104.8


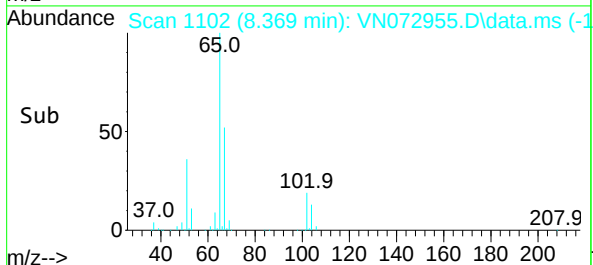
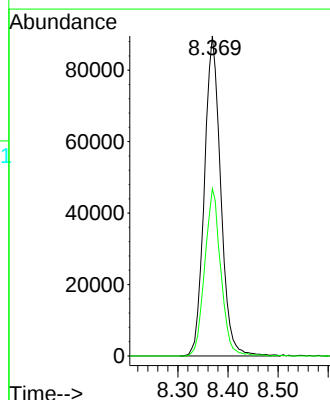
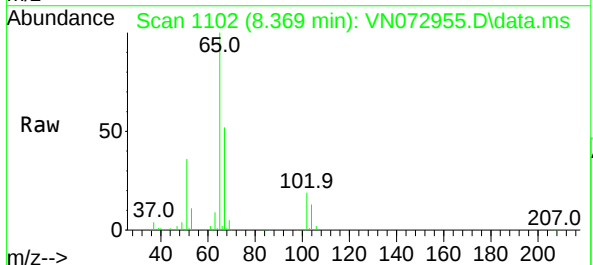


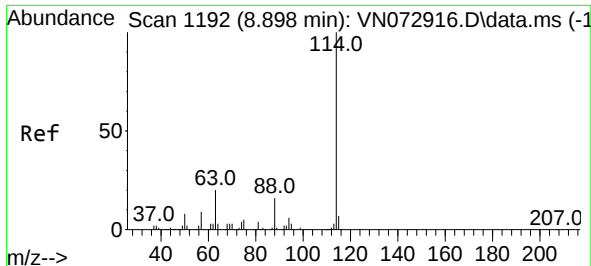

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.898 min Scan# 1192
Delta R.T. 0.000 min
Lab File: VN072955.D
Acq: 20 Jun 2022 12:39




Instrument :
MSVOA_N
ClientSampleId :
MW-1MS


Tgt Ion:114 Resp: 555026
Ion Ratio Lower Upper
114 100
63 20.7 0.0 40.0
88 15.3 0.0 32.6

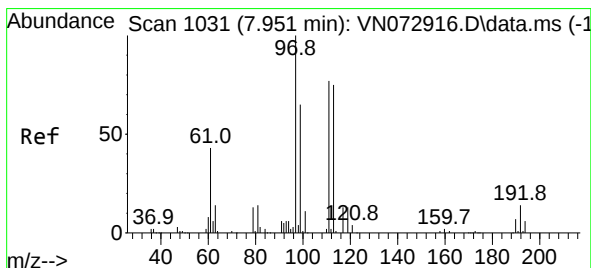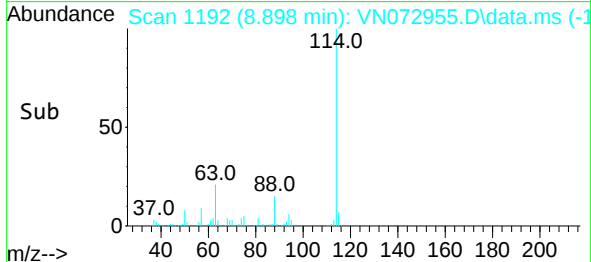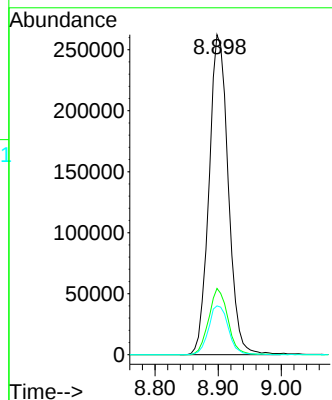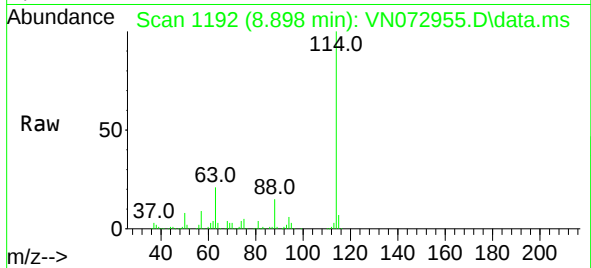

#35
Dibromofluoromethane
Concen: 51.658 ug/l
RT: 7.951 min Scan# 1031
Delta R.T. 0.000 min
Lab File: VN072955.D
Acq: 20 Jun 2022 12:39

Tgt Ion:113 Resp: 177217
Ion Ratio Lower Upper
113 100
111 103.1 81.4 122.0
192 18.8 17.0 25.6


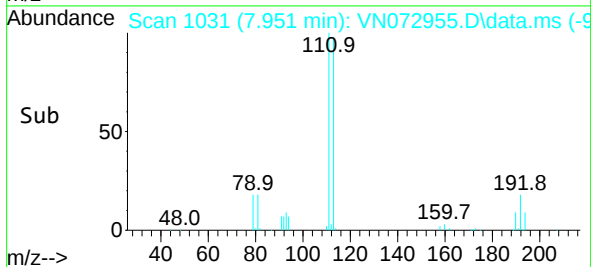
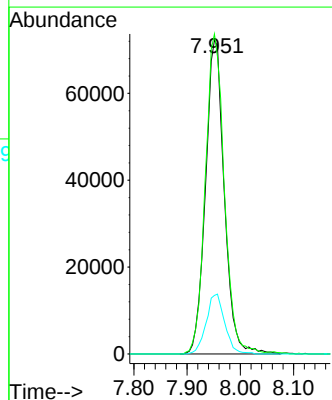
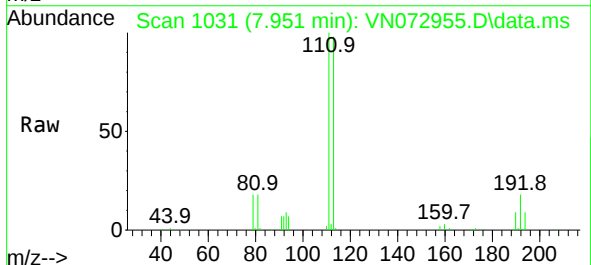


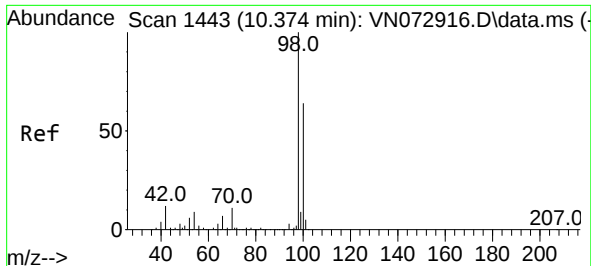

#50
Toluene-d8
Concen: 44.830 ug/l
RT: 10.374 min Scan# 1443
Delta R.T. 0.000 min
Lab File: VN072955.D
Acq: 20 Jun 2022 12:39




Instrument :
MSVOA_N
ClientSampleId :
MW-1MS


Tgt Ion: 98 Resp: 572270
Ion Ratio Lower Upper
98 100
100 65.8 52.6 78.8

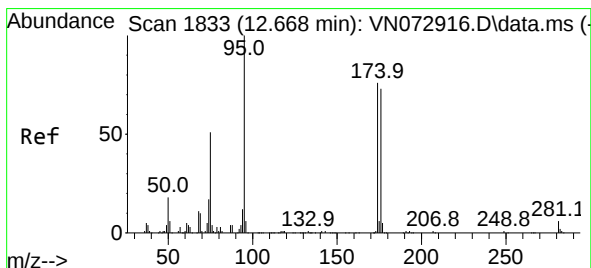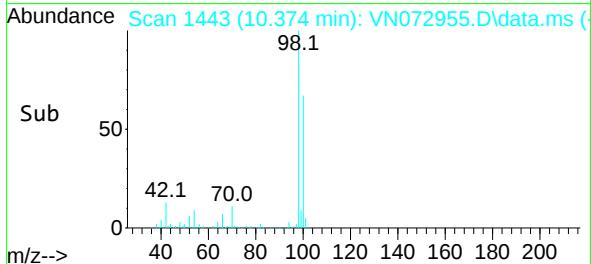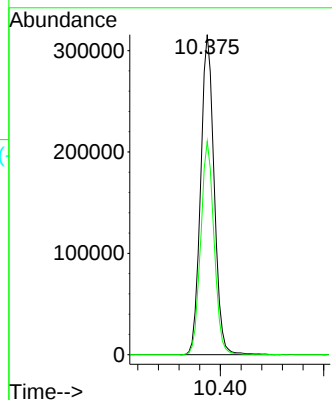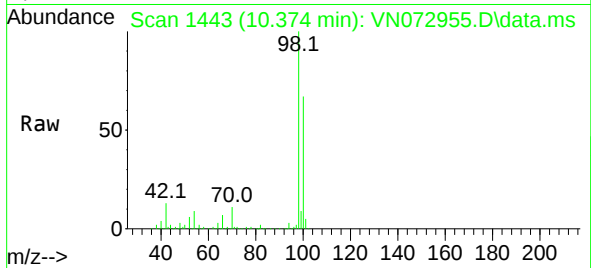

#62
4-Bromofluorobenzene
Concen: 55.518 ug/l
RT: 12.668 min Scan# 1833
Delta R.T. 0.000 min
Lab File: VN072955.D
Acq: 20 Jun 2022 12:39

Tgt Ion: 95 Resp: 254839
Ion Ratio Lower Upper
95 100
174 74.9 0.0 167.6
176 72.0 0.0 163.4


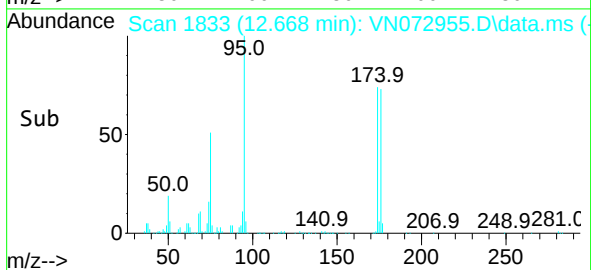
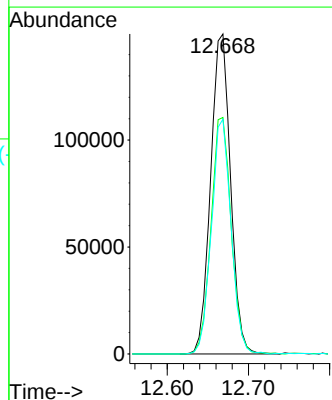
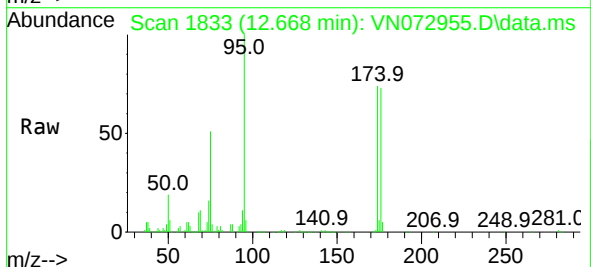


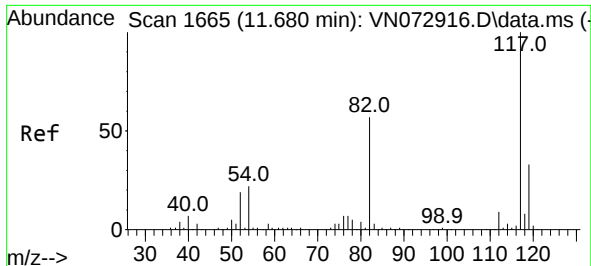

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.680 min Scan# 1166
Delta R.T. 0.000 min
Lab File: VN072955.D
Acq: 20 Jun 2022 12:39

Instrument :
MSVOA_N
ClientSampleId :
MW-1MS

Tgt Ion:117 Resp: 497874
Ion Ratio Lower Upper
117 100
82 56.3 44.2 66.2
119 32.8 25.4 38.0

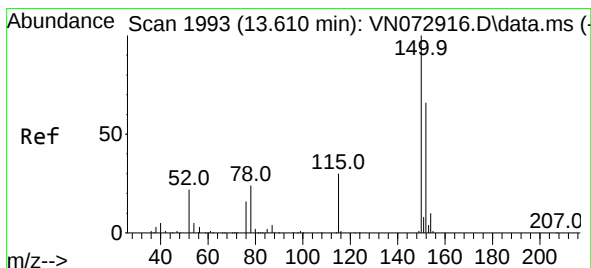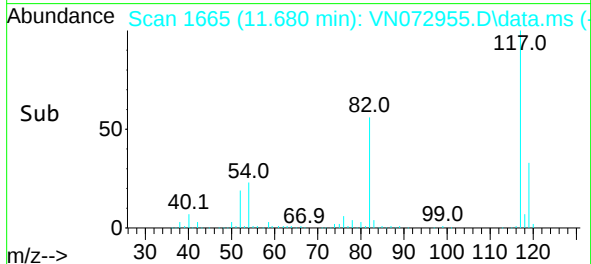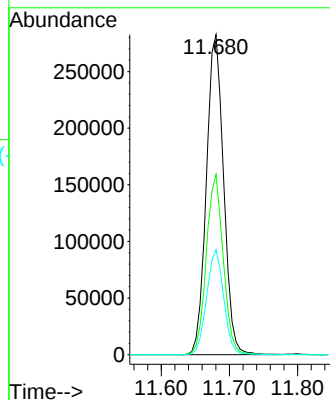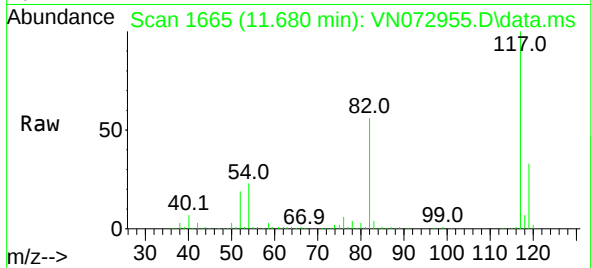

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.610 min Scan# 1993
Delta R.T. 0.000 min
Lab File: VN072955.D
Acq: 20 Jun 2022 12:39

Tgt Ion:152 Resp: 243748
Ion Ratio Lower Upper
152 100
115 59.9 28.9 86.7
150 158.0 0.0 356.2

