
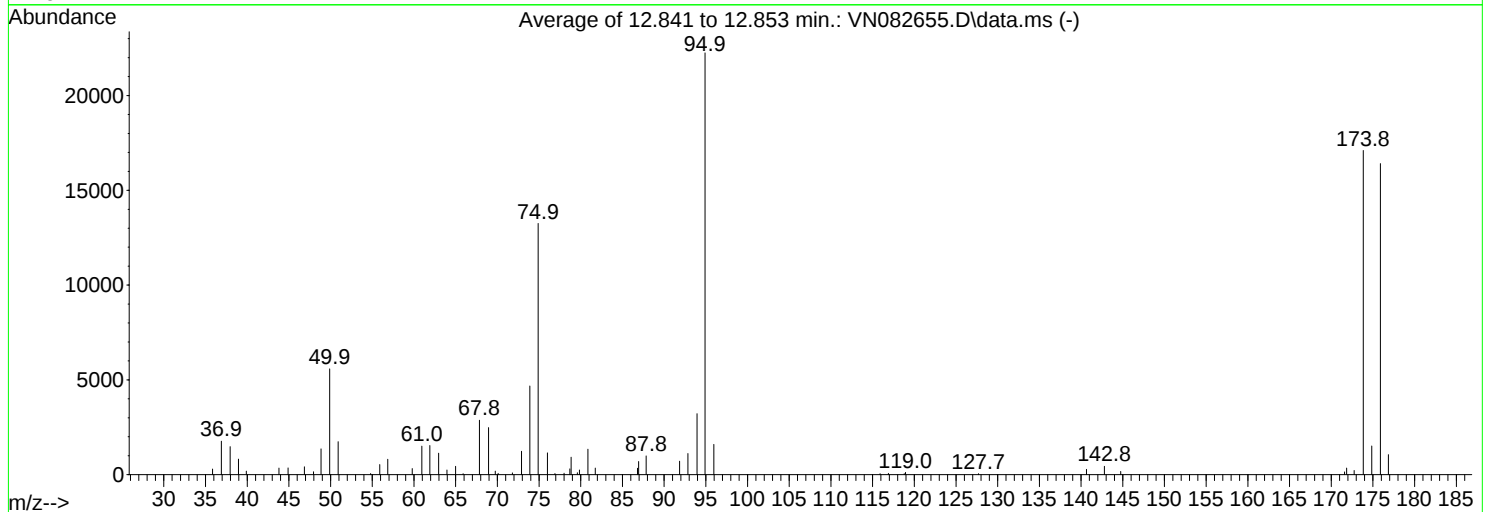


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN062024\
Data File : VN082655.D
Acq On : 20 Jun 2024 09:12
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N061724W.M
Title : SW846 8260
Last Update : Tue Jun 18 04:52:44 2024

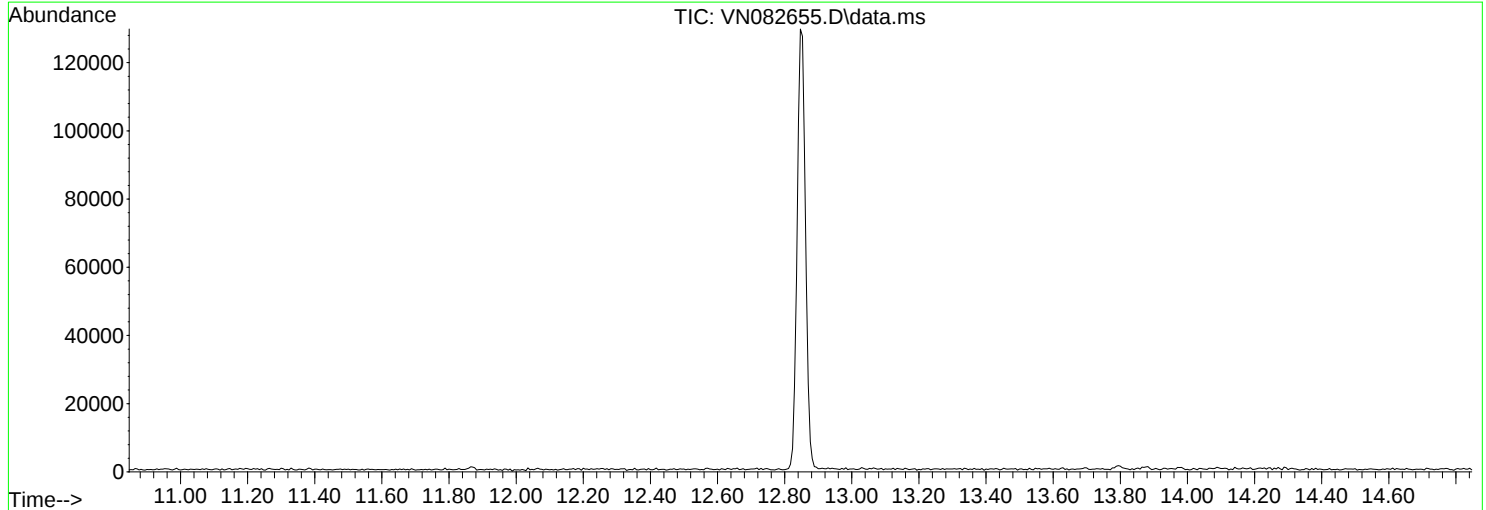

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1844

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	25.1	5583	PASS
75	95	30	60	59.6	13252	PASS
95	95	100	100	100.0	22253	PASS
96	95	5	9	7.2	1595	PASS
173	174	0.00	2	1.3	219	PASS
174	95	50	100	76.9	17103	PASS
175	174	5	9	8.8	1508	PASS
176	174	95	101	95.9	16408	PASS
177	176	5	9	6.4	1052	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.85	294	50.90	1741	67.85	2871	78.70	301
36.90	1761	54.80	60	68.95	2484	78.85	91
37.95	1475	55.90	535	69.75	185	79.60	9
38.95	820	56.85	813	70.10	65	79.85	24
39.90	185	59.80	323	71.80	92	80.85	1339
43.80	343	60.95	1507	72.90	1229	81.75	344
44.90	359	61.90	1537	73.90	4678	86.80	338
46.85	414	62.95	1134	74.90	13252	86.95	691
47.95	156	63.95	249	76.00	1150	87.85	985
48.85	1359	65.00	436	76.90	56	91.85	712
49.90	5583	65.90	53	78.00	78	92.85	1117

Average of 12.841 to 12.853 min.: VN082655.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
93.95	3213	171.60	147				
94.90	22253	171.85	344				
95.95	1595	172.75	219				
115.90	50	173.85	17103				
116.90	72	174.85	1508				
118.80	52	175.90	16408				
118.95	118	176.85	1052				
127.70	50						
140.65	278						
142.80	443						
144.75	166						

Instrument :

MSVOA_N

ClientSampleId :

BFB