

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN062121\
 Data File : VN067407.D
 Acq On : 21 Jun 2021 11:02
 Operator : JC/MD
 Sample : VN0621MBL01
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN0621MBL01

Quant Time: Jun 22 03:09:11 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N061421W.M
 Quant Title : SW846 8260
 QLast Update : Tue Jun 15 05:19:42 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.088	168	299296	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.971	114	589712	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.749	117	520238	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.678	152	182492	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.440	65	286593	48.54	ug/l	0.00
Spiked Amount 50.000	Range 61 - 141		Recovery =	97.08%		
35) Dibromofluoromethane	8.024	113	184125	46.95	ug/l	0.00
Spiked Amount 50.000	Range 69 - 133		Recovery =	93.90%		
50) Toluene-d8	10.443	98	777733	51.74	ug/l	0.00
Spiked Amount 50.000	Range 65 - 126		Recovery =	103.48%		
62) 4-Bromofluorobenzene	12.736	95	273423	44.07	ug/l	0.00
Spiked Amount 50.000	Range 58 - 135		Recovery =	88.14%		
Target Compounds						Qvalue
10) Methyl Iodide	4.422	142	199	6.79	ug/l #	48
13) Acrolein	4.025	56	486	0.80	ug/l #	1
16) Acetone	4.296	43	766	0.34	ug/l	93
17) Carbon Disulfide	4.519	76	2777	0.24	ug/l #	71
18) Methyl Acetate	4.867	43	1299	0.24	ug/l #	83
20) Methylene Chloride	5.098	84	1627	0.35	ug/l	84
25) 2-Butanone	7.359	43	2089	0.65	ug/l #	51
29) Tetrahydrofuran	7.705	42	643	0.31	ug/l #	79
31) Cyclohexane	8.094	56	10779	1.34	ug/l #	34
36) 1,1-Dichloropropene	8.086	75	36136	5.47	ug/l #	51
38) Carbon Tetrachloride	8.088	117	37944	5.34	ug/l #	16
49) 1,4-Dioxane	9.577	88	139	1.77	ug/l #	84
51) 4-Methyl-2-Pentanone	10.331	43	1933	0.27	ug/l #	41
59) 2-Hexanone	11.087	43	8190	1.54	ug/l	98
74) N-amyl acetate	12.390	43	5311	0.62	ug/l #	85
76) 1,2,3-Trichloropropane	12.734	75	160662	33.90	ug/l #	100
81) trans-1,4-Dichloro-2-b...	12.734	75	160662	84.02	ug/l #	6
82) 4-Chlorotoluene	13.112	91	3136	0.24	ug/l	98
84) 1,2,4-Trimethylbenzene	13.372	105	3082	0.21	ug/l	93
86) p-Isopropyltoluene	13.619	119	2811	0.21	ug/l	89
87) 1,3-Dichlorobenzene	13.619	146	1734	0.27	ug/l	91
88) 1,4-Dichlorobenzene	13.619	146	1734	0.27	ug/l	92
89) n-Butylbenzene	13.948	91	6227	0.49	ug/l	94
91) 1,2-Dichlorobenzene	13.991	146	1898	0.31	ug/l #	74
92) 1,2-Dibromo-3-Chloropr...	14.606	75	484	0.37	ug/l	83
93) 1,2,4-Trichlorobenzene	15.268	180	3903	1.22	ug/l	89
94) Hexachlorobutadiene	15.375	225	823	0.45	ug/l	85
95) Naphthalene	15.509	128	22654	4.54	ug/l	99
96) 1,2,3-Trichlorobenzene	15.711	180	4511	1.47	ug/l	84


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN062121\
Data File : VN067407.D
Acq On : 21 Jun 2021 11:02
Operator : JC/MD
Sample : VN0621MBL01
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN0621MBL01

Quant Time: Jun 22 03:09:11 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N061421W.M
Quant Title : SW846 8260
QLast Update : Tue Jun 15 05:19:42 2021
Response via : Initial Calibration




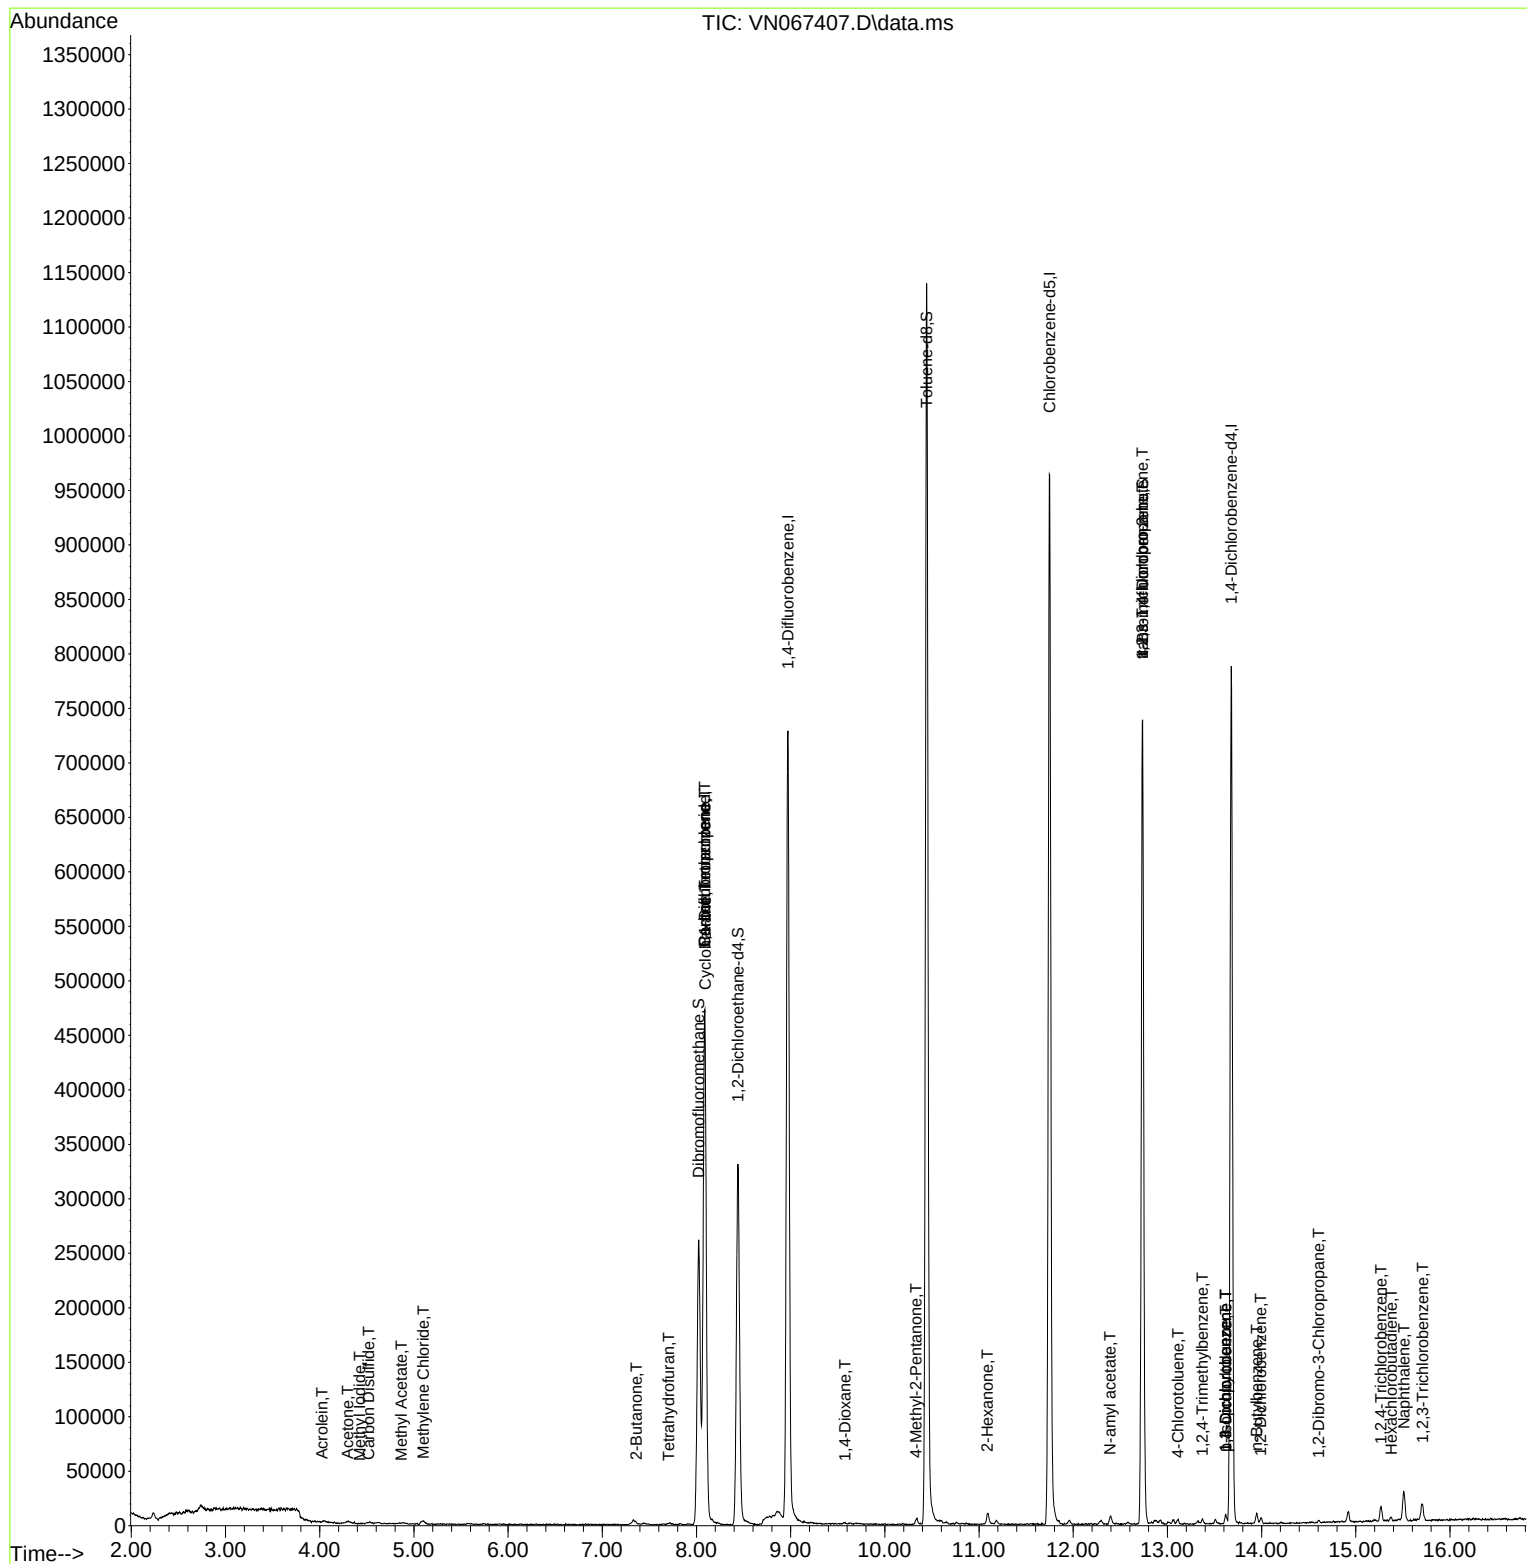


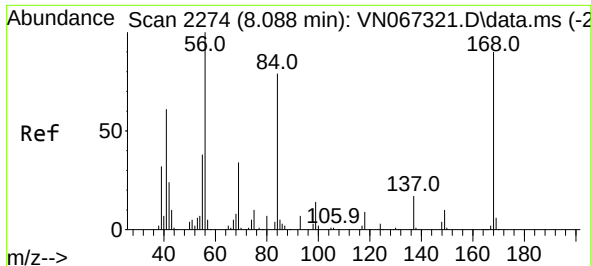

#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 8.088 min Scan# 2274
Delta R.T. 0.000 min
Lab File: VN067407.D
Acq: 21 Jun 2021 11:02




Instrument :
MSVOA_N
ClientSampleId :
VN0621MBL01


Tgt Ion:168 Resp: 299296
Ion Ratio Lower Upper
168 100
99 80.0 62.9 94.3

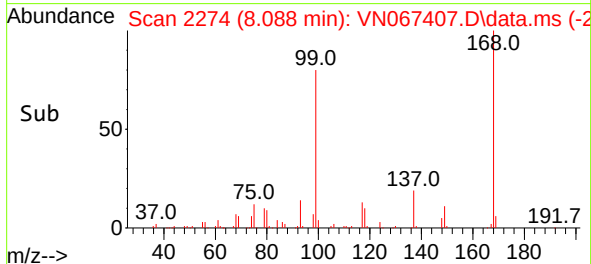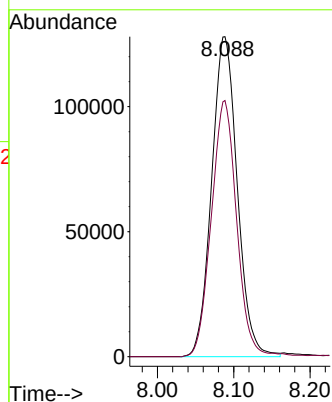

#10
Methyl Iodide
Concen: 6.79 ug/l
RT: 4.422 min Scan# 907
Delta R.T. 0.008 min
Lab File: VN067407.D
Acq: 21 Jun 2021 11:02

Tgt Ion:142 Resp: 199
Ion Ratio Lower Upper
142 100
127 13.1 43.1 64.7#
141 0.0 11.4 17.0#


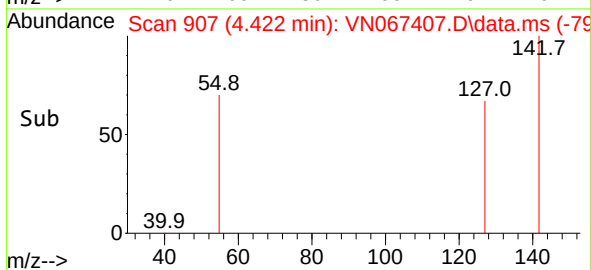

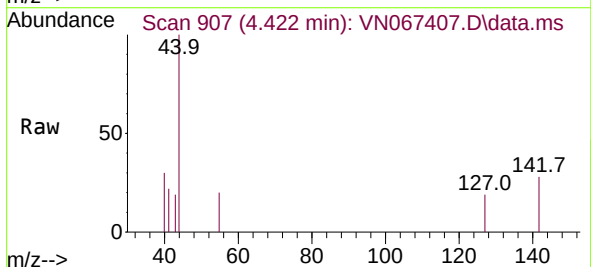


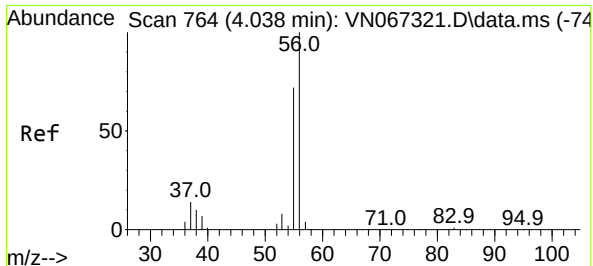

#13
Acrolein
Concen: 0.80 ug/l
RT: 4.025 min Scan# 759
Delta R.T. -0.013 min
Lab File: VN067407.D
Acq: 21 Jun 2021 11:02




Instrument :
MSVOA_N
ClientSampleId :
VN0621MBL01


Tgt Ion: 56 Resp: 486
Ion Ratio Lower Upper
56 100
55 179.0 57.4 86.0#

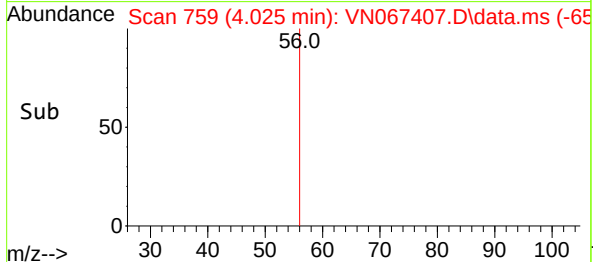

#16
Acetone
Concen: 0.34 ug/l
RT: 4.296 min Scan# 860
Delta R.T. 0.005 min
Lab File: VN067407.D
Acq: 21 Jun 2021 11:02

Tgt Ion: 43 Resp: 766
Ion Ratio Lower Upper
43 100
58 30.2 21.2 31.8


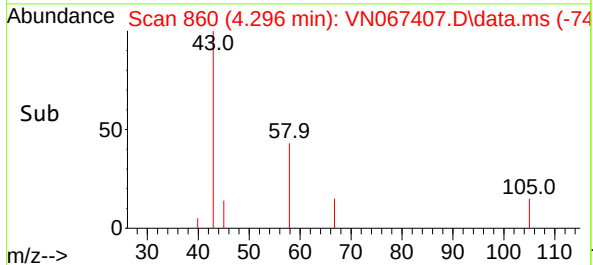

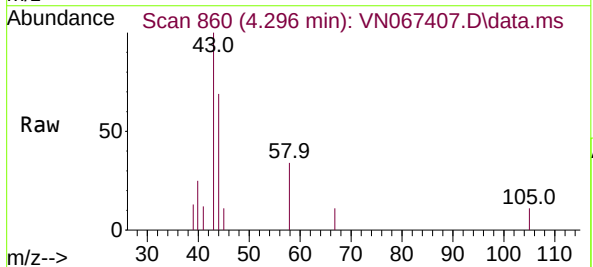




#17
Carbon Disulfide
Concen: 0.24 ug/l
RT: 4.519 min Scan# 943
Delta R.T. -0.002 min
Lab File: VN067407.D
Acq: 21 Jun 2021 11:02




Instrument :
MSVOA_N
ClientSampleId :
VN0621MBL01


Tgt Ion: 76 Resp: 2777
Ion Ratio Lower Upper
76 100
78 20.4 7.7 11.5#

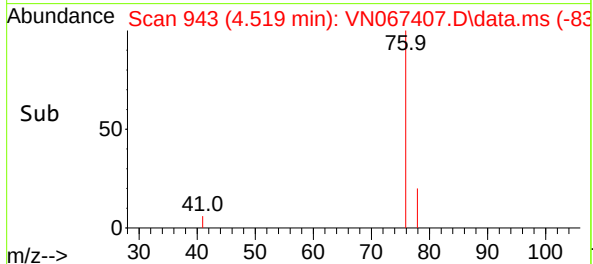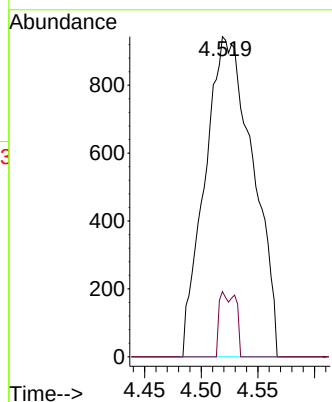

#18
Methyl Acetate
Concen: 0.24 ug/l
RT: 4.867 min Scan# 1073
Delta R.T. 0.011 min
Lab File: VN067407.D
Acq: 21 Jun 2021 11:02

Tgt Ion: 43 Resp: 1299
Ion Ratio Lower Upper
43 100
74 13.5 17.4 26.0#

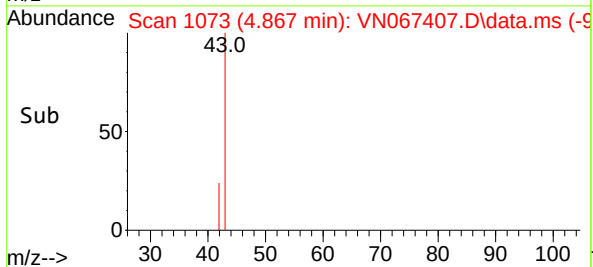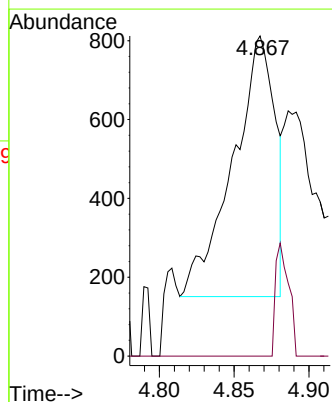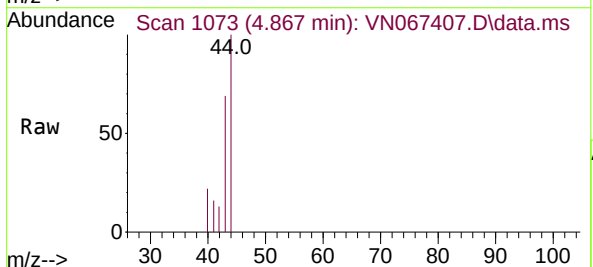

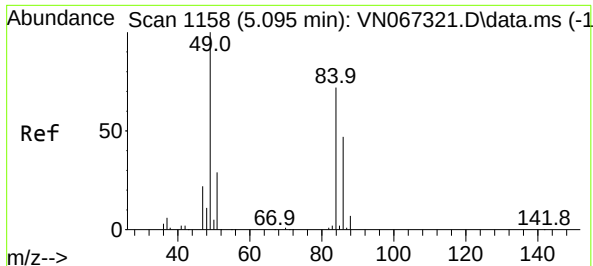

#20

Methylene Chloride

Concen: 0.35 ug/l

RT: 5.098 min Scan# 1159

Delta R.T. 0.003 min

Lab File: VN067407.D

Acq: 21 Jun 2021 11:02

Instrument :

MSVOA_N

ClientSampleId :

VN0621MBL01

Tgt Ion: 84 Resp: 1627





Ion Ratio Lower Upper

84 100

49 113.2 110.9 166.3

51 34.6 32.6 49.0

86 57.8 51.6 77.4

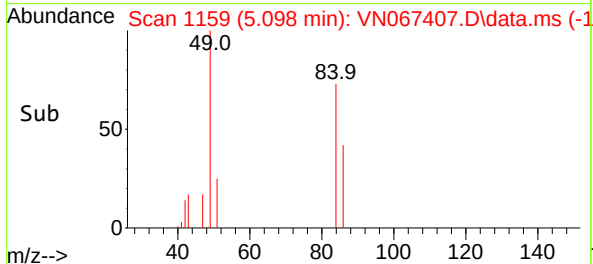

#25

2-Butanone

Concen: 0.65 ug/l

RT: 7.359 min Scan# 2002

Delta R.T. 0.016 min

Lab File: VN067407.D




Acq: 21 Jun 2021 11:02


Tgt Ion: 43 Resp: 2089

Ion Ratio Lower Upper

43 100

72 0.0 19.7 29.5#

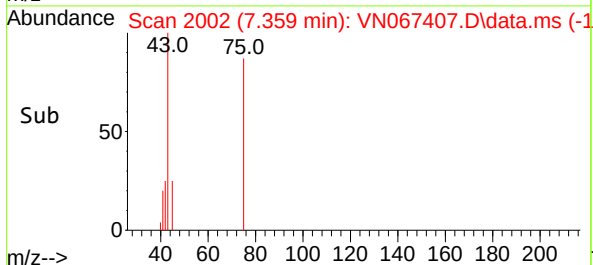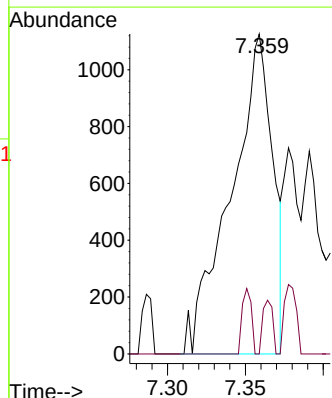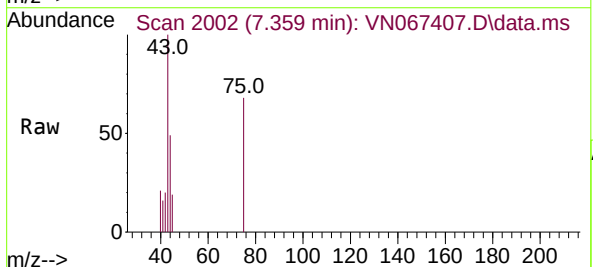

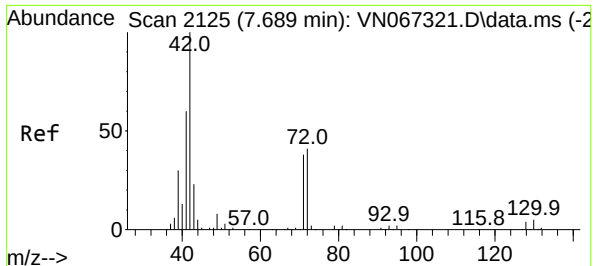

#29

Tetrahydrofuran

Concen: 0.31 ug/l

RT: 7.705 min Scan# 2131





Delta R.T. 0.016 min

Lab File: VN067407.D

Acq: 21 Jun 2021 11:02

Tgt Ion:	42	Resp:	643
Ion	Ratio	Lower	Upper
42	100		
72	31.6	32.8	49.2#
71	22.7	31.2	46.8#

Instrument :
MSVOA_N
ClientSampleId :
VN0621MBL01

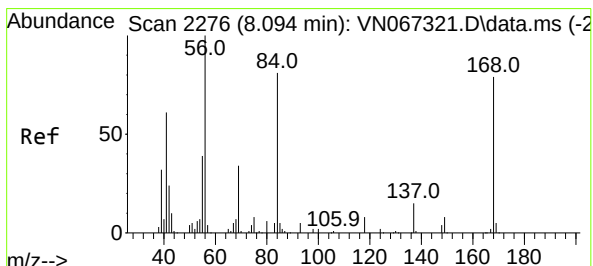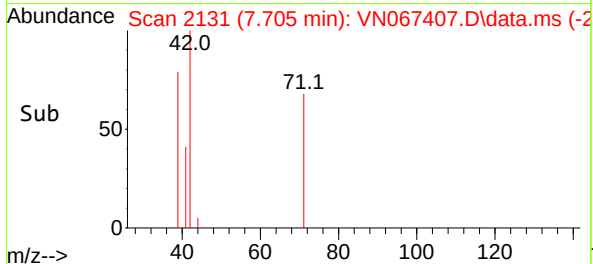

#31

Cyclohexane

Concen: 1.34 ug/l




RT: 8.094 min Scan# 2276


Delta R.T. -0.000 min

Lab File: VN067407.D

Acq: 21 Jun 2021 11:02

Tgt Ion:	56	Resp:	10779
Ion	Ratio	Lower	Upper
56	100		
69	154.7	27.3	40.9#
84	86.1	64.9	97.3


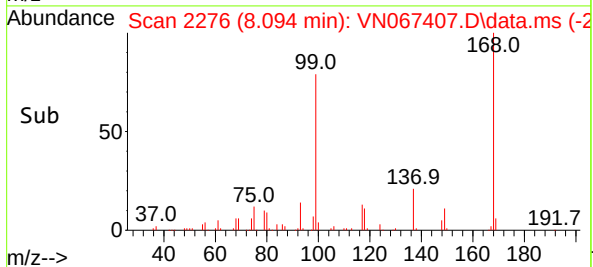

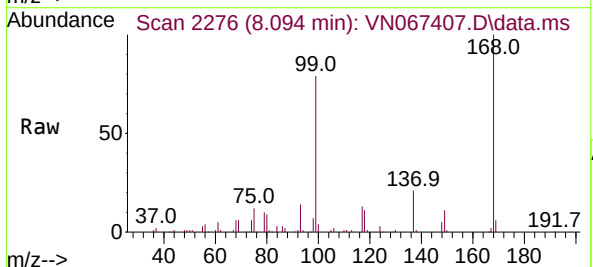


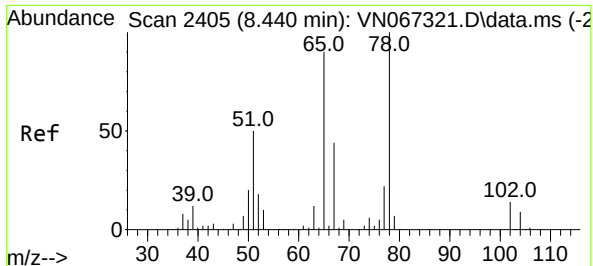

#33
 1,2-Dichloroethane-d4
 Concen: 48.54 ug/l
 RT: 8.440 min Scan# 2405
 Delta R.T. -0.000 min
 Lab File: VN067407.D
 Acq: 21 Jun 2021 11:02




Instrument :
 MSVOA_N
 ClientSampleId :
 VN0621MBL01


Tgt Ion: 65 Resp: 286593
 Ion Ratio Lower Upper
 65 100
 67 51.3 0.0 98.6

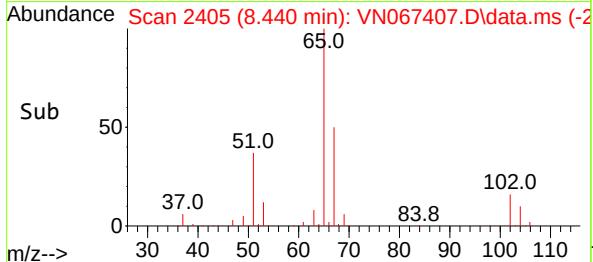

#34
 1,4-Difluorobenzene
 Concen: 50.00 ug/l
 RT: 8.971 min Scan# 2603
 Delta R.T. 0.000 min
 Lab File: VN067407.D
 Acq: 21 Jun 2021 11:02

Tgt Ion: 114 Resp: 589712
 Ion Ratio Lower Upper
 114 100
 63 26.5 0.0 49.0
 88 18.7 0.0 36.6


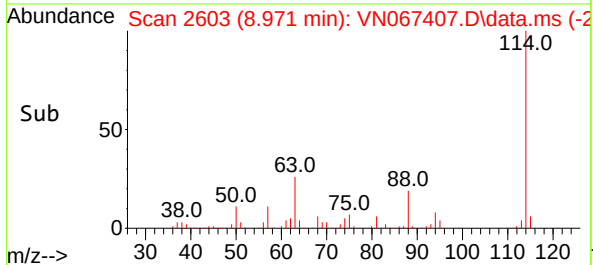

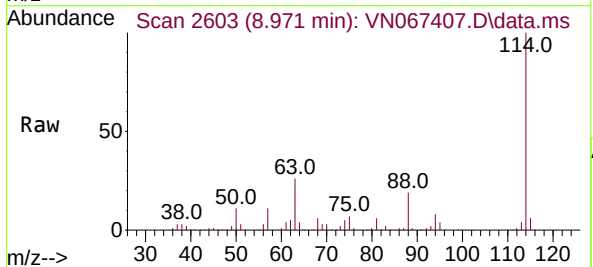


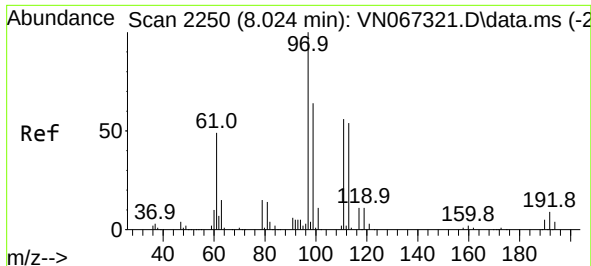

#35
Dibromofluoromethane
Concen: 46.95 ug/l
RT: 8.024 min Scan# 2250
Delta R.T. 0.000 min
Lab File: VN067407.D
Acq: 21 Jun 2021 11:02




Instrument :
MSVOA_N
ClientSampleId :
VN0621MBL01


Tgt Ion:113 Resp: 184125
Ion Ratio Lower Upper
113 100
111 105.2 83.8 125.8
192 15.0 13.4 20.0

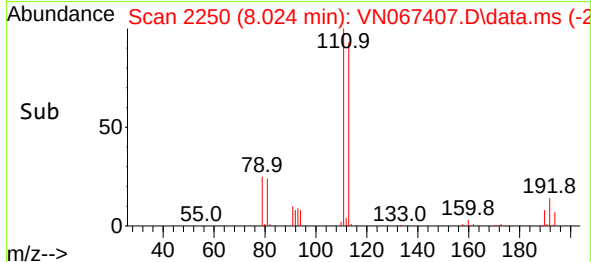

#36
1,1-Dichloropropene
Concen: 5.47 ug/l
RT: 8.086 min Scan# 2273
Delta R.T. -0.136 min
Lab File: VN067407.D
Acq: 21 Jun 2021 11:02

Tgt Ion: 75 Resp: 36136
Ion Ratio Lower Upper
75 100
110 8.2 15.7 47.0#
77 0.0 24.6 37.0#


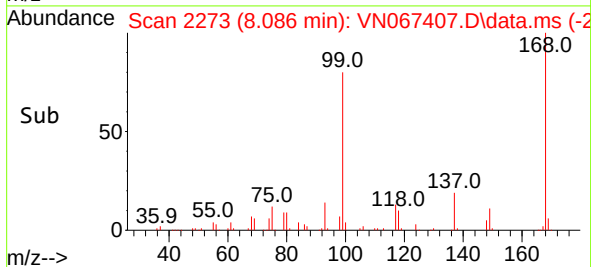

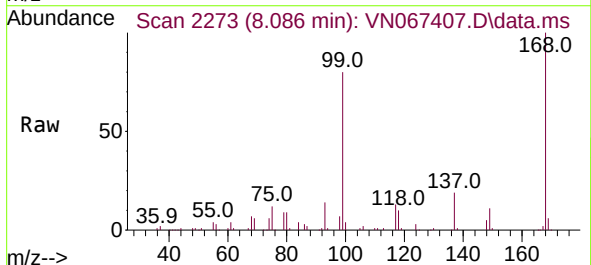


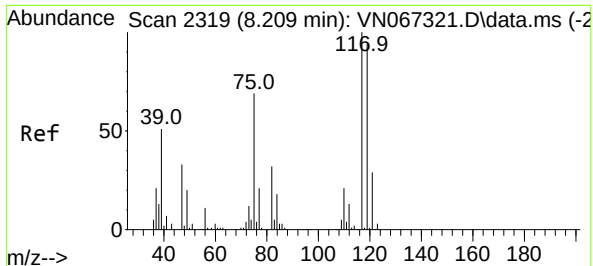

#38
Carbon Tetrachloride
Concen: 5.34 ug/l
RT: 8.088 min Scan# 2274
Delta R.T. -0.121 min
Lab File: VN067407.D
Acq: 21 Jun 2021 11:02




Instrument :
MSVOA_N
ClientSampleId :
VN0621MBL01


Tgt Ion:117 Resp: 37944
Ion Ratio Lower Upper
117 100
119 3.8 75.4 113.2#
121 0.0 23.5 35.3#

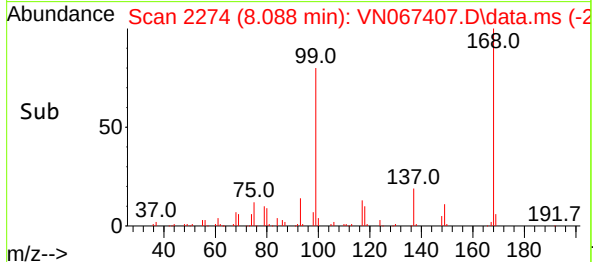

#49
1,4-Dioxane
Concen: 1.77 ug/l
RT: 9.577 min Scan# 2829
Delta R.T. 0.003 min
Lab File: VN067407.D
Acq: 21 Jun 2021 11:02

Tgt Ion: 88 Resp: 139
Ion Ratio Lower Upper
88 100
43 43.9 28.8 43.2#
58 89.9 60.4 90.6


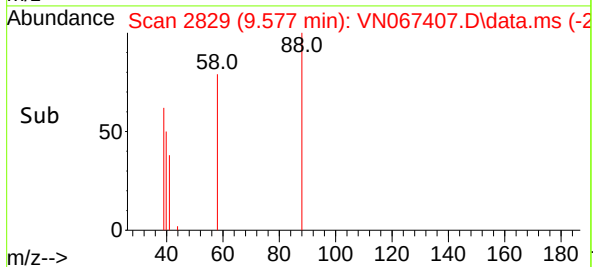

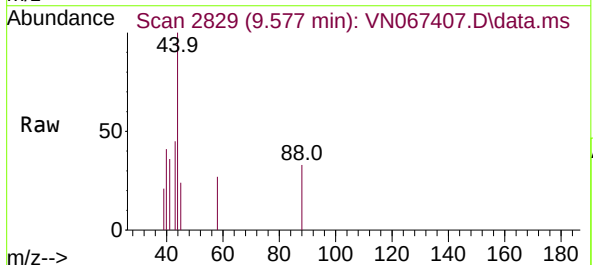


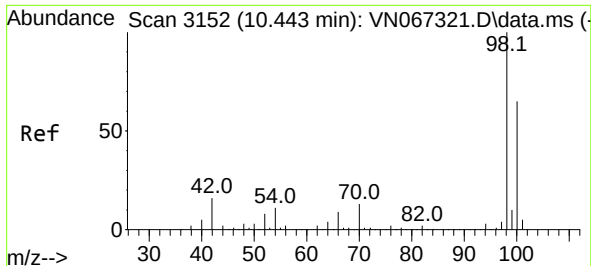

#50
Toluene-d8
Concen: 51.74 ug/l
RT: 10.443 min Scan# 3152
Delta R.T. 0.000 min
Lab File: VN067407.D
Acq: 21 Jun 2021 11:02




Instrument :
MSVOA_N
ClientSampleId :
VN0621MBL01


Tgt Ion: 98 Resp: 777733
Ion Ratio Lower Upper
98 100
100 63.5 51.7 77.5

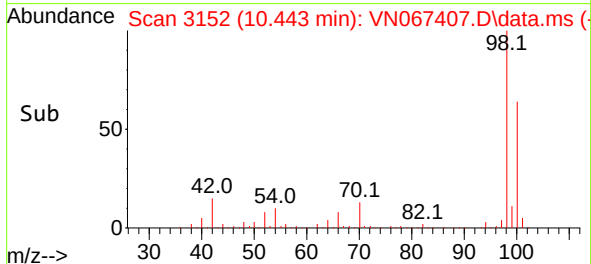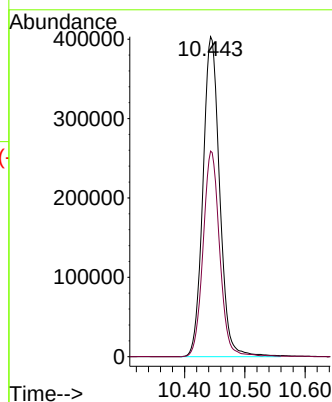

#51
4-Methyl-2-Pentanone
Concen: 0.27 ug/l
RT: 10.331 min Scan# 3110
Delta R.T. -0.002 min
Lab File: VN067407.D
Acq: 21 Jun 2021 11:02

Tgt Ion: 43 Resp: 1933
Ion Ratio Lower Upper
43 100
58 70.7 28.6 43.0#


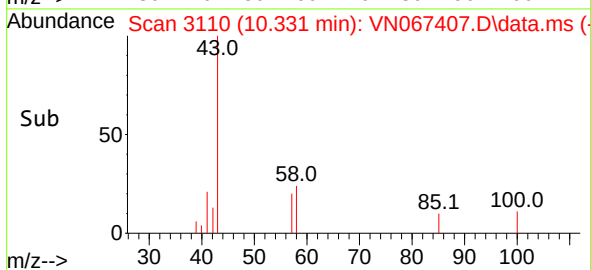
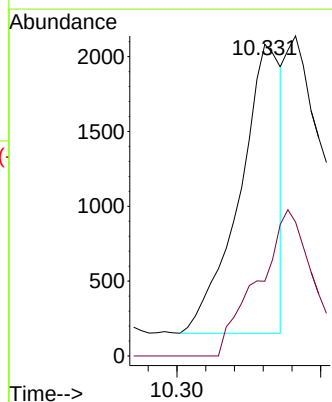
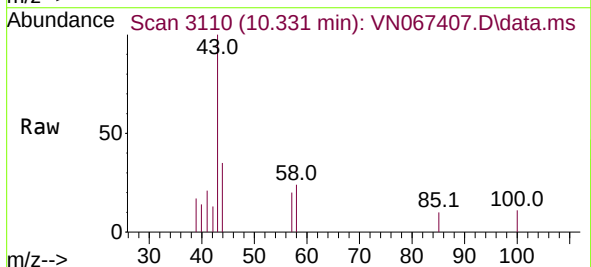


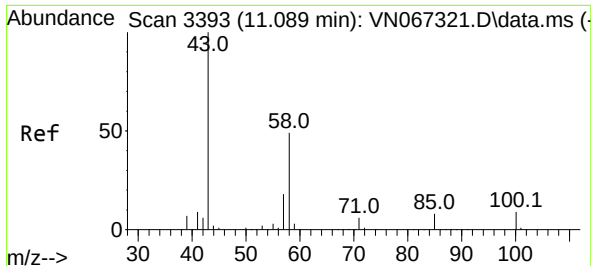

#59
2-Hexanone
Concen: 1.54 ug/l
RT: 11.087 min Scan# 3392
Delta R.T. -0.002 min
Lab File: VN067407.D
Acq: 21 Jun 2021 11:02




Instrument :
MSVOA_N
ClientSampleId :
VN0621MBL01


Tgt Ion: 43 Resp: 8190
Ion Ratio Lower Upper
43 100
58 48.3 24.7 74.1

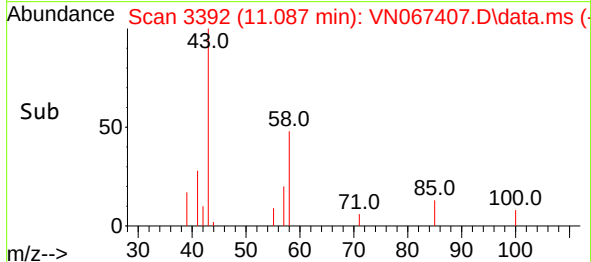

#62
4-Bromofluorobenzene
Concen: 44.07 ug/l
RT: 12.736 min Scan# 4007
Delta R.T. 0.003 min
Lab File: VN067407.D
Acq: 21 Jun 2021 11:02

Tgt Ion: 95 Resp: 273423
Ion Ratio Lower Upper
95 100
174 58.2 0.0 122.0
176 55.8 0.0 117.6


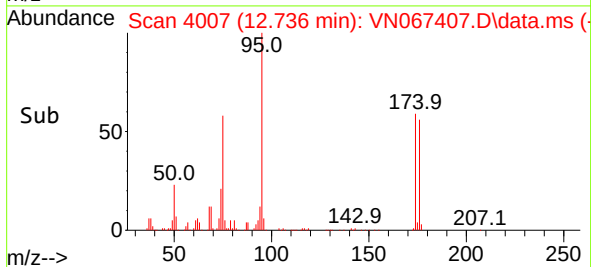

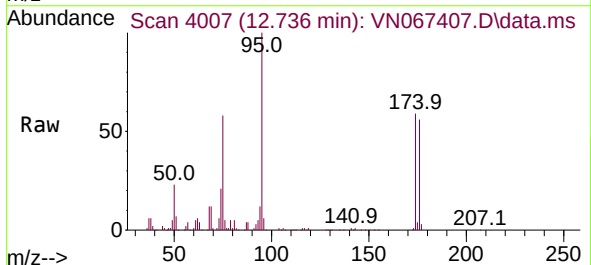




#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 11.749 min Scan# 3639
Delta R.T. 0.003 min
Lab File: VN067407.D
Acq: 21 Jun 2021 11:02




Instrument :
MSVOA_N
ClientSampleId :
VN0621MBL01


Tgt Ion:117 Resp: 520238
Ion Ratio Lower Upper
117 100
82 67.3 53.1 79.7
119 32.2 25.5 38.3

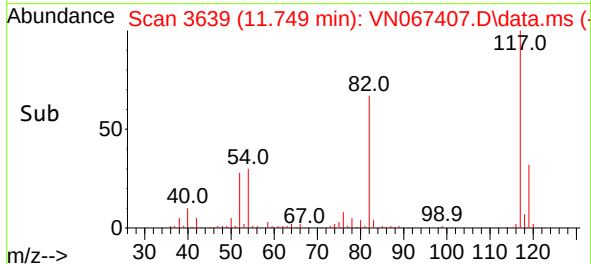

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 13.678 min Scan# 4358
Delta R.T. 0.003 min
Lab File: VN067407.D
Acq: 21 Jun 2021 11:02

Tgt Ion:152 Resp: 182492
Ion Ratio Lower Upper
152 100
115 69.5 36.1 108.5
150 157.1 0.0 351.8


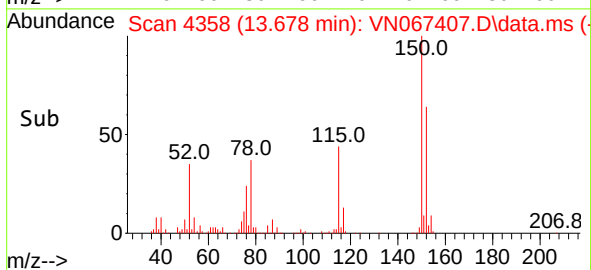

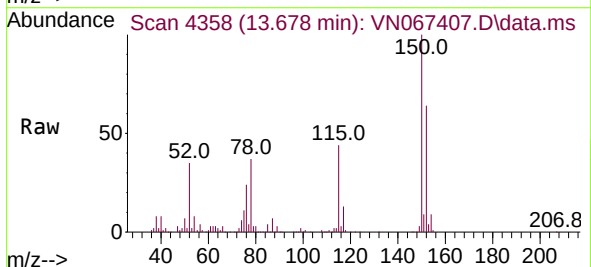


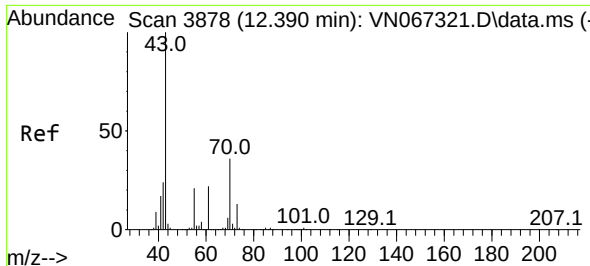

#74
N-amy1 acetate
Concen: 0.62 ug/l
RT: 12.390 min Scan# 3878
Delta R.T. 0.000 min
Lab File: VN067407.D
Acq: 21 Jun 2021 11:02




Instrument :
MSVOA_N
ClientSampleId :
VN0621MBL01


Tgt Ion:	43	Resp:	5311
Ion	Ratio	Lower	Upper
43	100		
70	23.2	29.4	44.2#
55	21.7	17.0	25.4
61	14.9	17.6	26.4#

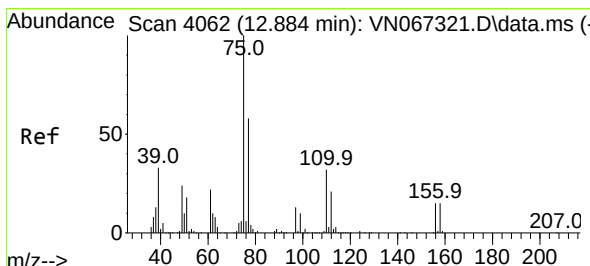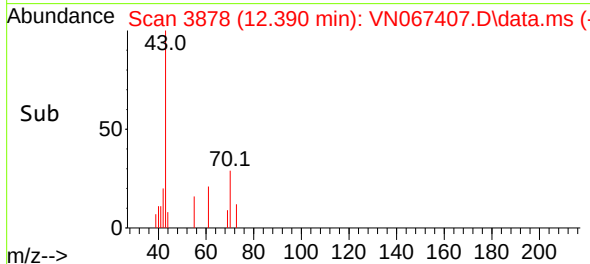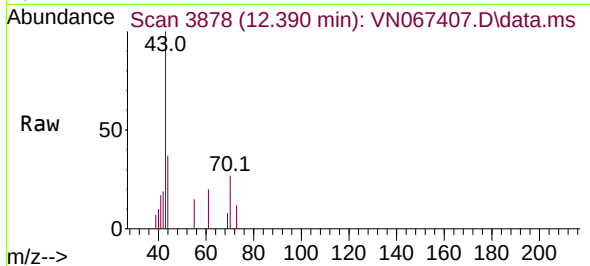

#76
1,2,3-Trichloropropane
Concen: 33.90 ug/l
RT: 12.734 min Scan# 4006
Delta R.T. -0.150 min
Lab File: VN067407.D
Acq: 21 Jun 2021 11:02


Tgt Ion:	75	Resp:	160662
Ion	Ratio	Lower	Upper
75	100		
77	1.0	0.0	0.0#

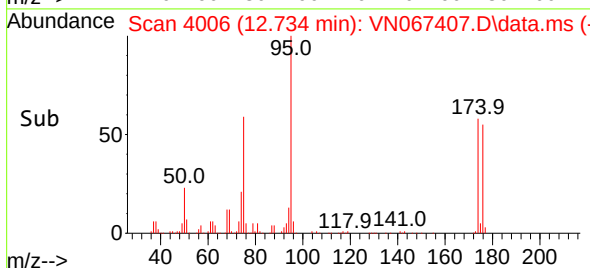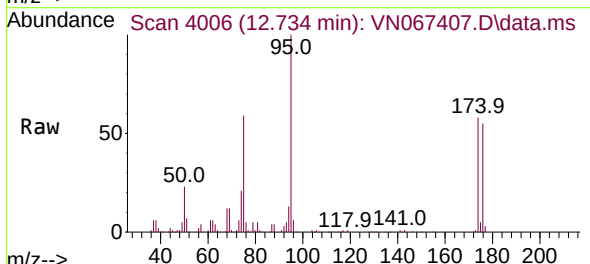



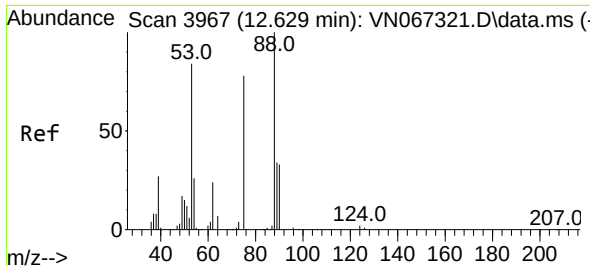


#81
trans-1,4-Dichloro-2-butene
Concen: 84.02 ug/l
RT: 12.734 min Scan# 4006
Delta R.T. 0.105 min
Lab File: VN067407.D
Acq: 21 Jun 2021 11:02


Instrument :
MSVOA_N
ClientSampleId :
VN0621MBL01

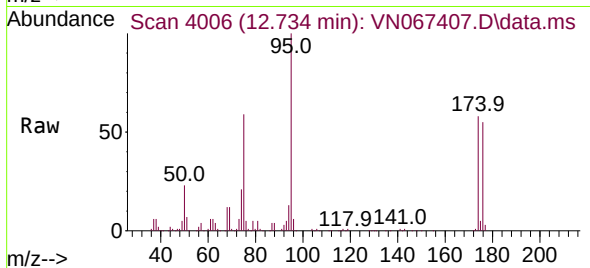



Tgt Ion: 75 Resp: 160662
Ion Ratio Lower Upper
75 100
53 0.0 87.6 131.4#
89 0.0 37.8 56.8#

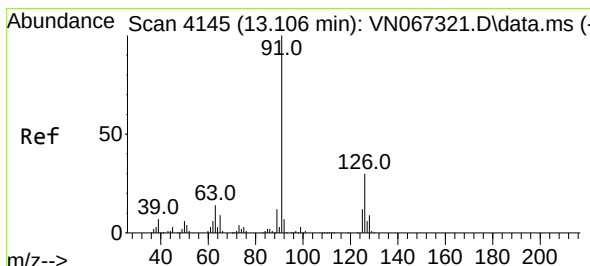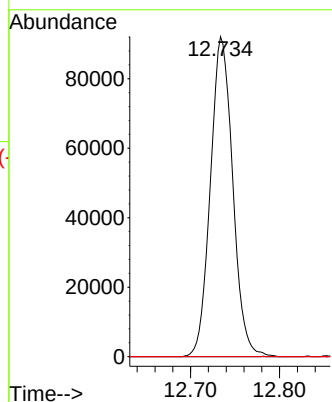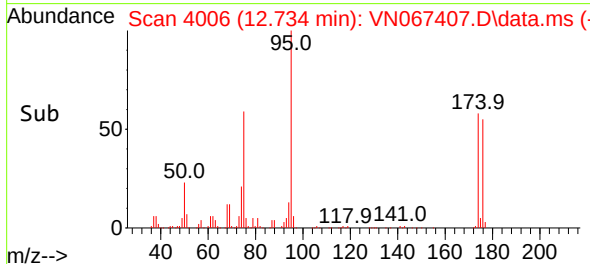


#82
4-Chlorotoluene
Concen: 0.24 ug/l
RT: 13.112 min Scan# 4147
Delta R.T. 0.006 min
Lab File: VN067407.D
Acq: 21 Jun 2021 11:02

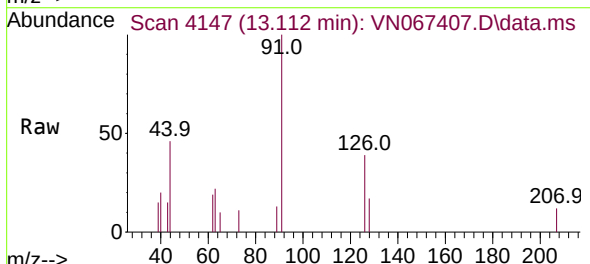

Tgt Ion: 91 Resp: 3136
Ion Ratio Lower Upper
91 100
126 30.8 14.8 44.4




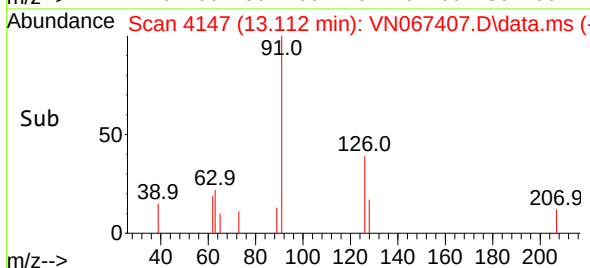


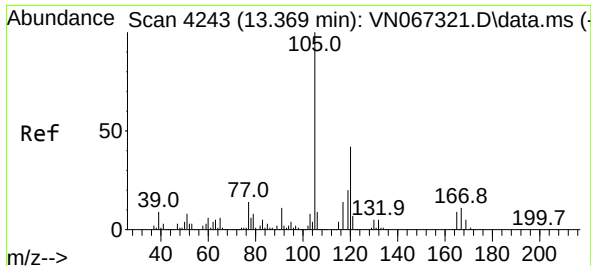

#84
1,2,4-Trimethylbenzene
Concen: 0.21 ug/l
RT: 13.372 min Scan# 4244
Delta R.T. 0.003 min
Lab File: VN067407.D
Acq: 21 Jun 2021 11:02




Instrument :
MSVOA_N
ClientSampleId :
VN0621MBL01


Tgt Ion:105 Resp: 3082
Ion Ratio Lower Upper
105 100
120 37.1 20.6 61.8

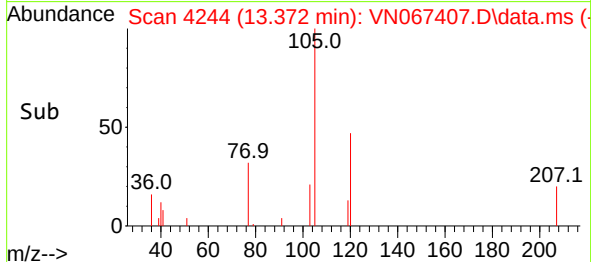

#86
p-Isopropyltoluene
Concen: 0.21 ug/l
RT: 13.619 min Scan# 4336
Delta R.T. 0.001 min
Lab File: VN067407.D
Acq: 21 Jun 2021 11:02

Tgt Ion:119 Resp: 2811
Ion Ratio Lower Upper
119 100
134 17.7 12.4 37.4
91 34.3 14.8 44.3

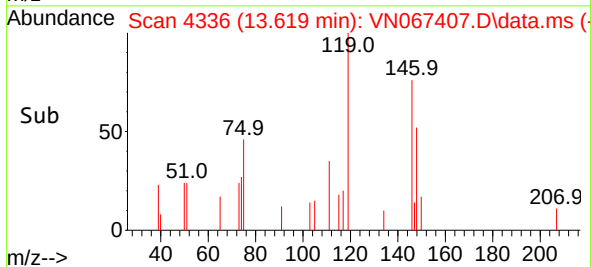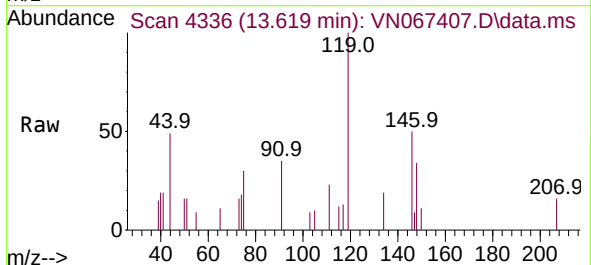

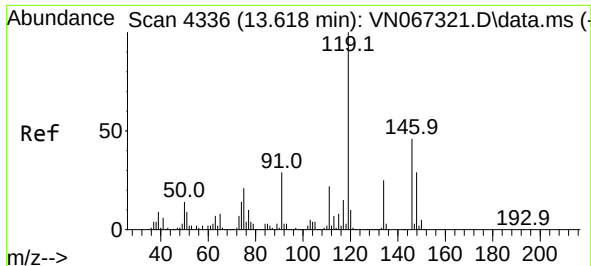

#87

1,3-Dichlorobenzene

Concen: 0.27 ug/l

RT: 13.619 min Scan# 4336





Delta R.T. 0.001 min

Lab File: VN067407.D

Acq: 21 Jun 2021 11:02

Tgt Ion:	146	Resp:	1734
Ion	Ratio	Lower	Upper
146	100		
111	38.7	24.3	72.8
148	67.5	32.0	96.0

Instrument :
MSVOA_N
ClientSampled :
VN0621MBL01

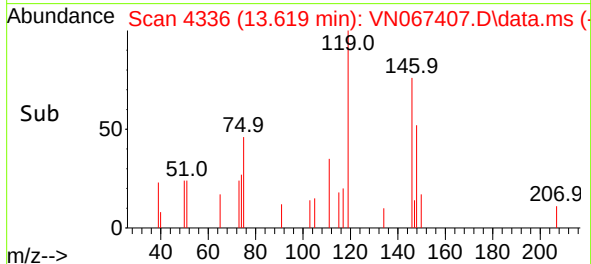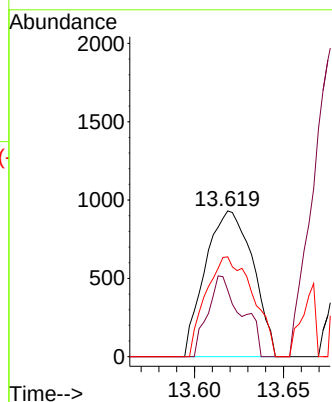

#88

1,4-Dichlorobenzene

Concen: 0.27 ug/l




RT: 13.619 min Scan# 4336


Delta R.T. -0.077 min

Lab File: VN067407.D

Acq: 21 Jun 2021 11:02

Tgt Ion:	146	Resp:	1734
Ion	Ratio	Lower	Upper
146	100		
111	38.7	23.4	70.2
148	67.5	31.8	95.3


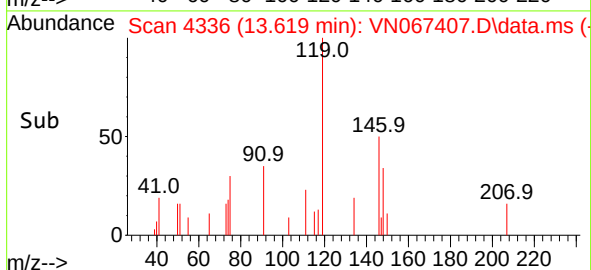

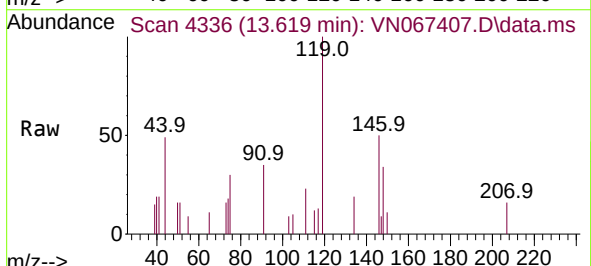


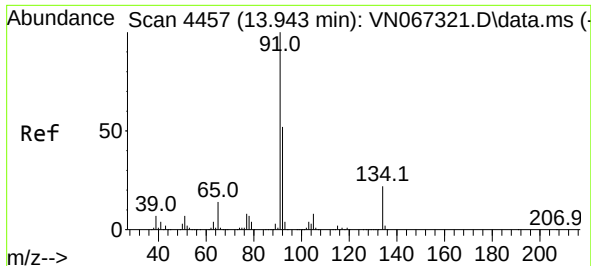

#89
n-Butylbenzene
Concen: 0.49 ug/l
RT: 13.948 min Scan# 4459
Delta R.T. 0.005 min
Lab File: VN067407.D
Acq: 21 Jun 2021 11:02




Instrument :
MSVOA_N
ClientSampleId :
VN0621MBL01


Tgt Ion: 91	Resp: 6227
Ion Ratio	Lower Upper
91	100
92	48.0 25.7 77.1
134	18.8 11.2 33.6

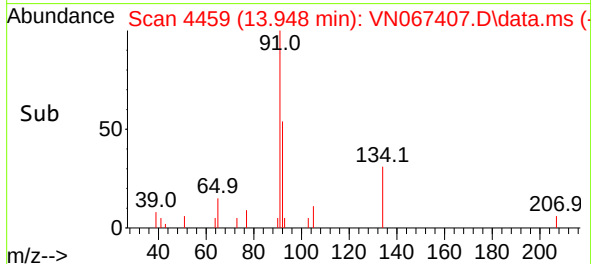

#91
1,2-Dichlorobenzene
Concen: 0.31 ug/l
RT: 13.991 min Scan# 4475
Delta R.T. 0.002 min
Lab File: VN067407.D
Acq: 21 Jun 2021 11:02

Tgt Ion: 146	Resp: 1898
Ion Ratio	Lower Upper
146	100
111	20.2 24.9 74.6#
148	73.9 31.6 95.0


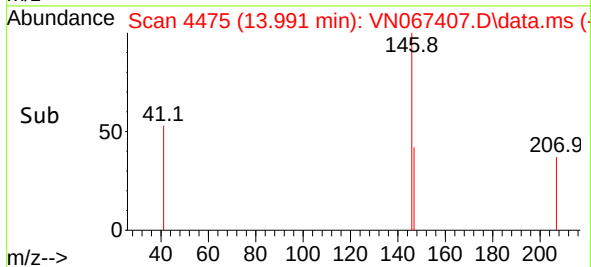

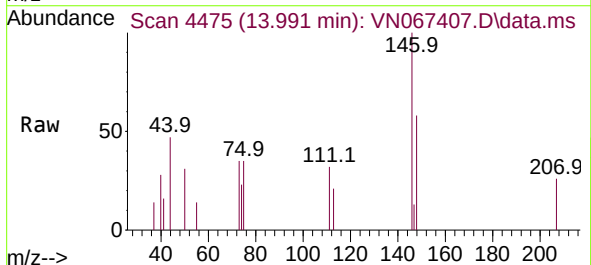


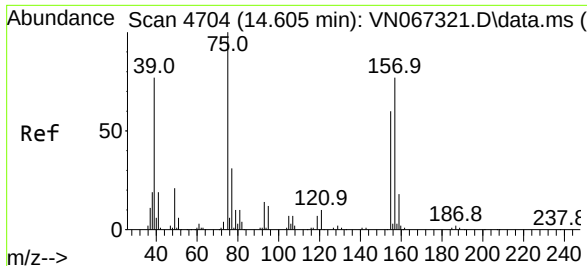

#92
 1,2-Dibromo-3-Chloropropane
 Concen: 0.37 ug/l
 RT: 14.606 min Scan# 4704
 Delta R.T. 0.001 min
 Lab File: VN067407.D
 Acq: 21 Jun 2021 11:02




Instrument :
 MSVOA_N
 ClientSampleId :
 VN0621MBL01


Tgt Ion: 75 Resp: 484
 Ion Ratio Lower Upper
 75 100
 155 57.6 29.8 89.5
 157 51.0 37.6 112.8

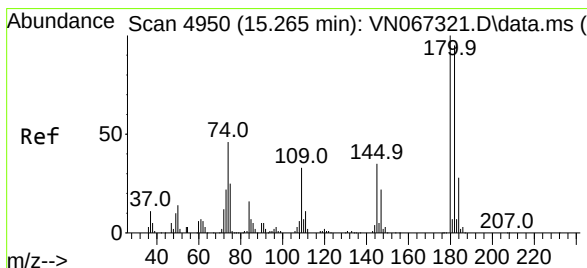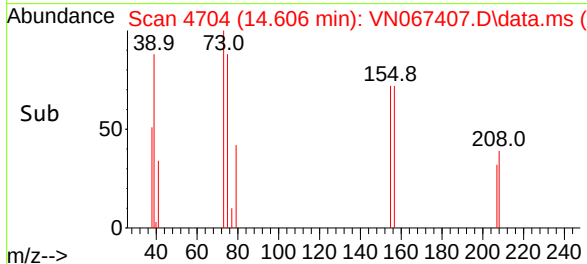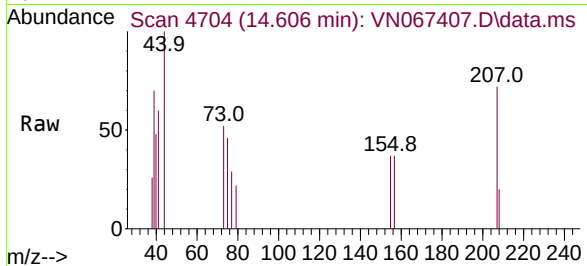

#93
 1,2,4-Trichlorobenzene
 Concen: 1.22 ug/l
 RT: 15.268 min Scan# 4951
 Delta R.T. 0.003 min
 Lab File: VN067407.D
 Acq: 21 Jun 2021 11:02

Tgt Ion:180 Resp: 3903
 Ion Ratio Lower Upper
 180 100
 182 90.7 47.5 142.5
 145 17.9 17.2 51.6


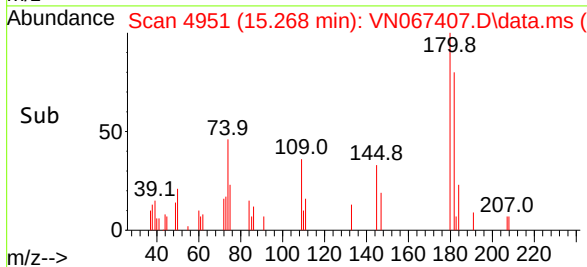

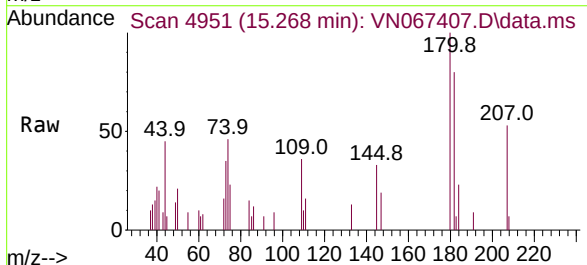


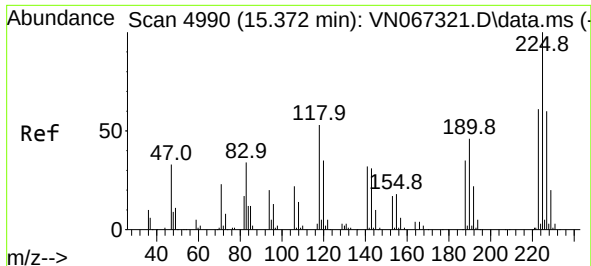

#94
Hexachlorobutadiene
Concen: 0.45 ug/l
RT: 15.375 min Scan# 4991
Delta R.T. 0.003 min
Lab File: VN067407.D
Acq: 21 Jun 2021 11:02




Instrument :
MSVOA_N
ClientSampleId :
VN0621MBL01


Tgt Ion:225 Resp: 823
Ion Ratio Lower Upper
225 100
223 52.7 31.4 94.0
227 49.2 31.2 93.6

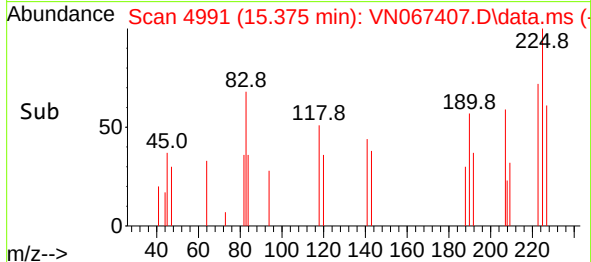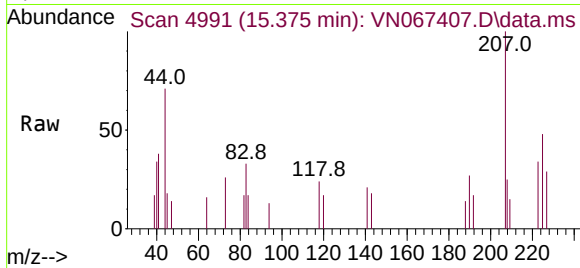

#95
Naphthalene
Concen: 4.54 ug/l
RT: 15.509 min Scan# 5041
Delta R.T. 0.002 min
Lab File: VN067407.D
Acq: 21 Jun 2021 11:02

Tgt Ion:128 Resp: 22654
Ion Ratio Lower Upper
128 100
127 13.1 10.6 15.8
129 10.2 8.6 12.8

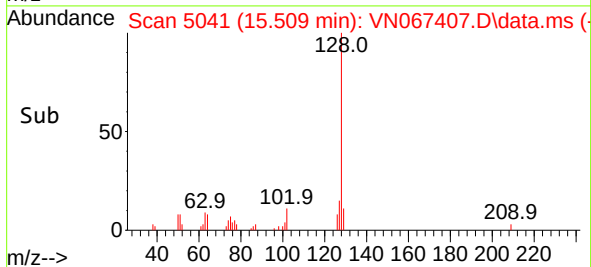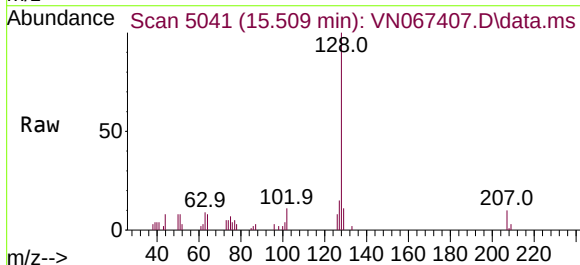



#96
 1,2,3-Trichlorobenzene
 Concen: 1.47 ug/l
 RT: 15.711 min Scan# 5116
 Delta R.T. 0.009 min
 Lab File: VN067407.D
 Acq: 21 Jun 2021 11:02

Instrument :
 MSVOA_N
 ClientSampleId :
 VN0621MBL01

Tgt Ion:180 Resp: 4511
 Ion Ratio Lower Upper
 180 100
 182 105.9 47.8 143.3
 145 19.2 18.2 54.6

