

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN062121\
 Data File : VN067407.D
 Acq On : 21 Jun 2021 11:02
 Operator : JC/MD
 Sample : VN0621MBL01
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN0621MBL01

Quant Time: Jun 22 03:09:11 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N061421W.M
 Quant Title : SW846 8260
 QLast Update : Tue Jun 15 05:19:42 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.088	168	299296	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.971	114	589712	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.749	117	520238	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.678	152	182492	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.440	65	286593	48.540	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	=	97.080%
35) Dibromofluoromethane	8.024	113	184125	46.946	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	=	93.900%
50) Toluene-d8	10.443	98	777733	51.737	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	=	103.480%
62) 4-Bromofluorobenzene	12.736	95	273423	44.074	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	=	88.140%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN062121\
Data File : VN067407.D
Acq On : 21 Jun 2021 11:02
Operator : JC/MD
Sample : VN0621MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN0621MBL01

Quant Time: Jun 22 03:09:11 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N061421W.M
Quant Title : SW846 8260
QLast Update : Tue Jun 15 05:19:42 2021
Response via : Initial Calibration




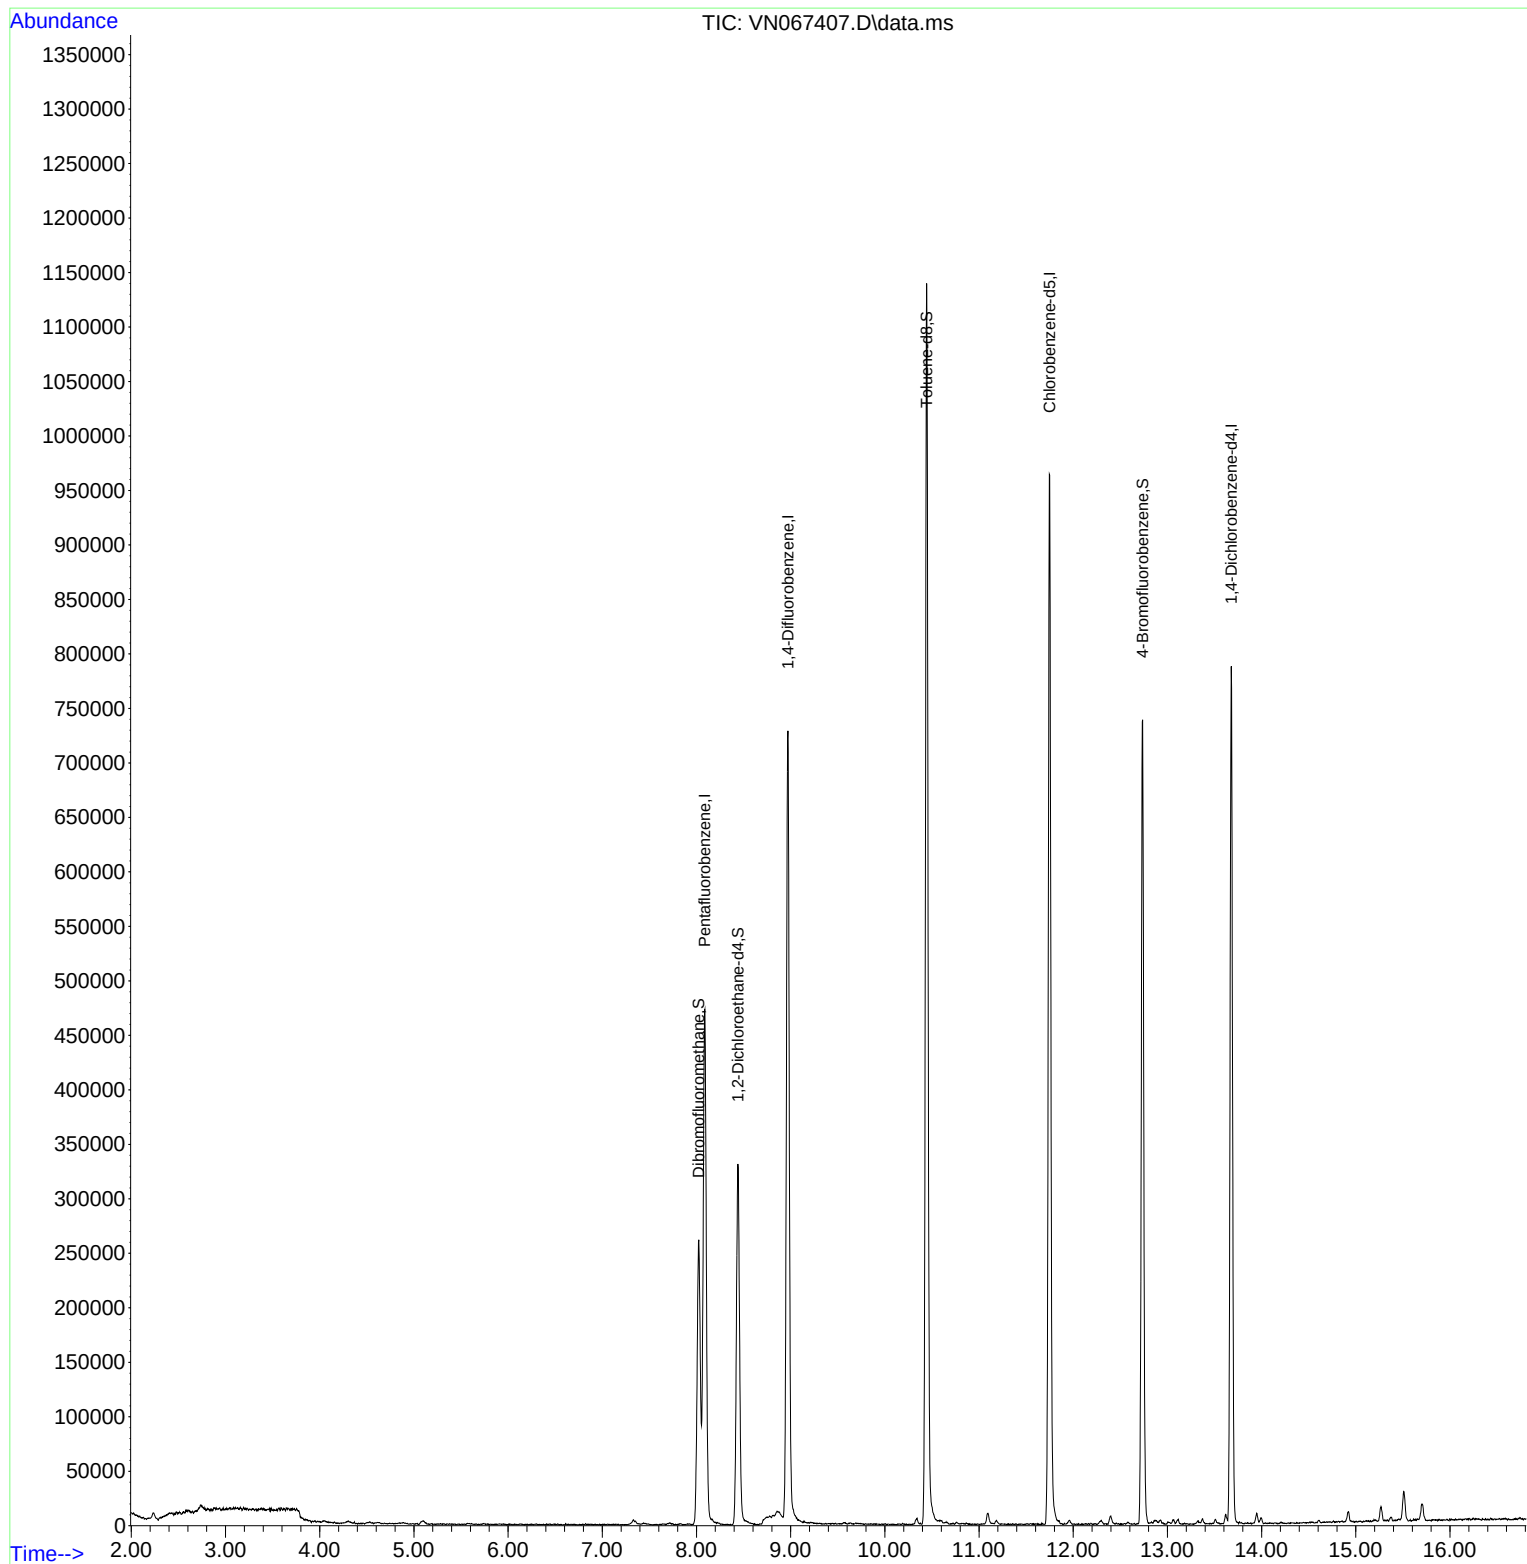


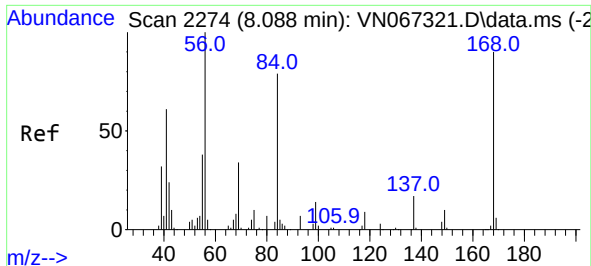

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.088 min Scan# 2274
Delta R.T. 0.000 min
Lab File: VN067407.D
Acq: 21 Jun 2021 11:02




Instrument :
MSVOA_N
ClientSampleId :
VN0621MBL01


Tgt Ion:168 Resp: 299296
Ion Ratio Lower Upper
168 100
99 80.0 62.9 94.3

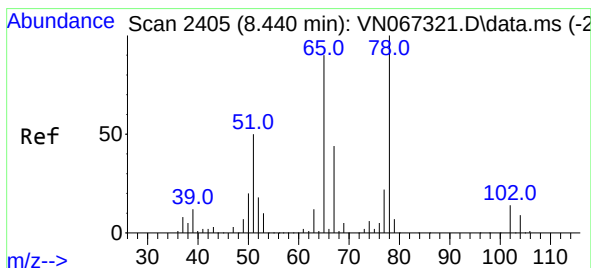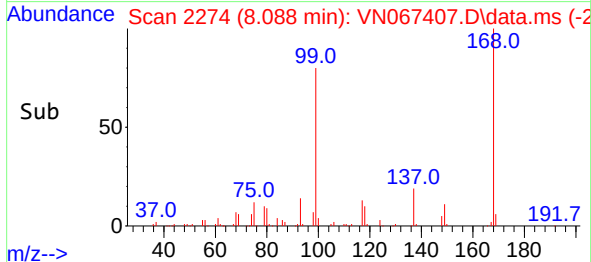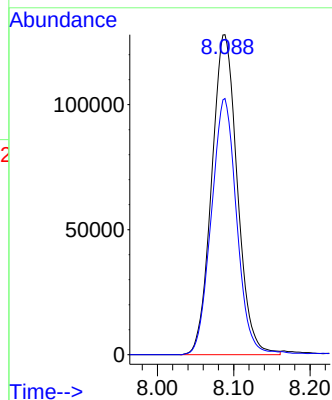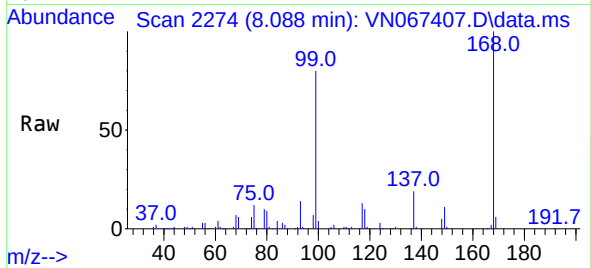

#33
1,2-Dichloroethane-d4
Concen: 48.540 ug/l
RT: 8.440 min Scan# 2405
Delta R.T. -0.000 min
Lab File: VN067407.D
Acq: 21 Jun 2021 11:02

Tgt Ion: 65 Resp: 286593
Ion Ratio Lower Upper
65 100
67 51.3 0.0 98.6

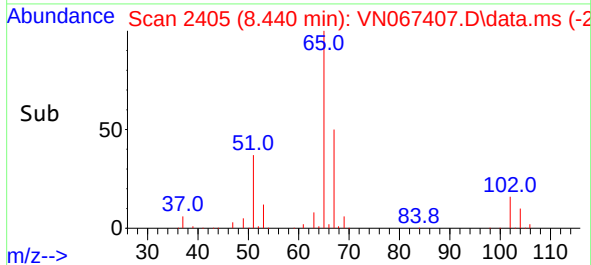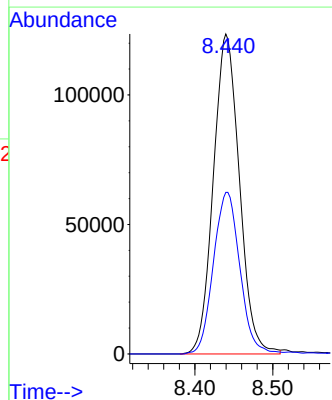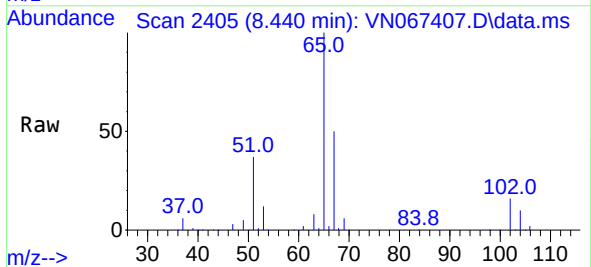




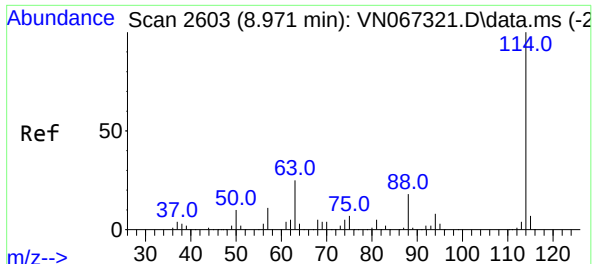


#34

1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.971 min Scan# 2603
Delta R.T. 0.000 min
Lab File: VN067407.D
Acq: 21 Jun 2021 11:02

Instrument :
MSVOA_N
ClientSampleId :
VN0621MBL01




Tgt Ion:114 Resp: 589712
Ion Ratio Lower Upper
114 100
63 26.5 0.0 49.0
88 18.7 0.0 36.6

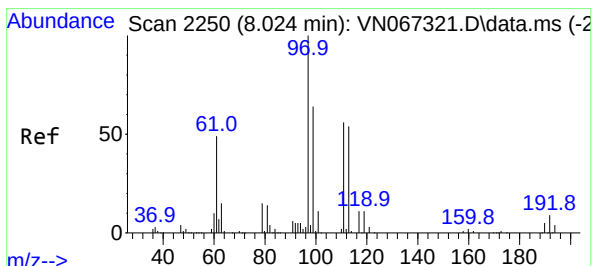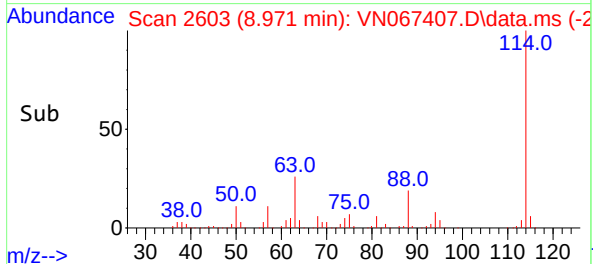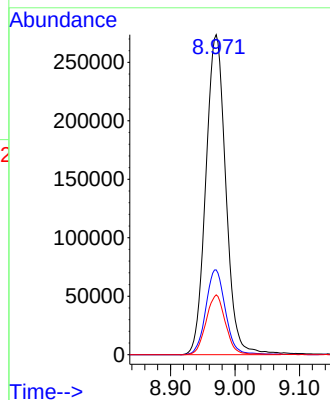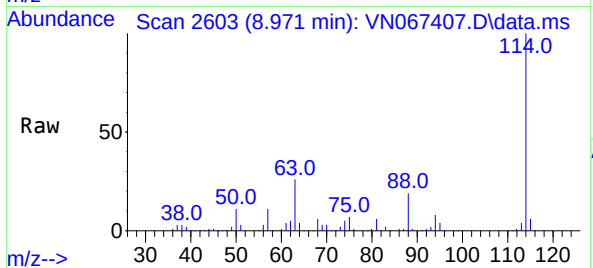


#35

Dibromofluoromethane
Concen: 46.946 ug/l
RT: 8.024 min Scan# 2250
Delta R.T. 0.000 min
Lab File: VN067407.D
Acq: 21 Jun 2021 11:02

Tgt Ion:113 Resp: 184125
Ion Ratio Lower Upper
113 100
111 105.2 83.8 125.8
192 15.0 13.4 20.0


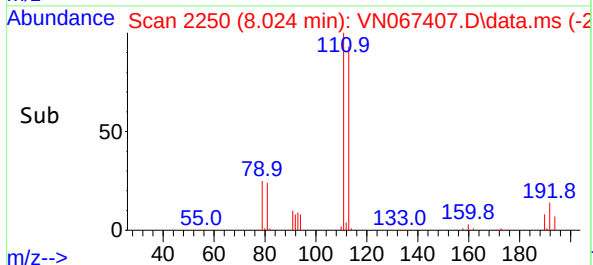
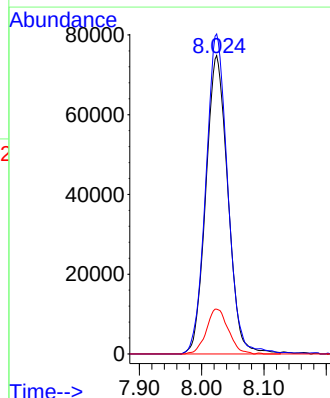
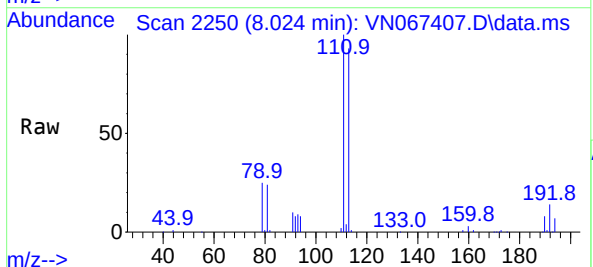


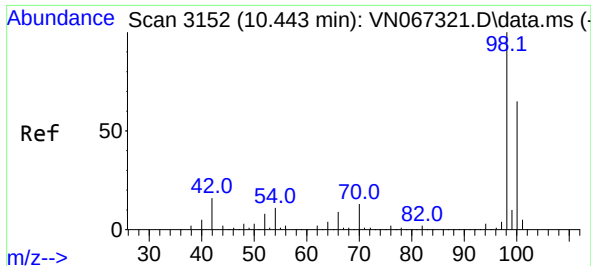

#50
Toluene-d8
Concen: 51.737 ug/l
RT: 10.443 min Scan# 3152
Delta R.T. 0.000 min
Lab File: VN067407.D
Acq: 21 Jun 2021 11:02




Instrument :
MSVOA_N
ClientSampleId :
VN0621MBL01


Tgt Ion: 98 Resp: 777733
Ion Ratio Lower Upper
98 100
100 63.5 51.7 77.5

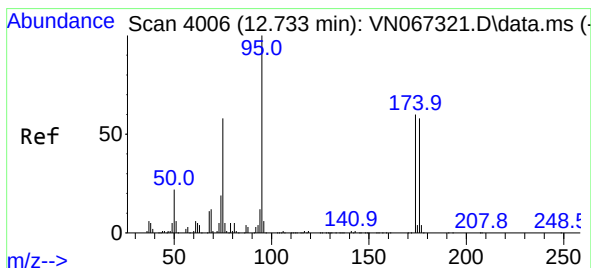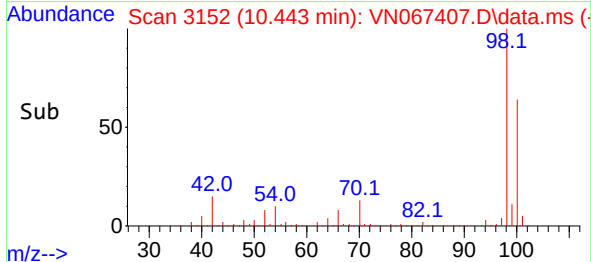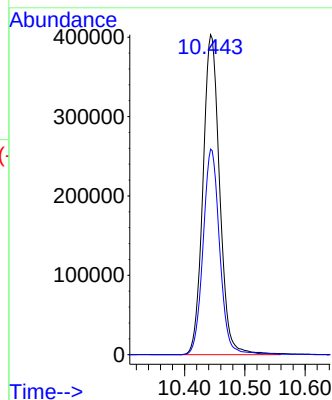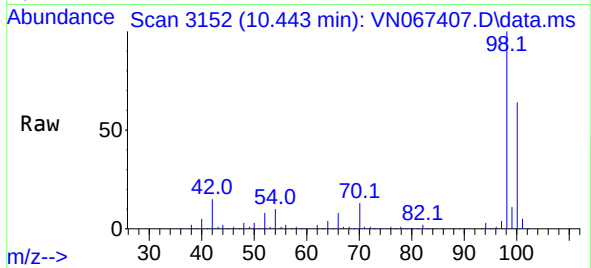

#62
4-Bromofluorobenzene
Concen: 44.074 ug/l
RT: 12.736 min Scan# 4007
Delta R.T. 0.003 min
Lab File: VN067407.D
Acq: 21 Jun 2021 11:02

Tgt Ion: 95 Resp: 273423
Ion Ratio Lower Upper
95 100
174 58.2 0.0 122.0
176 55.8 0.0 117.6


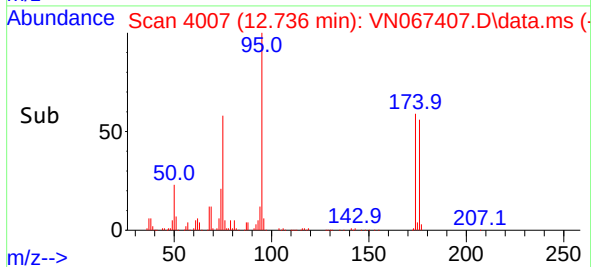
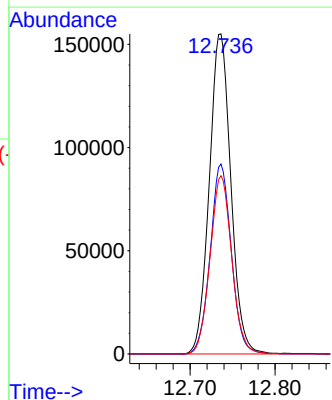
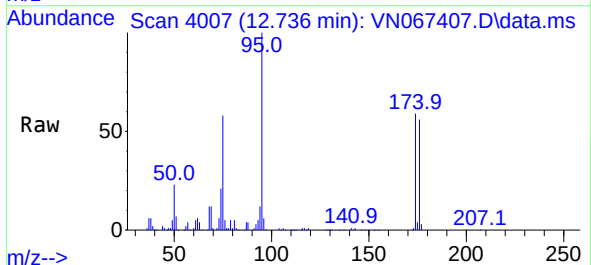


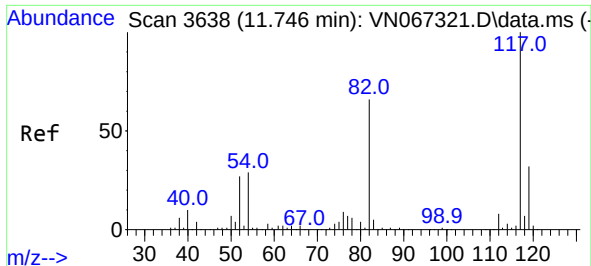

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.749 min Scan# 3639
Delta R.T. 0.003 min
Lab File: VN067407.D
Acq: 21 Jun 2021 11:02

Instrument :
MSVOA_N
ClientSampleId :
VN0621MBL01

Tgt Ion:117 Resp: 520238
Ion Ratio Lower Upper
117 100
82 67.3 53.1 79.7
119 32.2 25.5 38.3

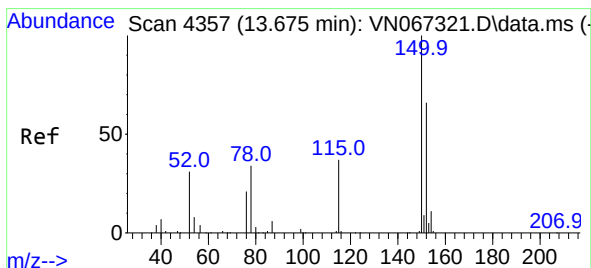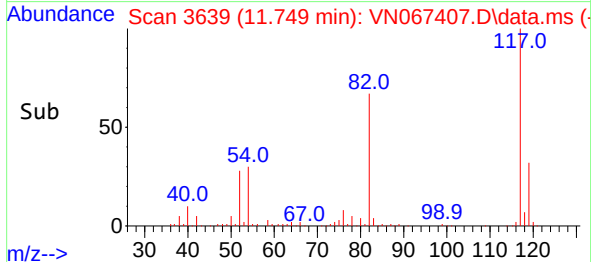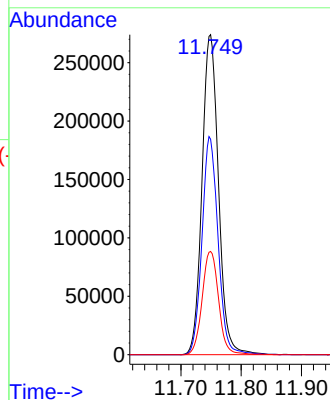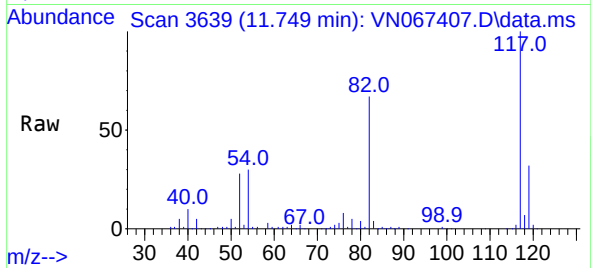

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.678 min Scan# 4358
Delta R.T. 0.003 min
Lab File: VN067407.D
Acq: 21 Jun 2021 11:02

Tgt Ion:152 Resp: 182492
Ion Ratio Lower Upper
152 100
115 69.5 36.1 108.5
150 157.1 0.0 351.8

