
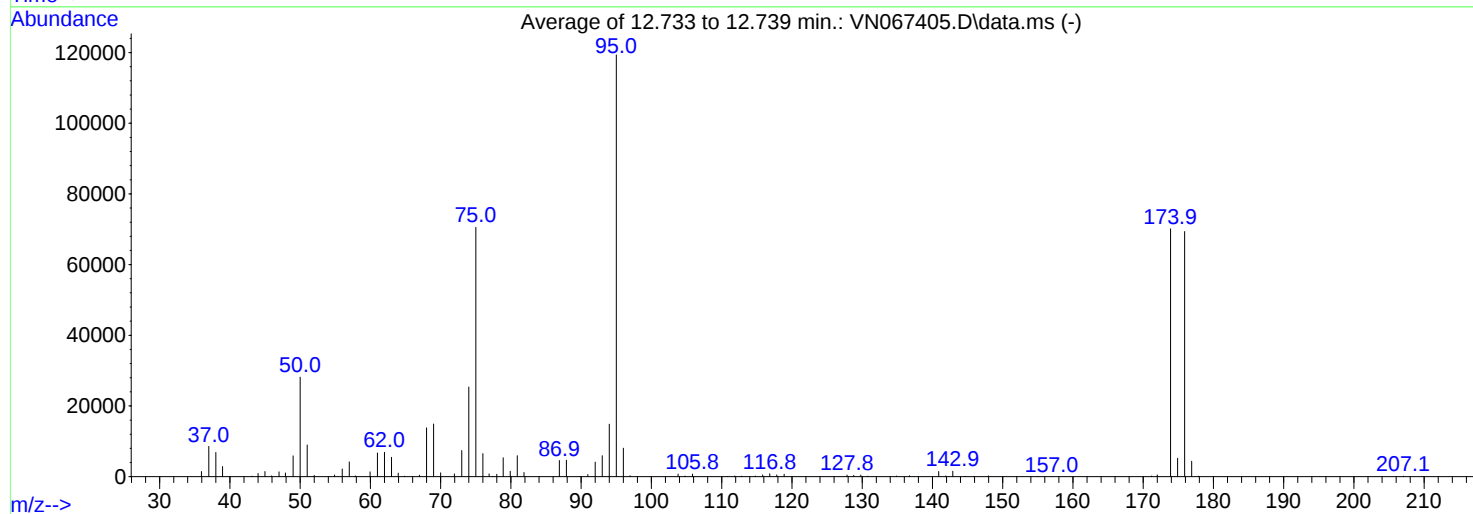


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN062121\
 Data File : VN067405.D
 Acq On : 21 Jun 2021 9:06
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N061421W.M
 Title : SW846 8260
 Last Update : Tue Jun 15 05:19:42 2021

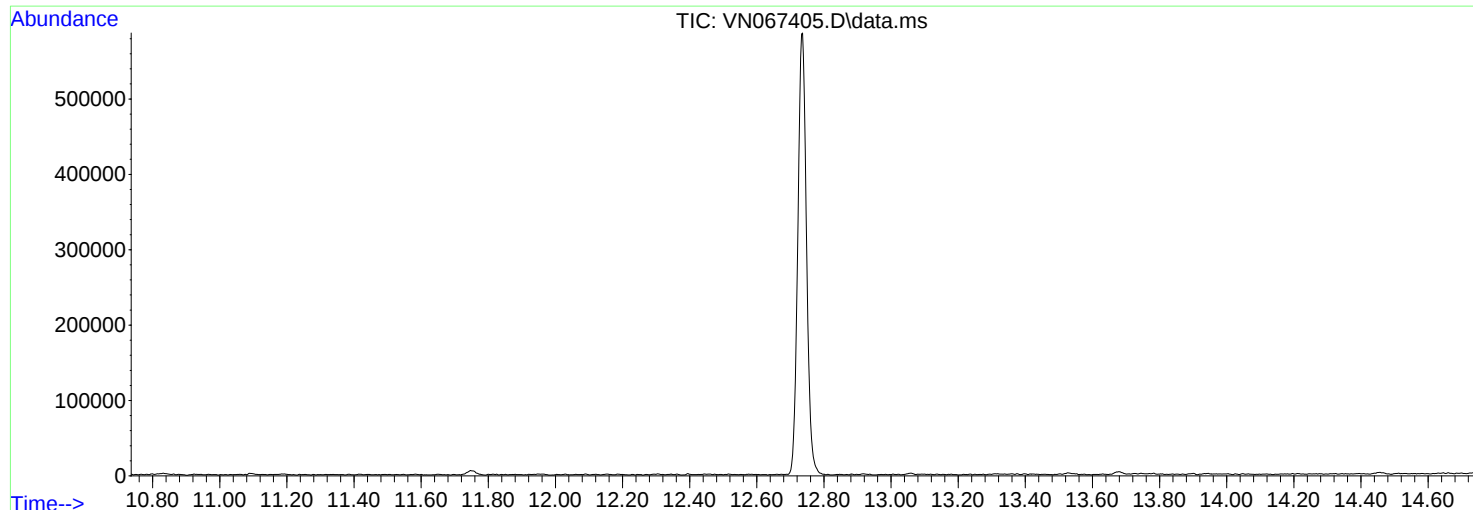

AutoFind: Scans 4006, 4007, 4008; Background Corrected with Scan 3989

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.6	28155	PASS
75	95	30	60	59.1	70544	PASS
95	95	100	100	100.0	119352	PASS
96	95	5	9	6.8	8064	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	58.8	70139	PASS
175	174	5	9	7.4	5222	PASS
176	174	95	101	98.9	69376	PASS
177	176	5	9	6.3	4348	PASS