

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN062122\
 Data File : VN072976.D
 Acq On : 21 Jun 2022 12:16
 Operator : JC\MD
 Sample : N3357-10DL 20X
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 MW-44DL

Quant Time: Jun 22 06:59:36 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N061722W.M
 Quant Title : SW846 8260
 QLast Update : Sat Jun 18 06:22:45 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.016	168	340642	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.904	114	540102	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.680	117	489382	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.610	152	250609	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.369	65	199425	43.302	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery =	86.600%		
35) Dibromofluoromethane	7.951	113	169803	50.865	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	101.720%		
50) Toluene-d8	10.374	98	553955	44.595	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery =	89.180%		
62) 4-Bromofluorobenzene	12.663	95	247517	55.413	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	110.820%		
Target Compounds						Qvalue
3) Chloromethane	2.263	50	582	0.734	ug/l #	43
6) Chloroethane	2.898	64	516	0.284	ug/l #	84
11) Tert butyl alcohol	5.234	59	1441	1.211	ug/l #	72
16) Acetone	4.245	43	1286	0.508	ug/l #	87
25) 2-Butanone	7.275	43	912	0.227	ug/l #	45
26) 2,2-Dichloropropane	7.228	77	2219	Below Cal	#	53
31) Cyclohexane	8.016	56	8803	1.413	ug/l #	26
36) 1,1-Dichloropropene	8.016	75	27186	6.018	ug/l #	49
38) Carbon Tetrachloride	8.010	117	34593	7.281	ug/l #	17
39) Methylcyclohexane	9.392	83	2771	0.509	ug/l	88
51) 4-Methyl-2-Pentanone	10.263	43	1406	0.209	ug/l #	56
52) Toluene	10.439	92	5998	0.688	ug/l	90
55) 1,1,2-Trichloroethane	10.798	97	1246	0.326	ug/l #	16
59) 2-Hexanone	11.069	43	2090	0.401	ug/l	94
67) Ethyl Benzene	11.780	91	1126962	66.984	ug/l	100
68) m/p-Xylenes	11.886	106	525419	79.623	ug/l	98
69) o-Xylene	12.216	106	27436	4.161	ug/l	95
73) Isopropylbenzene	12.516	105	51915	2.678	ug/l	97
76) 1,2,3-Trichloropropane	12.663	75	127942	21.057	ug/l #	1
78) n-propylbenzene	12.857	91	224252	10.516	ug/l	99
79) 2-Chlorotoluene	12.951	91	24331	1.762	ug/l #	41
80) 1,3,5-Trimethylbenzene	12.992	105	225252	14.144	ug/l	97
81) trans-1,4-Dichloro-2-b...	12.663	75	127942	56.867	ug/l #	10
82) 4-Chlorotoluene	12.992	91	23134	1.771	ug/l #	40
83) tert-Butylbenzene	13.304	119	164231	11.260	ug/l #	60
84) 1,2,4-Trimethylbenzene	13.304	105	1371403	86.458	ug/l	98
85) sec-Butylbenzene	13.304	105	1371403	70.485	ug/l #	56
86) p-Isopropyltoluene	13.492	119	9485	0.602	ug/l #	74
89) n-Butylbenzene	13.810	91	83131	6.463	ug/l #	43
90) Hexachloroethane	14.151	117	14485	4.878	ug/l #	9
95) Naphthalene	15.427	128	502048	25.932	ug/l	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN062122\
Data File : VN072976.D
Acq On : 21 Jun 2022 12:16
Operator : JC\MD
Sample : N3357-10DL 20X
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
MW-44DL

Quant Time: Jun 22 06:59:36 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N061722W.M
Quant Title : SW846 8260
QLast Update : Sat Jun 18 06:22:45 2022
Response via : Initial Calibration




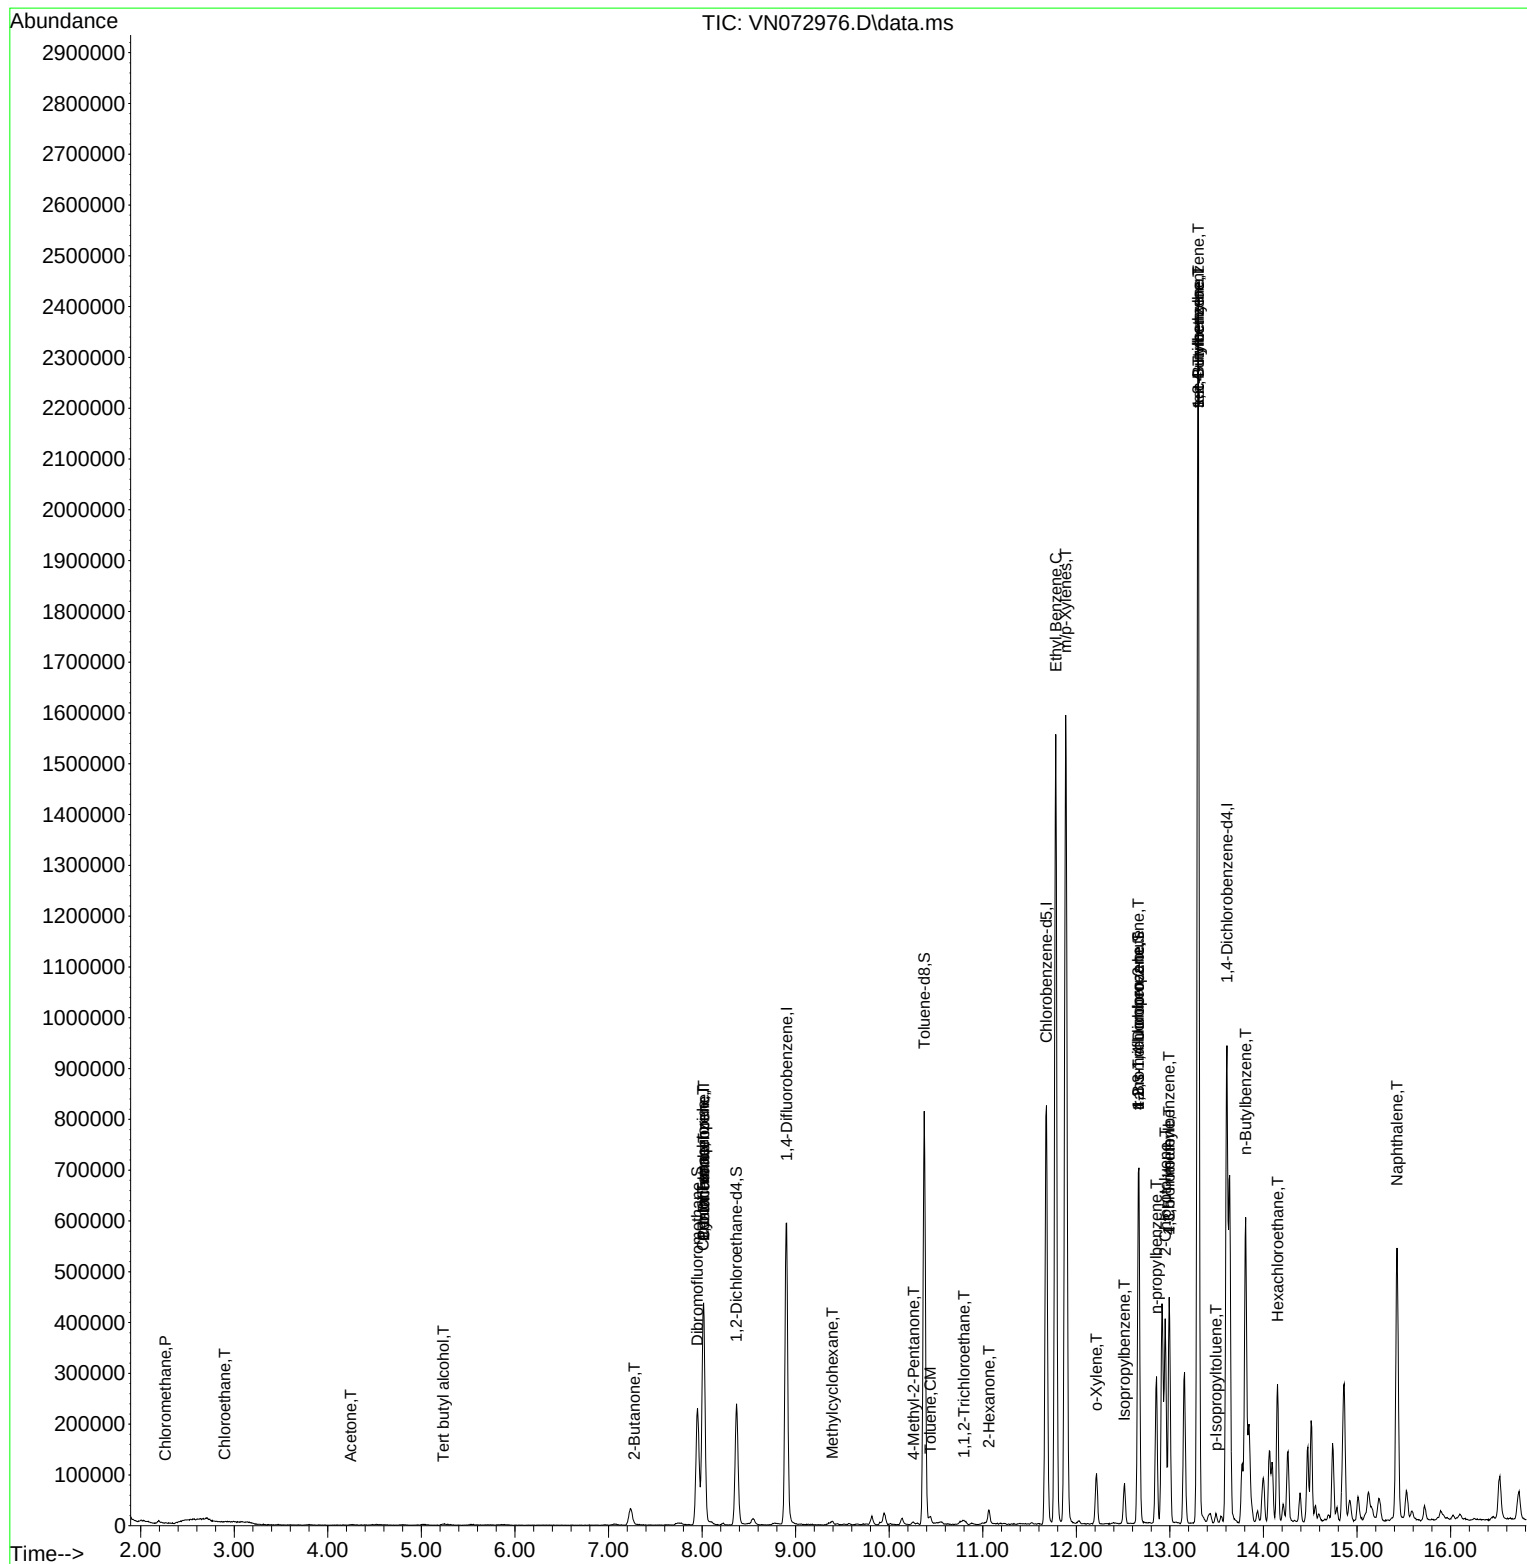




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.016 min Scan# 1042
Delta R.T. -0.000 min
Lab File: VN072976.D
Acq: 21 Jun 2022 12:16




Instrument :
MSVOA_N
ClientSampleId :
MW-44DL


Tgt Ion:168 Resp: 340642
Ion Ratio Lower Upper
168 100
99 58.8 42.3 63.5

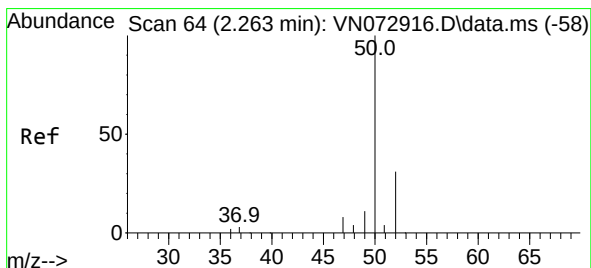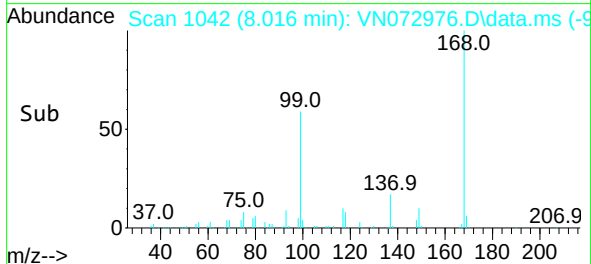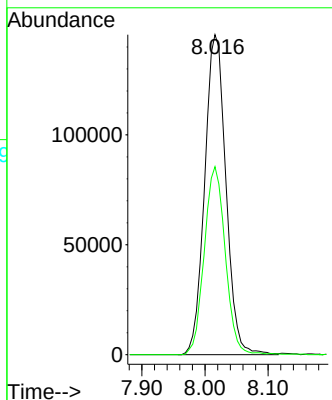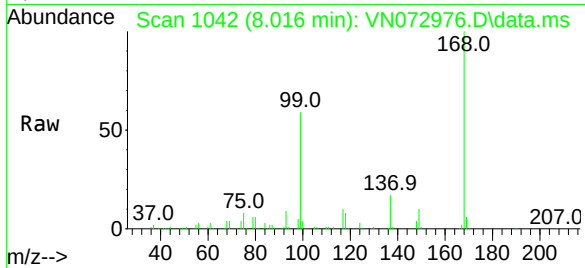

#3
Chloromethane
Concen: 0.734 ug/l
RT: 2.263 min Scan# 64
Delta R.T. 0.000 min
Lab File: VN072976.D
Acq: 21 Jun 2022 12:16

Tgt Ion: 50 Resp: 582
Ion Ratio Lower Upper
50 100
52 0.0 25.7 38.5#


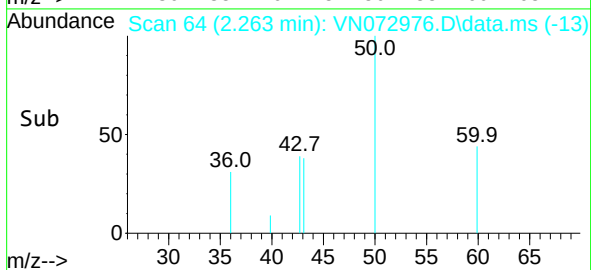
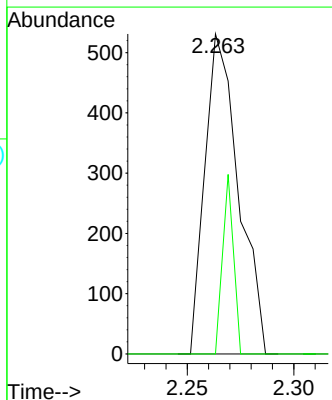
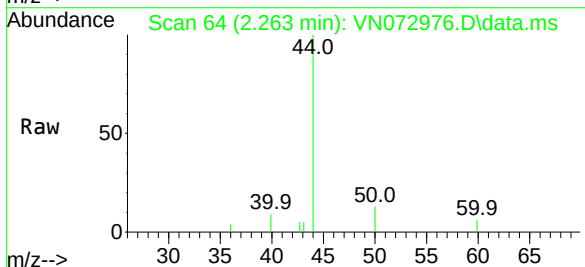




#6
Chloroethane
Concen: 0.284 ug/l
RT: 2.898 min Scan# 11
Delta R.T. -0.053 min
Lab File: VN072976.D
Acq: 21 Jun 2022 12:16




Instrument :
MSVOA_N
ClientSampleId :
MW-44DL


Tgt Ion: 64 Resp: 516
Ion Ratio Lower Upper
64 100
66 24.0 26.2 39.4#

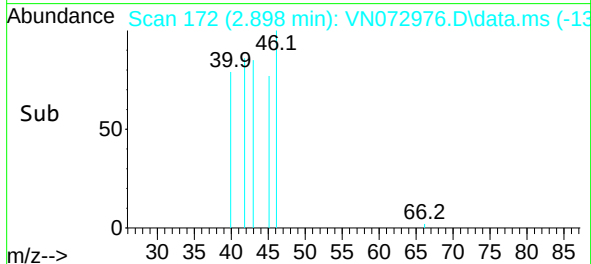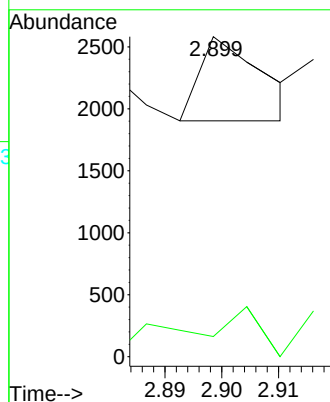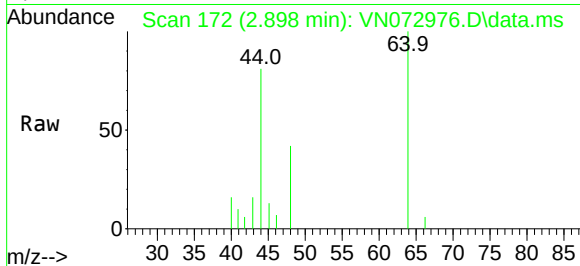

#11
Tert butyl alcohol
Concen: 1.211 ug/l
RT: 5.234 min Scan# 569
Delta R.T. -0.071 min
Lab File: VN072976.D
Acq: 21 Jun 2022 12:16

Tgt Ion: 59 Resp: 1441
Ion Ratio Lower Upper
59 100
57 0.0 8.3 12.5#


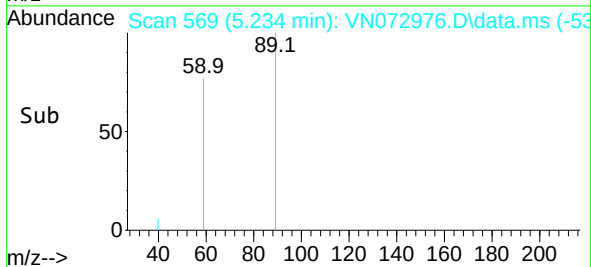
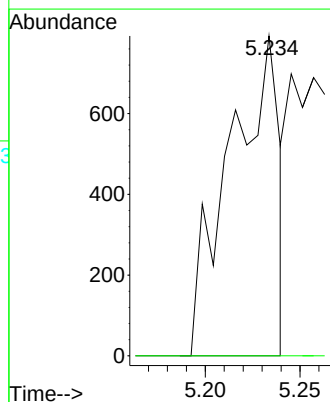
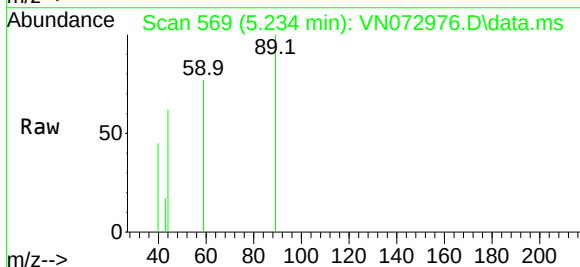




#16
Acetone
Concen: 0.508 ug/l
RT: 4.245 min Scan# 401
Delta R.T. 0.018 min
Lab File: VN072976.D
Acq: 21 Jun 2022 12:16




Instrument :
MSVOA_N
ClientSampleId :
MW-44DL


Tgt Ion: 43 Resp: 1286
Ion Ratio Lower Upper
43 100
58 40.0 26.0 39.0#

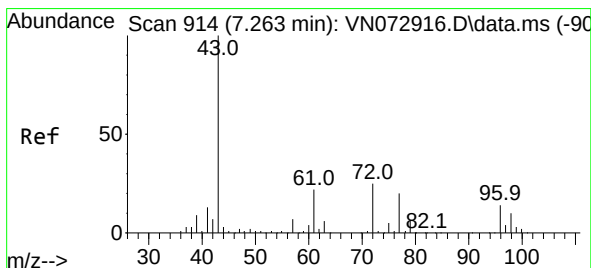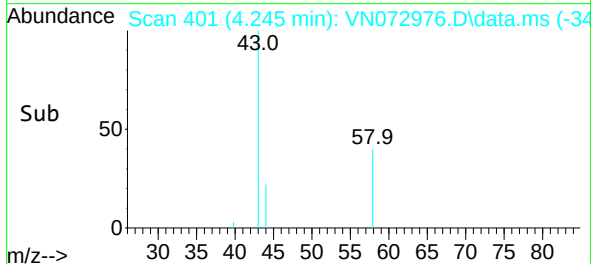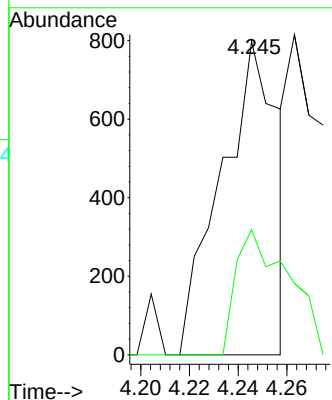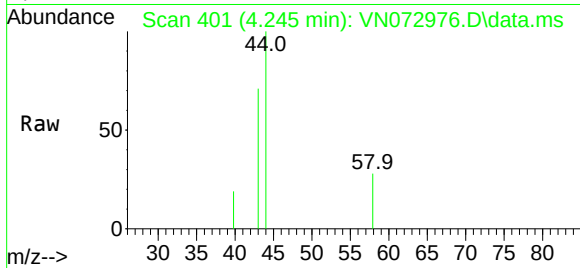

#25
2-Butanone
Concen: 0.227 ug/l
RT: 7.275 min Scan# 916
Delta R.T. 0.012 min
Lab File: VN072976.D
Acq: 21 Jun 2022 12:16

Tgt Ion: 43 Resp: 912
Ion Ratio Lower Upper
43 100
72 0.0 23.7 35.5#


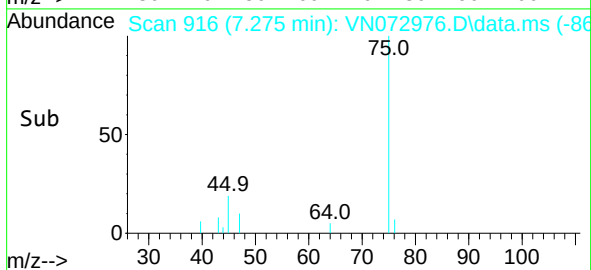
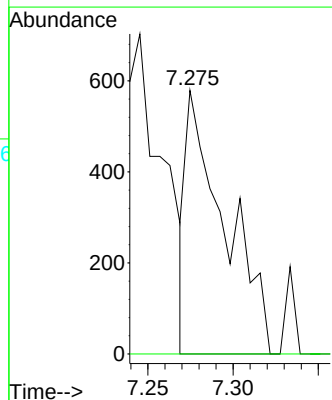
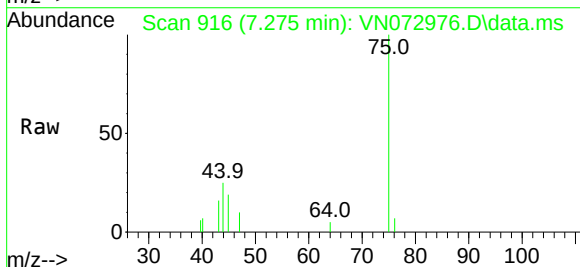




#31
Cyclohexane
Concen: 1.413 ug/l
RT: 8.016 min Scan# 1042
Delta R.T. -0.006 min
Lab File: VN072976.D
Acq: 21 Jun 2022 12:16




Instrument :
MSVOA_N
ClientSampleId :
MW-44DL


Tgt Ion: 56 Resp: 8803
Ion Ratio Lower Upper
56 100
69 150.1 27.8 41.8#
84 124.1 76.9 115.3#

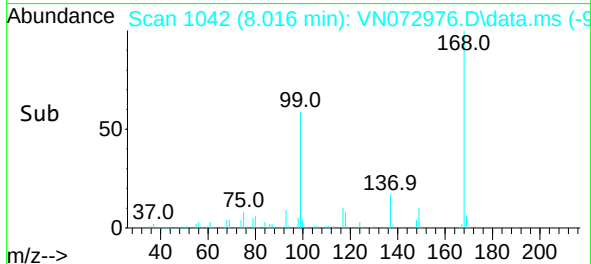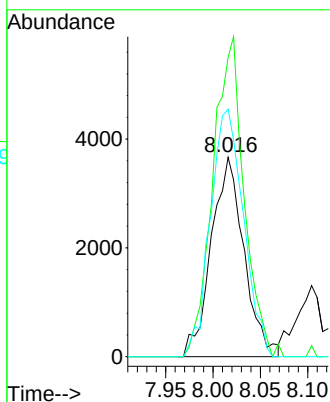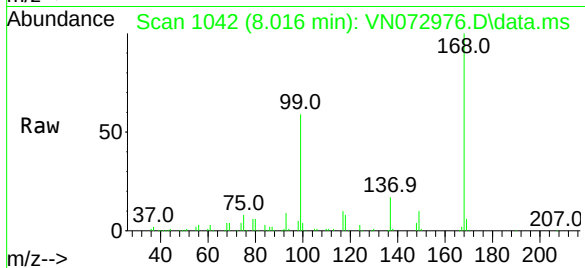

#33
1,2-Dichloroethane-d4
Concen: 43.302 ug/l
RT: 8.369 min Scan# 1102
Delta R.T. 0.000 min
Lab File: VN072976.D
Acq: 21 Jun 2022 12:16

Tgt Ion: 65 Resp: 199425
Ion Ratio Lower Upper
65 100
67 51.5 0.0 104.8

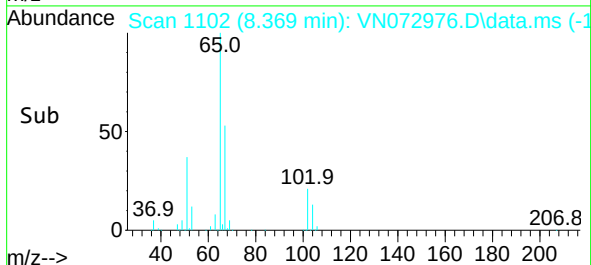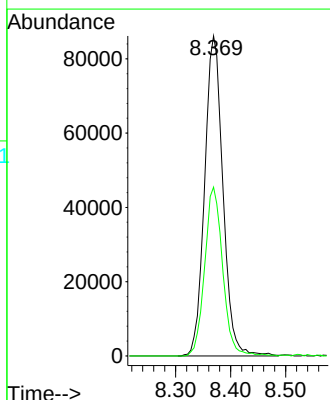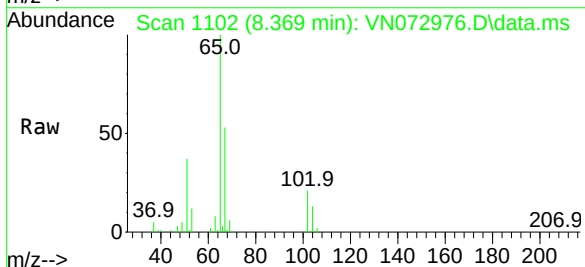

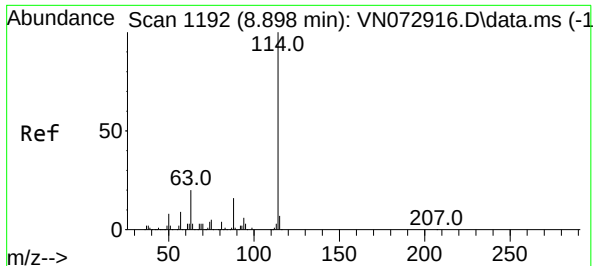

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.904 min Scan# 1193

Delta R.T. 0.006 min

Lab File: VN072976.D

Acq: 21 Jun 2022 12:16

Instrument :

MSVOA_N

ClientSampleId :

MW-44DL





Tgt Ion:114 Resp: 540102

Ion Ratio Lower Upper

114 100

63 20.3 0.0 40.0

88 15.4 0.0 32.6

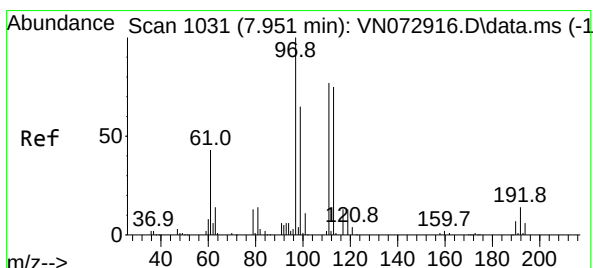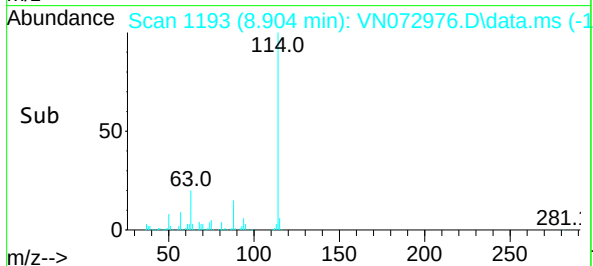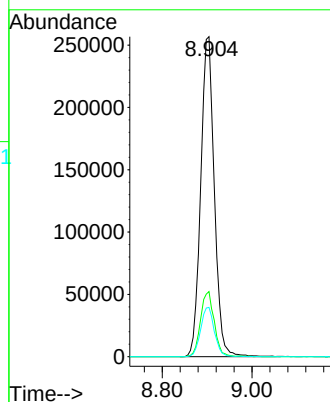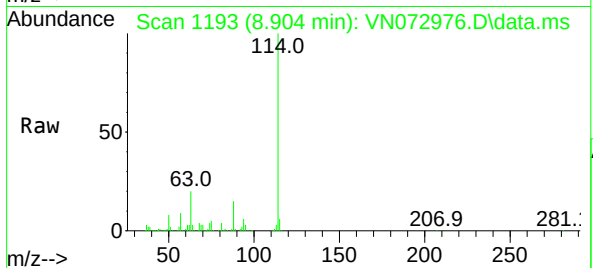

#35

Dibromofluoromethane

Concen: 50.865 ug/l

RT: 7.951 min Scan# 1031

Delta R.T. 0.000 min

Lab File: VN072976.D

Acq: 21 Jun 2022 12:16




Tgt Ion:113 Resp: 169803


Ion Ratio Lower Upper

113 100

111 104.9 81.4 122.0

192 19.2 17.0 25.6

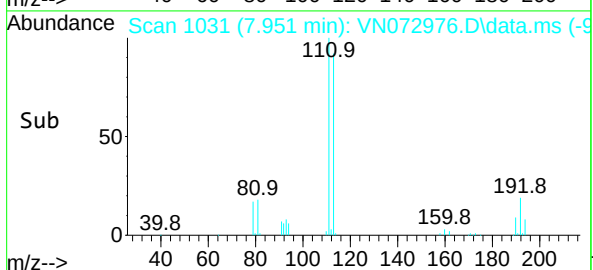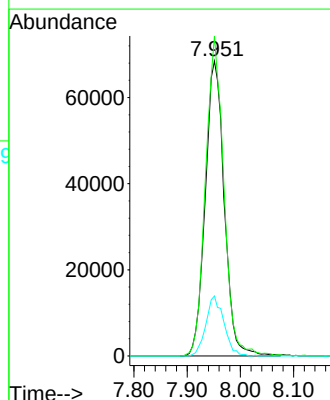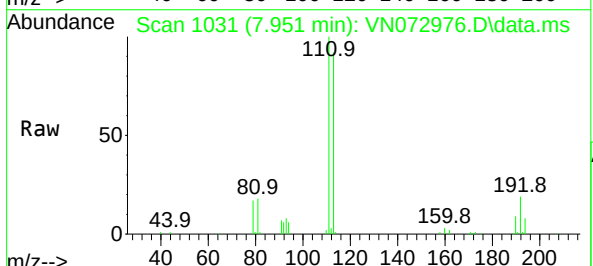

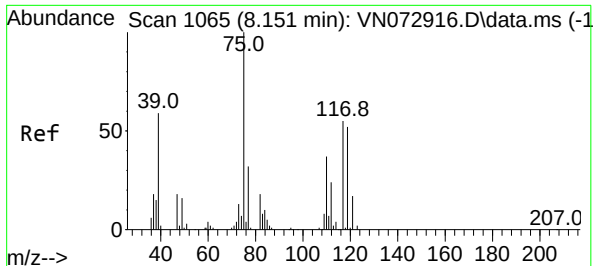

#36

1,1-Dichloropropene

Concen: 6.018 ug/l

RT: 8.016 min Scan# 1042

Delta R.T. -0.135 min

Lab File: VN072976.D

Acq: 21 Jun 2022 12:16





Instrument :

MSVOA_N

ClientSampleId :

MW-44DL

Tgt Ion: 75	Resp: 27186
Ion Ratio	Lower Upper
75	100
110	8.7 18.3 54.8#
77	0.0 25.1 37.7#

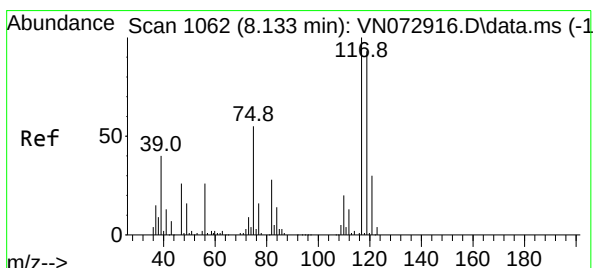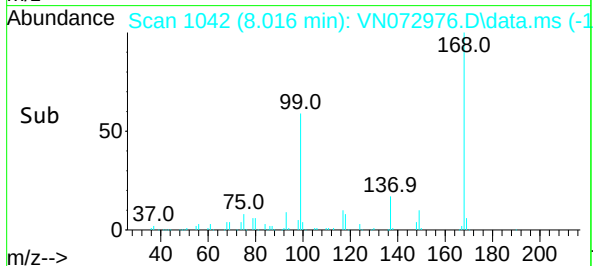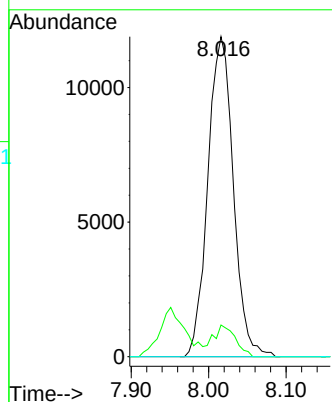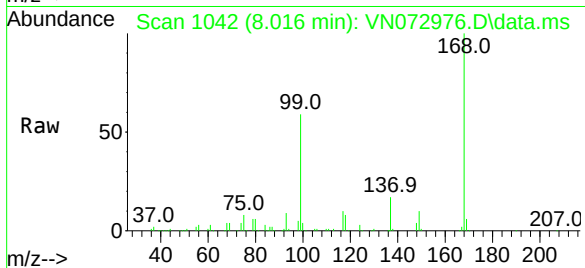

#38

Carbon Tetrachloride

Concen: 7.281 ug/l




RT: 8.010 min Scan# 1041


Delta R.T. -0.123 min

Lab File: VN072976.D

Acq: 21 Jun 2022 12:16

Tgt Ion: 117	Resp: 34593
Ion Ratio	Lower Upper
117	100
119	6.2 75.8 113.8#
121	0.0 24.6 37.0#

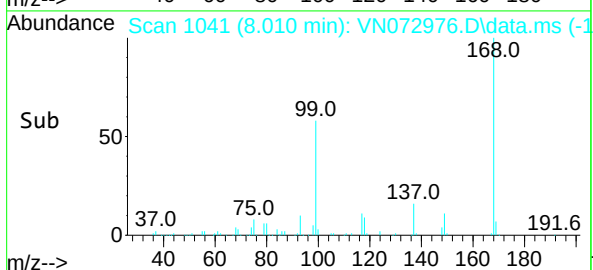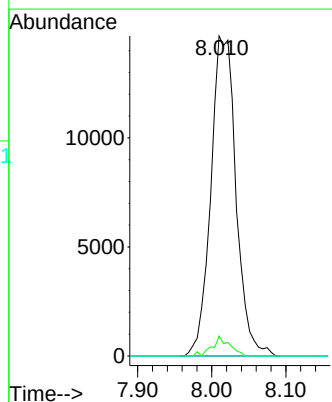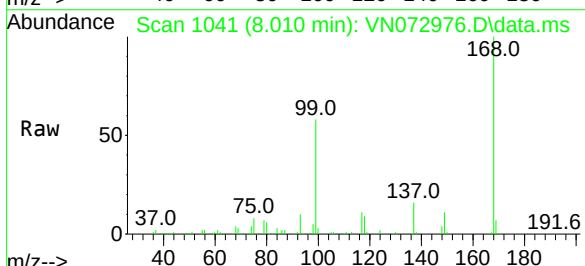

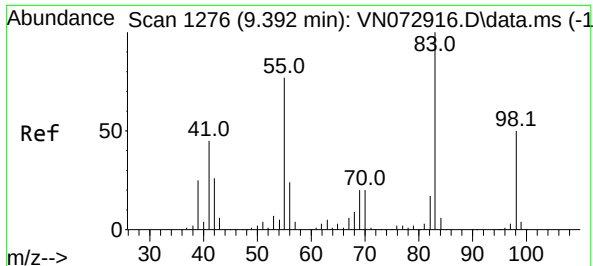

#39

Methylcyclohexane

Concen: 0.509 ug/l

RT: 9.392 min Scan# 1276

Delta R.T. 0.000 min

Lab File: VN072976.D

Acq: 21 Jun 2022 12:16

Instrument :

MSVOA_N

ClientSampleId :

MW-44DL





Tgt Ion: 83 Resp: 2771

Ion Ratio Lower Upper

83 100

55 81.2 57.8 86.8

98 58.5 39.4 59.2

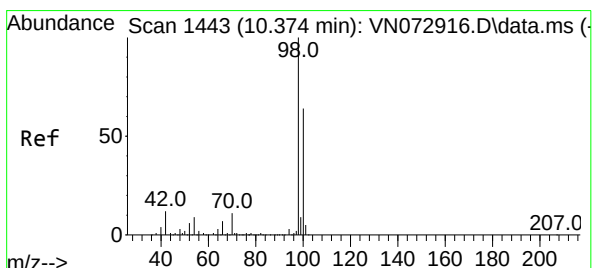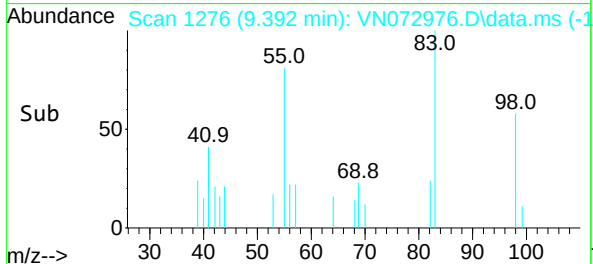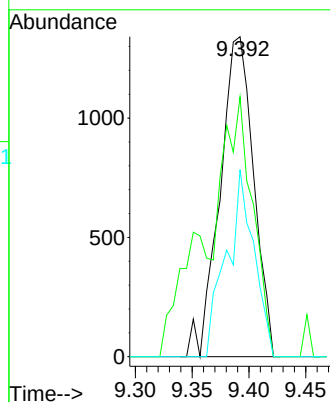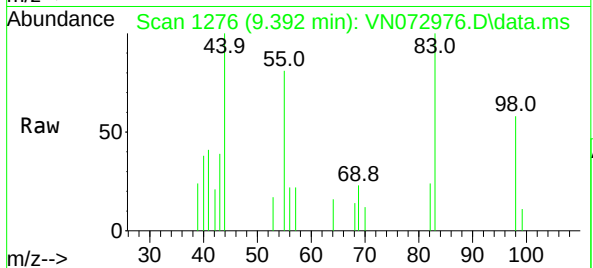

#50

Toluene-d8

Concen: 44.595 ug/l

RT: 10.374 min Scan# 1443

Delta R.T. 0.000 min

Lab File: VN072976.D




Acq: 21 Jun 2022 12:16


Tgt Ion: 98 Resp: 553955

Ion Ratio Lower Upper

98 100

100 66.3 52.6 78.8

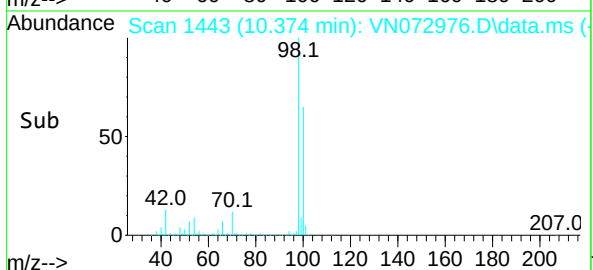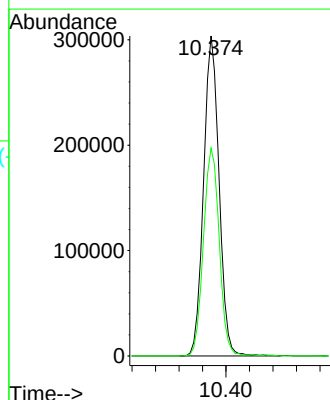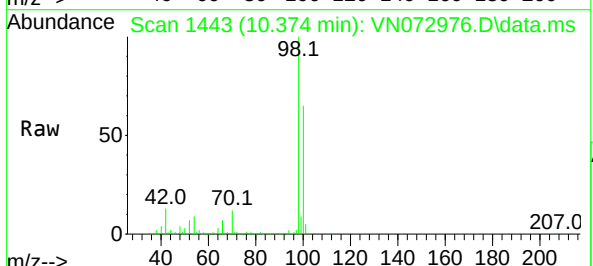

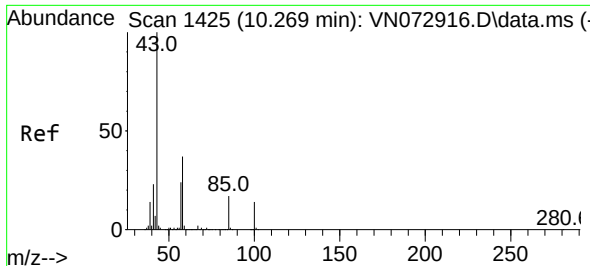

#51

4-Methyl-2-Pentanone

Concen: 0.209 ug/l

RT: 10.263 min Scan# 1424

Delta R.T. -0.006 min

Lab File: VN072976.D

Acq: 21 Jun 2022 12:16

Instrument :

MSVOA_N

ClientSampleId :





MW-44DL

Tgt Ion: 43 Resp: 1406

Ion Ratio Lower Upper

43 100

58 14.9 34.1 51.1#

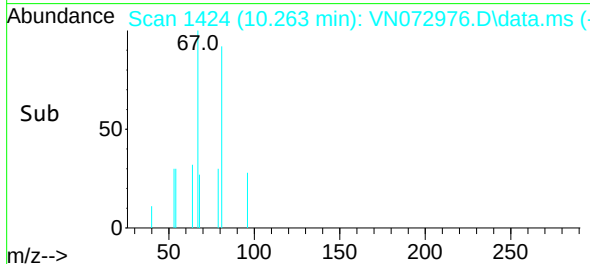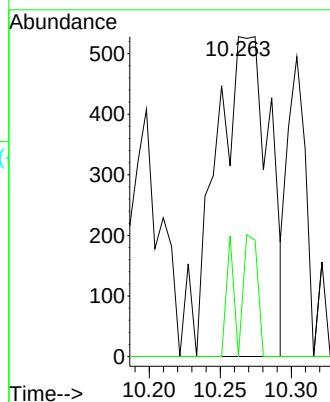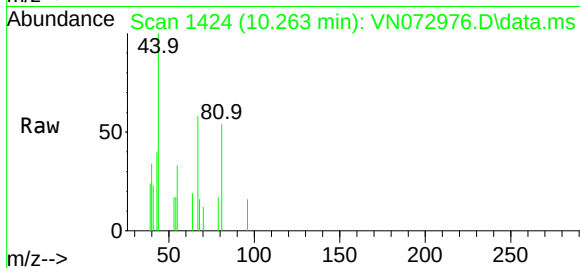

#52

Toluene

Concen: 0.688 ug/l

RT: 10.439 min Scan# 1454

Delta R.T. 0.000 min

Lab File: VN072976.D




Acq: 21 Jun 2022 12:16


Tgt Ion: 92 Resp: 5998

Ion Ratio Lower Upper

92 100


91 159.2 138.6 207.8

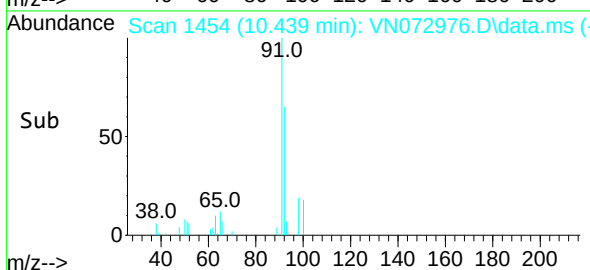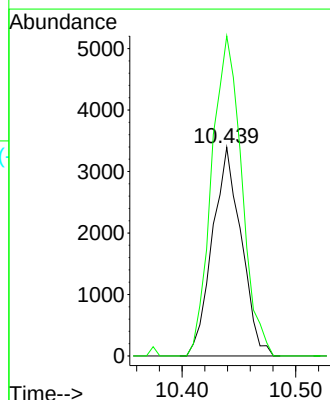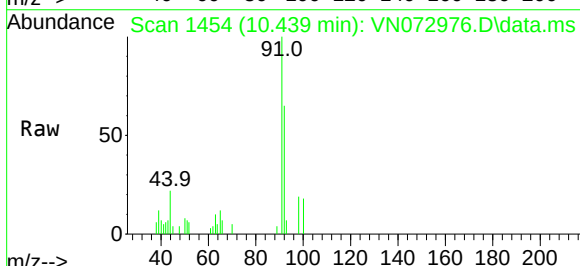






#55
1,1,2-Trichloroethane
Concen: 0.326 ug/l
RT: 10.798 min Scan# 1515
Delta R.T. -0.035 min
Lab File: VN072976.D
Acq: 21 Jun 2022 12:16

Instrument :
MSVOA_N
ClientSampleId :
MW-44DL



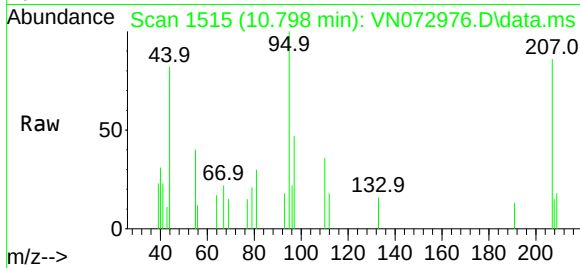



Tgt Ion:	97	Resp:	1246
Ion	Ratio	Lower	Upper
97	100		
83	0.0	66.2	99.4#
85	0.0	43.9	65.9#
99	0.0	50.6	76.0#

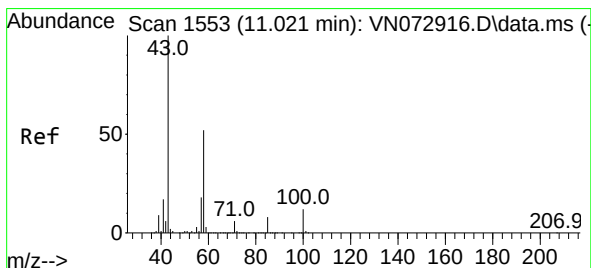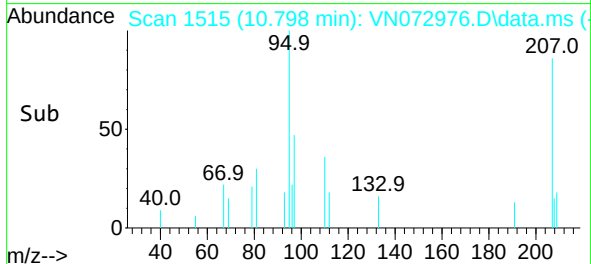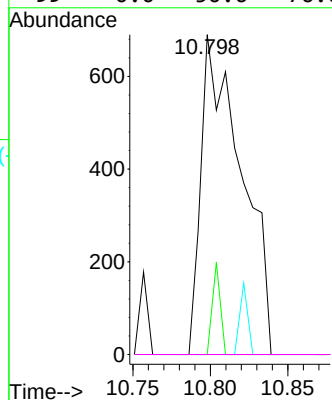

#59
2-Hexanone
Concen: 0.401 ug/l
RT: 11.069 min Scan# 1561
Delta R.T. 0.047 min
Lab File: VN072976.D
Acq: 21 Jun 2022 12:16

Tgt Ion:	43	Resp:	2090
Ion	Ratio	Lower	Upper
43	100		
58	63.9	29.7	89.1


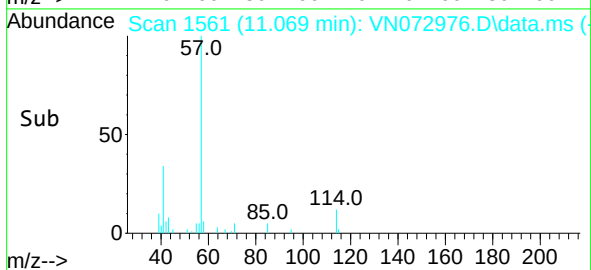
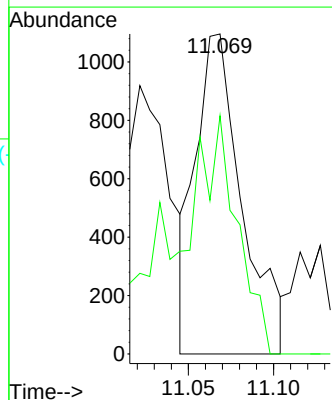
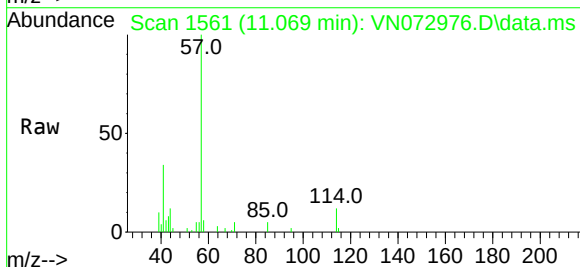




#62
4-Bromofluorobenzene
Concen: 55.413 ug/l
RT: 12.663 min Scan# 1833
Delta R.T. -0.006 min
Lab File: VN072976.D
Acq: 21 Jun 2022 12:16




Instrument :
MSVOA_N
ClientSampleId :
MW-44DL


Tgt Ion: 95 Resp: 247517
Ion Ratio Lower Upper
95 100
174 76.0 0.0 167.6
176 74.6 0.0 163.4

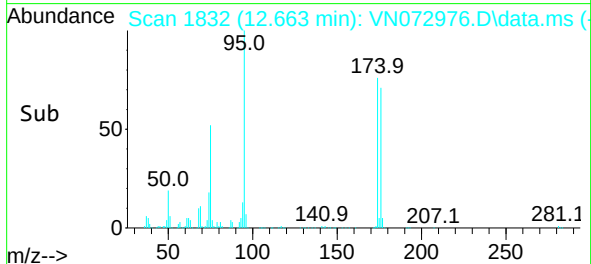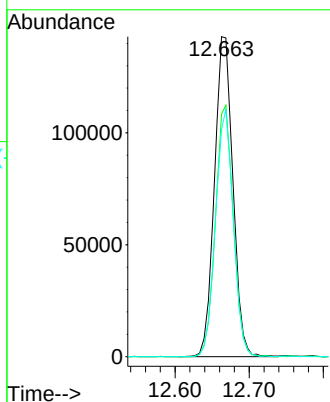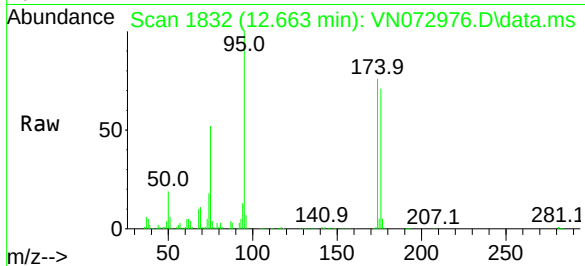

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.680 min Scan# 1665
Delta R.T. 0.000 min
Lab File: VN072976.D
Acq: 21 Jun 2022 12:16

Tgt Ion: 117 Resp: 489382
Ion Ratio Lower Upper
117 100
82 55.0 44.2 66.2
119 32.6 25.4 38.0

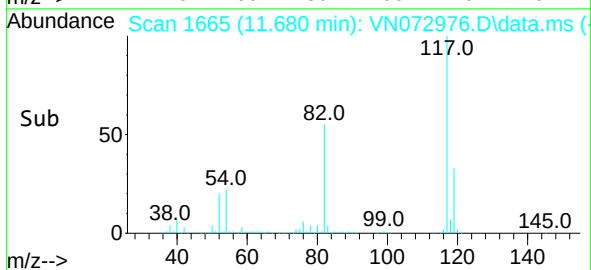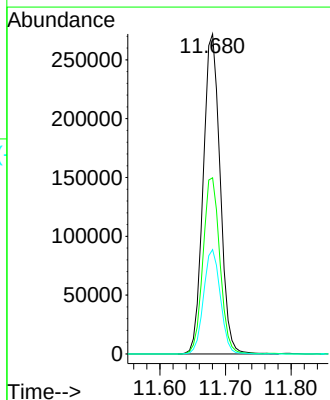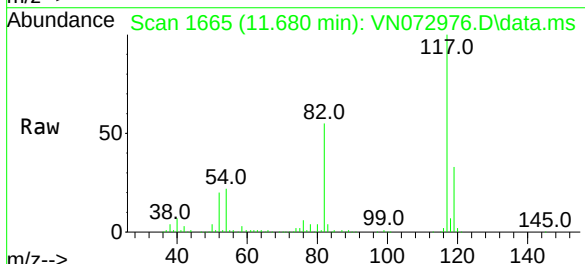

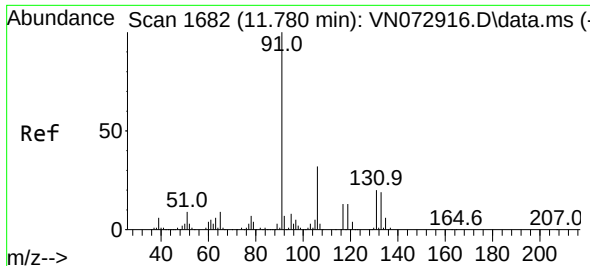

#67

Ethyl Benzene

Concen: 66.984 ug/l

RT: 11.780 min Scan# 1

Delta R.T. 0.000 min

Lab File: VN072976.D

Acq: 21 Jun 2022 12:16

Instrument :

MSVOA_N

ClientSampleId :





MW-44DL

Tgt Ion: 91 Resp: 1126962

Ion Ratio Lower Upper

91 100

106 31.2 24.9 37.3

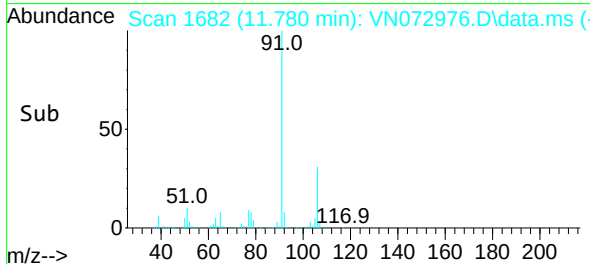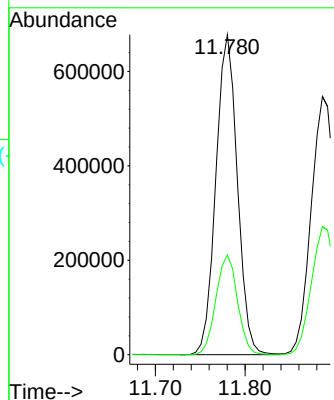

#68

m/p-Xylenes

Concen: 79.623 ug/l

RT: 11.886 min Scan# 1700

Delta R.T. 0.000 min

Lab File: VN072976.D




Acq: 21 Jun 2022 12:16


Tgt Ion:106 Resp: 525419

Ion Ratio Lower Upper

106 100

91 201.6 158.9 238.3


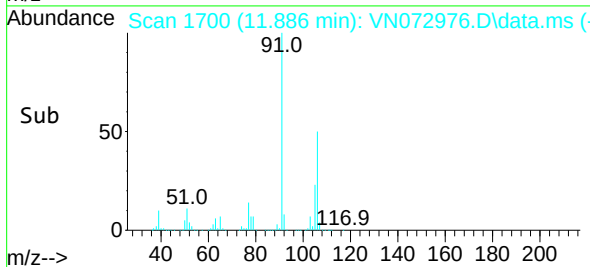
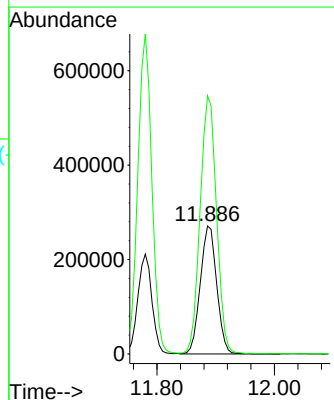
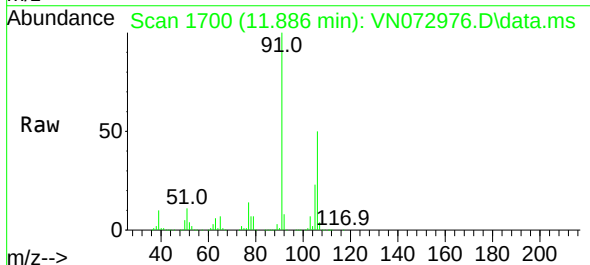




#69
o-Xylene
Concen: 4.161 ug/l
RT: 12.216 min Scan# 11
Delta R.T. 0.000 min
Lab File: VN072976.D
Acq: 21 Jun 2022 12:16




Instrument :
MSVOA_N
ClientSampleId :
MW-44DL


Tgt Ion:106 Resp: 27436
Ion Ratio Lower Upper
106 100
91 219.3 106.0 318.0

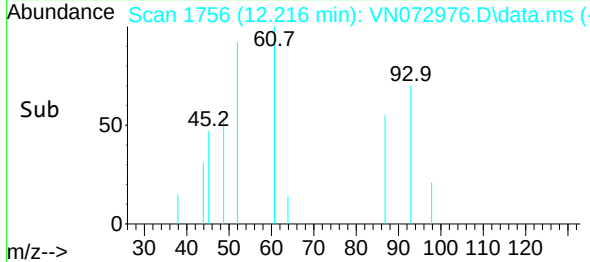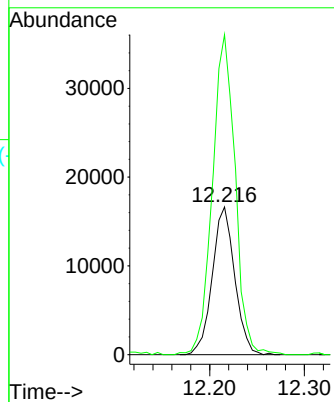

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.610 min Scan# 1993
Delta R.T. 0.000 min
Lab File: VN072976.D
Acq: 21 Jun 2022 12:16

Tgt Ion:152 Resp: 250609
Ion Ratio Lower Upper
152 100
115 63.9 28.9 86.7
150 156.8 0.0 356.2


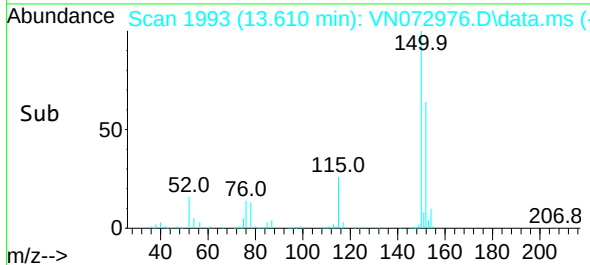
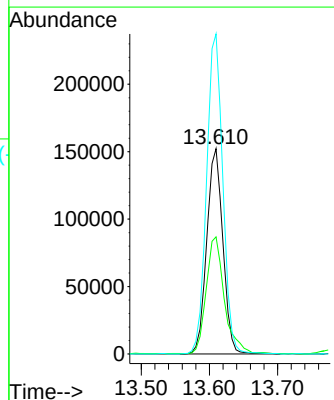
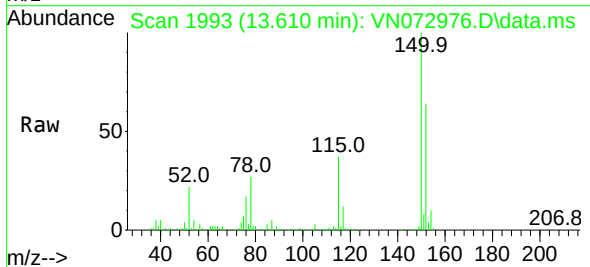




#73
Isopropylbenzene
Concen: 2.678 ug/l
RT: 12.516 min Scan# 1807
Delta R.T. 0.000 min
Lab File: VN072976.D
Acq: 21 Jun 2022 12:16




Instrument :
MSVOA_N
ClientSampleId :
MW-44DL


Tgt Ion:105 Resp: 51915
Ion Ratio Lower Upper
105 100
120 25.4 13.5 40.4

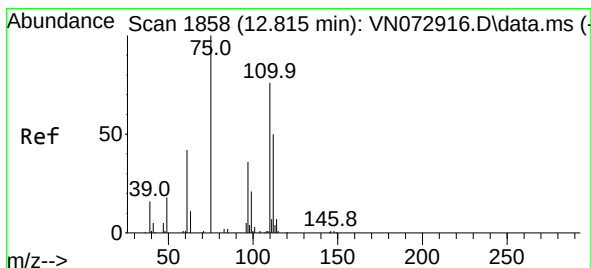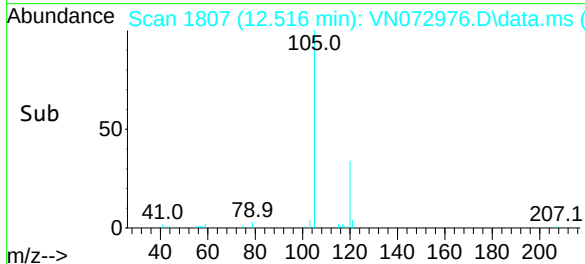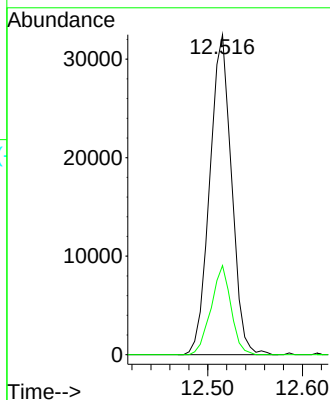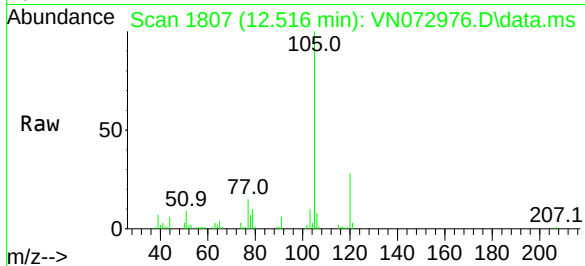

#76
1,2,3-Trichloropropane
Concen: 21.057 ug/l
RT: 12.663 min Scan# 1832
Delta R.T. -0.153 min
Lab File: VN072976.D
Acq: 21 Jun 2022 12:16

Tgt Ion: 75 Resp: 127942
Ion Ratio Lower Upper
75 100
77 1.3 98.5 295.5#


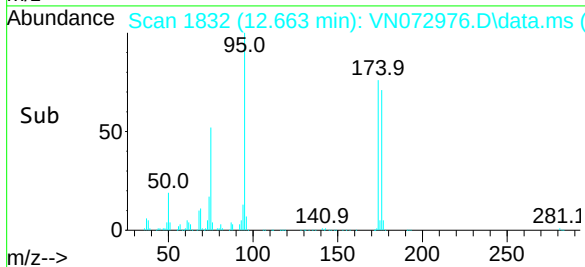
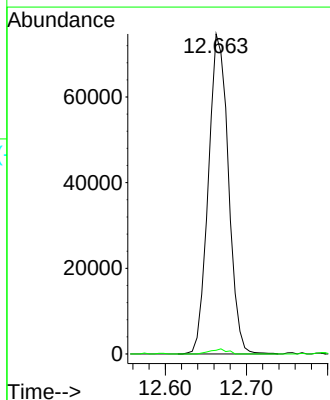
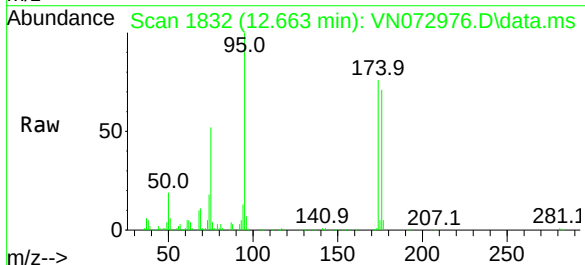


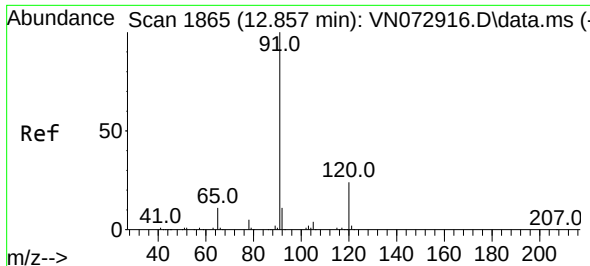

#78
n-propylbenzene
Concen: 10.516 ug/l
RT: 12.857 min Scan# 1865
Delta R.T. 0.000 min
Lab File: VN072976.D
Acq: 21 Jun 2022 12:16




Instrument :
MSVOA_N
ClientSampleId :
MW-44DL


Tgt Ion: 91 Resp: 224252
Ion Ratio Lower Upper
91 100
120 23.3 11.9 35.5

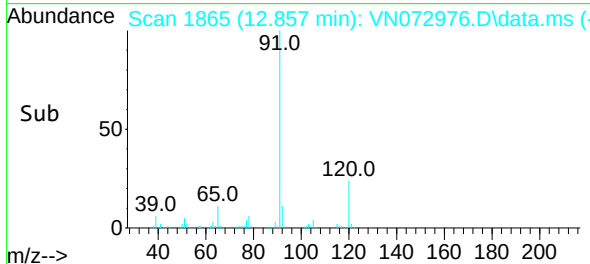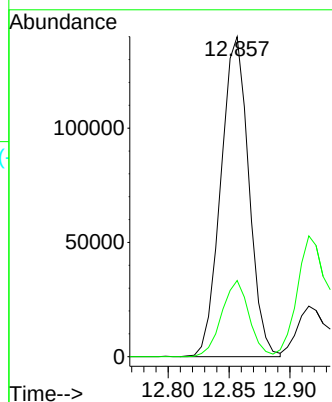

#79
2-Chlorotoluene
Concen: 1.762 ug/l
RT: 12.951 min Scan# 1881
Delta R.T. 0.006 min
Lab File: VN072976.D
Acq: 21 Jun 2022 12:16

Tgt Ion: 91 Resp: 24331
Ion Ratio Lower Upper
91 100
126 0.3 17.3 51.9#



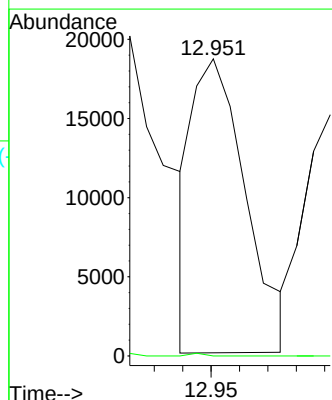
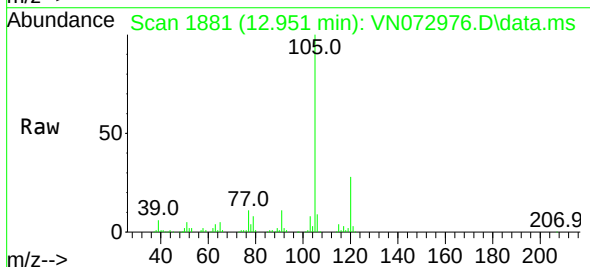




#80
1,3,5-Trimethylbenzene
Concen: 14.144 ug/l
RT: 12.992 min Scan# 1888
Delta R.T. -0.006 min
Lab File: VN072976.D
Acq: 21 Jun 2022 12:16




Instrument :
MSVOA_N
ClientSampleId :
MW-44DL


Tgt Ion:105 Resp: 225252
Ion Ratio Lower Upper
105 100
120 52.1 24.9 74.7

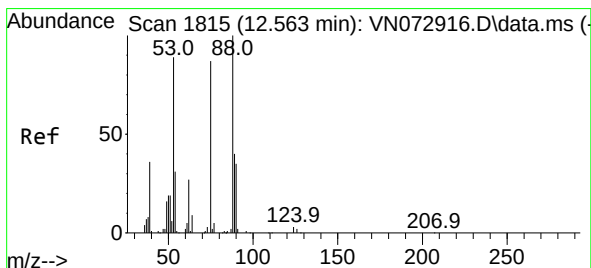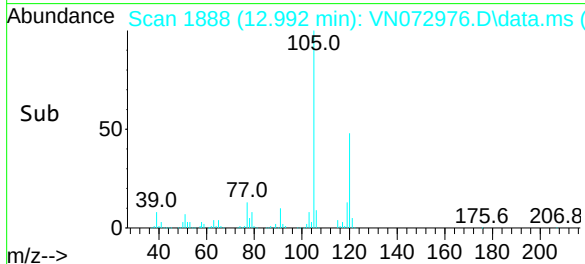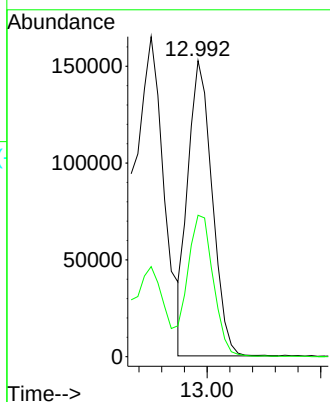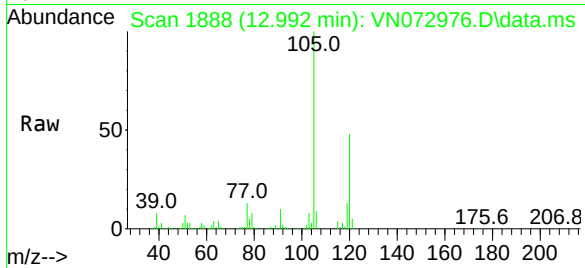

#81
trans-1,4-Dichloro-2-butene
Concen: 56.867 ug/l
RT: 12.663 min Scan# 1832
Delta R.T. 0.100 min
Lab File: VN072976.D
Acq: 21 Jun 2022 12:16

Tgt Ion: 75 Resp: 127942
Ion Ratio Lower Upper
75 100
53 0.0 78.0 117.0#
89 0.0 37.2 55.8#

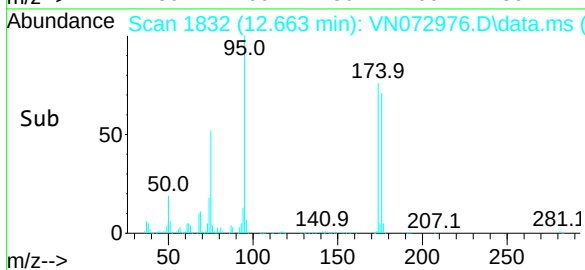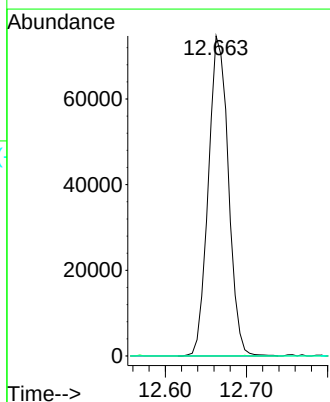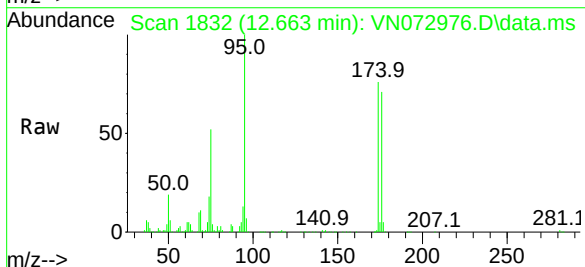



#82

4-Chlorotoluene

Concen: 1.771 ug/l

RT: 12.992 min Scan# 1888

Delta R.T. -0.047 min

Lab File: VN072976.D

Acq: 21 Jun 2022 12:16

Instrument :

MSVOA_N

ClientSampleId :





MW-44DL

Tgt Ion: 91 Resp: 23134

Ion Ratio Lower Upper

91 100

126 0.0 17.2 51.6#

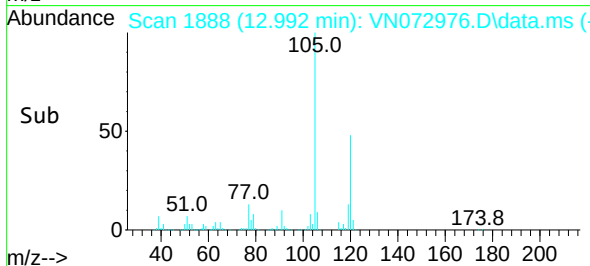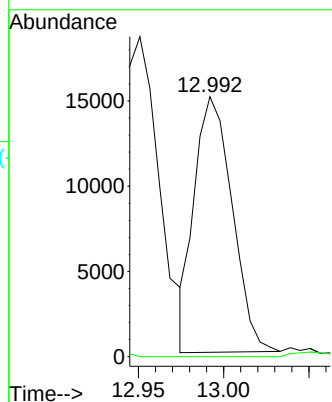

#83

tert-Butylbenzene

Concen: 11.260 ug/l

RT: 13.304 min Scan# 1941

Delta R.T. 0.047 min

Lab File: VN072976.D

Acq: 21 Jun 2022 12:16




Tgt Ion: 119 Resp: 164231


Ion Ratio Lower Upper

119 100

91 90.0 31.6 94.8

134 0.0 13.7 41.1#

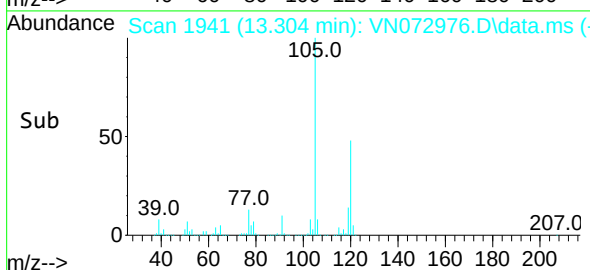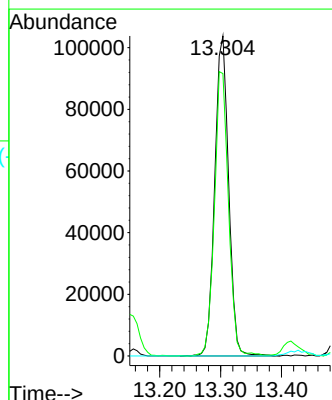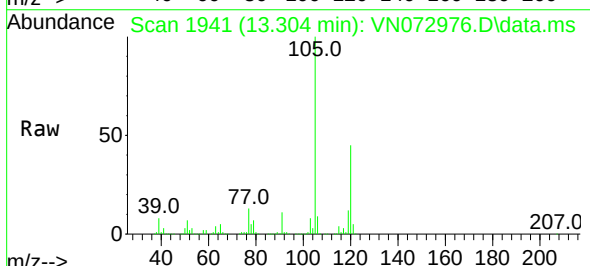

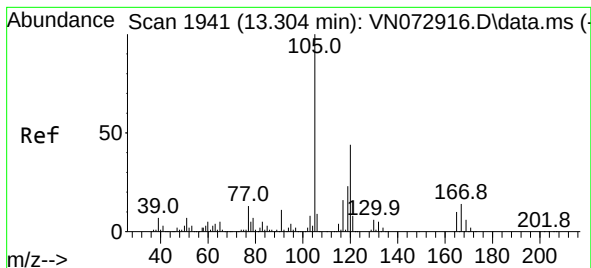

#84

1,2,4-Trimethylbenzene

Concen: 86.458 ug/l

RT: 13.304 min Scan# 1941

Delta R.T. 0.000 min

Lab File: VN072976.D

Acq: 21 Jun 2022 12:16

Instrument :

MSVOA_N

ClientSampleId :





MW-44DL

Tgt Ion:105 Resp: 1371403

Ion Ratio Lower Upper

105 100

120 45.1 23.3 69.8

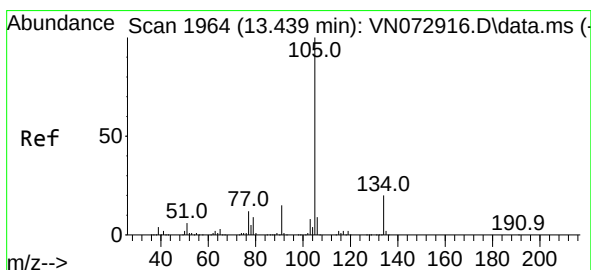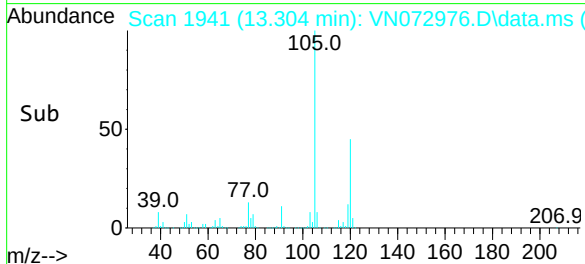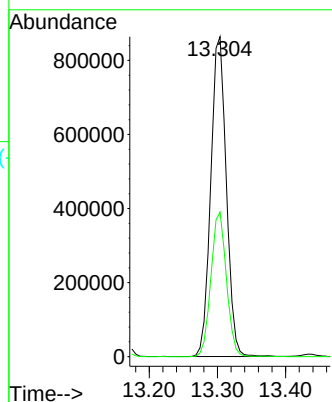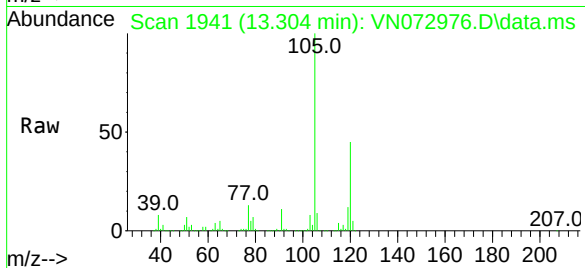

#85

sec-Butylbenzene

Concen: 70.485 ug/l

RT: 13.304 min Scan# 1941

Delta R.T. -0.135 min

Lab File: VN072976.D




Acq: 21 Jun 2022 12:16


Tgt Ion:105 Resp: 1371403

Ion Ratio Lower Upper

105 100

134 0.0 10.4 31.1#


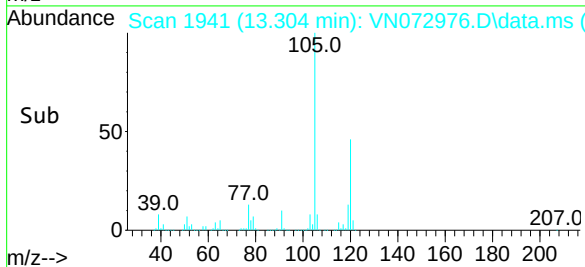
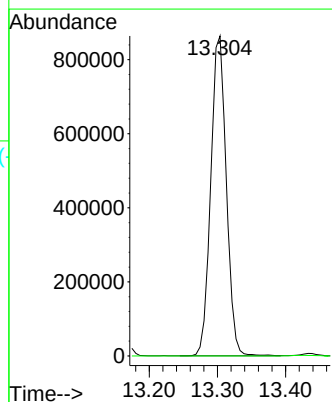
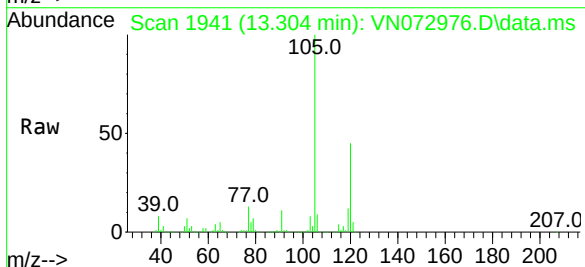


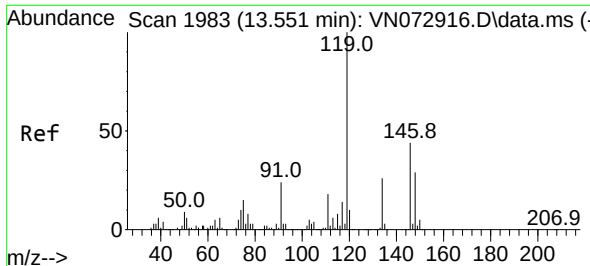

#86
p-Isopropyltoluene
Concen: 0.602 ug/l
RT: 13.492 min Scan# 1983
Delta R.T. -0.059 min
Lab File: VN072976.D
Acq: 21 Jun 2022 12:16




Instrument :
MSVOA_N
ClientSampleId :
MW-44DL


Tgt Ion:119 Resp: 9485
Ion Ratio Lower Upper
119 100
134 30.7 13.3 39.8
91 0.0 11.3 33.9#

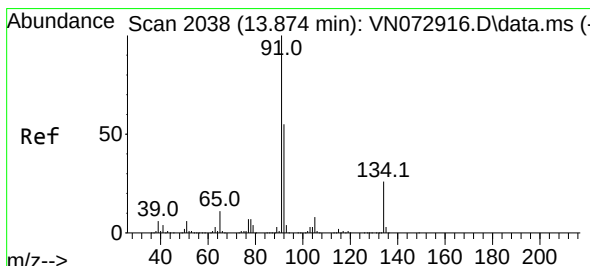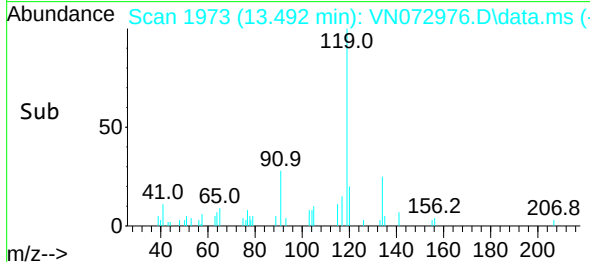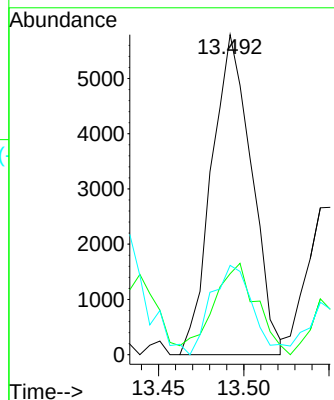

#89
n-Butylbenzene
Concen: 6.463 ug/l
RT: 13.810 min Scan# 2027
Delta R.T. -0.065 min
Lab File: VN072976.D
Acq: 21 Jun 2022 12:16

Tgt Ion: 91 Resp: 83131
Ion Ratio Lower Upper
91 100
92 11.0 26.9 80.7#
134 0.0 13.6 40.8#


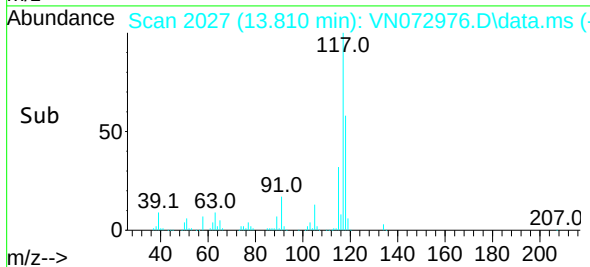
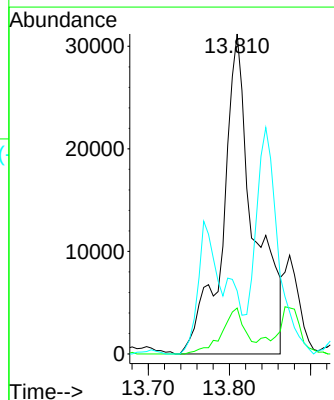
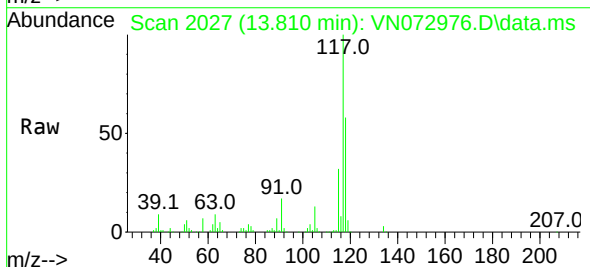




#90
Hexachloroethane
Concen: 4.878 ug/l
RT: 14.151 min Scan# 2085
Delta R.T. 0.006 min
Lab File: VN072976.D
Acq: 21 Jun 2022 12:16

Instrument :
MSVOA_N
ClientSampleId :
MW-44DL

Tgt Ion:117 Resp: 14485
Ion Ratio Lower Upper
117 100
201 0.0 40.6 122.0#

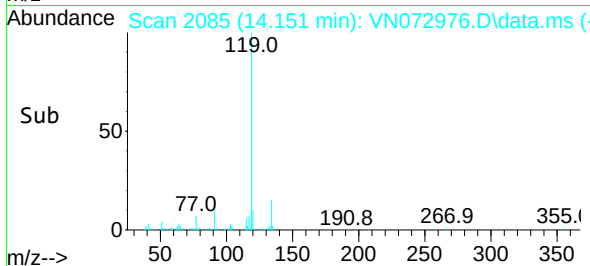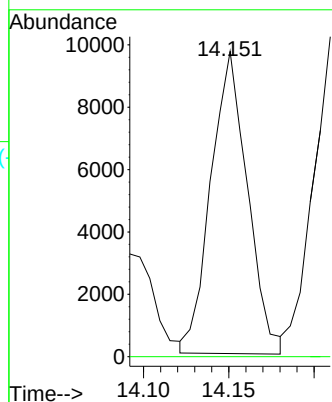

#95
Naphthalene
Concen: 25.932 ug/l
RT: 15.427 min Scan# 2302
Delta R.T. 0.000 min
Lab File: VN072976.D
Acq: 21 Jun 2022 12:16

Tgt Ion:128 Resp: 502048
Ion Ratio Lower Upper
128 100
127 13.0 10.3 15.5
129 10.7 8.6 13.0

