

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN062122\
 Data File : VN072971.D
 Acq On : 21 Jun 2022 09:55
 Operator : JC\MD
 Sample : VN0621MBL01
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN0621MBL01

Quant Time: Jun 22 06:58:38 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N061722W.M
 Quant Title : SW846 8260
 QLast Update : Sat Jun 18 06:22:45 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.016	168	337773	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.898	114	538073	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.674	117	491982	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.604	152	240664	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.369	65	195439	42.797	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	85.600%
35) Dibromofluoromethane	7.951	113	172106	51.749	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	103.500%
50) Toluene-d8	10.375	98	550808	44.509	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	89.020%
62) 4-Bromofluorobenzene	12.663	95	243843	54.796	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	109.600%


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN062122\
Data File : VN072971.D
Acq On : 21 Jun 2022 09:55
Operator : JC\MD
Sample : VN0621MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN0621MBL01

Quant Time: Jun 22 06:58:38 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N061722W.M
Quant Title : SW846 8260
QLast Update : Sat Jun 18 06:22:45 2022
Response via : Initial Calibration




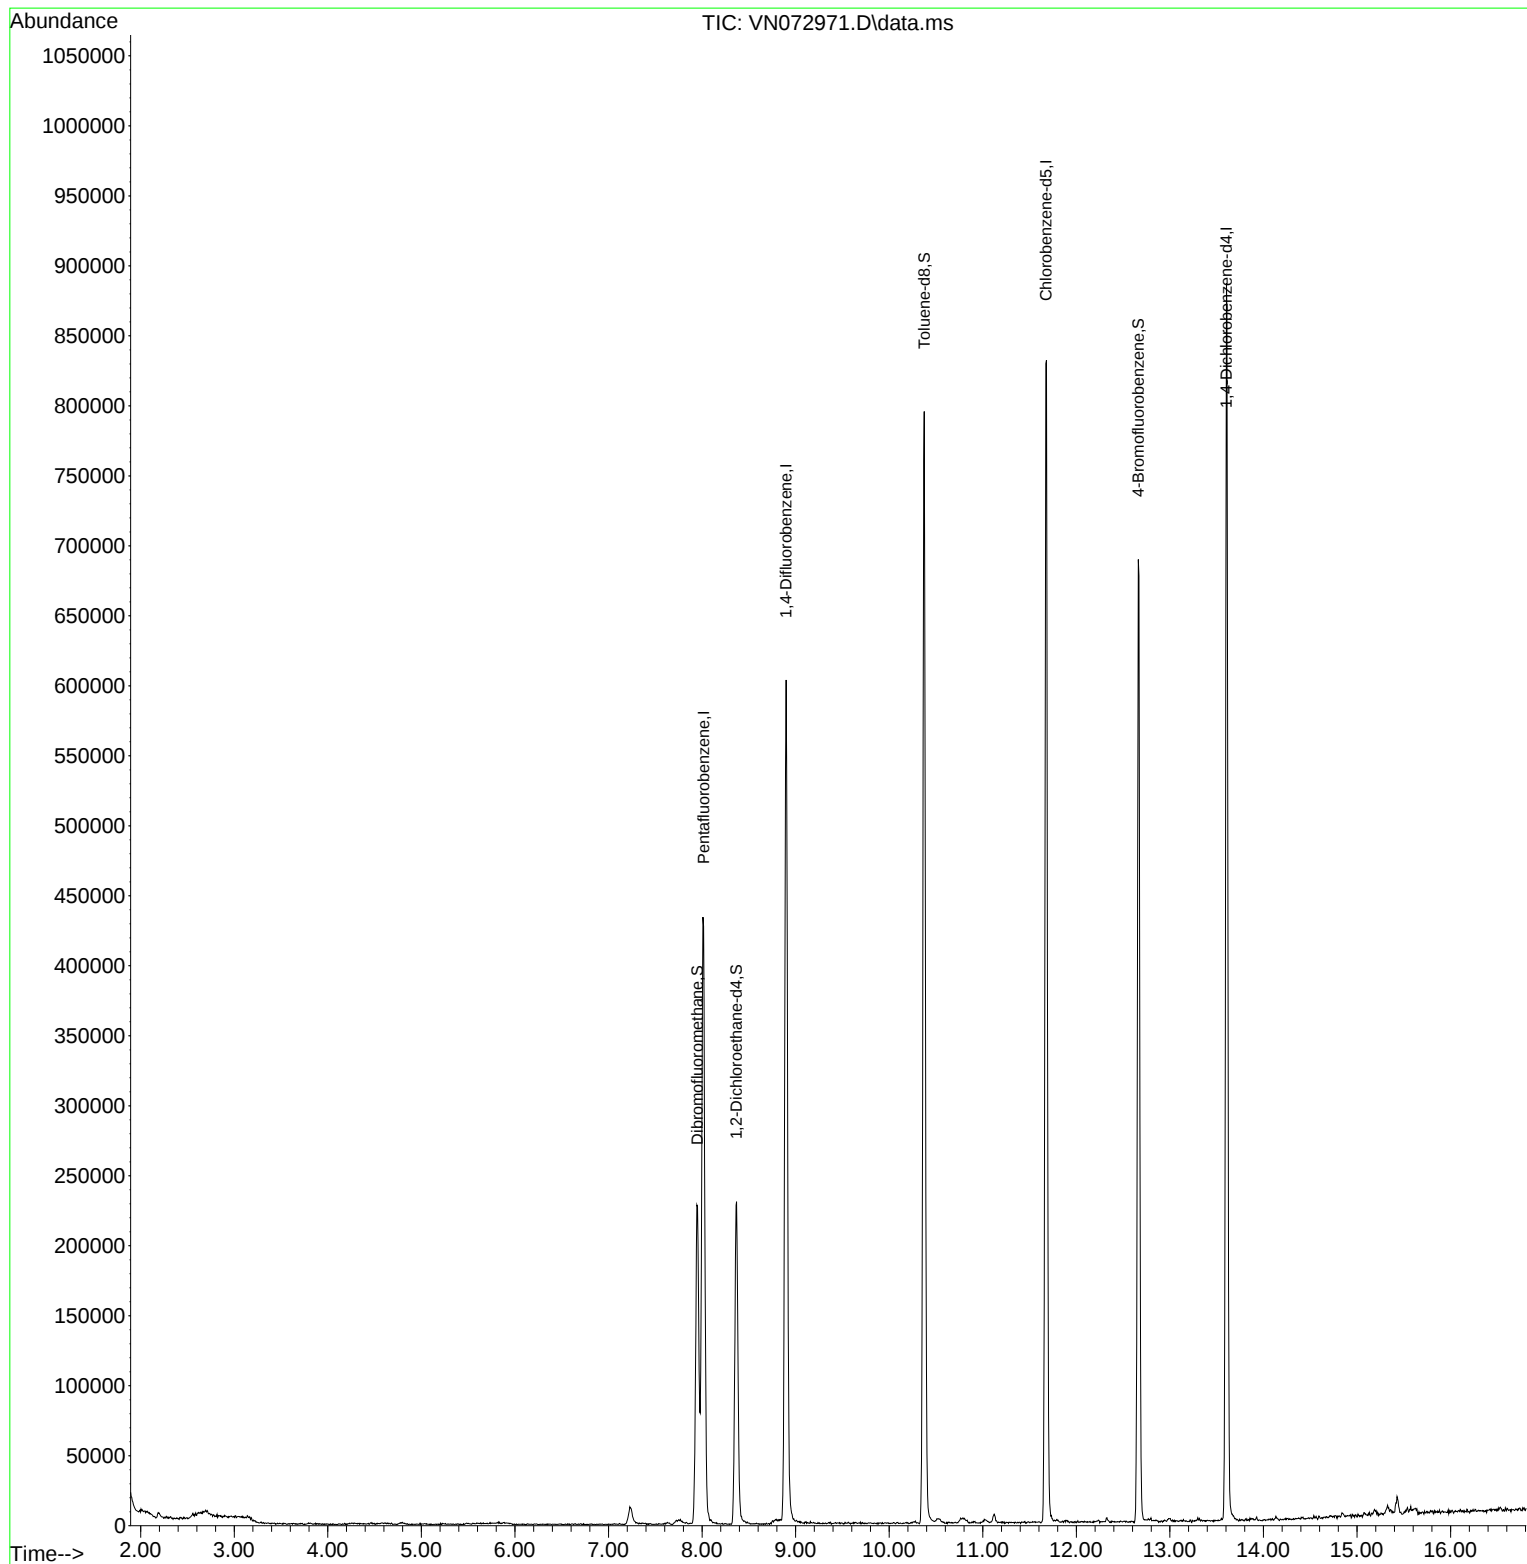




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.016 min Scan# 1042
Delta R.T. -0.000 min
Lab File: VN072971.D
Acq: 21 Jun 2022 09:55




Instrument :
MSVOA_N
ClientSampleId :
VN0621MBL01

Tgt Ion:168 Resp: 337773
Ion Ratio Lower Upper
168 100
99 57.1 42.3 63.5

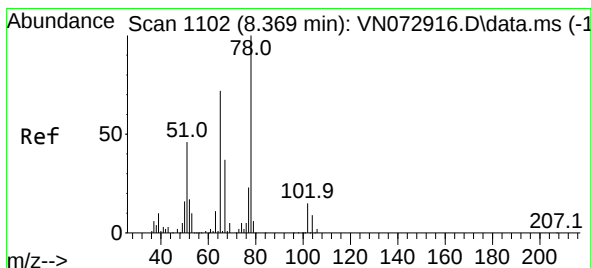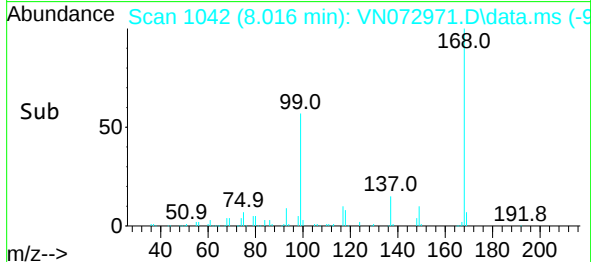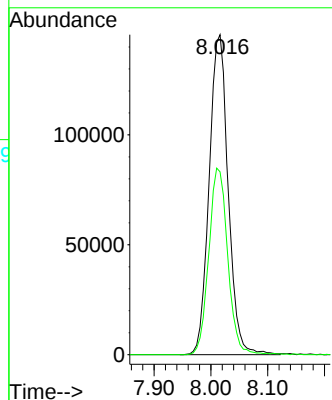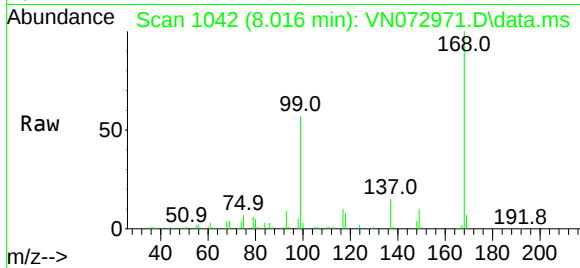

#33
1,2-Dichloroethane-d4
Concen: 42.797 ug/l
RT: 8.369 min Scan# 1102
Delta R.T. 0.000 min
Lab File: VN072971.D
Acq: 21 Jun 2022 09:55

Tgt Ion: 65 Resp: 195439
Ion Ratio Lower Upper
65 100
67 52.4 0.0 104.8

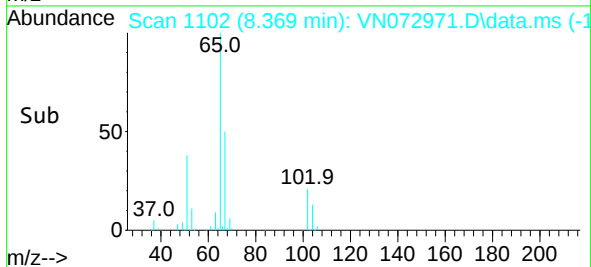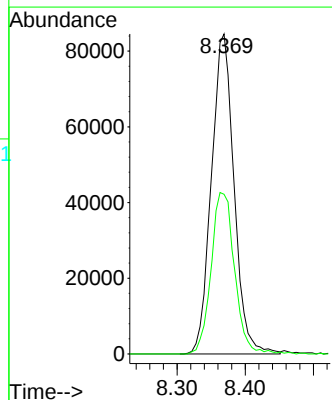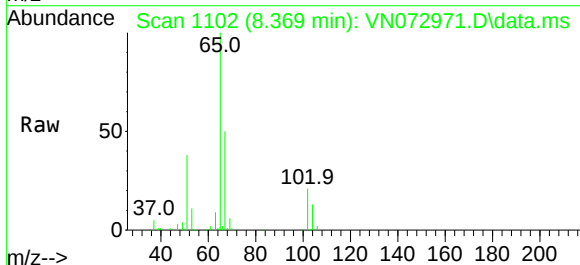



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.898 min Scan# 1192

Delta R.T. 0.000 min

Lab File: VN072971.D

Acq: 21 Jun 2022 09:55

Instrument :

MSVOA_N

ClientSampleId :

VN0621MBL01





Tgt Ion:114 Resp: 538073

Ion Ratio Lower Upper

114 100

63 21.5 0.0 40.0

88 16.4 0.0 32.6

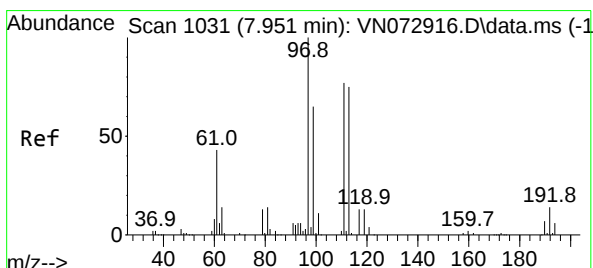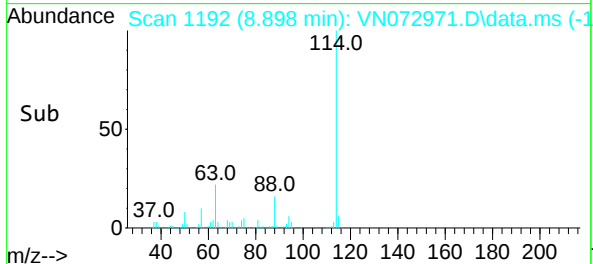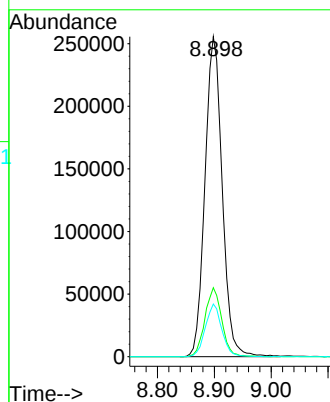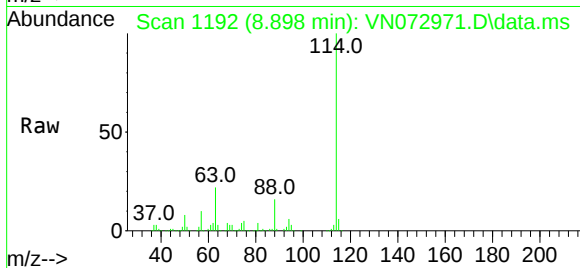

#35

Dibromofluoromethane

Concen: 51.749 ug/l

RT: 7.951 min Scan# 1031

Delta R.T. 0.000 min

Lab File: VN072971.D

Acq: 21 Jun 2022 09:55




Tgt Ion:113 Resp: 172106


Ion Ratio Lower Upper

113 100

111 103.4 81.4 122.0

192 18.8 17.0 25.6


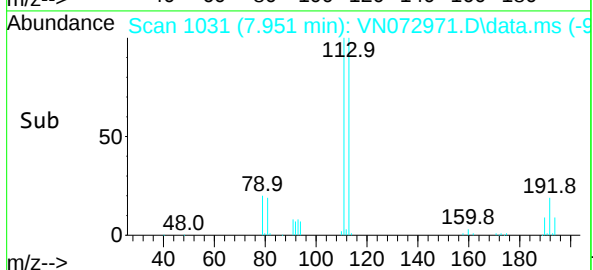
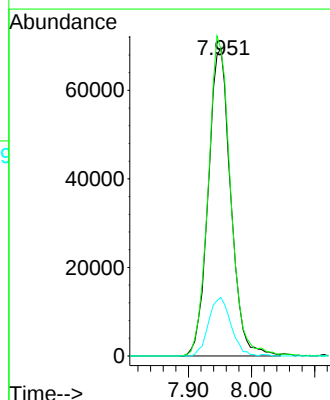
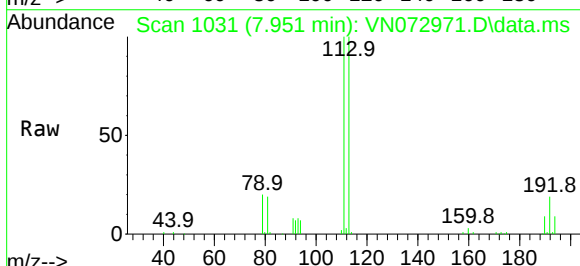


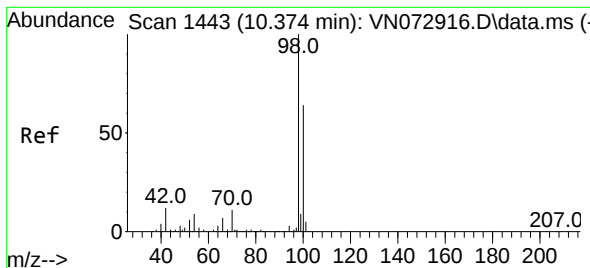

#50
Toluene-d8
Concen: 44.509 ug/l
RT: 10.375 min Scan# 1443
Delta R.T. 0.000 min
Lab File: VN072971.D
Acq: 21 Jun 2022 09:55




Instrument :
MSVOA_N
ClientSampleId :
VN0621MBL01


Tgt Ion: 98 Resp: 550808
Ion Ratio Lower Upper
98 100
100 66.0 52.6 78.8

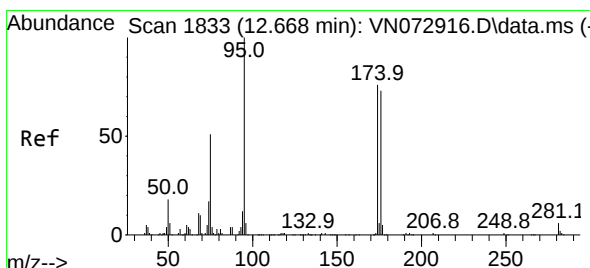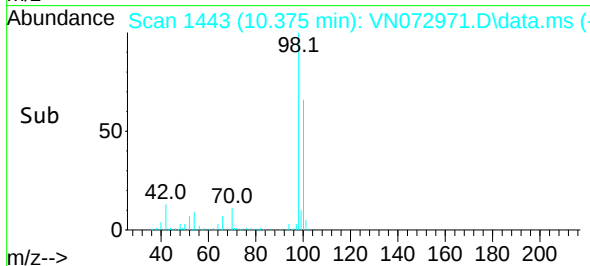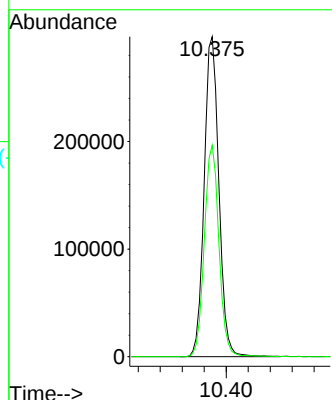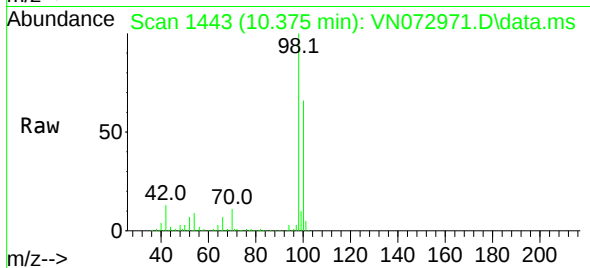

#62
4-Bromofluorobenzene
Concen: 54.796 ug/l
RT: 12.663 min Scan# 1832
Delta R.T. -0.006 min
Lab File: VN072971.D
Acq: 21 Jun 2022 09:55

Tgt Ion: 95 Resp: 243843
Ion Ratio Lower Upper
95 100
174 76.5 0.0 167.6
176 74.1 0.0 163.4


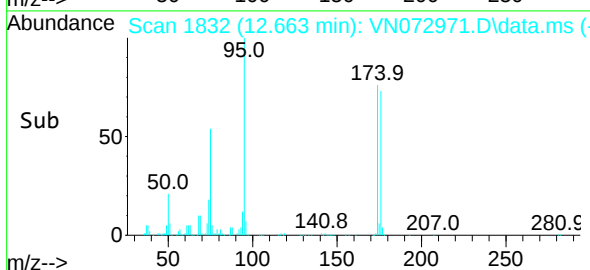
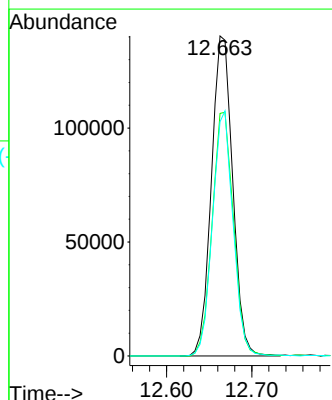
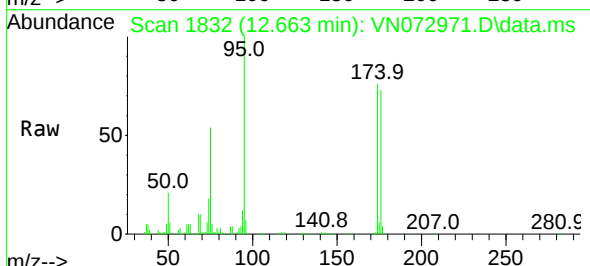


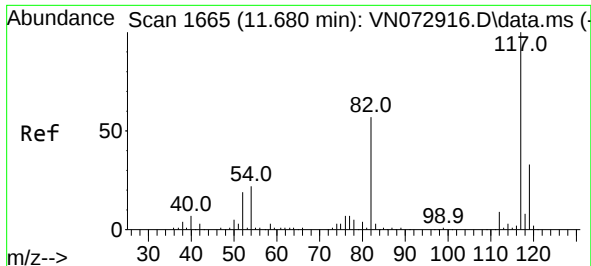

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.674 min Scan# 11
Delta R.T. -0.006 min
Lab File: VN072971.D
Acq: 21 Jun 2022 09:55

Instrument :
MSVOA_N
ClientSampleId :
VN0621MBL01

Tgt Ion:117 Resp: 491982
Ion Ratio Lower Upper
117 100
82 52.9 44.2 66.2
119 31.4 25.4 38.0

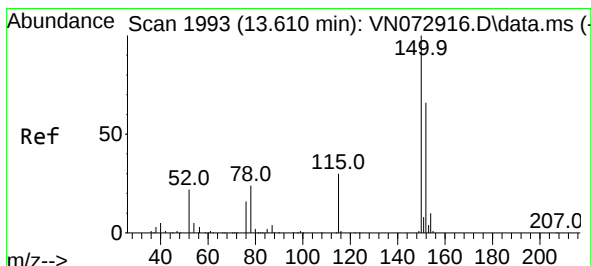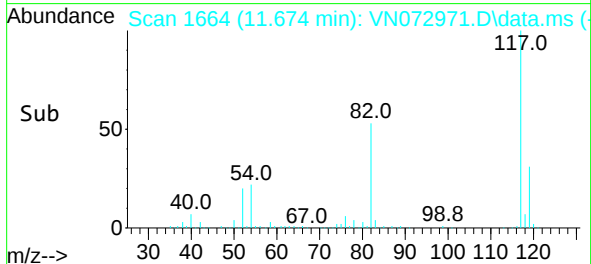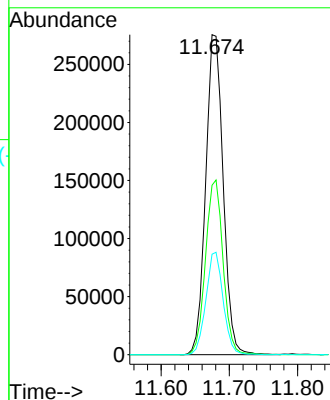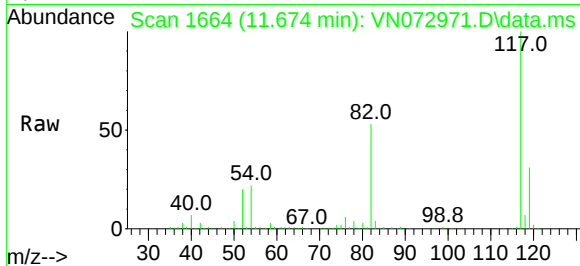

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.604 min Scan# 1992
Delta R.T. -0.006 min
Lab File: VN072971.D
Acq: 21 Jun 2022 09:55

Tgt Ion:152 Resp: 240664
Ion Ratio Lower Upper
152 100
115 60.3 28.9 86.7
150 160.9 0.0 356.2

