

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN062122\
 Data File : VN072980.D
 Acq On : 21 Jun 2022 13:53
 Operator : JC\MD
 Sample : N3379-06
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 TB-2022-06-16

Quant Time: Jun 22 07:00:20 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N061722W.M
 Quant Title : SW846 8260
 QLast Update : Sat Jun 18 06:22:45 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.016	168	331932	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.904	114	526236	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.680	117	475752	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.610	152	237723	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.375	65	193271	43.067	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	86.140%
35) Dibromofluoromethane	7.951	113	166850	51.297	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	102.600%
50) Toluene-d8	10.375	98	540407	44.650	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	89.300%
62) 4-Bromofluorobenzene	12.669	95	238335	54.763	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	109.520%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN062122\
Data File : VN072980.D
Acq On : 21 Jun 2022 13:53
Operator : JC\MD
Sample : N3379-06
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
TB-2022-06-16

Quant Time: Jun 22 07:00:20 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N061722W.M
Quant Title : SW846 8260
QLast Update : Sat Jun 18 06:22:45 2022
Response via : Initial Calibration




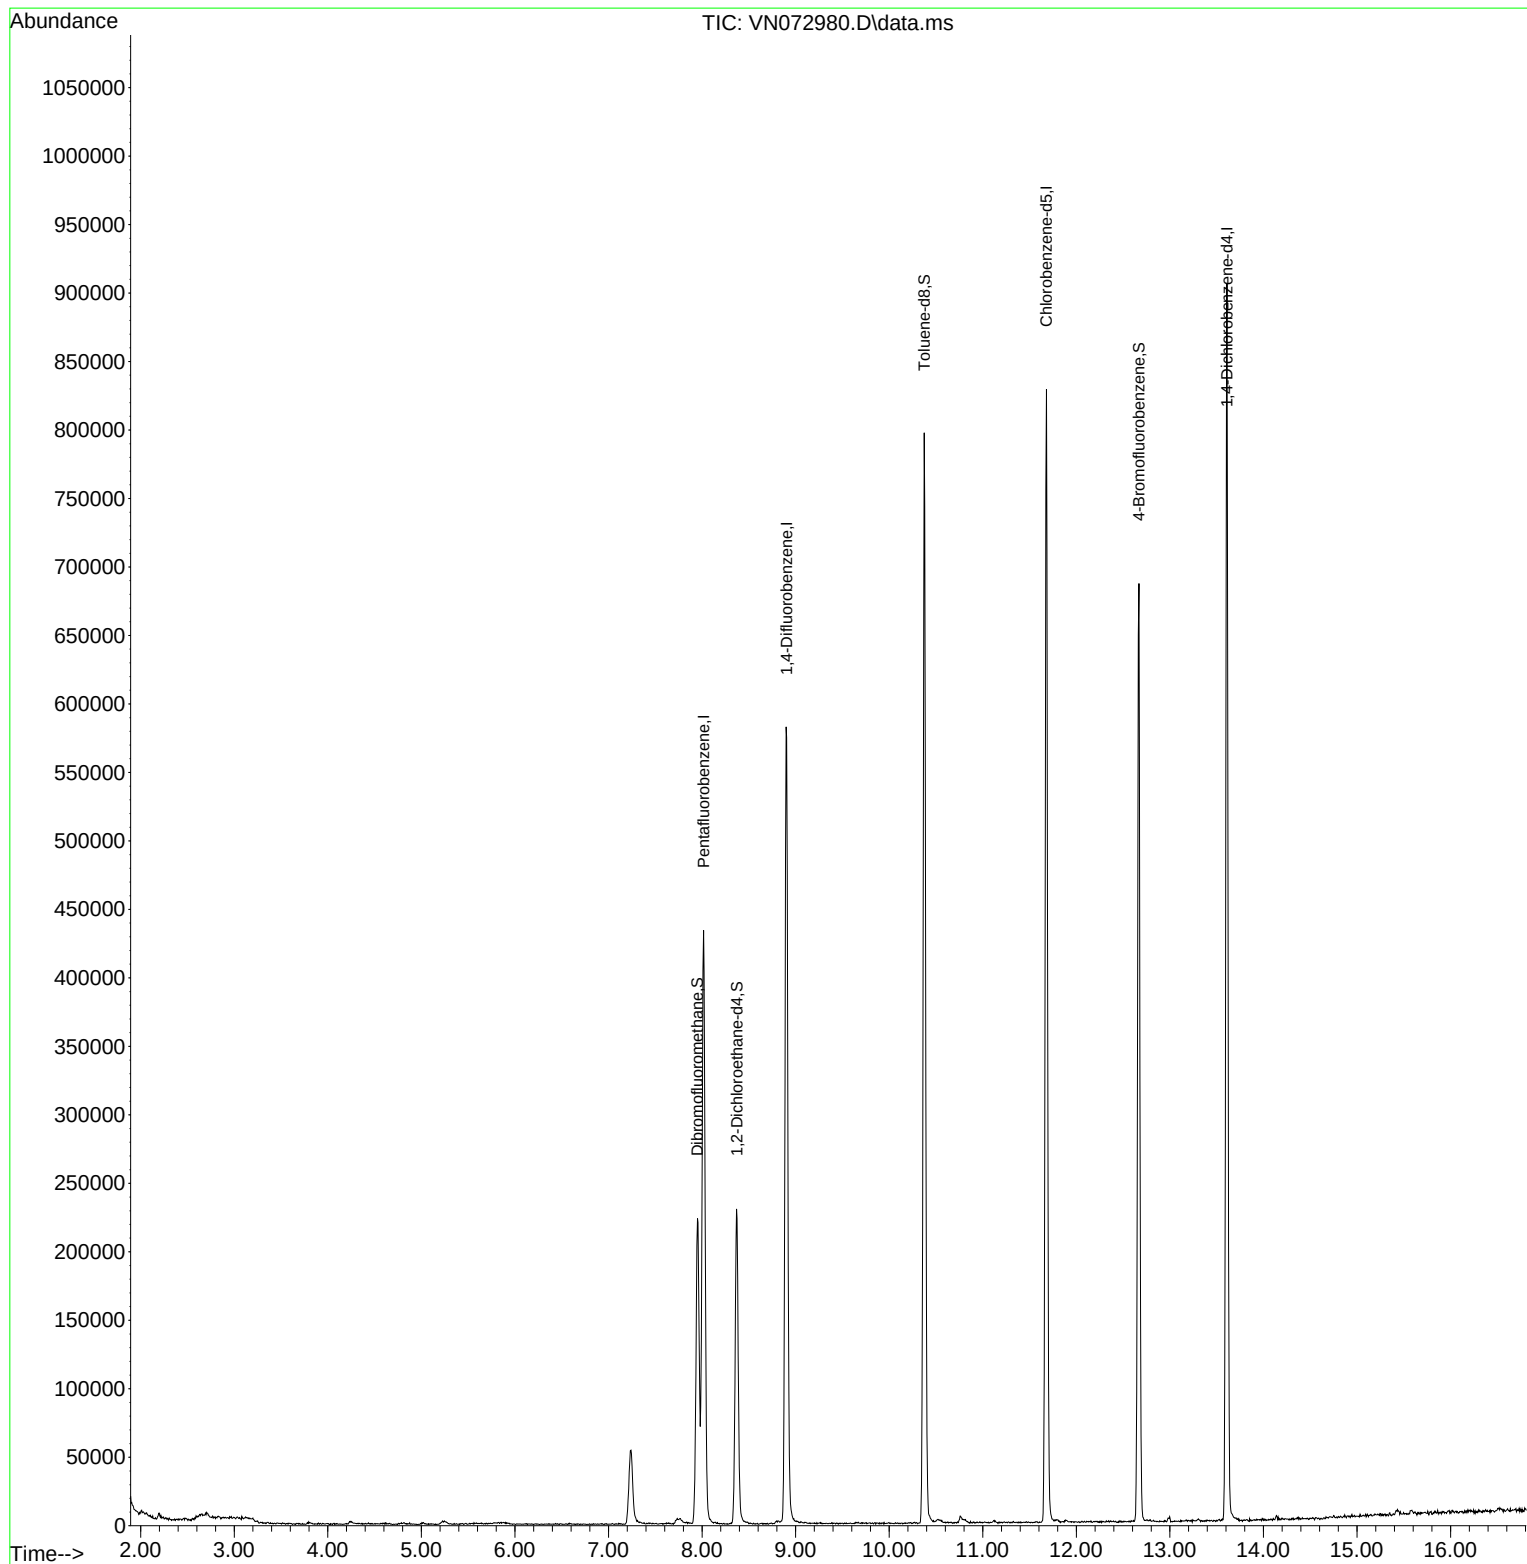


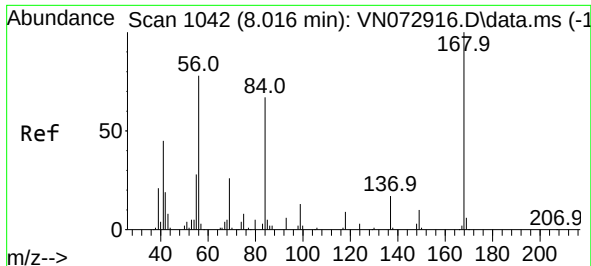

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.016 min Scan# 1103
Delta R.T. -0.000 min
Lab File: VN072980.D
Acq: 21 Jun 2022 13:53




Instrument :
MSVOA_N
ClientSampleId :
TB-2022-06-16


Tgt Ion:168 Resp: 331932
Ion Ratio Lower Upper
168 100
99 56.9 42.3 63.5

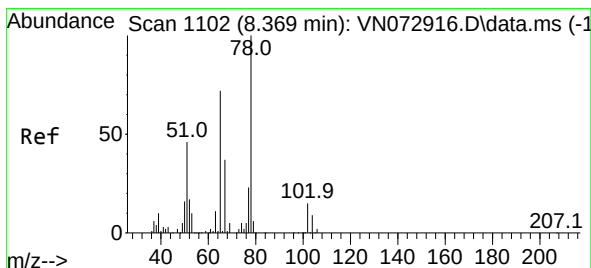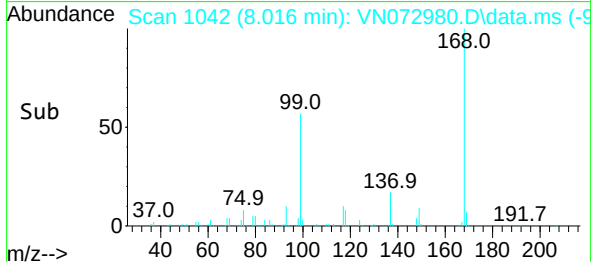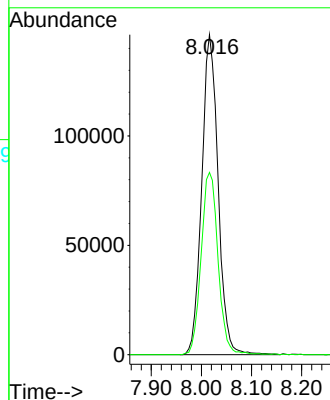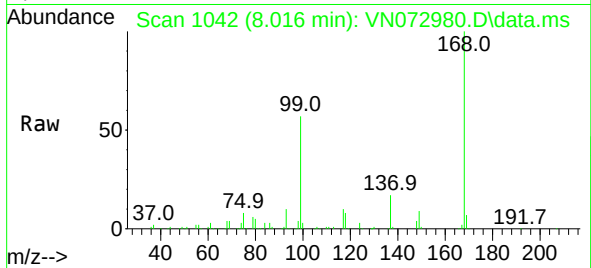

#33
1,2-Dichloroethane-d4
Concen: 43.067 ug/l
RT: 8.375 min Scan# 1103
Delta R.T. 0.006 min
Lab File: VN072980.D
Acq: 21 Jun 2022 13:53

Tgt Ion: 65 Resp: 193271
Ion Ratio Lower Upper
65 100
67 52.4 0.0 104.8

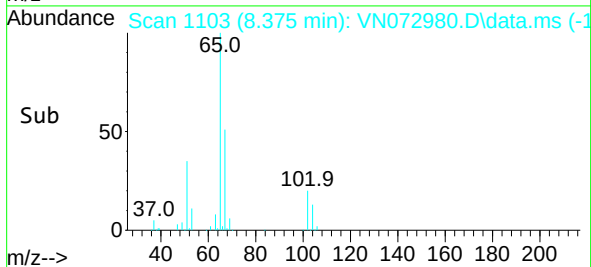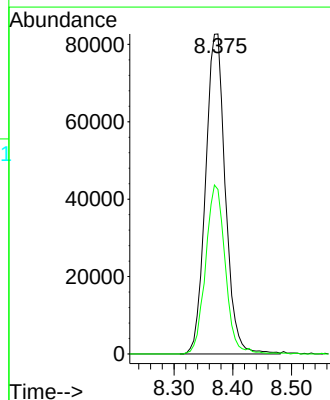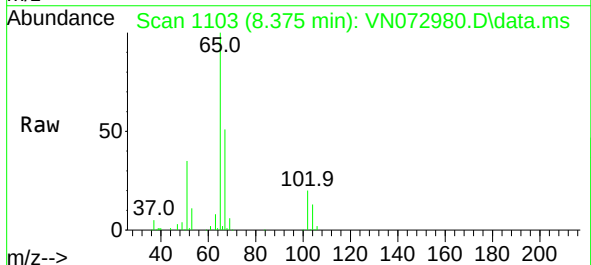

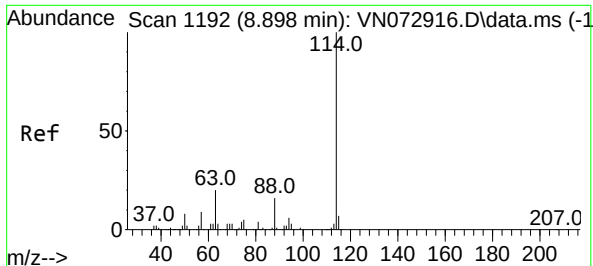

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.904 min Scan# 1192

Delta R.T. 0.006 min

Lab File: VN072980.D

Acq: 21 Jun 2022 13:53

Instrument :

MSVOA_N

ClientSampleId :

TB-2022-06-16





Tgt Ion:114 Resp: 526236

Ion Ratio Lower Upper

114 100

63 20.2 0.0 40.0

88 15.5 0.0 32.6

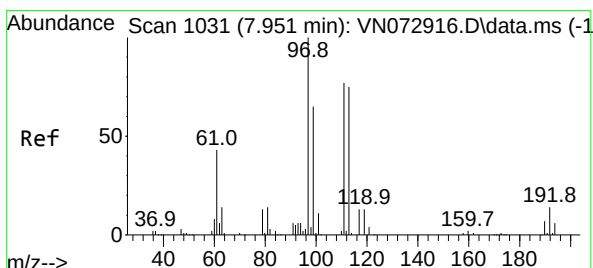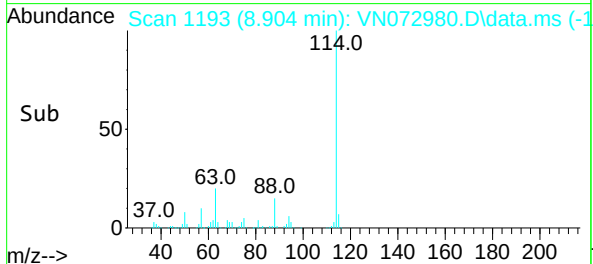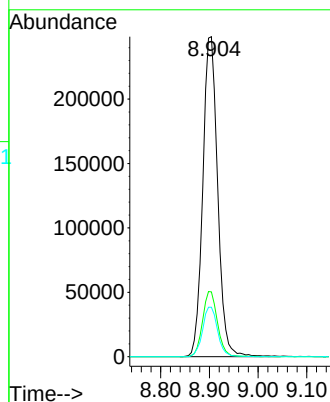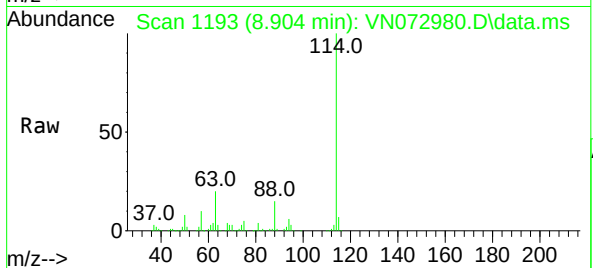

#35

Dibromofluoromethane

Concen: 51.297 ug/l

RT: 7.951 min Scan# 1031

Delta R.T. 0.000 min

Lab File: VN072980.D

Acq: 21 Jun 2022 13:53




Tgt Ion:113 Resp: 166850


Ion Ratio Lower Upper

113 100

111 104.5 81.4 122.0

192 19.0 17.0 25.6


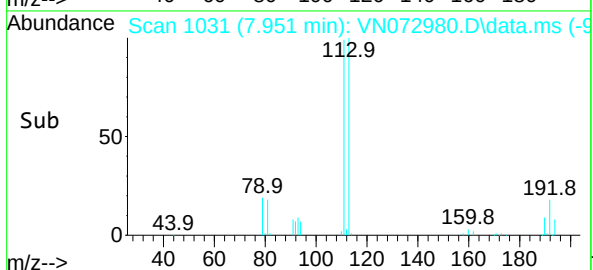
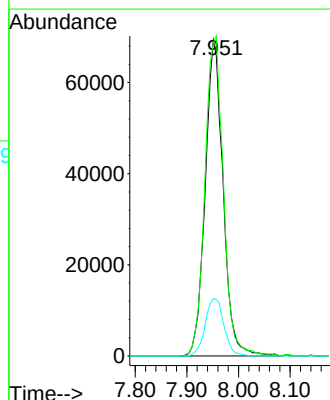
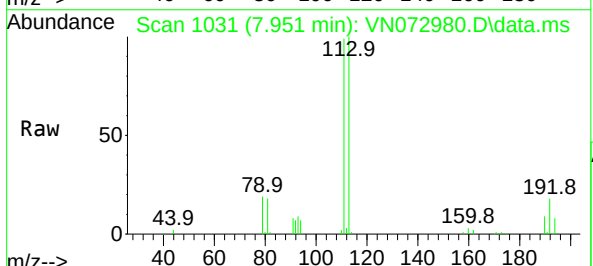


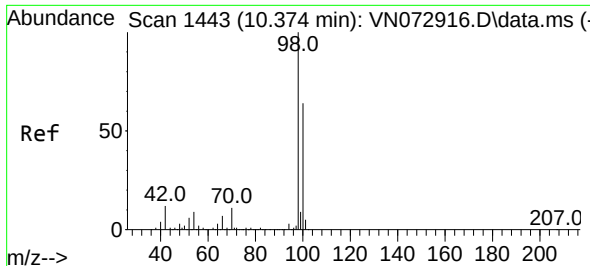

#50
Toluene-d8
Concen: 44.650 ug/l
RT: 10.375 min Scan# 1443
Delta R.T. 0.000 min
Lab File: VN072980.D
Acq: 21 Jun 2022 13:53




Instrument :
MSVOA_N
ClientSampleId :
TB-2022-06-16


Tgt Ion: 98 Resp: 540407
Ion Ratio Lower Upper
98 100
100 65.6 52.6 78.8

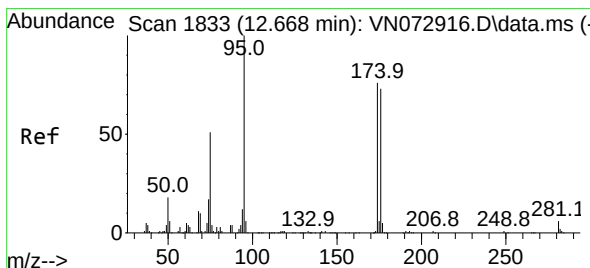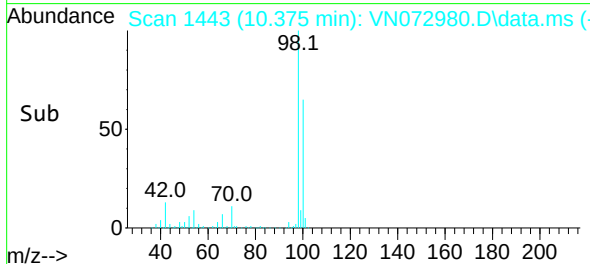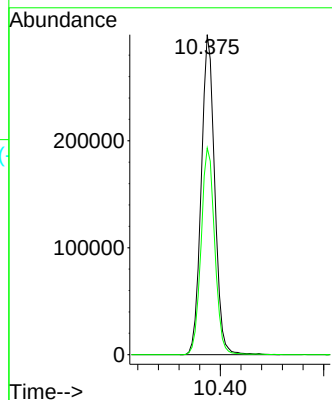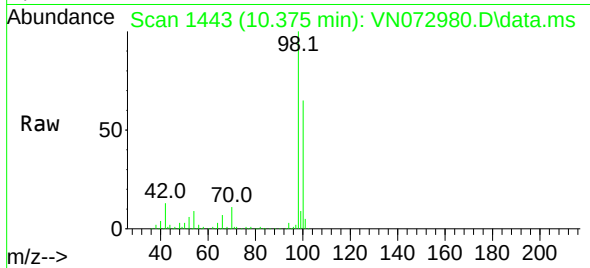

#62
4-Bromofluorobenzene
Concen: 54.763 ug/l
RT: 12.669 min Scan# 1833
Delta R.T. 0.000 min
Lab File: VN072980.D
Acq: 21 Jun 2022 13:53

Tgt Ion: 95 Resp: 238335
Ion Ratio Lower Upper
95 100
174 76.8 0.0 167.6
176 73.9 0.0 163.4

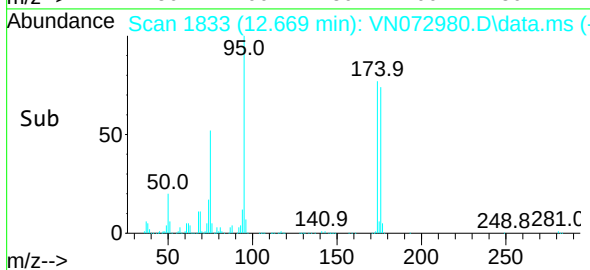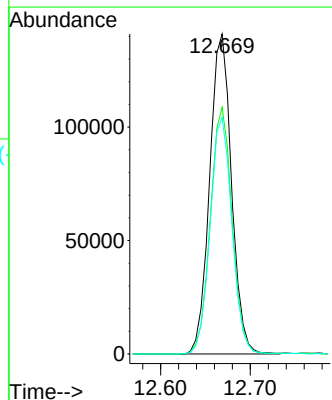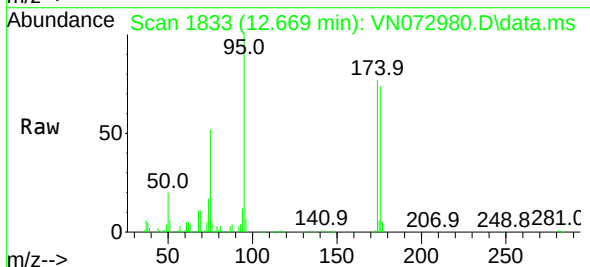

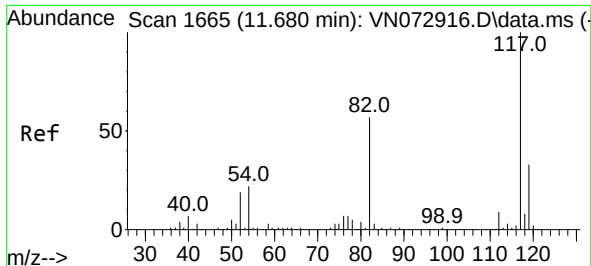

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.680 min Scan# 1

Delta R.T. 0.000 min

Lab File: VN072980.D

Acq: 21 Jun 2022 13:53

Instrument :

MSVOA_N

ClientSampleId :

TB-2022-06-16





Tgt Ion:117 Resp: 475752

Ion Ratio Lower Upper

117 100

82 56.3 44.2 66.2

119 32.0 25.4 38.0

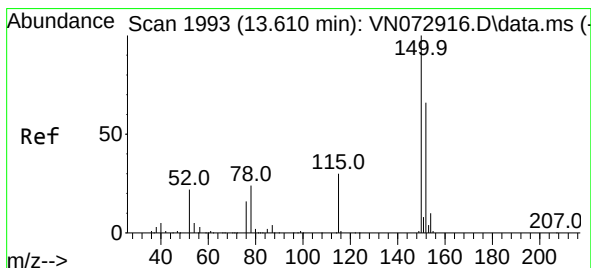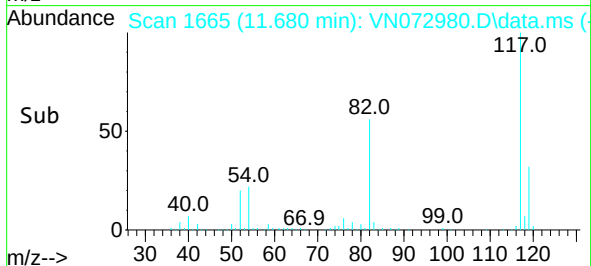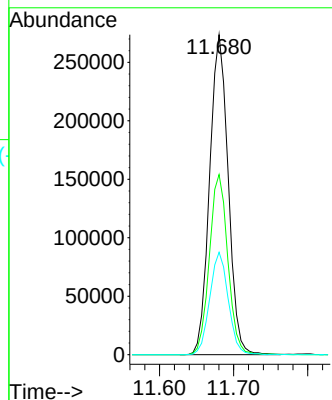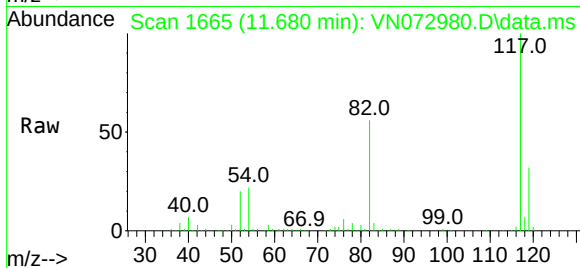

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.610 min Scan# 1993

Delta R.T. 0.000 min

Lab File: VN072980.D

Acq: 21 Jun 2022 13:53

Tgt Ion:152 Resp: 237723

Ion Ratio Lower Upper

152 100

115 61.1 28.9 86.7

150 157.7 0.0 356.2

