
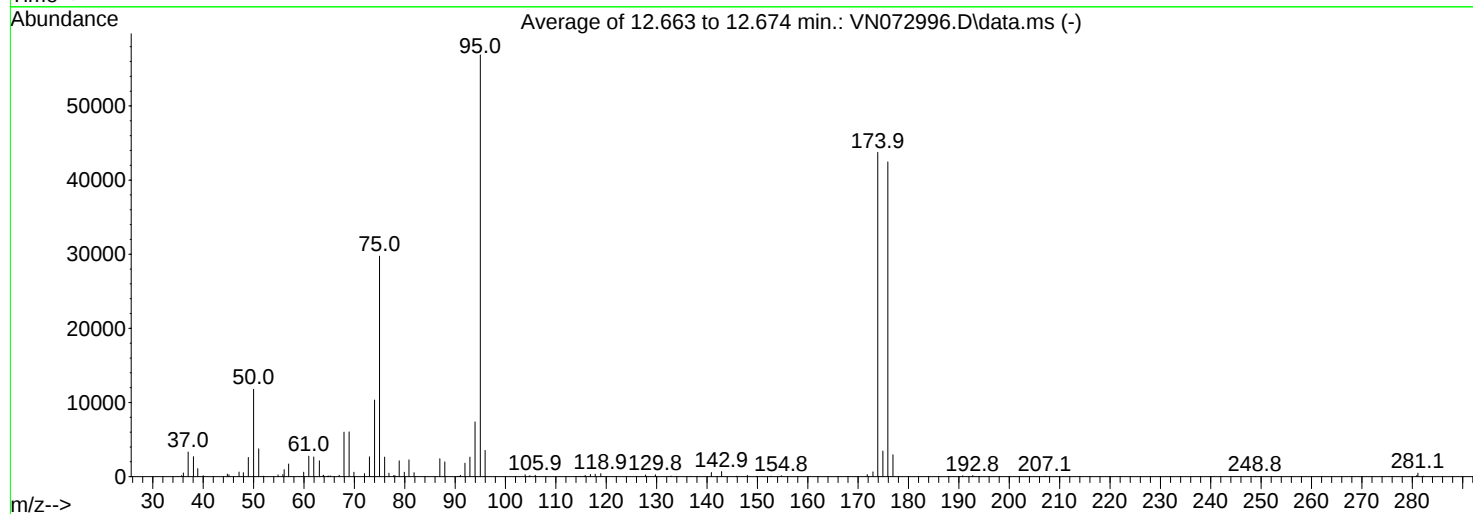


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN062122\
Data File : VN072996.D
Acq On : 22 Jun 2022 01:14
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N061722W.M
Title : SW846 8260
Last Update : Sat Jun 18 06:22:45 2022

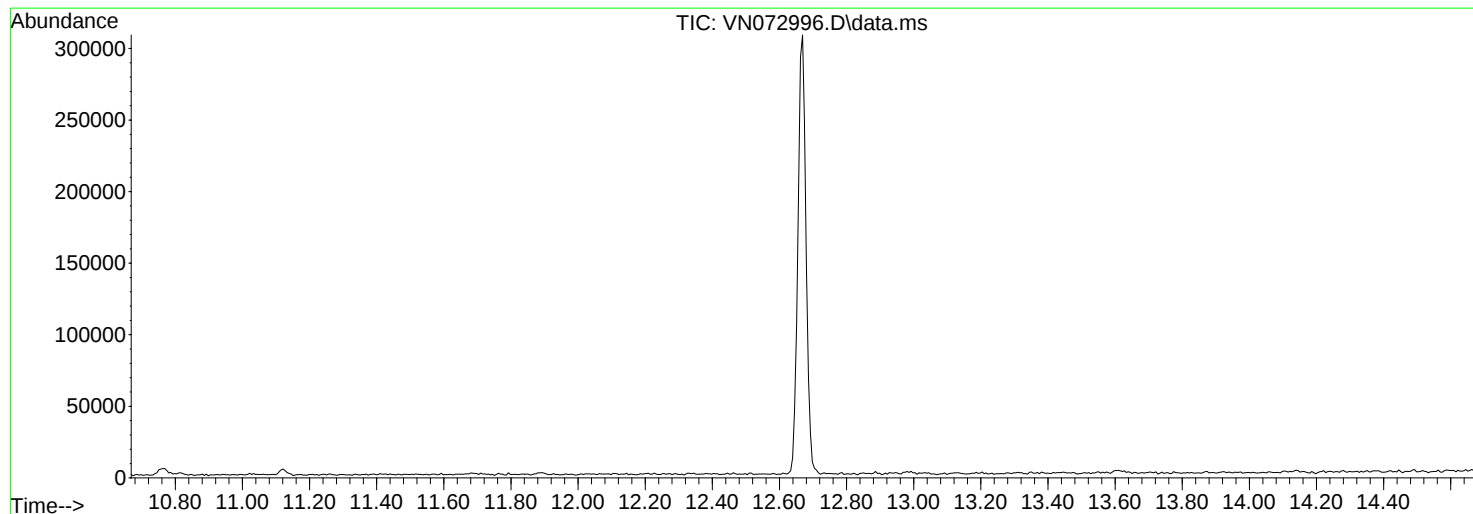

AutoFind: Scans 1832, 1833, 1834; Background Corrected with Scan 1823

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.7	11787	PASS
75	95	30	60	52.3	29744	PASS
95	95	100	100	100.0	56893	PASS
96	95	5	9	6.2	3548	PASS
173	174	0.00	2	1.5	650	PASS
174	95	50	100	76.9	43739	PASS
175	174	5	9	7.9	3463	PASS
176	174	95	101	97.0	42445	PASS
177	176	5	9	7.0	2966	PASS