

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN062123\  
 Data File : VN078327.D  
 Acq On : 21 Jun 2023 17:10  
 Operator : JC\MD  
 Sample : 03336-08  
 Misc : 5.0mL/MSVOA\_N/WATER  
 ALS Vial : 14 Sample Multiplier: 1

Instrument :  
 MSVOA\_N  
 ClientSampleId :

Quant Time: Jun 22 04:52:06 2023  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N060623W.M  
 Quant Title : SW846 8260  
 QLast Update : Wed Jun 07 05:05:00 2023  
 Response via : Initial Calibration


| Compound                      | R.T.           | QIon | Response            | Conc      | Units  | Dev(Min) |
|-------------------------------|----------------|------|---------------------|-----------|--------|----------|
| -----                         |                |      |                     |           |        |          |
| Internal Standards            |                |      |                     |           |        |          |
| 1) Pentafluorobenzene         | 8.229          | 168  | 459241              | 50.000    | ug/l   | 0.00     |
| 34) 1,4-Difluorobenzene       | 9.112          | 114  | 866972              | 50.000    | ug/l   | 0.00     |
| 63) Chlorobenzene-d5          | 11.870         | 117  | 814077              | 50.000    | ug/l   | 0.00     |
| 72) 1,4-Dichlorobenzene-d4    | 13.800         | 152  | 260720              | 50.000    | ug/l   | 0.00     |
|                               |                |      |                     |           |        |          |
| System Monitoring Compounds   |                |      |                     |           |        |          |
| 33) 1,2-Dichloroethane-d4     | 8.588          | 65   | 327095              | 53.420    | ug/l   | 0.00     |
| Spiked Amount 50.000          | Range 74 - 125 |      | Recovery = 106.840% |           |        |          |
| 35) Dibromofluoromethane      | 8.177          | 113  | 303637              | 55.391    | ug/l   | 0.00     |
| Spiked Amount 50.000          | Range 75 - 124 |      | Recovery = 110.780% |           |        |          |
| 50) Toluene-d8                | 10.576         | 98   | 1040418             | 49.233    | ug/l   | 0.00     |
| Spiked Amount 50.000          | Range 86 - 113 |      | Recovery = 98.460%  |           |        |          |
| 62) 4-Bromofluorobenzene      | 12.853         | 95   | 337943              | 51.440    | ug/l   | 0.00     |
| Spiked Amount 50.000          | Range 83 - 123 |      | Recovery = 102.880% |           |        |          |
|                               |                |      |                     |           |        |          |
| Target Compounds              |                |      |                     |           |        | Qvalue   |
| 3) Chloromethane              | 2.383          | 50   | 990                 | Below Cal | #      | 87       |
| 11) Tert butyl alcohol        | 5.536          | 59   | 2138                | 2.529     | ug/l # | 88       |
| 16) Acetone                   | 4.453          | 43   | 38811               | 22.021    | ug/l   | 95       |
| 18) Methyl Acetate            | 5.059          | 43   | 4084                | 0.503     | ug/l # | 71       |
| 20) Methylene Chloride        | 5.294          | 84   | 23571               | 4.047     | ug/l   | 92       |
| 25) 2-Butanone                | 7.506          | 43   | 14231               | 5.251     | ug/l # | 69       |
| 29) Tetrahydrofuran           | 7.859          | 42   | 751                 | 0.414     | ug/l # | 38       |
| 31) Cyclohexane               | 8.235          | 56   | 11157               | 1.420     | ug/l # | 41       |
| 36) 1,1-Dichloropropene       | 8.229          | 75   | 37723               | 4.798     | ug/l # | 48       |
| 37) Ethyl Acetate             | 7.571          | 43   | 57650               | 9.385     | ug/l # | 94       |
| 38) Carbon Tetrachloride      | 8.235          | 117  | 47405               | 5.710     | ug/l # | 16       |
| 42) 1,2-Dichloroethane        | 8.694          | 62   | 2118                | 0.263     | ug/l # | 73       |
| 43) Isopropyl Acetate         | 8.700          | 43   | 317043              | 26.989    | ug/l # | 80       |
| 45) 1,2-Dichloropropane       | 9.741          | 63   | 2938                | 0.503     | ug/l # | 45       |
| 48) Methyl methacrylate       | 9.676          | 41   | 8342                | 1.692     | ug/l # | 32       |
| 49) 1,4-Dioxane               | 9.682          | 88   | 180                 | 1.737     | ug/l # | 1        |
| 51) 4-Methyl-2-Pentanone      | 10.365         | 43   | 196123              | 31.704    | ug/l # | 41       |
| 53) t-1,3-Dichloropropene     | 10.735         | 75   | 1879                | 0.226     | ug/l # | 52       |
| 54) cis-1,3-Dichloropropene   | 10.365         | 75   | 104074              | 11.313    | ug/l # | 68       |
| 57) 1,3-Dichloropropane       | 11.206         | 76   | 11036               | 1.166     | ug/l # | 43       |
| 59) 2-Hexanone                | 11.176         | 43   | 233511              | 54.213    | ug/l # | 19       |
| 71) Bromoform                 | 12.853         | 173  | 2561                | 0.619     | ug/l # | 1        |
| 74) N-amyl acetate            | 12.470         | 43   | 1824                | 0.225     | ug/l # | 47       |
| 75) 1,1,2,2-Tetrachloroethane | 12.912         | 83   | 102                 | Below Cal | #      | 26       |
| 76) 1,2,3-Trichloropropane    | 12.853         | 75   | 181416              | 29.434    | ug/l # | 1        |
| 81) trans-1,4-Dichloro-2-b... | 12.853         | 75   | 181416              | 90.430    | ug/l # | 15       |
| 94) Hexachlorobutadiene       | 15.506         | 225  | 60                  | Below Cal | #      | 19       |
| -----                         |                |      |                     |           |        |          |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN062123\  
Data File : VN078327.D  
Acq On : 21 Jun 2023 17:10  
Operator : JC\MD  
Sample : 03336-08  
Misc : 5.0mL/MSVOA\_N/WATER  
ALS Vial : 14 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :

Quant Time: Jun 22 04:52:06 2023  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N060623W.M  
Quant Title : SW846 8260  
QLast Update : Wed Jun 07 05:05:00 2023  
Response via : Initial Calibration

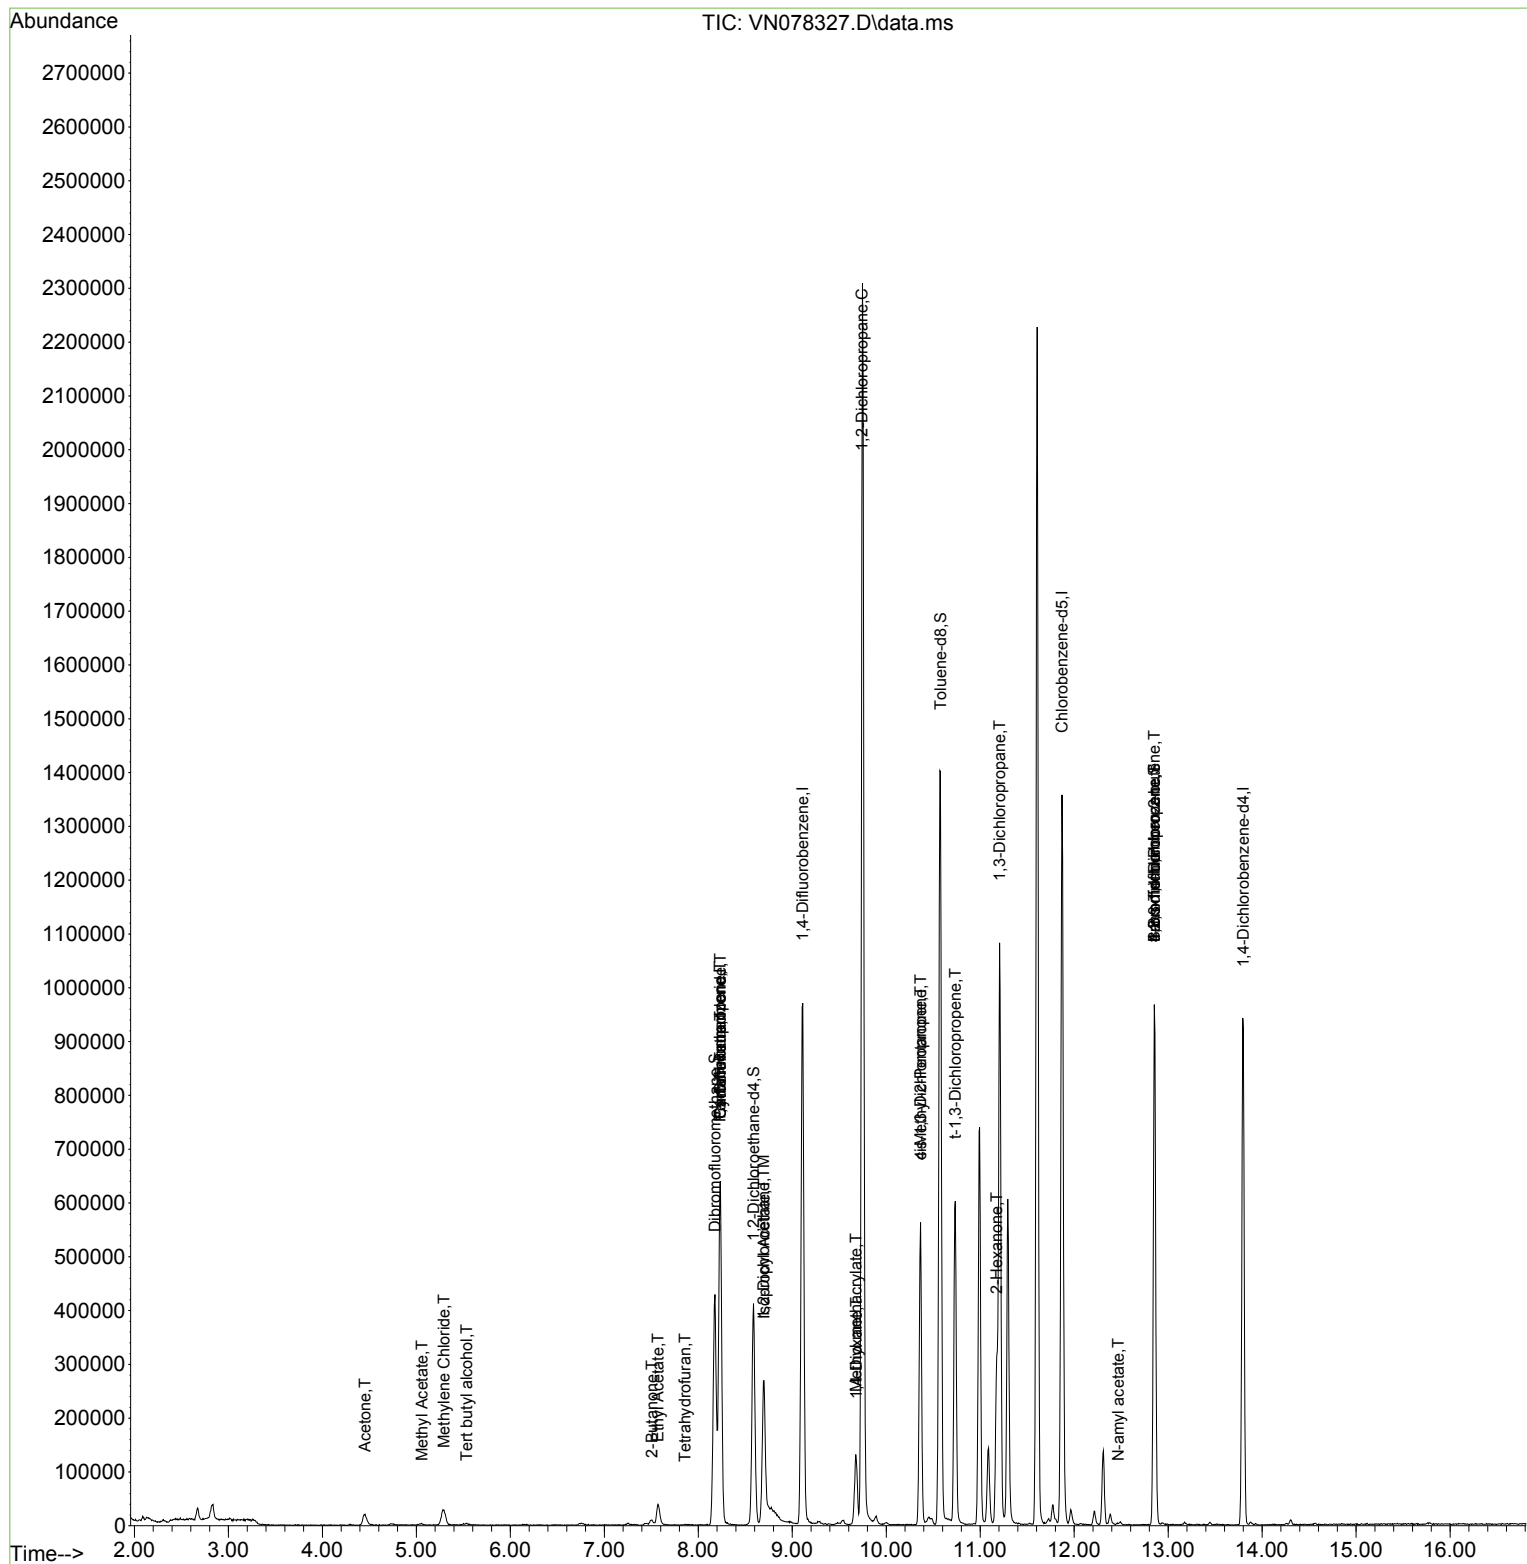

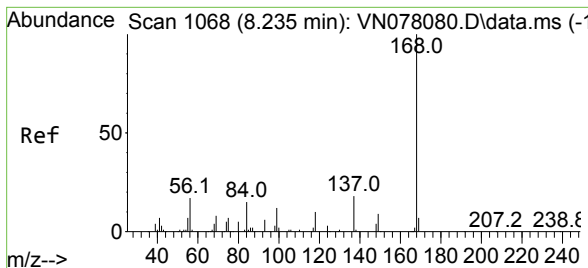

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 8.229 min Scan# 11

Delta R.T. -0.005 min

Lab File: VN078327.D

Acq: 21 Jun 2023 17:10

Instrument :

MSVOA\_N





ClientSampleId :

Tgt Ion:168 Resp: 459241

Ion Ratio Lower Upper

168 100

99 62.5 53.0 79.6

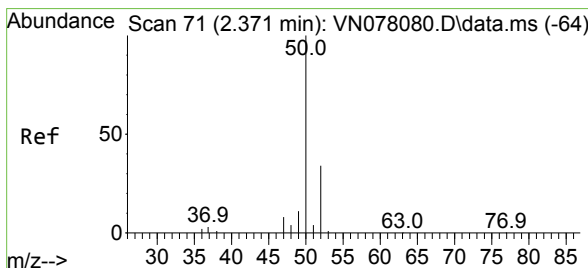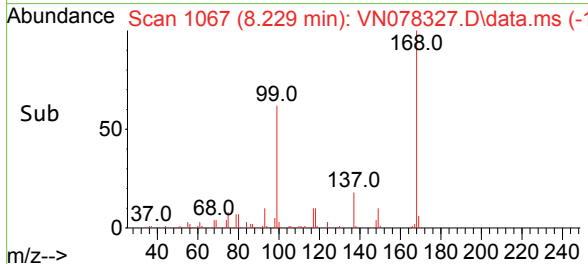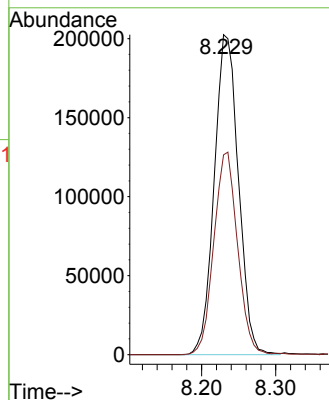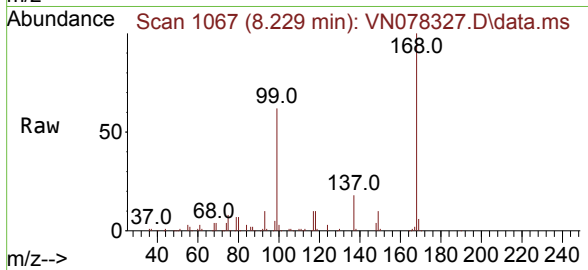

#3

Chloromethane

Concen: Below Cal

RT: 2.383 min Scan# 73

Delta R.T. 0.012 min

Lab File: VN078327.D




Acq: 21 Jun 2023 17:10


Tgt Ion: 50 Resp: 990

Ion Ratio Lower Upper

50 100


52 40.5 26.5 39.7#

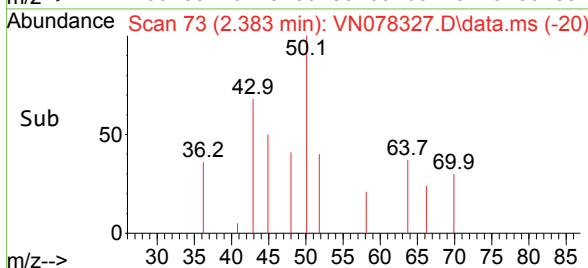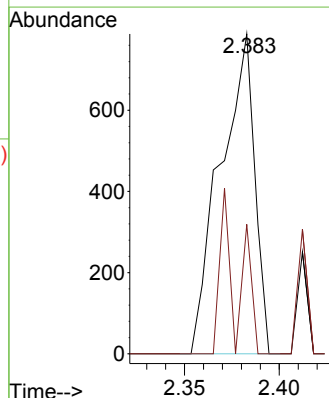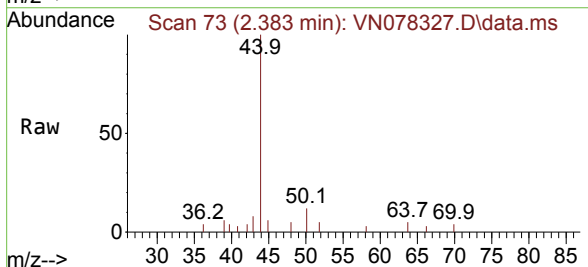






#11  
Tert butyl alcohol  
Concen: 2.529 ug/l  
RT: 5.536 min Scan# 609  
Delta R.T. -0.000 min  
Lab File: VN078327.D  
Acq: 21 Jun 2023 17:10

Instrument :  
MSVOA\_N  
ClientSampleId :







Tgt Ion: 59 Resp: 2138  
Ion Ratio Lower Upper  
59 100  
57 5.9 8.2 12.4#

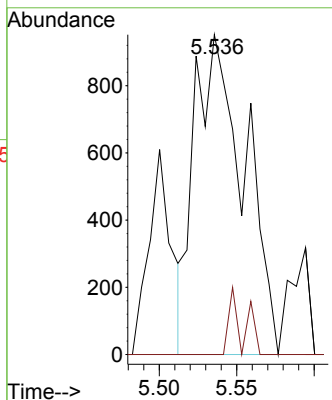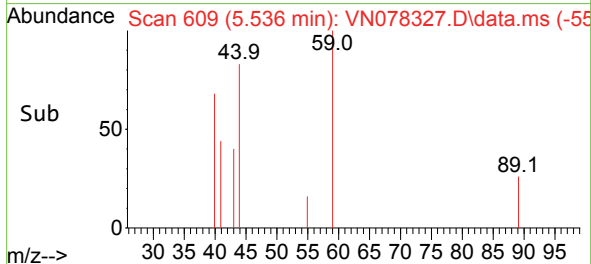

#16  
Acetone  
Concen: 22.021 ug/l  
RT: 4.453 min Scan# 425  
Delta R.T. 0.018 min  
Lab File: VN078327.D  
Acq: 21 Jun 2023 17:10

Tgt Ion: 43 Resp: 38811  
Ion Ratio Lower Upper  
43 100  
58 37.7 28.0 42.0


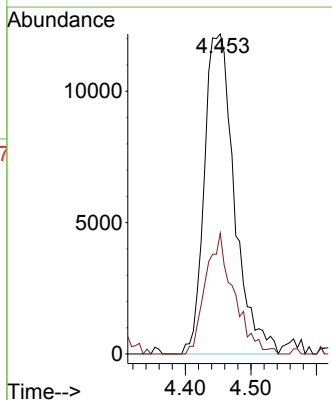
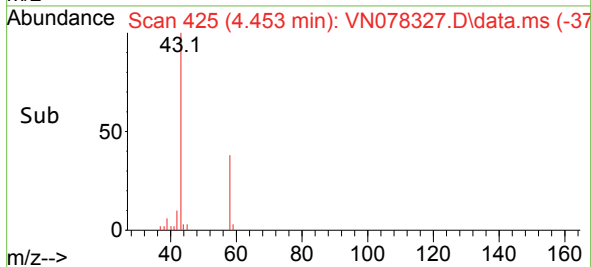
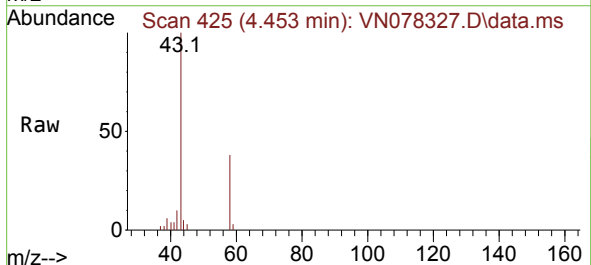




#18  
Methyl Acetate  
Concen: 0.503 ug/l  
RT: 5.059 min Scan# 51  
Delta R.T. 0.024 min  
Lab File: VN078327.D  
Acq: 21 Jun 2023 17:10




Instrument :  
MSVOA\_N  
ClientSampleId :


Tgt Ion: 43 Resp: 4084  
Ion Ratio Lower Upper  
43 100  
74 16.3 26.2 39.4#

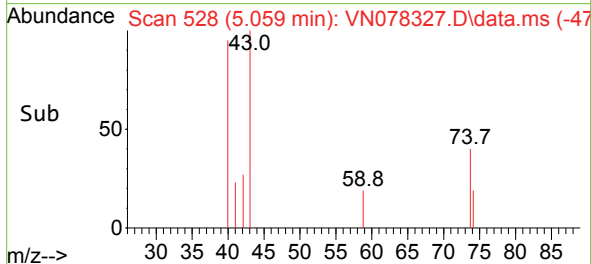

#20  
Methylene Chloride  
Concen: 4.047 ug/l  
RT: 5.294 min Scan# 568  
Delta R.T. 0.012 min  
Lab File: VN078327.D  
Acq: 21 Jun 2023 17:10

Tgt Ion: 84 Resp: 23571  
Ion Ratio Lower Upper  
84 100  
49 96.0 79.7 119.5  
51 33.6 25.2 37.8  
86 53.9 53.3 79.9


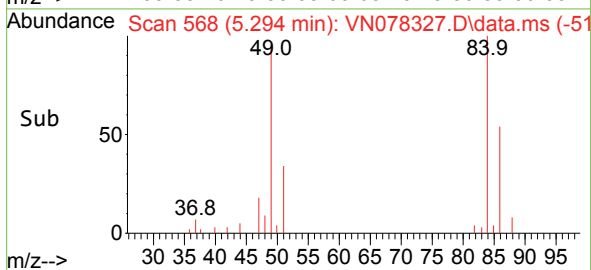
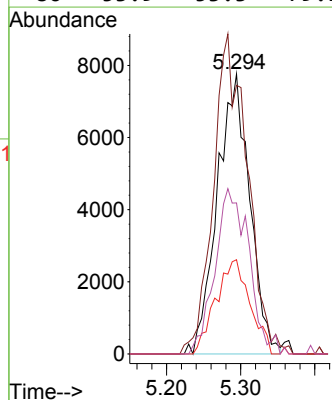
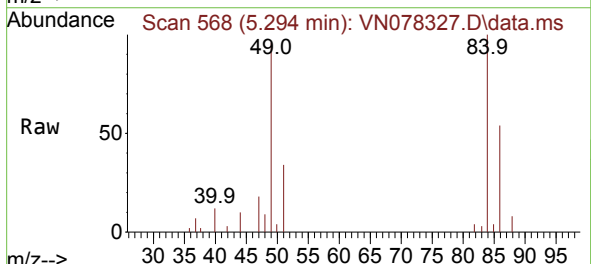




#25  
2-Butanone  
Concen: 5.251 ug/l  
RT: 7.506 min Scan# 94  
Delta R.T. 0.012 min  
Lab File: VN078327.D  
Acq: 21 Jun 2023 17:10




Instrument :  
MSVOA\_N  
ClientSampleId :


Tgt Ion: 43 Resp: 14231  
Ion Ratio Lower Upper  
43 100  
72 18.9 30.2 45.2#

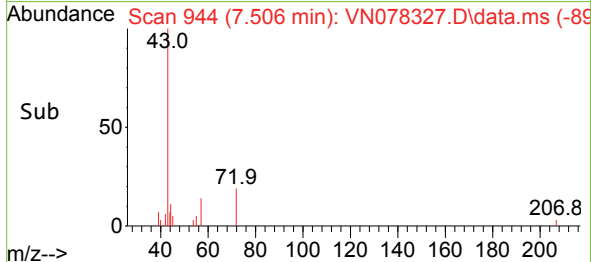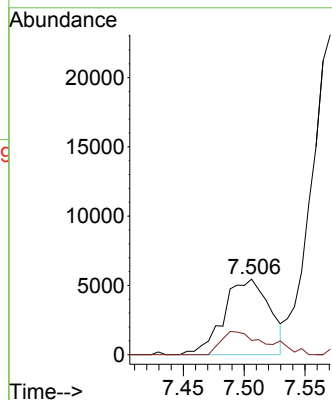

#29  
Tetrahydrofuran  
Concen: 0.414 ug/l  
RT: 7.859 min Scan# 1004  
Delta R.T. 0.012 min  
Lab File: VN078327.D  
Acq: 21 Jun 2023 17:10

Tgt Ion: 42 Resp: 751  
Ion Ratio Lower Upper  
42 100  
72 26.6 49.8 74.6#  
71 0.0 47.4 71.2#

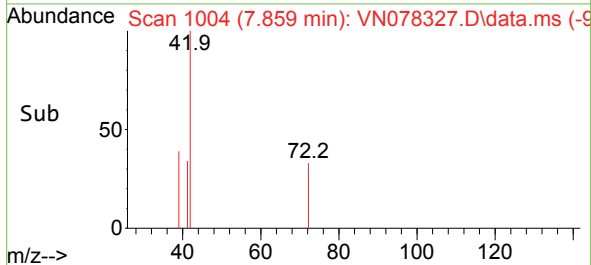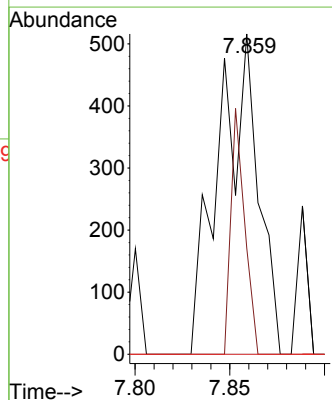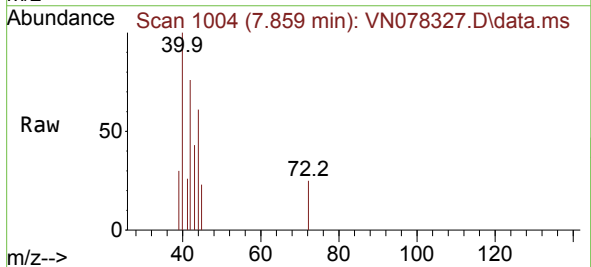



#31

Cyclohexane

Concen: 1.420 ug/l

RT: 8.235 min Scan# 1068

Delta R.T. -0.029 min


Lab File: VN078327.D

Acq: 21 Jun 2023 17:10

Instrument :

MSVOA\_N

ClientSampleId :

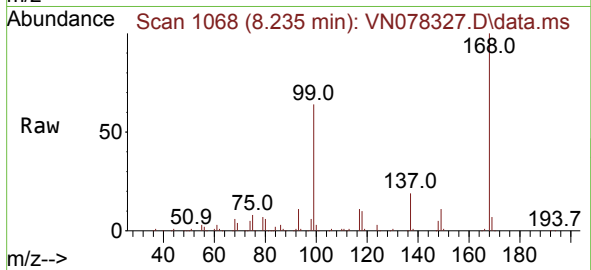




Tgt Ion: 56 Resp: 11157

Ion Ratio Lower Upper

56 100

69 163.6 26.8 40.2#

84 98.2 81.8 122.6

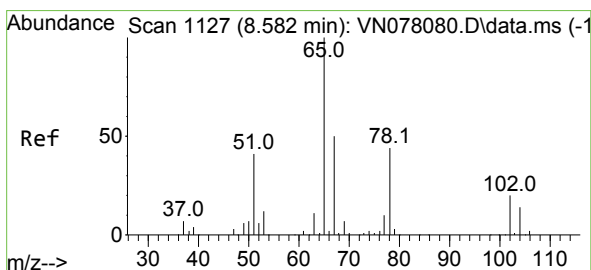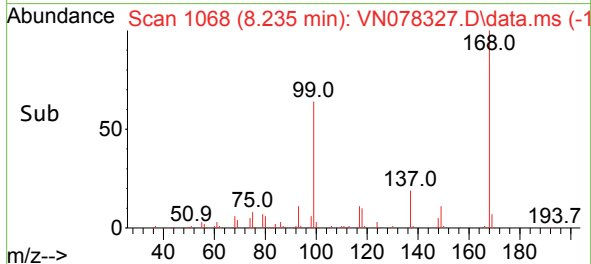

#33

1,2-Dichloroethane-d4

Concen: 53.420 ug/l

RT: 8.588 min Scan# 1128

Delta R.T. 0.006 min

Lab File: VN078327.D




Acq: 21 Jun 2023 17:10


Tgt Ion: 65 Resp: 327095

Ion Ratio Lower Upper

65 100

67 52.1 0.0 106.6

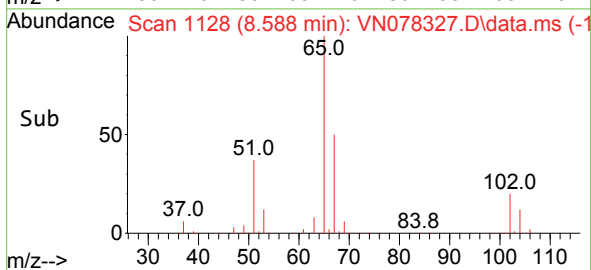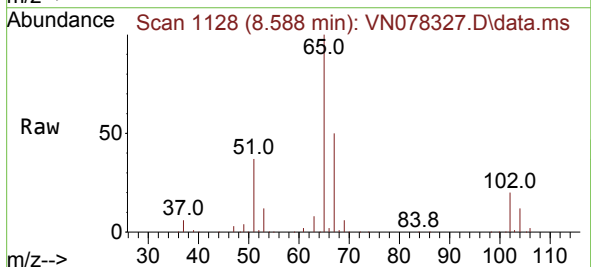



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.112 min Scan# 1

Delta R.T. 0.006 min

Lab File: VN078327.D

Acq: 21 Jun 2023 17:10

Instrument :

MSVOA\_N

ClientSampleId :





Tgt Ion:114 Resp: 866972

Ion Ratio Lower Upper

114 100

63 19.6 0.0 36.4

88 15.0 0.0 30.6

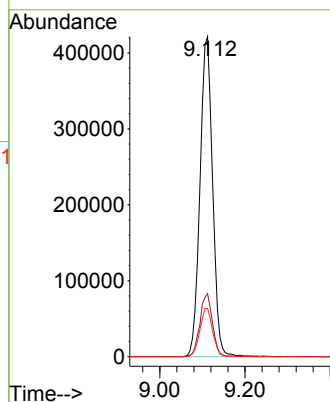

#35

Dibromofluoromethane

Concen: 55.391 ug/l

RT: 8.177 min Scan# 1058

Delta R.T. -0.000 min

Lab File: VN078327.D

Acq: 21 Jun 2023 17:10




Tgt Ion:113 Resp: 303637


Ion Ratio Lower Upper

113 100

111 102.5 82.6 123.8


192 17.0 12.7 19.1

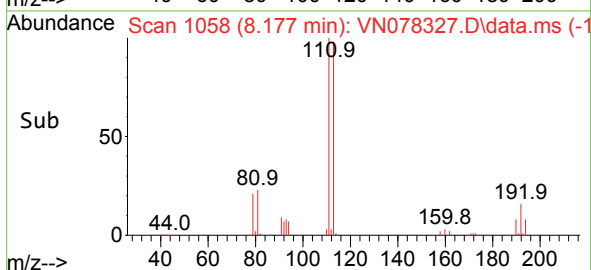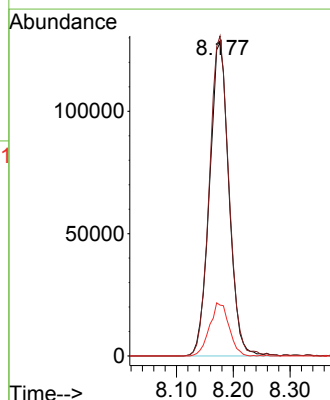






#36  
1,1-Dichloropropene  
Concen: 4.798 ug/l  
RT: 8.229 min Scan# 1067  
Delta R.T. -0.147 min  
Lab File: VN078327.D  
Acq: 21 Jun 2023 17:10

Instrument :  
MSVOA\_N  
ClientSampleId :







Tgt Ion: 75 Resp: 37723  
Ion Ratio Lower Upper  
75 100  
110 9.3 19.1 57.3#  
77 0.0 25.0 37.4#

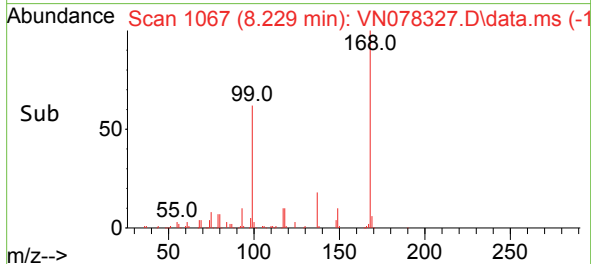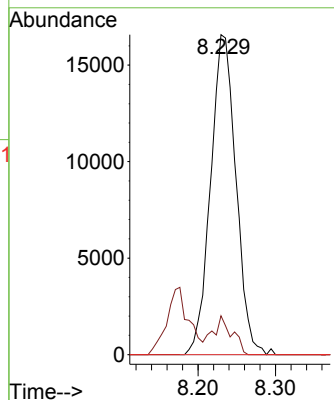

#37  
Ethyl Acetate  
Concen: 9.385 ug/l  
RT: 7.571 min Scan# 955  
Delta R.T. -0.000 min  
Lab File: VN078327.D  
Acq: 21 Jun 2023 17:10

Tgt Ion: 43 Resp: 57650  
Ion Ratio Lower Upper  
43 100  
61 14.9 13.2 19.8  
70 10.4 11.3 16.9#

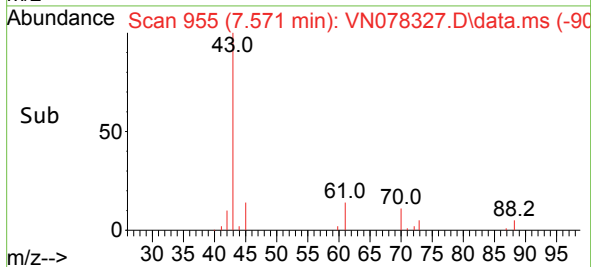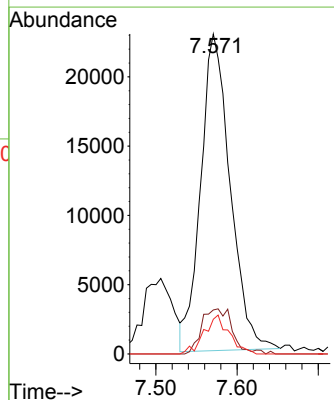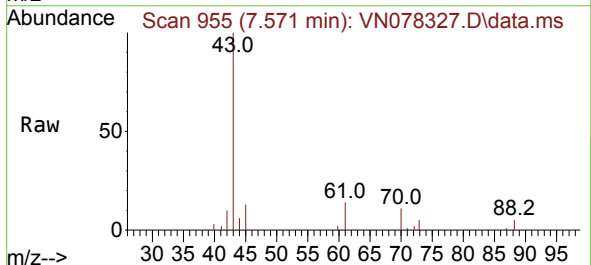



#38

Carbon Tetrachloride

Concen: 5.710 ug/l

RT: 8.235 min Scan# 1068

Delta R.T. -0.135 min


Lab File: VN078327.D

Acq: 21 Jun 2023 17:10

Instrument :

MSVOA\_N

ClientSampleId :

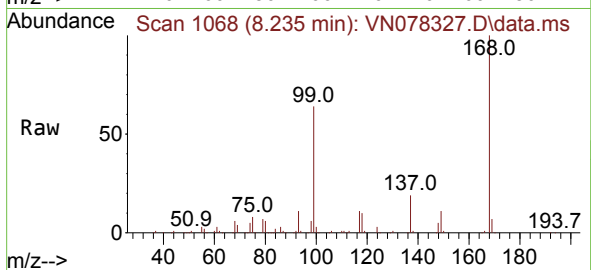




Tgt Ion:117 Resp: 47405

Ion Ratio Lower Upper

117 100

119 5.0 77.3 115.9#

121 0.0 23.3 34.9#

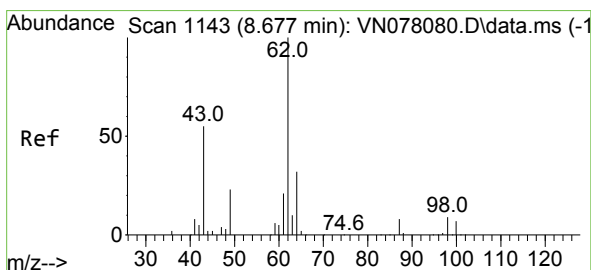

#42

1,2-Dichloroethane

Concen: 0.263 ug/l

RT: 8.694 min Scan# 1146

Delta R.T. 0.018 min

Lab File: VN078327.D




Acq: 21 Jun 2023 17:10


Tgt Ion: 62 Resp: 2118

Ion Ratio Lower Upper

62 100


98 0.0 0.0 19.8

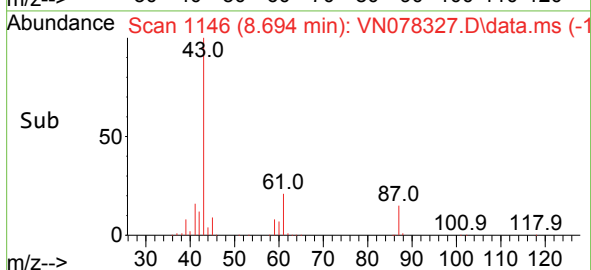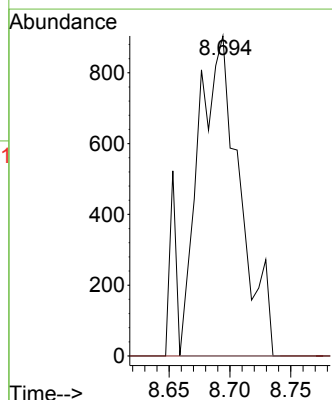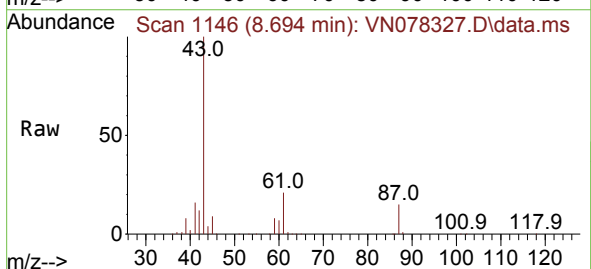






#43  
Isopropyl Acetate  
Concen: 26.989 ug/l  
RT: 8.700 min Scan# 1146  
Delta R.T. 0.006 min  
Lab File: VN078327.D  
Acq: 21 Jun 2023 17:10

Instrument :  
MSVOA\_N  
ClientSampleId :







Tgt Ion: 43 Resp: 317043  
Ion Ratio Lower Upper  
43 100  
61 18.1 24.7 37.1#  
87 12.4 14.6 21.8#

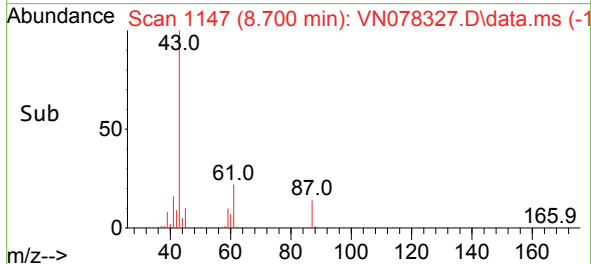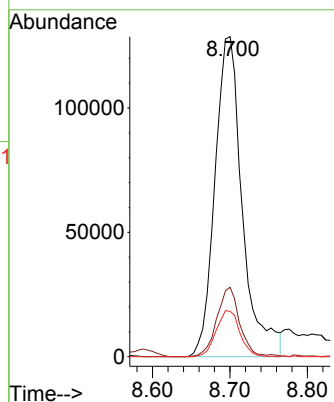

#45  
1,2-Dichloropropane  
Concen: 0.503 ug/l  
RT: 9.741 min Scan# 1324  
Delta R.T. 0.112 min  
Lab File: VN078327.D  
Acq: 21 Jun 2023 17:10

Tgt Ion: 63 Resp: 2938  
Ion Ratio Lower Upper  
63 100  
65 0.0 23.9 35.9#


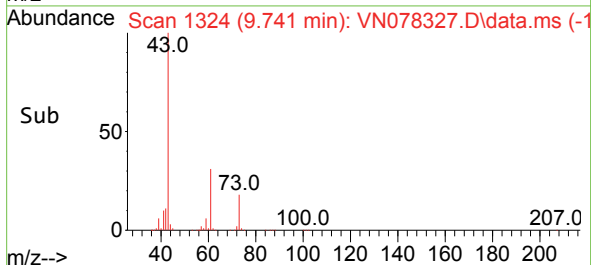
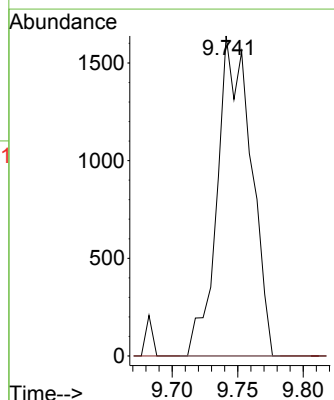
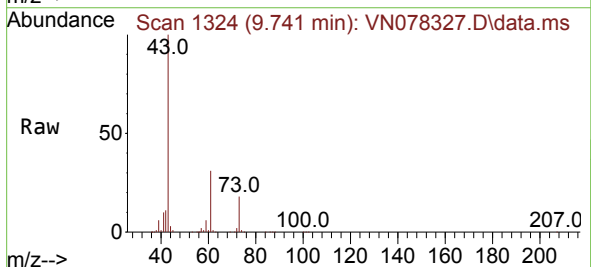




#48  
Methyl methacrylate  
Concen: 1.692 ug/l  
RT: 9.676 min Scan# 11  
Delta R.T. -0.012 min  
Lab File: VN078327.D  
Acq: 21 Jun 2023 17:10




Instrument :  
MSVOA\_N  
ClientSampleId :


Tgt Ion: 41 Resp: 8342  
Ion Ratio Lower Upper  
41 100  
69 1.1 90.4 135.6#  
39 61.4 54.6 81.8

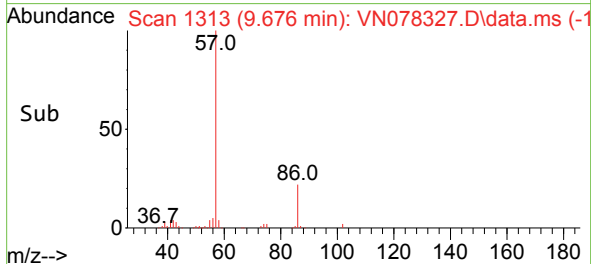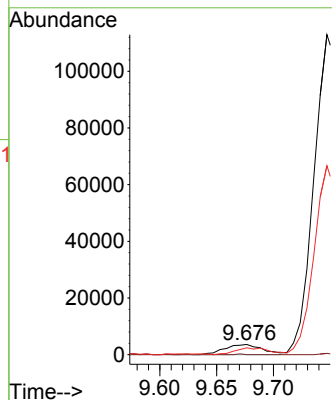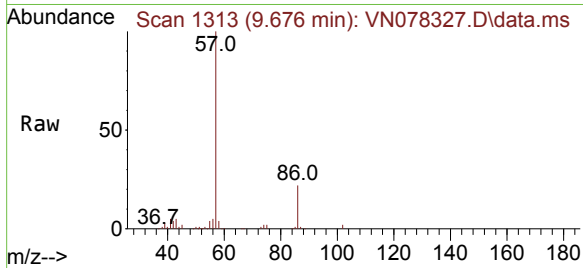

#49  
1,4-Dioxane  
Concen: 1.737 ug/l  
RT: 9.682 min Scan# 1314  
Delta R.T. -0.018 min  
Lab File: VN078327.D  
Acq: 21 Jun 2023 17:10

Tgt Ion: 88 Resp: 180  
Ion Ratio Lower Upper  
88 100  
43 0.0 17.0 25.6#  
58 3389.4 47.0 70.4#

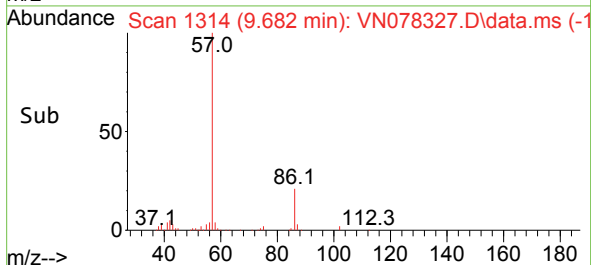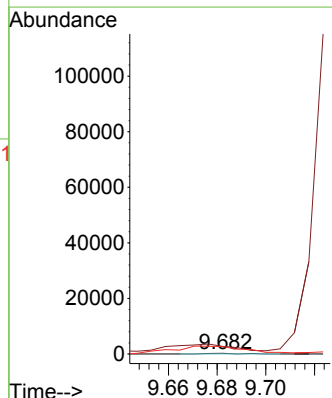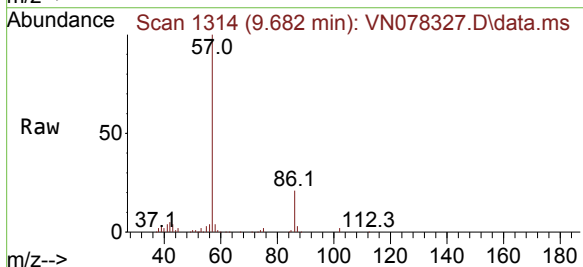



#50

Toluene-d8

Concen: 49.233 ug/l

RT: 10.576 min Scan# 1465

Delta R.T. 0.006 min

Lab File: VN078327.D

Acq: 21 Jun 2023 17:10

Instrument :

MSVOA\_N





ClientSampleId :

Tgt Ion: 98 Resp: 1040418

Ion Ratio Lower Upper

98 100

100 62.3 52.0 78.0

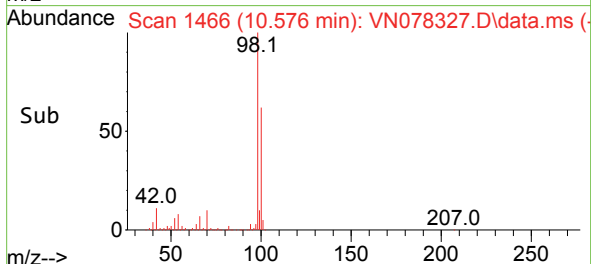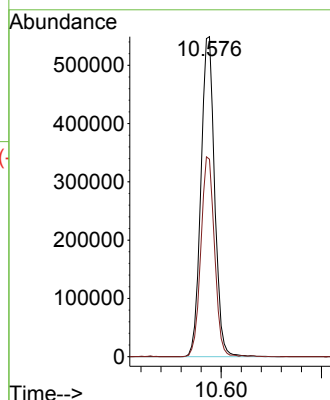

#51

4-Methyl-2-Pentanone

Concen: 31.704 ug/l

RT: 10.365 min Scan# 1430

Delta R.T. -0.088 min

Lab File: VN078327.D




Acq: 21 Jun 2023 17:10


Tgt Ion: 43 Resp: 196123

Ion Ratio Lower Upper

43 100


58 7.1 36.6 54.8#

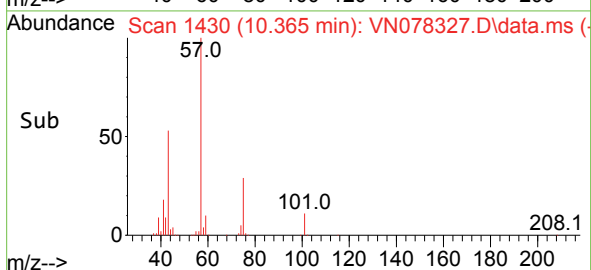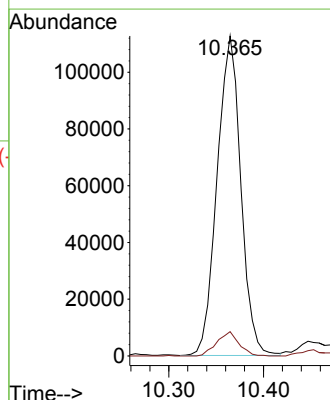






#53  
 t-1,3-Dichloropropene  
 Concen: 0.226 ug/l  
 RT: 10.735 min Scan# 14  
 Delta R.T. -0.106 min  
 Lab File: VN078327.D  
 Acq: 21 Jun 2023 17:10

Instrument :  
 MSVOA\_N  
 ClientSampleId :







Tgt Ion: 75 Resp: 1879  
 Ion Ratio Lower Upper  
 75 100  
 77 5.1 25.4 38.0#

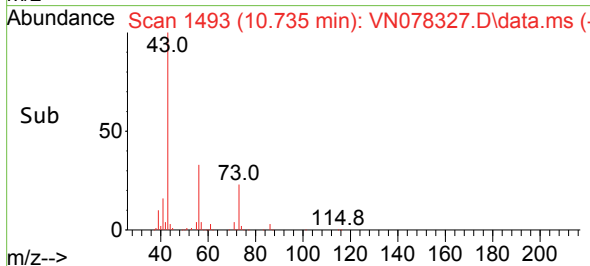

#54  
 cis-1,3-Dichloropropene  
 Concen: 11.313 ug/l  
 RT: 10.365 min Scan# 1430  
 Delta R.T. 0.047 min  
 Lab File: VN078327.D  
 Acq: 21 Jun 2023 17:10

Tgt Ion: 75 Resp: 104074  
 Ion Ratio Lower Upper  
 75 100  
 77 0.5 26.1 39.1#  
 39 32.3 31.6 47.4

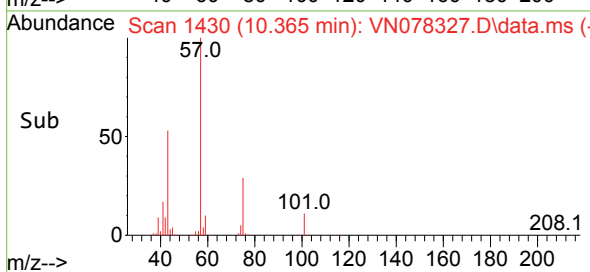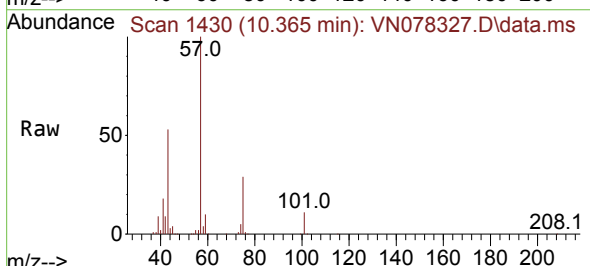

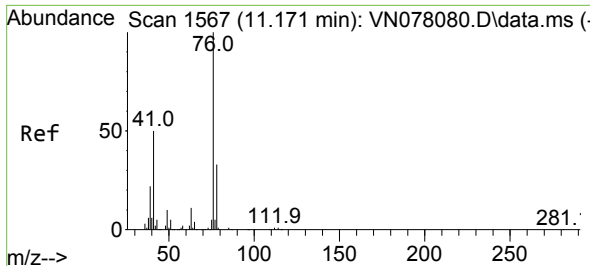

#57

1,3-Dichloropropane

Concen: 1.166 ug/l

RT: 11.206 min Scan# 11

Delta R.T. 0.035 min


Lab File: VN078327.D

Acq: 21 Jun 2023 17:10

Instrument :

MSVOA\_N

ClientSampleId :






Tgt Ion: 76 Resp: 11036

Ion Ratio Lower Upper

76 100

78 0.5 26.1 39.1#

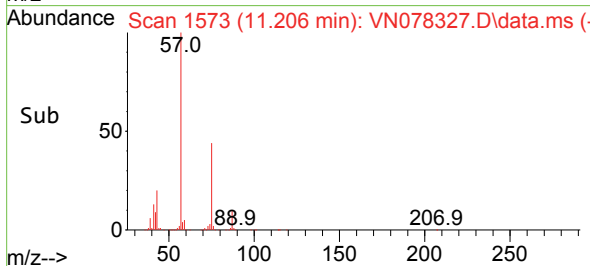

#59

2-Hexanone

Concen: 54.213 ug/l

RT: 11.176 min Scan# 1568

Delta R.T. -0.024 min

Lab File: VN078327.D




Acq: 21 Jun 2023 17:10


Tgt Ion: 43 Resp: 233511

Ion Ratio Lower Upper

43 100

58 0.0 31.7 95.1#


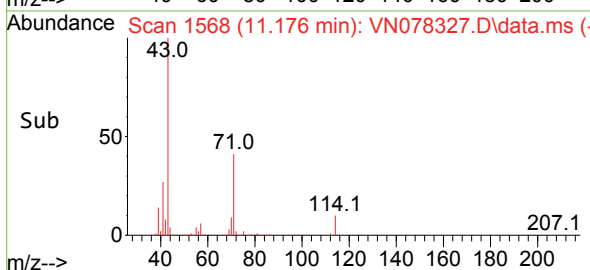

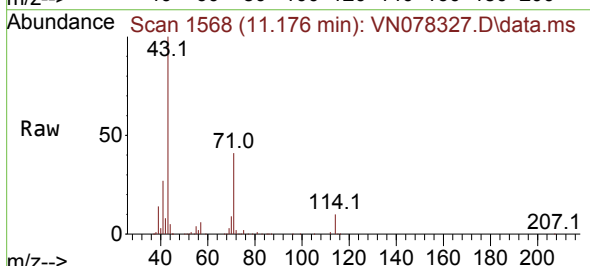




#62  
4-Bromofluorobenzene  
Concen: 51.440 ug/l  
RT: 12.853 min Scan# 1853  
Delta R.T. -0.000 min  
Lab File: VN078327.D  
Acq: 21 Jun 2023 17:10




Instrument :  
MSVOA\_N  
ClientSampleId :


Tgt Ion: 95 Resp: 337943  
Ion Ratio Lower Upper  
95 100  
174 76.9 0.0 143.8  
176 72.5 0.0 135.8

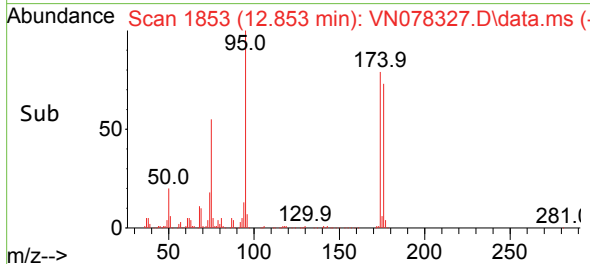

#63  
Chlorobenzene-d5  
Concen: 50.000 ug/l  
RT: 11.870 min Scan# 1686  
Delta R.T. -0.000 min  
Lab File: VN078327.D  
Acq: 21 Jun 2023 17:10

Tgt Ion: 117 Resp: 814077  
Ion Ratio Lower Upper  
117 100  
82 56.1 44.0 66.0  
119 31.6 25.6 38.4

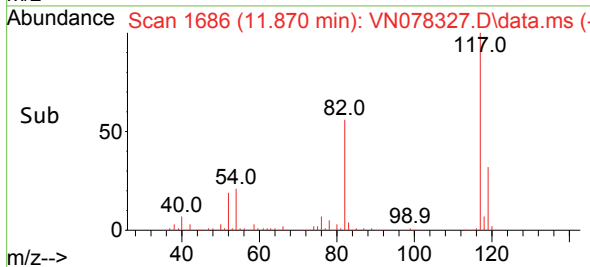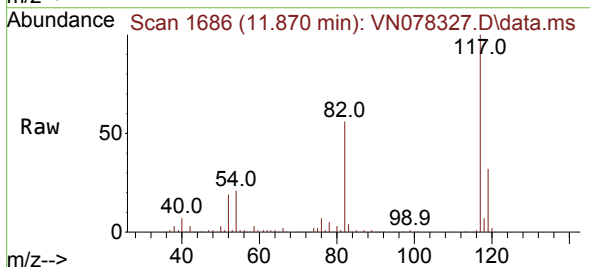



#71

Bromoform

Concen: 0.619 ug/l

RT: 12.853 min Scan# 1808

Delta R.T. 0.265 min


Lab File: VN078327.D

Acq: 21 Jun 2023 17:10

Instrument :

MSVOA\_N

ClientSampleId :






Tgt Ion:173 Resp: 2561

Ion Ratio Lower Upper

173 100

175 660.2 24.3 73.0#

254 0.0 0.0 0.0

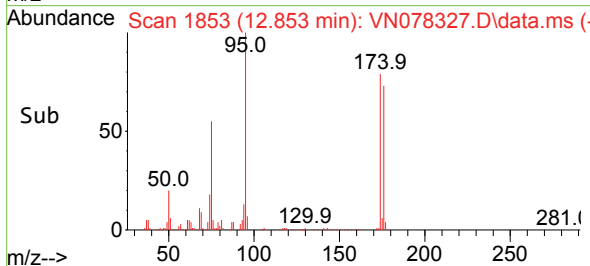

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.800 min Scan# 2014

Delta R.T. -0.000 min

Lab File: VN078327.D

Acq: 21 Jun 2023 17:10




Tgt Ion:152 Resp: 260720


Ion Ratio Lower Upper

152 100

115 63.2 32.3 96.8


150 155.7 0.0 355.8

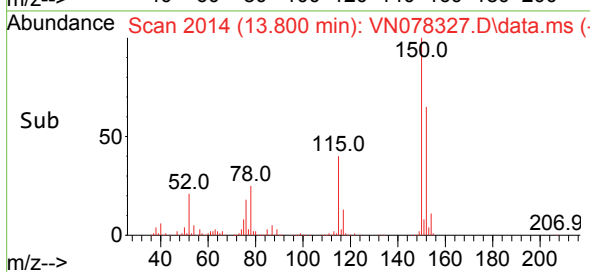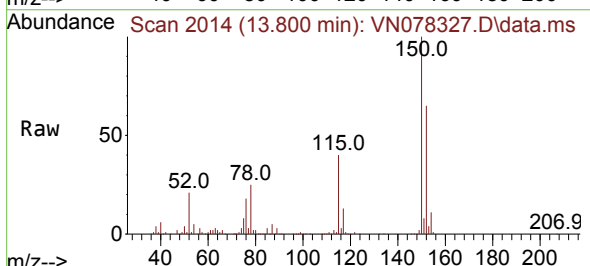






#74  
N-amy1 acetate  
Concen: 0.225 ug/l  
RT: 12.470 min Scan# 1793  
Delta R.T. -0.029 min  
Lab File: VN078327.D  
Acq: 21 Jun 2023 17:10

Instrument :  
MSVOA\_N  
ClientSampleId :







Tgt Ion: 43 Resp: 1824  
Ion Ratio Lower Upper  
43 100  
70 0.0 43.4 65.2#  
55 23.0 21.4 32.0  
61 0.0 22.8 34.2#

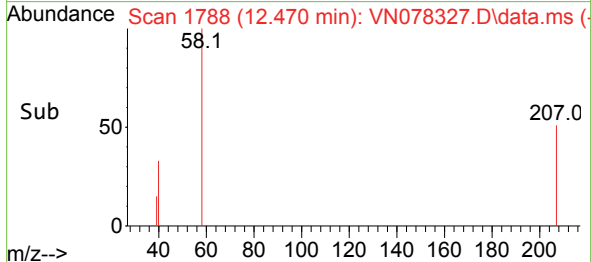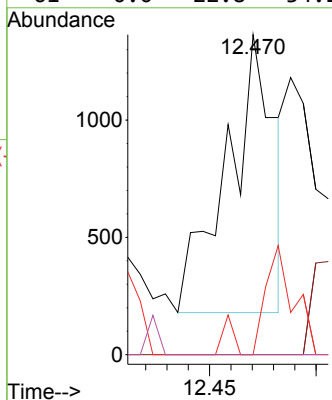

#75  
1,1,2,2-Tetrachloroethane  
Concen: Below Cal  
RT: 12.912 min Scan# 1863  
Delta R.T. -0.029 min  
Lab File: VN078327.D  
Acq: 21 Jun 2023 17:10

Tgt Ion: 83 Resp: 102  
Ion Ratio Lower Upper  
83 100  
131 0.0 5.0 15.0#  
85 0.0 31.9 95.7#

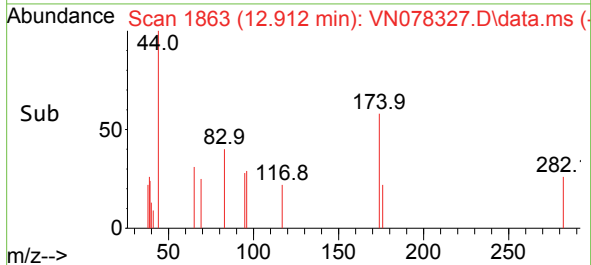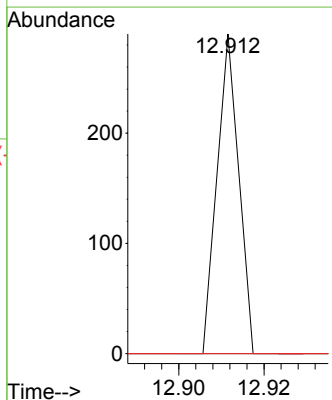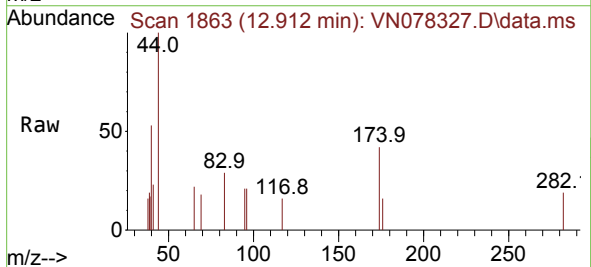



#76

1,2,3-Trichloropropane

Concen: 29.434 ug/l

RT: 12.853 min Scan# 1853

Delta R.T. -0.147 min

Lab File: VN078327.D

Acq: 21 Jun 2023 17:10

Instrument :

MSVOA\_N





ClientSampleId :

Tgt Ion: 75 Resp: 181416

Ion Ratio Lower Upper

75 100

77 1.3 84.5 253.5#

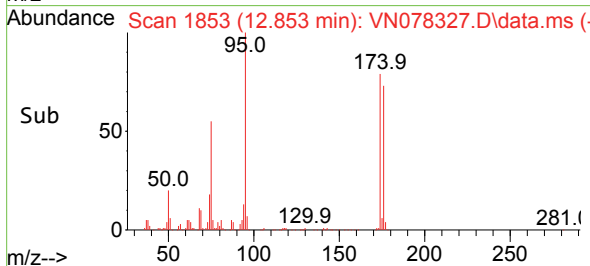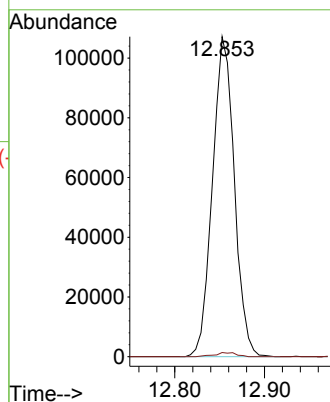

#81

trans-1,4-Dichloro-2-butene

Concen: 90.430 ug/l

RT: 12.853 min Scan# 1853

Delta R.T. 0.112 min

Lab File: VN078327.D

Acq: 21 Jun 2023 17:10




Tgt Ion: 75 Resp: 181416


Ion Ratio Lower Upper

75 100

53 0.1 67.4 101.2#


89 0.1 38.8 58.2#

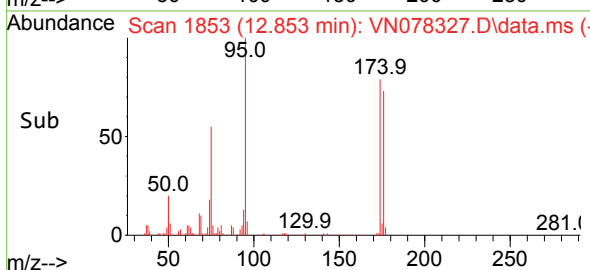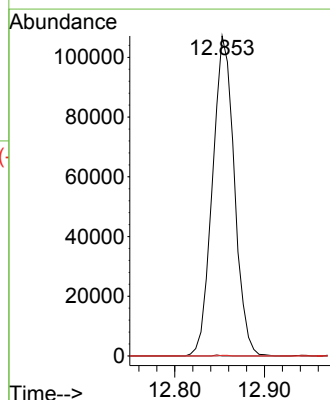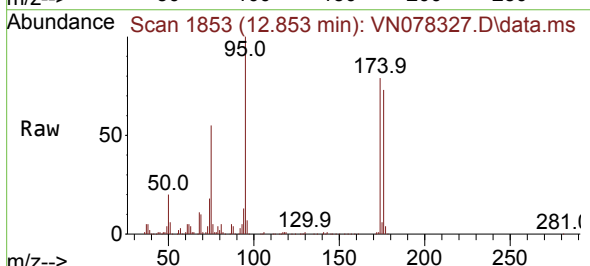



#94  
Hexachlorobutadiene  
Concen: Below Cal  
RT: 15.506 min Scan# 21  
Delta R.T. -0.001 min  
Lab File: VN078327.D  
Acq: 21 Jun 2023 17:10

Instrument :  
MSVOA\_N  
ClientSampleId :



Tgt Ion:225 Resp: 60  
Ion Ratio Lower Upper  
225 100  
223 0.0 31.3 93.8#  
227 0.0 31.9 95.9#

