
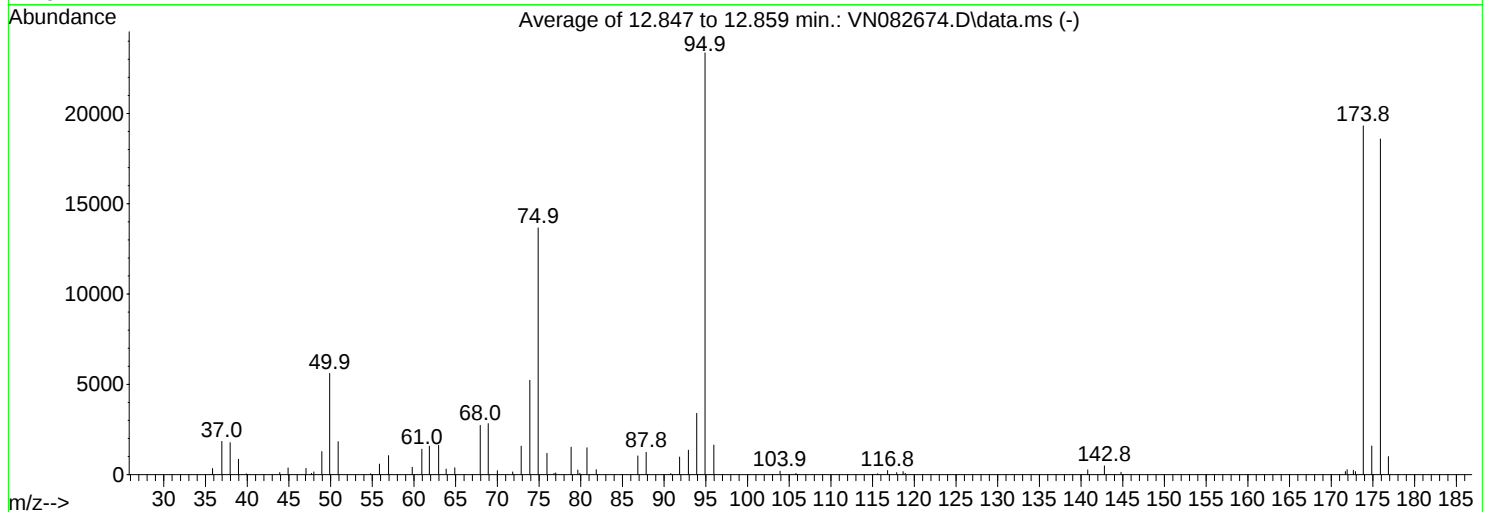


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN062124\
Data File : VN082674.D
Acq On : 21 Jun 2024 13:11
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N061724W.M
Title : SW846 8260
Last Update : Tue Jun 18 04:52:44 2024

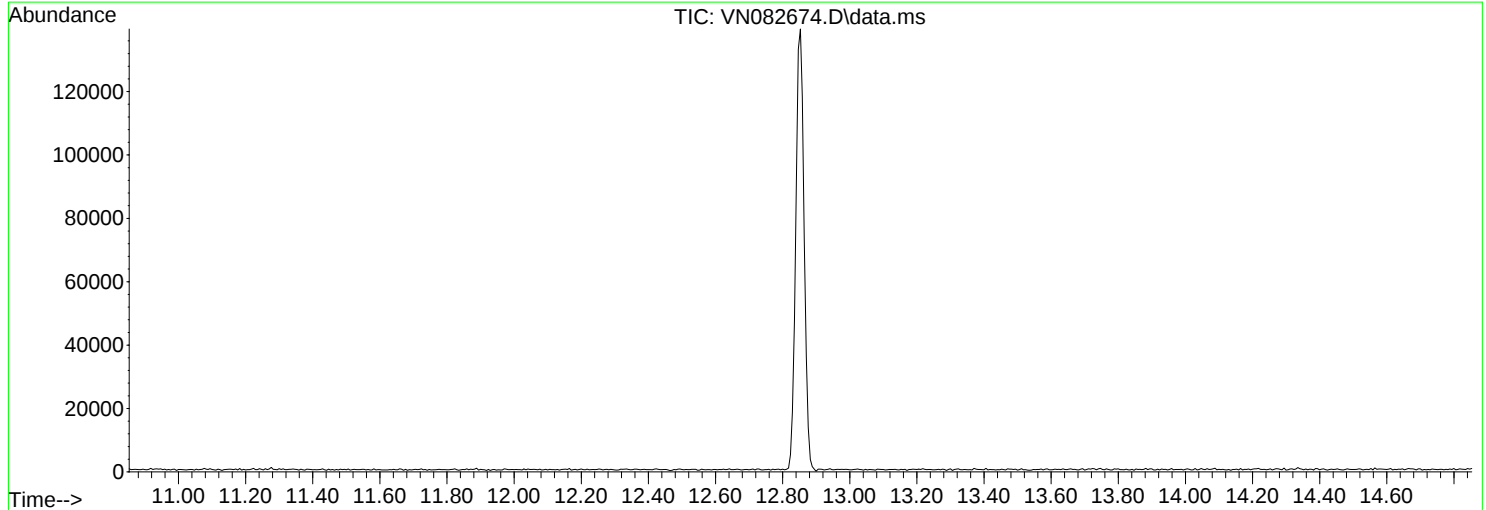

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1844

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	24.0	5607	PASS
75	95	30	60	58.5	13662	PASS
95	95	100	100	100.0	23355	PASS
96	95	5	9	7.0	1636	PASS
173	174	0.00	2	0.9	170	PASS
174	95	50	100	82.7	19317	PASS
175	174	5	9	8.2	1583	PASS
176	174	95	101	96.2	18589	PASS
177	176	5	9	5.4	1002	PASS

Average of 12.847 to 12.859 min.: VN082674.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.85	336	49.90	5607	67.95	2732	79.65	26
36.95	1840	50.90	1824	68.90	2829	79.90	8
37.95	1774	54.80	52	70.00	223	80.75	149
38.95	854	55.85	588	71.85	147	81.85	27
39.90	47	56.95	1058	72.85	1573	86.85	1034
43.90	115	59.80	406	73.90	5230	87.85	1242
44.90	373	60.95	1406	74.90	13662	90.80	64
47.05	342	61.85	1575	75.95	1182	91.85	971
47.70	73	62.95	1624	76.80	73	92.90	1359
48.00	147	63.85	312	77.00	98	93.90	3390
48.95	1277	64.90	382	78.85	1527	94.90	23355

Average of 12.847 to 12.859 min.: VN082674.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
95.95	1636	171.70	166				
103.90	198	171.90	272				
105.80	71	172.65	239				
115.60	57	172.90	170				
116.80	234	173.85	19317				
117.90	116	174.85	1583				
118.65	165	175.90	18589				
118.90	69	176.85	1002				
140.80	265						
142.80	484						
144.80	136						

Instrument :

MSVOA_N

ClientSampleId :

BFB