


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN062220\
Data File : VN061989.D
Acq On : 22 Jun 2020 9:53
Operator : JC/MD
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N061620W.M
Title : SW846 8260
Last Update : Wed Jun 17 01:19:44 2020

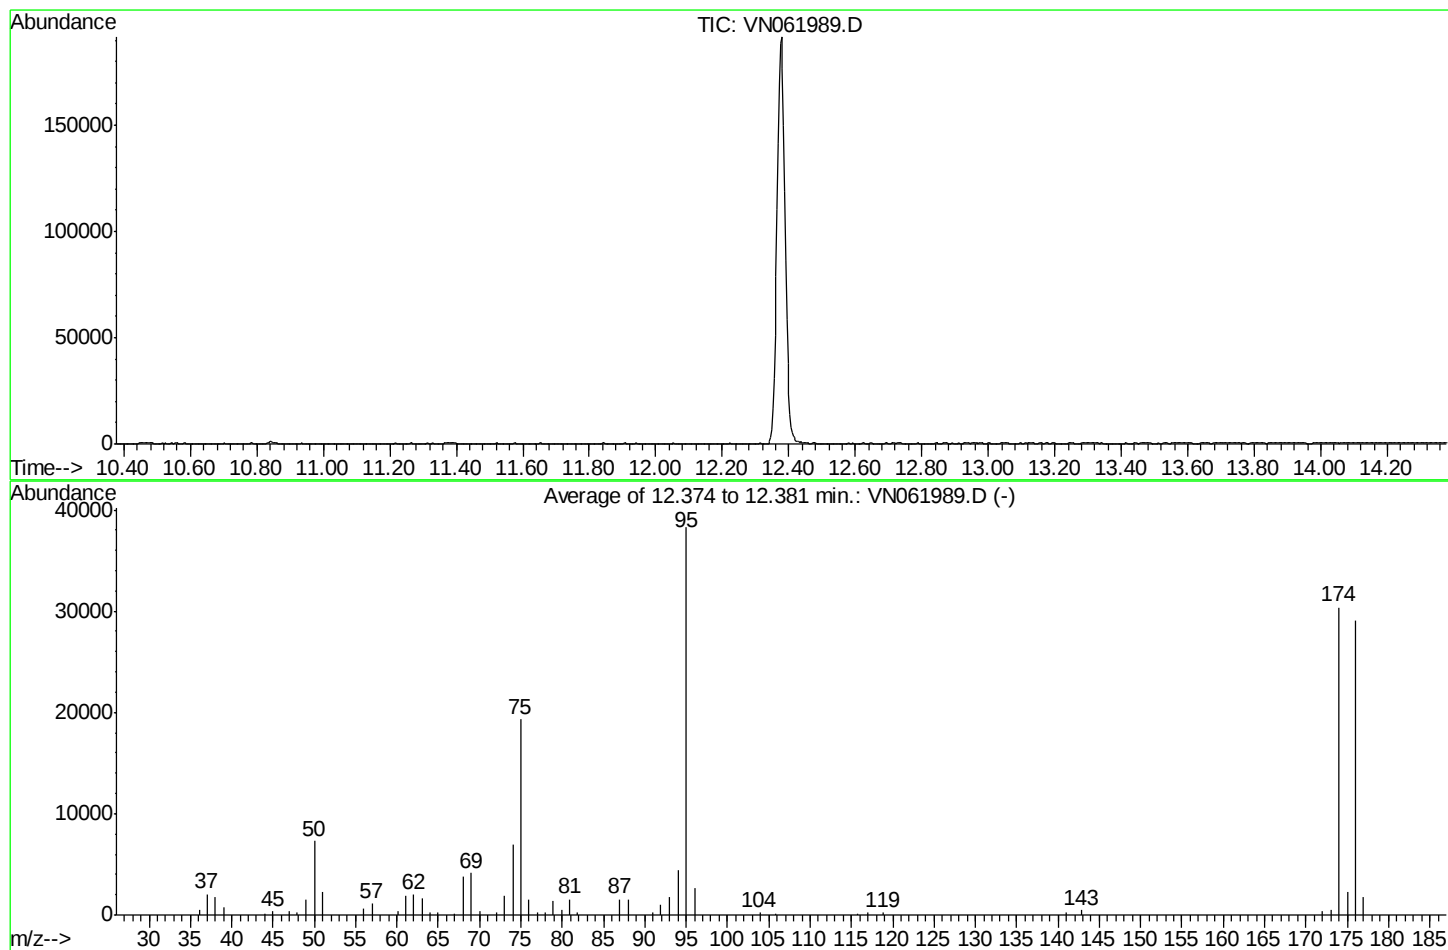

AutoFind: Scans 3297, 3298, 3299; Background Corrected with Scan 3284

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.1	7326	PASS
75	95	30	60	50.5	19320	PASS
95	95	100	100	100.0	38272	PASS
96	95	5	9	6.8	2617	PASS
173	174	0.00	2	1.5	458	PASS
174	95	50	100	79.3	30336	PASS
175	174	5	9	7.5	2279	PASS
176	174	95	101	95.8	29064	PASS
177	176	5	9	6.1	1771	PASS