

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN062222\
 Data File : VN073028.D
 Acq On : 22 Jun 2022 16:29
 Operator : JC\MD
 Sample : N3357-09DL 40X
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 MW-14DL

Quant Time: Jun 23 07:32:38 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N061722W.M
 Quant Title : SW846 8260
 QLast Update : Sat Jun 18 06:22:45 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.016	168	291100	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.904	114	477087	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.680	117	438084	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.610	152	223800	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.369	65	176812	44.926	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery =	89.860%		
35) Dibromofluoromethane	7.951	113	151335	51.320	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	102.640%		
50) Toluene-d8	10.374	98	493920	45.014	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery =	90.020%		
62) 4-Bromofluorobenzene	12.668	95	219504	55.632	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	111.260%		
Target Compounds						Qvalue
3) Chloromethane	2.275	50	438	0.715	ug/l #	43
6) Chloroethane	3.010	64	672	0.432	ug/l #	42
11) Tert butyl alcohol	5.322	59	337	0.331	ug/l #	72
16) Acetone	4.257	43	1828	0.845	ug/l #	84
18) Methyl Acetate	4.798	43	1450	0.252	ug/l #	67
20) Methylene Chloride	5.016	84	185	Below Cal	#	73
25) 2-Butanone	7.239	43	1980	0.577	ug/l #	45
26) 2,2-Dichloropropane	7.228	77	1145	Below Cal	#	53
31) Cyclohexane	8.016	56	6785	1.275	ug/l #	22
36) 1,1-Dichloropropene	8.016	75	23565	5.906	ug/l #	50
38) Carbon Tetrachloride	8.016	117	29234	6.965	ug/l #	17
39) Methylcyclohexane	9.398	83	1157	0.241	ug/l #	85
40) Benzene	8.392	78	5369	0.428	ug/l	99
52) Toluene	10.439	92	2962	0.385	ug/l	80
55) 1,1,2-Trichloroethane	10.810	97	716	0.212	ug/l #	16
67) Ethyl Benzene	11.780	91	516057	34.265	ug/l	98
68) m/p-Xylenes	11.886	106	241772	40.929	ug/l	96
69) o-Xylene	12.216	106	12711	2.153	ug/l	98
73) Isopropylbenzene	12.516	105	23770	1.373	ug/l	99
76) 1,2,3-Trichloropropane	12.668	75	115420	21.272	ug/l #	1
78) n-propylbenzene	12.857	91	108471	5.696	ug/l	97
79) 2-Chlorotoluene	12.951	91	12284	0.996	ug/l #	41
80) 1,3,5-Trimethylbenzene	12.998	105	115167	8.098	ug/l	98
81) trans-1,4-Dichloro-2-b...	12.668	75	115420	57.447	ug/l #	10
82) 4-Chlorotoluene	12.992	91	13690	1.173	ug/l #	40
83) tert-Butylbenzene	13.304	119	80424	6.175	ug/l #	61
84) 1,2,4-Trimethylbenzene	13.304	105	670708	47.349	ug/l	98
85) sec-Butylbenzene	13.304	105	670708	38.602	ug/l #	56
89) n-Butylbenzene	13.810	91	18988	1.653	ug/l #	54
90) Hexachloroethane	14.151	117	7300	2.753	ug/l #	9
95) Naphthalene	15.433	128	213667	12.359	ug/l	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN062222\
Data File : VN073028.D
Acq On : 22 Jun 2022 16:29
Operator : JC\MD
Sample : N3357-09DL 40X
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
MW-14DL

Quant Time: Jun 23 07:32:38 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N061722W.M
Quant Title : SW846 8260
QLast Update : Sat Jun 18 06:22:45 2022
Response via : Initial Calibration




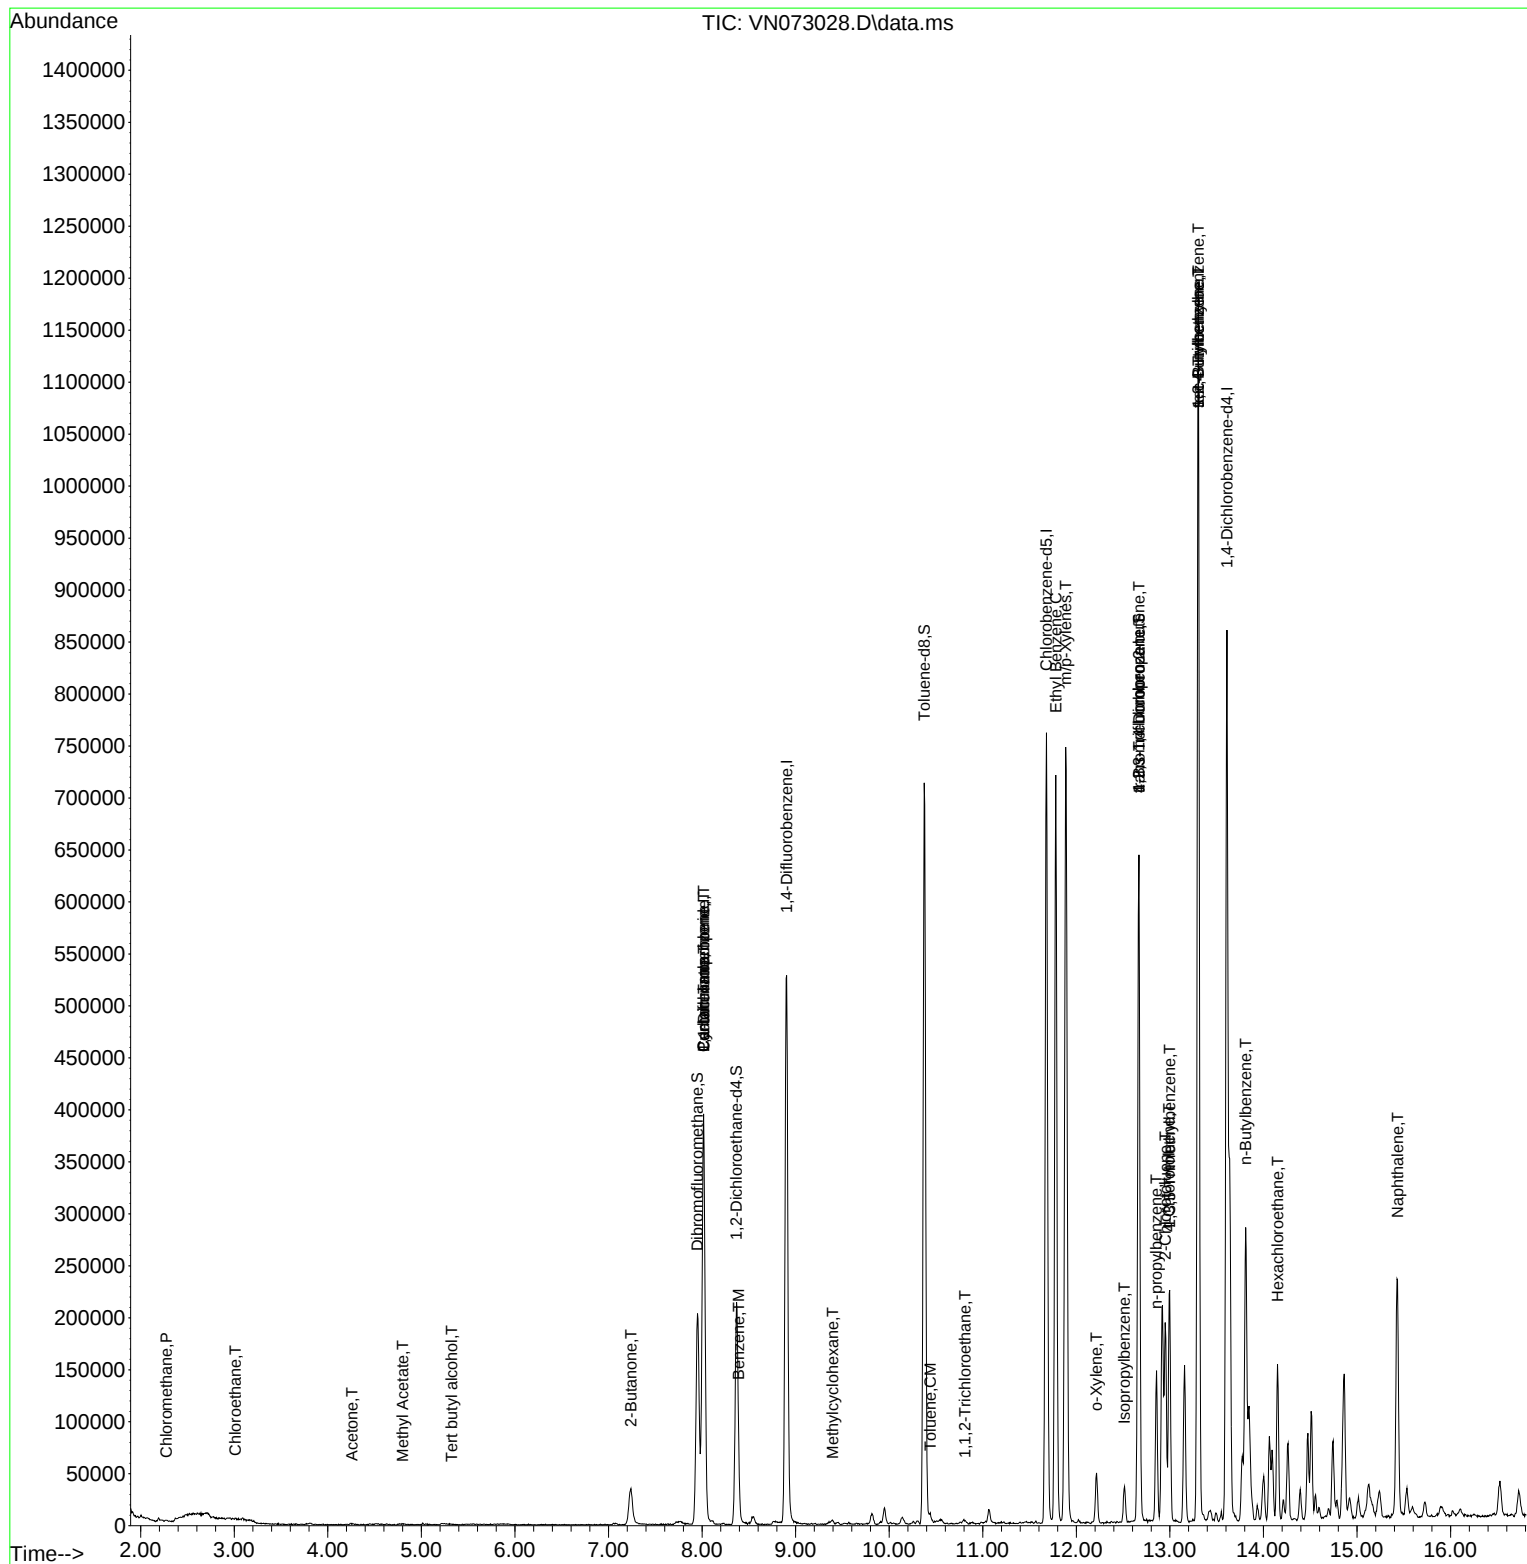




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.016 min Scan# 1042
Delta R.T. -0.000 min
Lab File: VN073028.D
Acq: 22 Jun 2022 16:29




Instrument :
MSVOA_N
ClientSampleId :
MW-14DL


Tgt Ion:168 Resp: 291100
Ion Ratio Lower Upper
168 100
99 60.9 42.3 63.5

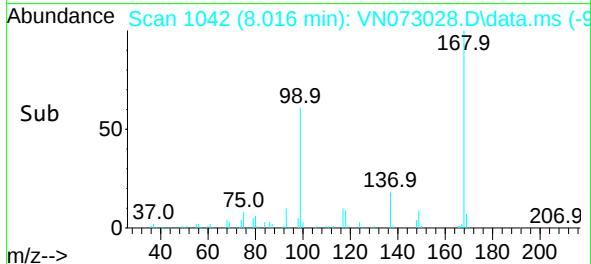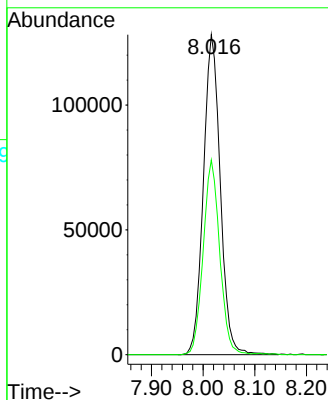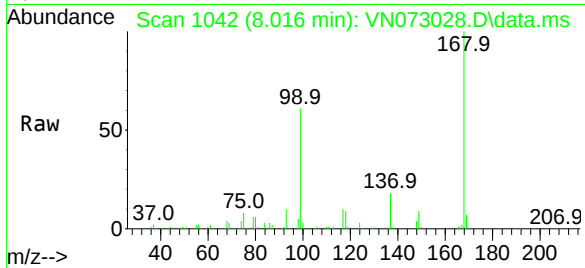

#3
Chloromethane
Concen: 0.715 ug/l
RT: 2.275 min Scan# 66
Delta R.T. 0.012 min
Lab File: VN073028.D
Acq: 22 Jun 2022 16:29

Tgt Ion: 50 Resp: 438
Ion Ratio Lower Upper
50 100
52 0.0 25.7 38.5


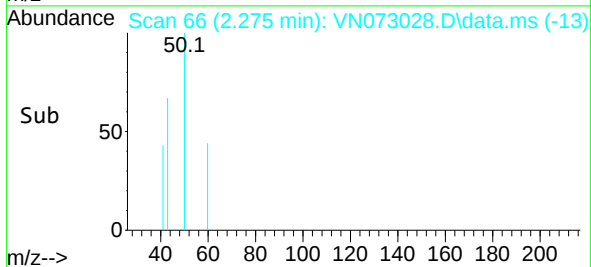
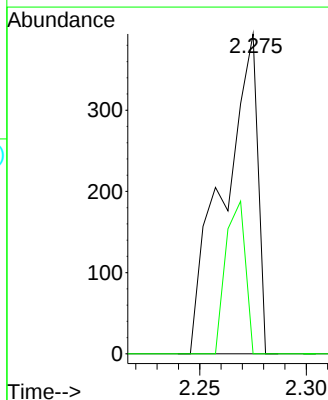
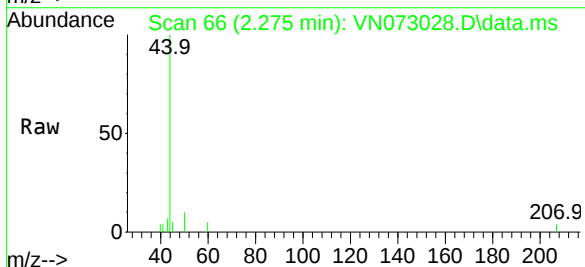


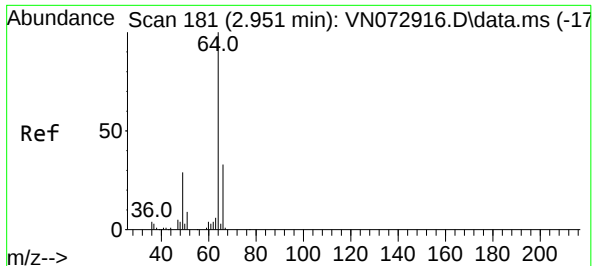

#6
Chloroethane
Concen: 0.432 ug/l
RT: 3.010 min Scan# 191
Delta R.T. 0.059 min
Lab File: VN073028.D
Acq: 22 Jun 2022 16:29




Instrument :
MSVOA_N
ClientSampleId :
MW-14DL


Tgt Ion: 64 Resp: 672
Ion Ratio Lower Upper
64 100
66 0.0 26.2 39.4#

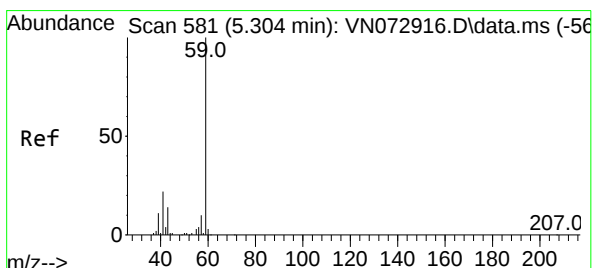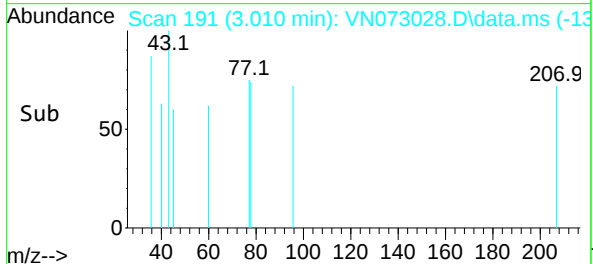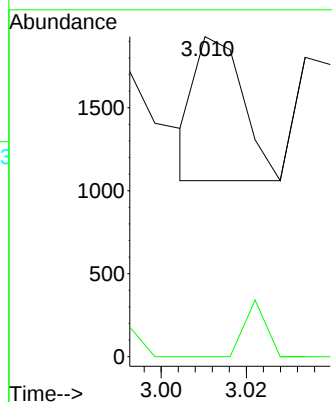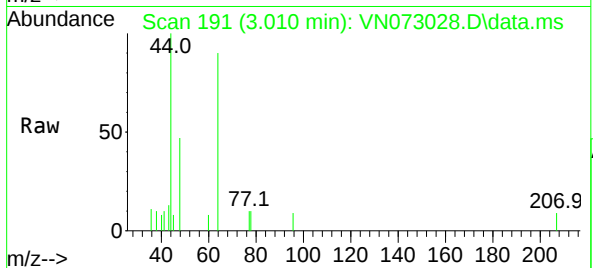

#11
Tert butyl alcohol
Concen: 0.331 ug/l
RT: 5.322 min Scan# 584
Delta R.T. 0.018 min
Lab File: VN073028.D
Acq: 22 Jun 2022 16:29

Tgt Ion: 59 Resp: 337
Ion Ratio Lower Upper
59 100
57 0.0 8.3 12.5#


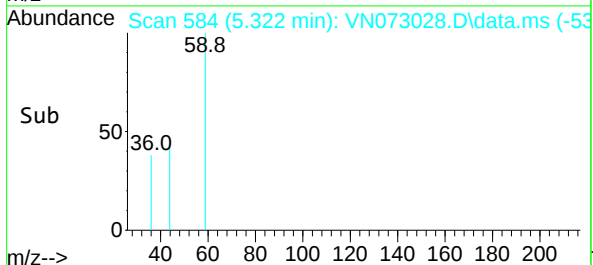

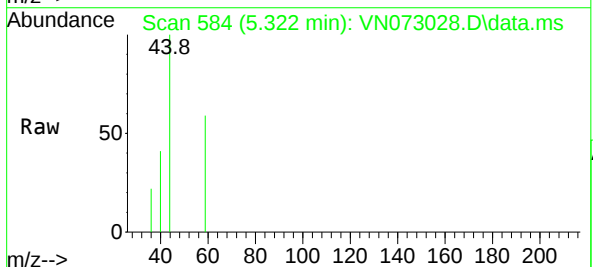


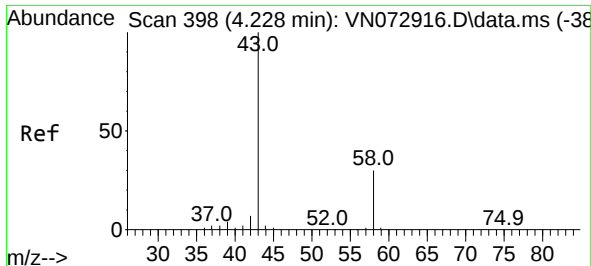

#16
Acetone
Concen: 0.845 ug/l
RT: 4.257 min Scan# 403
Delta R.T. 0.029 min
Lab File: VN073028.D
Acq: 22 Jun 2022 16:29




Instrument :
MSVOA_N
ClientSampleId :
MW-14DL


Tgt Ion: 43 Resp: 1828
Ion Ratio Lower Upper
43 100
58 23.4 26.0 39.0#

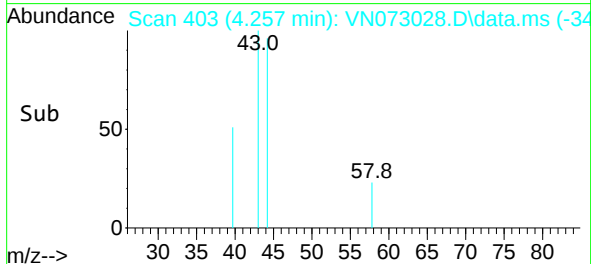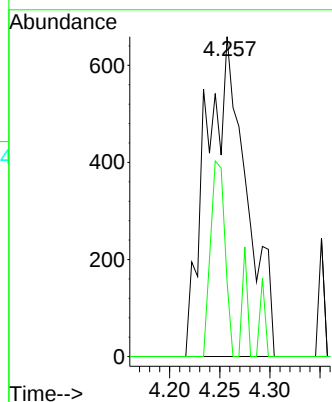

#18
Methyl Acetate
Concen: 0.252 ug/l
RT: 4.798 min Scan# 495
Delta R.T. 0.018 min
Lab File: VN073028.D
Acq: 22 Jun 2022 16:29

Tgt Ion: 43 Resp: 1450
Ion Ratio Lower Upper
43 100
74 9.8 21.6 32.4#

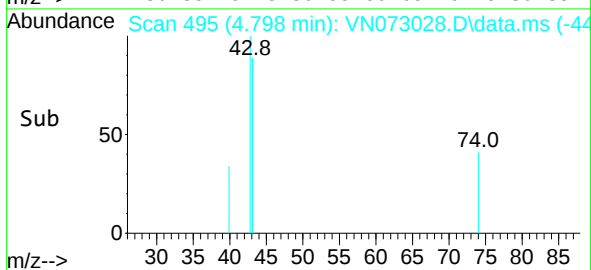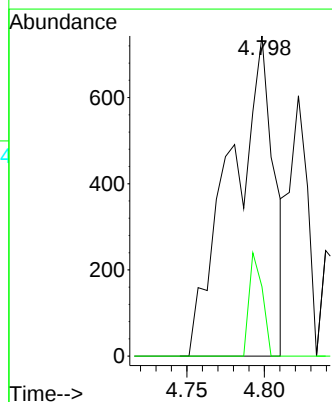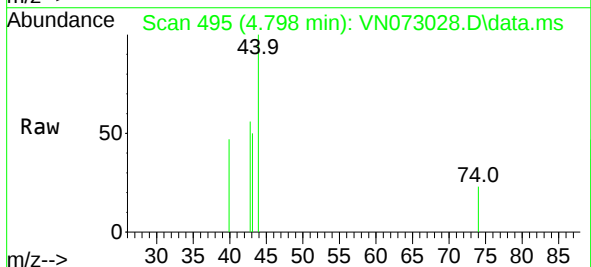

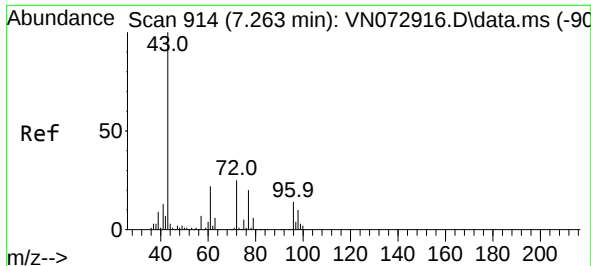

#25

2-Butanone

Concen: 0.577 ug/l

RT: 7.239 min Scan# 91

Delta R.T. -0.023 min

Lab File: VN073028.D

Acq: 22 Jun 2022 16:29

Instrument :

MSVOA_N

ClientSampleId :





MW-14DL

Tgt Ion: 43 Resp: 1980

Ion Ratio Lower Upper

43 100

72 0.0 23.7 35.5#

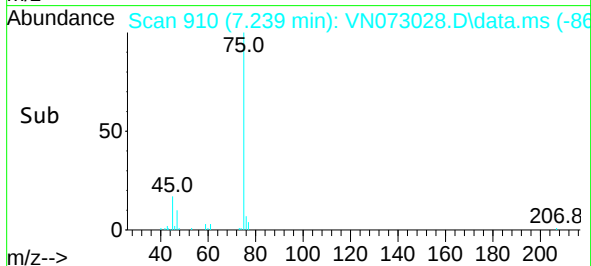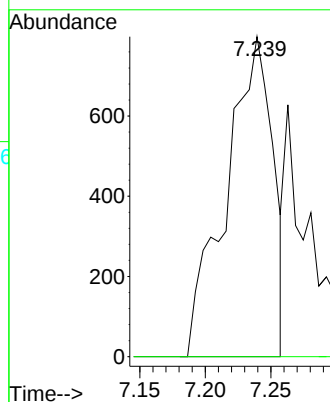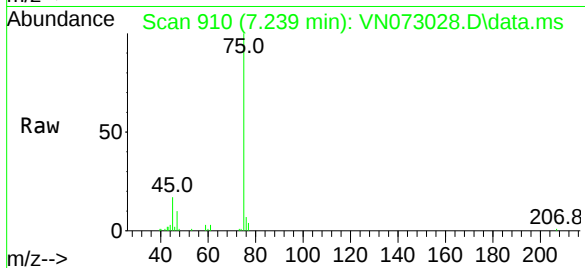

#26

2,2-Dichloropropane

Concen: Below Cal

RT: 7.228 min Scan# 908

Delta R.T. -0.023 min

Lab File: VN073028.D




Acq: 22 Jun 2022 16:29


Tgt Ion: 77 Resp: 1145

Ion Ratio Lower Upper

77 100

97 0.0 11.4 34.2#


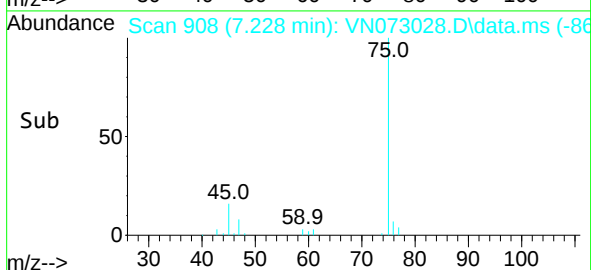
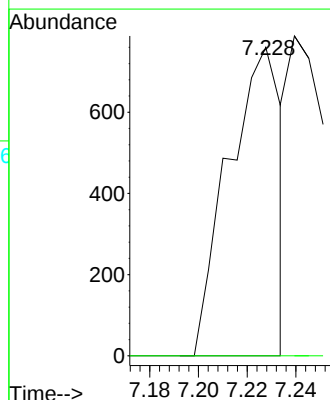
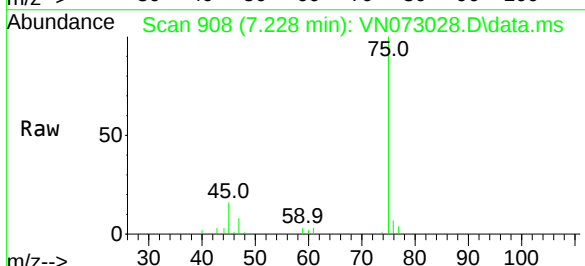


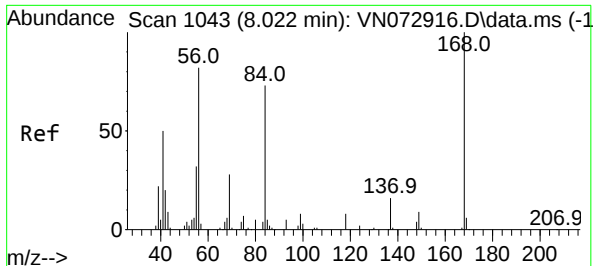

#31
Cyclohexane
Concen: 1.275 ug/l
RT: 8.016 min Scan# 1042
Delta R.T. -0.006 min
Lab File: VN073028.D
Acq: 22 Jun 2022 16:29




Instrument :
MSVOA_N
ClientSampleId :
MW-14DL


Tgt Ion: 56 Resp: 6785
Ion Ratio Lower Upper
56 100
69 137.7 27.8 41.8#
84 137.5 76.9 115.3#

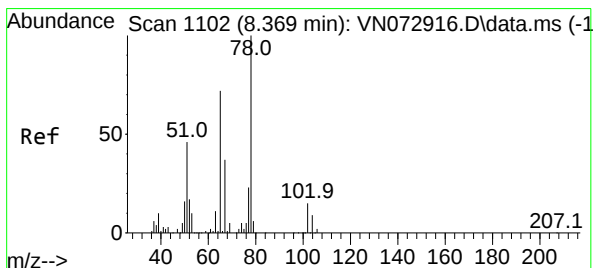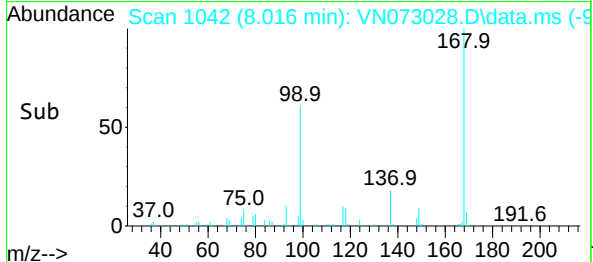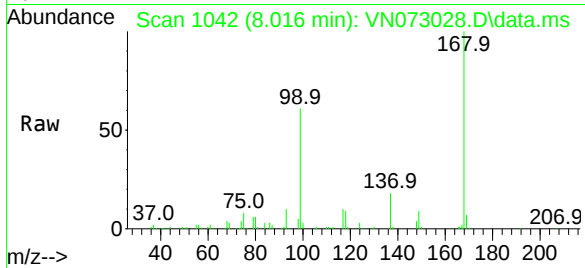

#33
1,2-Dichloroethane-d4
Concen: 44.926 ug/l
RT: 8.369 min Scan# 1102
Delta R.T. 0.000 min
Lab File: VN073028.D
Acq: 22 Jun 2022 16:29

Tgt Ion: 65 Resp: 176812
Ion Ratio Lower Upper
65 100
67 52.7 0.0 104.8

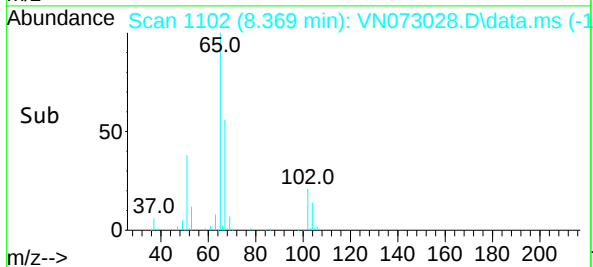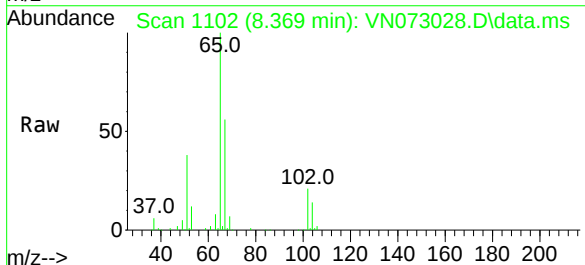

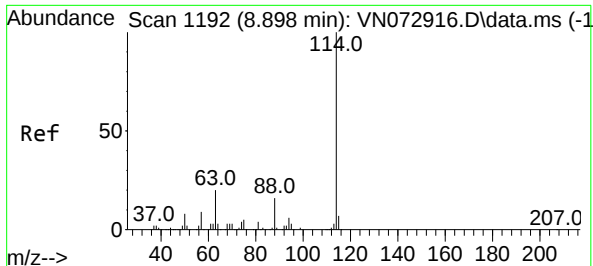

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.904 min Scan# 1192

Delta R.T. 0.006 min

Lab File: VN073028.D

Acq: 22 Jun 2022 16:29

Instrument :

MSVOA_N

ClientSampleId :

MW-14DL





Tgt Ion:114 Resp: 477087

Ion Ratio Lower Upper

114 100

63 21.2 0.0 40.0

88 16.0 0.0 32.6

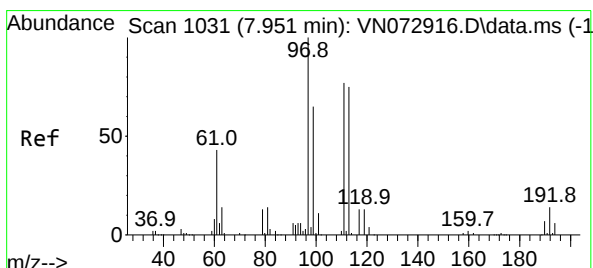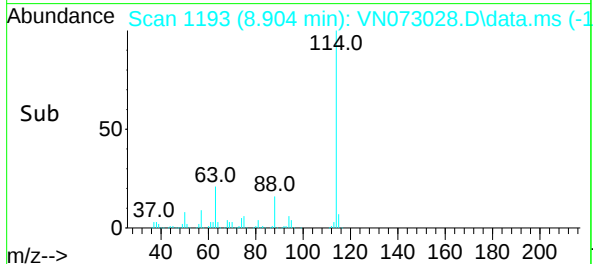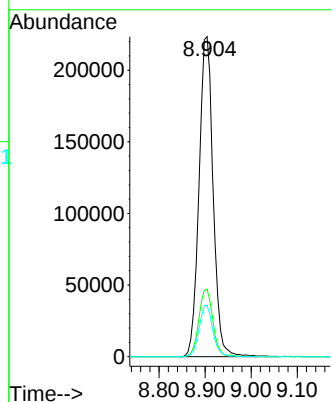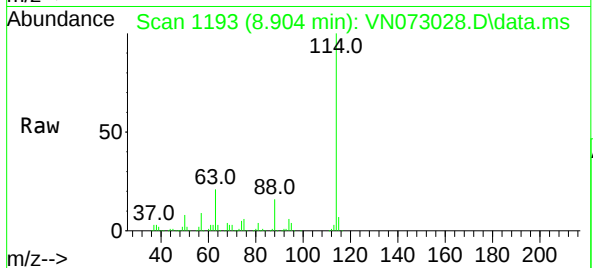

#35

Dibromofluoromethane

Concen: 51.320 ug/l

RT: 7.951 min Scan# 1031

Delta R.T. 0.000 min

Lab File: VN073028.D

Acq: 22 Jun 2022 16:29




Tgt Ion:113 Resp: 151335


Ion Ratio Lower Upper

113 100

111 102.8 81.4 122.0

192 18.3 17.0 25.6

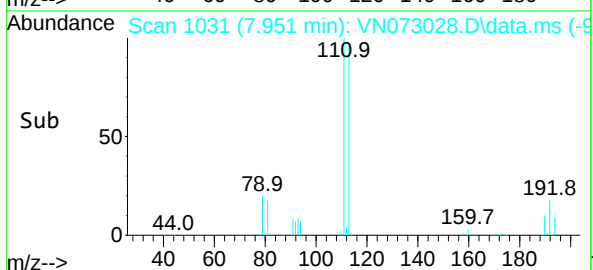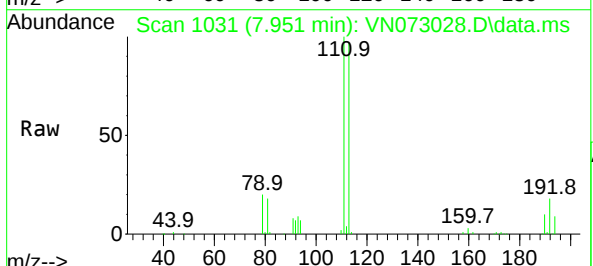

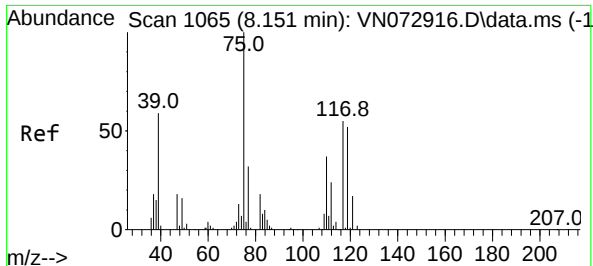

#36

1,1-Dichloropropene

Concen: 5.906 ug/l

RT: 8.016 min Scan# 1042

Delta R.T. -0.135 min

Lab File: VN073028.D

Acq: 22 Jun 2022 16:29

Instrument :

MSVOA_N

ClientSampleId :

MW-14DL





Tgt Ion: 75 Resp: 23565

Ion Ratio Lower Upper

75 100

110 10.7 18.3 54.8#

77 0.0 25.1 37.7#

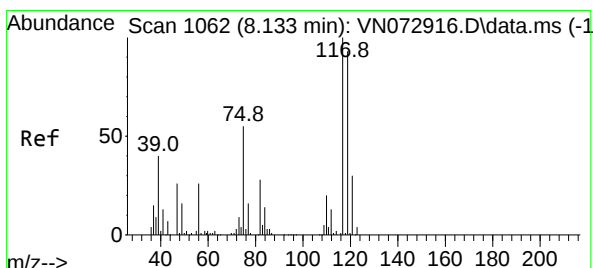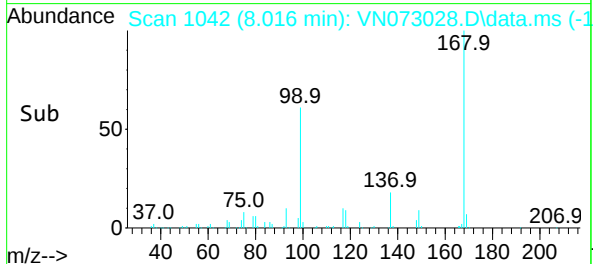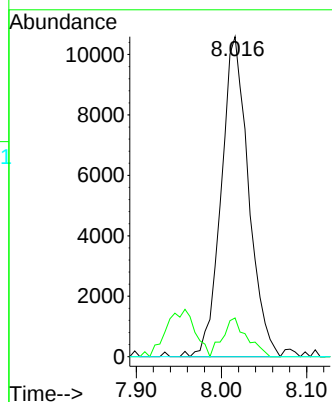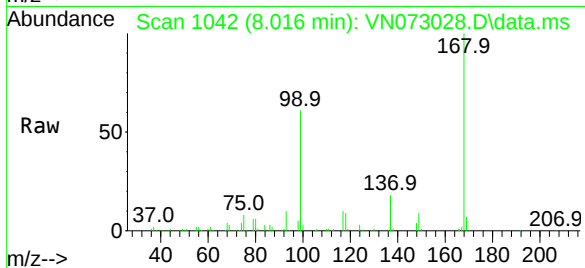

#38

Carbon Tetrachloride

Concen: 6.965 ug/l

RT: 8.016 min Scan# 1042

Delta R.T. -0.118 min

Lab File: VN073028.D

Acq: 22 Jun 2022 16:29




Tgt Ion: 117 Resp: 29234


Ion Ratio Lower Upper

117 100

119 5.5 75.8 113.8#

121 0.0 24.6 37.0#

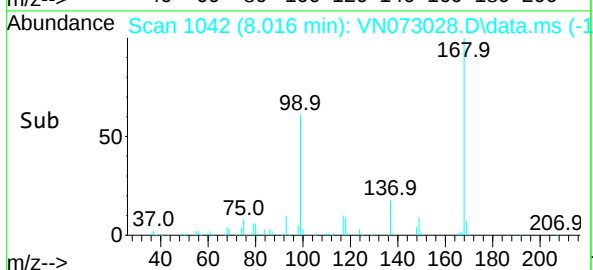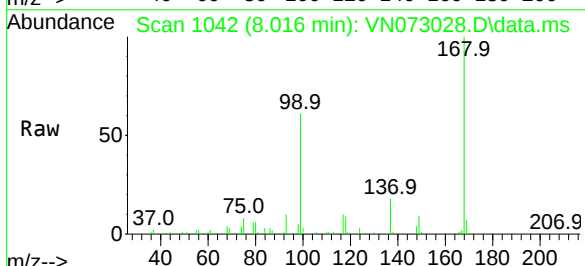

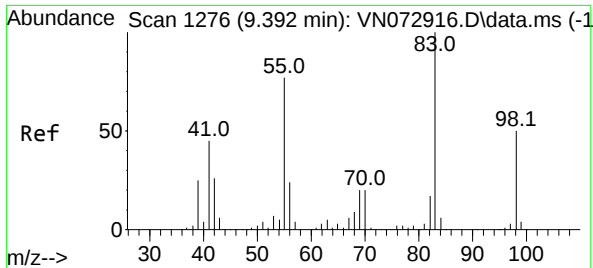

#39

Methylcyclohexane

Concen: 0.241 ug/l

RT: 9.398 min Scan# 1127

Delta R.T. 0.006 min

Lab File: VN073028.D

Acq: 22 Jun 2022 16:29

Instrument :

MSVOA_N

ClientSampleId :

MW-14DL





Tgt Ion: 83 Resp: 1157

Ion Ratio Lower Upper

83 100

55 70.5 57.8 86.8

98 26.8 39.4 59.2#

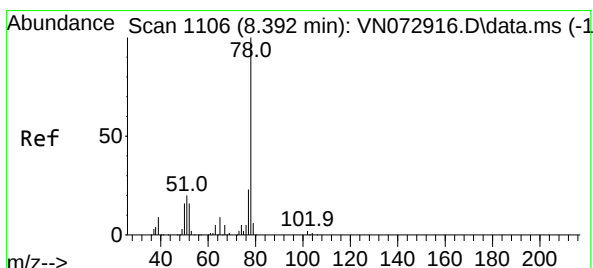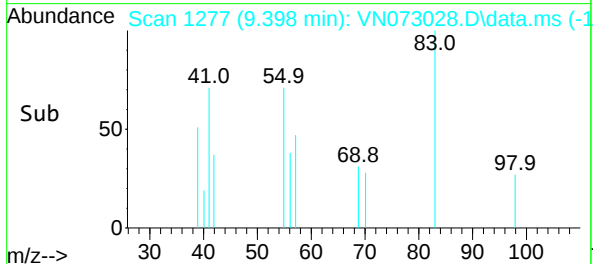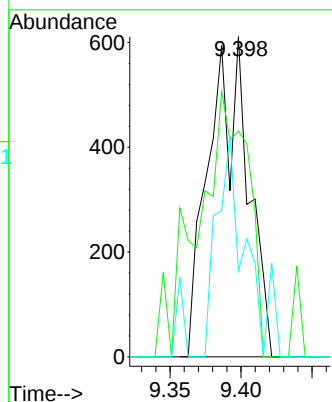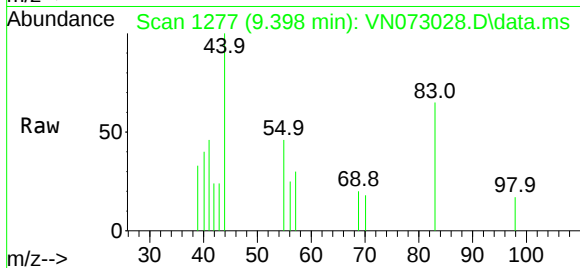

#40

Benzene

Concen: 0.428 ug/l

RT: 8.392 min Scan# 1106

Delta R.T. 0.000 min

Lab File: VN073028.D




Acq: 22 Jun 2022 16:29


Tgt Ion: 78 Resp: 5369

Ion Ratio Lower Upper

78 100

77 23.9 19.4 29.0

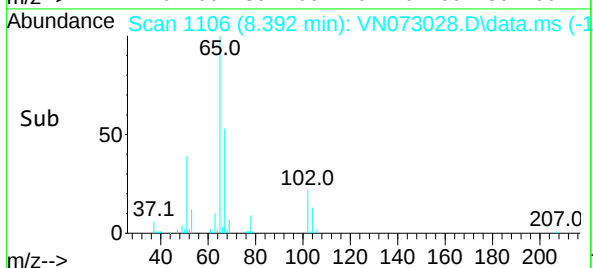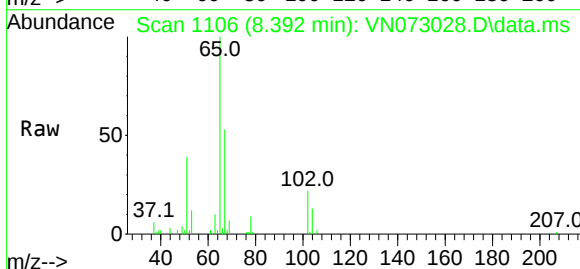



#50

Toluene-d8

Concen: 45.014 ug/l

RT: 10.374 min Scan# 1443

Delta R.T. 0.000 min

Lab File: VN073028.D

Acq: 22 Jun 2022 16:29

Instrument :

MSVOA_N

ClientSampleId :





MW-14DL

Tgt Ion: 98 Resp: 493920

Ion Ratio Lower Upper

98 100

100 66.5 52.6 78.8

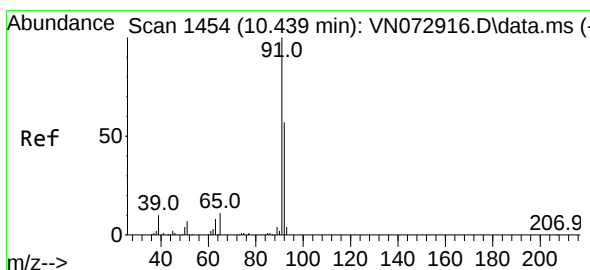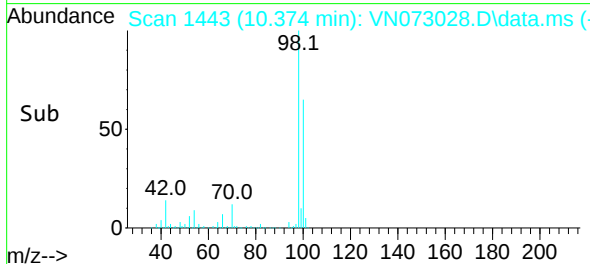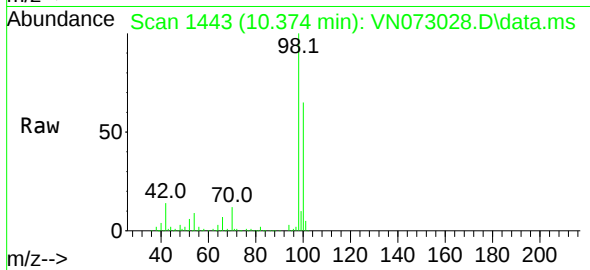

#52

Toluene

Concen: 0.385 ug/l

RT: 10.439 min Scan# 1454

Delta R.T. 0.000 min

Lab File: VN073028.D




Acq: 22 Jun 2022 16:29


Tgt Ion: 92 Resp: 2962

Ion Ratio Lower Upper

92 100

91 145.4 138.6 207.8




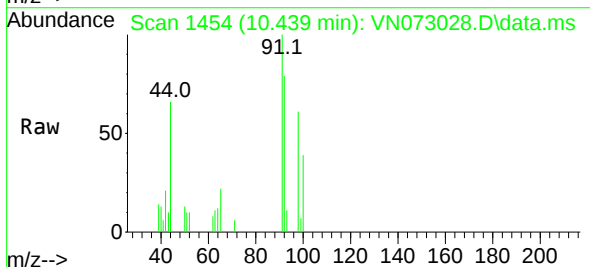


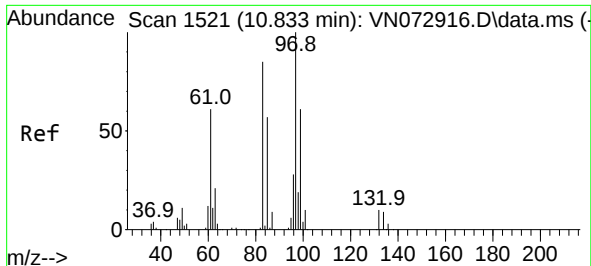

#55
1,1,2-Trichloroethane
Concen: 0.212 ug/l
RT: 10.810 min Scan# 1517
Delta R.T. -0.023 min
Lab File: VN073028.D
Acq: 22 Jun 2022 16:29




Instrument :
MSVOA_N
ClientSampleId :
MW-14DL


Tgt Ion:	97	Resp:	716
Ion	Ratio	Lower	Upper
97	100		
83	0.0	66.2	99.4#
85	0.0	43.9	65.9#
99	0.0	50.6	76.0#

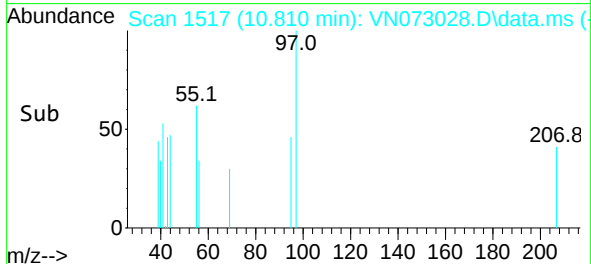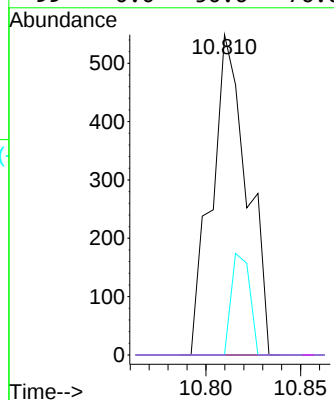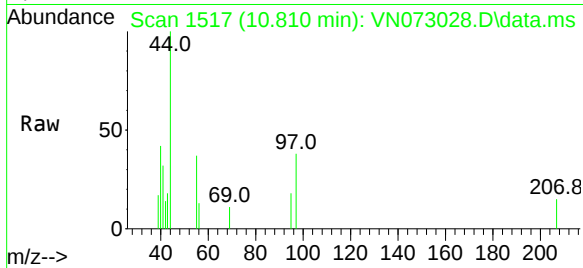

#62
4-Bromofluorobenzene
Concen: 55.632 ug/l
RT: 12.668 min Scan# 1833
Delta R.T. 0.000 min
Lab File: VN073028.D
Acq: 22 Jun 2022 16:29

Tgt Ion:	95	Resp:	219504
Ion	Ratio	Lower	Upper
95	100		
174	75.6	0.0	167.6
176	73.3	0.0	163.4


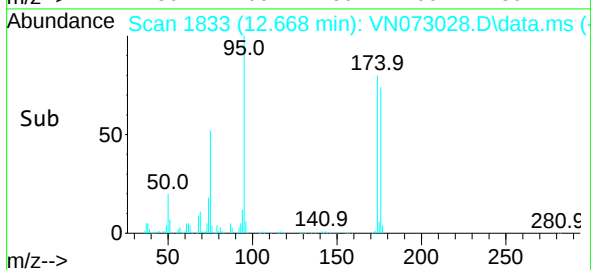
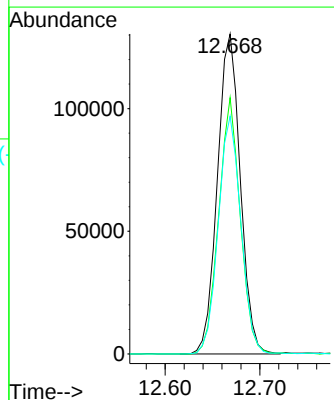
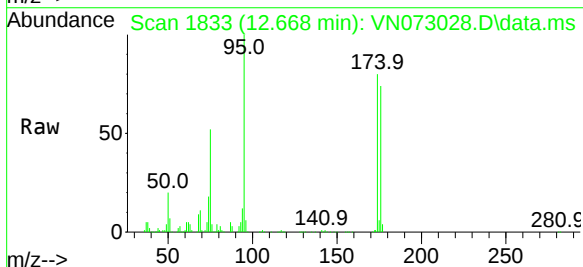




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.680 min Scan# 117
Delta R.T. 0.000 min
Lab File: VN073028.D
Acq: 22 Jun 2022 16:29




Instrument :
MSVOA_N
ClientSampleId :
MW-14DL


Tgt Ion:117 Resp: 438084
Ion Ratio Lower Upper
117 100
82 55.3 44.2 66.2
119 31.4 25.4 38.0

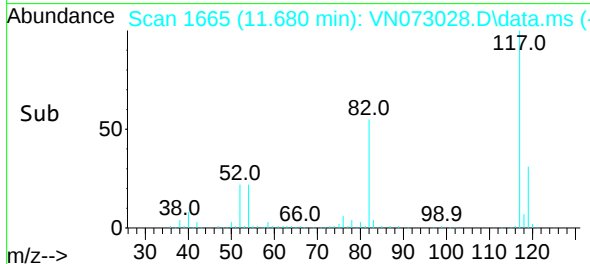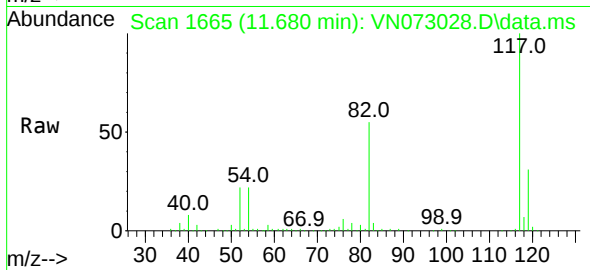

#67
Ethyl Benzene
Concen: 34.265 ug/l
RT: 11.780 min Scan# 1682
Delta R.T. 0.000 min
Lab File: VN073028.D
Acq: 22 Jun 2022 16:29

Tgt Ion: 91 Resp: 516057
Ion Ratio Lower Upper
91 100
106 30.3 24.9 37.3




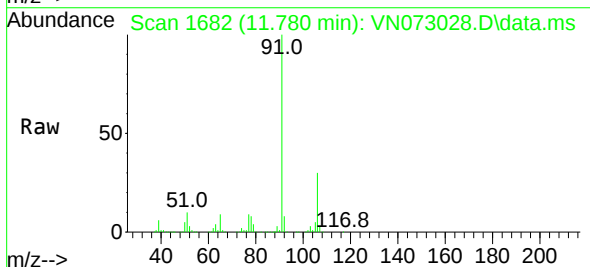


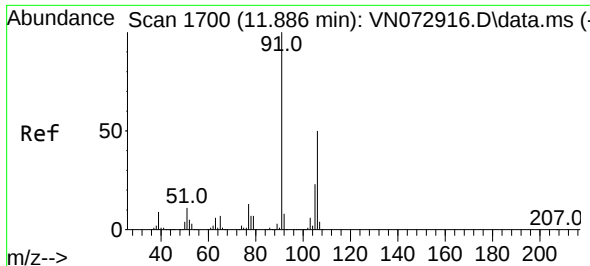

#68
m/p-Xylenes
Concen: 40.929 ug/l
RT: 11.886 min Scan# 11
Delta R.T. 0.000 min
Lab File: VN073028.D
Acq: 22 Jun 2022 16:29




Instrument :
MSVOA_N
ClientSampleId :
MW-14DL


Tgt Ion:106 Resp: 241772
Ion Ratio Lower Upper
106 100
91 204.7 158.9 238.3

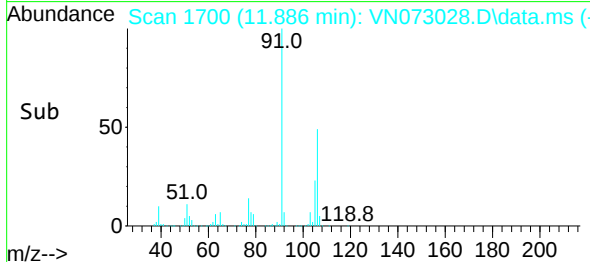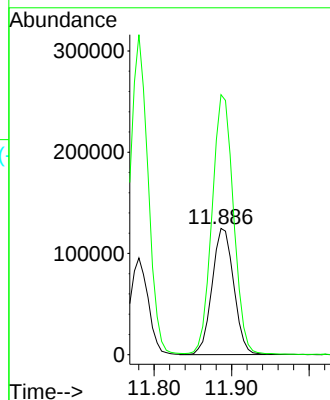

#69
o-Xylene
Concen: 2.153 ug/l
RT: 12.216 min Scan# 1756
Delta R.T. 0.000 min
Lab File: VN073028.D
Acq: 22 Jun 2022 16:29

Tgt Ion:106 Resp: 12711
Ion Ratio Lower Upper
106 100
91 215.9 106.0 318.0


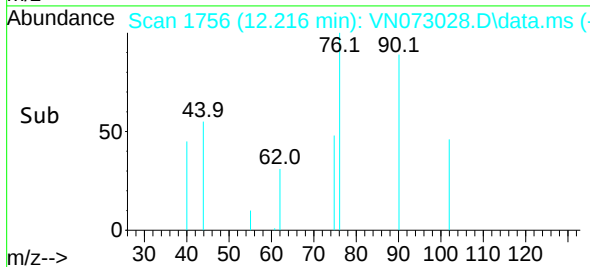
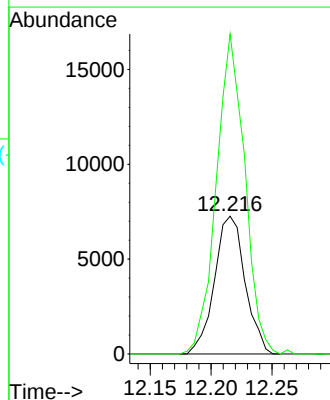
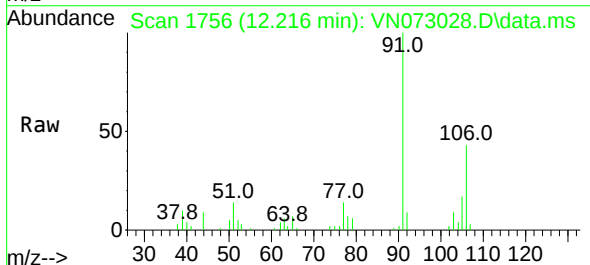




#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.610 min Scan# 1993
Delta R.T. 0.000 min
Lab File: VN073028.D
Acq: 22 Jun 2022 16:29




Instrument :
MSVOA_N
ClientSampleId :
MW-14DL


Tgt Ion:152 Resp: 223800
Ion Ratio Lower Upper
152 100
115 62.7 28.9 86.7
150 157.5 0.0 356.2

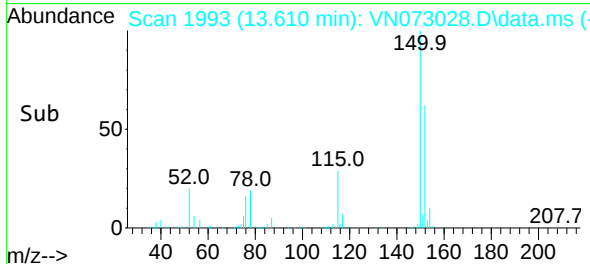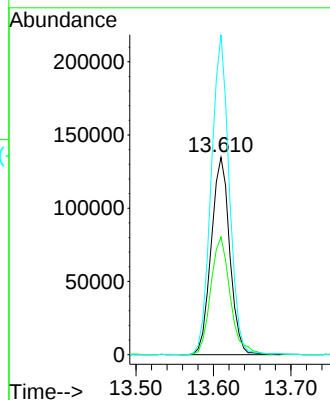

#73
Isopropylbenzene
Concen: 1.373 ug/l
RT: 12.516 min Scan# 1807
Delta R.T. 0.000 min
Lab File: VN073028.D
Acq: 22 Jun 2022 16:29

Tgt Ion:105 Resp: 23770
Ion Ratio Lower Upper
105 100
120 26.6 13.5 40.4



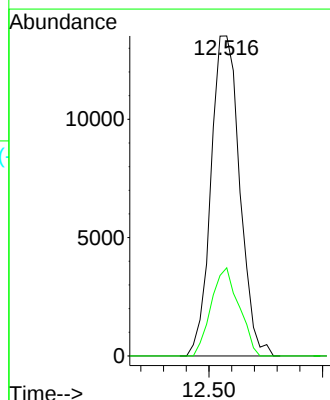
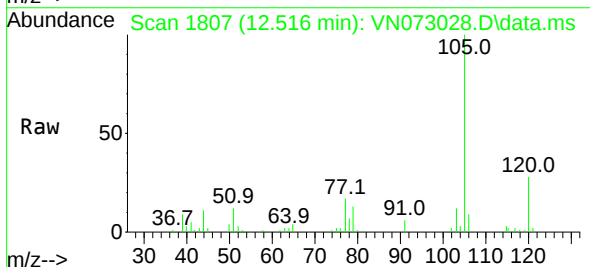


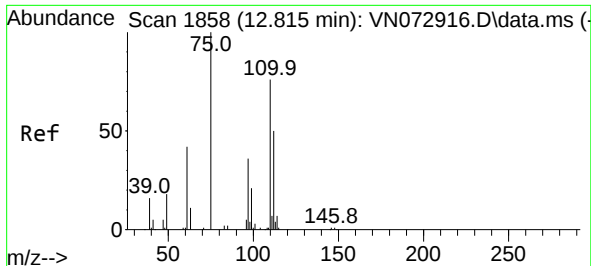

#76
1,2,3-Trichloropropane
Concen: 21.272 ug/l
RT: 12.668 min Scan# 1833
Delta R.T. -0.147 min
Lab File: VN073028.D
Acq: 22 Jun 2022 16:29




Instrument :
MSVOA_N
ClientSampleId :
MW-14DL


Tgt Ion: 75 Resp: 115420
Ion Ratio Lower Upper
75 100
77 1.1 98.5 295.5#

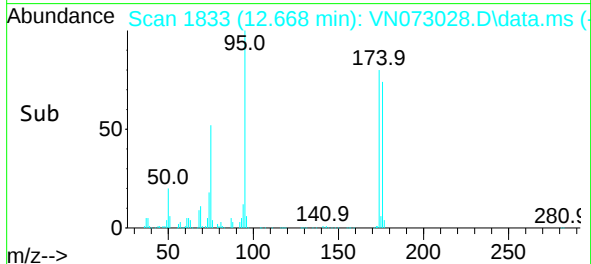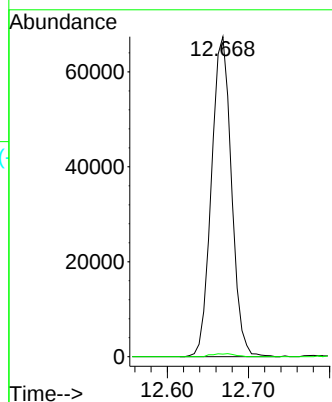

#78
n-propylbenzene
Concen: 5.696 ug/l
RT: 12.857 min Scan# 1865
Delta R.T. 0.000 min
Lab File: VN073028.D
Acq: 22 Jun 2022 16:29

Tgt Ion: 91 Resp: 108471
Ion Ratio Lower Upper
91 100
120 22.0 11.9 35.5

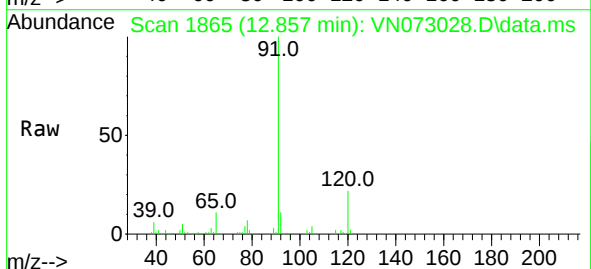



#79

2-Chlorotoluene

Concen: 0.996 ug/l

RT: 12.951 min Scan# 1881

Delta R.T. 0.006 min

Lab File: VN073028.D

Acq: 22 Jun 2022 16:29

Instrument :

MSVOA_N

ClientSampleId :





MW-14DL

Tgt Ion: 91 Resp: 12284

Ion Ratio Lower Upper

91 100

126 0.7 17.3 51.9#

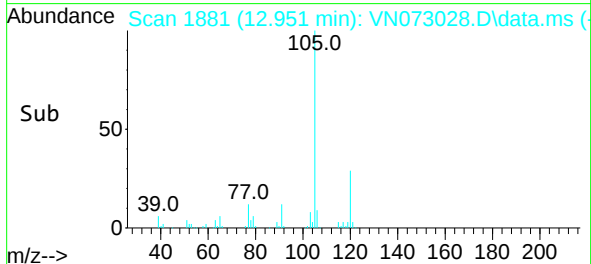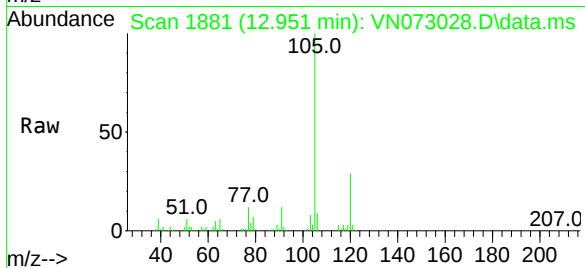

#80

1,3,5-Trimethylbenzene

Concen: 8.098 ug/l

RT: 12.998 min Scan# 1889

Delta R.T. 0.000 min

Lab File: VN073028.D




Acq: 22 Jun 2022 16:29


Tgt Ion: 105 Resp: 115167

Ion Ratio Lower Upper

105 100

120 48.4 24.9 74.7


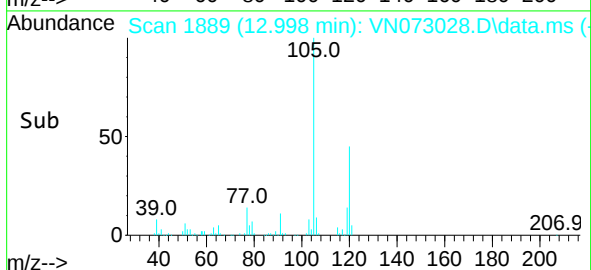

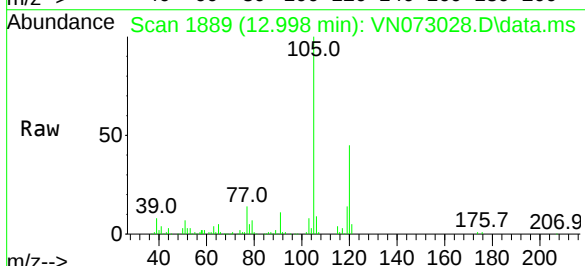


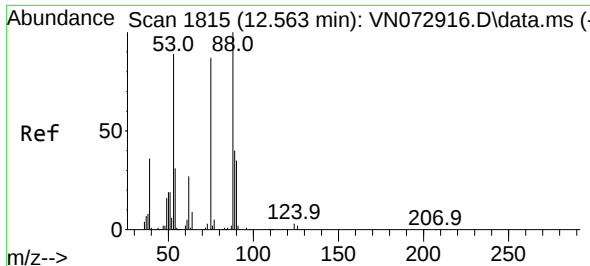

#81
trans-1,4-Dichloro-2-butene
Concen: 57.447 ug/l
RT: 12.668 min Scan# 1833
Delta R.T. 0.106 min
Lab File: VN073028.D
Acq: 22 Jun 2022 16:29




Instrument :
MSVOA_N
ClientSampleId :
MW-14DL


Tgt Ion: 75 Resp: 115420
Ion Ratio Lower Upper
75 100
53 0.0 78.0 117.0#
89 0.0 37.2 55.8#

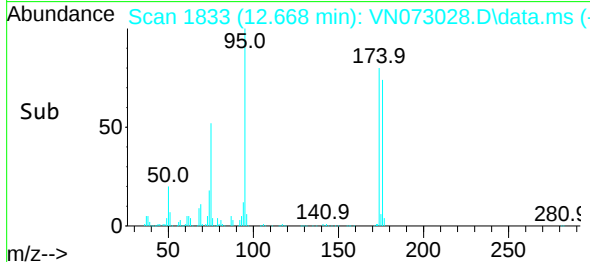

#82
4-Chlorotoluene
Concen: 1.173 ug/l
RT: 12.992 min Scan# 1888
Delta R.T. -0.047 min
Lab File: VN073028.D
Acq: 22 Jun 2022 16:29

Tgt Ion: 91 Resp: 13690
Ion Ratio Lower Upper
91 100
126 0.0 17.2 51.6#

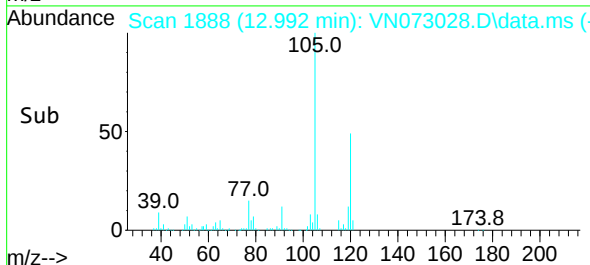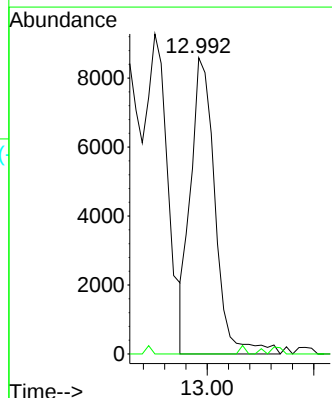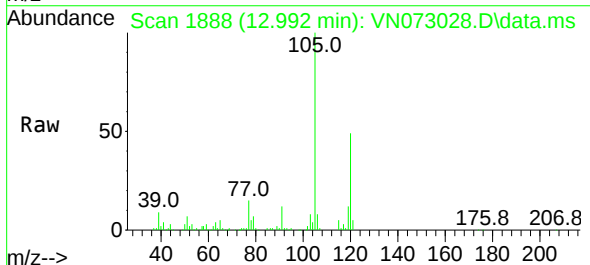



#83

tert-Butylbenzene

Concen: 6.175 ug/l

RT: 13.304 min Scan# 1941

Delta R.T. 0.047 min

Lab File: VN073028.D

Acq: 22 Jun 2022 16:29

Instrument :

MSVOA_N

ClientSampleId :

MW-14DL





Tgt Ion:119 Resp: 80424

Ion Ratio Lower Upper

119 100

91 88.9 31.6 94.8

134 0.0 13.7 41.1#

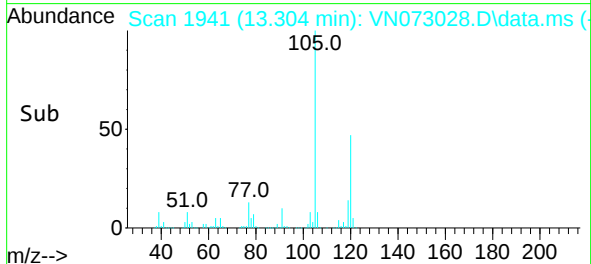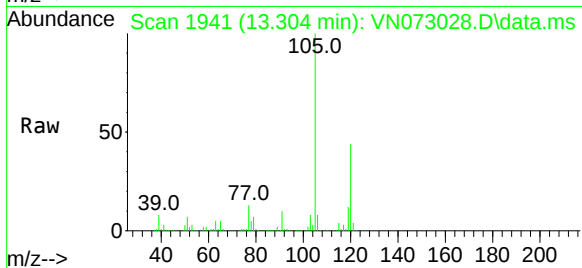

#84

1,2,4-Trimethylbenzene

Concen: 47.349 ug/l

RT: 13.304 min Scan# 1941

Delta R.T. 0.000 min

Lab File: VN073028.D




Acq: 22 Jun 2022 16:29


Tgt Ion:105 Resp: 670708

Ion Ratio Lower Upper

105 100

120 45.2 23.3 69.8


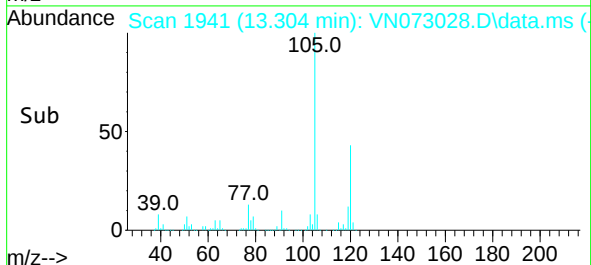

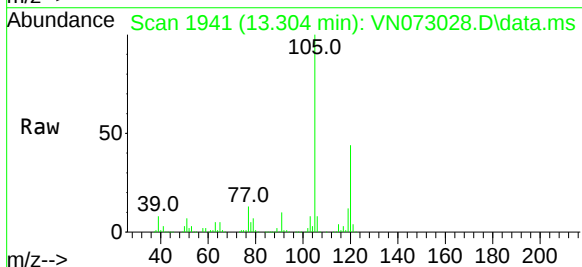




#85
 sec-Butylbenzene
 Concen: 38.602 ug/l
 RT: 13.304 min Scan# 1964
 Delta R.T. -0.135 min
 Lab File: VN073028.D
 Acq: 22 Jun 2022 16:29




Instrument :
 MSVOA_N
 ClientSampleId :
 MW-14DL


Tgt Ion:105 Resp: 670708
 Ion Ratio Lower Upper
 105 100
 134 0.0 10.4 31.1#

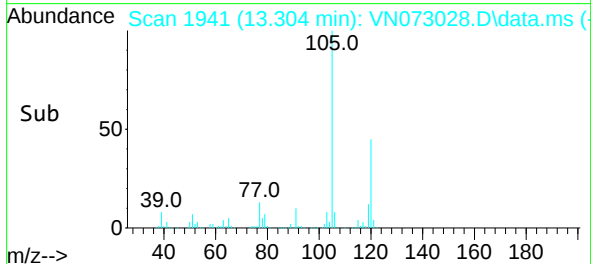

#89
 n-Butylbenzene
 Concen: 1.653 ug/l
 RT: 13.810 min Scan# 2027
 Delta R.T. -0.065 min
 Lab File: VN073028.D
 Acq: 22 Jun 2022 16:29

Tgt Ion: 91 Resp: 18988
 Ion Ratio Lower Upper
 91 100
 92 23.0 26.9 80.7#
 134 0.0 13.6 40.8#

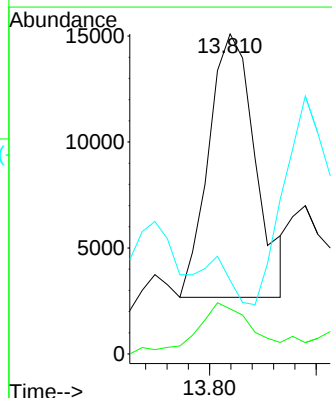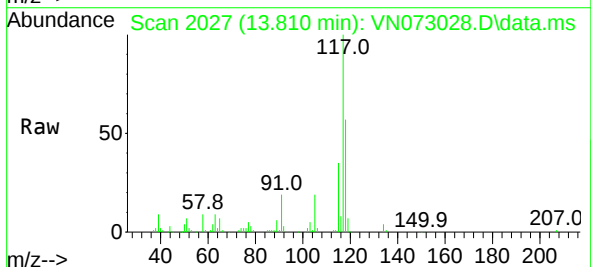



#90

Hexachloroethane

Concen: 2.753 ug/l

RT: 14.151 min Scan# 2084

Delta R.T. 0.006 min

Lab File: VN073028.D

Acq: 22 Jun 2022 16:29

Instrument :

MSVOA_N

ClientSampleId :





MW-14DL

Tgt Ion:117 Resp: 7300

Ion Ratio Lower Upper

117 100

201 0.0 40.6 122.0#

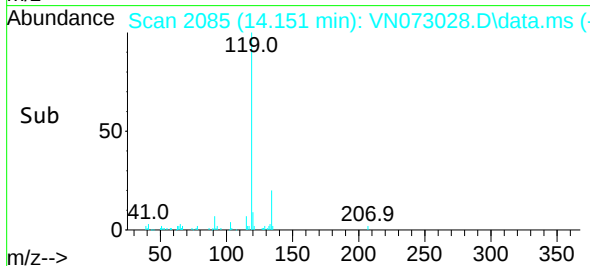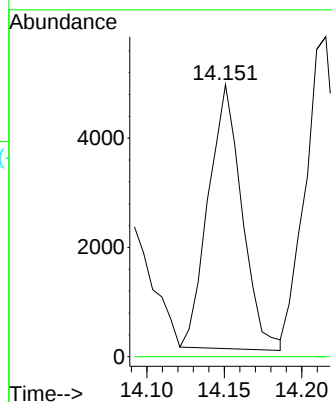

#95

Naphthalene

Concen: 12.359 ug/l

RT: 15.433 min Scan# 2303

Delta R.T. 0.006 min

Lab File: VN073028.D

Acq: 22 Jun 2022 16:29

Tgt Ion:128 Resp: 213667

Ion Ratio Lower Upper

128 100

127 13.0 10.3 15.5

129 11.1 8.6 13.0

