

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN062222\
 Data File : VN073033.D
 Acq On : 22 Jun 2022 18:31
 Operator : JC\MD
 Sample : N3381-06 50X
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 MW-7

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N061722W.M
 Title : SW846 8260

Signal : TIC: VN073033.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.404	83	88	93	rVB	23353	35682	1.62%	0.290%
2	3.087	196	204	213	rVB3	28931	61728	2.81%	0.502%
3	3.457	258	267	277	rVB4	11342	30381	1.38%	0.247%
4	3.663	293	302	310	rVB2	11147	25593	1.16%	0.208%
5	3.934	338	348	358	rBV3	16738	42211	1.92%	0.343%
6	4.881	501	509	521	rVB2	8271	25923	1.18%	0.211%
7	5.104	537	547	555	rBV2	8794	26808	1.22%	0.218%
8	7.063	871	880	889	rBV4	8529	25706	1.17%	0.209%
9	7.239	899	910	919	rBV	28405	78524	3.57%	0.639%
10	7.951	1021	1031	1036	rBV	193373	466198	21.19%	3.794%
11	8.016	1036	1042	1054	rVB	384690	858965	39.05%	6.990%
12	8.375	1092	1103	1114	rBV2	248940	671232	30.52%	5.462%
13	8.898	1183	1192	1210	rBV	512686	1078684	49.04%	8.778%
14	10.374	1435	1443	1450	rBV	692580	1279319	58.16%	10.410%
15	10.439	1450	1454	1461	rVB	107850	191074	8.69%	1.555%
16	11.680	1655	1665	1676	rBV	718892	1270248	57.75%	10.337%
17	11.780	1676	1682	1691	rVV	307816	505582	22.99%	4.114%
18	11.886	1691	1700	1713	rVV	1184424	2199595	100.00%	17.899%
19	12.216	1749	1756	1768	rBV	315573	529715	24.08%	4.311%
20	12.668	1825	1833	1845	rVB	591488	986078	44.83%	8.024%
21	12.915	1869	1875	1879	rBV	63996	109589	4.98%	0.892%
22	12.992	1884	1888	1894	rVB2	28954	47446	2.16%	0.386%
23	13.157	1911	1916	1924	rVB	41262	65752	2.99%	0.535%
24	13.304	1935	1941	1948	rBV	97712	156134	7.10%	1.271%
25	13.610	1983	1993	2007	rBV	728433	1292208	58.75%	10.515%
26	13.810	2019	2027	2040	rVB	60653	106990	4.86%	0.871%
27	15.433	2295	2303	2311	rVB	58854	121501	5.52%	0.989%




Sum of corrected areas: 12288866

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN062222\
Data File : VN073033.D
Acq On : 22 Jun 2022 18:31
Operator : JC\MD
Sample : N3381-06 50X
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
MW-7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N061722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

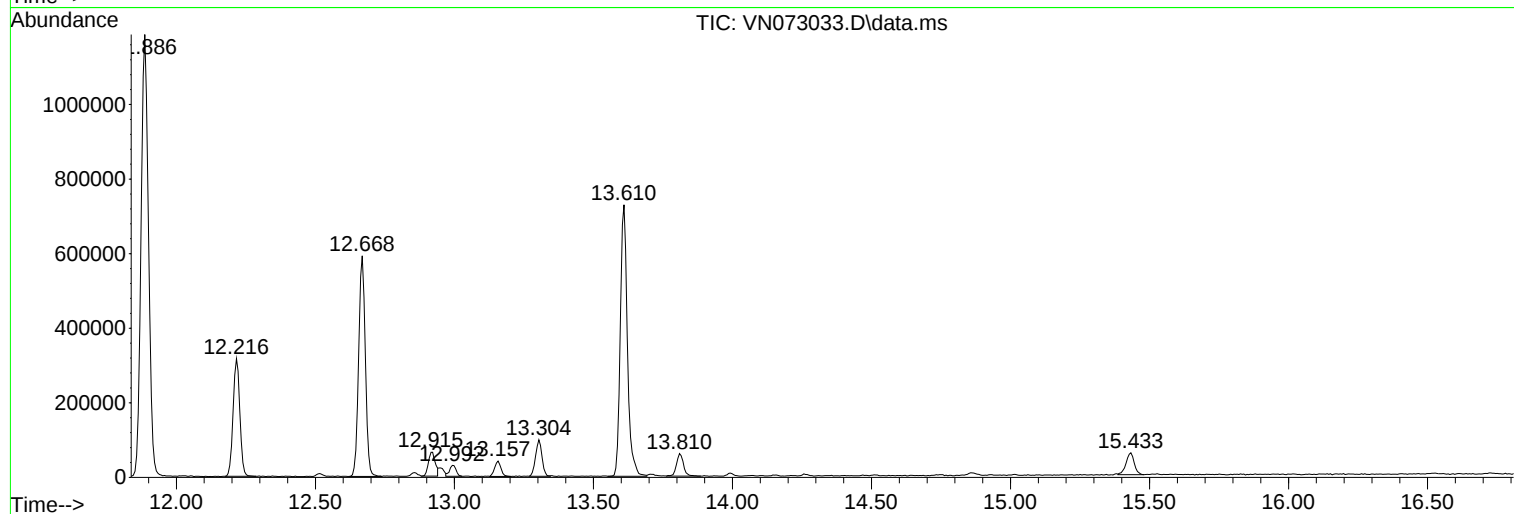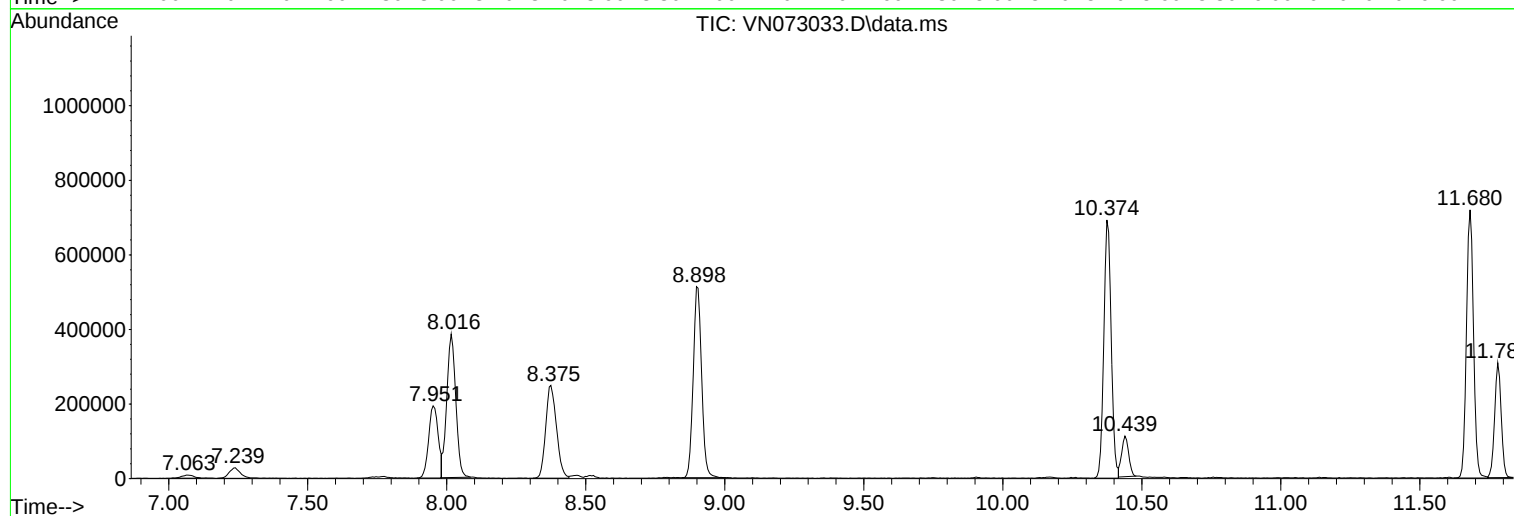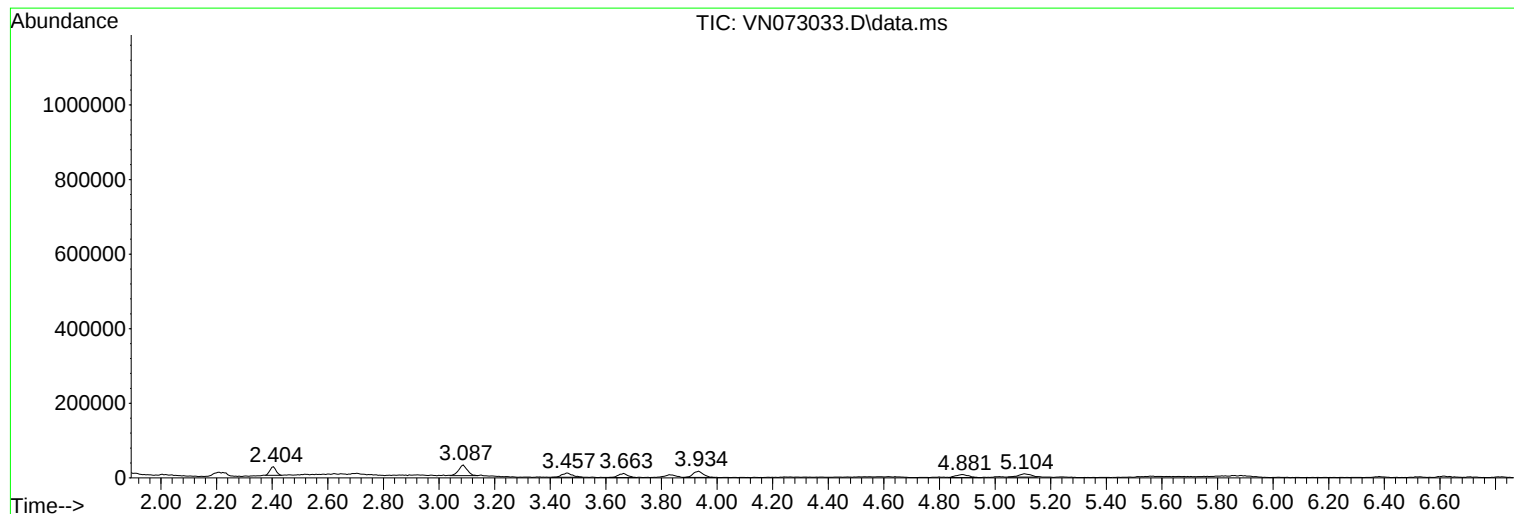

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN062222\
Data File : VN073033.D
Acq On : 22 Jun 2022 18:31
Operator : JC\MD
Sample : N3381-06 50X
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
MW-7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N061722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN062222\
Data File : VN073033.D
Acq On : 22 Jun 2022 18:31
Operator : JC\MD
Sample : N3381-06 50X
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
MW-7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N061722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------