
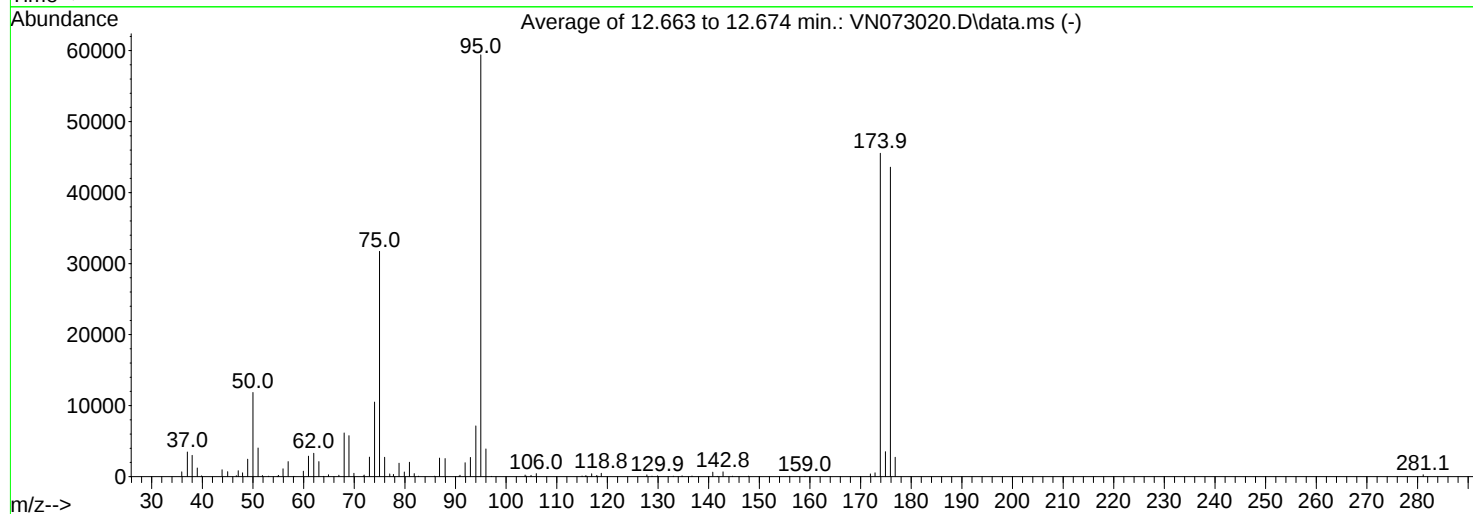


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN062222\
Data File : VN073020.D
Acq On : 22 Jun 2022 11:52
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N061722W.M
Title : SW846 8260
Last Update : Sat Jun 18 06:22:45 2022

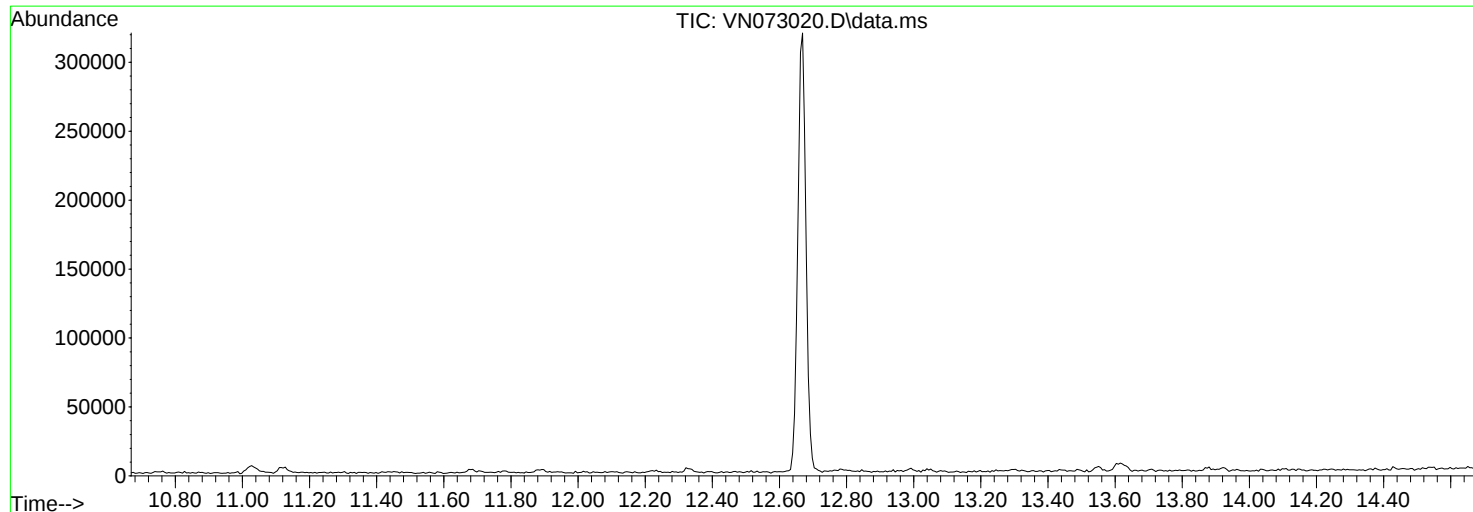

AutoFind: Scans 1832, 1833, 1834; Background Corrected with Scan 1823

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.0	11853	PASS
75	95	30	60	53.4	31725	PASS
95	95	100	100	100.0	59403	PASS
96	95	5	9	6.6	3905	PASS
173	174	0.00	2	1.2	532	PASS
174	95	50	100	76.7	45539	PASS
175	174	5	9	7.7	3508	PASS
176	174	95	101	95.7	43589	PASS
177	176	5	9	6.3	2737	PASS