
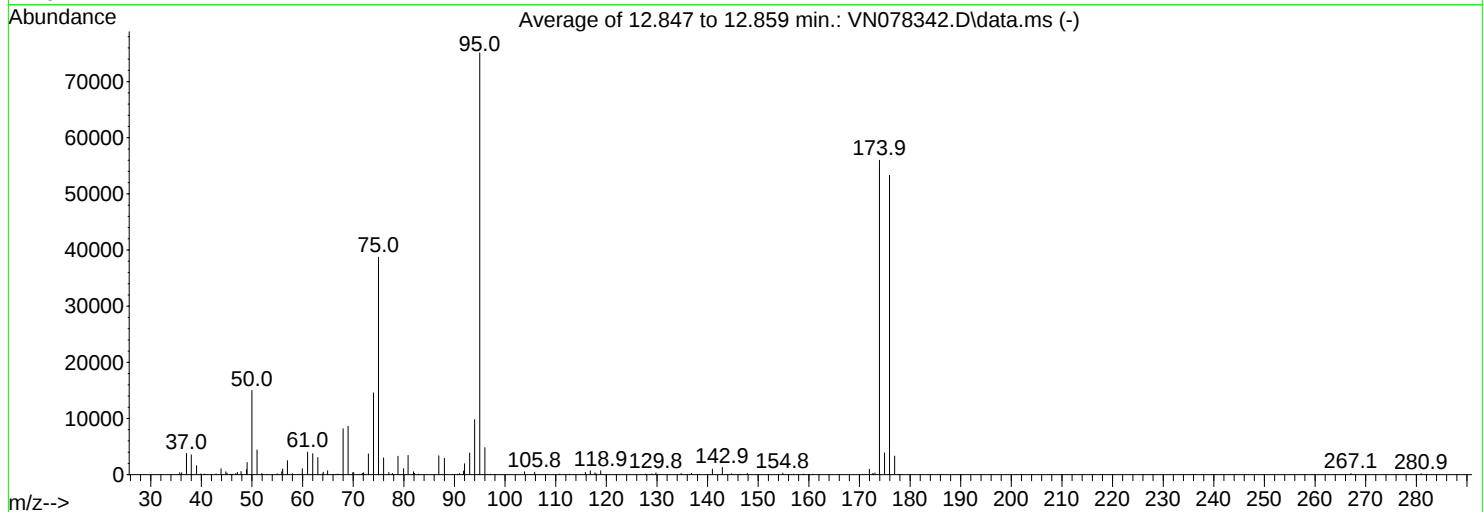


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN062223\
 Data File : VN078342.D
 Acq On : 22 Jun 2023 09:40
 Operator : JC\MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N060623W.M
 Title : SW846 8260
 Last Update : Wed Jun 07 05:05:00 2023

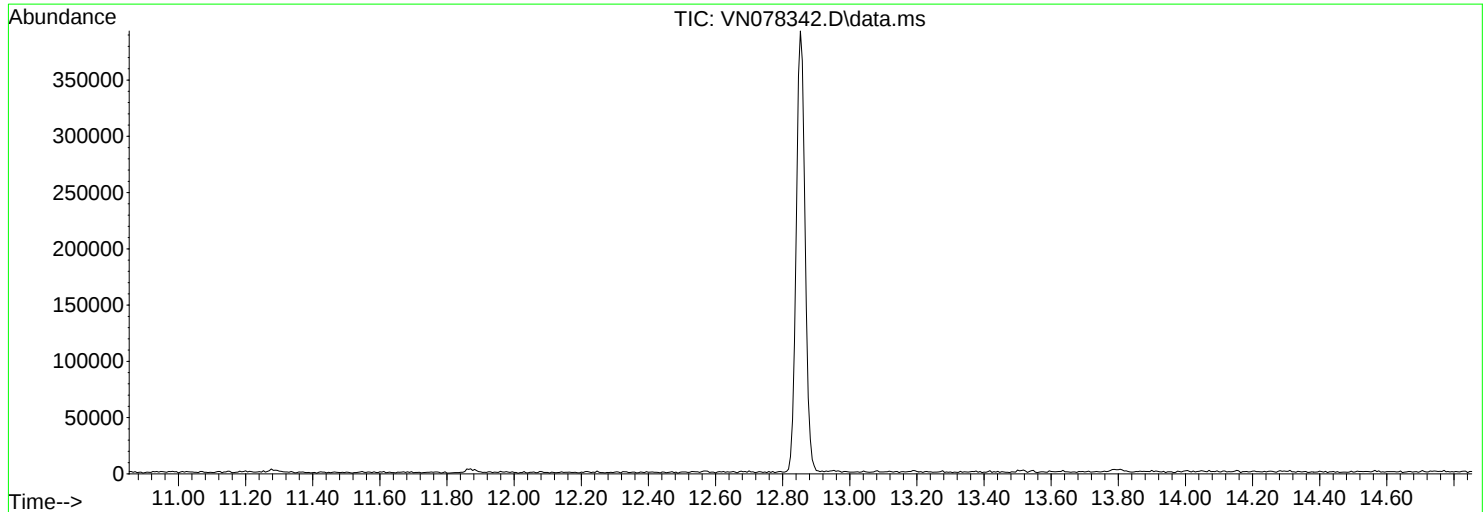

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1844

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.9	14976	PASS
75	95	30	60	51.6	38733	PASS
95	95	100	100	100.0	75123	PASS
96	95	5	9	6.4	4811	PASS
173	174	0.00	2	0.5	306	PASS
174	95	50	100	74.5	55984	PASS
175	174	5	9	6.9	3883	PASS
176	174	95	101	95.2	53283	PASS
177	176	5	9	6.2	3310	PASS

Average of 12.847 to 12.859 min.: VN078342.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.75	349	45.80	85	54.80	67	64.10	421
36.10	338	46.10	82	55.00	145	64.95	69
37.05	3764	46.80	198	55.90	528	66.10	5
38.00	3537	47.10	401	56.05	1008	66.60	9
39.05	1610	47.85	560	57.00	2480	67.00	111
39.95	144	48.90	914	58.00	183	68.00	8186
40.70	119	49.05	2156	59.95	1048	69.00	8636
42.90	155	50.00	14976	61.00	4011	69.90	340
43.90	1070	51.00	4399	62.00	3751	70.10	406
44.85	522	51.95	195	63.00	3062	71.20	57
45.10	272	52.90	61	63.90	128	71.80	237

Average of 12.847 to 12.859 min.: VN078342.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
72.05	343	82.10	219	96.00	4811	127.70	111
73.00	3666	82.90	89	97.10	55	129.00	156
74.00	14569	86.90	3361	103.85	529	129.80	328
75.00	38733	88.00	2909	105.85	435	134.80	214
76.00	2991	90.60	79	110.80	120	136.80	222
77.05	405	91.00	209	112.70	86	140.95	970
77.75	240	91.80	663	115.85	388	142.90	1273
78.85	3278	92.00	1930	116.85	677	144.70	185
79.95	1050	93.00	3855	117.75	315	145.00	63
80.85	3414	94.00	9808	118.00	142	146.40	64
81.90	504	95.00	75123	118.90	681	147.85	223

Average of 12.847 to 12.859 min.: VN078342.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
154.85	272	176.95	3310				
157.00	86	177.80	54				
158.90	131	267.10	236				
160.80	99	280.95	163				
171.95	966						
172.60	175						
172.80	134						
173.05	306						
173.95	55984						
174.95	3883						
175.95	53283						