


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN062320\
 Data File : VN062041.D
 Acq On : 23 Jun 2020 12:08
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N061620W.M
 Title : SW846 8260
 Last Update : Wed Jun 17 01:19:44 2020

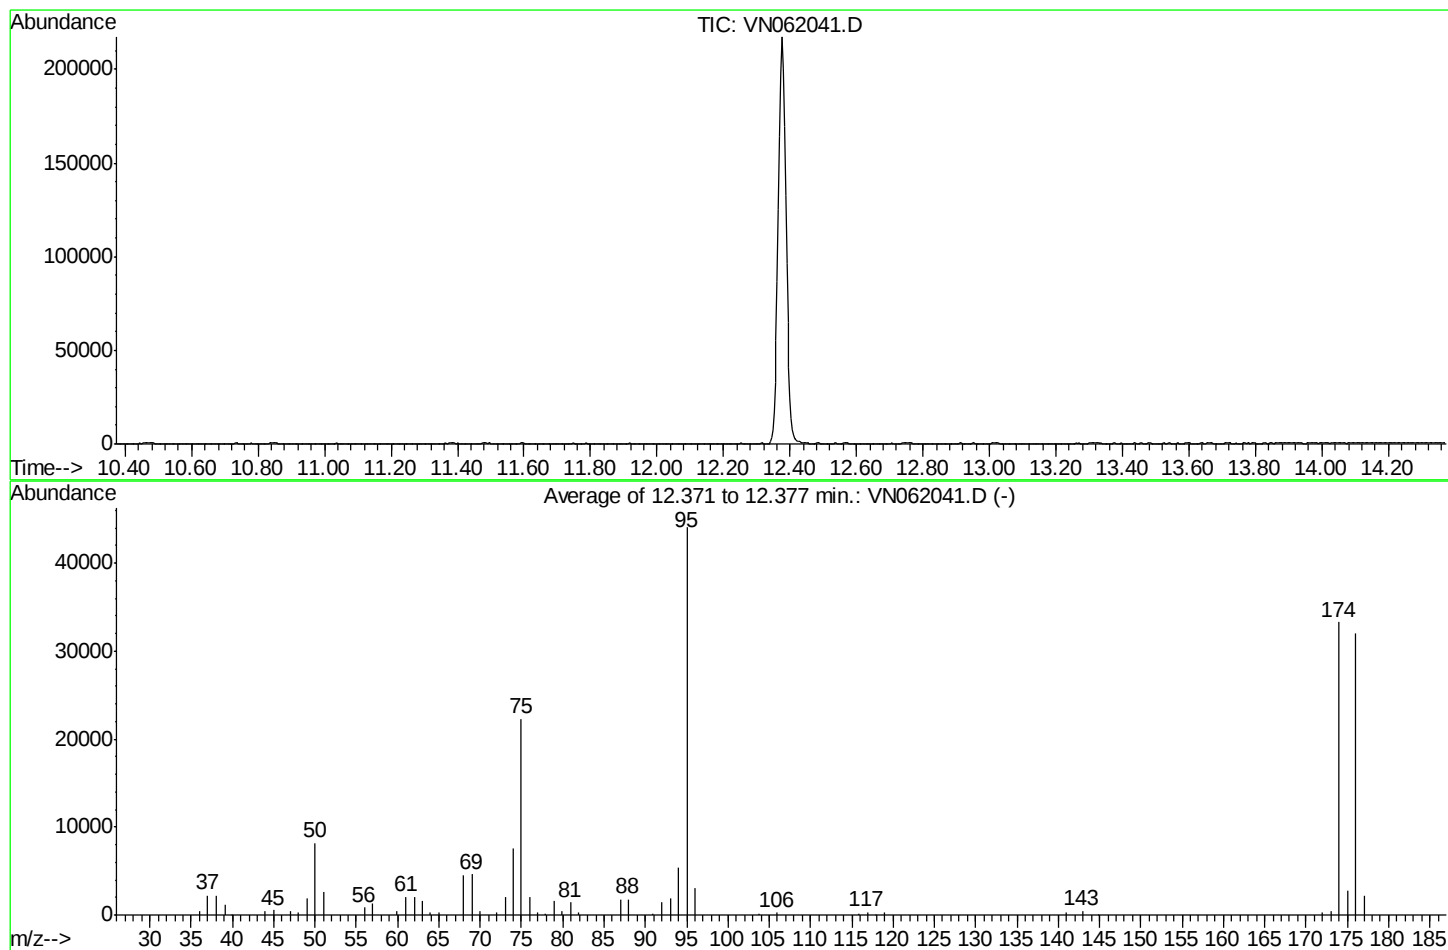

AutoFind: Scans 3296, 3297, 3298; Background Corrected with Scan 3284

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.6	8217	PASS
75	95	30	60	50.7	22317	PASS
95	95	100	100	100.0	44061	PASS
96	95	5	9	6.9	3040	PASS
173	174	0.00	2	1.4	462	PASS
174	95	50	100	75.6	33309	PASS
175	174	5	9	8.1	2706	PASS
176	174	95	101	96.1	31994	PASS
177	176	5	9	6.9	2212	PASS