

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN062322\
 Data File : VN073048.D
 Acq On : 23 Jun 2022 15:03
 Operator : JC\MD
 Sample : N3381-16DL 10X
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 PZ-7DL

Quant Time: Jun 24 01:18:55 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N061722W.M
 Quant Title : SW846 8260
 QLast Update : Sat Jun 18 06:22:45 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.016	168	326621	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.904	114	528597	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.680	117	476305	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.610	152	233127	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.369	65	196848	44.578	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery =	89.160%		
35) Dibromofluoromethane	7.951	113	166367	50.920	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	101.840%		
50) Toluene-d8	10.375	98	543571	44.711	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery =	89.420%		
62) 4-Bromofluorobenzene	12.669	95	241174	55.168	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	110.340%		
Target Compounds						Qvalue
3) Chloromethane	2.269	50	756	0.793	ug/l #	43
6) Chloroethane	3.022	64	534	0.306	ug/l #	42
13) Acrolein	3.934	56	4429	9.859	ug/l #	1
14) Allyl chloride	4.875	41	5936	0.888	ug/l #	63
15) Acrylonitrile	5.534	53	769	0.292	ug/l #	29
16) Acetone	4.246	43	6237	2.569	ug/l #	88
18) Methyl Acetate	4.793	43	7338	1.135	ug/l #	82
20) Methylene Chloride	5.004	84	533	Below Cal	#	88
25) 2-Butanone	7.245	43	1454	0.377	ug/l #	45
26) 2,2-Dichloropropane	7.239	77	1347	Below Cal	#	53
29) Tetrahydrofuran	7.639	42	880	0.346	ug/l #	29
31) Cyclohexane	8.022	56	34057	5.702	ug/l #	87
36) 1,1-Dichloropropene	8.016	75	26015	5.885	ug/l #	50
38) Carbon Tetrachloride	8.016	117	33850	7.279	ug/l #	16
39) Methylcyclohexane	9.381	83	4076	0.765	ug/l #	81
40) Benzene	8.392	78	25570	1.840	ug/l	96
52) Toluene	10.439	92	44447	5.211	ug/l	97
59) 2-Hexanone	11.151	43	3016	0.592	ug/l	92
67) Ethyl Benzene	11.780	91	155414	9.491	ug/l	96
68) m/p-Xylenes	11.886	106	212181	33.037	ug/l	92
69) o-Xylene	12.210	106	3596	0.560	ug/l	92
73) Isopropylbenzene	12.516	105	66857	3.707	ug/l	99
76) 1,2,3-Trichloropropane	12.669	75	123113	21.782	ug/l #	1
78) n-propylbenzene	12.857	91	93138	4.695	ug/l	98
79) 2-Chlorotoluene	12.857	91	93138	7.250	ug/l #	40
80) 1,3,5-Trimethylbenzene	12.992	105	16654	1.124	ug/l	97
81) trans-1,4-Dichloro-2-b...	12.669	75	123113	58.824	ug/l #	10
82) 4-Chlorotoluene	13.157	91	6605	0.543	ug/l #	40
84) 1,2,4-Trimethylbenzene	13.304	105	6059	0.411	ug/l	96
89) n-Butylbenzene	13.810	91	25826	2.158	ug/l #	42
95) Naphthalene	15.433	128	97287	5.402	ug/l	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN062322\
Data File : VN073048.D
Acq On : 23 Jun 2022 15:03
Operator : JC\MD
Sample : N3381-16DL 10X
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
PZ-7DL

Quant Time: Jun 24 01:18:55 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N061722W.M
Quant Title : SW846 8260
QLast Update : Sat Jun 18 06:22:45 2022
Response via : Initial Calibration




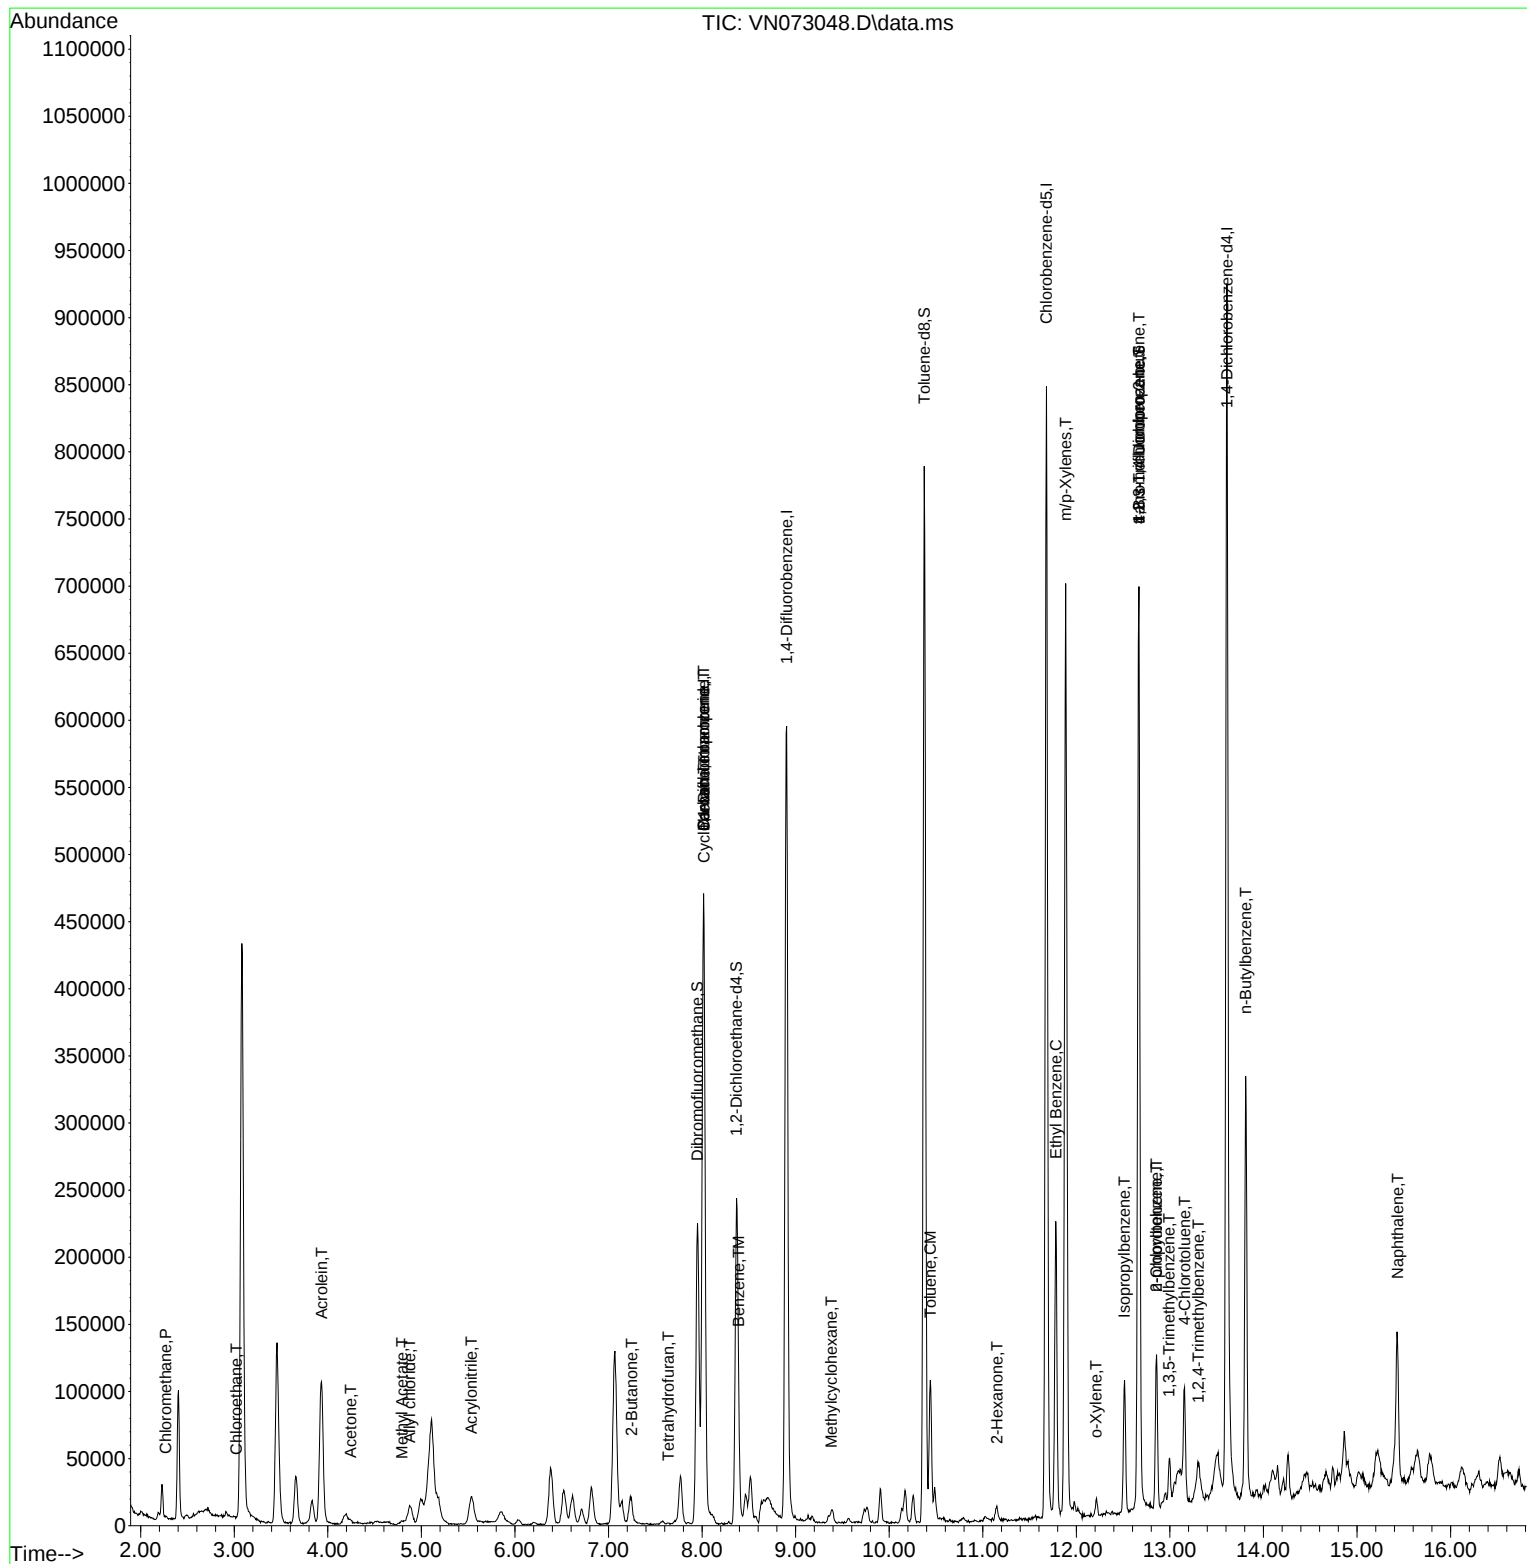




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.016 min Scan# 1042
Delta R.T. -0.000 min
Lab File: VN073048.D
Acq: 23 Jun 2022 15:03




Instrument :
MSVOA_N
ClientSampleId :
PZ-7DL


Tgt Ion:168 Resp: 326621
Ion Ratio Lower Upper
168 100
99 56.3 42.3 63.5

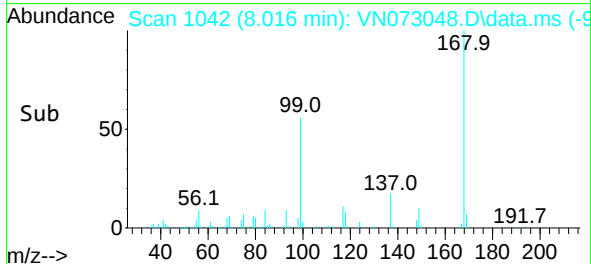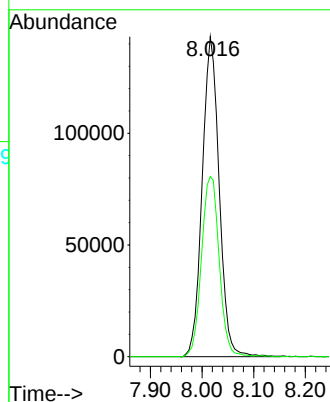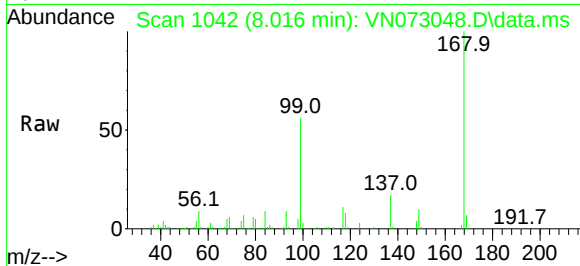

#3
Chloromethane
Concen: 0.793 ug/l
RT: 2.269 min Scan# 65
Delta R.T. 0.006 min
Lab File: VN073048.D
Acq: 23 Jun 2022 15:03

Tgt Ion: 50 Resp: 756
Ion Ratio Lower Upper
50 100
52 0.0 25.7 38.5#


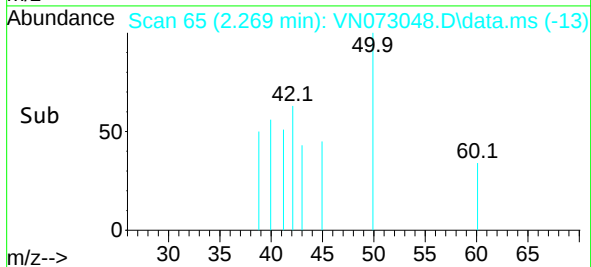
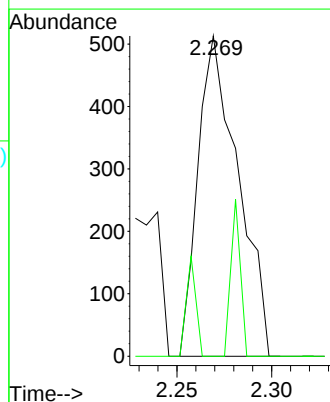
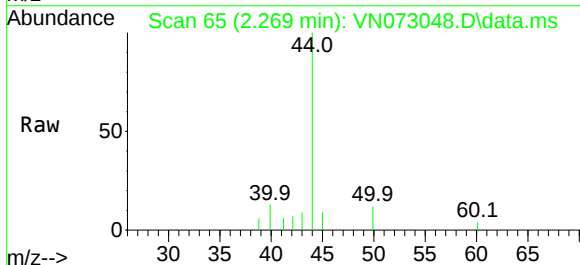




#6
Chloroethane
Concen: 0.306 ug/l
RT: 3.022 min Scan# 11
Delta R.T. 0.071 min
Lab File: VN073048.D
Acq: 23 Jun 2022 15:03




Instrument :
MSVOA_N
ClientSampleId :
PZ-7DL


Tgt Ion: 64 Resp: 534
Ion Ratio Lower Upper
64 100
66 0.0 26.2 39.4#

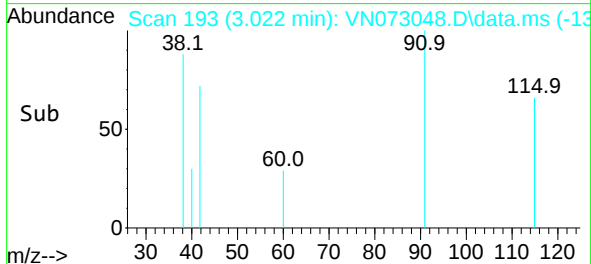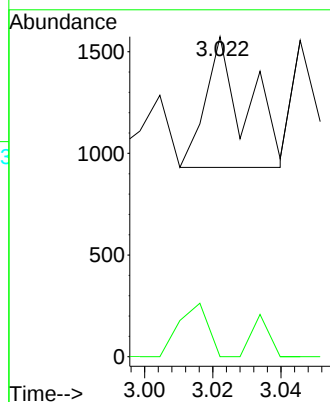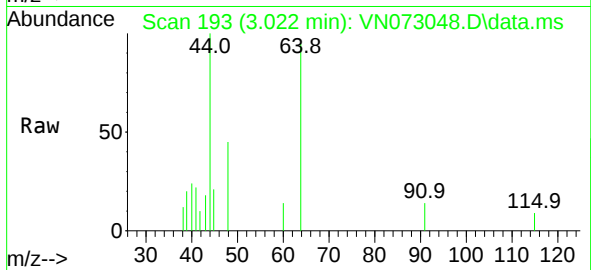

#13
Acrolein
Concen: 9.859 ug/l
RT: 3.934 min Scan# 348
Delta R.T. -0.047 min
Lab File: VN073048.D
Acq: 23 Jun 2022 15:03

Tgt Ion: 56 Resp: 4429
Ion Ratio Lower Upper
56 100
55 2231.2 54.8 82.2#

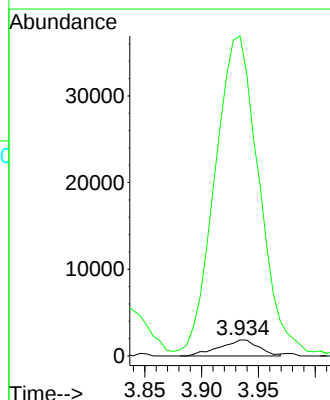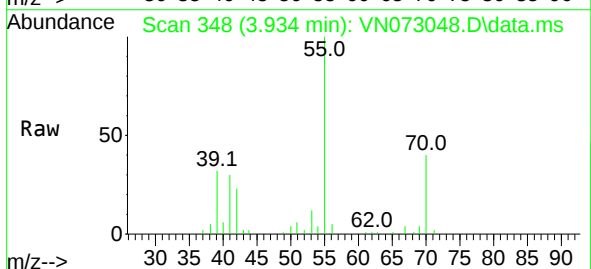



#14

Allyl chloride

Concen: 0.888 ug/l

RT: 4.875 min Scan# 50

Delta R.T. 0.118 min

Lab File: VN073048.D

Acq: 23 Jun 2022 15:03





Instrument :

MSVOA_N

ClientSampleId :

PZ-7DL

Tgt Ion: 41	Resp: 5936
Ion Ratio	Lower Upper
41 100	
39 84.9	53.2 79.8#
76 0.0	29.9 44.9#

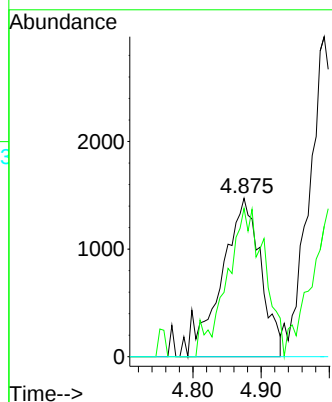

#15

Acrylonitrile

Concen: 0.292 ug/l




RT: 5.534 min Scan# 620


Delta R.T. 0.059 min

Lab File: VN073048.D

Acq: 23 Jun 2022 15:03

Tgt Ion: 53	Resp: 769
Ion Ratio	Lower Upper
53 100	
52 0.0	66.4 99.6#
51 23.0	28.5 42.7#

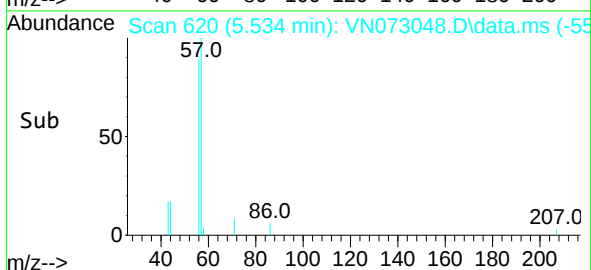



#16

Acetone

Concen: 2.569 ug/l

RT: 4.246 min Scan# 401

Delta R.T. 0.018 min

Lab File: VN073048.D

Acq: 23 Jun 2022 15:03

Instrument :

MSVOA_N

ClientSampleId :





PZ-7DL

Tgt Ion: 43 Resp: 6237

Ion Ratio Lower Upper

43 100

58 25.7 26.0 39.0#

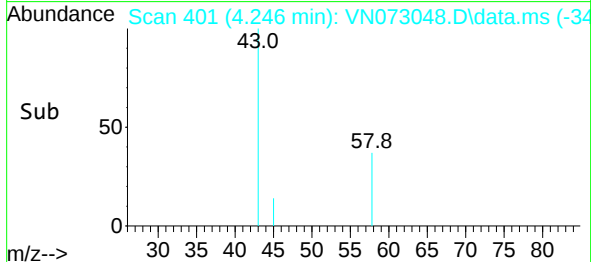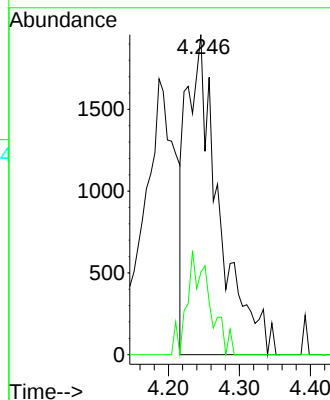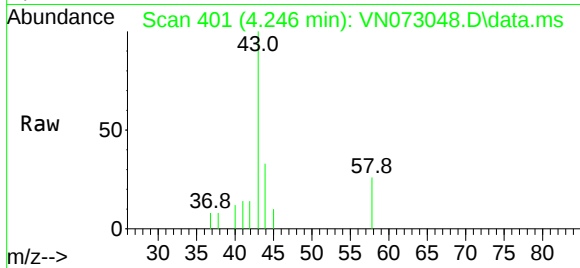

#18

Methyl Acetate

Concen: 1.135 ug/l

RT: 4.793 min Scan# 494

Delta R.T. 0.012 min

Lab File: VN073048.D




Acq: 23 Jun 2022 15:03


Tgt Ion: 43 Resp: 7338

Ion Ratio Lower Upper

43 100

74 17.7 21.6 32.4#

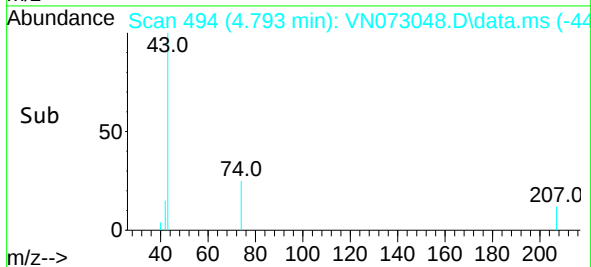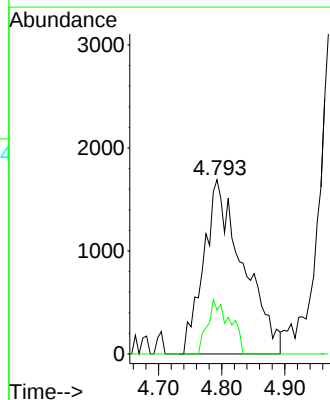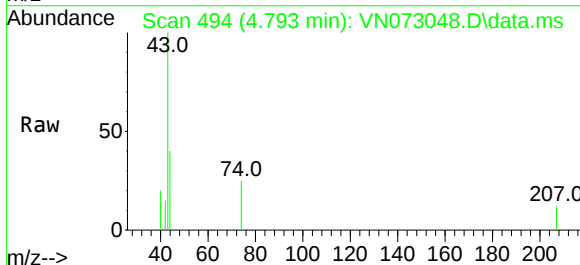



#25

2-Butanone

Concen: 0.377 ug/l

RT: 7.245 min Scan# 910

Delta R.T. -0.018 min

Lab File: VN073048.D

Acq: 23 Jun 2022 15:03

Instrument :

MSVOA_N

ClientSampleId :





PZ-7DL

Tgt Ion: 43 Resp: 1454

Ion Ratio Lower Upper

43 100

72 0.0 23.7 35.5#

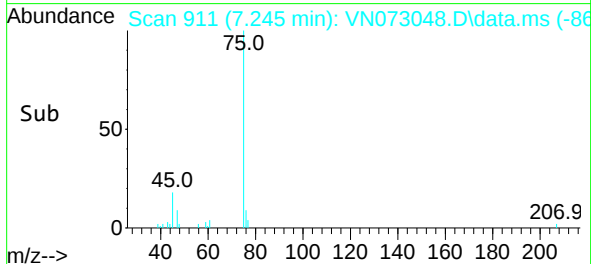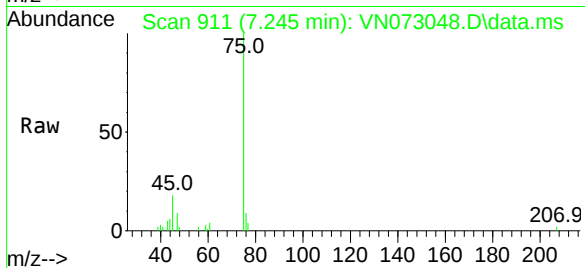

#26

2,2-Dichloropropane

Concen: Below Cal

RT: 7.239 min Scan# 910

Delta R.T. -0.012 min

Lab File: VN073048.D




Acq: 23 Jun 2022 15:03


Tgt Ion: 77 Resp: 1347

Ion Ratio Lower Upper

77 100

97 0.0 11.4 34.2#

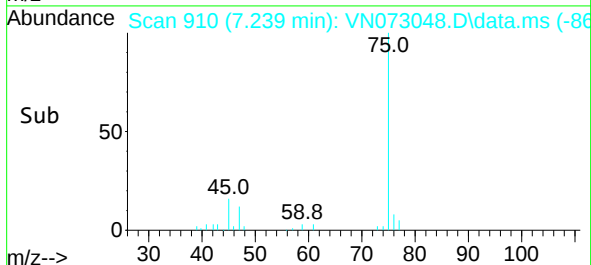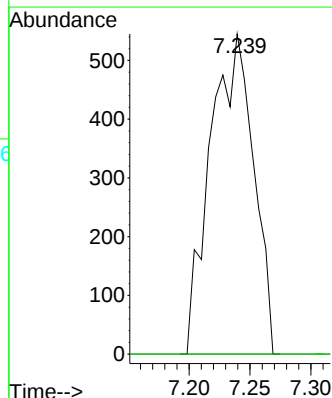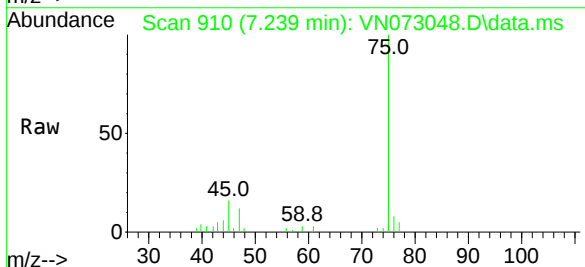



#29

Tetrahydrofuran

Concen: 0.346 ug/l

RT: 7.639 min Scan# 91

Delta R.T. 0.030 min

Lab File: VN073048.D


Acq: 23 Jun 2022 15:03

Instrument :




MSVOA_N

ClientSampleId :

PZ-7DL



Tgt Ion: 42	Resp: 880
Ion Ratio	Lower Upper
42	100
72	0.0 39.7 59.5#
71	0.0 36.6 55.0#

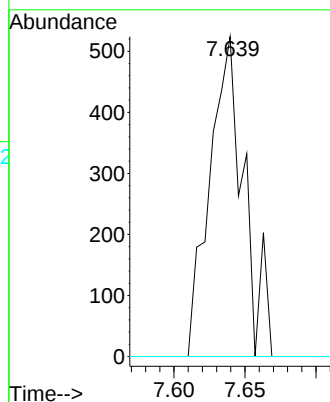

#31

Cyclohexane

Concen: 5.702 ug/l




RT: 8.022 min Scan# 1043


Delta R.T. 0.000 min

Lab File: VN073048.D

Acq: 23 Jun 2022 15:03

Tgt Ion: 56	Resp: 34057
Ion Ratio	Lower Upper
56	100
69	56.4 27.8 41.8#
84	91.5 76.9 115.3

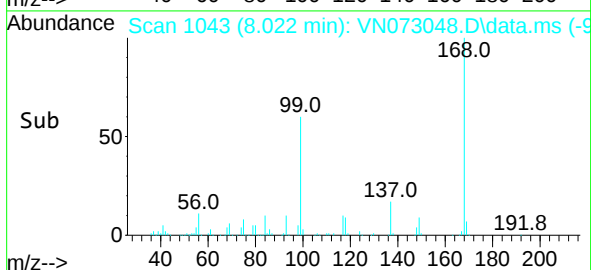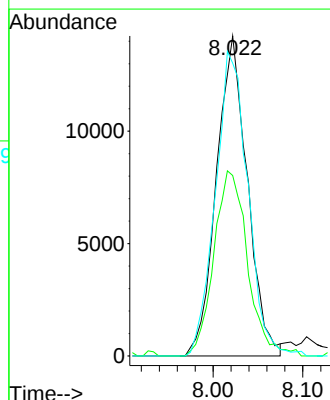

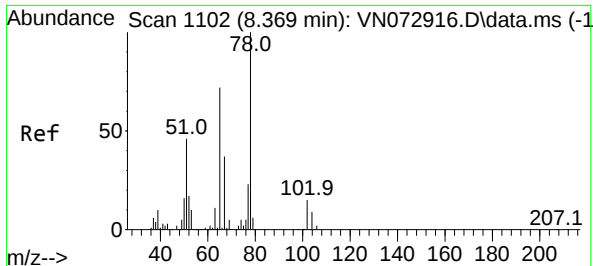

#33

1,2-Dichloroethane-d4

Concen: 44.578 ug/l

RT: 8.369 min Scan# 1102

Delta R.T. 0.000 min

Lab File: VN073048.D

Acq: 23 Jun 2022 15:03

Instrument :

MSVOA_N

ClientSampleId :





PZ-7DL

Tgt Ion: 65 Resp: 196848

Ion Ratio Lower Upper

65 100

67 51.7 0.0 104.8

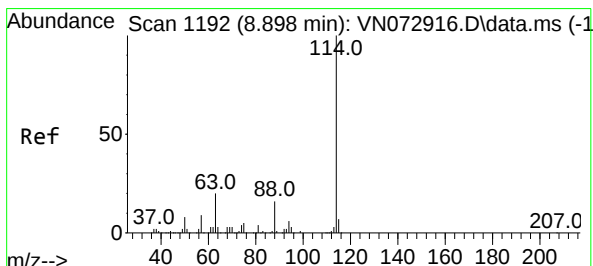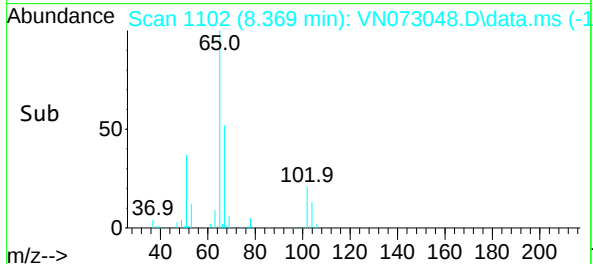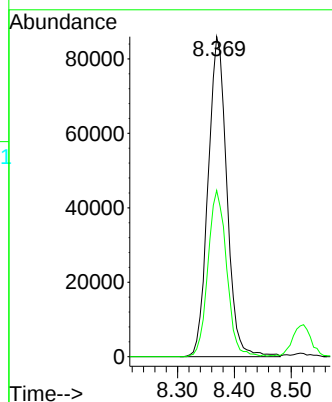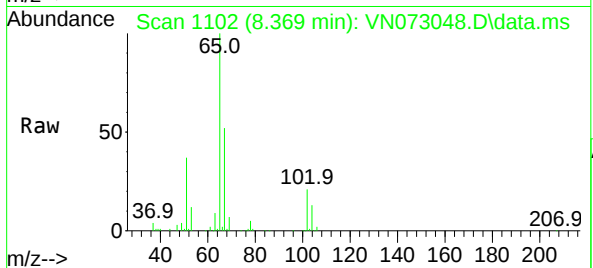

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.904 min Scan# 1193

Delta R.T. 0.006 min

Lab File: VN073048.D

Acq: 23 Jun 2022 15:03




Tgt Ion: 114 Resp: 528597


Ion Ratio Lower Upper

114 100

63 20.2 0.0 40.0

88 16.6 0.0 32.6

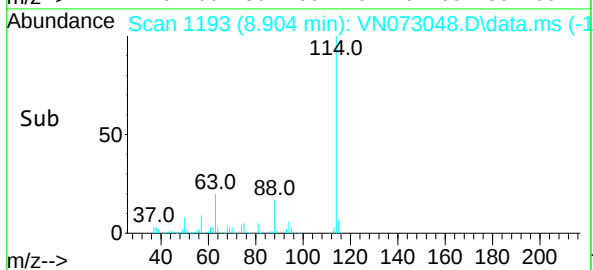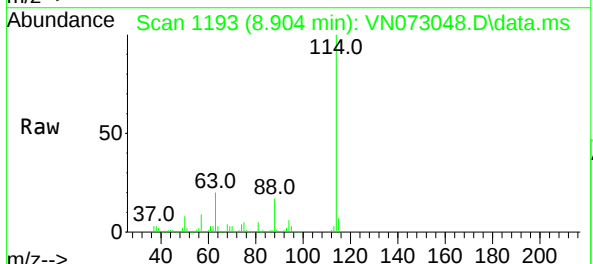

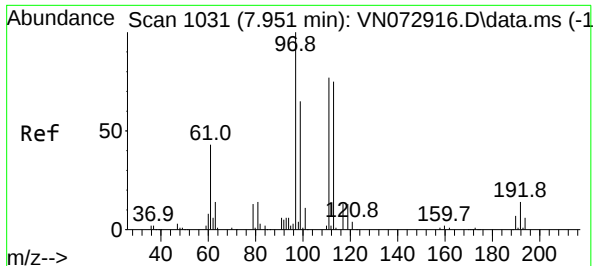

#35

Dibromofluoromethane

Concen: 50.920 ug/l

RT: 7.951 min Scan# 1042

Delta R.T. 0.000 min

Lab File: VN073048.D

Acq: 23 Jun 2022 15:03

Instrument :

MSVOA_N

ClientSampleId :

PZ-7DL





Tgt Ion:113 Resp: 166367

Ion Ratio Lower Upper

113 100

111 103.5 81.4 122.0

192 19.3 17.0 25.6

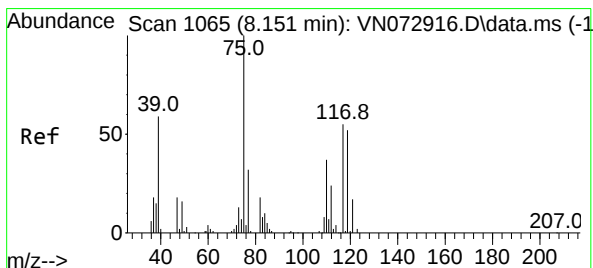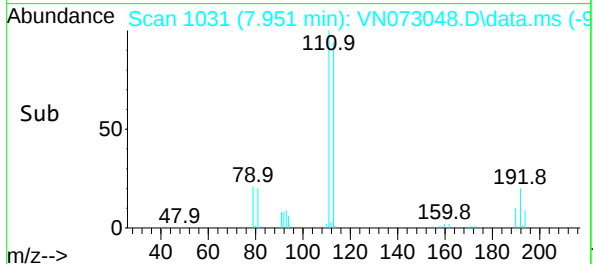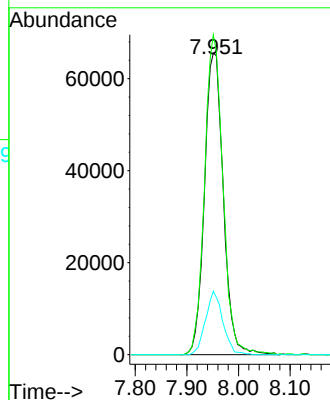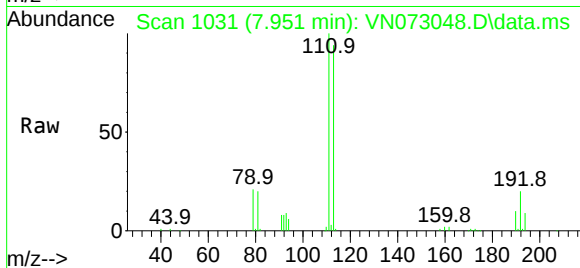

#36

1,1-Dichloropropene

Concen: 5.885 ug/l

RT: 8.016 min Scan# 1042

Delta R.T. -0.135 min

Lab File: VN073048.D

Acq: 23 Jun 2022 15:03




Tgt Ion: 75 Resp: 26015


Ion Ratio Lower Upper

75 100

110 8.8 18.3 54.8#

77 1.3 25.1 37.7#


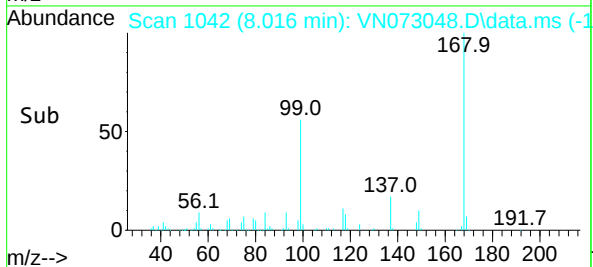
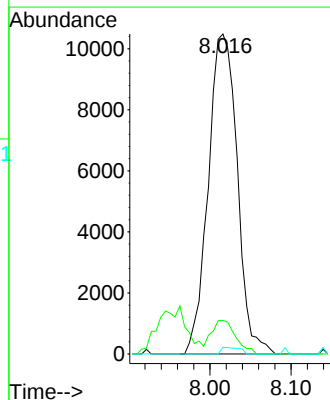
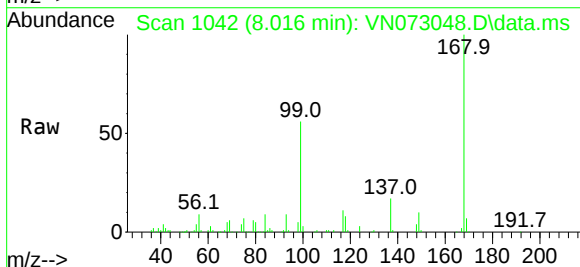


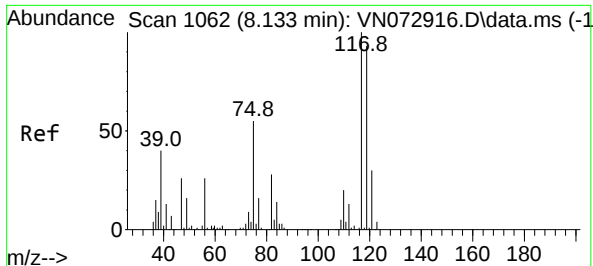

#38
Carbon Tetrachloride
Concen: 7.279 ug/l
RT: 8.016 min Scan# 1062
Delta R.T. -0.118 min
Lab File: VN073048.D
Acq: 23 Jun 2022 15:03




Instrument :
MSVOA_N
ClientSampleId :
PZ-7DL


Tgt Ion:117 Resp: 33850
Ion Ratio Lower Upper
117 100
119 4.8 75.8 113.8#
121 0.0 24.6 37.0#

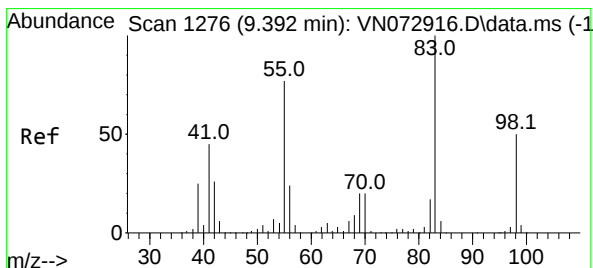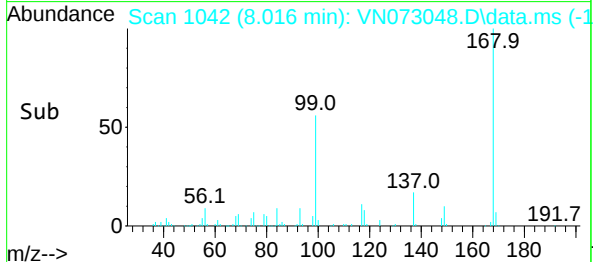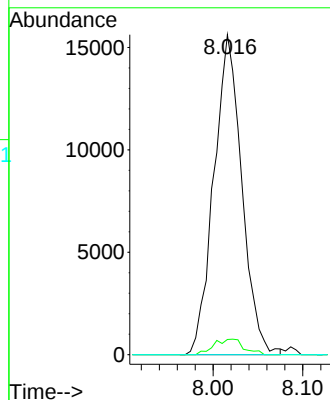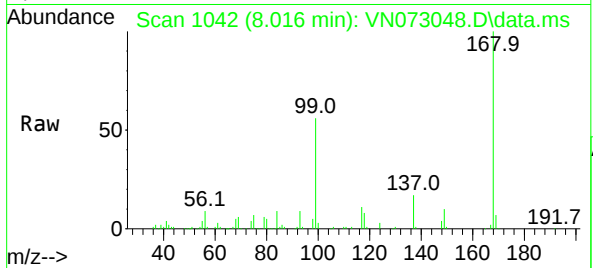

#39
Methylcyclohexane
Concen: 0.765 ug/l
RT: 9.381 min Scan# 1274
Delta R.T. -0.012 min
Lab File: VN073048.D
Acq: 23 Jun 2022 15:03

Tgt Ion: 83 Resp: 4076
Ion Ratio Lower Upper
83 100
55 86.0 57.8 86.8
98 33.9 39.4 59.2#


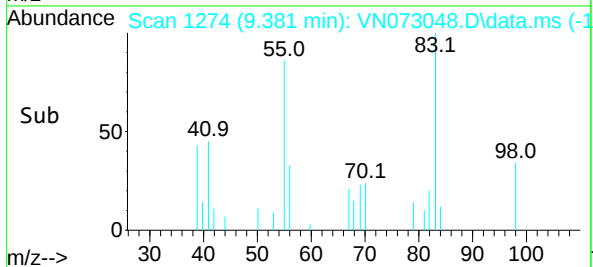
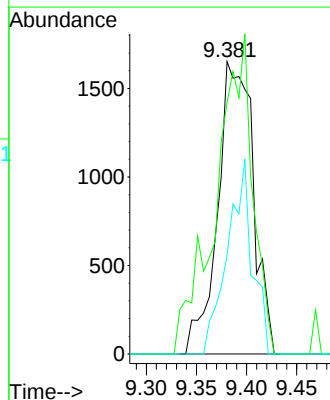
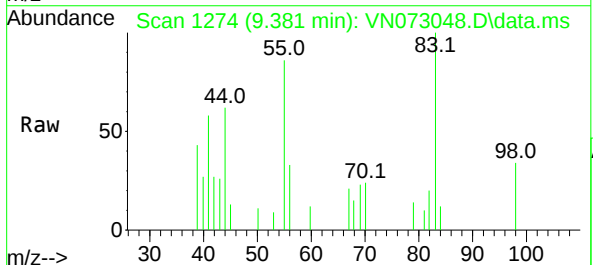


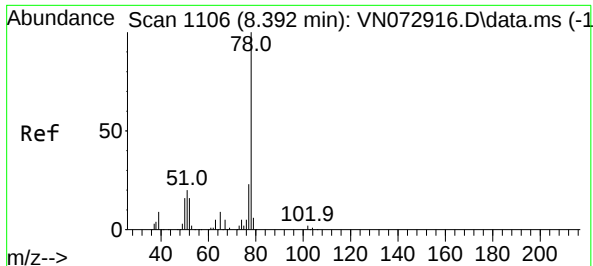

#40
Benzene
Concen: 1.840 ug/l
RT: 8.392 min Scan# 1106
Delta R.T. 0.000 min
Lab File: VN073048.D
Acq: 23 Jun 2022 15:03




Instrument :
MSVOA_N
ClientSampleId :
PZ-7DL


Tgt Ion: 78 Resp: 25570
Ion Ratio Lower Upper
78 100
77 26.3 19.4 29.0

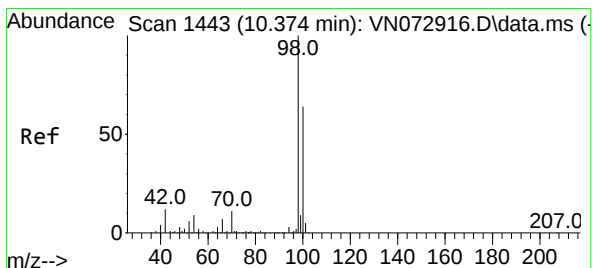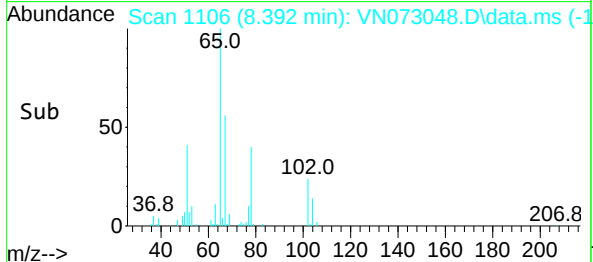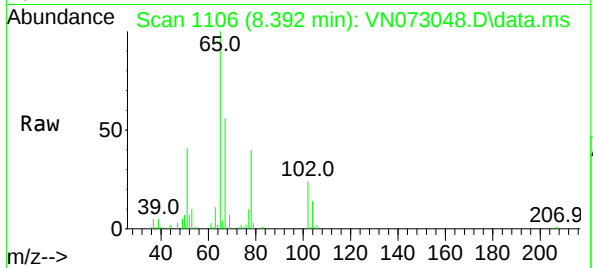

#50
Toluene-d8
Concen: 44.711 ug/l
RT: 10.375 min Scan# 1443
Delta R.T. 0.000 min
Lab File: VN073048.D
Acq: 23 Jun 2022 15:03

Tgt Ion: 98 Resp: 543571
Ion Ratio Lower Upper
98 100
100 64.8 52.6 78.8


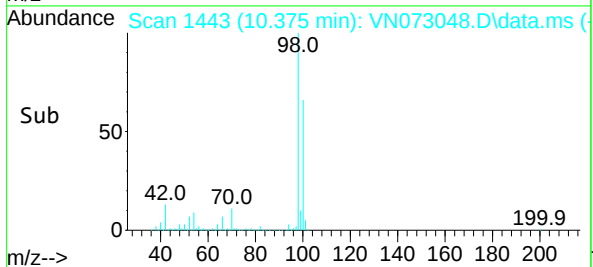

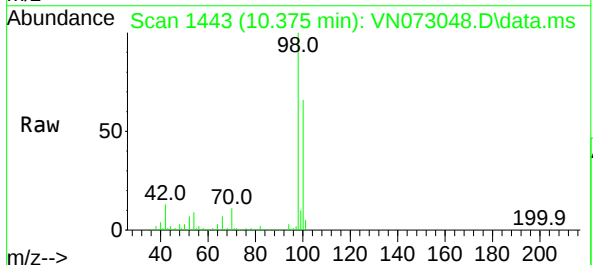


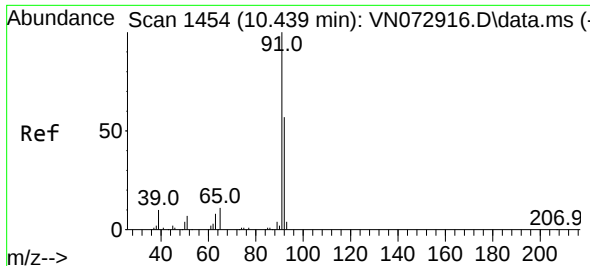

#52
Toluene
Concen: 5.211 ug/l
RT: 10.439 min Scan# 1454
Delta R.T. 0.000 min
Lab File: VN073048.D
Acq: 23 Jun 2022 15:03




Instrument :
MSVOA_N
ClientSampleId :
PZ-7DL


Tgt Ion: 92 Resp: 44447
Ion Ratio Lower Upper
92 100
91 169.0 138.6 207.8

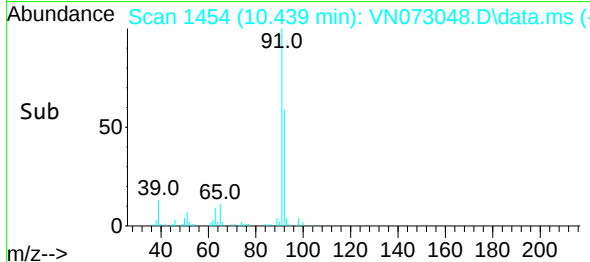

#59
2-Hexanone
Concen: 0.592 ug/l
RT: 11.151 min Scan# 1575
Delta R.T. 0.130 min
Lab File: VN073048.D
Acq: 23 Jun 2022 15:03

Tgt Ion: 43 Resp: 3016
Ion Ratio Lower Upper
43 100
58 65.3 29.7 89.1


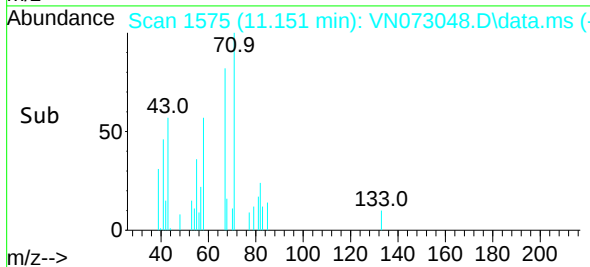

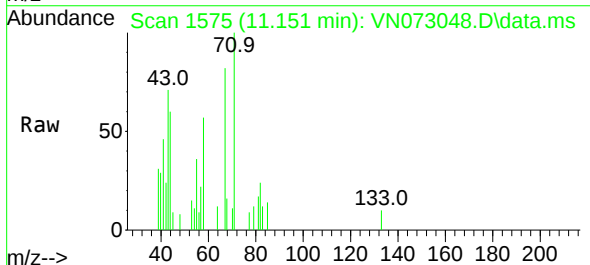




#62
4-Bromofluorobenzene
Concen: 55.168 ug/l
RT: 12.669 min Scan# 1833
Delta R.T. 0.000 min
Lab File: VN073048.D
Acq: 23 Jun 2022 15:03




Instrument :
MSVOA_N
ClientSampleId :
PZ-7DL


Tgt Ion: 95 Resp: 241174
Ion Ratio Lower Upper
95 100
174 75.0 0.0 167.6
176 72.8 0.0 163.4

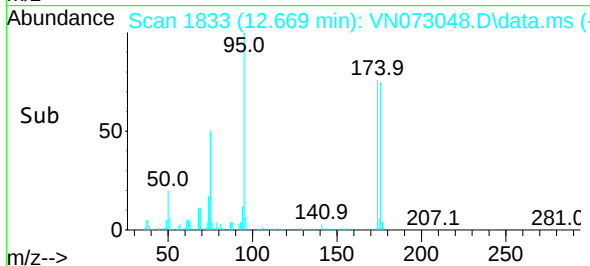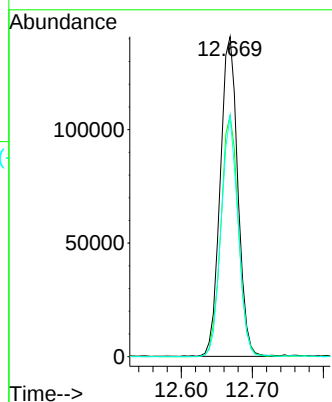

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.680 min Scan# 1665
Delta R.T. 0.000 min
Lab File: VN073048.D
Acq: 23 Jun 2022 15:03

Tgt Ion: 117 Resp: 476305
Ion Ratio Lower Upper
117 100
82 57.9 44.2 66.2
119 32.7 25.4 38.0


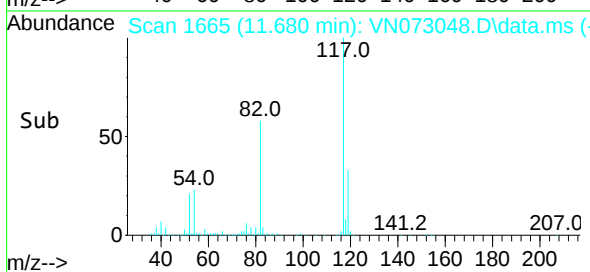
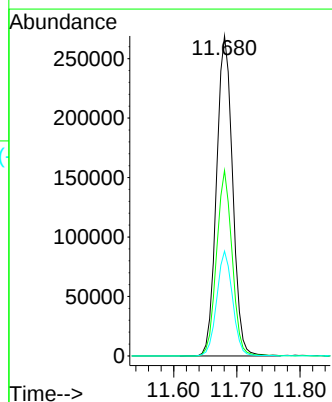
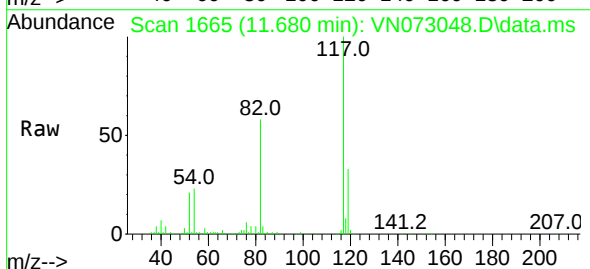


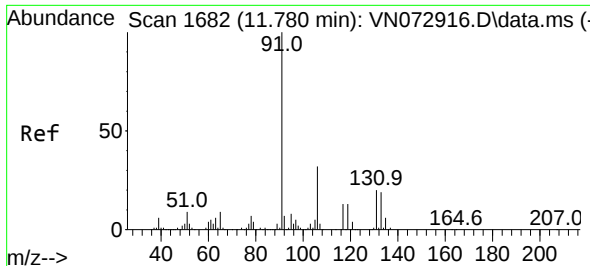

#67
Ethyl Benzene
Concen: 9.491 ug/l
RT: 11.780 min Scan# 1170
Delta R.T. 0.000 min
Lab File: VN073048.D
Acq: 23 Jun 2022 15:03




Instrument :
MSVOA_N
ClientSampleId :
PZ-7DL


Tgt Ion: 91 Resp: 155414
Ion Ratio Lower Upper
91 100
106 29.1 24.9 37.3

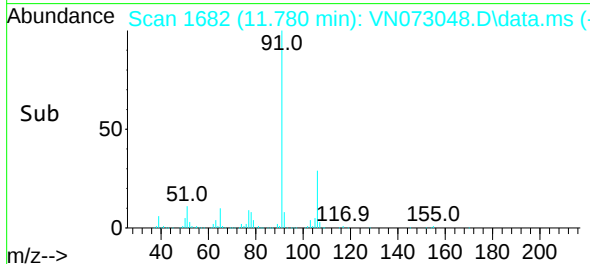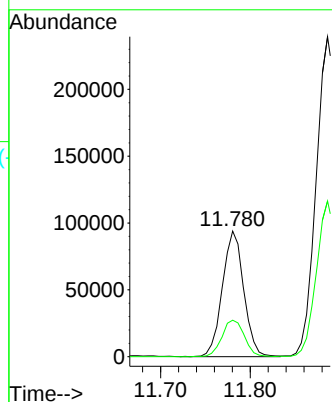

#68
m/p-Xylenes
Concen: 33.037 ug/l
RT: 11.886 min Scan# 1700
Delta R.T. 0.000 min
Lab File: VN073048.D
Acq: 23 Jun 2022 15:03

Tgt Ion: 106 Resp: 212181
Ion Ratio Lower Upper
106 100
91 210.3 158.9 238.3


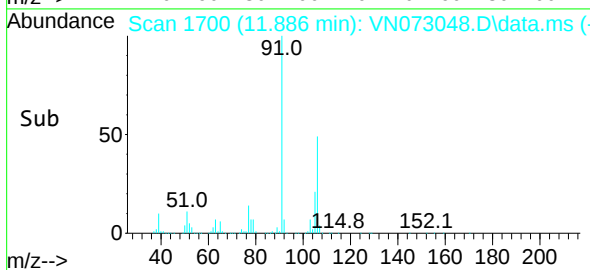
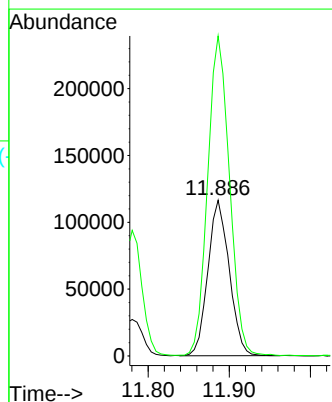
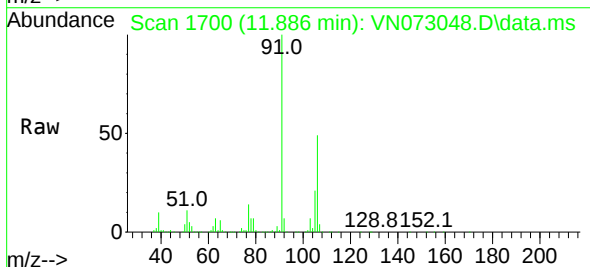




#69
o-Xylene
Concen: 0.560 ug/l
RT: 12.210 min Scan# 1755
Delta R.T. -0.006 min
Lab File: VN073048.D
Acq: 23 Jun 2022 15:03




Instrument :
MSVOA_N
ClientSampleId :
PZ-7DL


Tgt Ion:106 Resp: 3596
Ion Ratio Lower Upper
106 100
91 198.7 106.0 318.0

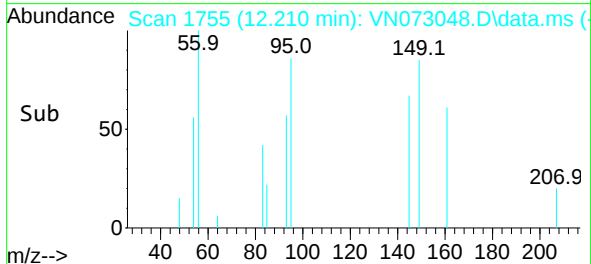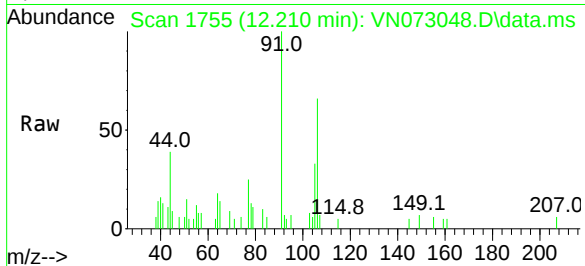

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.610 min Scan# 1993
Delta R.T. 0.000 min
Lab File: VN073048.D
Acq: 23 Jun 2022 15:03

Tgt Ion:152 Resp: 233127
Ion Ratio Lower Upper
152 100
115 62.2 28.9 86.7
150 156.9 0.0 356.2

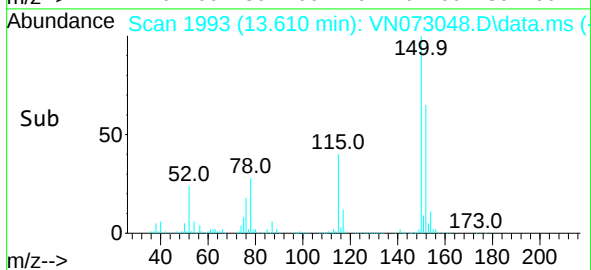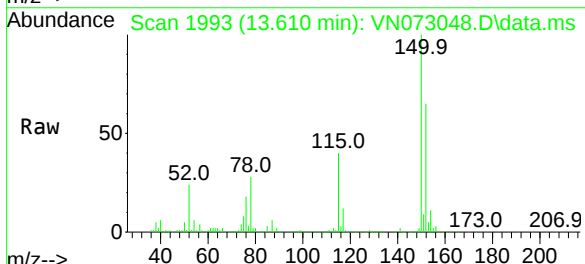



#73

Isopropylbenzene

Concen: 3.707 ug/l

RT: 12.516 min Scan# 11

Delta R.T. 0.000 min

Lab File: VN073048.D

Acq: 23 Jun 2022 15:03

Instrument :

MSVOA_N

ClientSampleId :





PZ-7DL

Tgt Ion:105 Resp: 66857

Ion Ratio Lower Upper

105 100

120 26.6 13.5 40.4

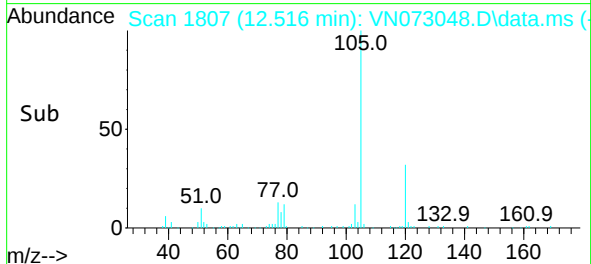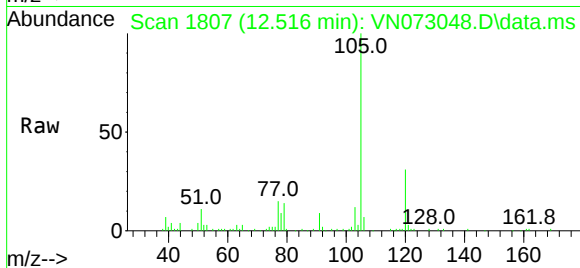

#76

1,2,3-Trichloropropane

Concen: 21.782 ug/l

RT: 12.669 min Scan# 1833

Delta R.T. -0.147 min

Lab File: VN073048.D




Acq: 23 Jun 2022 15:03


Tgt Ion: 75 Resp: 123113

Ion Ratio Lower Upper

75 100

77 1.8 98.5 295.5#


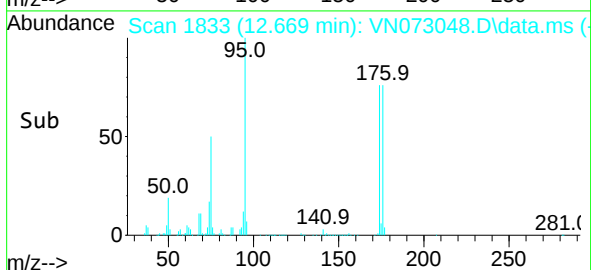

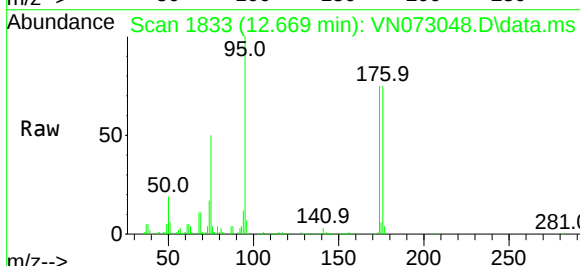


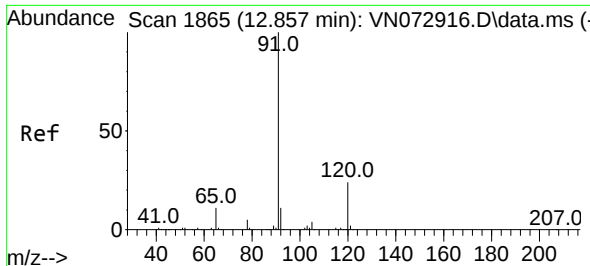

#78
n-propylbenzene
Concen: 4.695 ug/l
RT: 12.857 min Scan# 1865
Delta R.T. 0.000 min
Lab File: VN073048.D
Acq: 23 Jun 2022 15:03




Instrument :
MSVOA_N
ClientSampleId :
PZ-7DL


Tgt Ion: 91 Resp: 93138
Ion Ratio Lower Upper
91 100
120 22.8 11.9 35.5

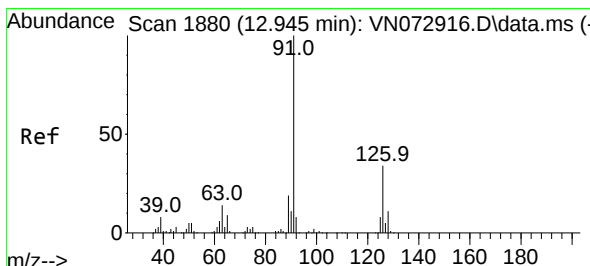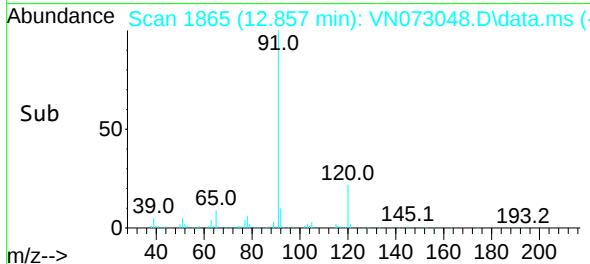

#79
2-Chlorotoluene
Concen: 7.250 ug/l
RT: 12.857 min Scan# 1865
Delta R.T. -0.088 min
Lab File: VN073048.D
Acq: 23 Jun 2022 15:03

Tgt Ion: 91 Resp: 93138
Ion Ratio Lower Upper
91 100
126 0.0 17.3 51.9#

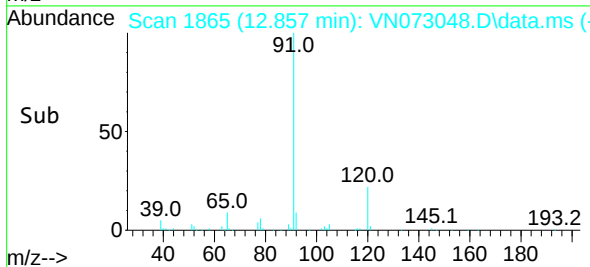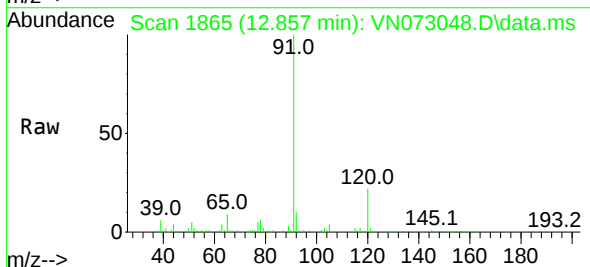



#80

1,3,5-Trimethylbenzene

Concen: 1.124 ug/l

RT: 12.992 min Scan# 1888

Delta R.T. -0.006 min

Lab File: VN073048.D

Acq: 23 Jun 2022 15:03

Instrument :

MSVOA_N

ClientSampleId :





PZ-7DL

Tgt Ion:105 Resp: 16654

Ion Ratio Lower Upper

105 100

120 47.5 24.9 74.7

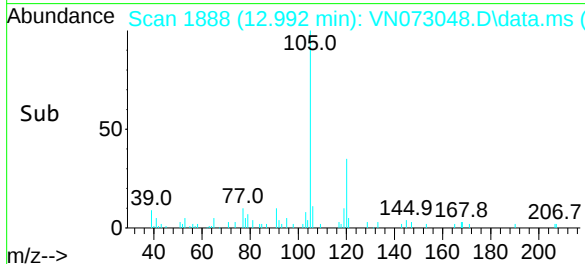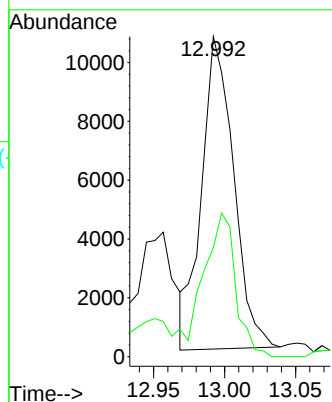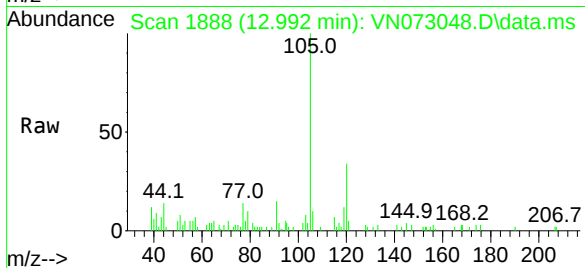

#81

trans-1,4-Dichloro-2-butene

Concen: 58.824 ug/l

RT: 12.669 min Scan# 1833

Delta R.T. 0.106 min

Lab File: VN073048.D

Acq: 23 Jun 2022 15:03




Tgt Ion: 75 Resp: 123113


Ion Ratio Lower Upper

75 100

53 0.1 78.0 117.0#

89 0.0 37.2 55.8#


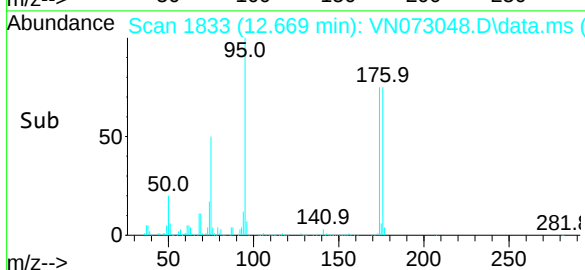

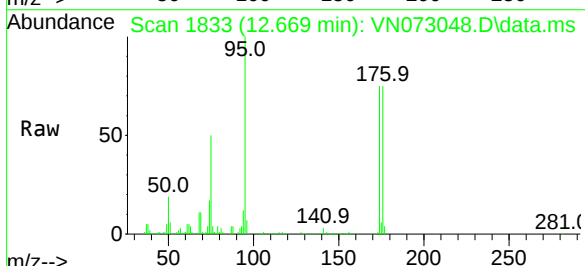


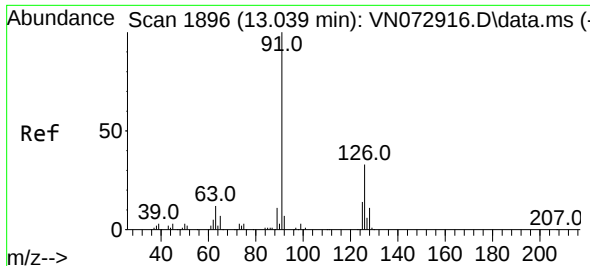

#82
4-Chlorotoluene
Concen: 0.543 ug/l
RT: 13.157 min Scan# 1916
Delta R.T. 0.118 min
Lab File: VN073048.D
Acq: 23 Jun 2022 15:03




Instrument :
MSVOA_N
ClientSampleId :
PZ-7DL


Tgt Ion: 91 Resp: 6605
Ion Ratio Lower Upper
91 100
126 0.0 17.2 51.6#

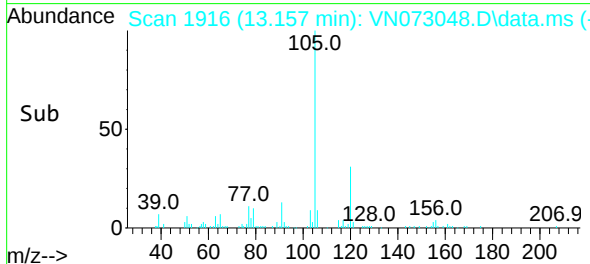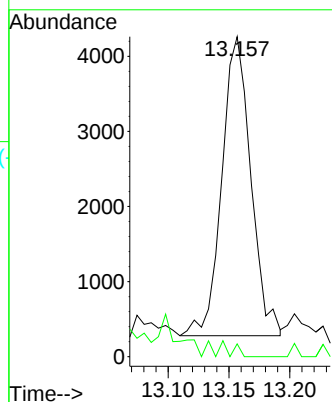

#84
1,2,4-Trimethylbenzene
Concen: 0.411 ug/l
RT: 13.304 min Scan# 1941
Delta R.T. 0.000 min
Lab File: VN073048.D
Acq: 23 Jun 2022 15:03

Tgt Ion: 105 Resp: 6059
Ion Ratio Lower Upper
105 100
120 49.3 23.3 69.8


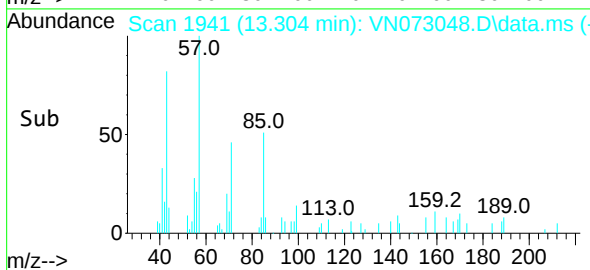
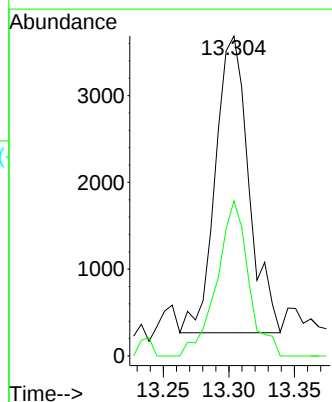
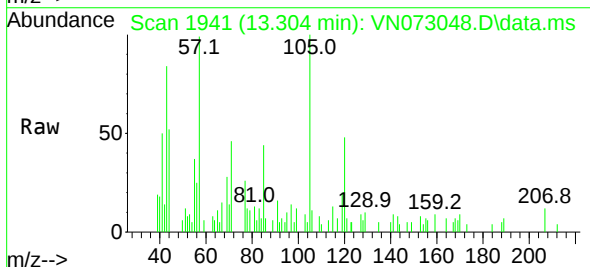


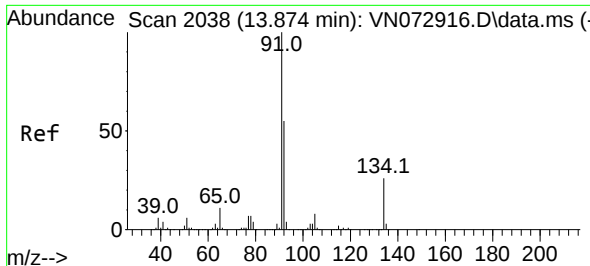

#89
n-Butylbenzene
Concen: 2.158 ug/l
RT: 13.810 min Scan# 2038
Delta R.T. -0.065 min
Lab File: VN073048.D
Acq: 23 Jun 2022 15:03

Instrument :
MSVOA_N
ClientSampleId :
PZ-7DL

Tgt Ion: 91 Resp: 25826
Ion Ratio Lower Upper
91 100
92 10.3 26.9 80.7#
134 0.0 13.6 40.8#

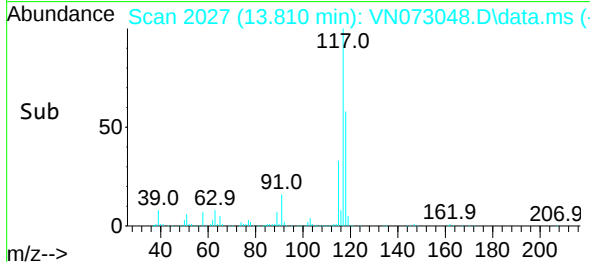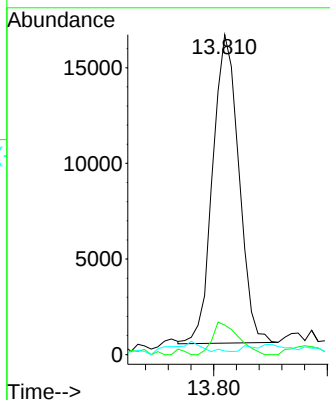

#95
Naphthalene
Concen: 5.402 ug/l
RT: 15.433 min Scan# 2303
Delta R.T. 0.006 min
Lab File: VN073048.D
Acq: 23 Jun 2022 15:03

Tgt Ion: 128 Resp: 97287
Ion Ratio Lower Upper
128 100
127 14.5 10.3 15.5
129 12.9 8.6 13.0

