
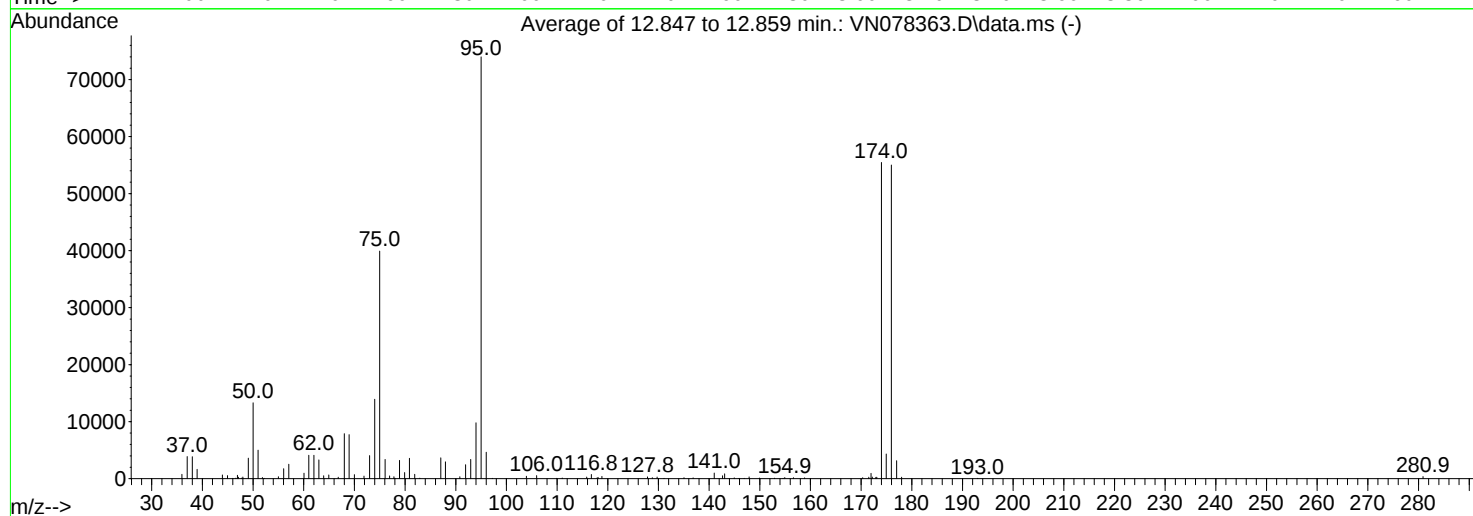


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN062323\
 Data File : VN078363.D
 Acq On : 23 Jun 2023 08:21
 Operator : JC\MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N062323W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Sat Jun 24 00:59:50 2023

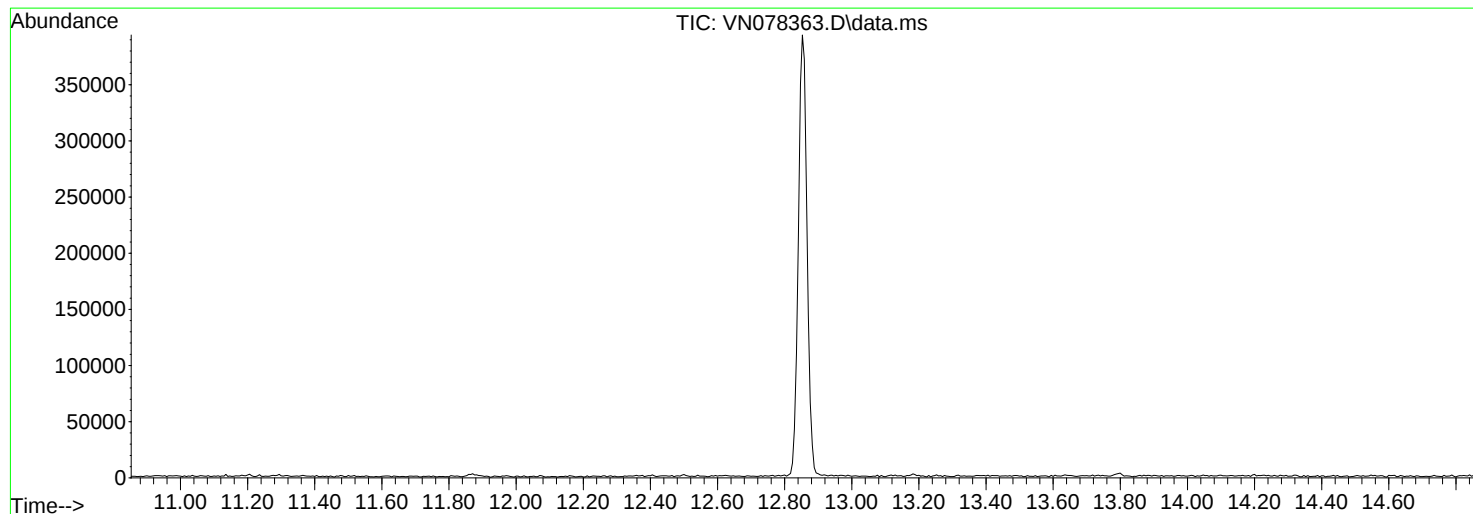

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1844

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.0	13315	PASS
75	95	30	60	54.0	39928	PASS
95	95	100	100	100.0	73997	PASS
96	95	5	9	6.3	4641	PASS
173	174	0.00	2	0.5	266	PASS
174	95	50	100	75.0	55461	PASS
175	174	5	9	7.8	4317	PASS
176	174	95	101	99.2	55024	PASS
177	176	5	9	5.7	3149	PASS