


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN062419\
 Data File : VN056440.D
 Acq On : 24 Jun 2019 8:22
 Operator : JC/SP
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N061919W.M
 Title : SW846 8260
 Last Update : Fri Jun 21 03:45:40 2019

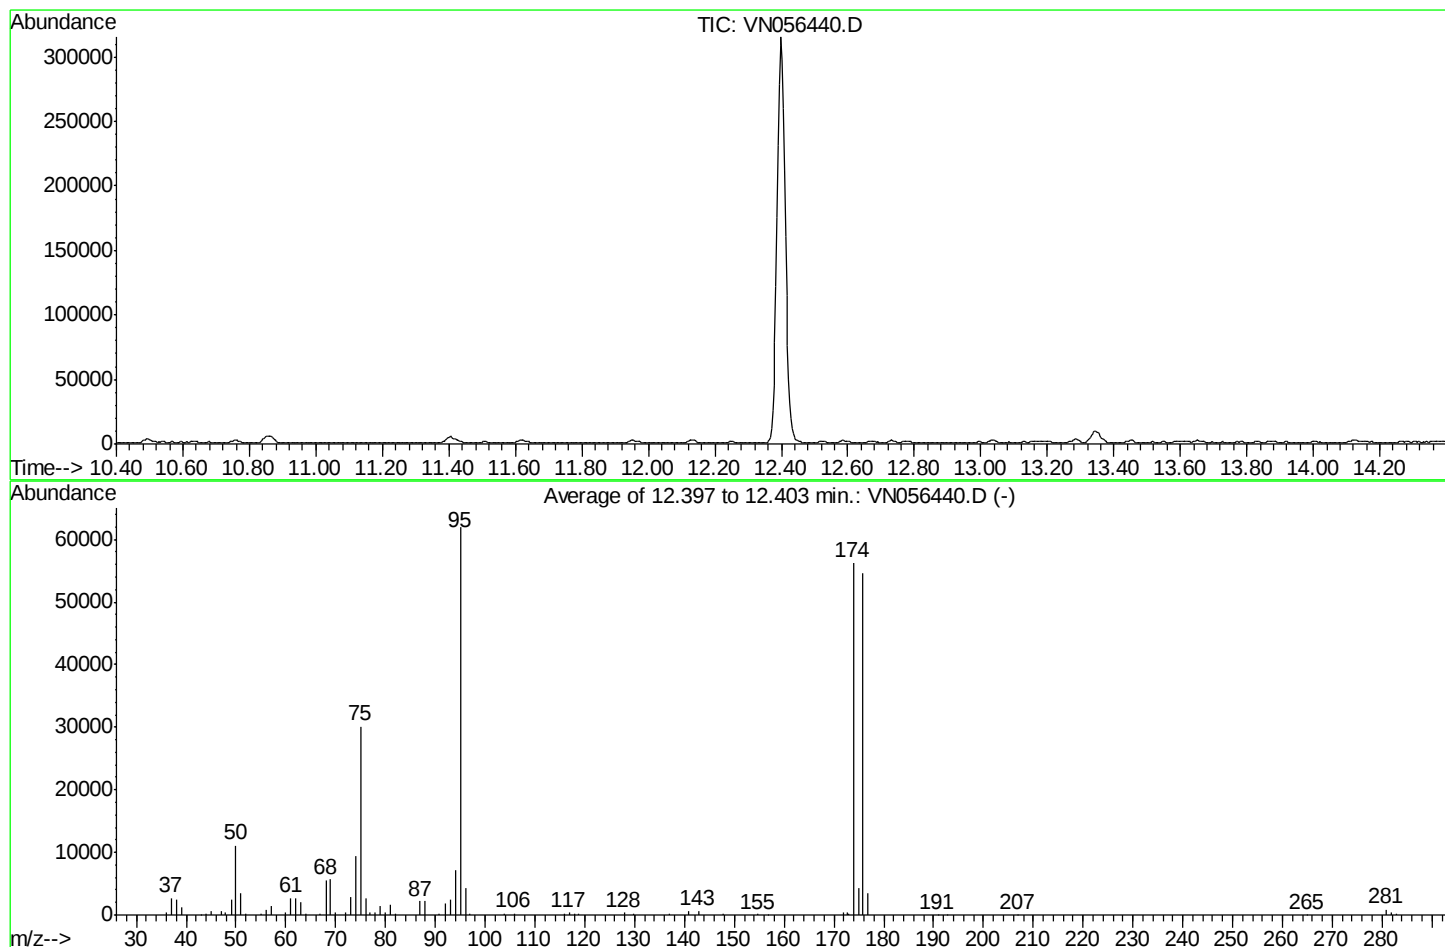

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3291

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.0	11118	PASS
75	95	30	60	48.6	30104	PASS
95	95	100	100	100.0	61928	PASS
96	95	5	9	6.8	4235	PASS
173	174	0.00	2	0.6	348	PASS
174	95	50	100	90.9	56280	PASS
175	174	5	9	7.7	4350	PASS
176	174	95	101	97.0	54613	PASS
177	176	5	9	6.4	3469	PASS