



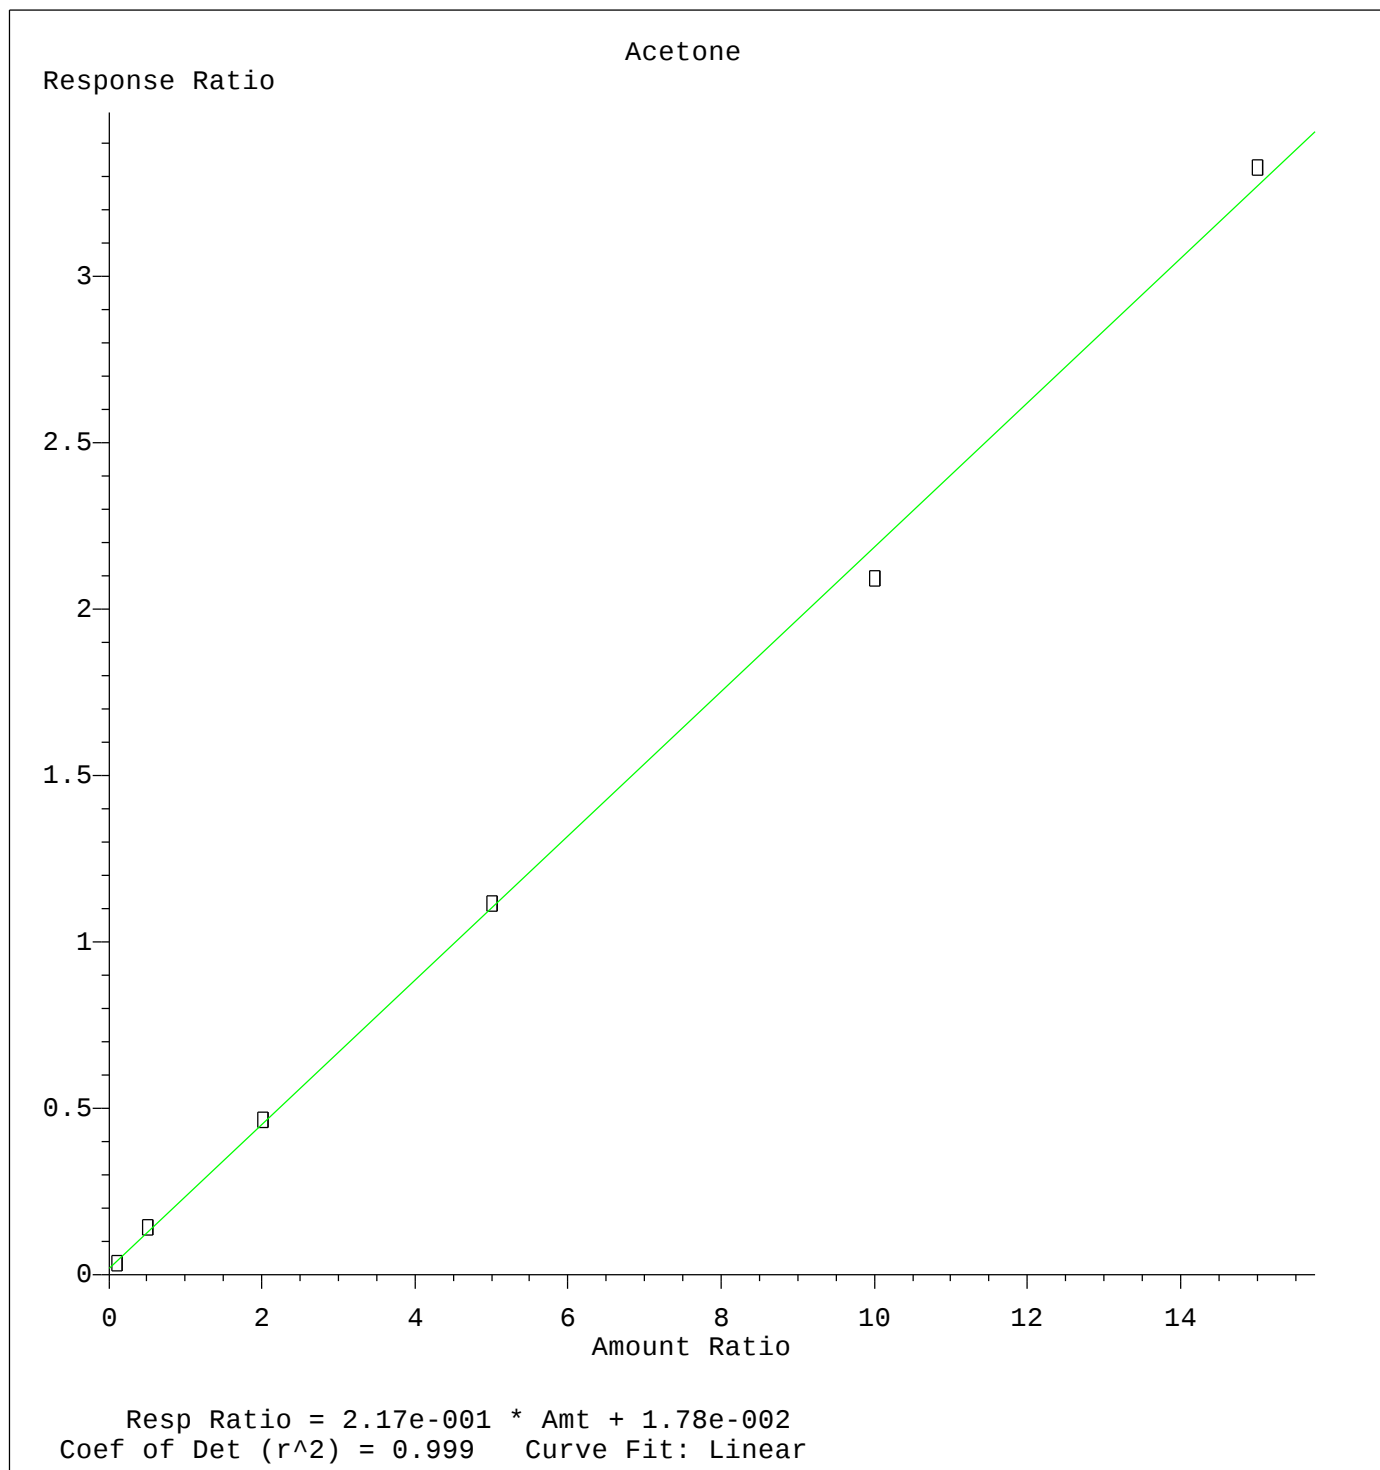


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N062420W.M
Calibration Table Last Updated: Wed Jun 24 15:33:00 2020

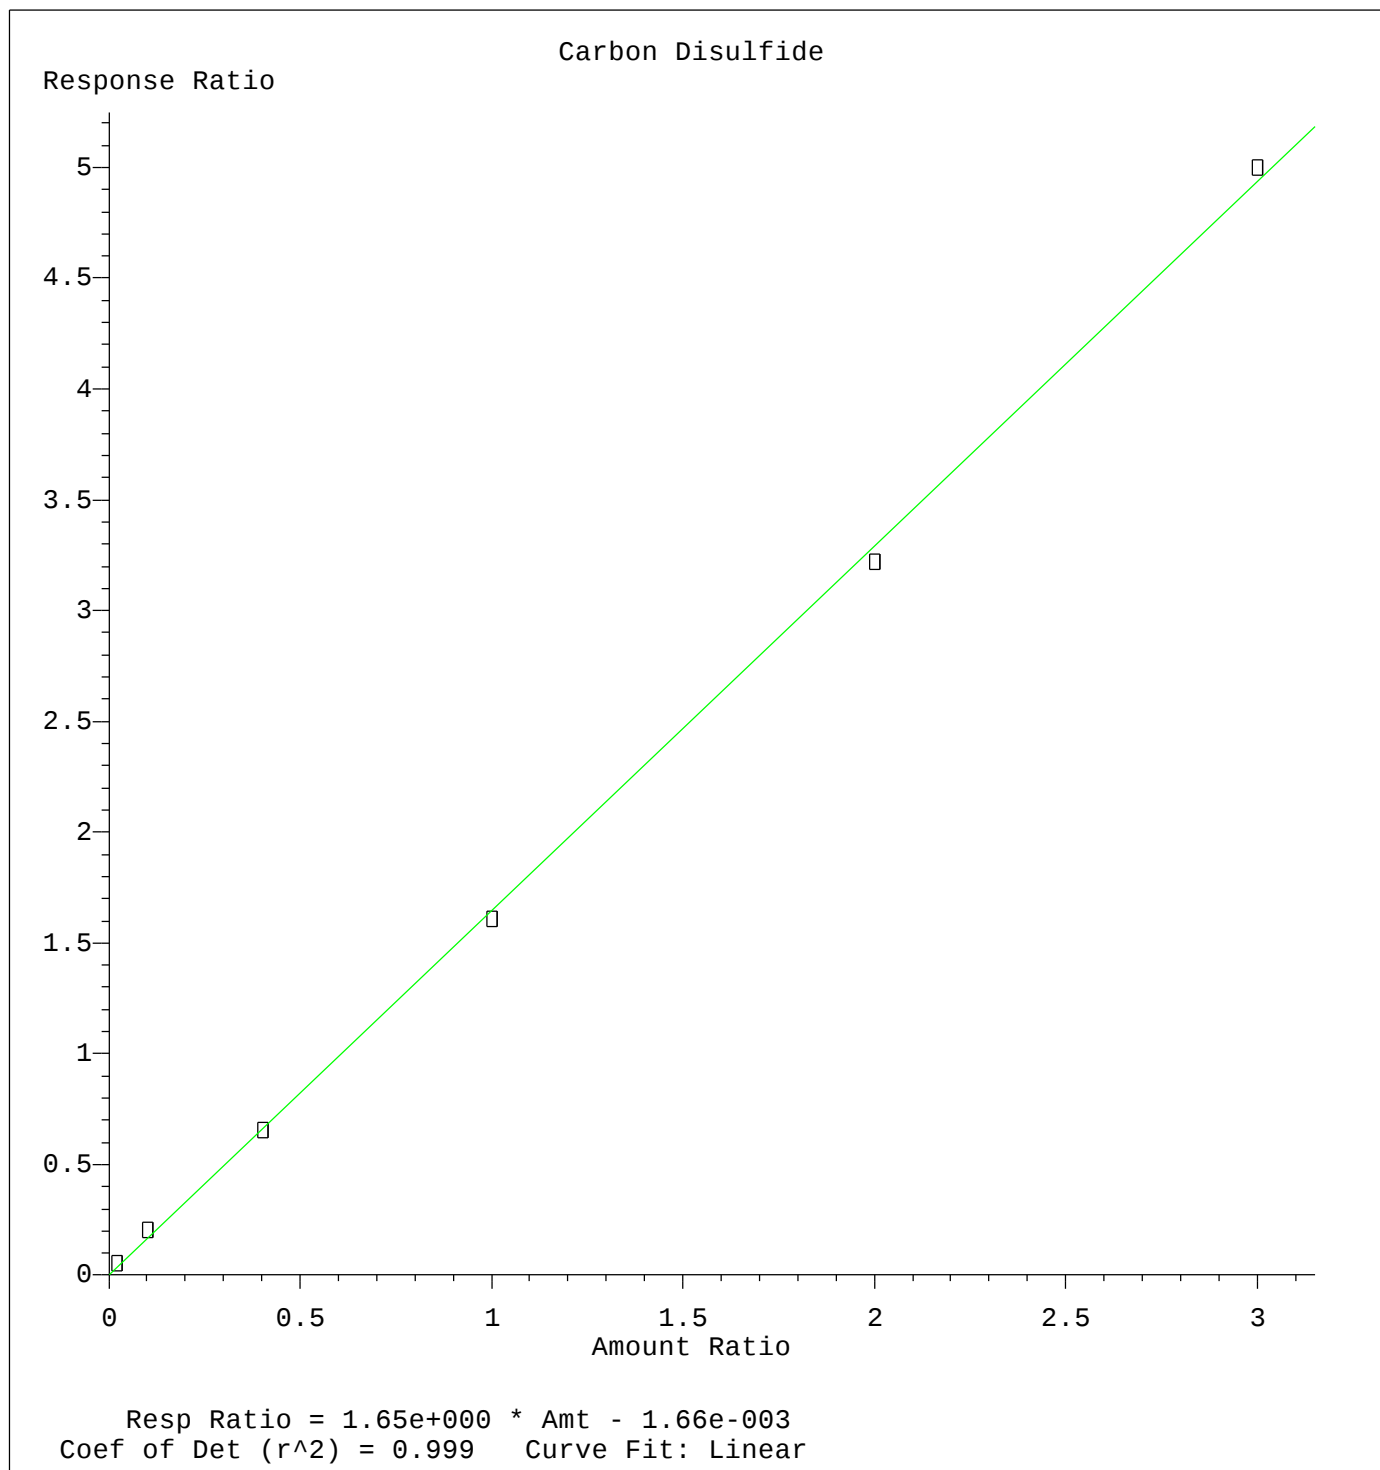

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N062420W.M
Calibration Table Last Updated: Wed Jun 24 15:33:00 2020

Methylene Chloride

Response Ratio

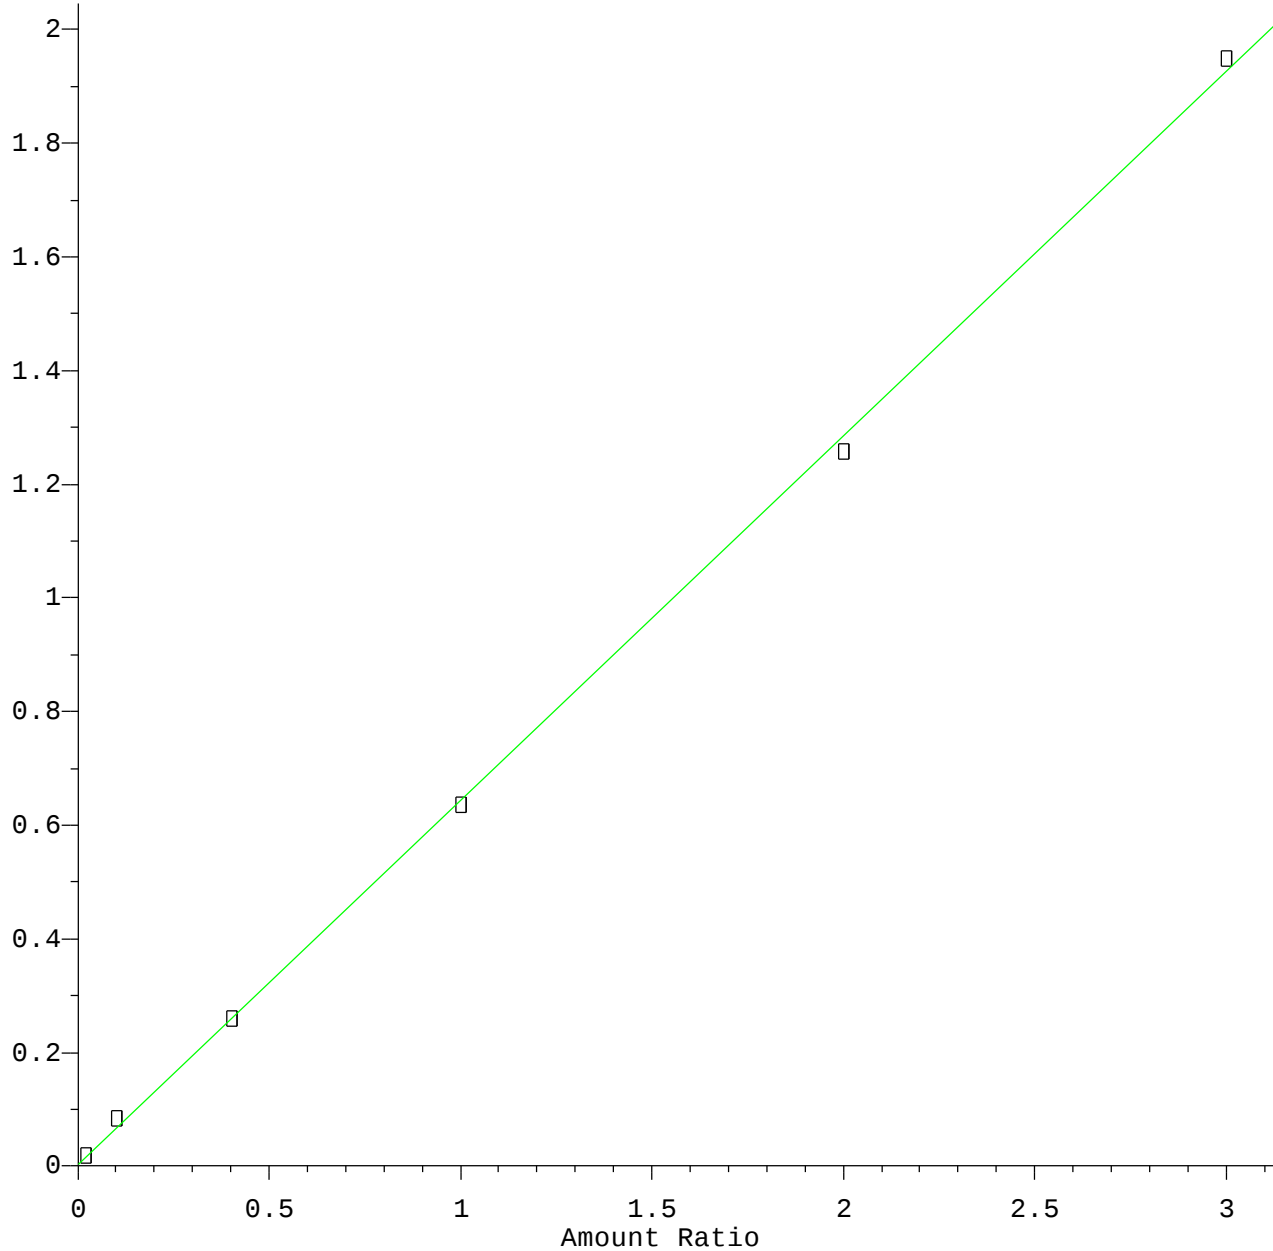


Resp Ratio = $6.41 \times 10^{-1} \times \text{Amt} + 2.79 \times 10^{-3}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N062420W.M
Calibration Table Last Updated: Wed Jun 24 15:33:00 2020


2-Chloroethyl Vinyl ether

Response Ratio

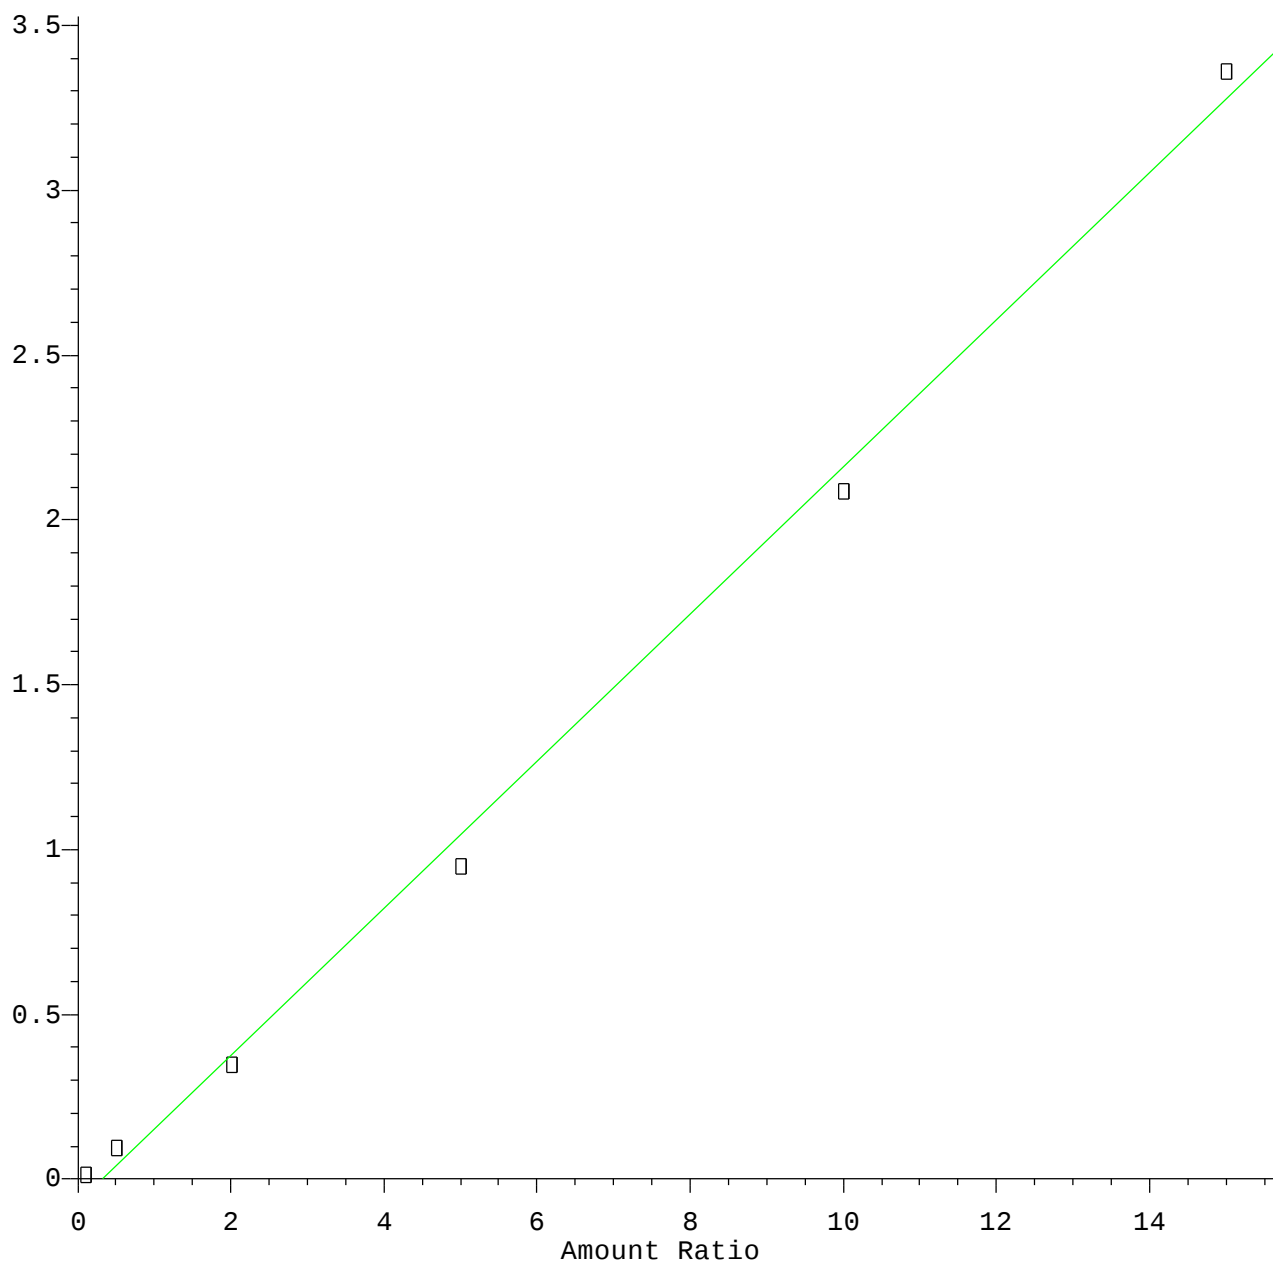

Resp Ratio = $2.23 \times 10^{-1} \times \text{Amt} - 7.19 \times 10^{-2}$
Coef of Det (r^2) = 0.997 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N062420W.M
Calibration Table Last Updated: Wed Jun 24 15:33:00 2020

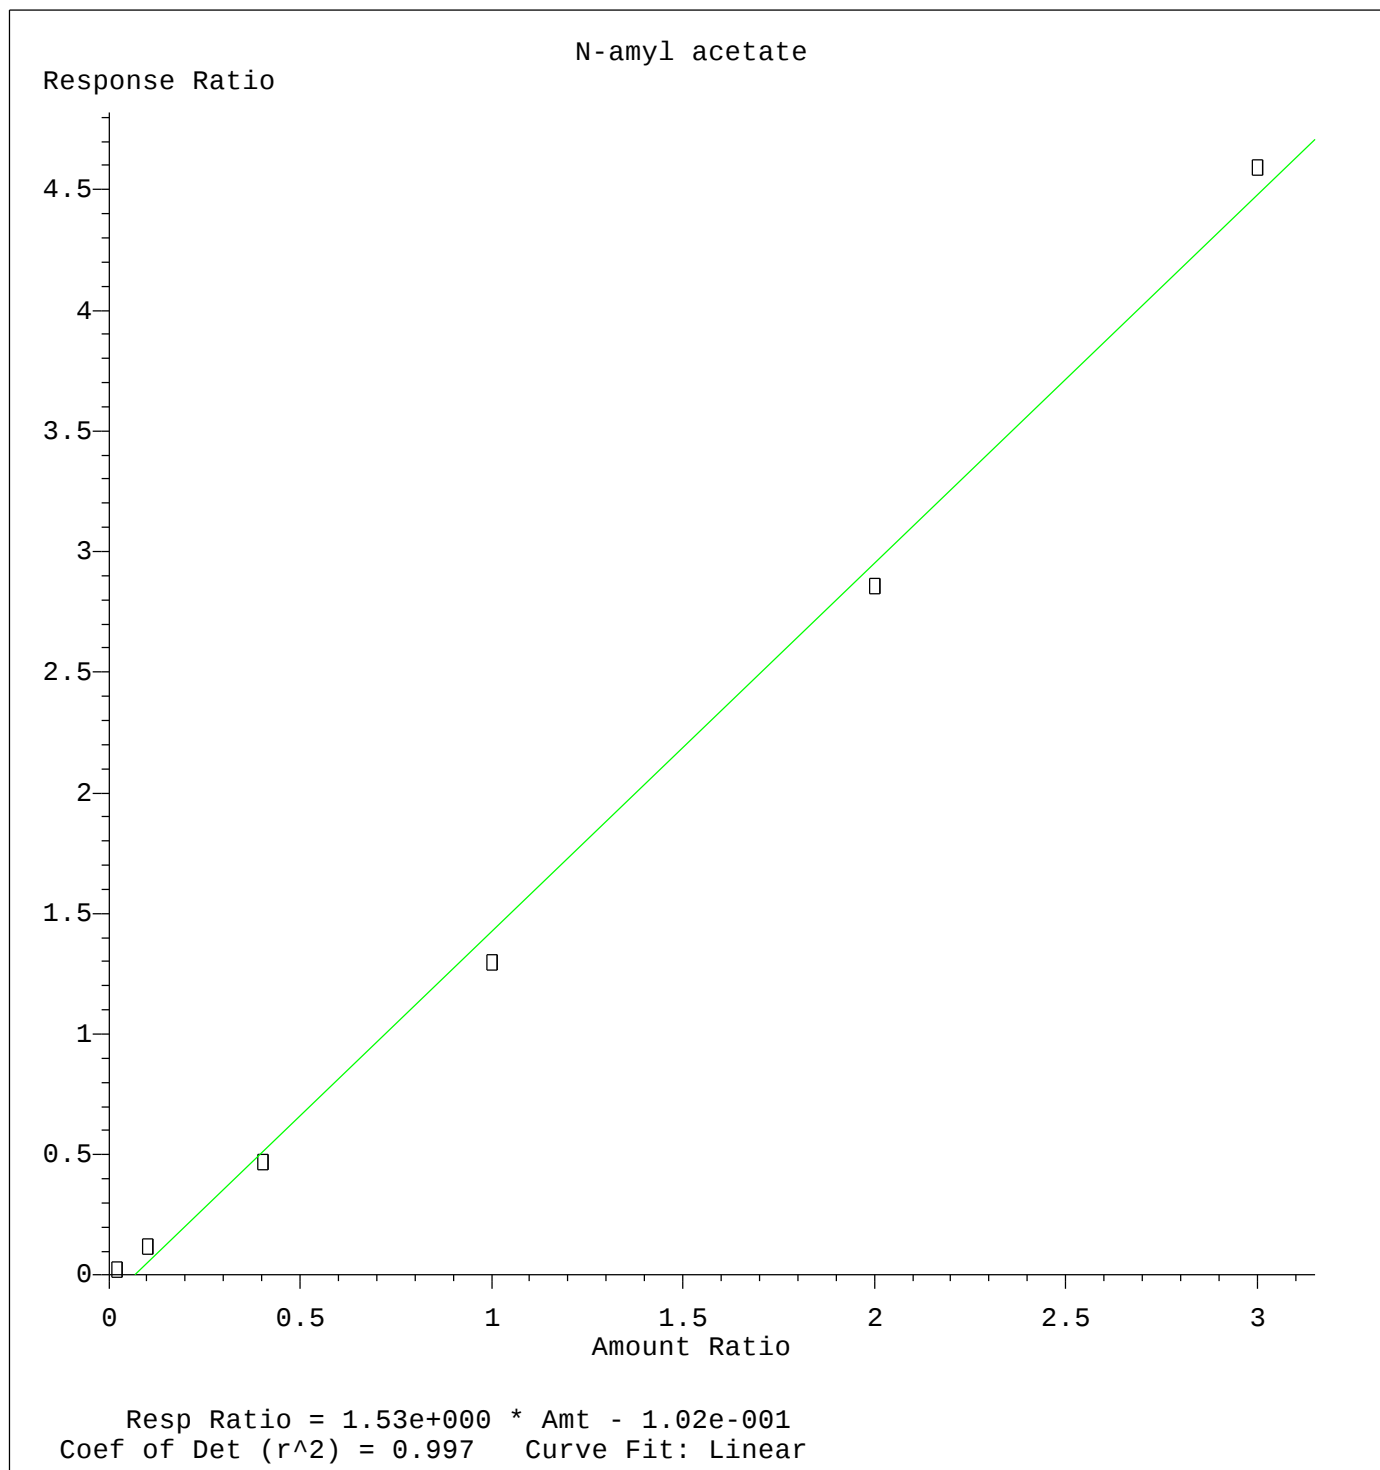

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N062420W.M
Calibration Table Last Updated: Wed Jun 24 15:33:00 2020


Naphthalene

Response Ratio

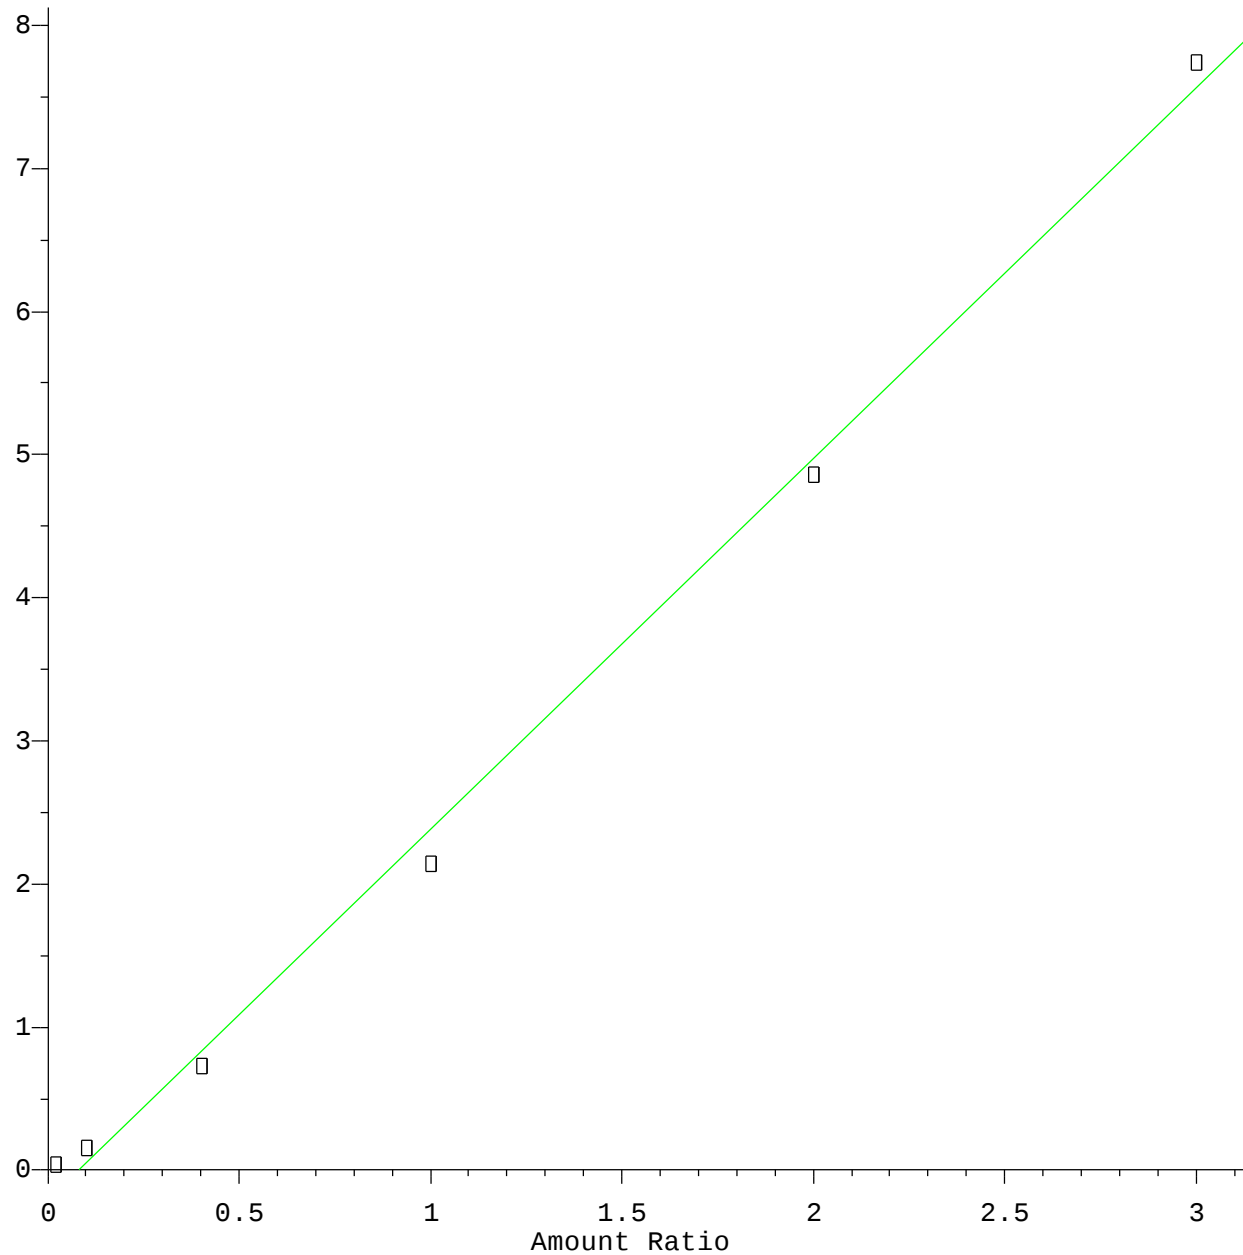

Resp Ratio = 2.59×10^0 * Amt - 2.07×10^{-1}
Coef of Det (r^2) = 0.997 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N062420W.M
Calibration Table Last Updated: Wed Jun 24 15:33:00 2020

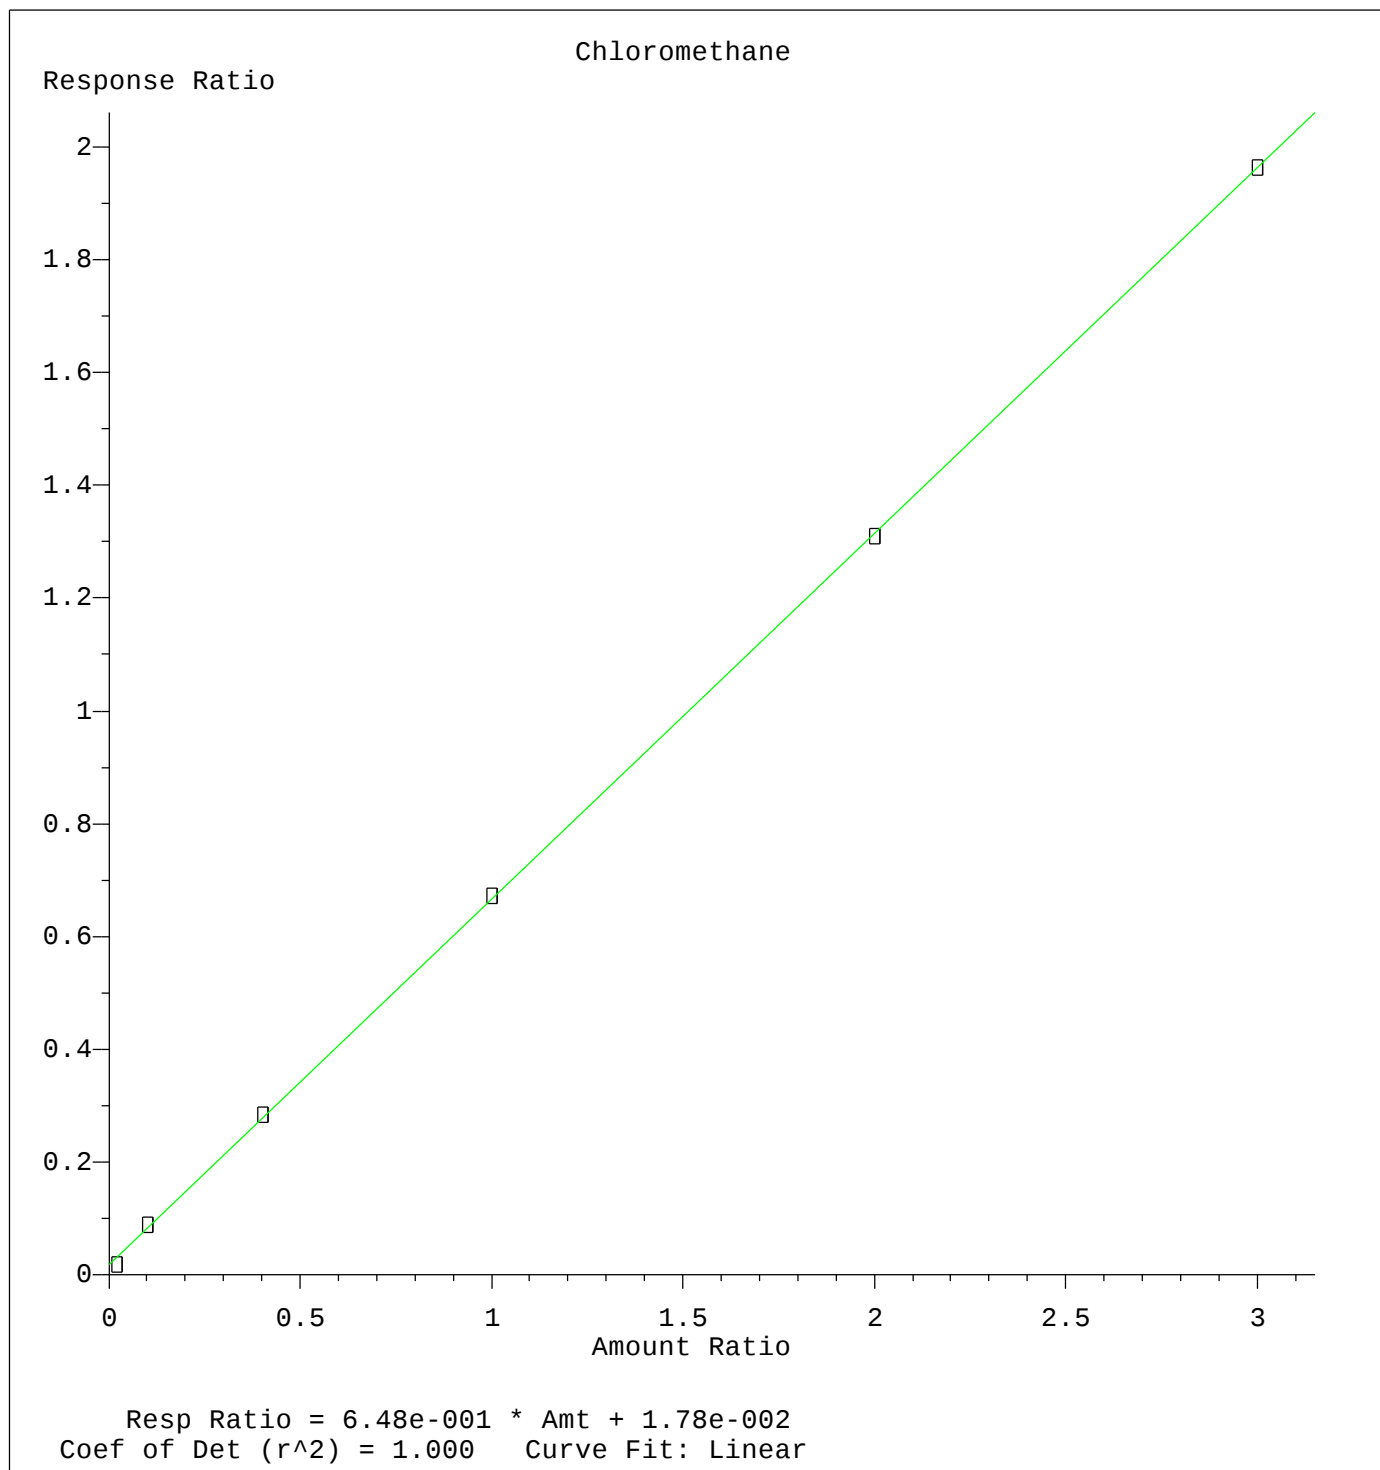

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N062420W.M
Calibration Table Last Updated: Wed Jun 24 15:09:49 2020