

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN062421\
 Data File : VN067484.D
 Acq On : 24 Jun 2021 15:42
 Operator : JC/MD
 Sample : M2746-02ME
 Misc : 10.85g/5mL/100uL/5.00mL/MSVOA_N/MEOH
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 NEW-DORP-2ME

Quant Time: Jun 25 02:14:28 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N062421W.M
 Quant Title : SW846 8260
 QLast Update : Thu Jun 24 12:18:45 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.080	168	231474	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.965	114	493885	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.749	117	460952	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.678	152	168757	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.434	65	229476	48.440	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	=	96.880%
35) Dibromofluoromethane	8.019	113	145866	47.940	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	=	95.880%
50) Toluene-d8	10.440	98	676186	52.105	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	=	104.200%
62) 4-Bromofluorobenzene	12.733	95	249289	53.916	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	=	107.840%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN062421\
Data File : VN067484.D
Acq On : 24 Jun 2021 15:42
Operator : JC/MD
Sample : M2746-02ME
Misc : 10.85g/5mL/100uL/5.00mL/MSVOA_N/MEOH
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
NEW-DORP-2ME

Quant Time: Jun 25 02:14:28 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N062421W.M
Quant Title : SW846 8260
QLast Update : Thu Jun 24 12:18:45 2021
Response via : Initial Calibration




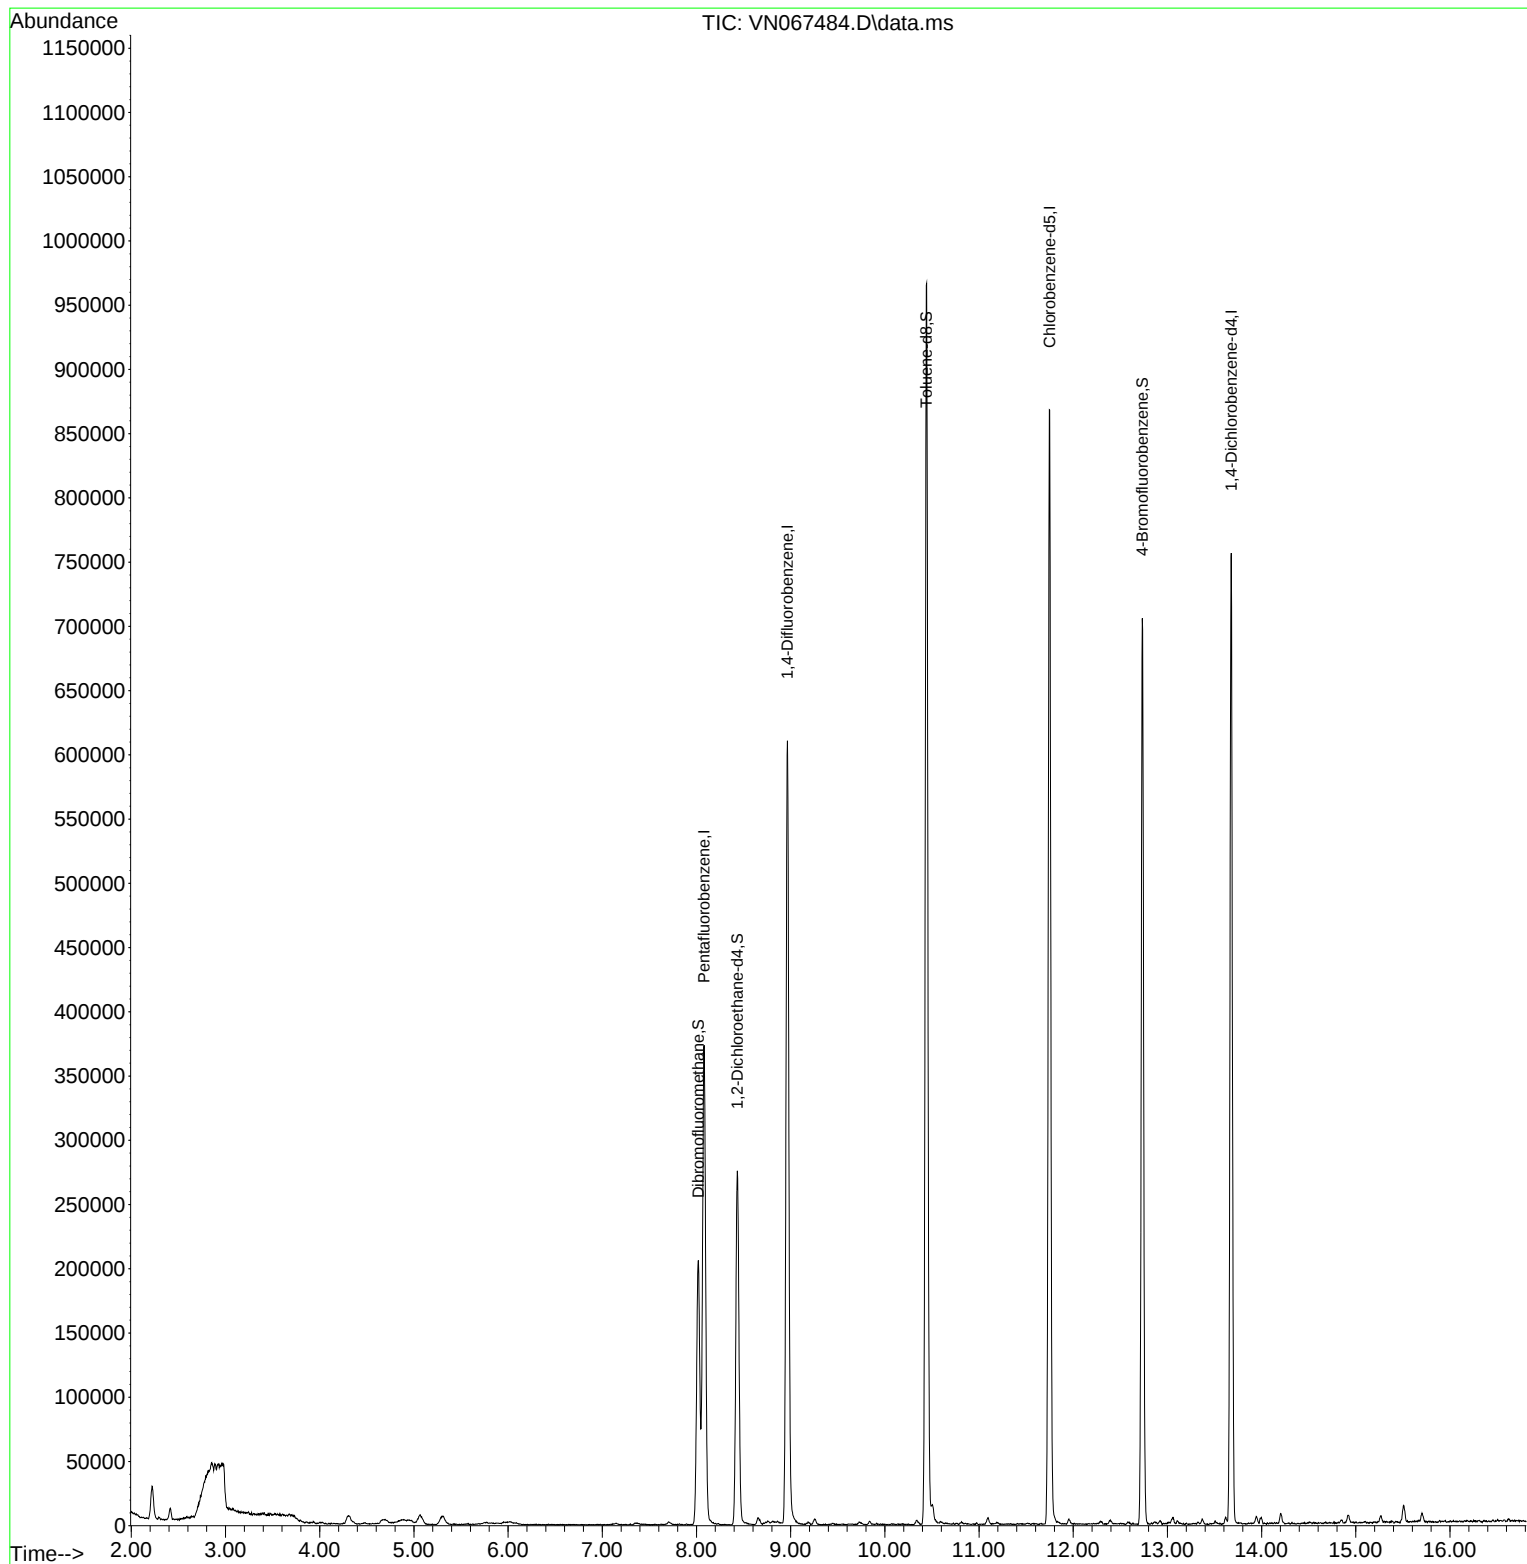


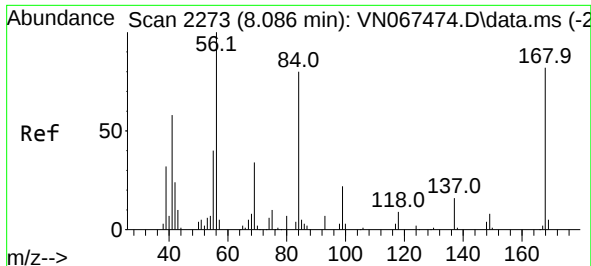

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.080 min Scan# 2271
Delta R.T. -0.006 min
Lab File: VN067484.D
Acq: 24 Jun 2021 15:42




Instrument :
MSVOA_N
ClientSampleId :
NEW-DORP-2ME


Tgt Ion:168 Resp: 231474
Ion Ratio Lower Upper
168 100
99 79.5 62.9 94.3

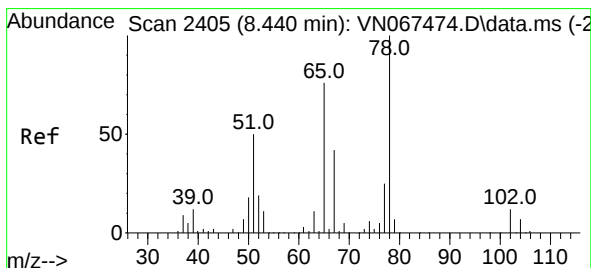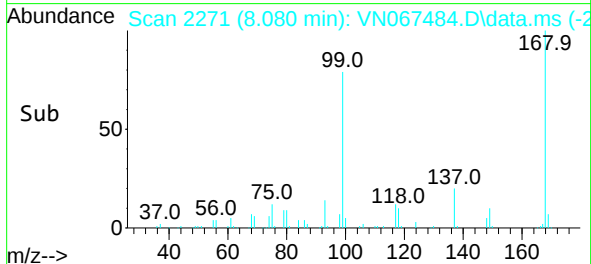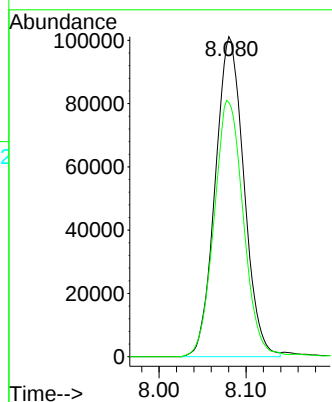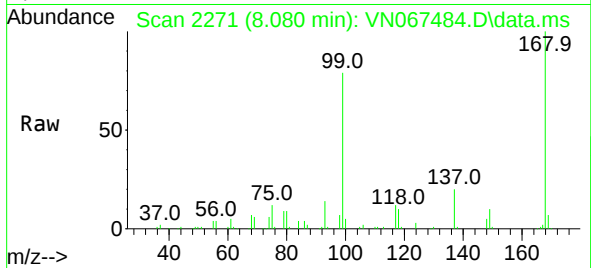

#33
1,2-Dichloroethane-d4
Concen: 48.440 ug/l
RT: 8.434 min Scan# 2403
Delta R.T. -0.006 min
Lab File: VN067484.D
Acq: 24 Jun 2021 15:42

Tgt Ion: 65 Resp: 229476
Ion Ratio Lower Upper
65 100
67 52.8 0.0 98.6


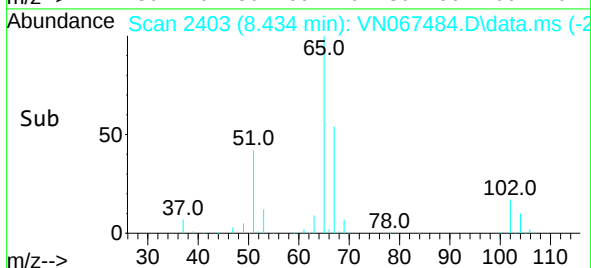
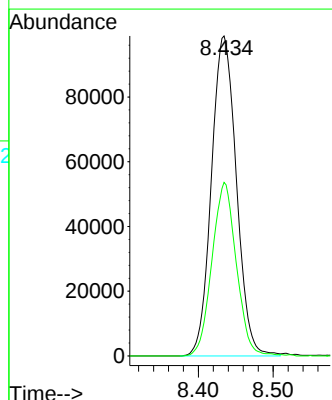
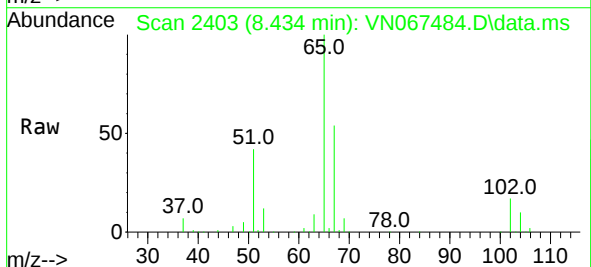


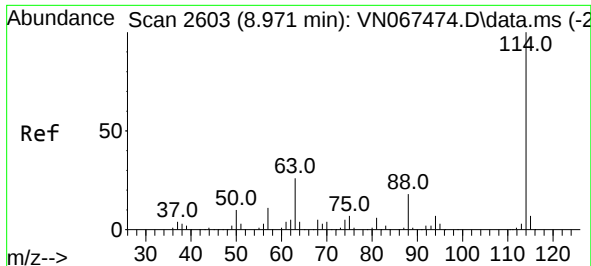

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.965 min Scan# 2601
Delta R.T. -0.006 min
Lab File: VN067484.D
Acq: 24 Jun 2021 15:42




Instrument :
MSVOA_N
ClientSampleId :
NEW-DORP-2ME


Tgt Ion:114 Resp: 493885
Ion Ratio Lower Upper
114 100
63 25.2 0.0 49.0
88 17.3 0.0 36.6

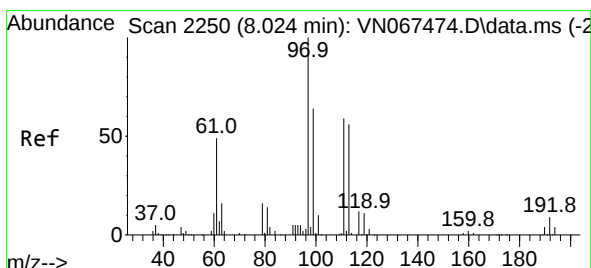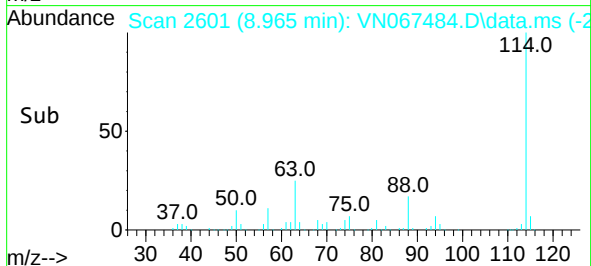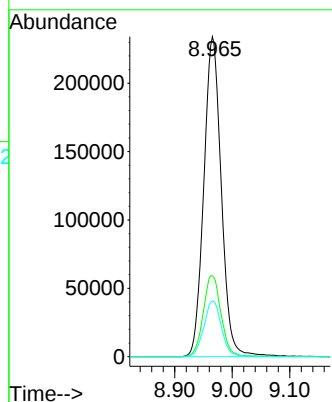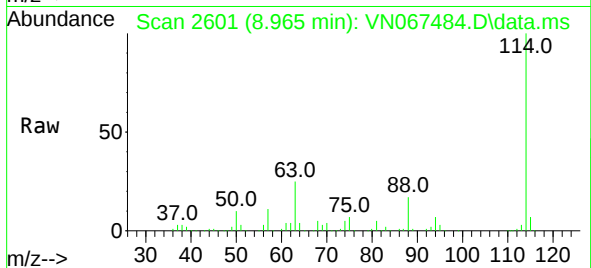

#35
Dibromofluoromethane
Concen: 47.940 ug/l
RT: 8.019 min Scan# 2248
Delta R.T. -0.005 min
Lab File: VN067484.D
Acq: 24 Jun 2021 15:42

Tgt Ion:113 Resp: 145866
Ion Ratio Lower Upper
113 100
111 105.5 83.8 125.8
192 14.5 13.4 20.0


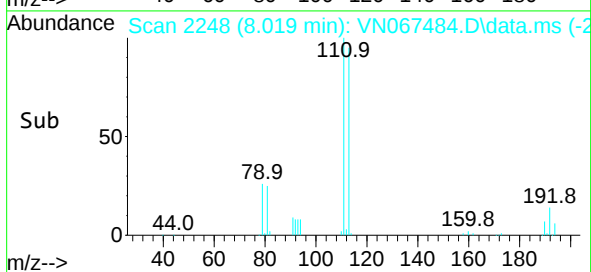
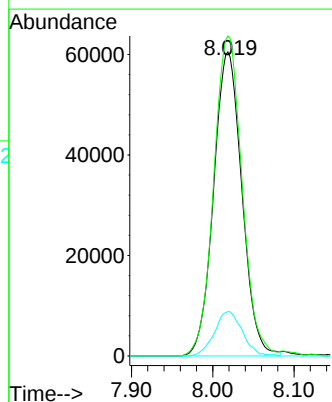
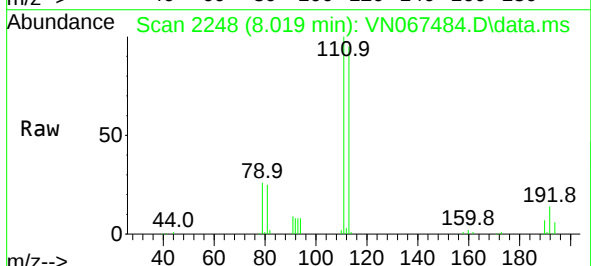


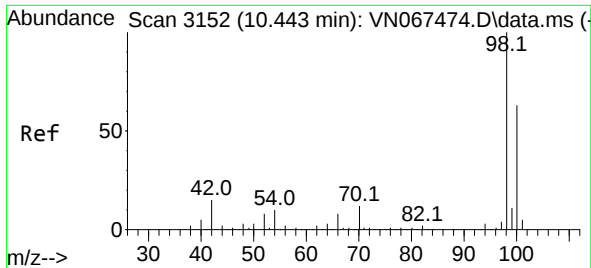

#50
Toluene-d8
Concen: 52.105 ug/l
RT: 10.440 min Scan# 3151
Delta R.T. -0.003 min
Lab File: VN067484.D
Acq: 24 Jun 2021 15:42




Instrument :
MSVOA_N
ClientSampleId :
NEW-DORP-2ME


Tgt Ion: 98 Resp: 676186
Ion Ratio Lower Upper
98 100
100 61.8 51.7 77.5

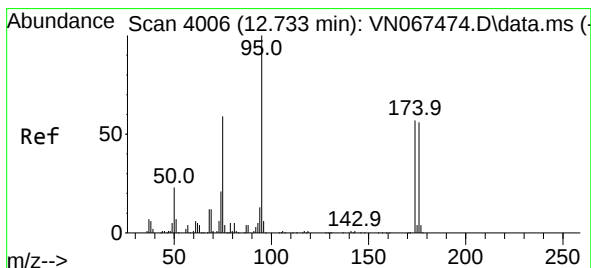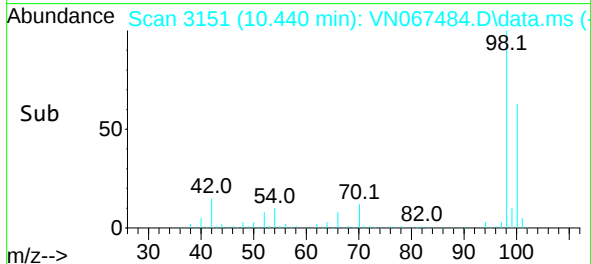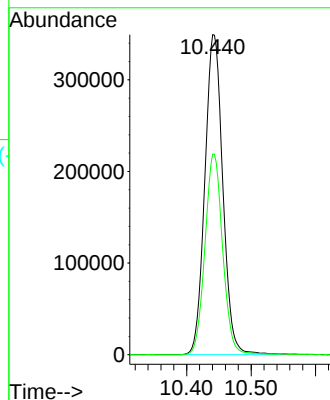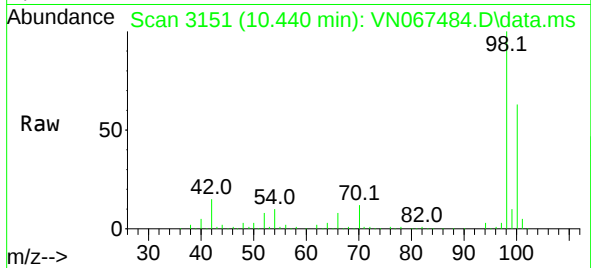

#62
4-Bromofluorobenzene
Concen: 53.916 ug/l
RT: 12.733 min Scan# 4006
Delta R.T. 0.000 min
Lab File: VN067484.D
Acq: 24 Jun 2021 15:42

Tgt Ion: 95 Resp: 249289
Ion Ratio Lower Upper
95 100
174 55.2 0.0 122.0
176 53.3 0.0 117.6


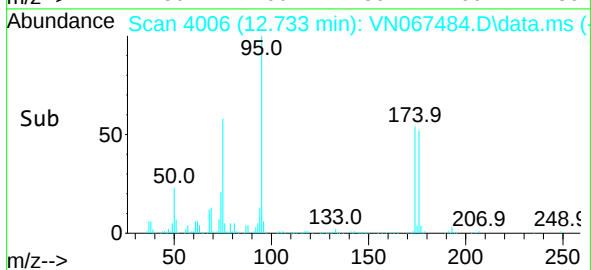
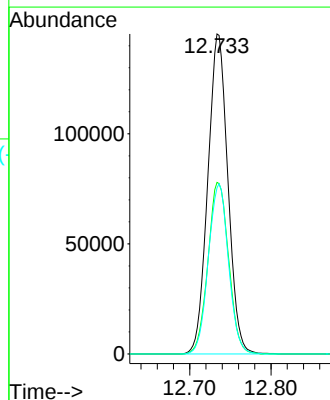
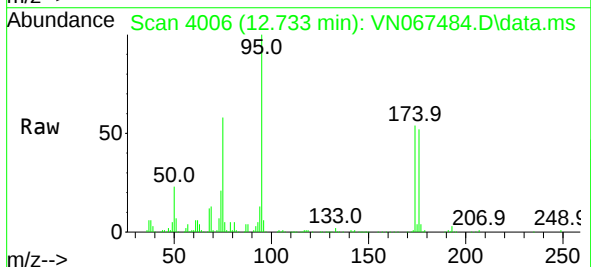


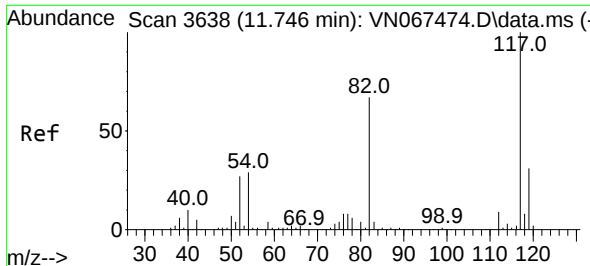

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.749 min Scan# 3639
Delta R.T. 0.003 min
Lab File: VN067484.D
Acq: 24 Jun 2021 15:42

Instrument :
MSVOA_N
ClientSampleId :
NEW-DORP-2ME

Tgt Ion:117 Resp: 460952
Ion Ratio Lower Upper
117 100
82 67.5 53.1 79.7
119 31.6 25.5 38.3

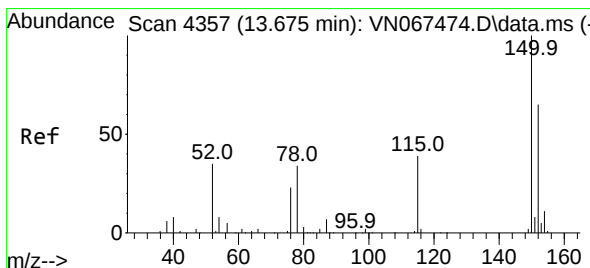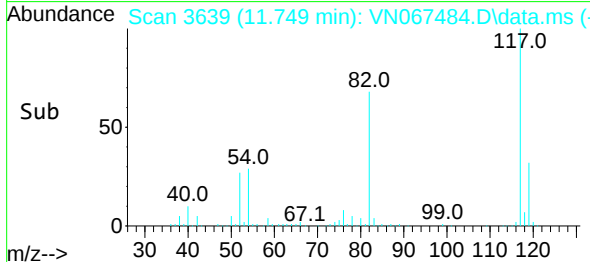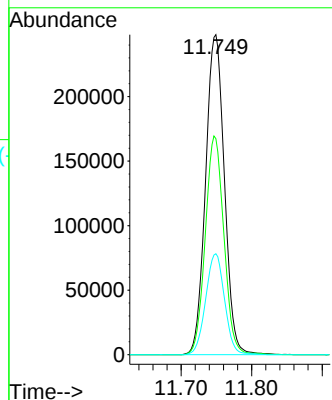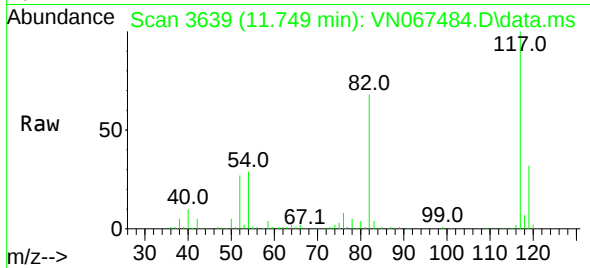

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.678 min Scan# 4358
Delta R.T. 0.003 min
Lab File: VN067484.D
Acq: 24 Jun 2021 15:42

Tgt Ion:152 Resp: 168757
Ion Ratio Lower Upper
152 100
115 71.8 36.1 108.5
150 158.0 0.0 351.8

