

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN062422\
 Data File : VN073079.D
 Acq On : 24 Jun 2022 13:09
 Operator : JC\MD
 Sample : N3376-02
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 220615002-01-TRIP-BLANK

Quant Time: Jun 24 23:33:54 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N062322W.M
 Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 QLast Update : Fri Jun 24 04:54:59 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	7.586	128	40713	30.000	ug/l	0.00
28) 1,4-Difluorobenzene	8.904	114	227591	30.000	ug/l	0.00
57) Chlorobenzene-d5	11.680	117	186800	30.000	ug/l	0.00
System Monitoring Compounds						
27) 1,2-Dichloroethane-d4	8.369	65	118935	30.304	ug/l	0.00
Spiked Amount	30.000	Range	91 - 110	Recovery	=	101.000%
60) 4-Bromofluorobenzene	12.668	95	97614	27.313	ug/l	0.00
Spiked Amount	30.000	Range	63 - 112	Recovery	=	91.033%
63) Toluene-d8	10.375	98	319967	31.631	ug/l	0.00
Spiked Amount	30.000	Range	91 - 112	Recovery	=	105.433%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN062422\
Data File : VN073079.D
Acq On : 24 Jun 2022 13:09
Operator : JC\MD
Sample : N3376-02
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
220615002-01-TRIP-BLANK

Quant Time: Jun 24 23:33:54 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N062322W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
QLast Update : Fri Jun 24 04:54:59 2022
Response via : Initial Calibration




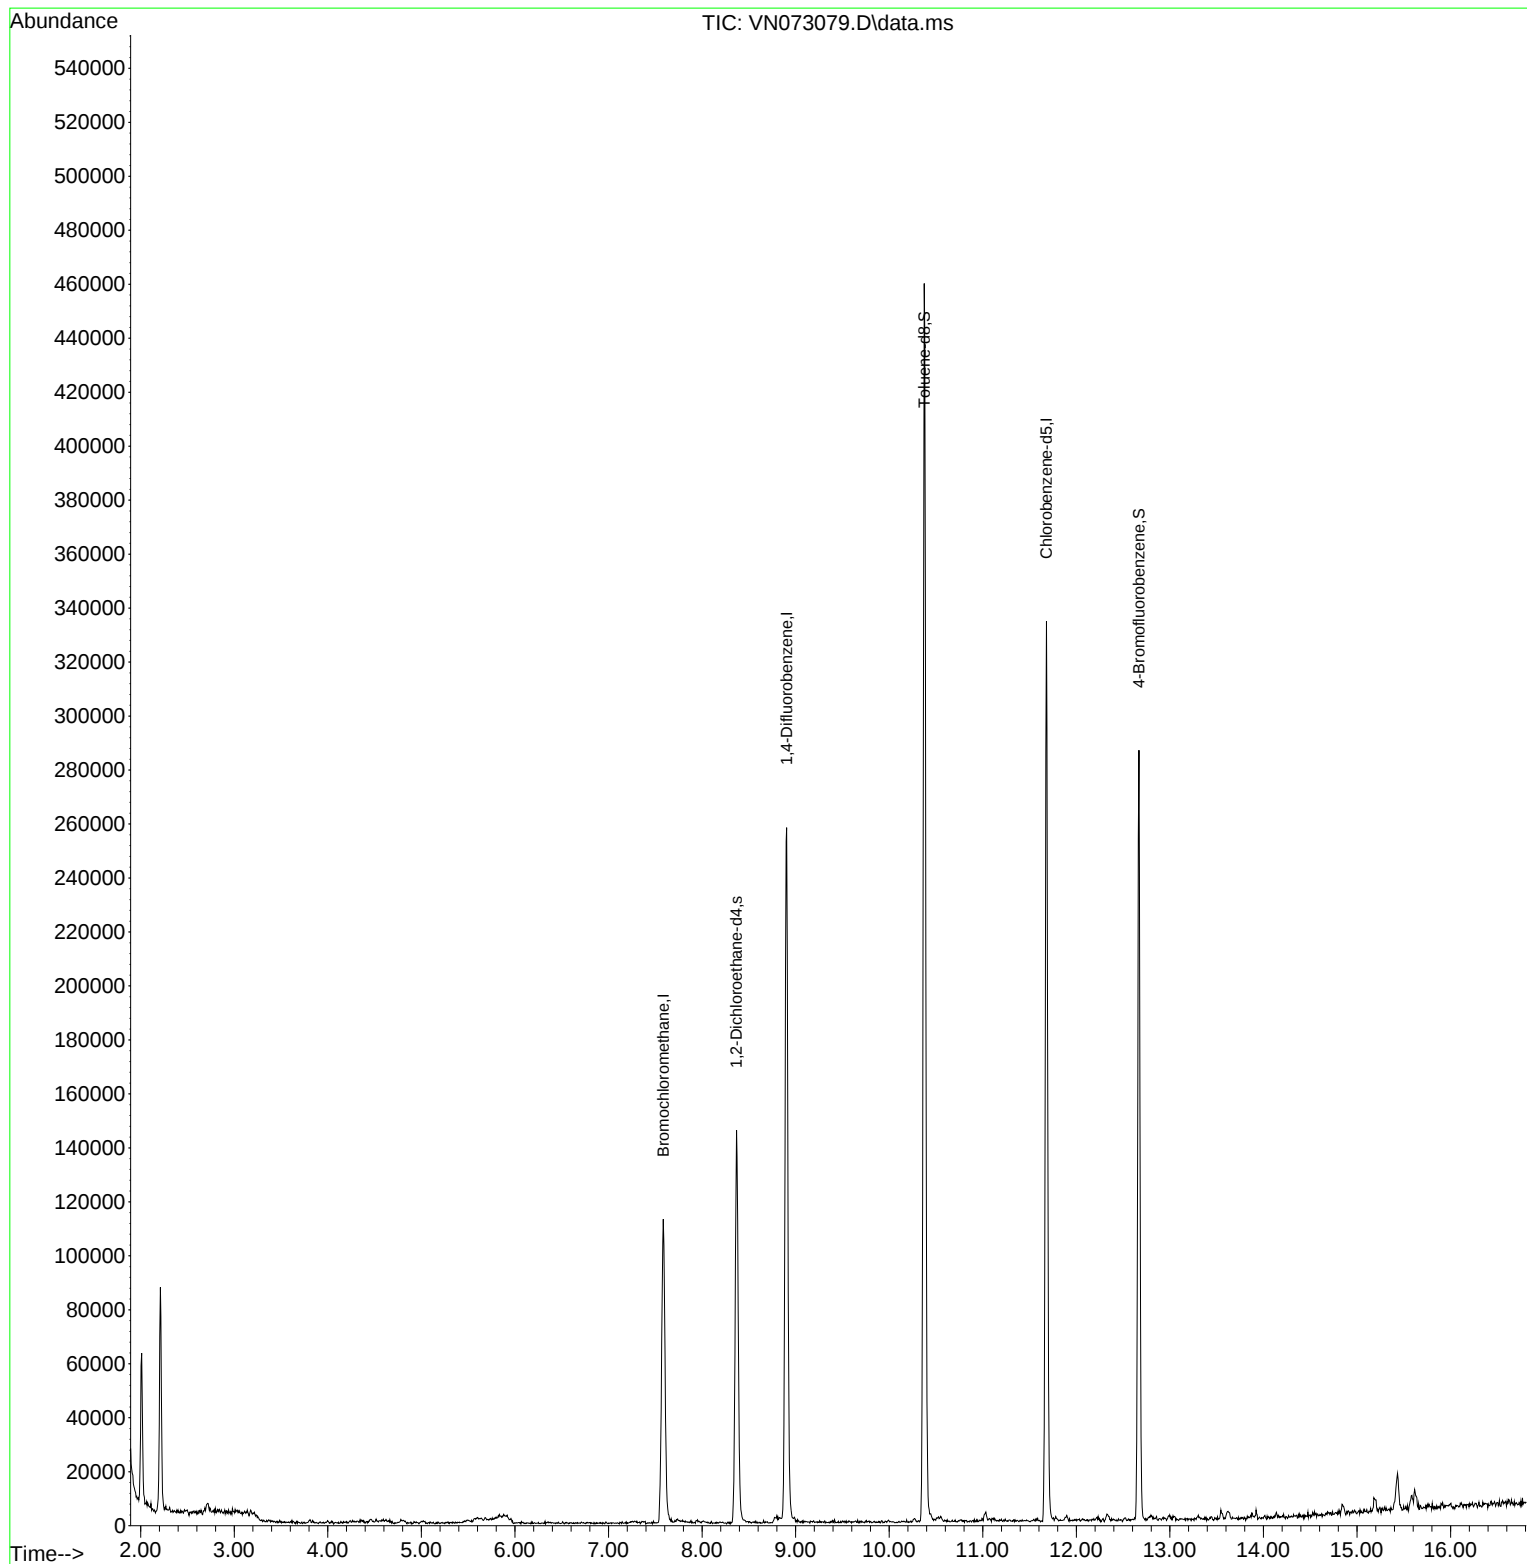


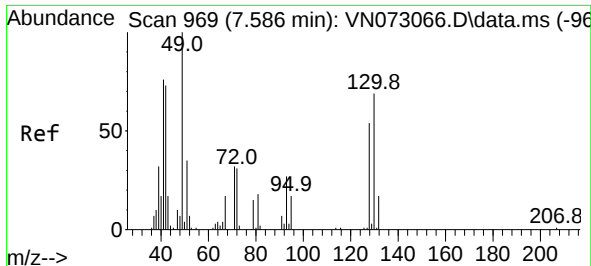

#1
Bromochloromethane
Concen: 30.000 ug/l
RT: 7.586 min Scan# 969
Delta R.T. 0.000 min
Lab File: VN073079.D
Acq: 24 Jun 2022 13:09




Instrument :
MSVOA_N
ClientSampleId :
220615002-01-TRIP-BLANK


Tgt Ion:128 Resp: 40713
Ion Ratio Lower Upper
128 100
49 172.6 0.0 392.3
130 128.2 0.0 320.2

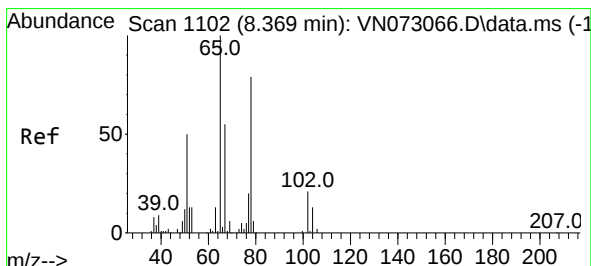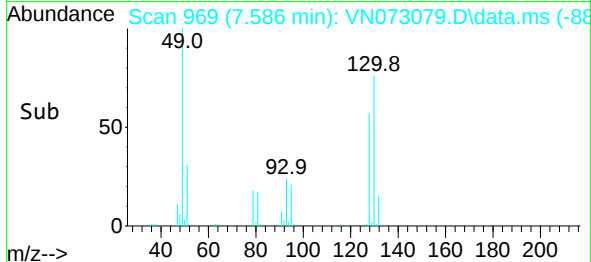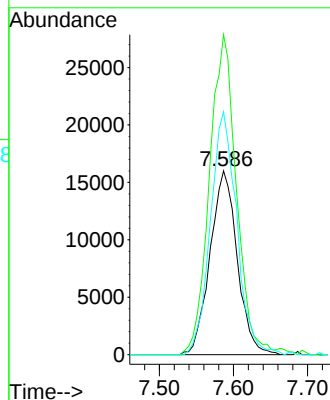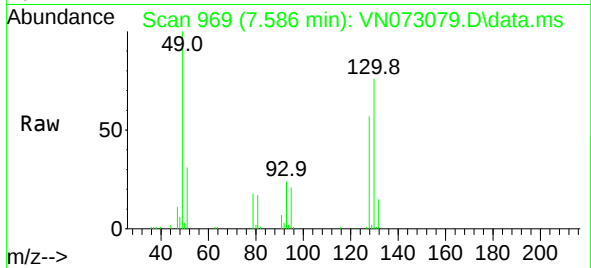

#27
1,2-Dichloroethane-d4
Concen: 30.304 ug/l
RT: 8.369 min Scan# 1102
Delta R.T. 0.000 min
Lab File: VN073079.D
Acq: 24 Jun 2022 13:09

Tgt Ion: 65 Resp: 118935
Ion Ratio Lower Upper
65 100
67 51.7 40.2 60.2

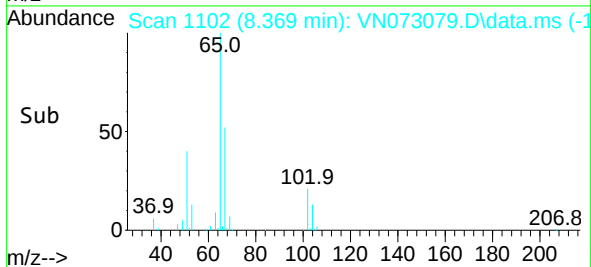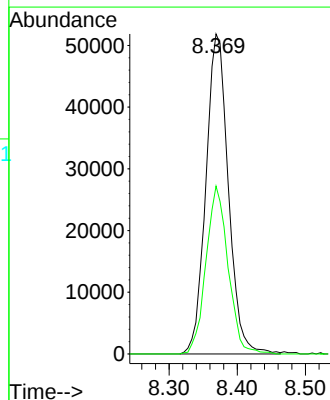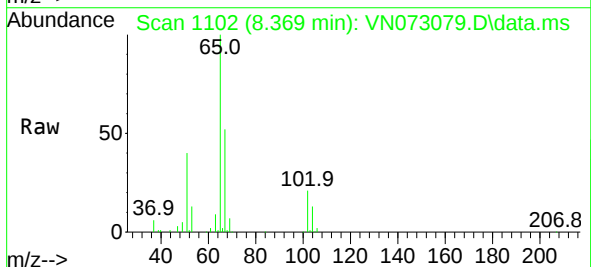

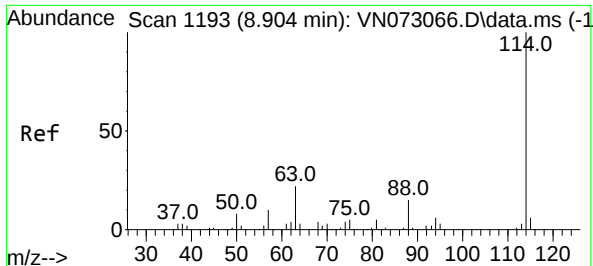

#28

1,4-Difluorobenzene

Concen: 30.000 ug/l

RT: 8.904 min Scan# 1193

Delta R.T. 0.000 min

Lab File: VN073079.D

Acq: 24 Jun 2022 13:09

Instrument :

MSVOA_N

ClientSampleId :

220615002-01-TRIP-BLANK





Tgt Ion:114 Resp: 227591

Ion Ratio Lower Upper

114 100

63 20.9 15.8 23.6

88 15.7 11.6 17.4

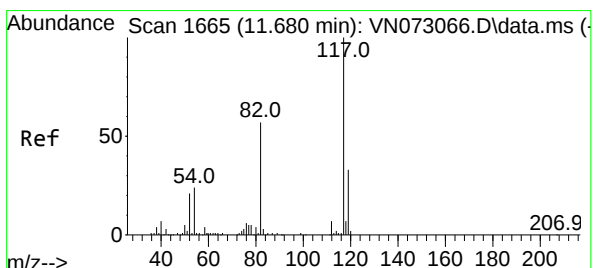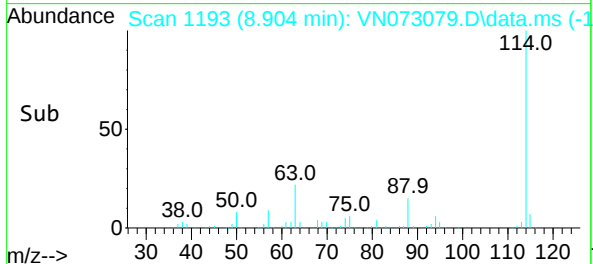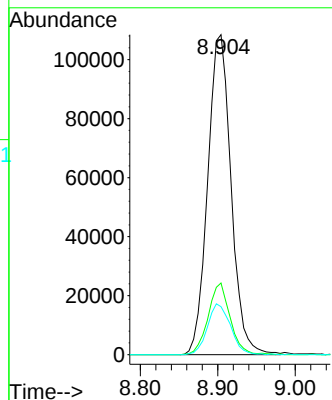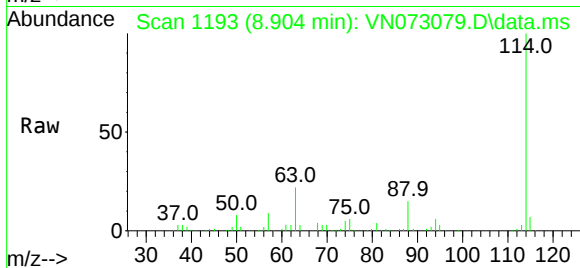

#57

Chlorobenzene-d5

Concen: 30.000 ug/l

RT: 11.680 min Scan# 1665

Delta R.T. 0.000 min

Lab File: VN073079.D

Acq: 24 Jun 2022 13:09




Tgt Ion:117 Resp: 186800


Ion Ratio Lower Upper

117 100

82 56.4 43.6 65.4

119 32.5 25.8 38.6


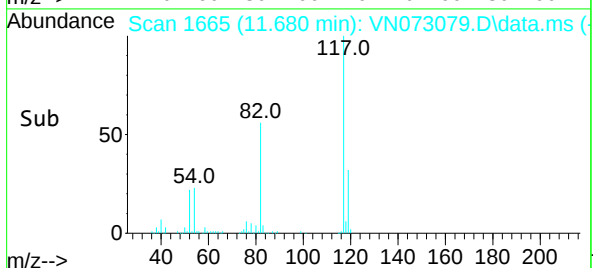
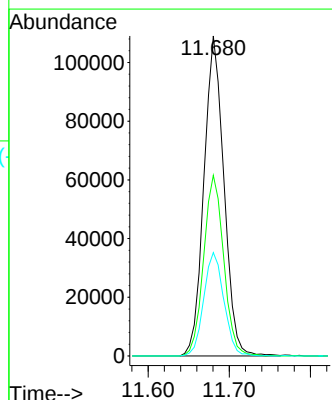
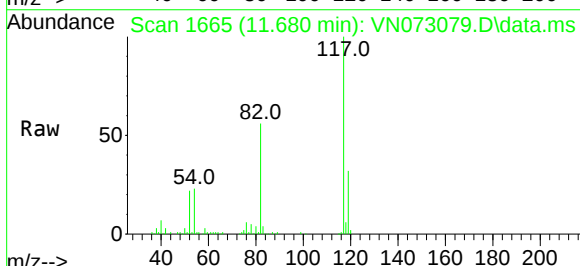


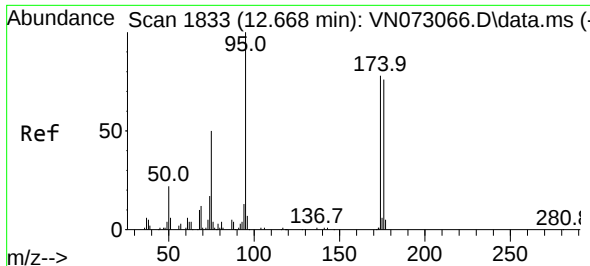

#60
4-Bromofluorobenzene
Concen: 27.313 ug/l
RT: 12.668 min Scan# 1833
Delta R.T. 0.000 min
Lab File: VN073079.D
Acq: 24 Jun 2022 13:09

Instrument :
MSVOA_N
ClientSampleId :
220615002-01-TRIP-BLANK

Tgt Ion: 95 Resp: 97614
Ion Ratio Lower Upper
95 100
174 76.6 62.9 94.3
176 73.0 61.0 91.4

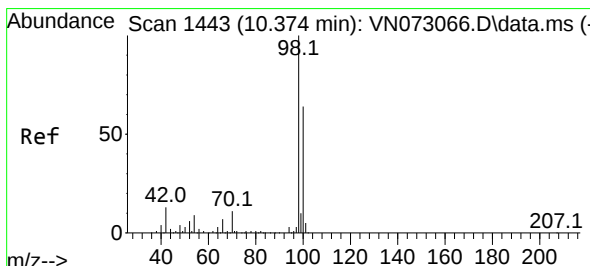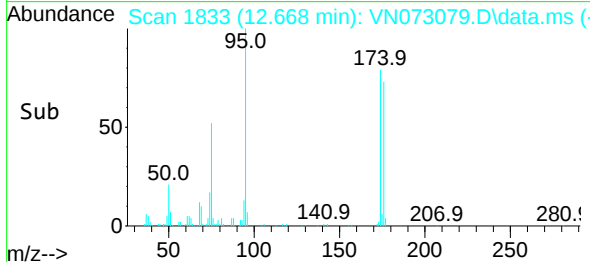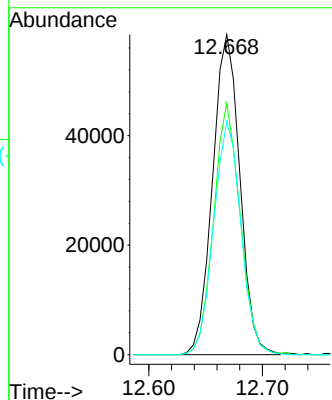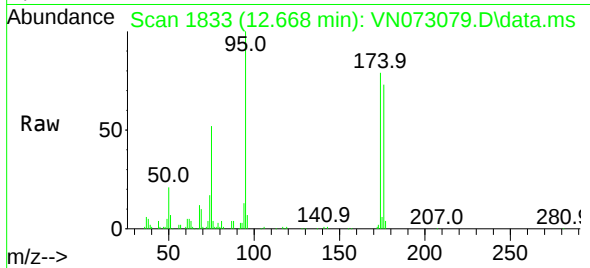

#63
Toluene-d8
Concen: 31.631 ug/l
RT: 10.375 min Scan# 1443
Delta R.T. 0.000 min
Lab File: VN073079.D
Acq: 24 Jun 2022 13:09

Tgt Ion: 98 Resp: 319967
Ion Ratio Lower Upper
98 100
100 65.1 50.6 76.0

