
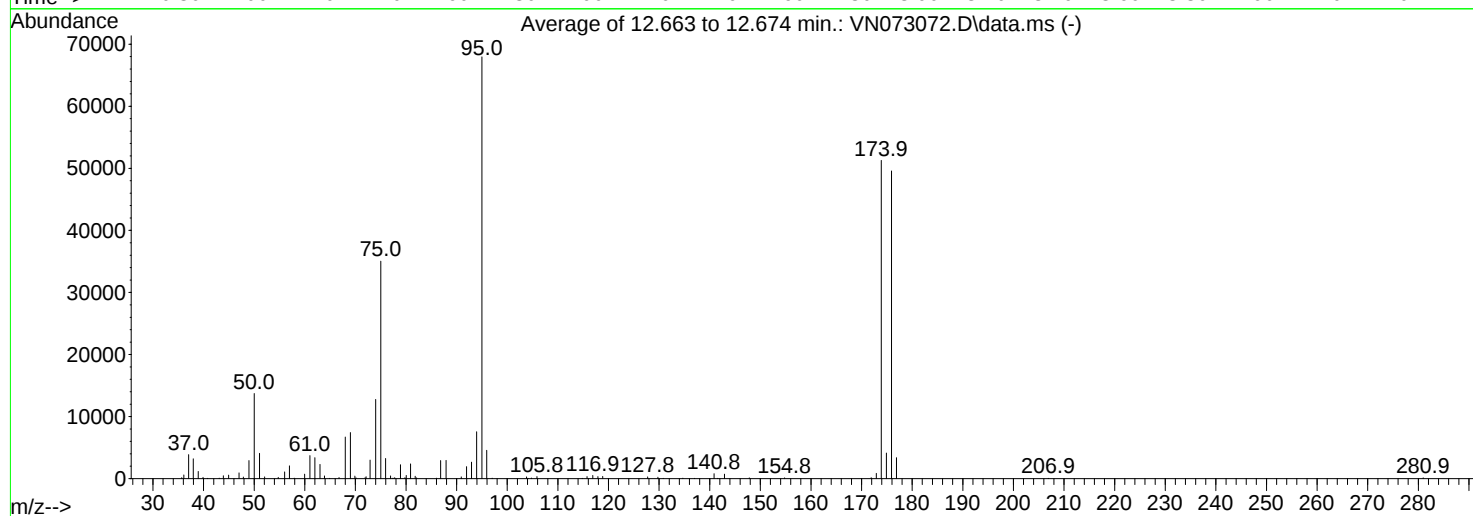


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN062422\
 Data File : VN073072.D
 Acq On : 24 Jun 2022 09:31
 Operator : JC\MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N062322W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Fri Jun 24 04:54:59 2022

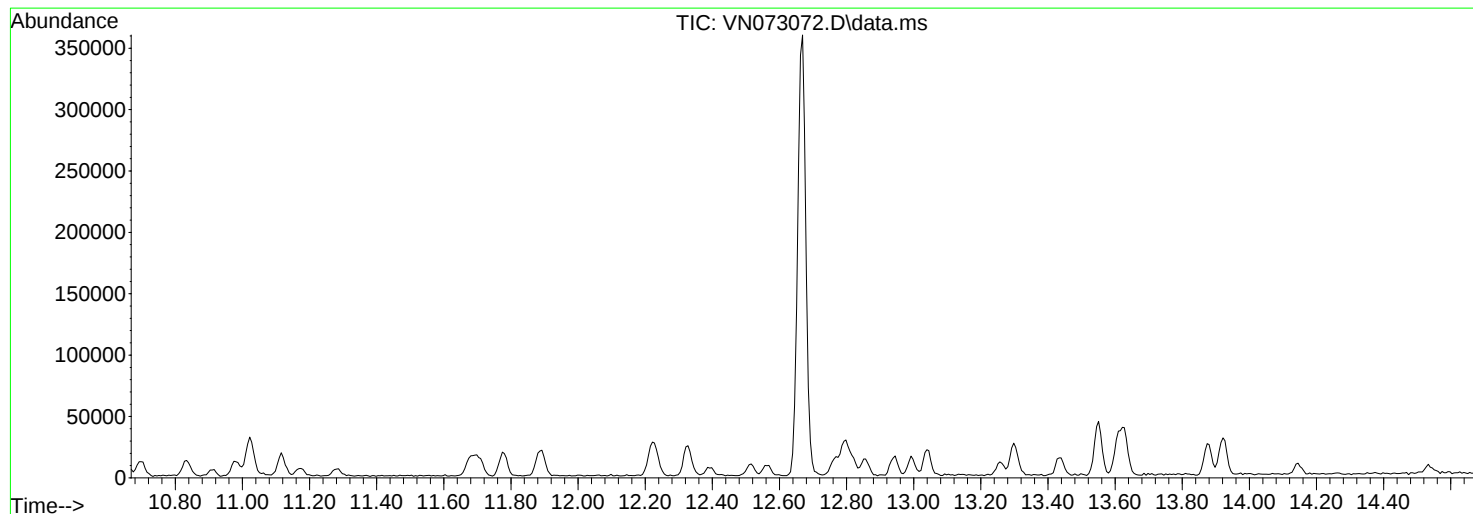

AutoFind: Scans 1832, 1833, 1834; Background Corrected with Scan 1824

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.2	13720	PASS
75	95	30	60	51.6	35043	PASS
95	95	100	100	100.0	67963	PASS
96	95	5	9	6.7	4564	PASS
173	174	0.00	2	1.7	858	PASS
174	95	50	100	75.4	51272	PASS
175	174	5	9	8.1	4136	PASS
176	174	95	101	96.7	49571	PASS
177	176	5	9	6.8	3383	PASS