
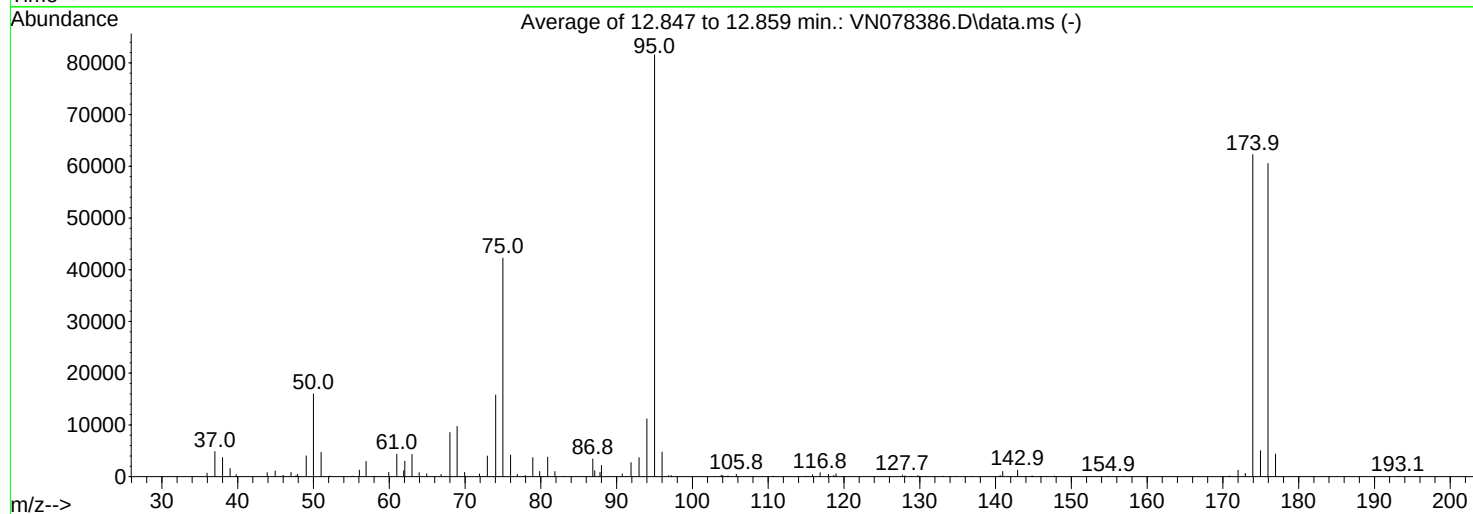


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN062423\
Data File : VN078386.D
Acq On : 24 Jun 2023 11:05
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N060623W.M
Title : SW846 8260
Last Update : Wed Jun 07 05:05:00 2023

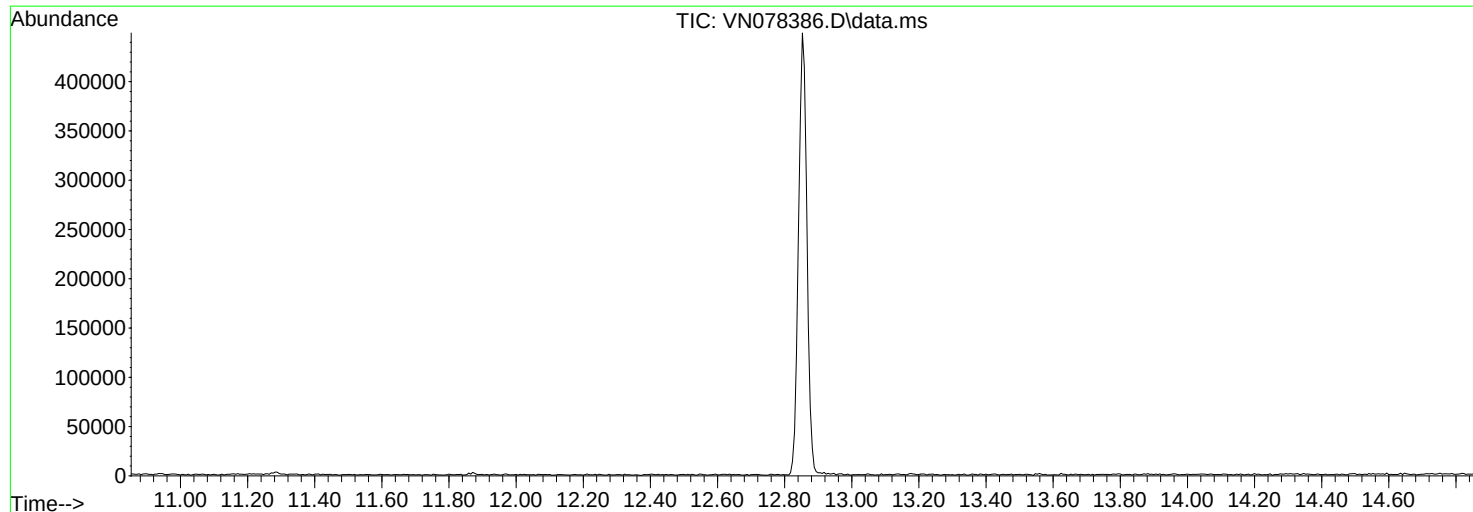

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1844

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.6	15989	PASS
75	95	30	60	51.8	42264	PASS
95	95	100	100	100.0	81549	PASS
96	95	5	9	5.9	4781	PASS
173	174	0.00	2	1.0	608	PASS
174	95	50	100	76.4	62264	PASS
175	174	5	9	8.1	5021	PASS
176	174	95	101	97.2	60547	PASS
177	176	5	9	7.2	4375	PASS

Average of 12.847 to 12.859 min.: VN078386.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	696	47.90	427	59.95	846	71.90	521
37.00	4871	49.05	4014	61.00	4336	72.95	397
38.00	3683	50.00	15989	61.90	1156	74.05	1578
39.00	1582	51.00	4716	62.05	2997	75.00	4226
39.80	417	52.00	65	63.00	4304	76.00	4175
43.10	52	52.15	124	63.95	772	76.90	423
43.90	776	55.00	62	64.95	565	77.80	128
44.95	1074	55.20	106	66.85	421	78.00	174
46.00	280	56.05	1263	68.00	8549	78.95	3686
47.05	798	56.95	2950	68.95	9729	79.85	1003
47.70	199	58.10	87	69.95	847	80.90	3781

Average of 12.847 to 12.859 min.: VN078386.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
81.85	983	96.00	4781	116.85	772	134.80	73
83.10	51	96.85	172	117.95	428	137.00	56
86.85	3404	97.20	215	118.65	224	140.00	71
87.10	1159	102.90	57	118.95	539	140.60	227
87.80	824	103.80	250	127.70	300	140.95	978
88.00	2159	104.00	215	128.05	164	142.90	1244
90.75	541	104.70	146	128.90	56	143.90	62
91.90	2723	105.80	442	129.75	212	144.70	111
92.95	3670	110.70	55	130.00	57	144.90	131
94.00	11181	115.00	83	130.80	53	145.90	76
95.00	81549	115.85	379	133.10	86	146.70	61

Average of 12.847 to 12.859 min.: VN078386.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
147.75	118						
154.90	65						
157.00	55						
170.85	148						
172.00	1252						
172.95	608						
173.95	62264						
174.95	5021						
175.95	60547						
176.95	4375						
193.10	64						

Instrument :

MSVOA_N

ClientSampleId :

BFB