

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN062424\
 Data File : VN082701.D
 Acq On : 24 Jun 2024 14:56
 Operator : JC\MD
 Sample : IBLK
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :

Quant Time: Jun 25 02:29:51 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N061724W.M
 Quant Title : SW846 8260
 QLast Update : Tue Jun 18 04:52:44 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.224	168	140232	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.106	114	253082	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.871	117	246687	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	102009	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.582	65	122501	54.474	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	= 108.940%	
35) Dibromofluoromethane	8.171	113	90950	52.974	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 105.940%	
50) Toluene-d8	10.571	98	332324	51.185	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	= 102.360%	
62) 4-Bromofluorobenzene	12.847	95	104806	46.821	ug/l	0.00
Spiked Amount	50.000	Range	64 - 133	Recovery	= 93.640%	
Target Compounds						
					Qvalue	
3) Chloromethane	2.365	50	929	0.396	ug/l	93
4) Vinyl Chloride	2.506	62	463	0.207	ug/l #	88
5) Bromomethane	2.959	94	1951	1.356	ug/l #	61
10) Methyl Iodide	4.595	142	960	0.617	ug/l #	84
13) Acrolein	4.177	56	138	0.368	ug/l #	78
15) Acrylonitrile	5.730	53	398	0.410	ug/l #	68
16) Acetone	4.436	43	754	0.737	ug/l #	88
17) Carbon Disulfide	4.712	76	3774	0.761	ug/l #	75
20) Methylene Chloride	5.283	84	1020	0.567	ug/l	94
21) trans-1,2-Dichloroethene	5.789	96	365	0.220	ug/l #	54
31) Cyclohexane	8.224	56	4617	1.423	ug/l #	40
36) 1,1-Dichloropropene	8.224	75	13159	5.127	ug/l #	50
38) Carbon Tetrachloride	8.230	117	14645	5.063	ug/l #	19
43) Isopropyl Acetate	8.694	43	14097	2.307	ug/l #	60
44) Trichloroethene	9.347	130	376	0.204	ug/l	1
59) 2-Hexanone	11.200	43	758	0.318	ug/l #	41
60) Dibromochloromethane	11.106	129	446	0.210	ug/l #	10
68) m/p-Xylenes	12.076	106	1021	0.285	ug/l	98
76) 1,2,3-Trichloropropane	12.853	75	62292	24.967	ug/l #	1
77) Bromobenzene	12.982	156	416	0.209	ug/l	98
78) n-propylbenzene	13.035	91	1890	0.206	ug/l	98
81) trans-1,4-Dichloro-2-b...	12.853	75	62292	59.731	ug/l #	6
82) 4-Chlorotoluene	13.223	91	1838	0.320	ug/l	95
87) 1,3-Dichlorobenzene	13.729	146	1271	0.352	ug/l	97
88) 1,4-Dichlorobenzene	13.729	146	1271	0.336	ug/l	97
89) n-Butylbenzene	14.064	91	2275	0.419	ug/l	92
91) 1,2-Dichlorobenzene	14.106	146	1087	0.308	ug/l	92
93) 1,2,4-Trichlorobenzene	15.394	180	1409	0.757	ug/l	87
94) Hexachlorobutadiene	15.500	225	1062	1.157	ug/l	98
95) Naphthalene	15.635	128	4163	0.727	ug/l #	73
96) 1,2,3-Trichlorobenzene	15.853	180	1848	0.974	ug/l #	82


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN062424\
Data File : VN082701.D
Acq On : 24 Jun 2024 14:56
Operator : JC\MD
Sample : IBLK
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :

Quant Time: Jun 25 02:29:51 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N061724W.M
Quant Title : SW846 8260
QLast Update : Tue Jun 18 04:52:44 2024
Response via : Initial Calibration




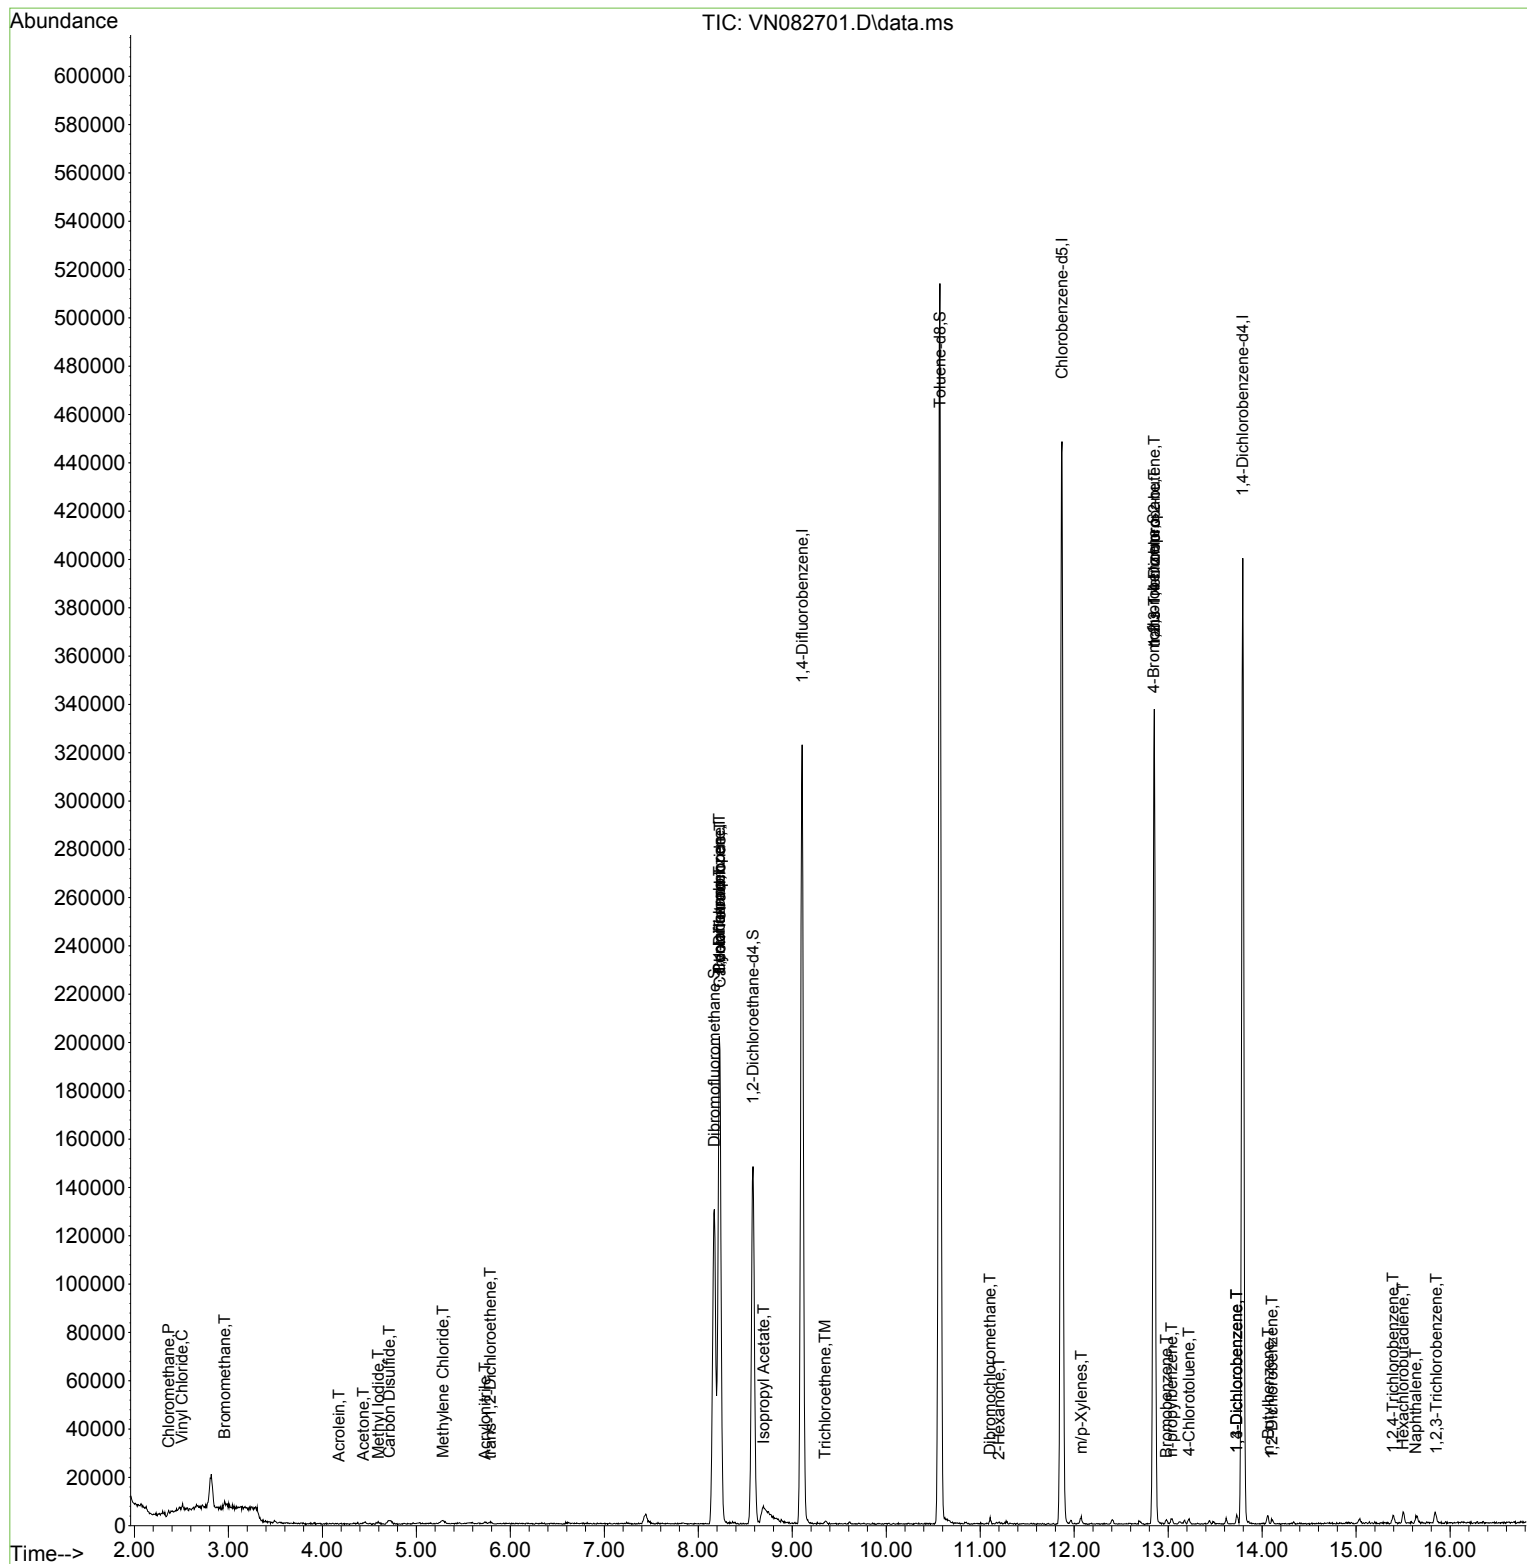




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.224 min Scan# 10
Delta R.T. -0.005 min
Lab File: VN082701.D
Acq: 24 Jun 2024 14:56




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:168 Resp: 140232
Ion Ratio Lower Upper
168 100
99 58.5 48.2 72.4

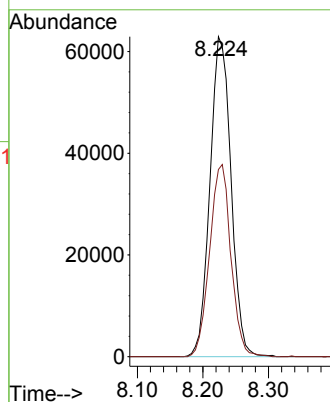

#3
Chloromethane
Concen: 0.396 ug/l
RT: 2.365 min Scan# 70
Delta R.T. 0.006 min
Lab File: VN082701.D
Acq: 24 Jun 2024 14:56

Tgt Ion: 50 Resp: 929
Ion Ratio Lower Upper
50 100
52 34.9 25.0 37.4

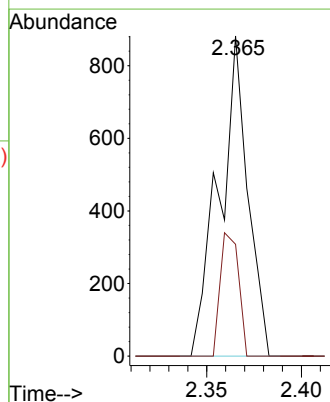

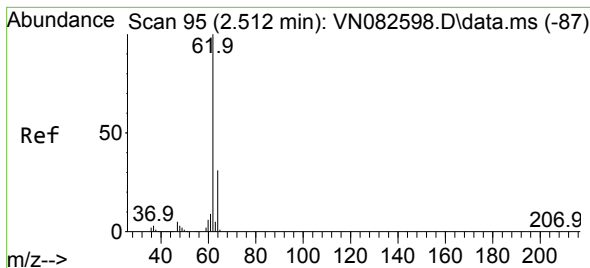

#4

Vinyl Chloride

Concen: 0.207 ug/l

RT: 2.506 min Scan# 94

Delta R.T. -0.006 min


Lab File: VN082701.D

Acq: 24 Jun 2024 14:56

Instrument :

MSVOA_N

ClientSampleId :



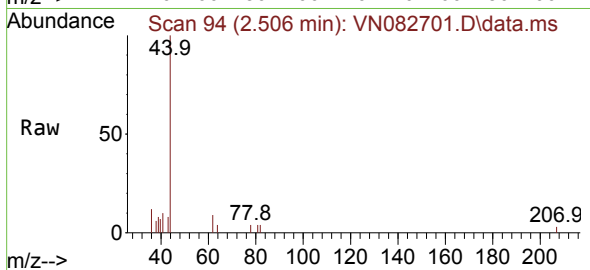


Tgt Ion: 62 Resp: 463

Ion Ratio Lower Upper

62 100

64 38.0 25.0 37.6#

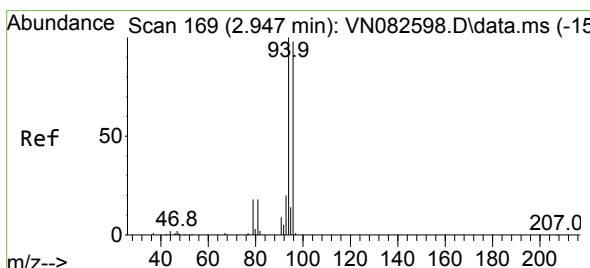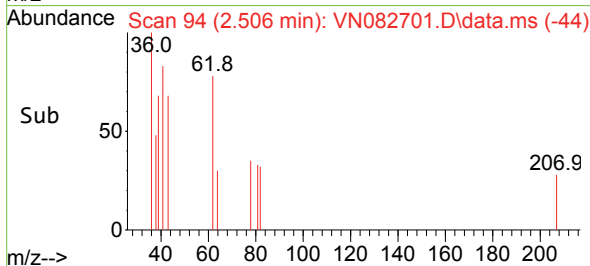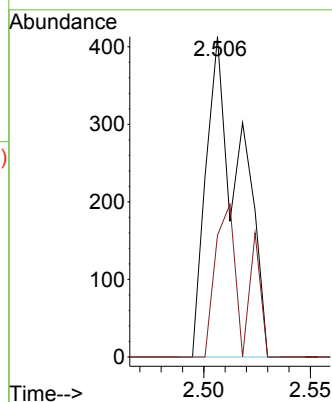

#5

Bromomethane

Concen: 1.356 ug/l

RT: 2.959 min Scan# 171

Delta R.T. 0.012 min

Lab File: VN082701.D




Acq: 24 Jun 2024 14:56


Tgt Ion: 94 Resp: 1951

Ion Ratio Lower Upper

94 100


96 58.7 78.0 117.0#

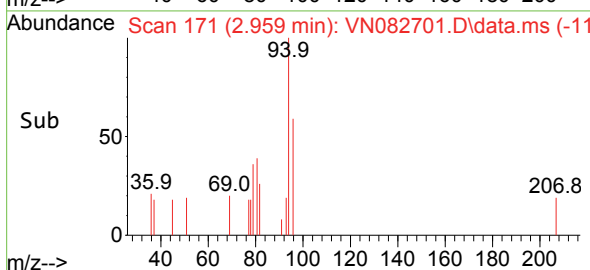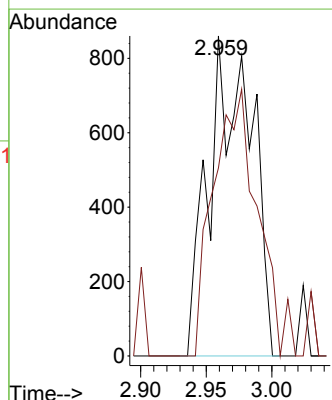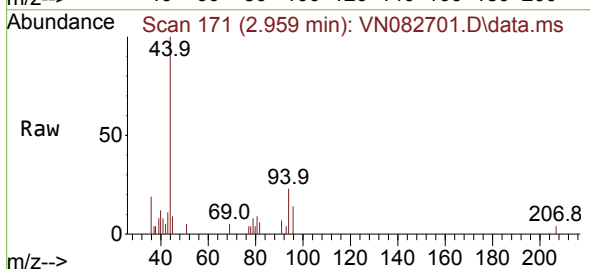






#10
Methyl Iodide
Concen: 0.617 ug/l
RT: 4.595 min Scan# 449
Delta R.T. 0.006 min
Lab File: VN082701.D
Acq: 24 Jun 2024 14:56

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion:142 Resp: 960
Ion Ratio Lower Upper
142 100
127 41.8 37.5 56.3
141 0.0 13.1 19.7#

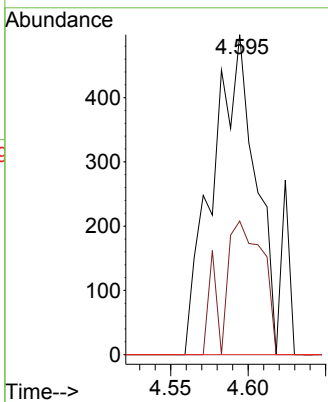

#13
Acrolein
Concen: 0.368 ug/l
RT: 4.177 min Scan# 378
Delta R.T. 0.000 min
Lab File: VN082701.D
Acq: 24 Jun 2024 14:56


Tgt Ion: 56 Resp: 138
Ion Ratio Lower Upper
56 100
55 88.4 56.4 84.6#

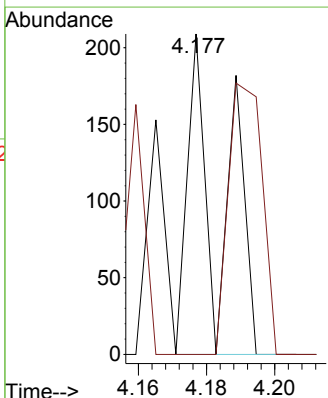






#15
Acrylonitrile
Concen: 0.410 ug/l
RT: 5.730 min Scan# 640
Delta R.T. 0.012 min
Lab File: VN082701.D
Acq: 24 Jun 2024 14:56

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion: 53 Resp: 398
Ion Ratio Lower Upper
53 100
52 66.8 66.6 100.0
51 0.0 30.1 45.1#

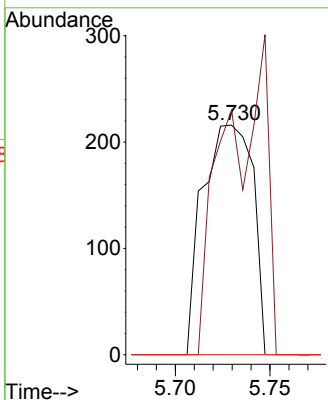

#16
Acetone
Concen: 0.737 ug/l
RT: 4.436 min Scan# 422
Delta R.T. 0.006 min
Lab File: VN082701.D
Acq: 24 Jun 2024 14:56

Tgt Ion: 43 Resp: 754
Ion Ratio Lower Upper
43 100
58 33.2 21.8 32.6#

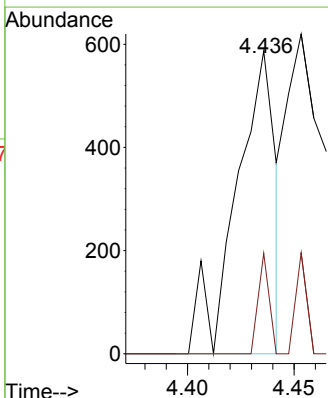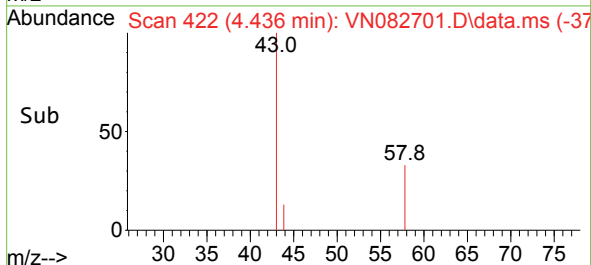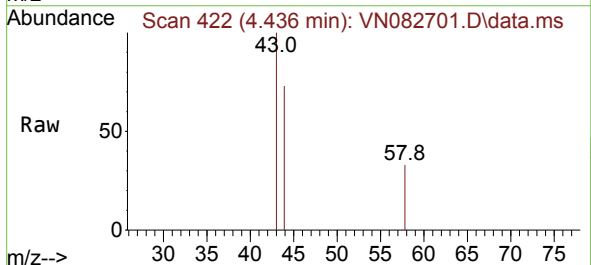



#17

Carbon Disulfide

Concen: 0.761 ug/l

RT: 4.712 min Scan# 4

Delta R.T. 0.000 min

Lab File: VN082701.D

Acq: 24 Jun 2024 14:56

Instrument :

MSVOA_N





ClientSampleId :

Tgt Ion: 76 Resp: 3774

Ion Ratio Lower Upper

76 100

78 0.0 7.2 10.8#

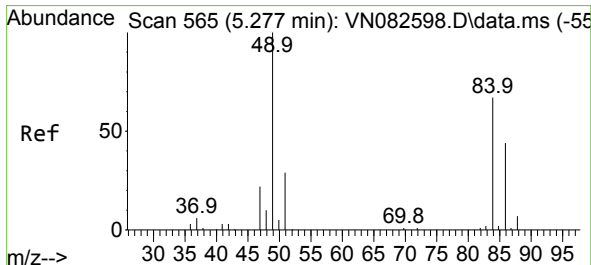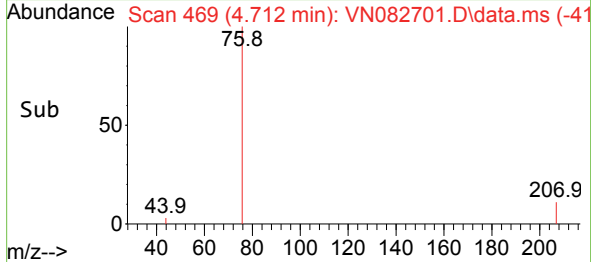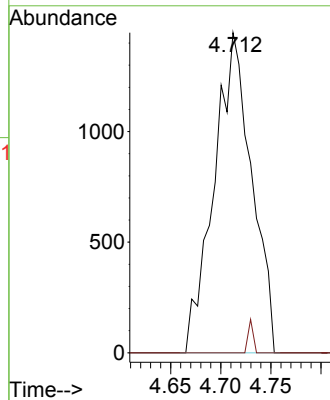

#20

Methylene Chloride

Concen: 0.567 ug/l

RT: 5.283 min Scan# 566

Delta R.T. 0.006 min

Lab File: VN082701.D

Acq: 24 Jun 2024 14:56

Tgt Ion: 84 Resp: 1020




Ion Ratio Lower Upper


84 100

49 154.2 119.6 179.4

51 41.6 34.8 52.2

86 55.2 52.9 79.3

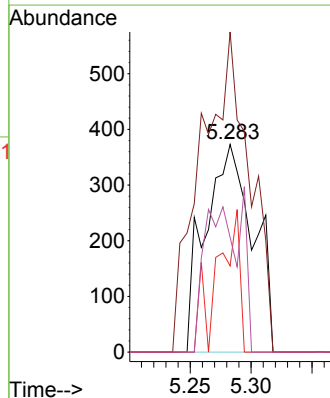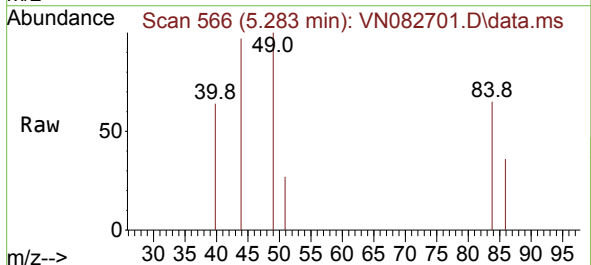



#21

trans-1,2-Dichloroethene

Concen: 0.220 ug/l

RT: 5.789 min Scan# 61

Delta R.T. 0.000 min


Lab File: VN082701.D

Acq: 24 Jun 2024 14:56

Instrument :

MSVOA_N

ClientSampleId :






Tgt Ion: 96 Resp: 365

Ion Ratio Lower Upper

96 100

61 111.8 123.4 185.2#

98 0.0 49.3 73.9#

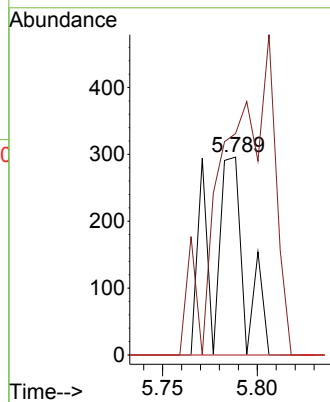

#31

Cyclohexane

Concen: 1.423 ug/l

RT: 8.224 min Scan# 1066

Delta R.T. -0.035 min

Lab File: VN082701.D

Acq: 24 Jun 2024 14:56




Tgt Ion: 56 Resp: 4617


Ion Ratio Lower Upper

56 100

69 131.5 24.5 36.7#

84 94.5 66.0 99.0




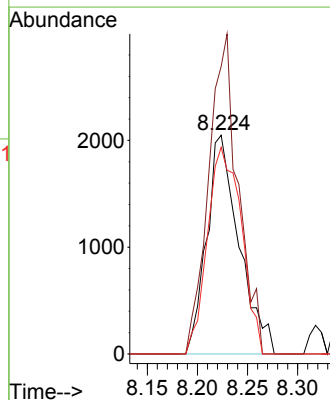




#33
 1,2-Dichloroethane-d4
 Concen: 54.474 ug/l
 RT: 8.582 min Scan# 1127
 Delta R.T. 0.000 min
 Lab File: VN082701.D
 Acq: 24 Jun 2024 14:56




Instrument :
 MSVOA_N
 ClientSampleId :


Tgt Ion: 65 Resp: 122501
 Ion Ratio Lower Upper
 65 100
 67 50.3 0.0 104.4

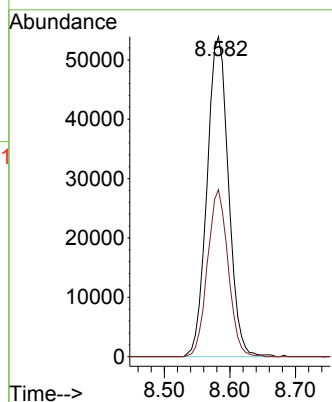

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 9.106 min Scan# 1216
 Delta R.T. 0.000 min
 Lab File: VN082701.D
 Acq: 24 Jun 2024 14:56


Tgt Ion: 114 Resp: 253082
 Ion Ratio Lower Upper
 114 100
 63 22.7 0.0 44.6
 88 16.4 0.0 31.4

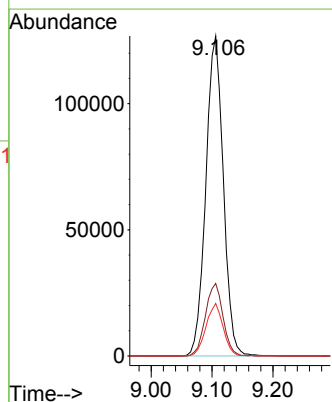






#35
Dibromofluoromethane
Concen: 52.974 ug/l
RT: 8.171 min Scan# 1057
Delta R.T. 0.006 min
Lab File: VN082701.D
Acq: 24 Jun 2024 14:56

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion:113 Resp: 90950
Ion Ratio Lower Upper
113 100
111 102.4 82.4 123.6
192 18.7 14.9 22.3

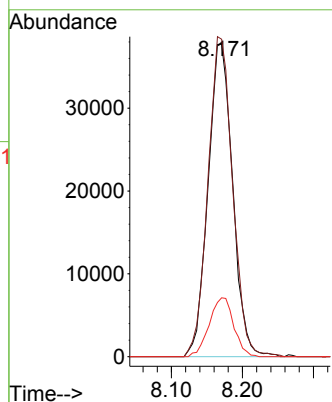

#36
1,1-Dichloropropene
Concen: 5.127 ug/l
RT: 8.224 min Scan# 1066
Delta R.T. -0.147 min
Lab File: VN082701.D
Acq: 24 Jun 2024 14:56

Tgt Ion: 75 Resp: 13159
Ion Ratio Lower Upper
75 100
110 7.3 16.3 48.9#
77 0.0 24.6 37.0#

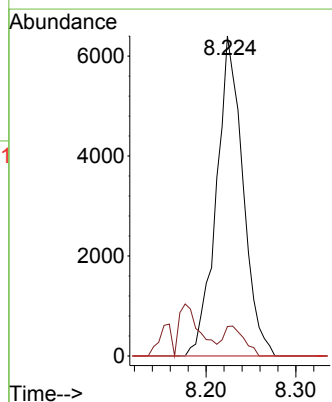

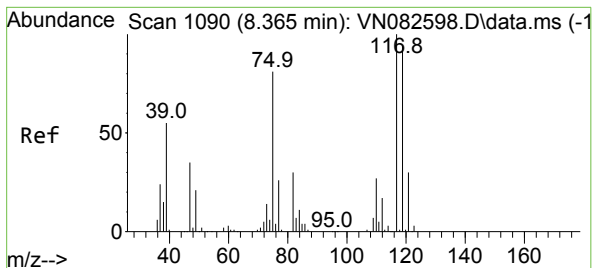

#38

Carbon Tetrachloride

Concen: 5.063 ug/l

RT: 8.230 min Scan# 1067

Delta R.T. -0.135 min


Lab File: VN082701.D

Acq: 24 Jun 2024 14:56

Instrument :

MSVOA_N

ClientSampleId :

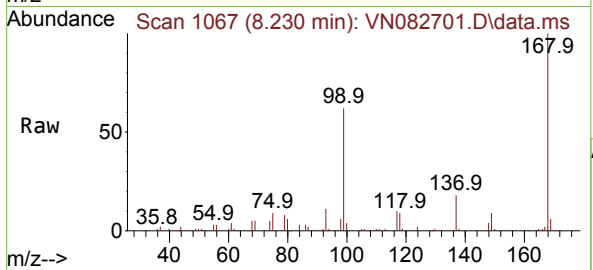




Tgt Ion:117 Resp: 14645

Ion Ratio Lower Upper

117 100

119 7.6 74.9 112.3#

121 0.0 24.3 36.5#

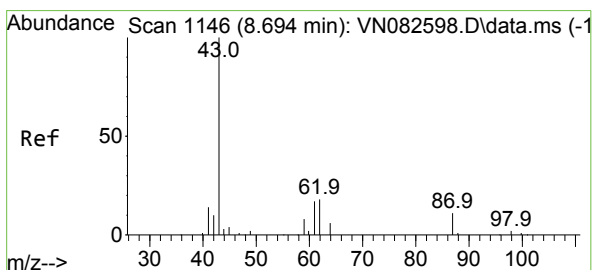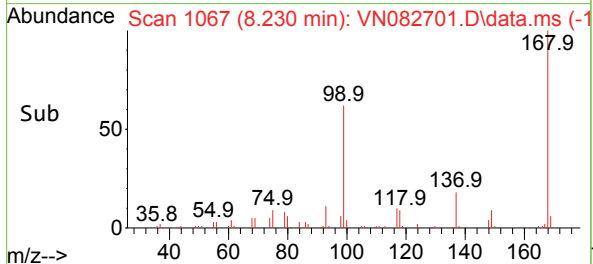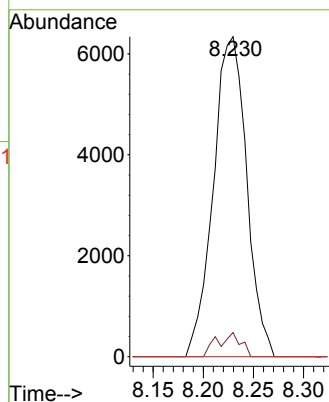

#43

Isopropyl Acetate

Concen: 2.307 ug/l

RT: 8.694 min Scan# 1146

Delta R.T. 0.000 min

Lab File: VN082701.D

Acq: 24 Jun 2024 14:56




Tgt Ion: 43 Resp: 14097


Ion Ratio Lower Upper

43 100

61 0.0 17.8 26.6#

87 0.0 8.2 12.2#

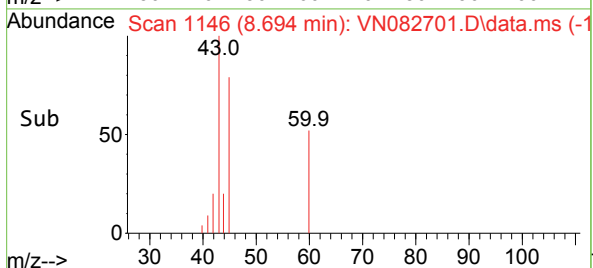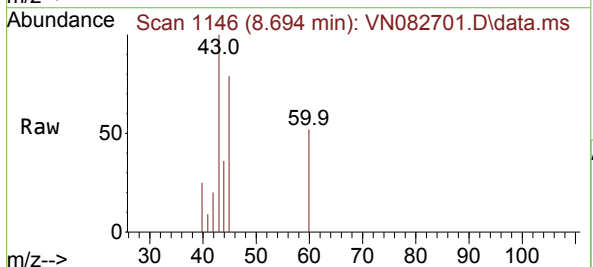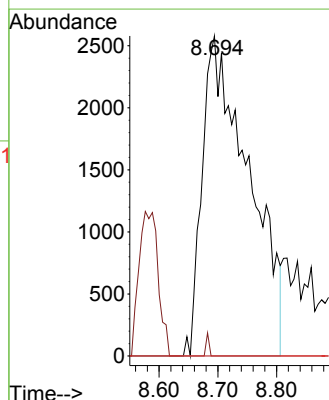



#44

Trichloroethene

Concen: 0.204 ug/l

RT: 9.347 min Scan# 11

Delta R.T. -0.006 min

Lab File: VN082701.D

Acq: 24 Jun 2024 14:56

Instrument :

MSVOA_N





ClientSampleId :

Tgt Ion:130 Resp: 376

Ion Ratio Lower Upper

130 100

95 0.0 0.0 197.8

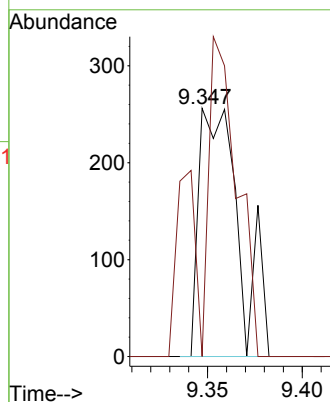

#50

Toluene-d8

Concen: 51.185 ug/l

RT: 10.571 min Scan# 1465

Delta R.T. 0.000 min

Lab File: VN082701.D




Acq: 24 Jun 2024 14:56


Tgt Ion: 98 Resp: 332324

Ion Ratio Lower Upper

98 100

100 63.2 51.5 77.3



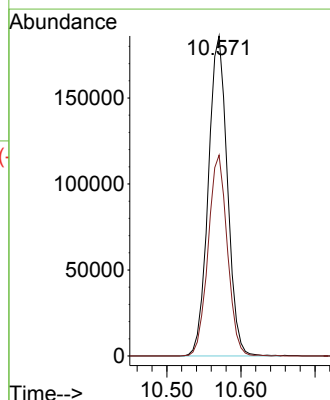





#59
2-Hexanone
Concen: 0.318 ug/l
RT: 11.200 min Scan# 11556
Delta R.T. 0.000 min
Lab File: VN082701.D
Acq: 24 Jun 2024 14:56




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 43 Resp: 758
Ion Ratio Lower Upper
43 100
58 8.8 24.6 73.8#

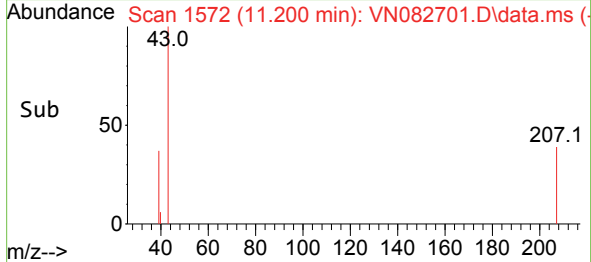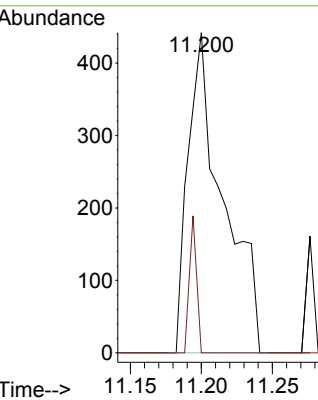

#60
Dibromochloromethane
Concen: 0.210 ug/l
RT: 11.106 min Scan# 1556
Delta R.T. -0.253 min
Lab File: VN082701.D
Acq: 24 Jun 2024 14:56

Tgt Ion: 129 Resp: 446
Ion Ratio Lower Upper
129 100
127 0.0 39.2 117.6#


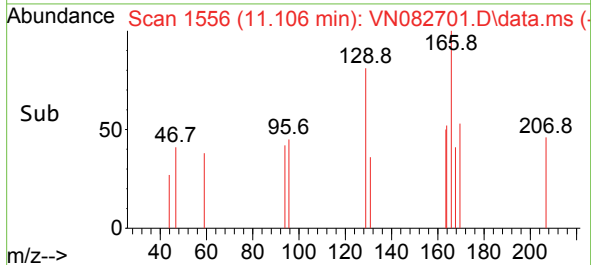
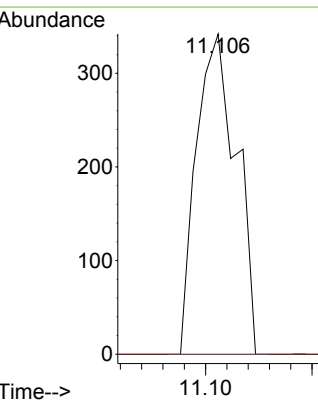





#62
4-Bromofluorobenzene
Concen: 46.821 ug/l
RT: 12.847 min Scan# 11
Delta R.T. 0.000 min
Lab File: VN082701.D
Acq: 24 Jun 2024 14:56




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 95 Resp: 104806
Ion Ratio Lower Upper
95 100
174 80.1 0.0 159.2
176 75.3 0.0 147.6

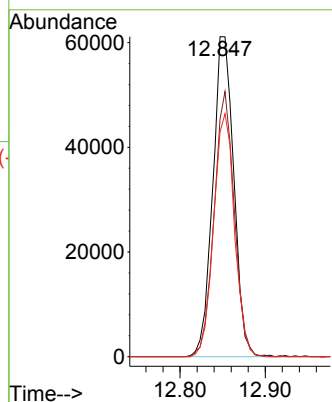

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.871 min Scan# 1686
Delta R.T. 0.000 min
Lab File: VN082701.D
Acq: 24 Jun 2024 14:56

Tgt Ion: 117 Resp: 246687
Ion Ratio Lower Upper
117 100
82 57.6 47.5 71.3
119 31.7 25.6 38.4



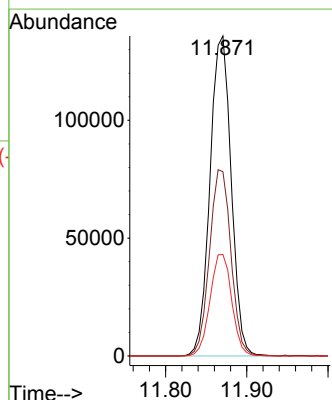





#68
m/p-Xylenes
Concen: 0.285 ug/l
RT: 12.076 min Scan# 1
Delta R.T. 0.006 min
Lab File: VN082701.D
Acq: 24 Jun 2024 14:56




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:106 Resp: 1021
Ion Ratio Lower Upper
106 100
91 204.2 166.1 249.1

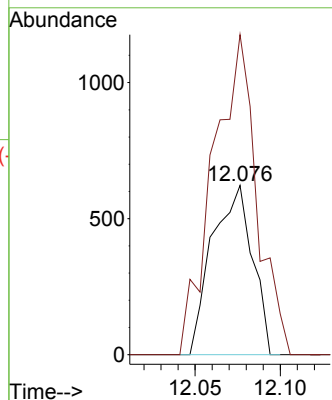

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.794 min Scan# 2013
Delta R.T. 0.000 min
Lab File: VN082701.D
Acq: 24 Jun 2024 14:56

Tgt Ion:152 Resp: 102009
Ion Ratio Lower Upper
152 100
115 59.7 30.6 91.6
150 155.7 0.0 348.6

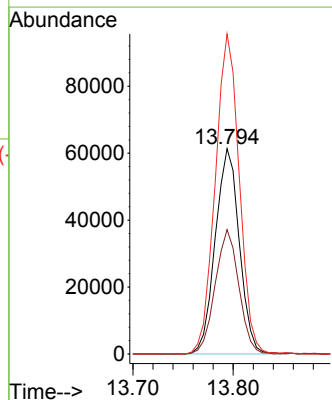



#76

1,2,3-Trichloropropane

Concen: 24.967 ug/l

RT: 12.853 min Scan# 1853

Delta R.T. -0.141 min

Lab File: VN082701.D

Acq: 24 Jun 2024 14:56

Instrument :

MSVOA_N





ClientSampleId :

Tgt Ion: 75 Resp: 62292

Ion Ratio Lower Upper

75 100

77 1.0 110.9 332.6#

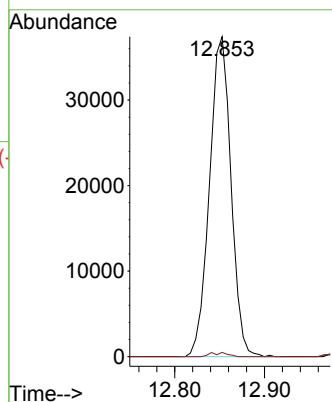

#77

Bromobenzene

Concen: 0.209 ug/l

RT: 12.982 min Scan# 1875

Delta R.T. 0.000 min

Lab File: VN082701.D

Acq: 24 Jun 2024 14:56




Tgt Ion:156 Resp: 416


Ion Ratio Lower Upper

156 100

77 223.3 111.3 333.8

158 90.1 48.3 144.9

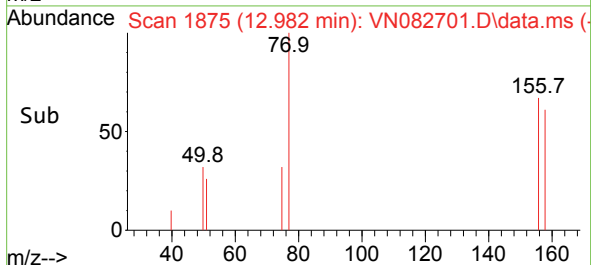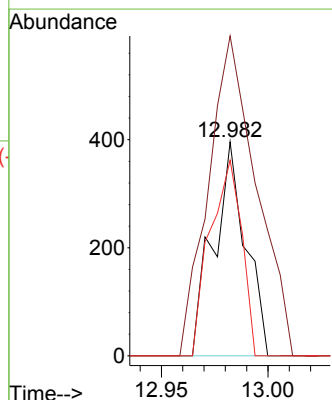



#78

n-propylbenzene

Concen: 0.206 ug/l

RT: 13.035 min Scan# 1884

Delta R.T. 0.000 min

Lab File: VN082701.D

Acq: 24 Jun 2024 14:56

Instrument :

MSVOA_N





ClientSampleId :

Tgt Ion: 91 Resp: 1890

Ion Ratio Lower Upper

91 100

120 20.9 10.9 32.9

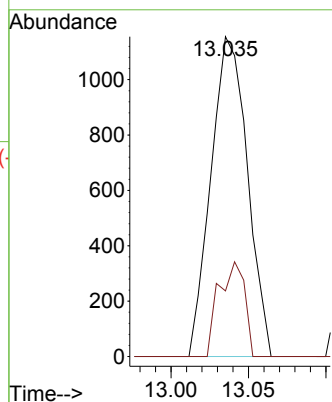

#81

trans-1,4-Dichloro-2-butene

Concen: 59.731 ug/l

RT: 12.853 min Scan# 1853

Delta R.T. 0.112 min

Lab File: VN082701.D

Acq: 24 Jun 2024 14:56




Tgt Ion: 75 Resp: 62292


Ion Ratio Lower Upper

75 100

53 0.1 88.4 132.6#

89 0.0 36.3 54.5#



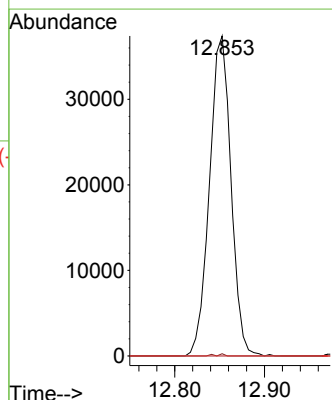





#82
4-Chlorotoluene
Concen: 0.320 ug/l
RT: 13.223 min Scan# 1916
Delta R.T. 0.000 min
Lab File: VN082701.D
Acq: 24 Jun 2024 14:56




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 91 Resp: 1838
Ion Ratio Lower Upper
91 100
126 34.9 16.2 48.6

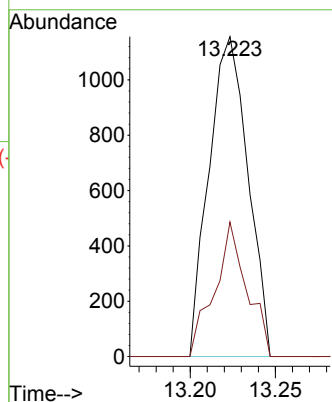

#87
1,3-Dichlorobenzene
Concen: 0.352 ug/l
RT: 13.729 min Scan# 2002
Delta R.T. -0.006 min
Lab File: VN082701.D
Acq: 24 Jun 2024 14:56


Tgt Ion: 146 Resp: 1271
Ion Ratio Lower Upper
146 100
111 38.3 20.6 61.9
148 61.9 31.8 95.3

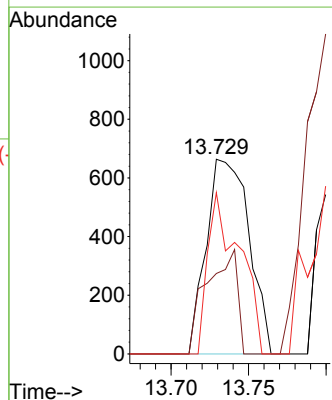






#88
1,4-Dichlorobenzene
Concen: 0.336 ug/l
RT: 13.729 min Scan# 2016
Delta R.T. -0.082 min
Lab File: VN082701.D
Acq: 24 Jun 2024 14:56


Instrument :
MSVOA_N
ClientSampleId :





Tgt Ion:146 Resp: 1271
Ion Ratio Lower Upper
146 100
111 38.3 20.1 60.3
148 61.9 32.2 96.6

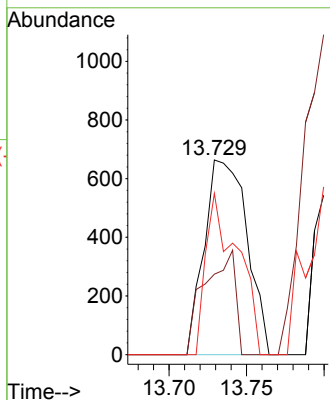


#89
n-Butylbenzene
Concen: 0.419 ug/l
RT: 14.064 min Scan# 2059
Delta R.T. 0.006 min
Lab File: VN082701.D
Acq: 24 Jun 2024 14:56



Tgt Ion: 91 Resp: 2275
Ion Ratio Lower Upper
91 100
92 46.0 26.1 78.3
134 20.6 12.1 36.3

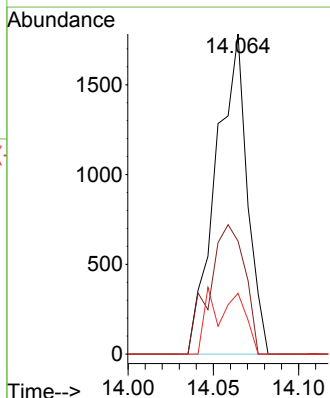

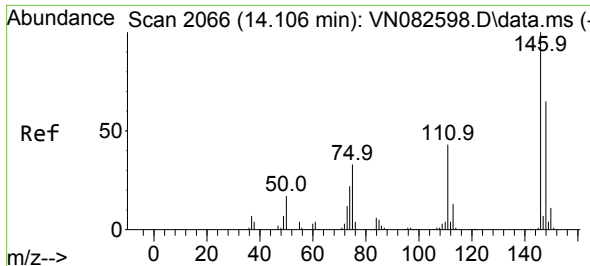

#91

1,2-Dichlorobenzene

Concen: 0.308 ug/l

RT: 14.106 min Scan# 2066

Delta R.T. 0.000 min

Lab File: VN082701.D

Acq: 24 Jun 2024 14:56

Instrument :

MSVOA_N

ClientSampleId :





Tgt Ion:146 Resp: 1087

Ion Ratio Lower Upper

146 100

111 31.5 21.4 64.2

148 63.8 32.1 96.5

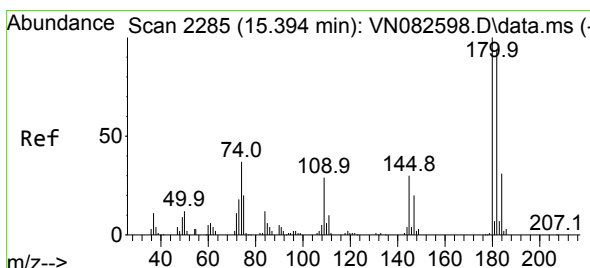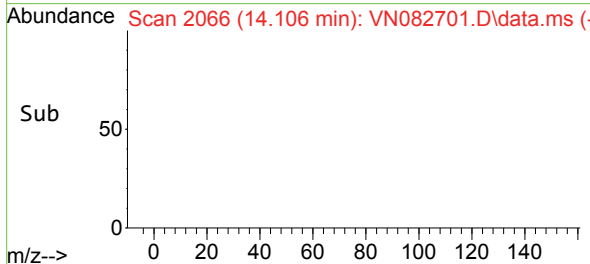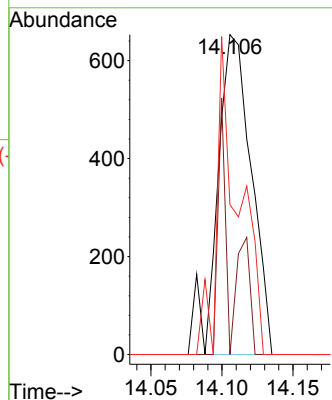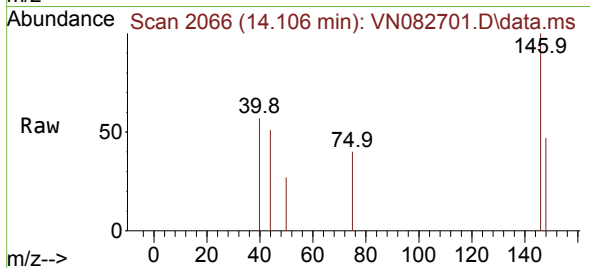

#93

1,2,4-Trichlorobenzene

Concen: 0.757 ug/l

RT: 15.394 min Scan# 2285

Delta R.T. -0.000 min

Lab File: VN082701.D

Acq: 24 Jun 2024 14:56




Tgt Ion:180 Resp: 1409


Ion Ratio Lower Upper

180 100

182 83.6 47.3 141.8

145 21.6 15.7 47.1


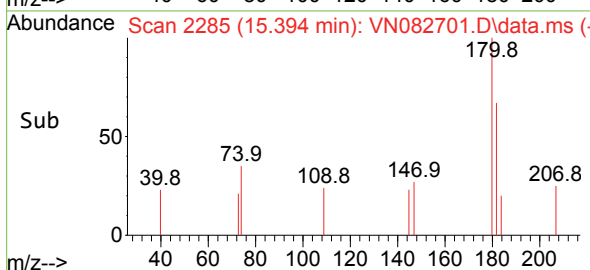
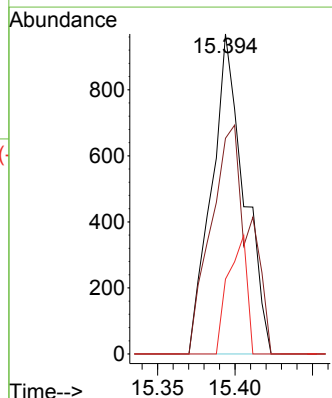
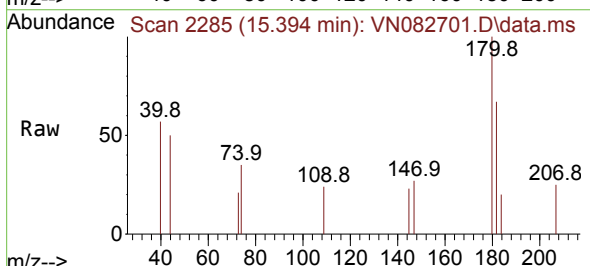




#94
Hexachlorobutadiene
Concen: 1.157 ug/l
RT: 15.500 min Scan# 21
Delta R.T. -0.005 min
Lab File: VN082701.D
Acq: 24 Jun 2024 14:56




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:225 Resp: 1062
Ion Ratio Lower Upper
225 100
223 65.6 31.9 95.7
227 66.3 32.5 97.5

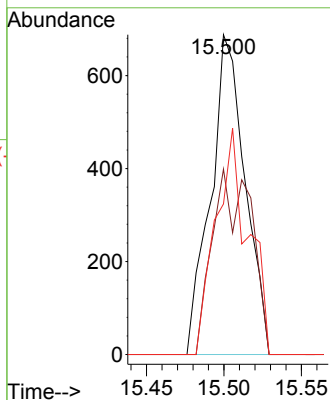

#95
Naphthalene
Concen: 0.727 ug/l
RT: 15.635 min Scan# 2326
Delta R.T. -0.006 min
Lab File: VN082701.D
Acq: 24 Jun 2024 14:56

Tgt Ion:128 Resp: 4163
Ion Ratio Lower Upper
128 100
127 0.0 10.6 16.0#
129 3.4 8.6 12.8#

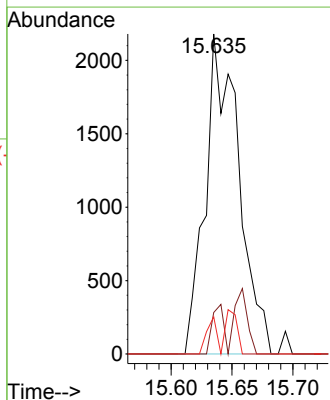



#96

1,2,3-Trichlorobenzene

Concen: 0.974 ug/l

RT: 15.853 min Scan# 21

Delta R.T. 0.012 min


Lab File: VN082701.D

Acq: 24 Jun 2024 14:56

Instrument :

MSVOA_N

ClientSampleId :



Tgt Ion:180 Resp: 1848

Ion Ratio Lower Upper

180 100

182 93.9 48.9 146.8

145 0.0 16.8 50.4#

