
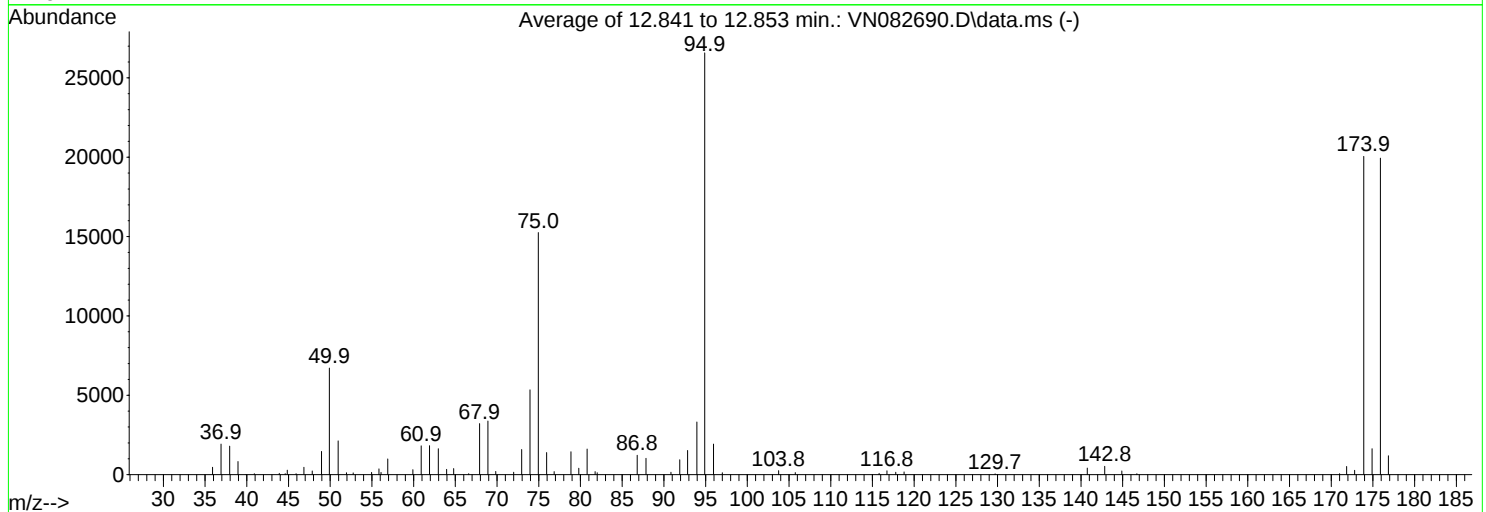


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN062424\
Data File : VN082690.D
Acq On : 24 Jun 2024 08:40
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N061724W.M
Title : SW846 8260
Last Update : Tue Jun 18 04:52:44 2024

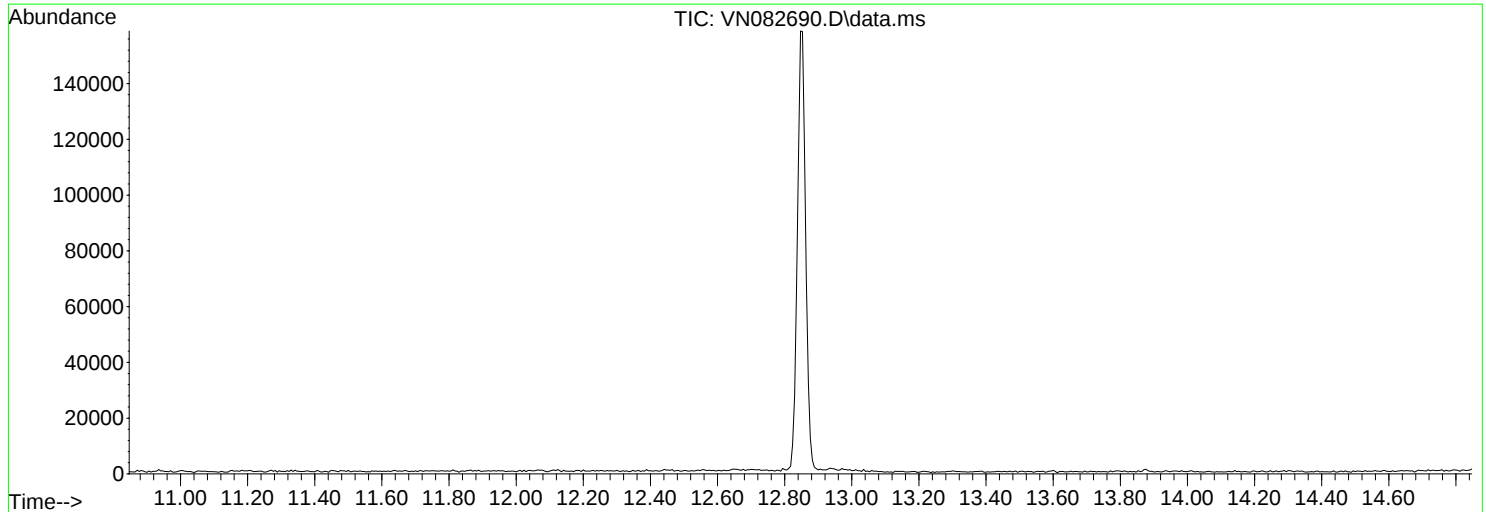

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	25.3	6717	PASS
75	95	30	60	57.4	15254	PASS
95	95	100	100	100.0	26576	PASS
96	95	5	9	7.3	1930	PASS
173	174	0.00	2	1.3	270	PASS
174	95	50	100	75.5	20055	PASS
175	174	5	9	8.1	1630	PASS
176	174	95	101	99.4	19941	PASS
177	176	5	9	6.0	1189	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.90	469	47.85	234	60.90	1815	73.95	534
36.90	1923	48.95	1463	61.90	1829	74.95	1525
37.95	1794	49.90	6717	62.95	1637	75.95	138
38.95	824	50.95	2128	63.95	329	76.85	19
39.90	14	51.95	122	64.80	385	78.85	1446
40.90	56	52.75	114	66.60	58	79.80	408
43.90	82	54.95	142	67.90	3221	80.80	1611
44.60	57	55.85	365	68.90	3376	81.75	193
44.85	279	56.10	141	69.85	201	82.00	126
45.90	56	56.90	985	72.00	155	86.80	1221
46.85	468	59.90	317	72.95	1584	87.85	1025

Average of 12.841 to 12.853 min.: VN082690.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
90.85	156	117.80	156	174.90	1630		
91.90	940	118.80	175	175.90	19941		
92.85	1522	129.70	52	176.85	1189		
93.95	3318	140.75	415				
94.90	26576	142.85	526				
95.95	1930	144.90	235				
97.00	119	146.70	56				
103.75	255	171.00	56				
105.75	133	171.85	516				
115.80	77	172.80	270				
116.75	240	173.90	20055				

Instrument :

MSVOA_N

ClientSampleId :

BFB