
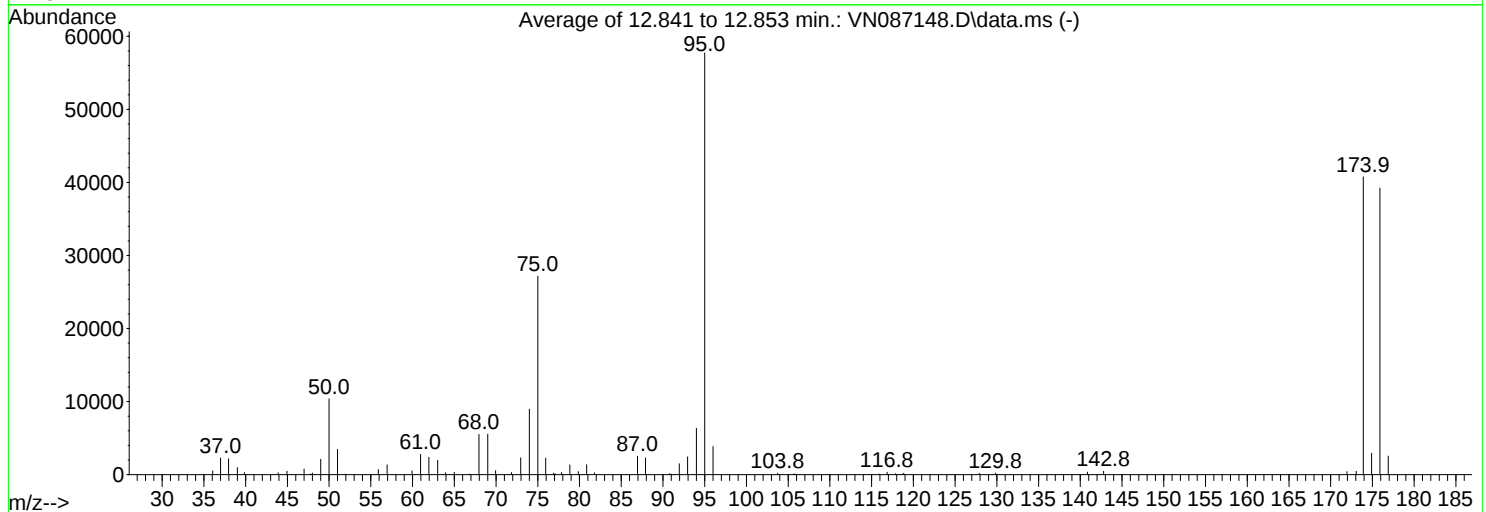


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN062425\
Data File : VN087148.D
Acq On : 24 Jun 2025 10:41
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N060625W.M
Title : SW846 8260
Last Update : Sat Jun 07 02:12:50 2025

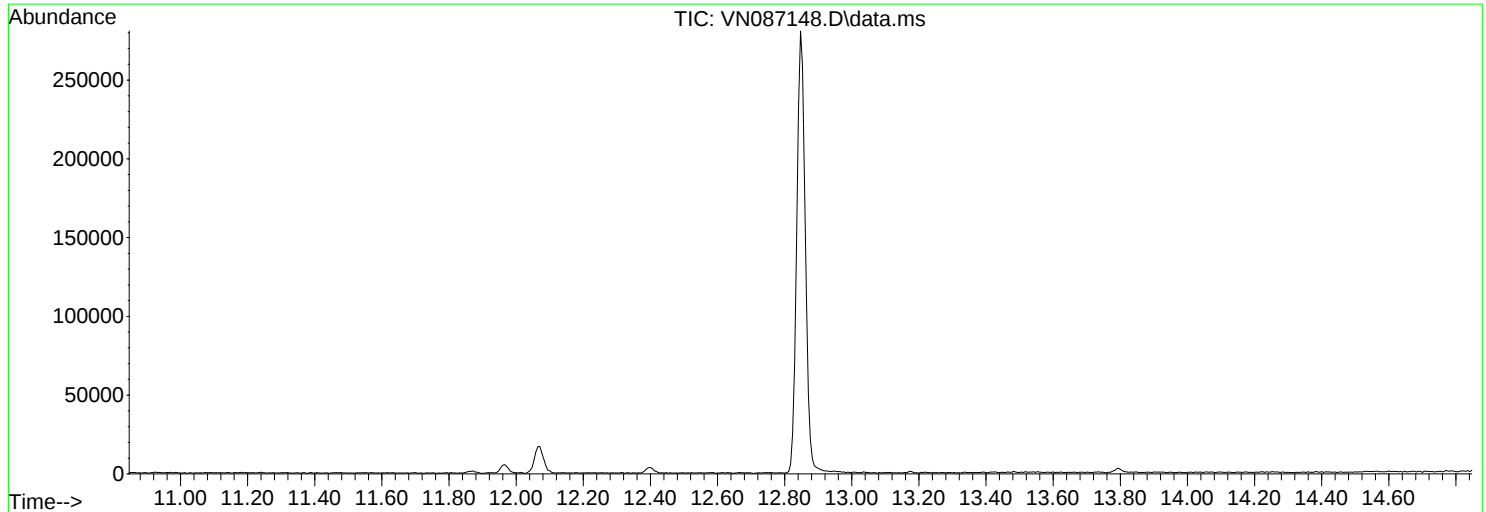

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.0	10375	PASS
75	95	30	60	47.1	27173	PASS
95	95	100	100	100.0	57736	PASS
96	95	5	9	6.7	3861	PASS
173	174	0.00	2	1.1	457	PASS
174	95	50	100	70.6	40760	PASS
175	174	5	9	7.2	2943	PASS
176	174	95	101	96.2	39221	PASS
177	176	5	9	6.5	2548	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	496	50.00	10375	66.80	59	77.85	281
37.00	2272	51.00	3462	67.95	5530	78.85	1331
37.95	2178	51.90	64	69.00	5537	79.85	400
39.00	970	55.90	711	69.95	553	80.85	135
39.85	276	56.95	1345	71.85	291	81.80	233
43.90	270	59.95	524	72.95	2311	86.95	2520
44.95	474	60.95	2789	74.00	8960	87.90	2285
47.00	768	61.95	2383	75.00	27173	90.80	130
47.80	84	63.00	1981	75.95	2250	91.00	63
48.00	225	63.95	263	76.90	218	91.95	1491
49.00	2103	65.00	339	77.10	101	92.95	2442

Average of 12.841 to 12.853 min.: VN087148.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
94.00	6339	127.90	194				
95.00	57736	129.85	225				
96.00	3861	140.85	363				
103.75	199	142.80	460				
105.70	107	171.95	417				
105.90	55	173.05	457				
115.90	81	173.90	40760				
116.85	330	174.90	2943				
117.85	136	175.90	39221				
118.70	86	176.90	2548				
118.85	194						

Instrument :

MSVOA_N

ClientSampleId :

BFB