


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN062518\
 Data File : VN049510.D
 Acq On : 25 Jun 2018 11:04
 Operator : MD\SY
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N061618W.M
 Title : SW846 8260
 Last Update : Sat Jun 16 01:02:01 2018

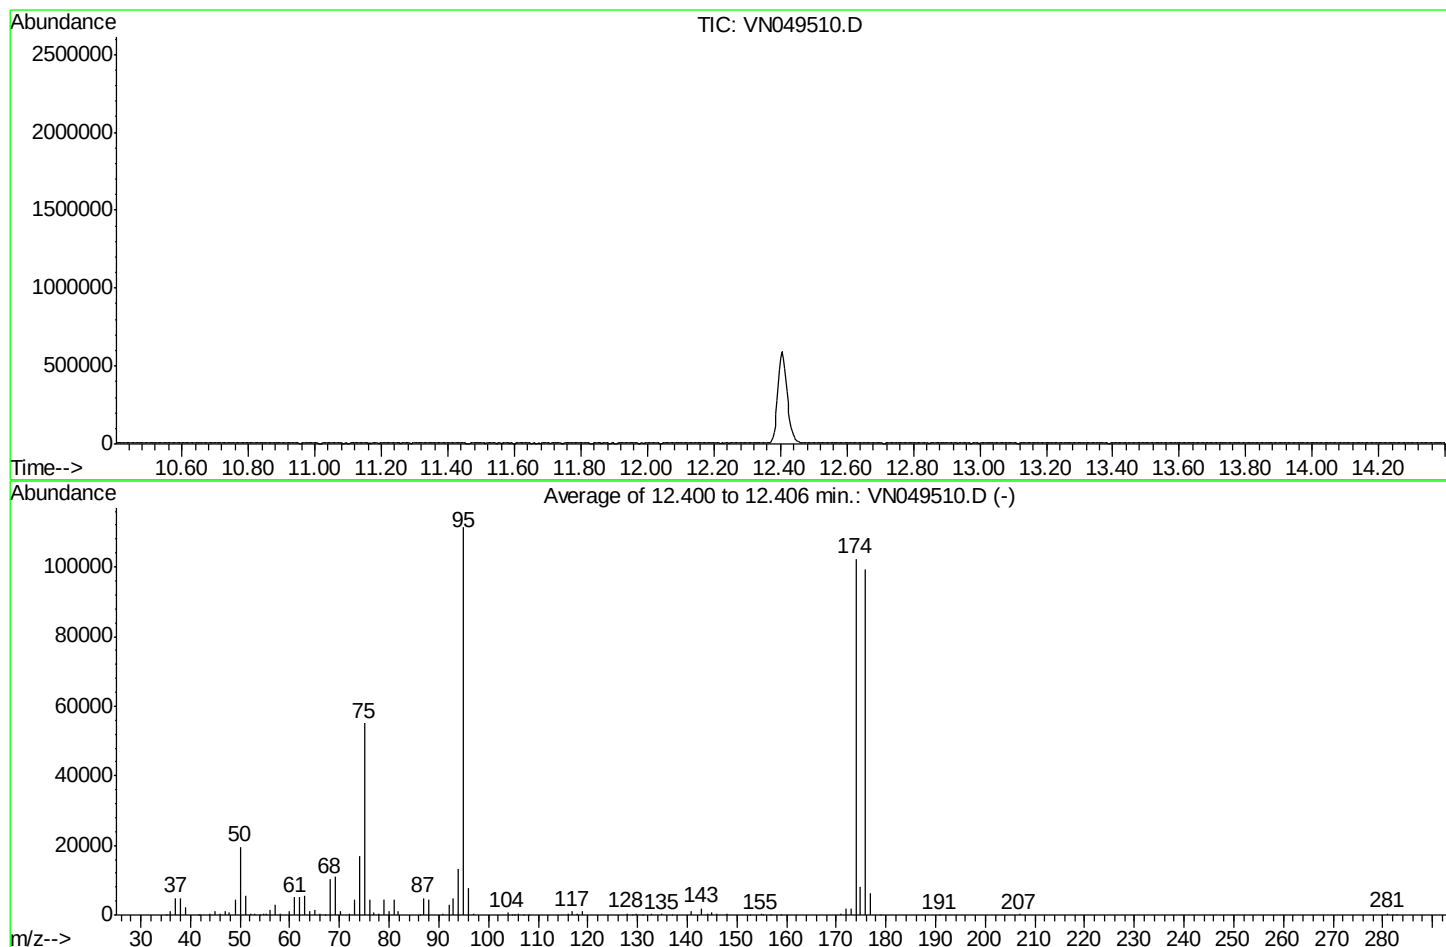

AutoFind: Scans 3362, 3363, 3364; Background Corrected with Scan 3348

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.6	19658	PASS
75	95	30	60	49.4	55008	PASS
95	95	100	100	100.0	111386	PASS
96	95	5	9	7.0	7815	PASS
173	174	0.00	2	1.8	1876	PASS
174	95	50	100	91.8	102282	PASS
175	174	5	9	7.8	7981	PASS
176	174	95	101	97.1	99269	PASS
177	176	5	9	6.3	6246	PASS