


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN062518\
Data File : VN049529.D
Acq On : 25 Jun 2018 23:38
Operator : MD\SY
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N061618W.M
Title : SW846 8260
Last Update : Sat Jun 16 01:02:01 2018

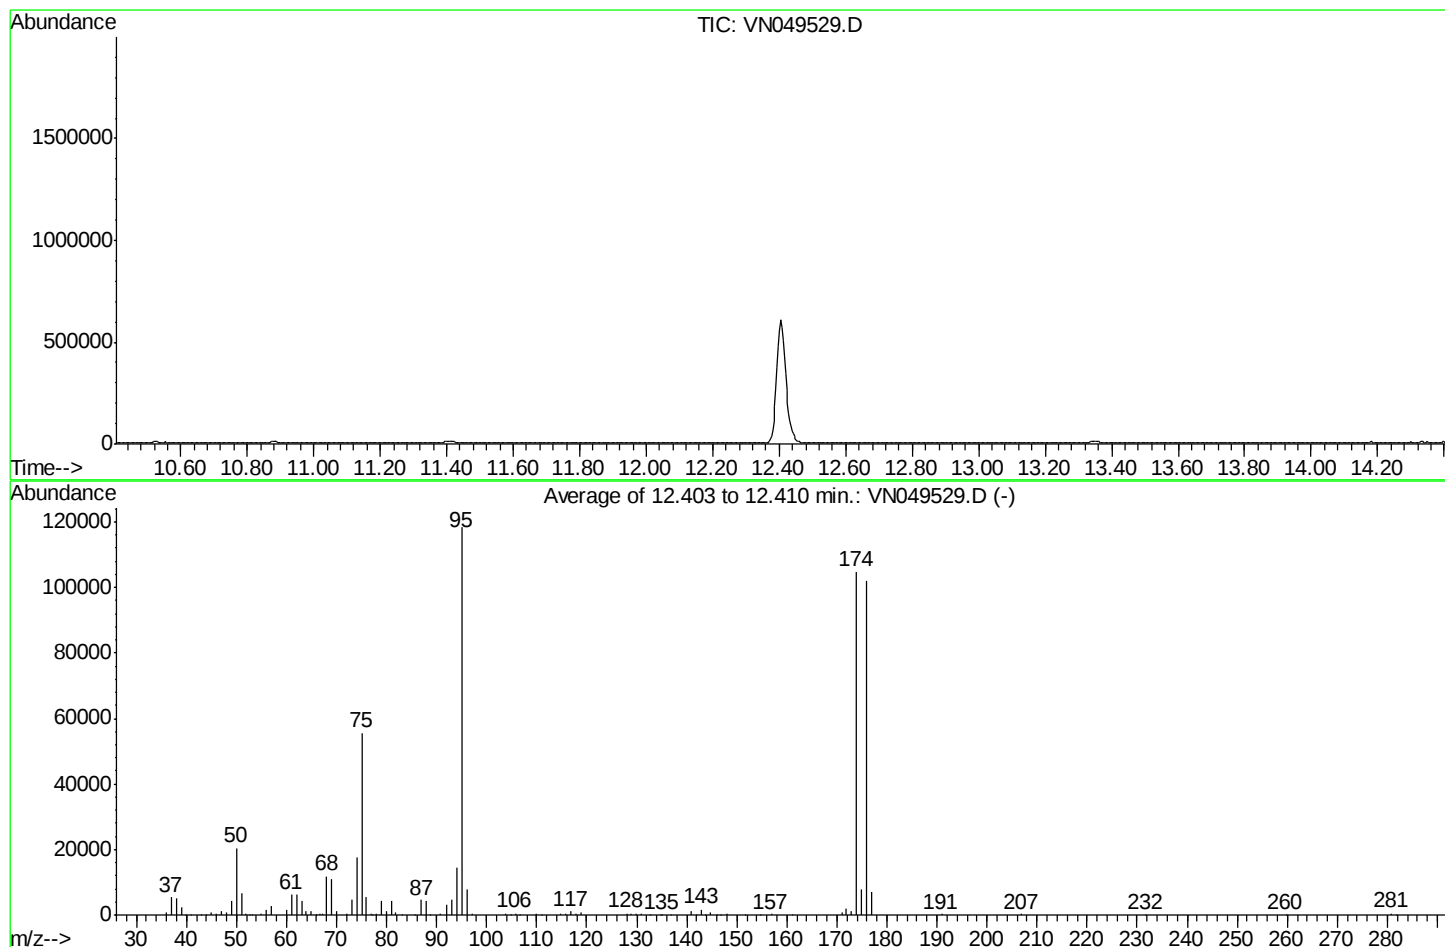

AutoFind: Scans 3363, 3364, 3365; Background Corrected with Scan 3349

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.3	20434	PASS
75	95	30	60	47.0	55642	PASS
95	95	100	100	100.0	118365	PASS
96	95	5	9	6.6	7838	PASS
173	174	0.00	2	1.2	1274	PASS
174	95	50	100	88.5	104746	PASS
175	174	5	9	7.5	7813	PASS
176	174	95	101	97.6	102202	PASS
177	176	5	9	6.9	7090	PASS