

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN062521\
 Data File : VN067502.D
 Acq On : 25 Jun 2021 14:18
 Operator : JC/MD
 Sample : M2806-09
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :

Quant Time: Jun 26 00:37:58 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N062421W.M
 Quant Title : SW846 8260
 QLast Update : Thu Jun 24 12:18:45 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.091	168	201503	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.971	114	457291	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.749	117	412603	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.677	152	132202	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.440	65	232014	56.26	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	=	112.52%
35) Dibromofluoromethane	8.024	113	141089	50.08	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	=	100.16%
50) Toluene-d8	10.443	98	639393	53.21	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	=	106.42%
62) 4-Bromofluorobenzene	12.733	95	214392	50.08	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	=	100.16%


Target Compounds						Qvalue
3) Chloromethane	2.300	50	962	0.25	ug/l #	80
5) Bromomethane	2.869	94	604	0.32	ug/l #	76
11) Tert butyl alcohol	5.331	59	326	0.48	ug/l #	71
13) Acrolein	4.038	56	455	0.79	ug/l #	4
16) Acetone	4.309	43	2465	1.56	ug/l #	48
17) Carbon Disulfide	4.532	76	2535	0.28	ug/l #	74
25) 2-Butanone	7.348	43	527	0.21	ug/l #	51
29) Tetrahydrofuran	7.705	42	429	0.28	ug/l #	45
31) Cyclohexane	8.088	56	8809	1.33	ug/l #	31
36) 1,1-Dichloropropene	8.088	75	28836	5.60	ug/l #	50
38) Carbon Tetrachloride	8.088	117	28279	6.45	ug/l #	17
51) 4-Methyl-2-Pentanone	10.336	43	3163	0.58	ug/l #	73
53) t-1,3-Dichloropropene	10.722	75	339	2.05	ug/l #	1
58) 2-Chloroethyl Vinyl ether	10.043	63	24	17.24	ug/l #	50
59) 2-Hexanone	11.095	43	5302	1.37	ug/l	93
60) Dibromochloromethane	10.985	129	188	2.08	ug/l #	11
71) Bromoform	12.736	173	1948	3.48	ug/l #	1
74) N-amyl acetate	12.393	43	3031	0.47	ug/l #	80
76) 1,2,3-Trichloropropane	12.733	75	129038	33.16	ug/l #	100
77) Bromobenzene	12.867	156	528	0.21	ug/l #	54
78) n-propylbenzene	12.921	91	3368	0.20	ug/l	92
81) trans-1,4-Dichloro-2-b...	12.733	75	129038	90.75	ug/l #	6
82) 4-Chlorotoluene	13.109	91	2716	0.28	ug/l	94
84) 1,2,4-Trimethylbenzene	13.369	105	2374	0.22	ug/l	99
87) 1,3-Dichlorobenzene	13.618	146	1200	0.27	ug/l	87
88) 1,4-Dichlorobenzene	13.618	146	1200	0.27	ug/l	88
89) n-Butylbenzene	13.948	91	4959	0.51	ug/l	96
91) 1,2-Dichlorobenzene	13.991	146	1357	0.31	ug/l	86
92) 1,2-Dibromo-3-Chloropr...	14.600	75	240	0.31	ug/l #	16
93) 1,2,4-Trichlorobenzene	15.265	180	2414	3.36	ug/l	97
95) Naphthalene	15.509	128	14267	5.14	ug/l #	77
96) 1,2,3-Trichlorobenzene	15.708	180	3063	3.90	ug/l	87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN062521\
Data File : VN067502.D
Acq On : 25 Jun 2021 14:18
Operator : JC/MD
Sample : M2806-09
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampled :

Quant Time: Jun 26 00:37:58 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N062421W.M
Quant Title : SW846 8260
QLast Update : Thu Jun 24 12:18:45 2021
Response via : Initial Calibration




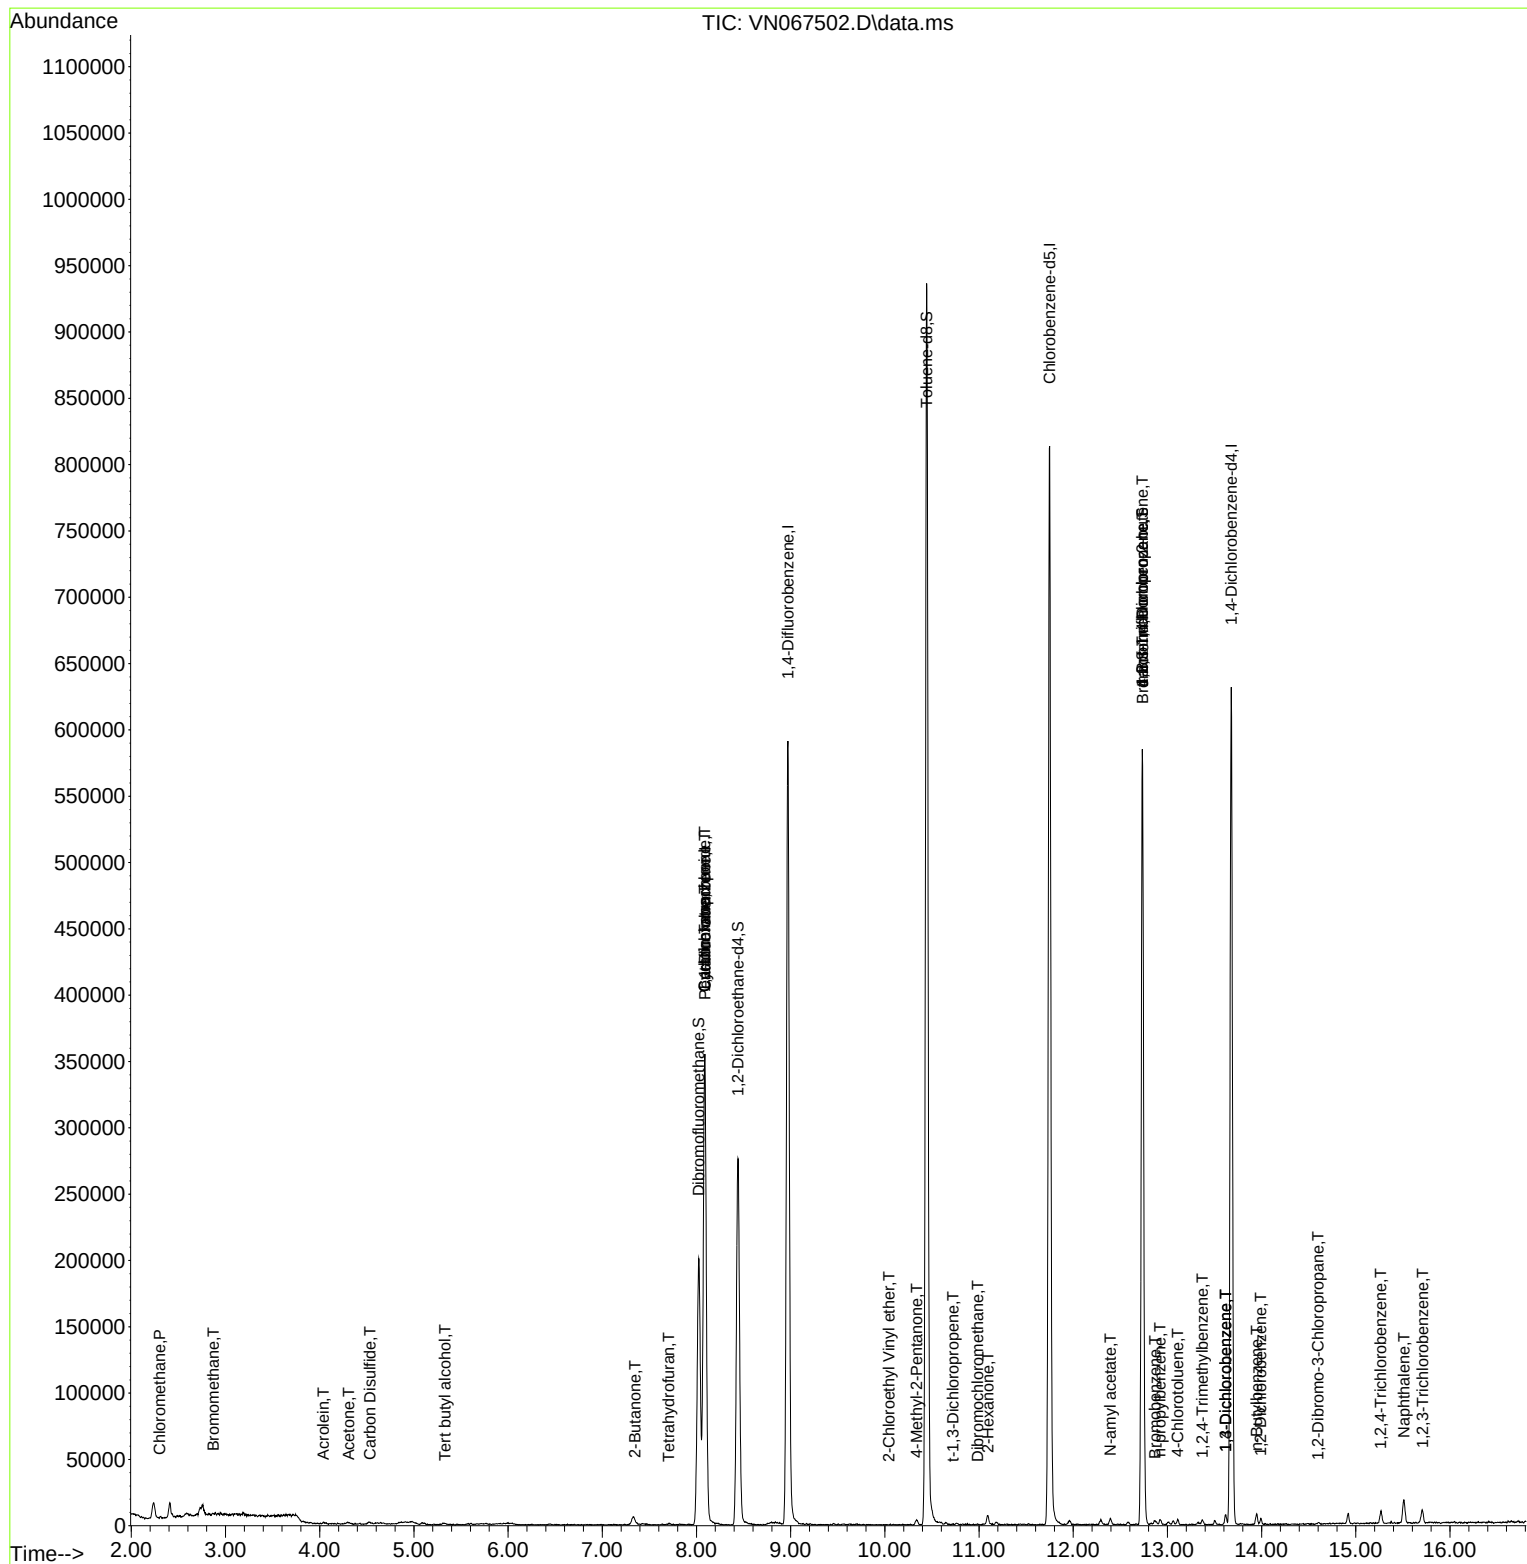


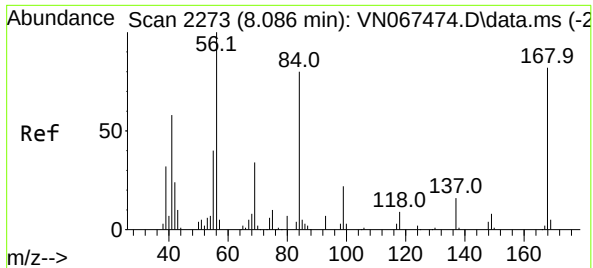

#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 8.091 min Scan# 2275
Delta R.T. 0.005 min
Lab File: VN067502.D
Acq: 25 Jun 2021 14:18




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion:168 Resp: 201503
Ion Ratio Lower Upper
168 100
99 88.2 62.9 94.3

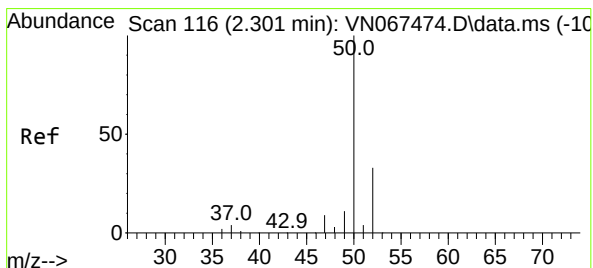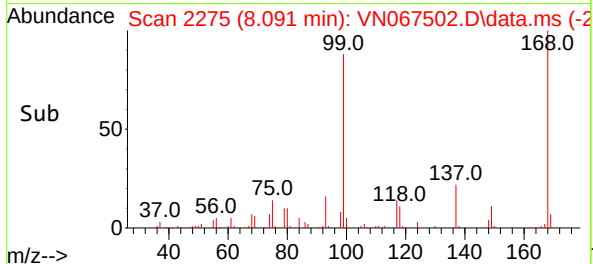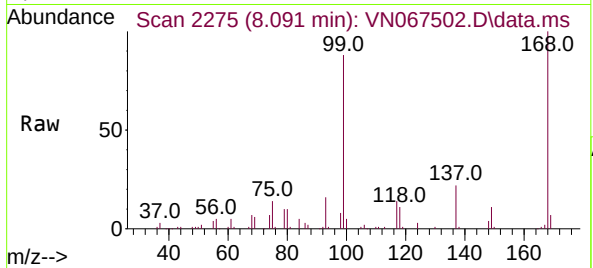

#3
Chloromethane
Concen: 0.25 ug/l
RT: 2.300 min Scan# 116
Delta R.T. -0.001 min
Lab File: VN067502.D
Acq: 25 Jun 2021 14:18


Tgt Ion: 50 Resp: 962
Ion Ratio Lower Upper
50 100
52 43.2 25.6 38.4#

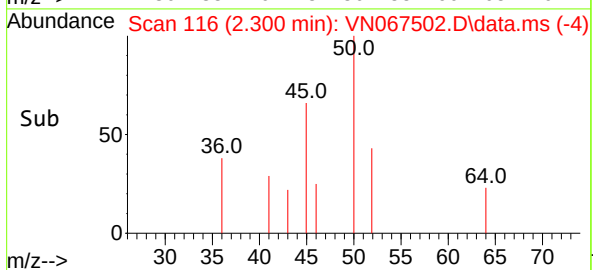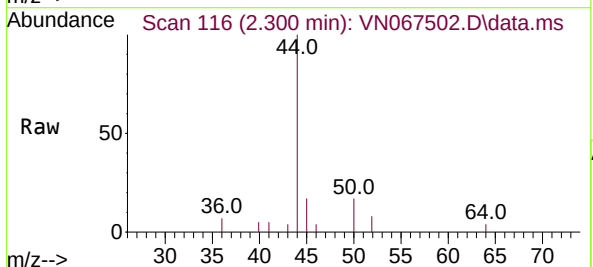






#5
Bromomethane
Concen: 0.32 ug/l
RT: 2.869 min Scan# 328
Delta R.T. 0.037 min
Lab File: VN067502.D
Acq: 25 Jun 2021 14:18

Instrument :
MSVOA_N
ClientSampled :







Tgt Ion: 94 Resp: 604
Ion Ratio Lower Upper
94 100
96 69.7 73.7 110.5#



#11
Tert butyl alcohol
Concen: 0.48 ug/l
RT: 5.331 min Scan# 1246
Delta R.T. -0.057 min
Lab File: VN067502.D
Acq: 25 Jun 2021 14:18

Tgt Ion: 59 Resp: 326
Ion Ratio Lower Upper
59 100
57 0.0 8.7 13.1#









#13
Acrolein
Concen: 0.79 ug/l
RT: 4.038 min Scan# 764
Delta R.T. -0.001 min
Lab File: VN067502.D
Acq: 25 Jun 2021 14:18




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 56 Resp: 455
Ion Ratio Lower Upper
56 100
55 151.6 57.4 86.0#



#16
Acetone
Concen: 1.56 ug/l
RT: 4.309 min Scan# 865
Delta R.T. 0.018 min
Lab File: VN067502.D
Acq: 25 Jun 2021 14:18

Tgt Ion: 43 Resp: 2465
Ion Ratio Lower Upper
43 100
58 0.0 21.2 31.8#

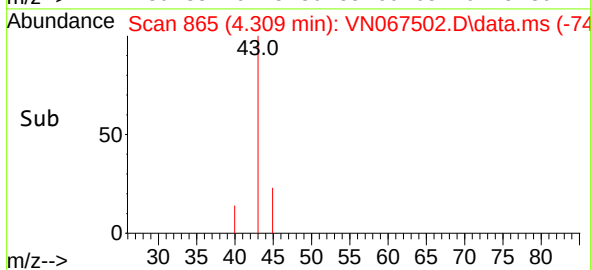

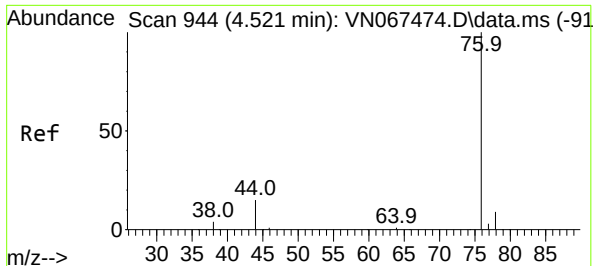

#17

Carbon Disulfide


Concen: 0.28 ug/l

RT: 4.532 min Scan# 948

Delta R.T. 0.011 min

Lab File: VN067502.D

Acq: 25 Jun 2021 14:18



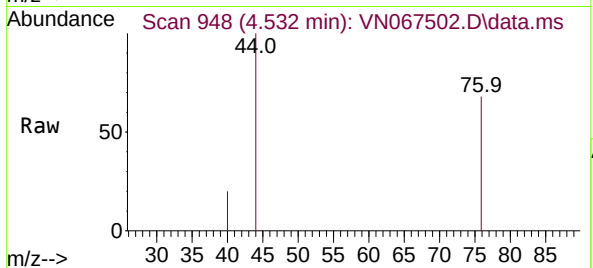


Tgt Ion: 76 Resp: 2535

Ion Ratio Lower Upper

76 100

78 0.0 7.7 11.5#

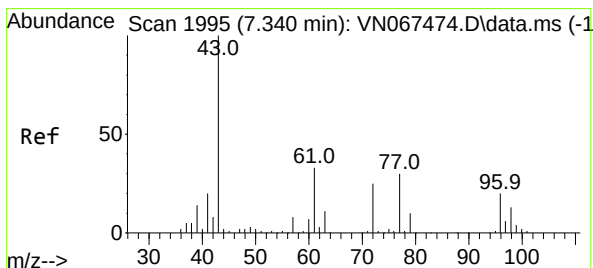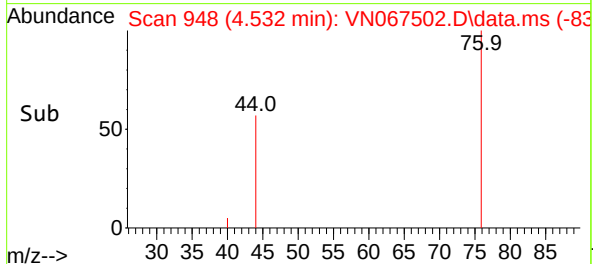

#25

2-Butanone


Concen: 0.21 ug/l

RT: 7.348 min Scan# 1998

Delta R.T. 0.008 min

Lab File: VN067502.D

Acq: 25 Jun 2021 14:18


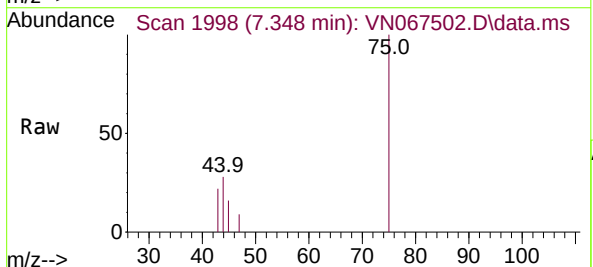



Tgt Ion: 43 Resp: 527

Ion Ratio Lower Upper

43 100

72 0.0 19.7 29.5#

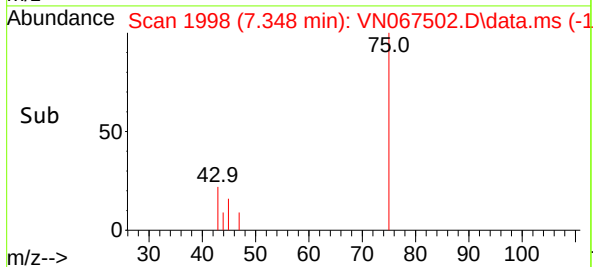



#29

Tetrahydrofuran

Concen: 0.28 ug/l


RT: 7.705 min Scan# 2131

Delta R.T. 0.016 min




Lab File: VN067502.D

Acq: 25 Jun 2021 14:18

Instrument :
MSVOA_N
ClientSampled :



Tgt Ion:	42	Resp:	429
Ion Ratio	Lower	Upper	
42	100		
72	0.0	32.8	49.2#
71	11.7	31.2	46.8#



#31

Cyclohexane

Concen: 1.33 ug/l




RT: 8.088 min Scan# 2274


Delta R.T. -0.008 min

Lab File: VN067502.D

Acq: 25 Jun 2021 14:18

Tgt Ion:	56	Resp:	8809
Ion Ratio	Lower	Upper	
56	100		
69	136.6	27.3	40.9#
84	101.8	64.9	97.3#

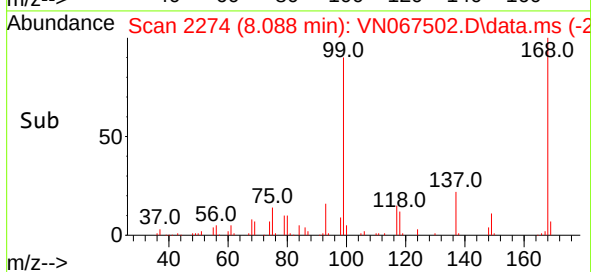



#33

1,2-Dichloroethane-d4

Concen: 56.26 ug/l

RT: 8.440 min Scan# 2405

Delta R.T. -0.000 min

Lab File: VN067502.D

Acq: 25 Jun 2021 14:18

Tgt Ion: 65 Resp: 232014

Ion Ratio Lower Upper





65 100

67 52.7 0.0 98.6

Instrument :

MSVOA_N

ClientSampled :

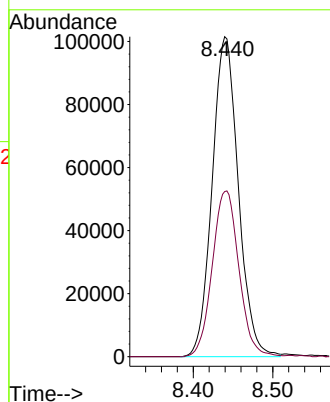

#34

1,4-Difluorobenzene

Concen: 50.00 ug/l

RT: 8.971 min Scan# 2603

Delta R.T. -0.000 min

Lab File: VN067502.D

Acq: 25 Jun 2021 14:18




Tgt Ion: 114 Resp: 457291


Ion Ratio Lower Upper

114 100

63 27.8 0.0 49.0

88 18.2 0.0 36.6



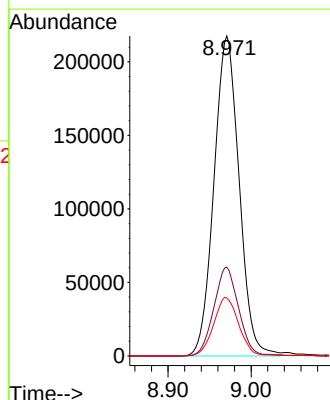





#35
Dibromofluoromethane
Concen: 50.08 ug/l
RT: 8.024 min Scan# 2250
Delta R.T. -0.000 min
Lab File: VN067502.D
Acq: 25 Jun 2021 14:18




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:113 Resp: 141089
Ion Ratio Lower Upper
113 100
111 105.8 83.8 125.8
192 12.6 13.4 20.0#

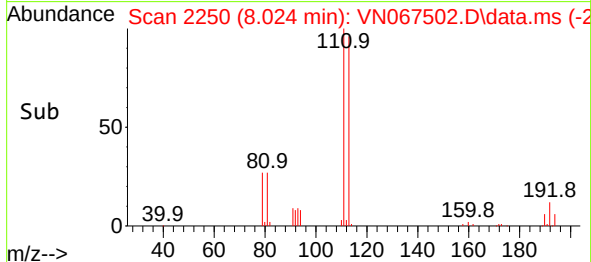

#36
1,1-Dichloropropene
Concen: 5.60 ug/l
RT: 8.088 min Scan# 2274
Delta R.T. -0.134 min
Lab File: VN067502.D
Acq: 25 Jun 2021 14:18


Tgt Ion: 75 Resp: 28836
Ion Ratio Lower Upper
75 100
110 7.2 15.7 47.0#
77 0.0 24.6 37.0#

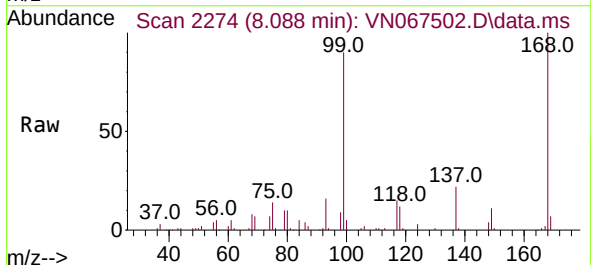






#38
Carbon Tetrachloride
Concen: 6.45 ug/l
RT: 8.088 min Scan# 2274
Delta R.T. -0.118 min
Lab File: VN067502.D
Acq: 25 Jun 2021 14:18

Instrument :
MSVOA_N
ClientSampled :



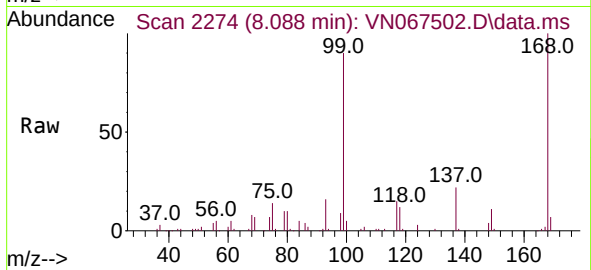



Tgt Ion:117 Resp: 28279
Ion Ratio Lower Upper
117 100
119 5.0 75.4 113.2#
121 0.0 23.5 35.3#

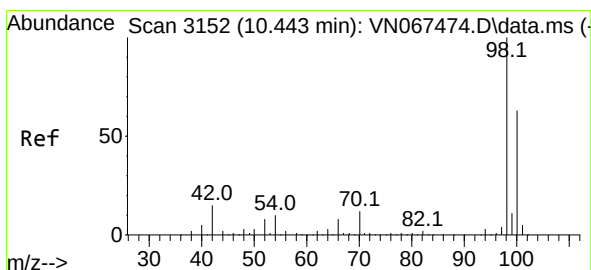

#50
Toluene-d8
Concen: 53.21 ug/l
RT: 10.443 min Scan# 3152
Delta R.T. -0.000 min
Lab File: VN067502.D
Acq: 25 Jun 2021 14:18

Tgt Ion: 98 Resp: 639393
Ion Ratio Lower Upper
98 100
100 61.3 51.7 77.5


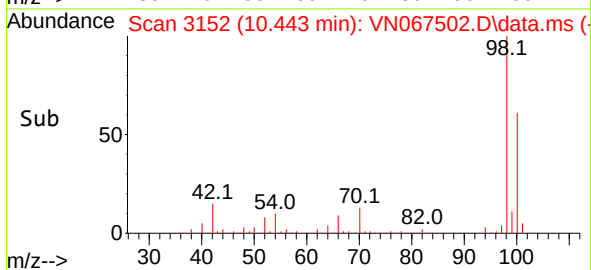






#51
4-Methyl-2-Pentanone
Concen: 0.58 ug/l
RT: 10.336 min Scan# 3112
Delta R.T. 0.003 min
Lab File: VN067502.D
Acq: 25 Jun 2021 14:18




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 43 Resp: 3163
Ion Ratio Lower Upper
43 100
58 19.8 28.6 43.0#



#53
t-1,3-Dichloropropene
Concen: 2.05 ug/l
RT: 10.722 min Scan# 3256
Delta R.T. -0.000 min
Lab File: VN067502.D
Acq: 25 Jun 2021 14:18

Tgt Ion: 75 Resp: 339
Ion Ratio Lower Upper
75 100
77 98.1 25.1 37.7#


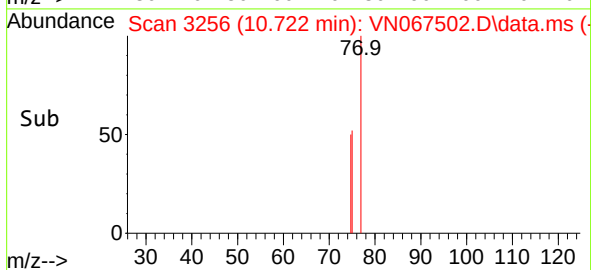






#58
2-Chloroethyl Vinyl ether
Concen: 17.24 ug/l
RT: 10.043 min Scan# 3003
Delta R.T. 0.000 min
Lab File: VN067502.D
Acq: 25 Jun 2021 14:18




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 63 Resp: 24
Ion Ratio Lower Upper
63 100
106 0.0 19.8 29.8#

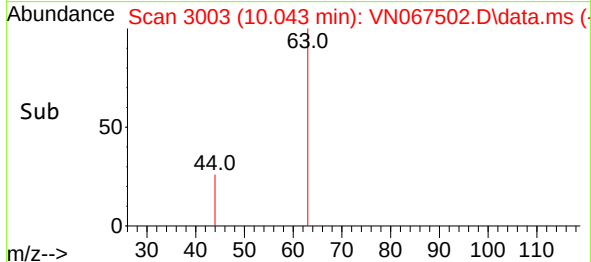

#59
2-Hexanone
Concen: 1.37 ug/l
RT: 11.095 min Scan# 3395
Delta R.T. 0.008 min
Lab File: VN067502.D
Acq: 25 Jun 2021 14:18

Tgt Ion: 43 Resp: 5302
Ion Ratio Lower Upper
43 100
58 44.9 24.7 74.1




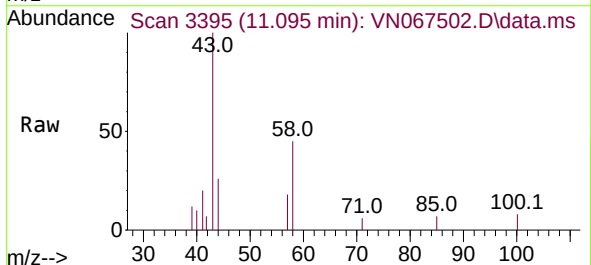




#60
Dibromochloromethane
Concen: 2.08 ug/l
RT: 10.985 min Scan# 3354
Delta R.T. -0.257 min
Lab File: VN067502.D
Acq: 25 Jun 2021 14:18




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion:129 Resp: 188
Ion Ratio Lower Upper
129 100
127 0.0 38.6 115.8#



#62
4-Bromofluorobenzene
Concen: 50.08 ug/l
RT: 12.733 min Scan# 4006
Delta R.T. 0.000 min
Lab File: VN067502.D
Acq: 25 Jun 2021 14:18

Tgt Ion: 95 Resp: 214392
Ion Ratio Lower Upper
95 100
174 50.4 0.0 122.0
176 48.7 0.0 117.6









#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 11.749 min Scan# 3639
Delta R.T. 0.003 min
Lab File: VN067502.D
Acq: 25 Jun 2021 14:18




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:117 Resp: 412603
Ion Ratio Lower Upper
117 100
82 70.3 53.1 79.7
119 31.8 25.5 38.3

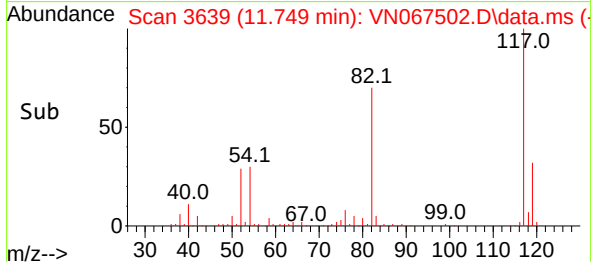

#71
Bromoform
Concen: 3.48 ug/l
RT: 12.736 min Scan# 4007
Delta R.T. 0.276 min
Lab File: VN067502.D
Acq: 25 Jun 2021 14:18

Tgt Ion:173 Resp: 1948
Ion Ratio Lower Upper
173 100
175 422.2 23.9 71.8#
254 0.0 0.0 0.0




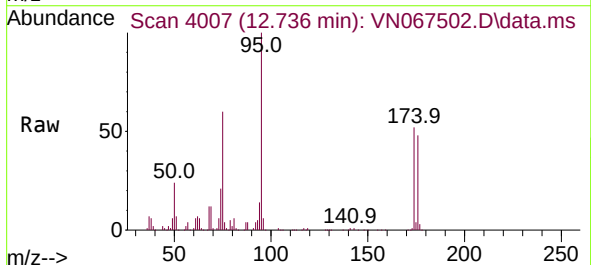




#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 13.677 min Scan# 4358
Delta R.T. 0.002 min
Lab File: VN067502.D
Acq: 25 Jun 2021 14:18




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:152 Resp: 132202
Ion Ratio Lower Upper
152 100
115 77.6 36.1 108.5
150 159.1 0.0 351.8

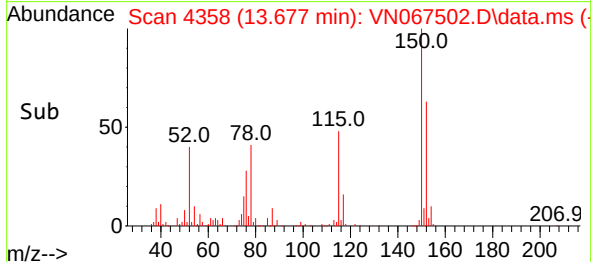

#74
N-amy1 acetate
Concen: 0.47 ug/l
RT: 12.393 min Scan# 3879
Delta R.T. 0.003 min
Lab File: VN067502.D
Acq: 25 Jun 2021 14:18

Tgt Ion: 43 Resp: 3031
Ion Ratio Lower Upper
43 100
70 37.6 29.4 44.2
55 9.2 17.0 25.4#
61 0.0 17.6 26.4#




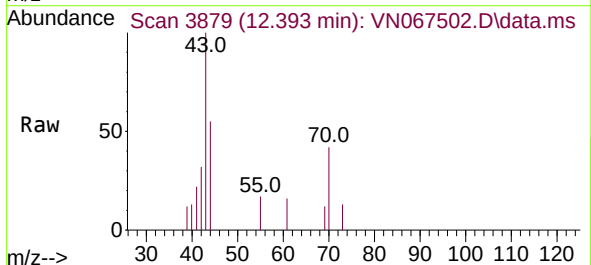




#76
1,2,3-Trichloropropane
Concen: 33.16 ug/l
RT: 12.733 min Scan# 4006
Delta R.T. -0.151 min
Lab File: VN067502.D
Acq: 25 Jun 2021 14:18




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 75 Resp: 129038
Ion Ratio Lower Upper
75 100
77 0.9 0.0 0.0#

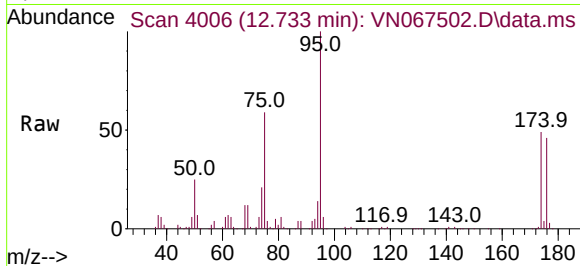

#77
Bromobenzene
Concen: 0.21 ug/l
RT: 12.867 min Scan# 4056
Delta R.T. 0.005 min
Lab File: VN067502.D
Acq: 25 Jun 2021 14:18

Tgt Ion:156 Resp: 528
Ion Ratio Lower Upper
156 100
77 350.8 136.2 408.6
158 43.6 48.4 145.3#




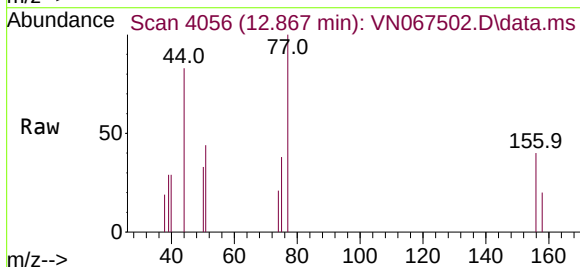




#78
n-propylbenzene
Concen: 0.20 ug/l
RT: 12.921 min Scan# 4076
Delta R.T. 0.000 min
Lab File: VN067502.D
Acq: 25 Jun 2021 14:18




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 91 Resp: 3368
Ion Ratio Lower Upper
91 100
120 17.1 10.4 31.4



#81
trans-1,4-Dichloro-2-butene
Concen: 90.75 ug/l
RT: 12.733 min Scan# 4006
Delta R.T. 0.104 min
Lab File: VN067502.D
Acq: 25 Jun 2021 14:18

Tgt Ion: 75 Resp: 129038
Ion Ratio Lower Upper
75 100
53 0.0 87.6 131.4#
89 0.0 37.8 56.8#



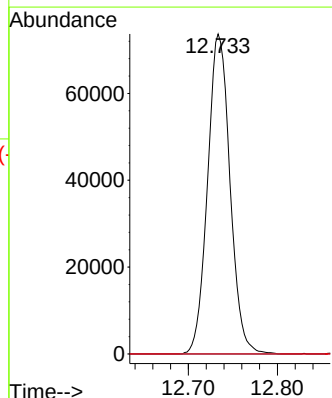



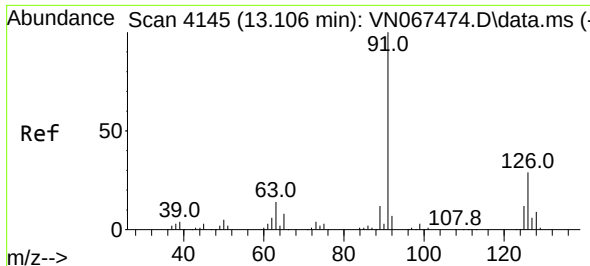

#82
4-Chlorotoluene
Concen: 0.28 ug/l
RT: 13.109 min Scan# 4146
Delta R.T. 0.003 min
Lab File: VN067502.D
Acq: 25 Jun 2021 14:18




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 91 Resp: 2716
Ion Ratio Lower Upper
91 100
126 26.6 14.8 44.4

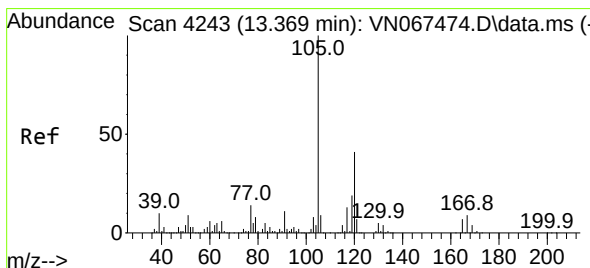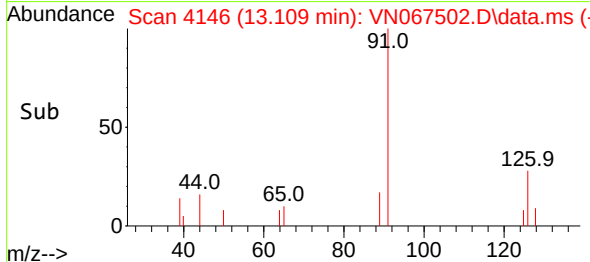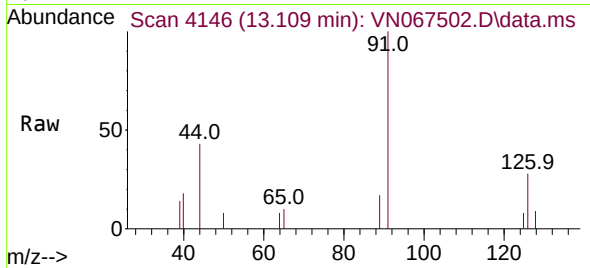

#84
1,2,4-Trimethylbenzene
Concen: 0.22 ug/l
RT: 13.369 min Scan# 4243
Delta R.T. -0.000 min
Lab File: VN067502.D
Acq: 25 Jun 2021 14:18

Tgt Ion: 105 Resp: 2374
Ion Ratio Lower Upper
105 100
120 40.7 20.6 61.8


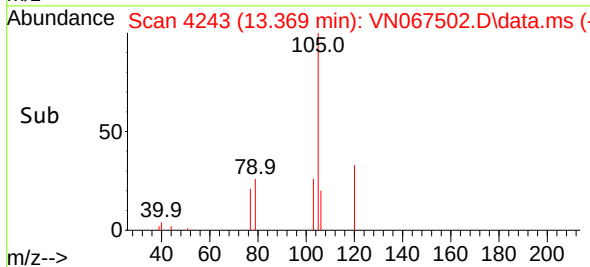

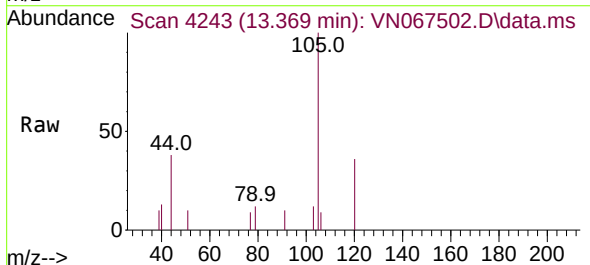




#87
1,3-Dichlorobenzene
Concen: 0.27 ug/l
RT: 13.618 min Scan# 4336
Delta R.T. 0.002 min
Lab File: VN067502.D
Acq: 25 Jun 2021 14:18




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:146 Resp: 1200
Ion Ratio Lower Upper
146 100
111 30.3 24.3 72.8
148 65.8 32.0 96.0

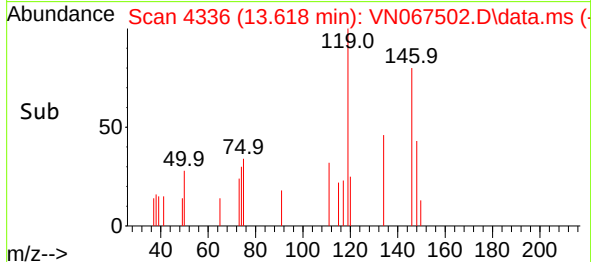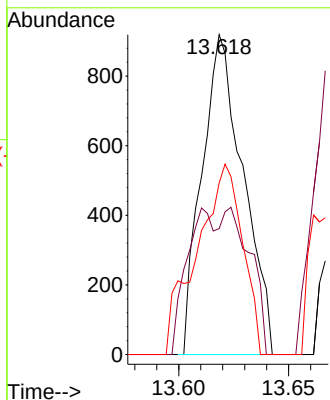

#88
1,4-Dichlorobenzene
Concen: 0.27 ug/l
RT: 13.618 min Scan# 4336
Delta R.T. -0.078 min
Lab File: VN067502.D
Acq: 25 Jun 2021 14:18

Tgt Ion:146 Resp: 1200
Ion Ratio Lower Upper
146 100
111 30.3 23.4 70.2
148 65.8 31.8 95.3



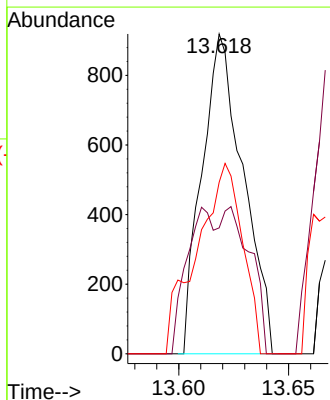
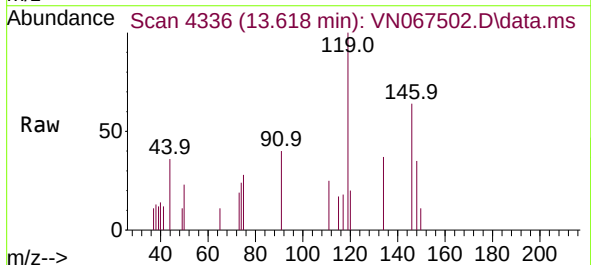


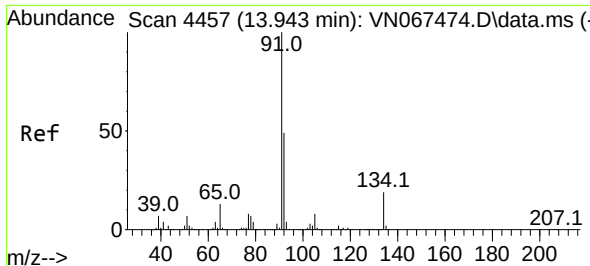

#89
n-Butylbenzene
Concen: 0.51 ug/l
RT: 13.948 min Scan# 4459
Delta R.T. 0.005 min
Lab File: VN067502.D
Acq: 25 Jun 2021 14:18




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 91	Resp:	4959
Ion Ratio	Lower	Upper
91	100	
92	52.7	25.7 77.1
134	17.9	11.2 33.6

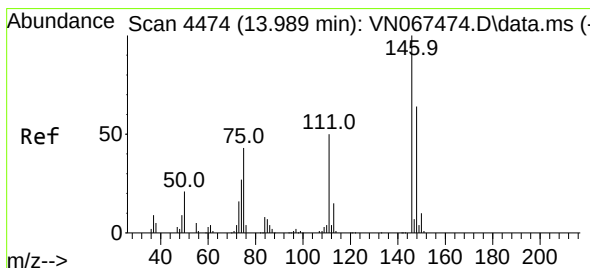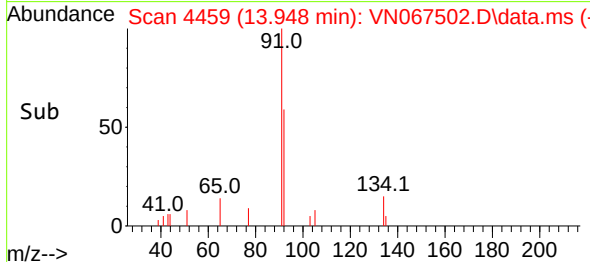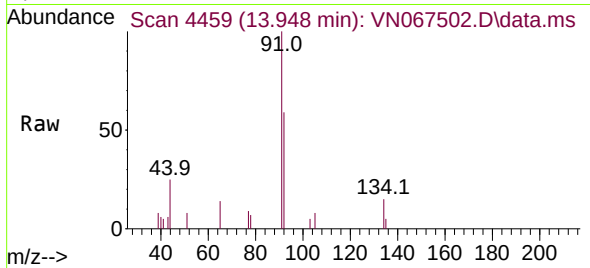

#91
1,2-Dichlorobenzene
Concen: 0.31 ug/l
RT: 13.991 min Scan# 4475
Delta R.T. 0.002 min
Lab File: VN067502.D
Acq: 25 Jun 2021 14:18

Tgt Ion: 146	Resp:	1357
Ion Ratio	Lower	Upper
146	100	
111	62.6	24.9 74.6
148	70.8	31.6 95.0


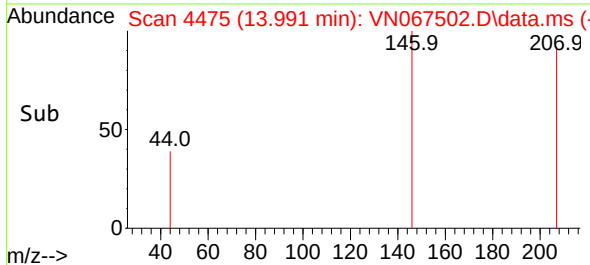

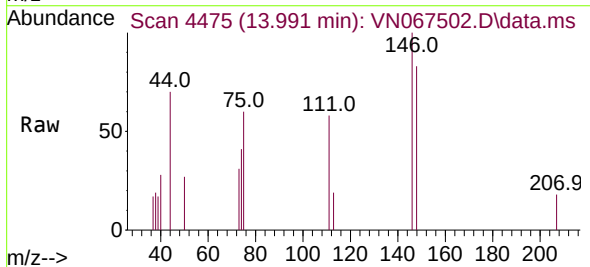




#92
1,2-Dibromo-3-Chloropropane
Concen: 0.31 ug/l
RT: 14.600 min Scan# 4702
Delta R.T. -0.003 min
Lab File: VN067502.D
Acq: 25 Jun 2021 14:18




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 75 Resp: 240
Ion Ratio Lower Upper
75 100
155 0.0 29.8 89.5#
157 0.0 37.6 112.8#

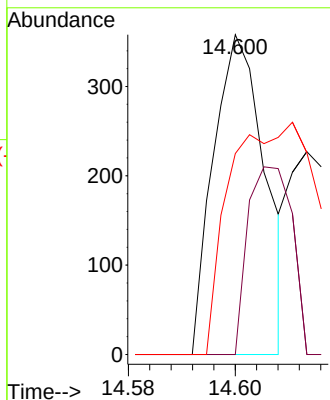

#93
1,2,4-Trichlorobenzene
Concen: 3.36 ug/l
RT: 15.265 min Scan# 4950
Delta R.T. 0.000 min
Lab File: VN067502.D
Acq: 25 Jun 2021 14:18

Tgt Ion:180 Resp: 2414
Ion Ratio Lower Upper
180 100
182 93.1 47.5 142.5
145 38.8 17.2 51.6



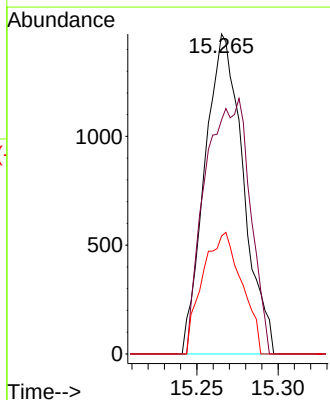
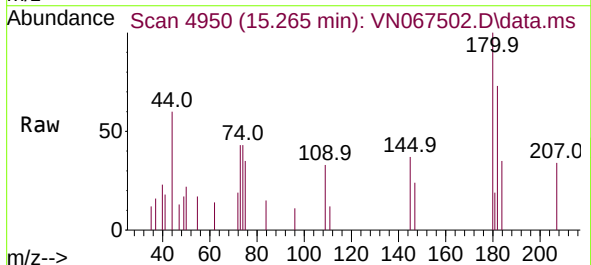




#95
Naphthalene
Concen: 5.14 ug/l
RT: 15.509 min Scan# 5041
Delta R.T. 0.002 min
Lab File: VN067502.D
Acq: 25 Jun 2021 14:18

Instrument :
MSVOA_N
ClientSampled :

Tgt Ion:128 Resp: 14267
Ion Ratio Lower Upper
128 100
127 5.6 10.6 15.8#
129 0.0 8.6 12.8#

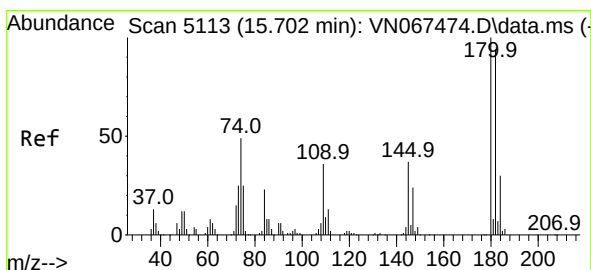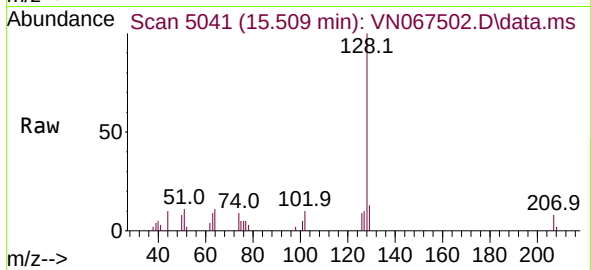

#96
1,2,3-Trichlorobenzene
Concen: 3.90 ug/l
RT: 15.708 min Scan# 5115
Delta R.T. 0.006 min
Lab File: VN067502.D
Acq: 25 Jun 2021 14:18

Tgt Ion:180 Resp: 3063
Ion Ratio Lower Upper
180 100
182 80.9 47.8 143.3
145 40.9 18.2 54.6

