

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN062521\
 Data File : VN067504.D
 Acq On : 25 Jun 2021 15:06
 Operator : JC/MD
 Sample : M2806-02 10X
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :

Quant Time: Jun 26 00:38:26 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N062421W.M
 Quant Title : SW846 8260
 QLast Update : Thu Jun 24 12:18:45 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.088	168	201952	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.971	114	459131	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.749	117	410048	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.678	152	150978	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.440	65	227835	55.12	ug/l	0.00
Spiked Amount 50.000	Range 61 - 141		Recovery = 110.24%			
35) Dibromofluoromethane	8.024	113	140250	49.58	ug/l	0.00
Spiked Amount 50.000	Range 69 - 133		Recovery = 99.16%			
50) Toluene-d8	10.443	98	636287	52.74	ug/l	0.00
Spiked Amount 50.000	Range 65 - 126		Recovery = 105.48%			
62) 4-Bromofluorobenzene	12.734	95	220928	51.40	ug/l	0.00
Spiked Amount 50.000	Range 58 - 135		Recovery = 102.80%			
Target Compounds						Qvalue
3) Chloromethane	2.295	50	793	0.21	ug/l	99
5) Bromomethane	2.869	94	375	0.20	ug/l #	55
11) Tert butyl alcohol	5.390	59	269	0.40	ug/l #	71
13) Acrolein	4.036	56	349	0.61	ug/l #	14
16) Acetone	4.296	43	494	0.31	ug/l #	89
31) Cyclohexane	8.086	56	9539	1.44	ug/l #	1
36) 1,1-Dichloropropene	8.088	75	28967	5.60	ug/l #	50
38) Carbon Tetrachloride	8.088	117	27485	6.24	ug/l #	16
53) t-1,3-Dichloropropene	10.448	75	26	2.01	ug/l #	1
55) 1,1,2-Trichloroethane	10.888	97	1459	0.43	ug/l #	14
67) Ethyl Benzene	11.848	91	205628	11.85	ug/l	100
68) m/p-Xylenes	11.961	106	67495	11.49	ug/l	98
71) Bromoform	12.720	173	309	2.79	ug/l #	1
73) Isopropylbenzene	12.581	105	378028	24.60	ug/l	98
76) 1,2,3-Trichloropropane	12.921	75	6078	1.37	ug/l #	100
78) n-propylbenzene	12.924	91	786227	41.48	ug/l	96
79) 2-Chlorotoluene	12.924	91	786227	69.09	ug/l #	46
80) 1,3,5-Trimethylbenzene	13.061	105	106509	8.49	ug/l	96
81) trans-1,4-Dichloro-2-b...	12.581	75	5660	3.49	ug/l #	75
82) 4-Chlorotoluene	12.924	91	786227	70.37	ug/l #	45
83) tert-Butylbenzene	13.326	119	27731	2.80	ug/l	98
84) 1,2,4-Trimethylbenzene	13.369	105	2303025	187.03	ug/l	98
85) sec-Butylbenzene	13.503	105	144914	9.77	ug/l	83
86) p-Isopropyltoluene	13.619	119	28609	2.59	ug/l	98
89) n-Butylbenzene	13.943	91	66426	6.01	ug/l #	82
90) Hexachloroethane	14.219	117	19258	9.16	ug/l #	16
92) 1,2-Dibromo-3-Chloropr...	14.581	75	1499	1.69	ug/l #	16
93) 1,2,4-Trichlorobenzene	15.268	180	747	2.61	ug/l	79
95) Naphthalene	15.507	128	53976	9.32	ug/l	99
96) 1,2,3-Trichlorobenzene	15.708	180	578	2.75	ug/l #	42


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN062521\
Data File : VN067504.D
Acq On : 25 Jun 2021 15:06
Operator : JC/MD
Sample : M2806-02 10X
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :


Quant Time: Jun 26 00:38:26 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N062421W.M
Quant Title : SW846 8260
QLast Update : Thu Jun 24 12:18:45 2021
Response via : Initial Calibration

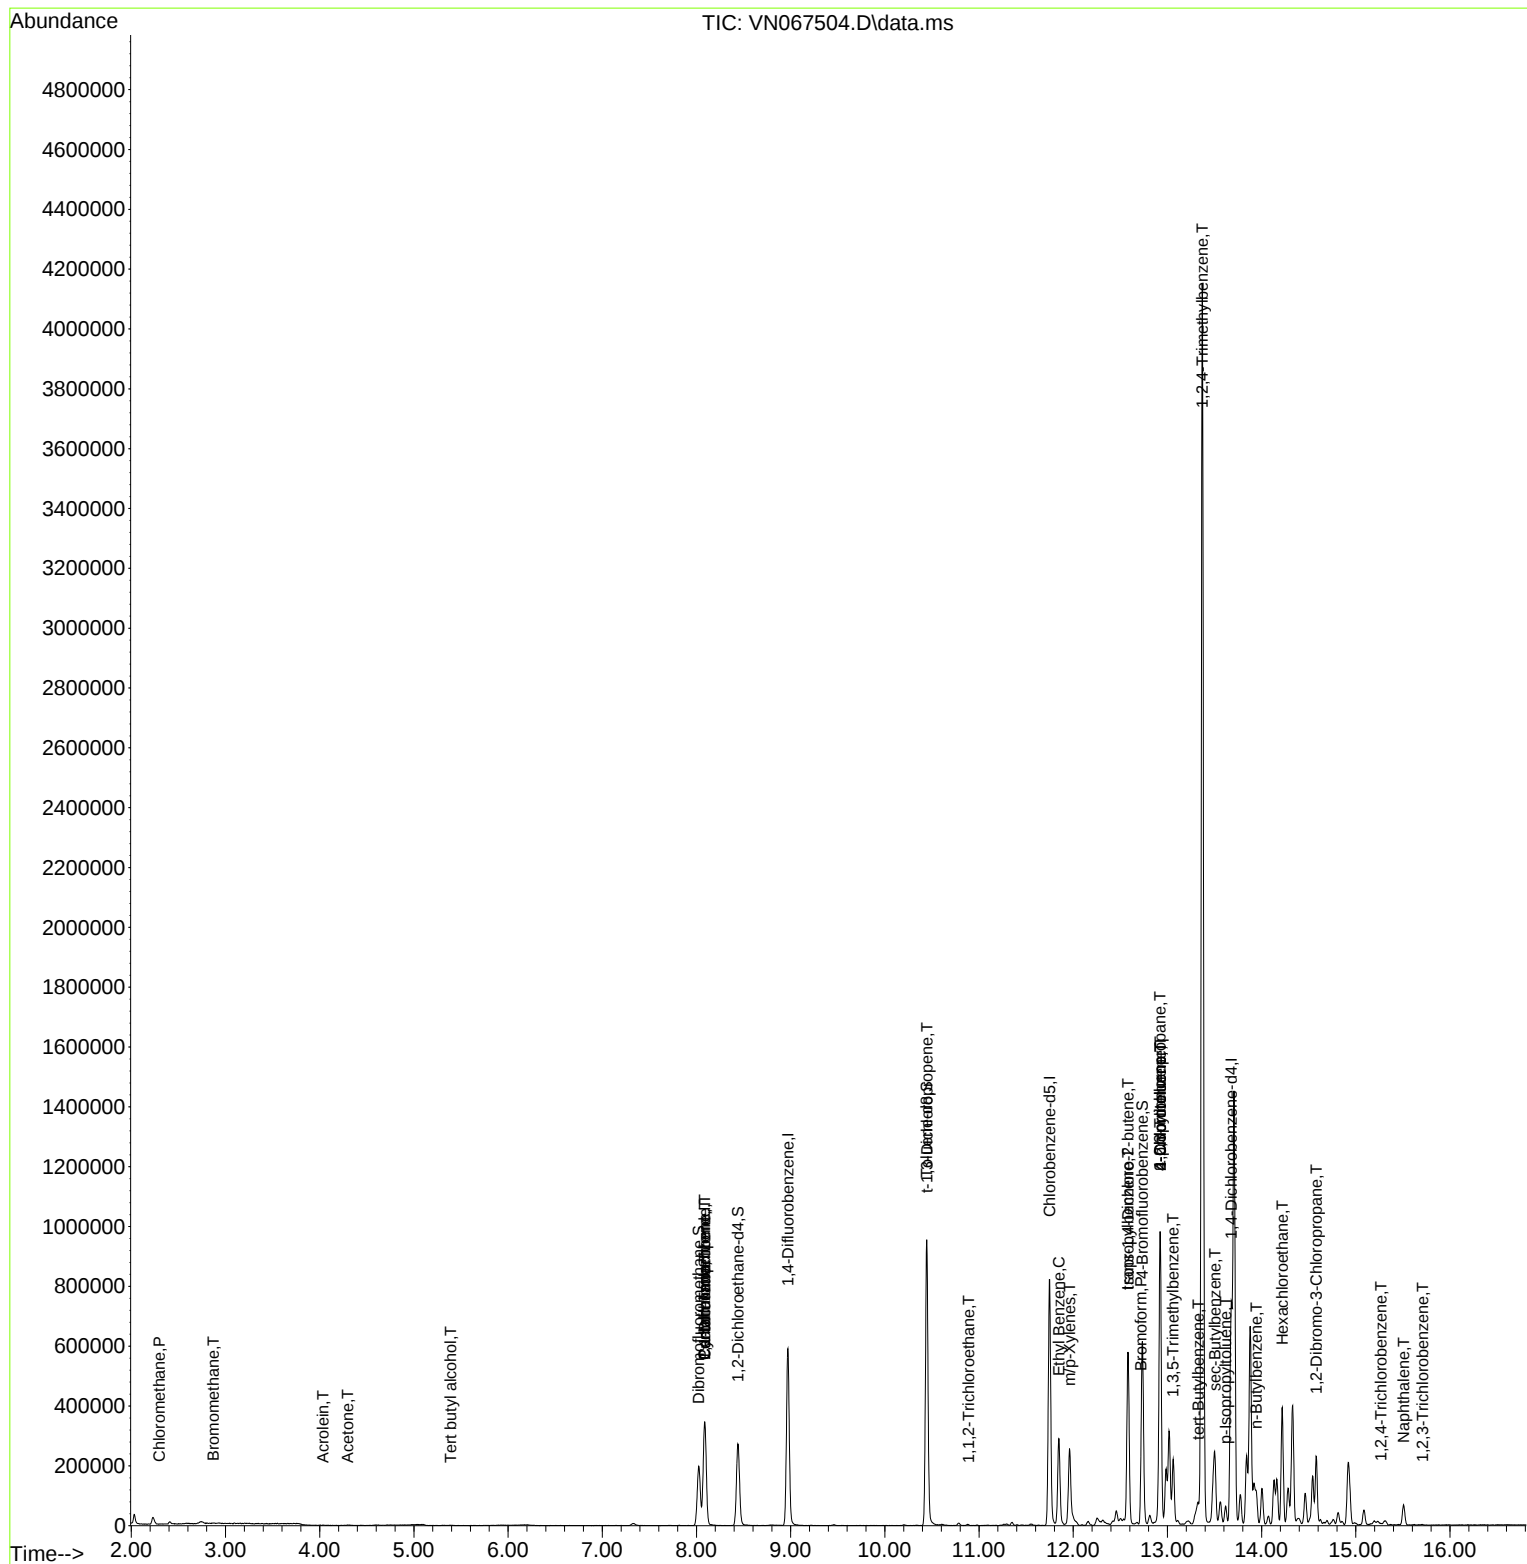



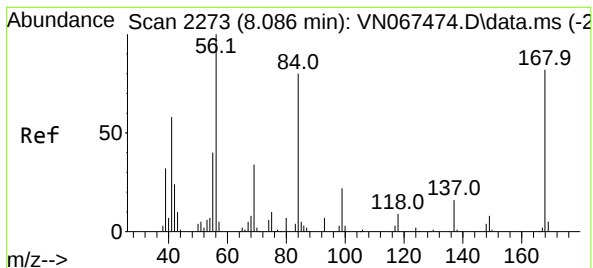


#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 8.088 min Scan# 2274
Delta R.T. 0.002 min
Lab File: VN067504.D
Acq: 25 Jun 2021 15:06

Instrument :
MSVOA_N
ClientSampled :



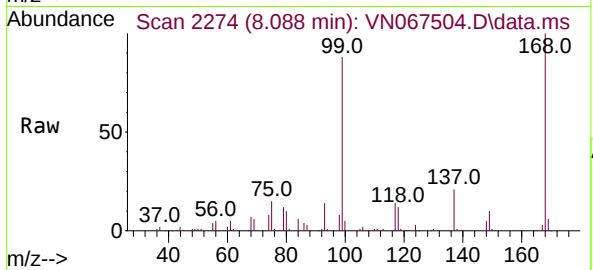



Tgt Ion:168 Resp: 201952
Ion Ratio Lower Upper
168 100
99 88.1 62.9 94.3

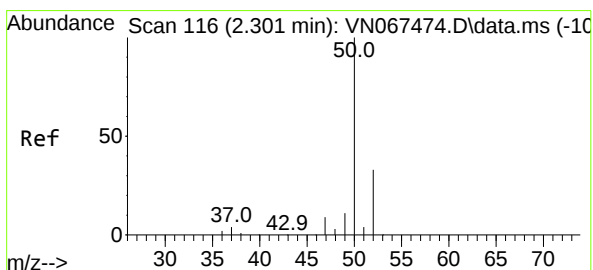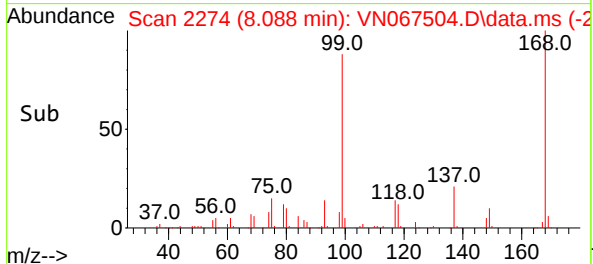

#3
Chloromethane
Concen: 0.21 ug/l
RT: 2.295 min Scan# 114
Delta R.T. -0.006 min
Lab File: VN067504.D
Acq: 25 Jun 2021 15:06


Tgt Ion: 50 Resp: 793
Ion Ratio Lower Upper
50 100
52 32.5 25.6 38.4

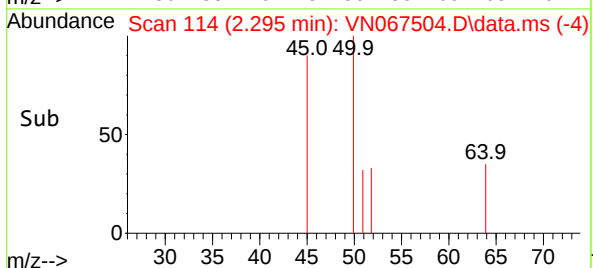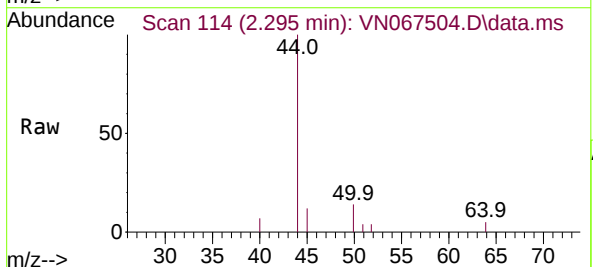






#5
Bromomethane
Concen: 0.20 ug/l
RT: 2.869 min Scan# 328
Delta R.T. 0.037 min
Lab File: VN067504.D
Acq: 25 Jun 2021 15:06

Instrument :
MSVOA_N
ClientSampled :







Tgt Ion: 94 Resp: 375
Ion Ratio Lower Upper
94 100
96 48.8 73.7 110.5#

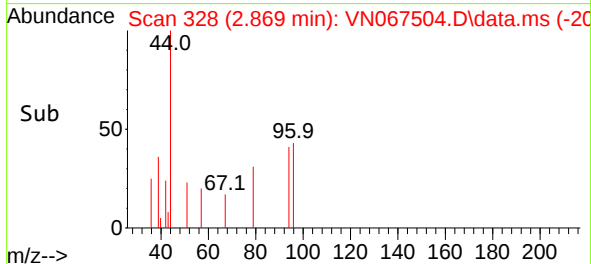

#11
Tert butyl alcohol
Concen: 0.40 ug/l
RT: 5.390 min Scan# 1268
Delta R.T. 0.002 min
Lab File: VN067504.D
Acq: 25 Jun 2021 15:06

Tgt Ion: 59 Resp: 269
Ion Ratio Lower Upper
59 100
57 0.0 8.7 13.1#




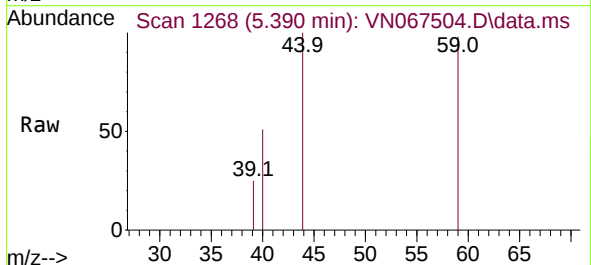


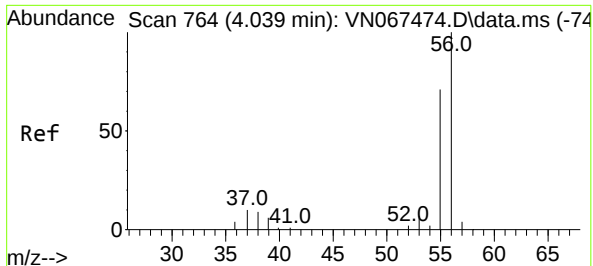

#13
Acrolein
Concen: 0.61 ug/l
RT: 4.036 min Scan# 763
Delta R.T. -0.003 min
Lab File: VN067504.D
Acq: 25 Jun 2021 15:06




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 56 Resp: 349
Ion Ratio Lower Upper
56 100
55 0.0 57.4 86.0#

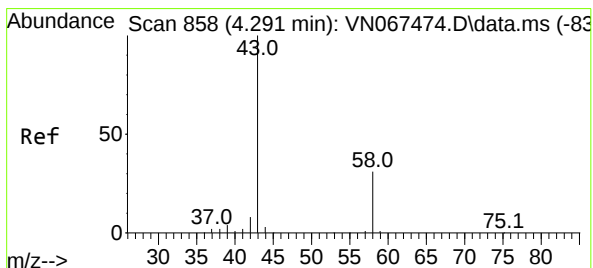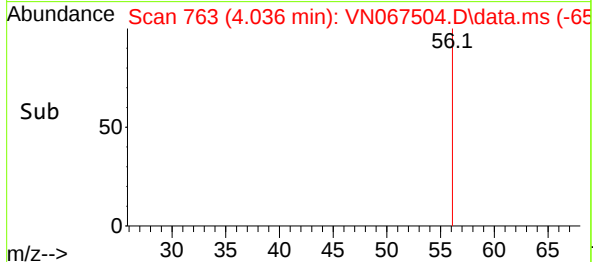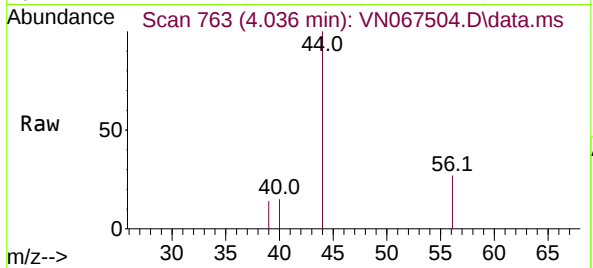

#16
Acetone
Concen: 0.31 ug/l
RT: 4.296 min Scan# 860
Delta R.T. 0.005 min
Lab File: VN067504.D
Acq: 25 Jun 2021 15:06


Tgt Ion: 43 Resp: 494
Ion Ratio Lower Upper
43 100
58 32.3 21.2 31.8#

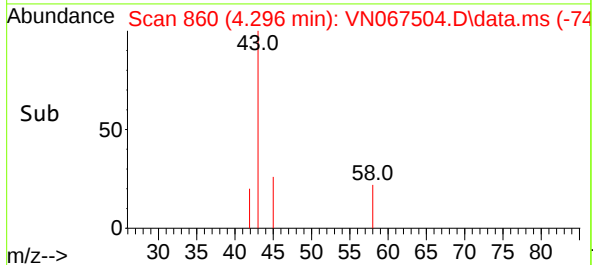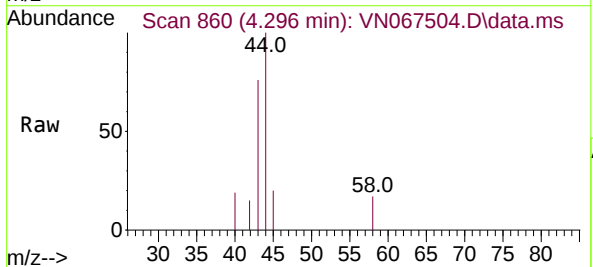






#31
Cyclohexane
Concen: 1.44 ug/l
RT: 8.086 min Scan# 2273
Delta R.T. -0.010 min
Lab File: VN067504.D
Acq: 25 Jun 2021 15:06


Instrument :
MSVOA_N
ClientSampleId :





Tgt Ion: 56 Resp: 9539
Ion Ratio Lower Upper
56 100
69 145.1 27.3 40.9#
84 133.6 64.9 97.3#




#33
1,2-Dichloroethane-d4
Concen: 55.12 ug/l
RT: 8.440 min Scan# 2405
Delta R.T. -0.000 min
Lab File: VN067504.D
Acq: 25 Jun 2021 15:06



Tgt Ion: 65 Resp: 227835
Ion Ratio Lower Upper
65 100
67 53.5 0.0 98.6



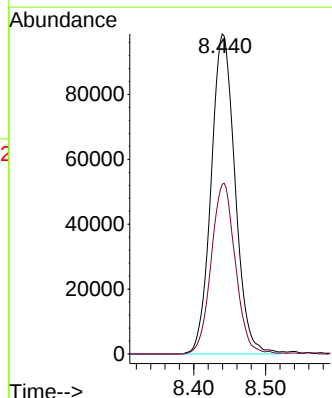





#34
1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 8.971 min Scan# 2603
Delta R.T. -0.000 min
Lab File: VN067504.D
Acq: 25 Jun 2021 15:06




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:114 Resp: 459131
Ion Ratio Lower Upper
114 100
63 27.8 0.0 49.0
88 18.7 0.0 36.6

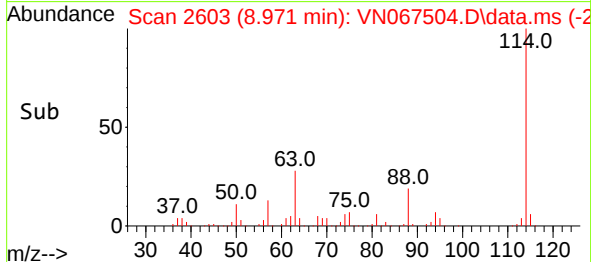

#35
Dibromofluoromethane
Concen: 49.58 ug/l
RT: 8.024 min Scan# 2250
Delta R.T. -0.000 min
Lab File: VN067504.D
Acq: 25 Jun 2021 15:06

Tgt Ion:113 Resp: 140250
Ion Ratio Lower Upper
113 100
111 103.7 83.8 125.8
192 12.4 13.4 20.0#




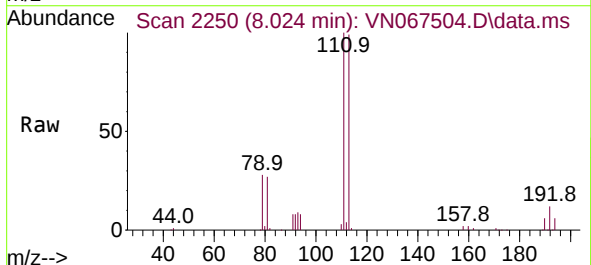




#36
1,1-Dichloropropene
Concen: 5.60 ug/l
RT: 8.088 min Scan# 2274
Delta R.T. -0.134 min
Lab File: VN067504.D
Acq: 25 Jun 2021 15:06




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 75 Resp: 28967
Ion Ratio Lower Upper
75 100
110 6.7 15.7 47.0#
77 0.0 24.6 37.0#

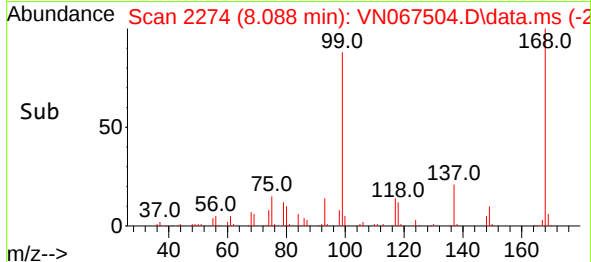

#38
Carbon Tetrachloride
Concen: 6.24 ug/l
RT: 8.088 min Scan# 2274
Delta R.T. -0.118 min
Lab File: VN067504.D
Acq: 25 Jun 2021 15:06

Tgt Ion:117 Resp: 27485
Ion Ratio Lower Upper
117 100
119 4.0 75.4 113.2#
121 0.0 23.5 35.3#




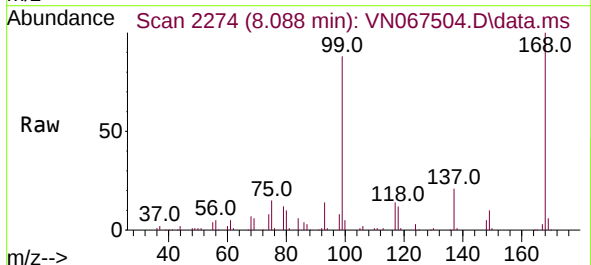




#50
Toluene-d8
Concen: 52.74 ug/l
RT: 10.443 min Scan# 3152
Delta R.T. 0.000 min
Lab File: VN067504.D
Acq: 25 Jun 2021 15:06




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 98 Resp: 636287
Ion Ratio Lower Upper
98 100
100 61.9 51.7 77.5

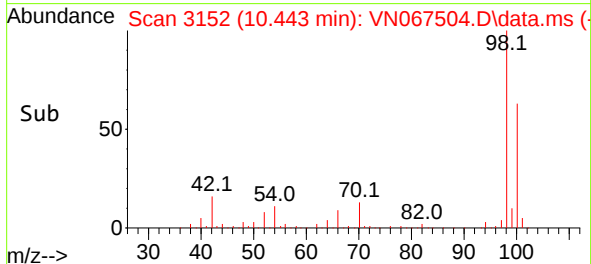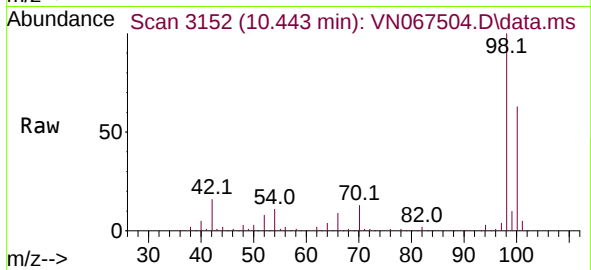

#53
t-1,3-Dichloropropene
Concen: 2.01 ug/l
RT: 10.448 min Scan# 3154
Delta R.T. -0.274 min
Lab File: VN067504.D
Acq: 25 Jun 2021 15:06


Tgt Ion: 75 Resp: 26
Ion Ratio Lower Upper
75 100
77 108.5 25.1 37.7#

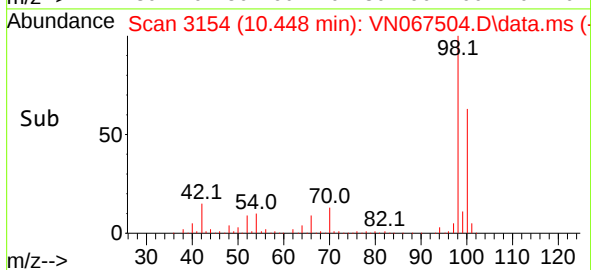






#55
1,1,2-Trichloroethane
Concen: 0.43 ug/l
RT: 10.888 min Scan# 3318
Delta R.T. -0.014 min
Lab File: VN067504.D
Acq: 25 Jun 2021 15:06

Instrument :
MSVOA_N
ClientSampled :







Tgt Ion:	97	Resp:	1459
Ion	Ratio	Lower	Upper
97	100		
83	0.0	72.0	108.0#
85	0.0	46.8	70.2#
99	0.0	49.8	74.6#

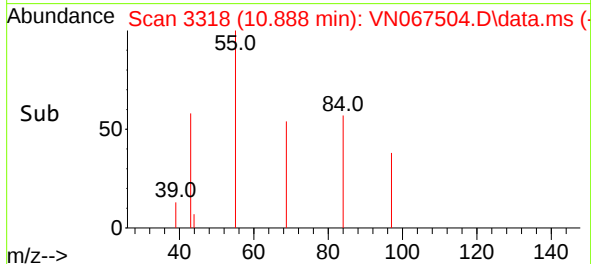

#62
4-Bromofluorobenzene
Concen: 51.40 ug/l
RT: 12.734 min Scan# 4006
Delta R.T. 0.001 min
Lab File: VN067504.D
Acq: 25 Jun 2021 15:06

Tgt Ion:	95	Resp:	220928
Ion	Ratio	Lower	Upper
95	100		
174	52.0	0.0	122.0
176	50.6	0.0	117.6


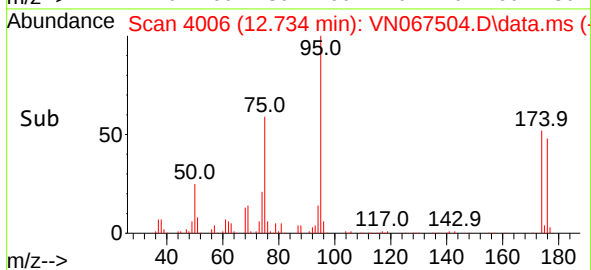

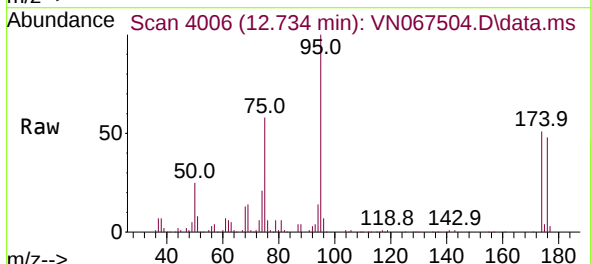




#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 11.749 min Scan# 3639
Delta R.T. 0.003 min
Lab File: VN067504.D
Acq: 25 Jun 2021 15:06




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion:117 Resp: 410048
Ion Ratio Lower Upper
117 100
82 71.9 53.1 79.7
119 32.7 25.5 38.3

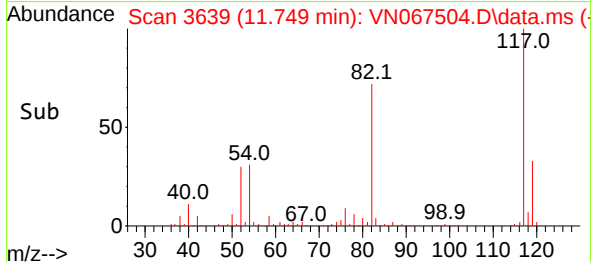

#67
Ethyl Benzene
Concen: 11.85 ug/l
RT: 11.848 min Scan# 3676
Delta R.T. 0.000 min
Lab File: VN067504.D
Acq: 25 Jun 2021 15:06

Tgt Ion: 91 Resp: 205628
Ion Ratio Lower Upper
91 100
106 29.1 23.4 35.0




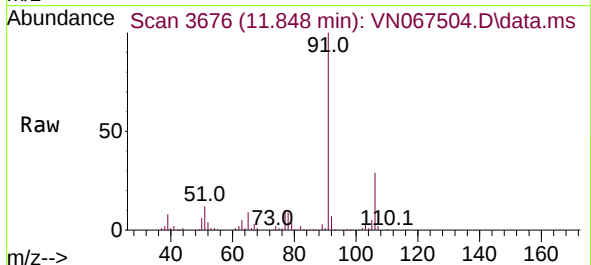




#68
m/p-Xylenes
Concen: 11.49 ug/l
RT: 11.961 min Scan# 3718
Delta R.T. 0.005 min
Lab File: VN067504.D
Acq: 25 Jun 2021 15:06




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion:106 Resp: 67495
Ion Ratio Lower Upper
106 100
91 229.4 180.6 270.8

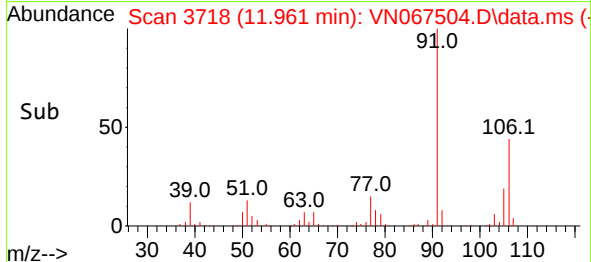

#71
Bromoform
Concen: 2.79 ug/l
RT: 12.720 min Scan# 4001
Delta R.T. 0.260 min
Lab File: VN067504.D
Acq: 25 Jun 2021 15:06

Tgt Ion:173 Resp: 309
Ion Ratio Lower Upper
173 100
175 2778.0 23.9 71.8#
254 0.0 0.0 0.0




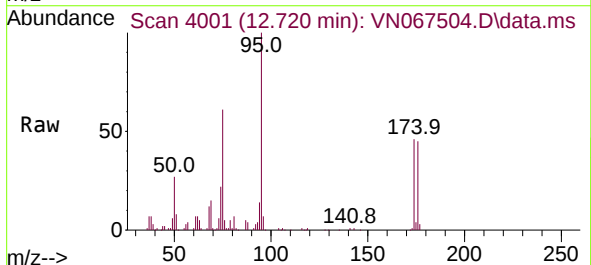


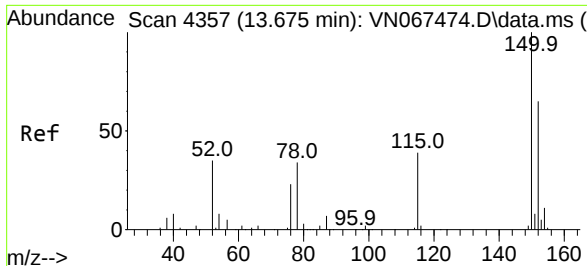

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 13.678 min Scan# 4358
Delta R.T. 0.003 min
Lab File: VN067504.D
Acq: 25 Jun 2021 15:06




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion:152 Resp: 150978
Ion Ratio Lower Upper
152 100
115 95.6 36.1 108.5
150 157.8 0.0 351.8

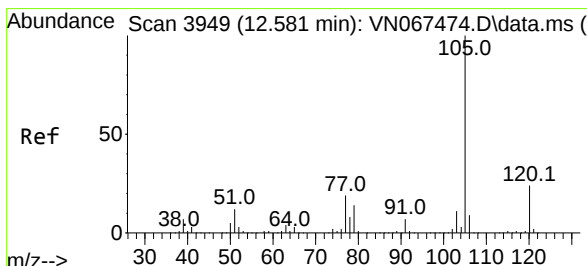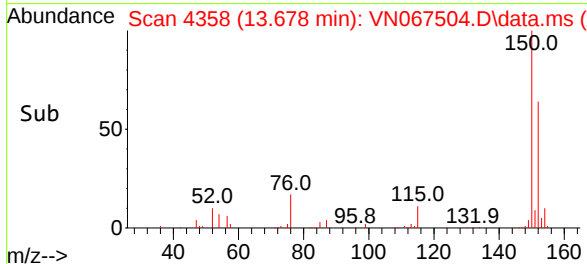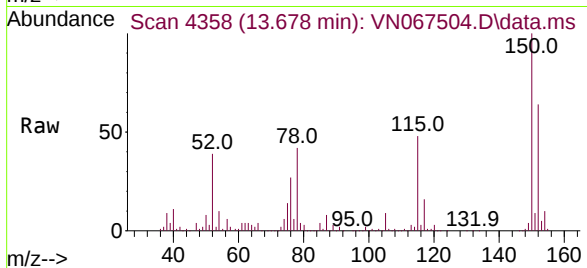

#73
Isopropylbenzene
Concen: 24.60 ug/l
RT: 12.581 min Scan# 3949
Delta R.T. -0.000 min
Lab File: VN067504.D
Acq: 25 Jun 2021 15:06

Tgt Ion:105 Resp: 378028
Ion Ratio Lower Upper
105 100
120 23.9 12.5 37.5


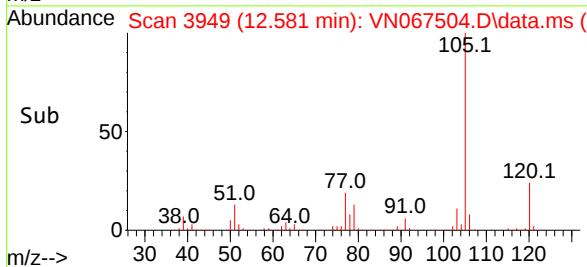

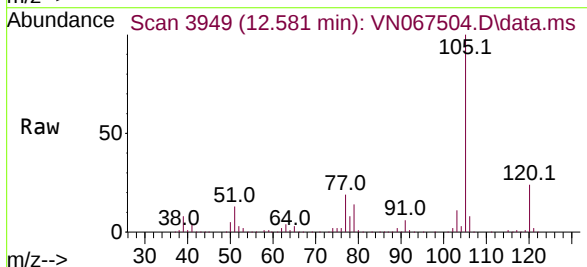




#76
1,2,3-Trichloropropane
Concen: 1.37 ug/l
RT: 12.921 min Scan# 4076
Delta R.T. 0.037 min
Lab File: VN067504.D
Acq: 25 Jun 2021 15:06




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 75 Resp: 6078
Ion Ratio Lower Upper
75 100
77 558.7 0.0 0.0#

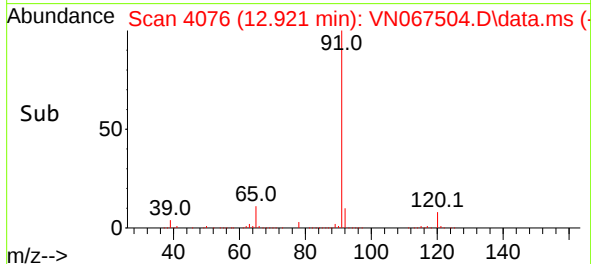

#78
n-propylbenzene
Concen: 41.48 ug/l
RT: 12.924 min Scan# 4077
Delta R.T. 0.003 min
Lab File: VN067504.D
Acq: 25 Jun 2021 15:06

Tgt Ion: 91 Resp: 786227
Ion Ratio Lower Upper
91 100
120 18.9 10.4 31.4




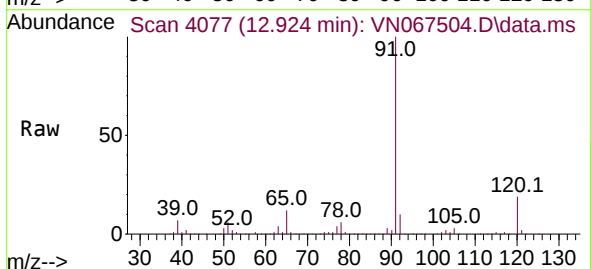




#79
2-Chlorotoluene
Concen: 69.09 ug/l
RT: 12.924 min Scan# 4077
Delta R.T. -0.086 min
Lab File: VN067504.D
Acq: 25 Jun 2021 15:06




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 91 Resp: 786227
Ion Ratio Lower Upper
91 100
126 0.0 14.5 43.5#

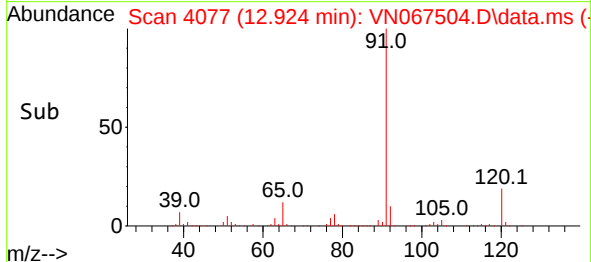

#80
1,3,5-Trimethylbenzene
Concen: 8.49 ug/l
RT: 13.061 min Scan# 4128
Delta R.T. -0.000 min
Lab File: VN067504.D
Acq: 25 Jun 2021 15:06

Tgt Ion: 105 Resp: 106509
Ion Ratio Lower Upper
105 100
120 41.5 22.2 66.6









#81
trans-1,4-Dichloro-2-butene
Concen: 3.49 ug/l
RT: 12.581 min Scan# 3949
Delta R.T. -0.048 min
Lab File: VN067504.D
Acq: 25 Jun 2021 15:06




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 75 Resp: 5660
Ion Ratio Lower Upper
75 100
53 105.2 87.6 131.4
89 97.5 37.8 56.8#

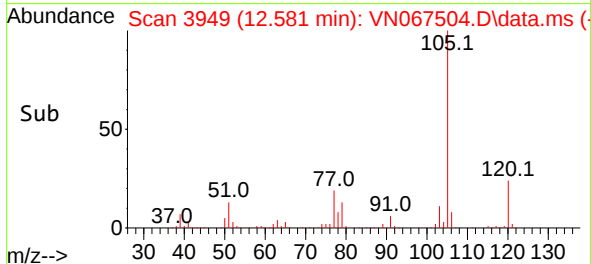

#82
4-Chlorotoluene
Concen: 70.37 ug/l
RT: 12.924 min Scan# 4077
Delta R.T. -0.182 min
Lab File: VN067504.D
Acq: 25 Jun 2021 15:06

Tgt Ion: 91 Resp: 786227
Ion Ratio Lower Upper
91 100
126 0.0 14.8 44.4#


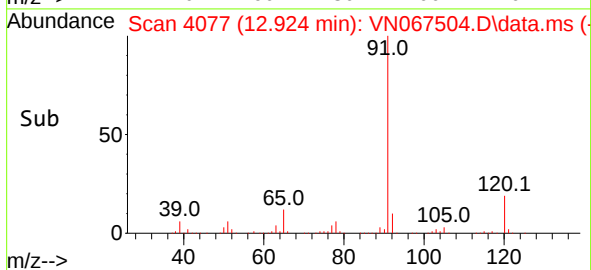

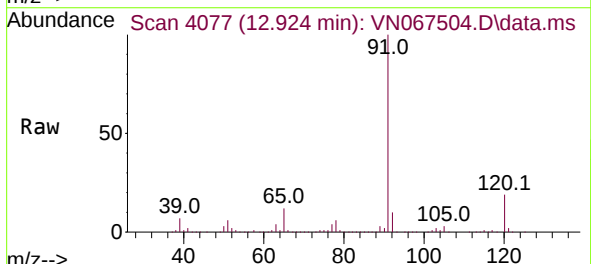




#83
tert-Butylbenzene
Concen: 2.80 ug/l
RT: 13.326 min Scan# 4227
Delta R.T. 0.000 min
Lab File: VN067504.D
Acq: 25 Jun 2021 15:06




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion:119 Resp: 27731
Ion Ratio Lower Upper
119 100
91 81.4 39.5 118.5
134 23.5 12.0 36.0

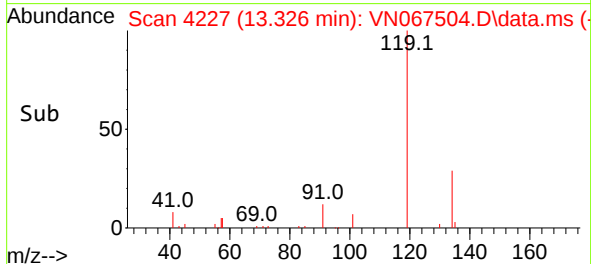

#84
1,2,4-Trimethylbenzene
Concen: 187.03 ug/l
RT: 13.369 min Scan# 4243
Delta R.T. 0.000 min
Lab File: VN067504.D
Acq: 25 Jun 2021 15:06

Tgt Ion:105 Resp: 2303025
Ion Ratio Lower Upper
105 100
120 40.1 20.6 61.8




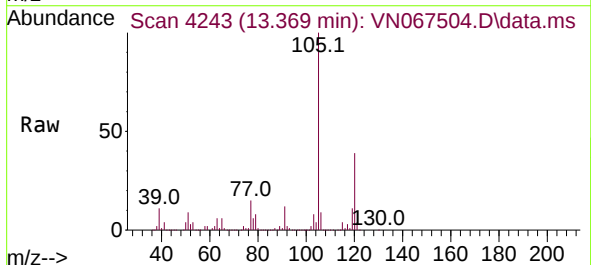




#85
 sec-Butylbenzene
 Concen: 9.77 ug/l
 RT: 13.503 min Scan# 4293
 Delta R.T. 0.000 min
 Lab File: VN067504.D
 Acq: 25 Jun 2021 15:06




Instrument :
 MSVOA_N
 ClientSampled :


Tgt Ion:105 Resp: 144914
 Ion Ratio Lower Upper
 105 100
 134 25.6 9.0 27.1

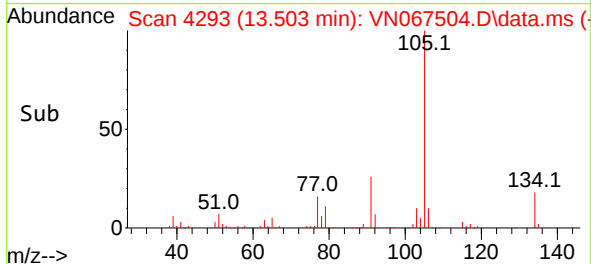

#86
 p-Isopropyltoluene
 Concen: 2.59 ug/l
 RT: 13.619 min Scan# 4336
 Delta R.T. 0.001 min
 Lab File: VN067504.D
 Acq: 25 Jun 2021 15:06

Tgt Ion:119 Resp: 28609
 Ion Ratio Lower Upper
 119 100
 134 23.5 12.4 37.4
 91 29.1 14.8 44.3


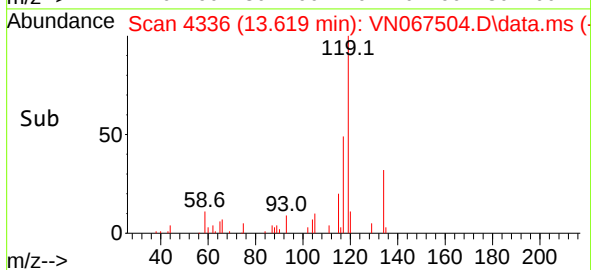




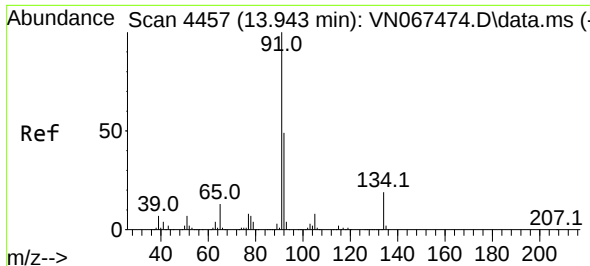

#89
n-Butylbenzene
Concen: 6.01 ug/l
RT: 13.943 min Scan# 4457
Delta R.T. 0.000 min
Lab File: VN067504.D
Acq: 25 Jun 2021 15:06




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 91 Resp: 66426
Ion Ratio Lower Upper
91 100
92 47.7 25.7 77.1
134 0.0 11.2 33.6#

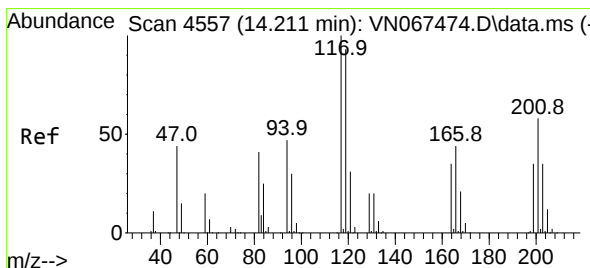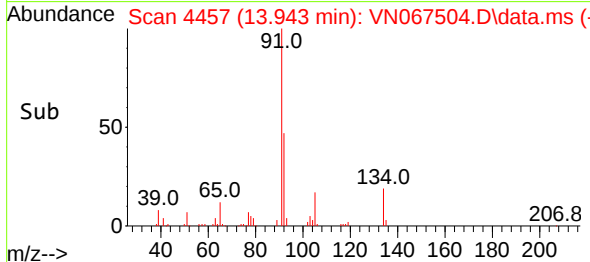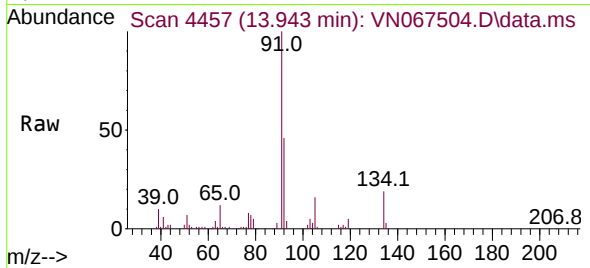

#90
Hexachloroethane
Concen: 9.16 ug/l
RT: 14.219 min Scan# 4560
Delta R.T. 0.008 min
Lab File: VN067504.D
Acq: 25 Jun 2021 15:06


Tgt Ion: 117 Resp: 19258
Ion Ratio Lower Upper
117 100
201 0.0 33.5 100.5#

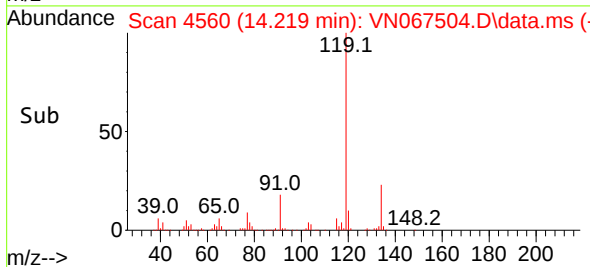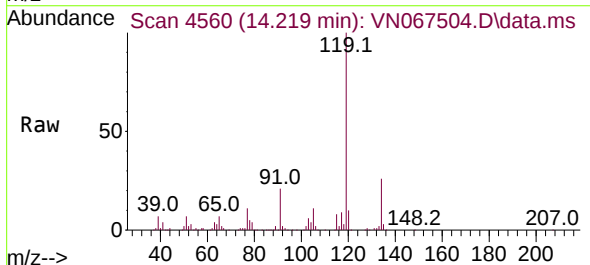






#92
 1,2-Dibromo-3-Chloropropane
 Concen: 1.69 ug/l
 RT: 14.581 min Scan# 4695
 Delta R.T. -0.022 min
 Lab File: VN067504.D
 Acq: 25 Jun 2021 15:06

Instrument :
 MSVOA_N
 ClientSampled :







Tgt Ion: 75 Resp: 1499
 Ion Ratio Lower Upper
 75 100
 155 0.0 29.8 89.5#
 157 0.0 37.6 112.8#

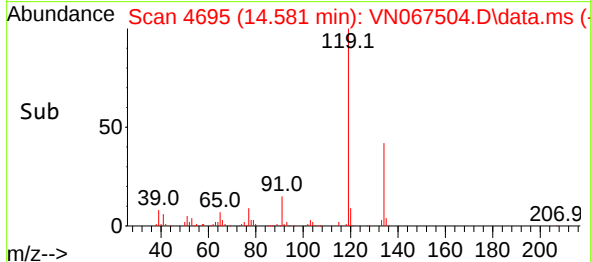

#93
 1,2,4-Trichlorobenzene
 Concen: 2.61 ug/l
 RT: 15.268 min Scan# 4951
 Delta R.T. 0.003 min
 Lab File: VN067504.D
 Acq: 25 Jun 2021 15:06

Tgt Ion: 180 Resp: 747
 Ion Ratio Lower Upper
 180 100
 182 71.4 47.5 142.5
 145 40.8 17.2 51.6




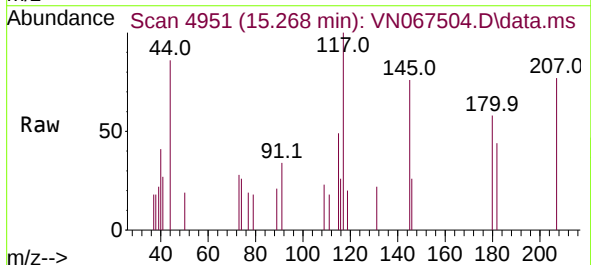


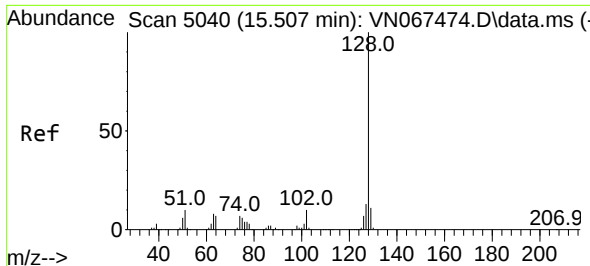

#95
Naphthalene
Concen: 9.32 ug/l
RT: 15.507 min Scan# 5040
Delta R.T. -0.000 min
Lab File: VN067504.D
Acq: 25 Jun 2021 15:06

Instrument :
MSVOA_N
ClientSampleId :

Tgt Ion:	128	Resp:	53976
Ion Ratio	Lower	Upper	
128	100		
127	13.2	10.6	15.8
129	11.3	8.6	12.8

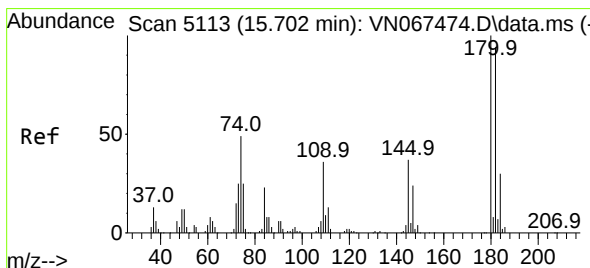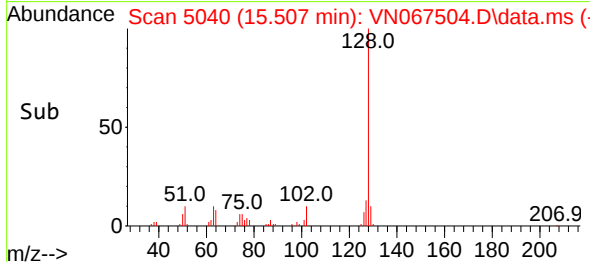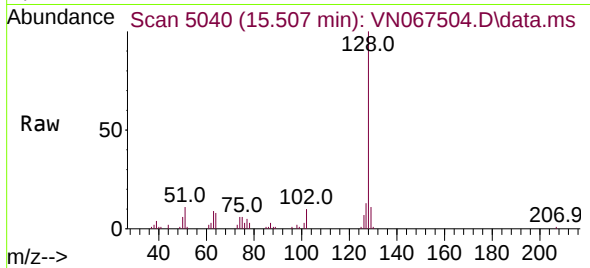

#96
1,2,3-Trichlorobenzene
Concen: 2.75 ug/l
RT: 15.708 min Scan# 5115
Delta R.T. 0.006 min
Lab File: VN067504.D
Acq: 25 Jun 2021 15:06

Tgt Ion:	180	Resp:	578
Ion Ratio	Lower	Upper	
180	100		
182	40.0	47.8	143.3#
145	0.0	18.2	54.6#

