

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN062521\
 Data File : VN067505.D
 Acq On : 25 Jun 2021 15:31
 Operator : JC/MD
 Sample : M2806-03 10X
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :

Quant Time: Jun 26 00:38:40 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N062421W.M
 Quant Title : SW846 8260
 QLast Update : Thu Jun 24 12:18:45 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.086	168	187446	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.971	114	421763	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.746	117	379314	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.675	152	124504	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.440	65	209774	54.68	ug/l	0.00
Spiked Amount 50.000	Range 61 - 141		Recovery = 109.36%			
35) Dibromofluoromethane	8.027	113	130086	50.06	ug/l	0.00
Spiked Amount 50.000	Range 69 - 133		Recovery = 100.12%			
50) Toluene-d8	10.443	98	588504	53.10	ug/l	0.00
Spiked Amount 50.000	Range 65 - 126		Recovery = 106.20%			
62) 4-Bromofluorobenzene	12.733	95	195900	49.61	ug/l	0.00
Spiked Amount 50.000	Range 58 - 135		Recovery = 99.22%			
Target Compounds						Qvalue
3) Chloromethane	2.303	50	721	0.20	ug/l #	65
11) Tert butyl alcohol	5.387	59	305	0.49	ug/l #	71
13) Acrolein	4.055	56	153	0.29	ug/l #	27
16) Acetone	4.293	43	336	0.23	ug/l #	48
31) Cyclohexane	8.086	56	9133	1.49	ug/l #	27
36) 1,1-Dichloropropene	8.086	75	27097	5.70	ug/l #	51
38) Carbon Tetrachloride	8.088	117	25273	6.25	ug/l #	15
39) Methylcyclohexane	9.461	83	2557	0.47	ug/l	93
48) Methyl methacrylate	9.461	41	1739	0.46	ug/l #	64
53) t-1,3-Dichloropropene	10.467	75	27	2.01	ug/l #	1
55) 1,1,2-Trichloroethane	10.877	97	1553	0.50	ug/l #	14
59) 2-Hexanone	11.089	43	784	0.22	ug/l	74
67) Ethyl Benzene	11.846	91	49618	3.09	ug/l	98
68) m/p-Xylenes	11.956	106	56355	10.37	ug/l	97
69) o-Xylene	12.283	106	5229	0.97	ug/l	91
71) Bromoform	12.725	173	451	2.87	ug/l #	29
73) Isopropylbenzene	12.581	105	127990	10.10	ug/l	100
76) 1,2,3-Trichloropropane	12.733	75	120893	32.99	ug/l #	100
78) n-propylbenzene	12.924	91	240151	15.37	ug/l	95
79) 2-Chlorotoluene	12.924	91	240151	25.59	ug/l #	46
80) 1,3,5-Trimethylbenzene	13.063	105	45651	4.41	ug/l	99
81) trans-1,4-Dichloro-2-b...	12.733	75	120893	90.27	ug/l #	6
82) 4-Chlorotoluene	12.924	91	240151	26.07	ug/l #	45
83) tert-Butylbenzene	13.326	119	14551	1.78	ug/l	96
84) 1,2,4-Trimethylbenzene	13.372	105	834006	82.13	ug/l	98
85) sec-Butylbenzene	13.503	105	84115	6.88	ug/l	86
86) p-Isopropyltoluene	13.562	119	20519	2.25	ug/l	97
89) n-Butylbenzene	13.943	91	37395	4.10	ug/l #	81
90) Hexachloroethane	14.222	117	9685	5.58	ug/l #	16
92) 1,2-Dibromo-3-Chloropr...	14.581	75	429	0.59	ug/l #	16
93) 1,2,4-Trichlorobenzene	15.262	180	235	2.44	ug/l #	58
95) Naphthalene	15.509	128	11611	4.90	ug/l	99
96) 1,2,3-Trichlorobenzene	15.708	180	540	2.78	ug/l #	17


(#) = qualifier out of range (m) = manual integration (+) = signals summed


Instrument :
MSVOA_N
ClientSampleId :

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN062521\
Data File : VN067505.D
Acq On : 25 Jun 2021 15:31
Operator : JC/MD
Sample : M2806-03 10X
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampled :

Quant Time: Jun 26 00:38:40 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N062421W.M
Quant Title : SW846 8260
QLast Update : Thu Jun 24 12:18:45 2021
Response via : Initial Calibration




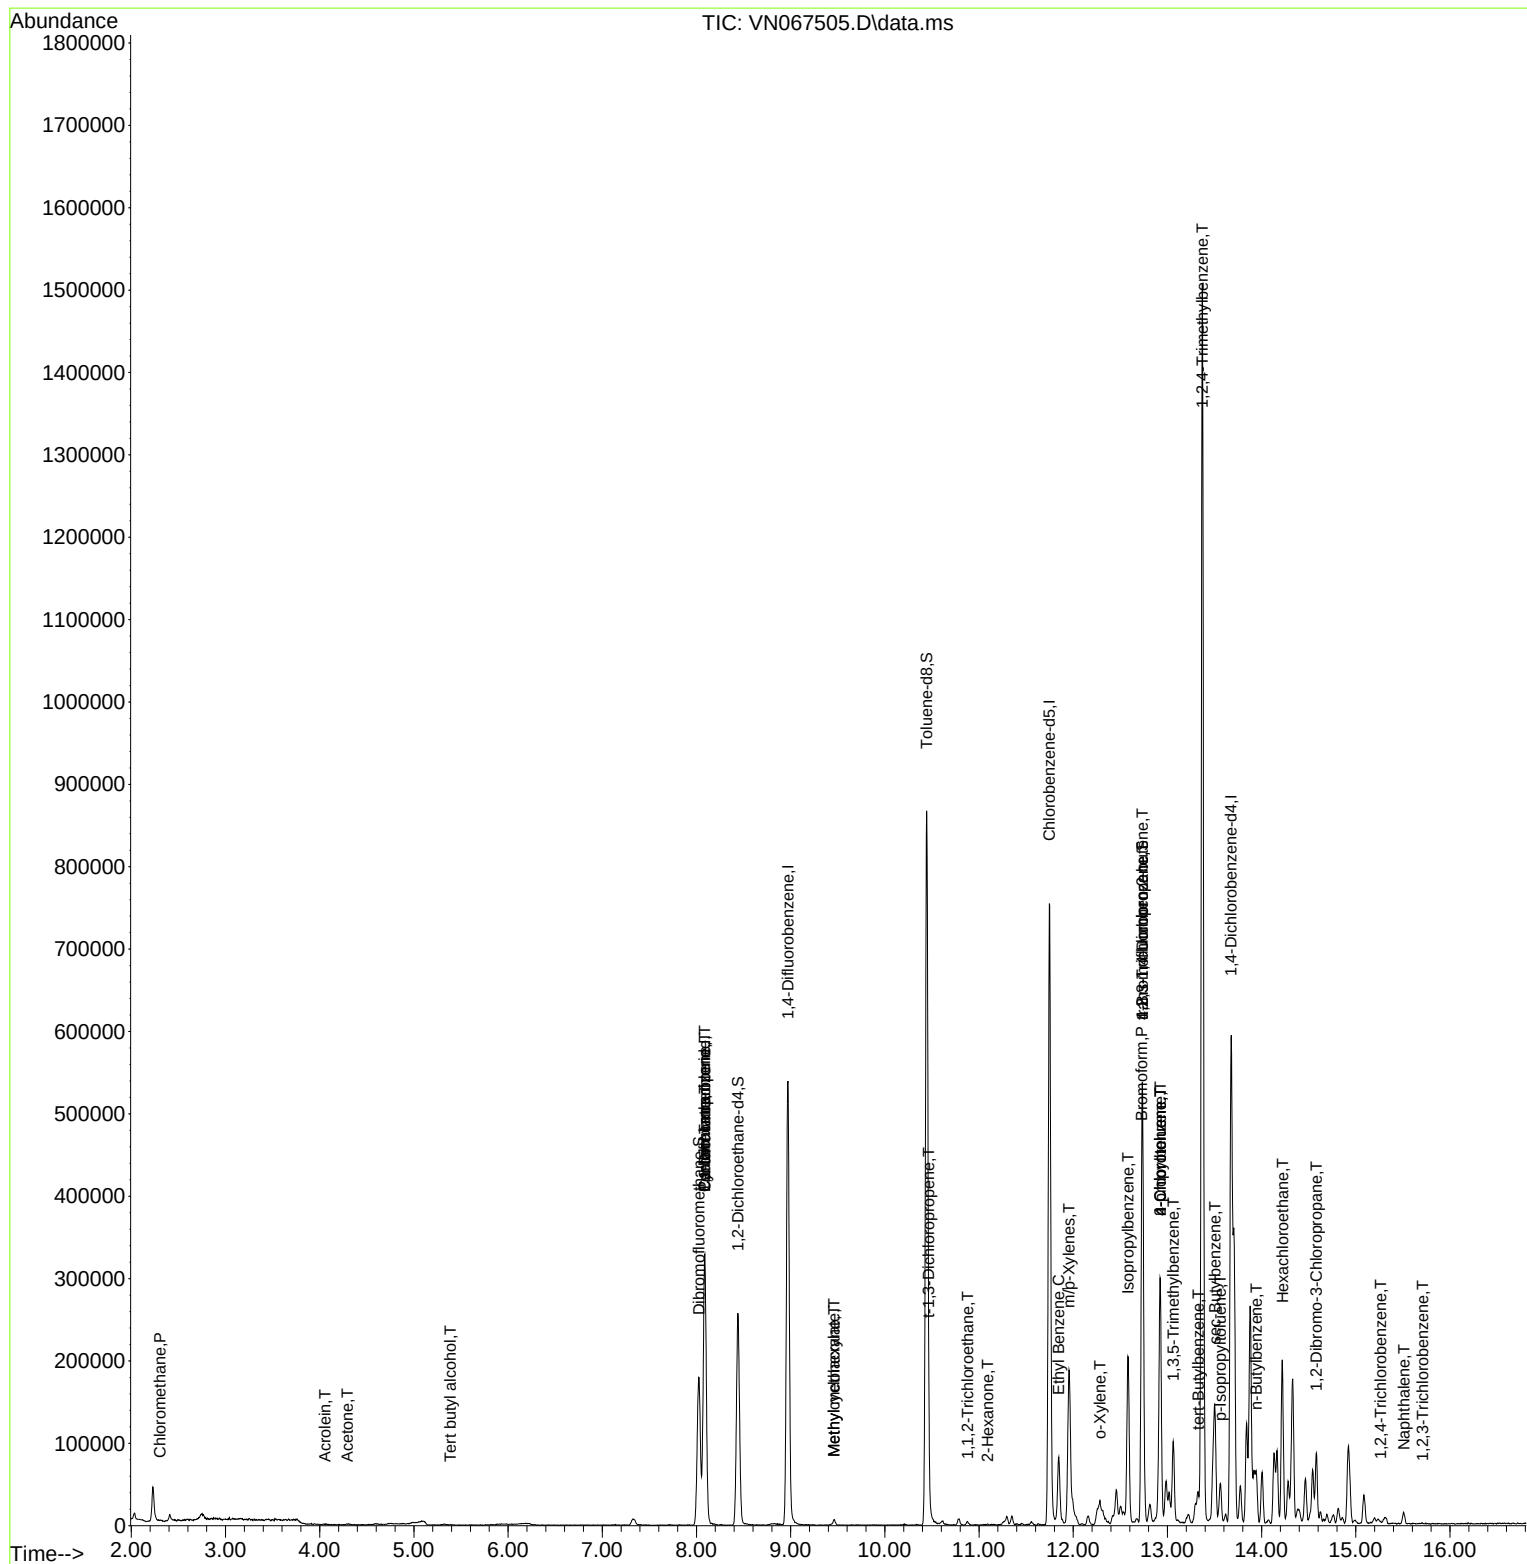


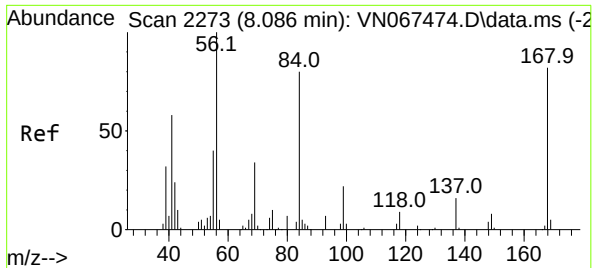

#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 8.086 min Scan# 2273
Delta R.T. -0.000 min
Lab File: VN067505.D
Acq: 25 Jun 2021 15:31




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion:168 Resp: 187446
Ion Ratio Lower Upper
168 100
99 86.1 62.9 94.3

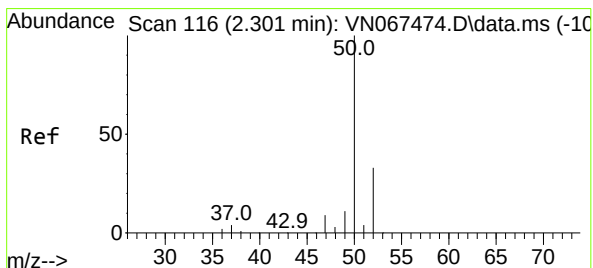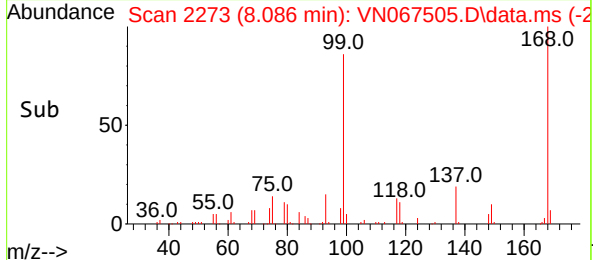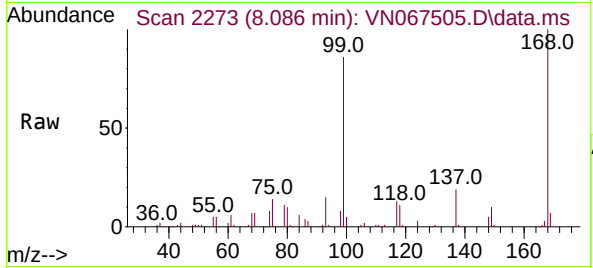

#3
Chloromethane
Concen: 0.20 ug/l
RT: 2.303 min Scan# 117
Delta R.T. 0.002 min
Lab File: VN067505.D
Acq: 25 Jun 2021 15:31

Tgt Ion: 50 Resp: 721
Ion Ratio Lower Upper
50 100
52 51.4 25.6 38.4#

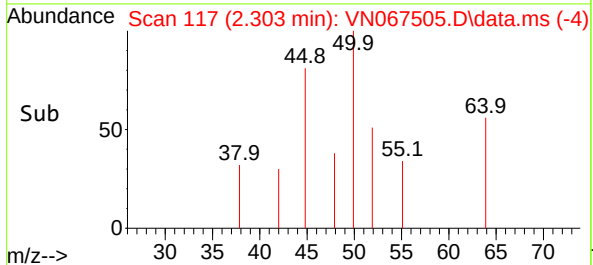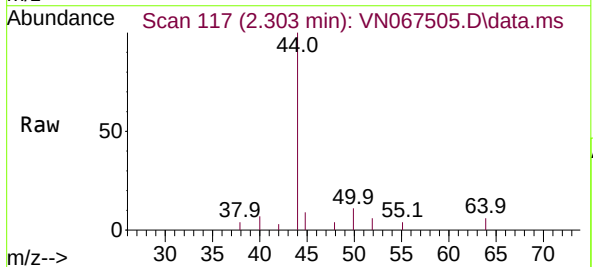




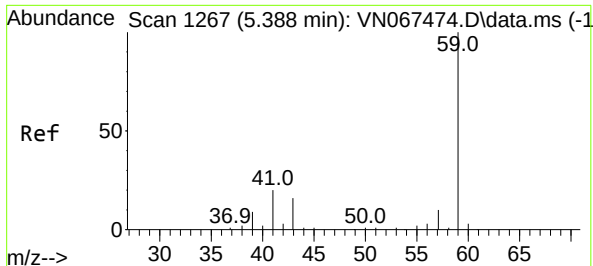


#11

Tert butyl alcohol
Concen: 0.49 ug/l
RT: 5.387 min Scan# 1267
Delta R.T. -0.001 min
Lab File: VN067505.D
Acq: 25 Jun 2021 15:31

Instrument :
MSVOA_N
ClientSampled :




Tgt Ion: 59 Resp: 305
Ion Ratio Lower Upper
59 100
57 0.0 8.7 13.1#

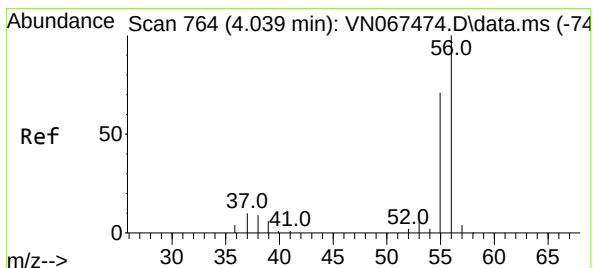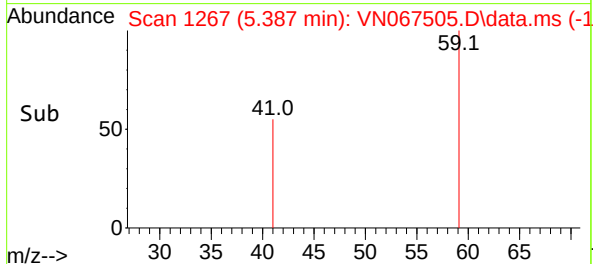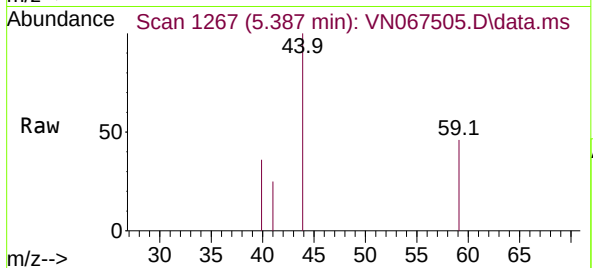


#13

Acrolein
Concen: 0.29 ug/l
RT: 4.055 min Scan# 770
Delta R.T. 0.016 min
Lab File: VN067505.D
Acq: 25 Jun 2021 15:31

Tgt Ion: 56 Resp: 153
Ion Ratio Lower Upper
56 100
55 132.7 57.4 86.0#


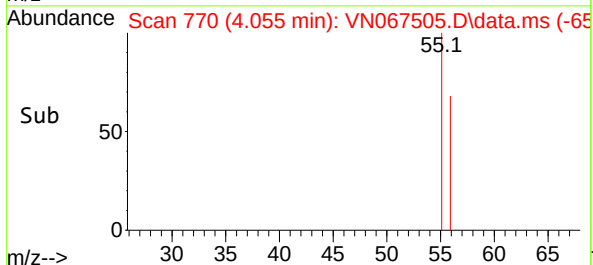

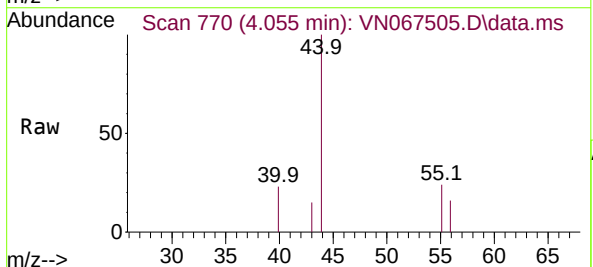




#16
Acetone
Concen: 0.23 ug/l
RT: 4.293 min Scan# 859
Delta R.T. 0.002 min
Lab File: VN067505.D
Acq: 25 Jun 2021 15:31




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 43 Resp: 336
Ion Ratio Lower Upper
43 100
58 0.0 21.2 31.8#

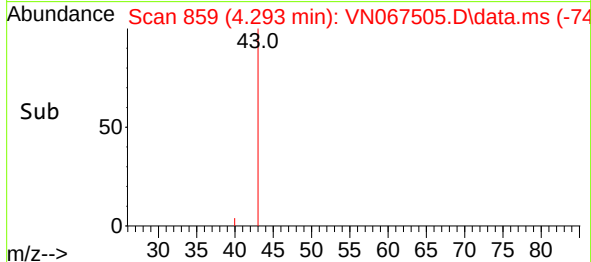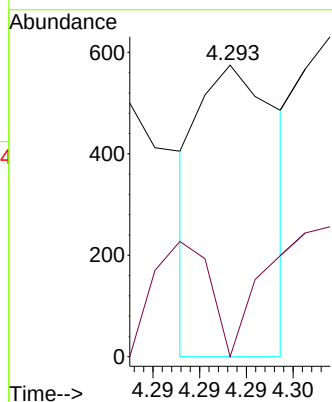

#31
Cyclohexane
Concen: 1.49 ug/l
RT: 8.086 min Scan# 2273
Delta R.T. -0.010 min
Lab File: VN067505.D
Acq: 25 Jun 2021 15:31

Tgt Ion: 56 Resp: 9133
Ion Ratio Lower Upper
56 100
69 130.4 27.3 40.9#
84 110.6 64.9 97.3#

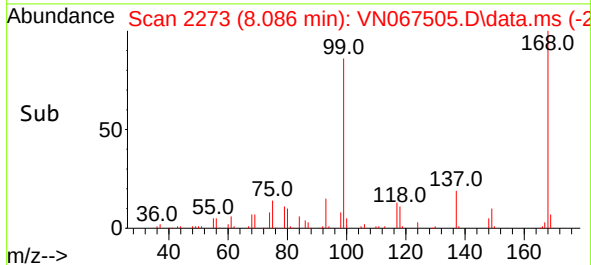



#33

1,2-Dichloroethane-d4

Concen: 54.68 ug/l

RT: 8.440 min Scan# 2405

Delta R.T. -0.000 min

Lab File: VN067505.D

Acq: 25 Jun 2021 15:31

Tgt Ion: 65 Resp: 209774

Ion Ratio Lower Upper





65 100

67 52.4 0.0 98.6

Instrument :

MSVOA_N

ClientSampleId :

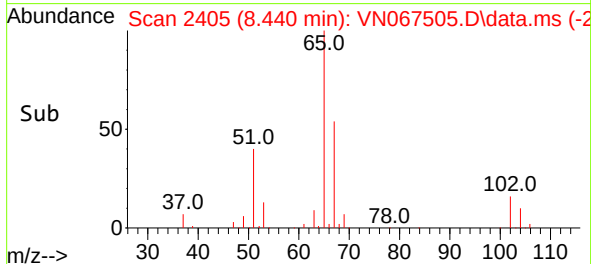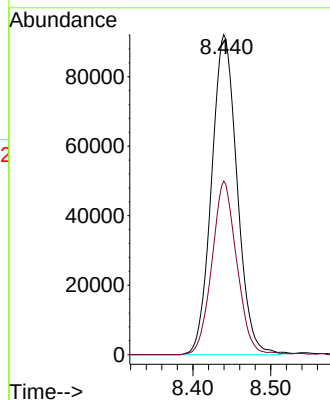

#34

1,4-Difluorobenzene

Concen: 50.00 ug/l

RT: 8.971 min Scan# 2603

Delta R.T. -0.000 min

Lab File: VN067505.D

Acq: 25 Jun 2021 15:31




Tgt Ion: 114 Resp: 421763


Ion Ratio Lower Upper

114 100

63 28.5 0.0 49.0

88 18.9 0.0 36.6



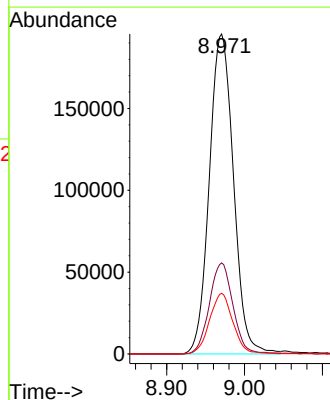





#35
Dibromofluoromethane
Concen: 50.06 ug/l
RT: 8.027 min Scan# 2251
Delta R.T. 0.003 min
Lab File: VN067505.D
Acq: 25 Jun 2021 15:31




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion:113 Resp: 130086
Ion Ratio Lower Upper
113 100
111 105.0 83.8 125.8
192 12.6 13.4 20.0#

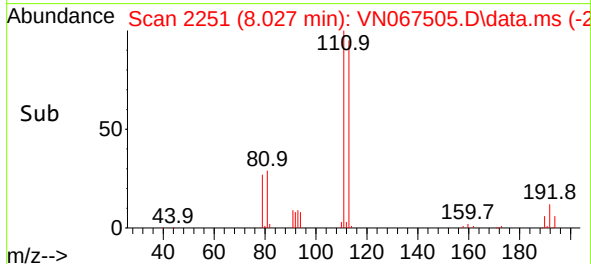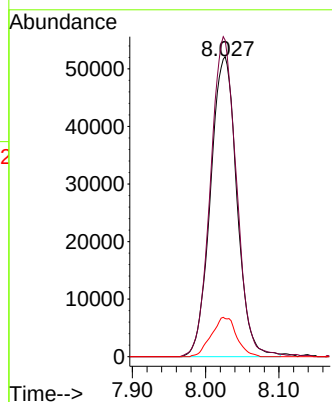

#36
1,1-Dichloropropene
Concen: 5.70 ug/l
RT: 8.086 min Scan# 2273
Delta R.T. -0.136 min
Lab File: VN067505.D
Acq: 25 Jun 2021 15:31


Tgt Ion: 75 Resp: 27097
Ion Ratio Lower Upper
75 100
110 7.7 15.7 47.0#
77 0.0 24.6 37.0#





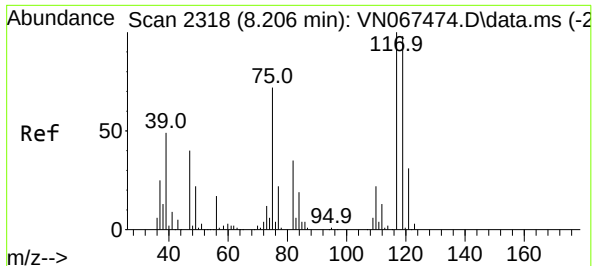


#38
Carbon Tetrachloride
Concen: 6.25 ug/l
RT: 8.088 min Scan# 2274
Delta R.T. -0.118 min
Lab File: VN067505.D
Acq: 25 Jun 2021 15:31


Instrument :
MSVOA_N
ClientSampled :

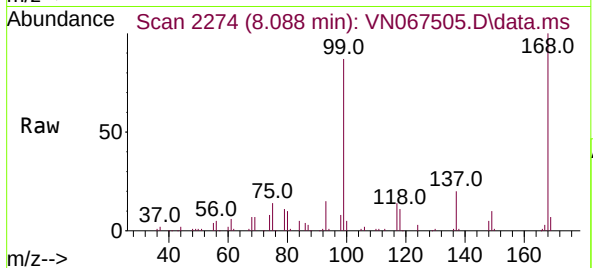



Tgt Ion:117 Resp: 25273
Ion Ratio Lower Upper
117 100
119 3.3 75.4 113.2#
121 0.0 23.5 35.3#

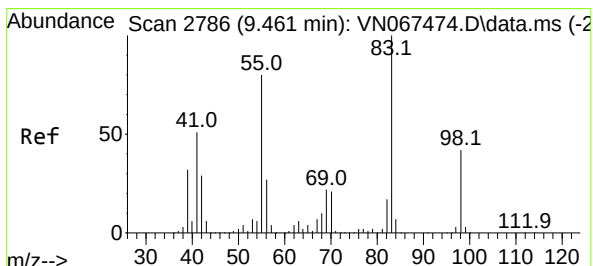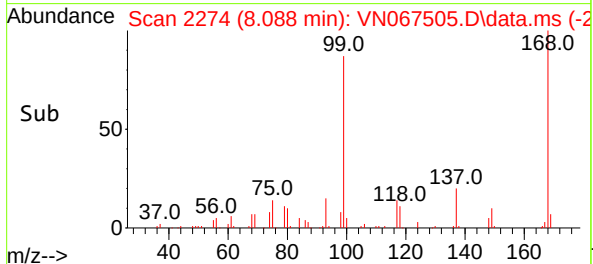


#39
Methylcyclohexane
Concen: 0.47 ug/l
RT: 9.461 min Scan# 2786
Delta R.T. 0.000 min
Lab File: VN067505.D
Acq: 25 Jun 2021 15:31

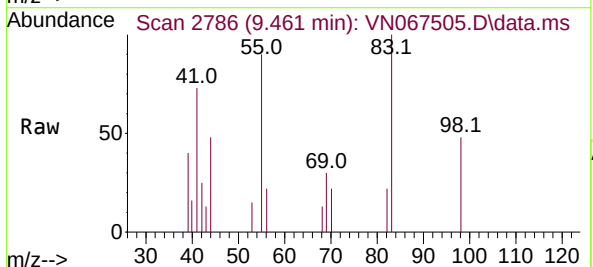

Tgt Ion: 83 Resp: 2557
Ion Ratio Lower Upper
83 100
55 90.1 66.6 99.8
98 47.9 35.3 52.9



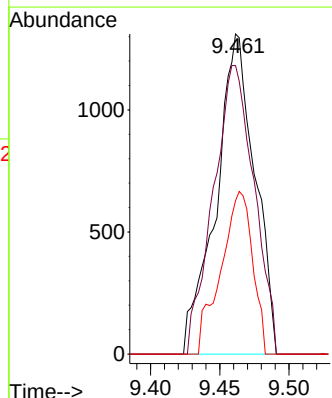
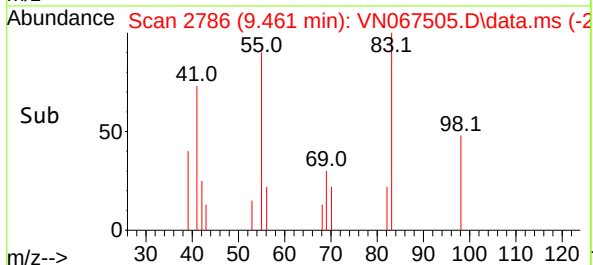


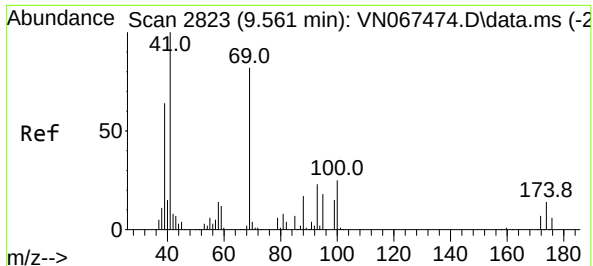

#48
Methyl methacrylate
Concen: 0.46 ug/l
RT: 9.461 min Scan# 2786
Delta R.T. -0.100 min
Lab File: VN067505.D
Acq: 25 Jun 2021 15:31




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 41 Resp: 1739
Ion Ratio Lower Upper
41 100
69 33.8 64.6 96.8#
39 53.8 53.3 79.9

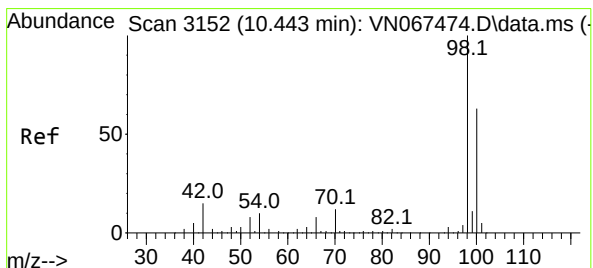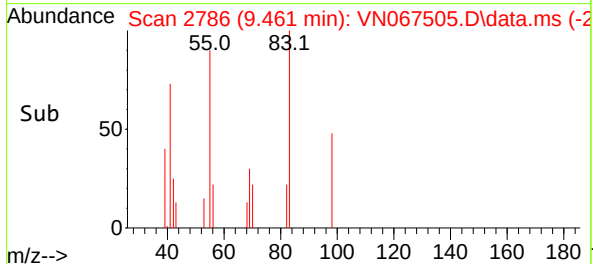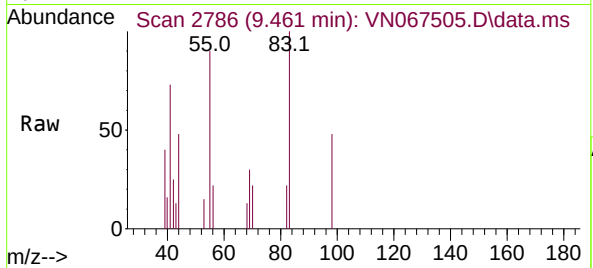

#50
Toluene-d8
Concen: 53.10 ug/l
RT: 10.443 min Scan# 3152
Delta R.T. 0.000 min
Lab File: VN067505.D
Acq: 25 Jun 2021 15:31

Tgt Ion: 98 Resp: 588504
Ion Ratio Lower Upper
98 100
100 62.1 51.7 77.5


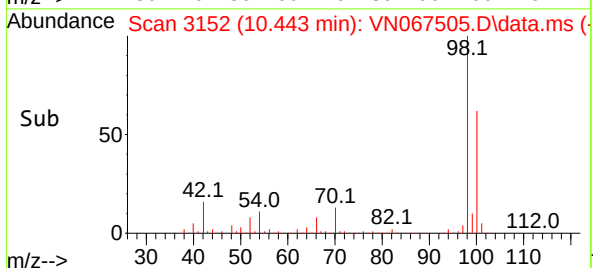

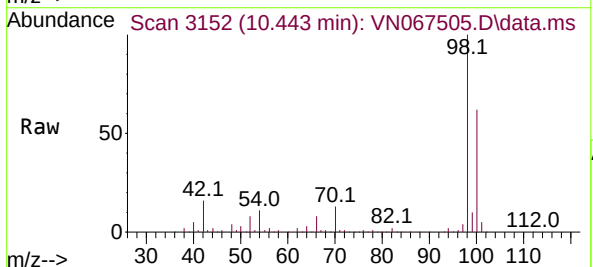




#53
t-1,3-Dichloropropene
Concen: 2.01 ug/l
RT: 10.467 min Scan# 3161
Delta R.T. -0.255 min
Lab File: VN067505.D
Acq: 25 Jun 2021 15:31




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 75 Resp: 27
Ion Ratio Lower Upper
75 100
77 89.8 25.1 37.7#

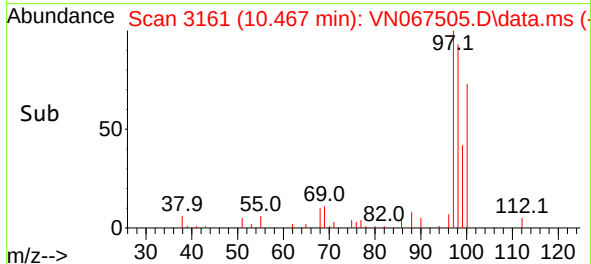

#55
1,1,2-Trichloroethane
Concen: 0.50 ug/l
RT: 10.877 min Scan# 3314
Delta R.T. -0.025 min
Lab File: VN067505.D
Acq: 25 Jun 2021 15:31

Tgt Ion: 97 Resp: 1553
Ion Ratio Lower Upper
97 100
83 0.0 72.0 108.0#
85 0.0 46.8 70.2#
99 0.0 49.8 74.6#


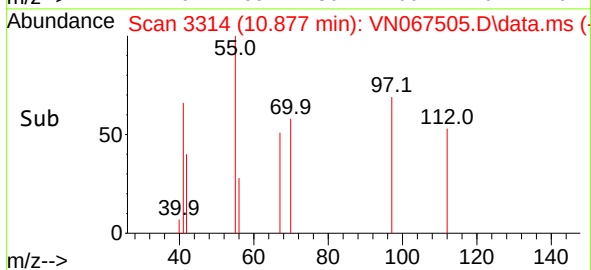






#59
2-Hexanone
Concen: 0.22 ug/l
RT: 11.089 min Scan# 3393
Delta R.T. 0.002 min
Lab File: VN067505.D
Acq: 25 Jun 2021 15:31




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 43 Resp: 784
Ion Ratio Lower Upper
43 100
58 31.9 24.7 74.1

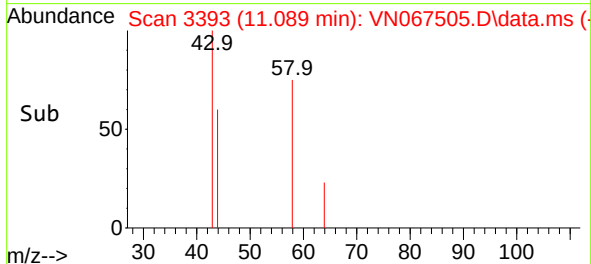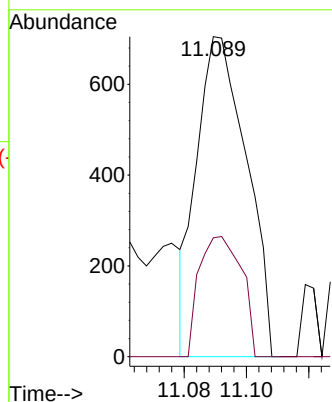

#62
4-Bromofluorobenzene
Concen: 49.61 ug/l
RT: 12.733 min Scan# 4006
Delta R.T. 0.000 min
Lab File: VN067505.D
Acq: 25 Jun 2021 15:31

Tgt Ion: 95 Resp: 195900
Ion Ratio Lower Upper
95 100
174 52.0 0.0 122.0
176 49.0 0.0 117.6


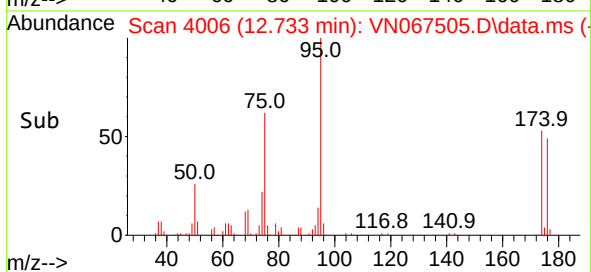
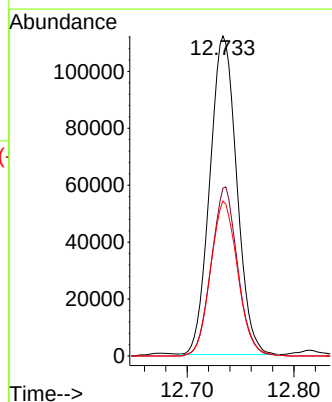
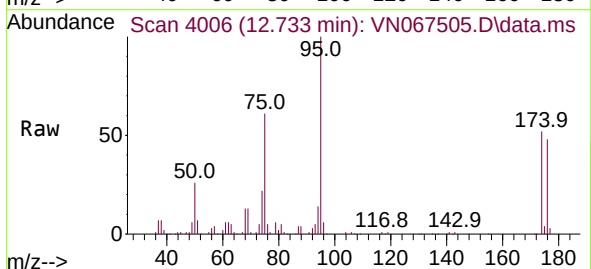




#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 11.746 min Scan# 3638
Delta R.T. 0.000 min
Lab File: VN067505.D
Acq: 25 Jun 2021 15:31




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:117 Resp: 379314
Ion Ratio Lower Upper
117 100
82 69.3 53.1 79.7
119 31.1 25.5 38.3

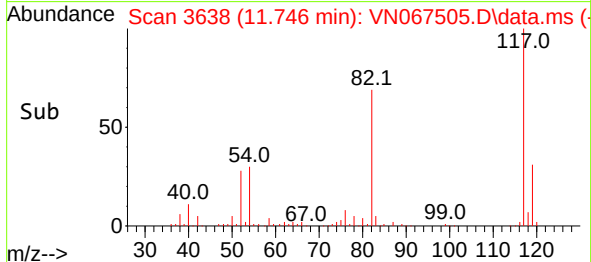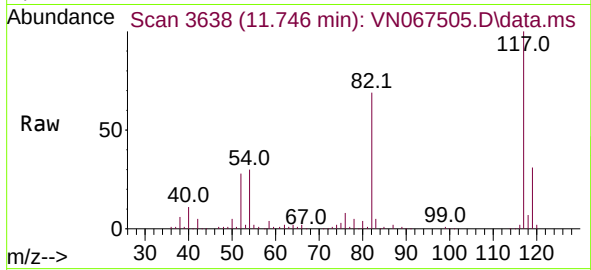

#67
Ethyl Benzene
Concen: 3.09 ug/l
RT: 11.846 min Scan# 3675
Delta R.T. -0.002 min
Lab File: VN067505.D
Acq: 25 Jun 2021 15:31

Tgt Ion: 91 Resp: 49618
Ion Ratio Lower Upper
91 100
106 28.2 23.4 35.0




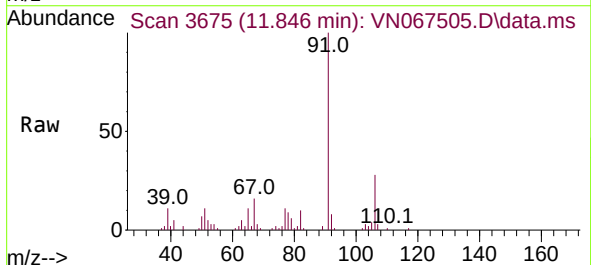




#68
m/p-Xylenes
Concen: 10.37 ug/l
RT: 11.956 min Scan# 3716
Delta R.T. -0.000 min
Lab File: VN067505.D
Acq: 25 Jun 2021 15:31




Tgt Ion:106 Resp: 56355
Ion Ratio Lower Upper
106 100
91 221.0 180.6 270.8


Instrument :
MSVOA_N
ClientSampled :

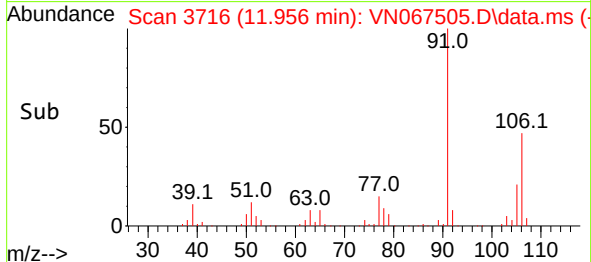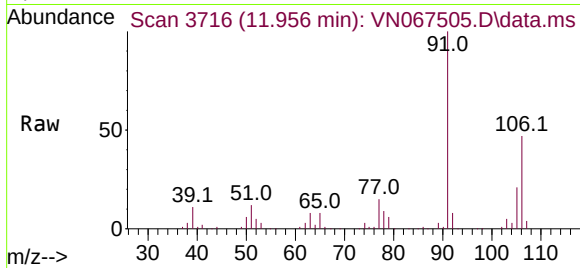

#69
o-Xylene
Concen: 0.97 ug/l
RT: 12.283 min Scan# 3838
Delta R.T. -0.000 min
Lab File: VN067505.D
Acq: 25 Jun 2021 15:31

Tgt Ion:106 Resp: 5229
Ion Ratio Lower Upper
106 100
91 251.2 118.3 354.9




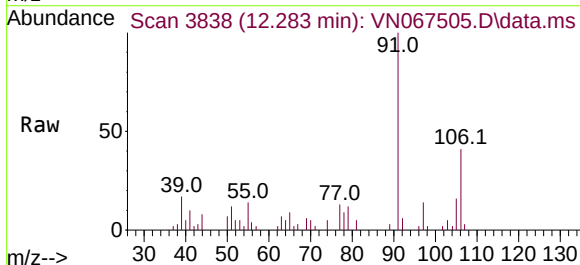


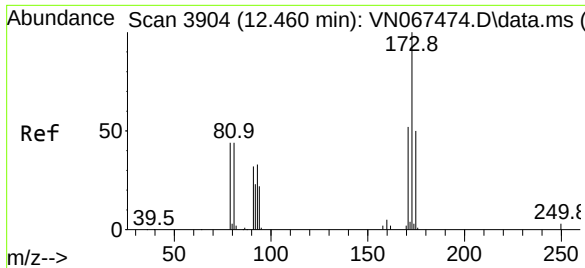

#71
Bromoform
Concen: 2.87 ug/l
RT: 12.725 min Scan# 4003
Delta R.T. 0.265 min
Lab File: VN067505.D
Acq: 25 Jun 2021 15:31




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion:173 Resp: 451
Ion Ratio Lower Upper
173 100
175 0.0 23.9 71.8#
254 0.0 0.0 0.0

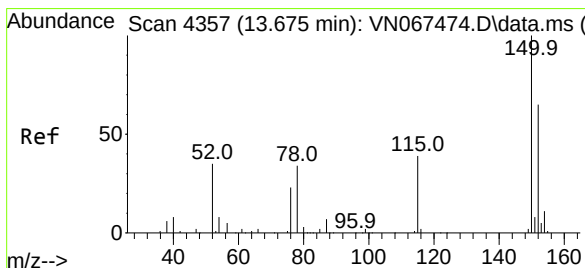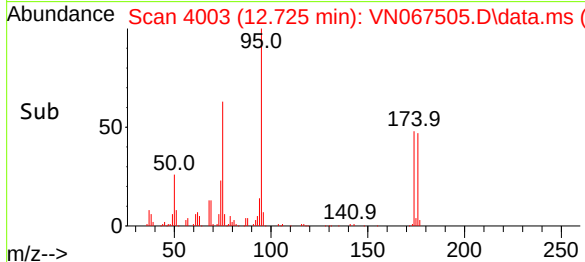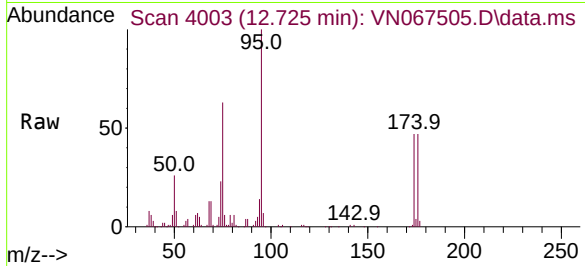

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 13.675 min Scan# 4357
Delta R.T. -0.000 min
Lab File: VN067505.D
Acq: 25 Jun 2021 15:31

Tgt Ion:152 Resp: 124504
Ion Ratio Lower Upper
152 100
115 82.5 36.1 108.5
150 160.1 0.0 351.8


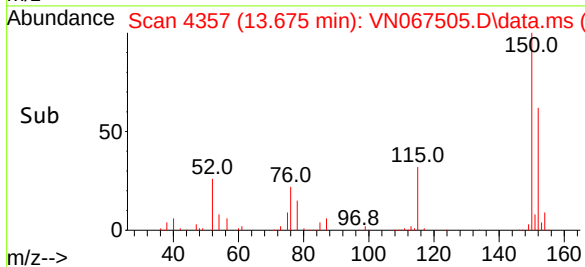

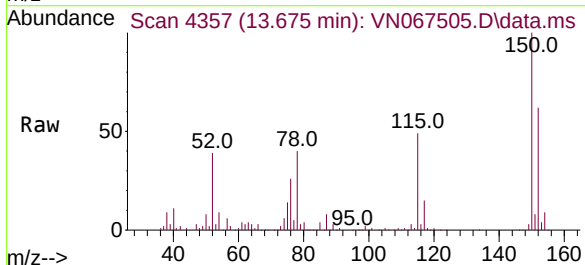




#73
Isopropylbenzene
Concen: 10.10 ug/l
RT: 12.581 min Scan# 3949
Delta R.T. -0.000 min
Lab File: VN067505.D
Acq: 25 Jun 2021 15:31




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion:105 Resp: 127990
Ion Ratio Lower Upper
105 100
120 25.0 12.5 37.5

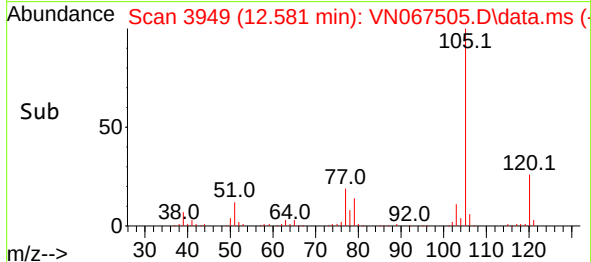

#76
1,2,3-Trichloropropane
Concen: 32.99 ug/l
RT: 12.733 min Scan# 4006
Delta R.T. -0.151 min
Lab File: VN067505.D
Acq: 25 Jun 2021 15:31

Tgt Ion: 75 Resp: 120893
Ion Ratio Lower Upper
75 100
77 1.2 0.0 0.0#


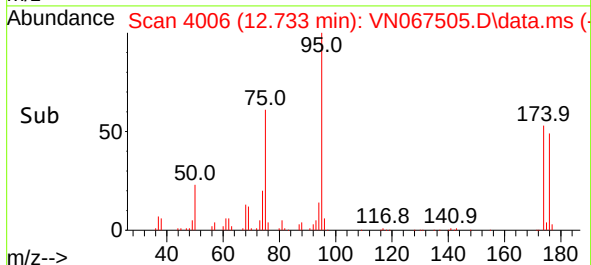






#78
n-propylbenzene
Concen: 15.37 ug/l
RT: 12.924 min Scan# 4077
Delta R.T. 0.003 min
Lab File: VN067505.D
Acq: 25 Jun 2021 15:31




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 91 Resp: 240151
Ion Ratio Lower Upper
91 100
120 18.5 10.4 31.4

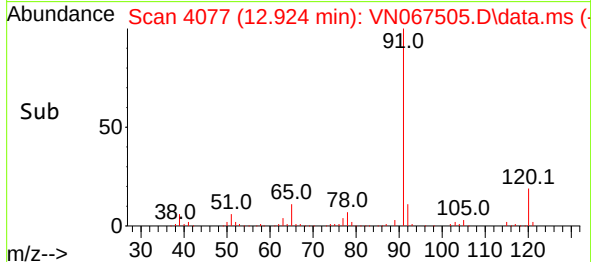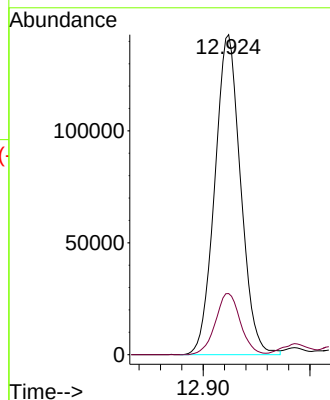

#79
2-Chlorotoluene
Concen: 25.59 ug/l
RT: 12.924 min Scan# 4077
Delta R.T. -0.086 min
Lab File: VN067505.D
Acq: 25 Jun 2021 15:31

Tgt Ion: 91 Resp: 240151
Ion Ratio Lower Upper
91 100
126 0.0 14.5 43.5#



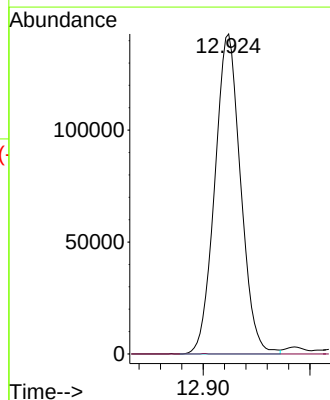
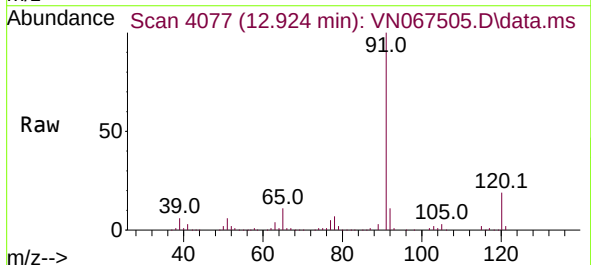


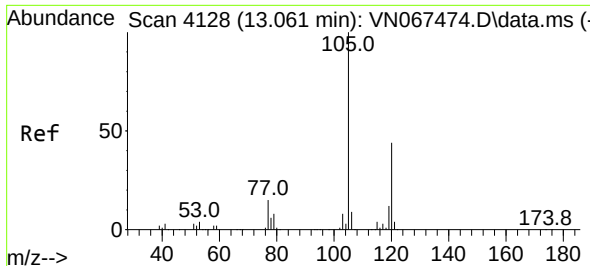

#80
1,3,5-Trimethylbenzene
Concen: 4.41 ug/l
RT: 13.063 min Scan# 4129
Delta R.T. 0.002 min
Lab File: VN067505.D
Acq: 25 Jun 2021 15:31




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion:105 Resp: 45651
Ion Ratio Lower Upper
105 100
120 44.0 22.2 66.6

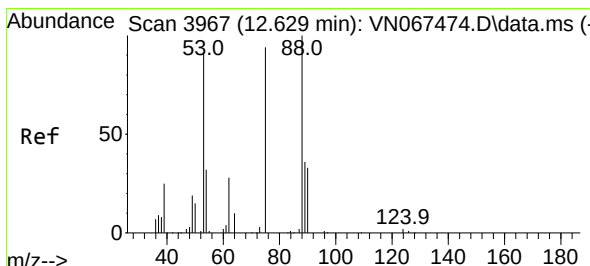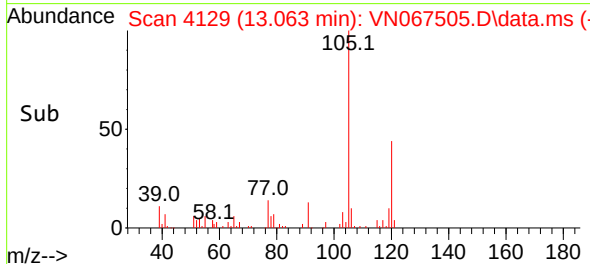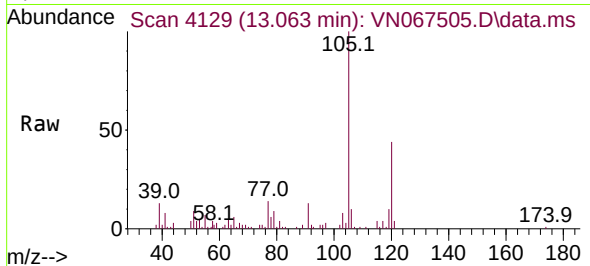

#81
trans-1,4-Dichloro-2-butene
Concen: 90.27 ug/l
RT: 12.733 min Scan# 4006
Delta R.T. 0.104 min
Lab File: VN067505.D
Acq: 25 Jun 2021 15:31

Tgt Ion: 75 Resp: 120893
Ion Ratio Lower Upper
75 100
53 0.0 87.6 131.4#
89 0.0 37.8 56.8#


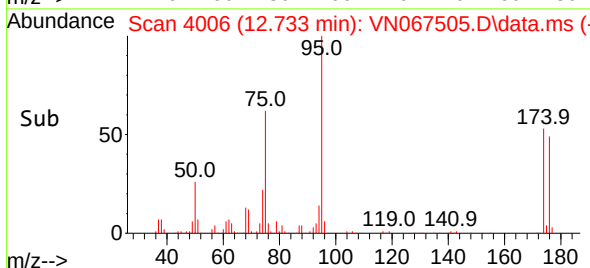
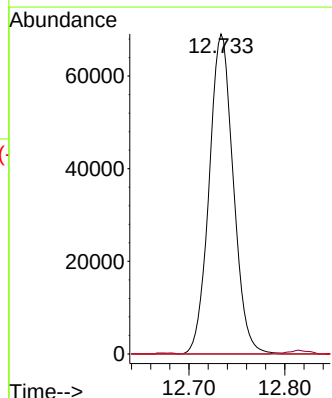
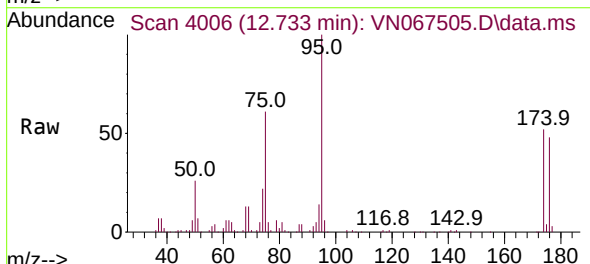




#82
4-Chlorotoluene
Concen: 26.07 ug/l
RT: 12.924 min Scan# 4077
Delta R.T. -0.182 min
Lab File: VN067505.D
Acq: 25 Jun 2021 15:31




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 91 Resp: 240151
Ion Ratio Lower Upper
91 100
126 0.0 14.8 44.4#

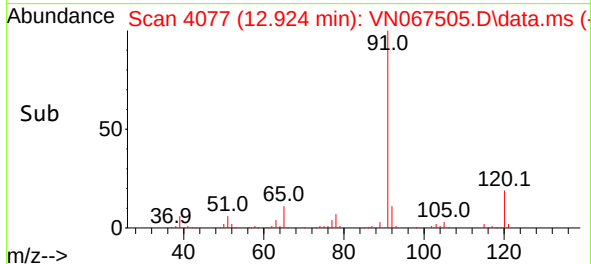

#83
tert-Butylbenzene
Concen: 1.78 ug/l
RT: 13.326 min Scan# 4227
Delta R.T. 0.000 min
Lab File: VN067505.D
Acq: 25 Jun 2021 15:31

Tgt Ion: 119 Resp: 14551
Ion Ratio Lower Upper
119 100
91 83.0 39.5 118.5
134 23.4 12.0 36.0









#84
1,2,4-Trimethylbenzene
Concen: 82.13 ug/l
RT: 13.372 min Scan# 4244
Delta R.T. 0.003 min
Lab File: VN067505.D
Acq: 25 Jun 2021 15:31




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:105 Resp: 834006
Ion Ratio Lower Upper
105 100
120 39.9 20.6 61.8

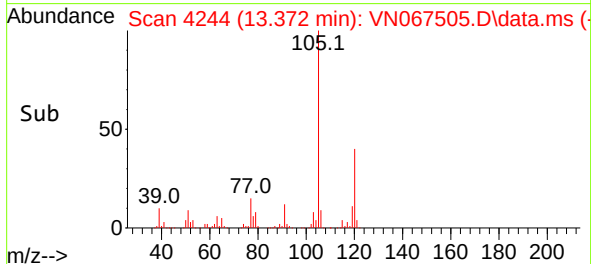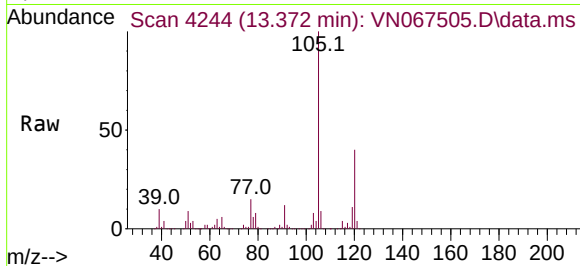

#85
sec-Butylbenzene
Concen: 6.88 ug/l
RT: 13.503 min Scan# 4293
Delta R.T. 0.000 min
Lab File: VN067505.D
Acq: 25 Jun 2021 15:31

Tgt Ion:105 Resp: 84115
Ion Ratio Lower Upper
105 100
134 24.2 9.0 27.1




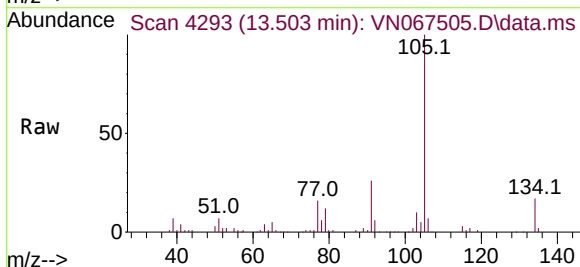


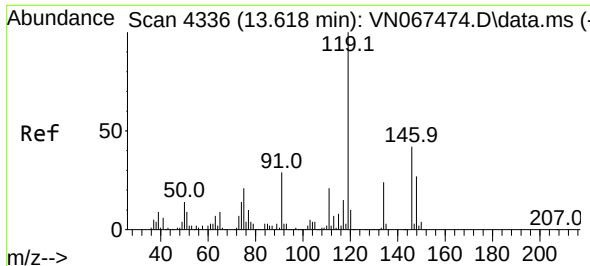

#86
p-Isopropyltoluene
Concen: 2.25 ug/l
RT: 13.562 min Scan# 4315
Delta R.T. -0.056 min
Lab File: VN067505.D
Acq: 25 Jun 2021 15:31




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion:119 Resp: 20519
Ion Ratio Lower Upper
119 100
134 25.2 12.4 37.4
91 27.1 14.8 44.3

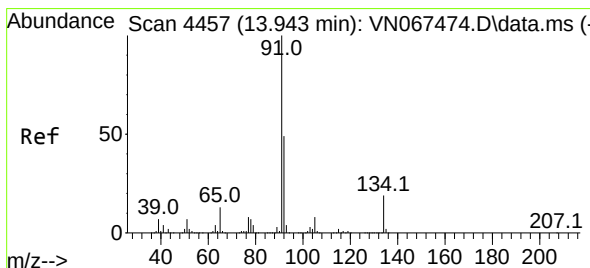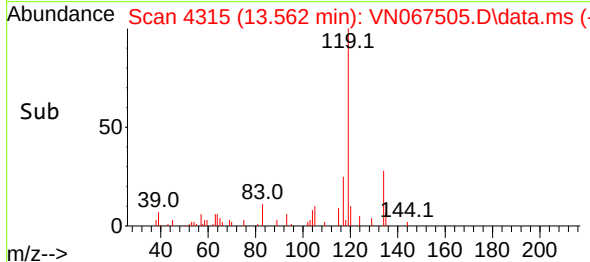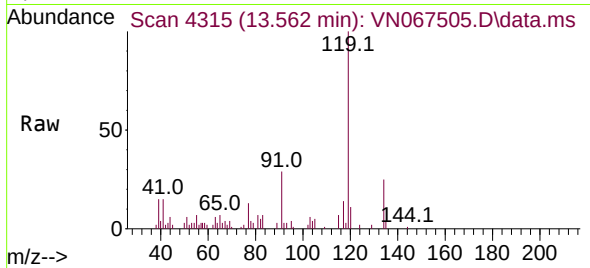

#89
n-Butylbenzene
Concen: 4.10 ug/l
RT: 13.943 min Scan# 4457
Delta R.T. -0.000 min
Lab File: VN067505.D
Acq: 25 Jun 2021 15:31

Tgt Ion: 91 Resp: 37395
Ion Ratio Lower Upper
91 100
92 46.7 25.7 77.1
134 0.0 11.2 33.6#


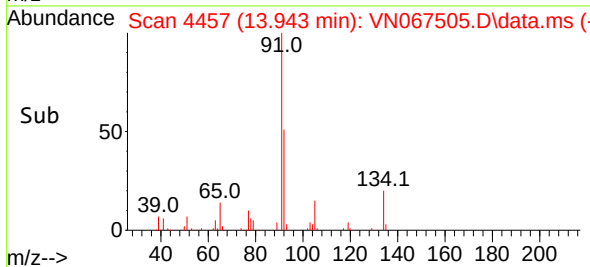

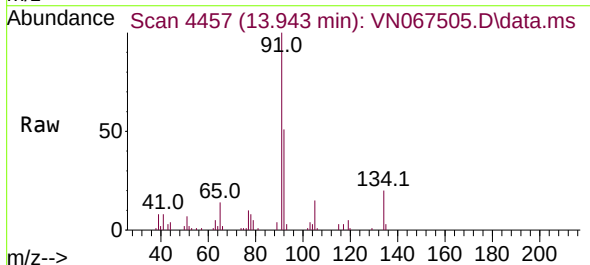




#90
Hexachloroethane
Concen: 5.58 ug/l
RT: 14.222 min Scan# 4561
Delta R.T. 0.011 min
Lab File: VN067505.D
Acq: 25 Jun 2021 15:31




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion:117 Resp: 9685
Ion Ratio Lower Upper
117 100
201 0.0 33.5 100.5#

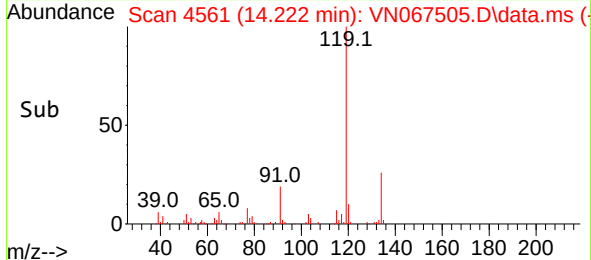

#92
1,2-Dibromo-3-Chloropropane
Concen: 0.59 ug/l
RT: 14.581 min Scan# 4695
Delta R.T. -0.022 min
Lab File: VN067505.D
Acq: 25 Jun 2021 15:31


Tgt Ion: 75 Resp: 429
Ion Ratio Lower Upper
75 100
155 0.0 29.8 89.5#
157 0.0 37.6 112.8#

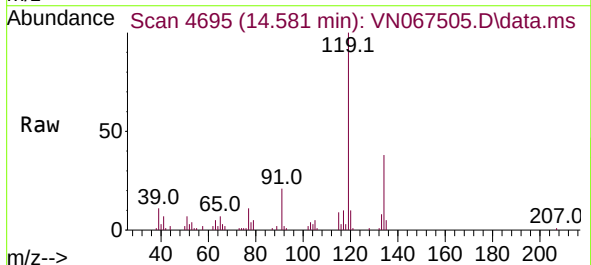



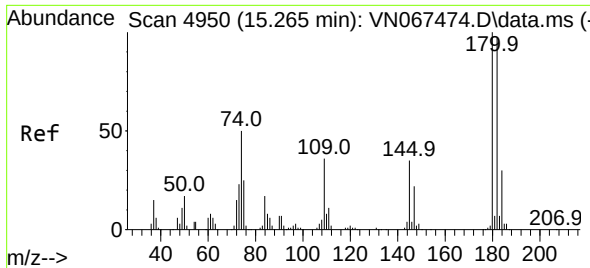


#93
1,2,4-Trichlorobenzene
Concen: 2.44 ug/l
RT: 15.262 min Scan# 4949
Delta R.T. -0.003 min
Lab File: VN067505.D
Acq: 25 Jun 2021 15:31


Instrument :
MSVOA_N
ClientSampled :

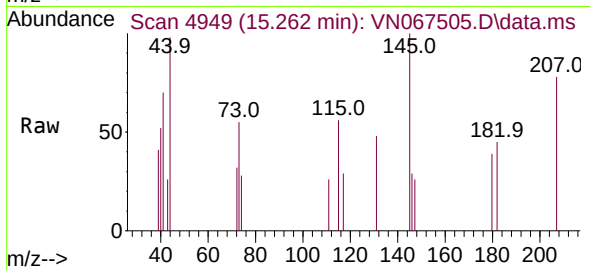



Tgt Ion:180 Resp: 235
Ion Ratio Lower Upper
180 100
182 72.8 47.5 142.5
145 88.9 17.2 51.6#

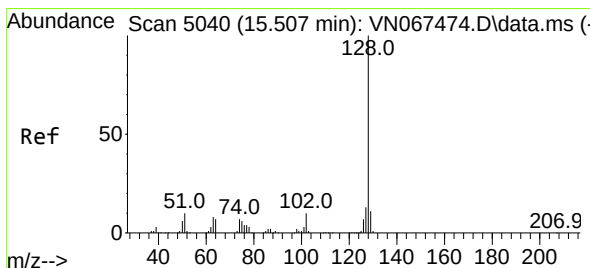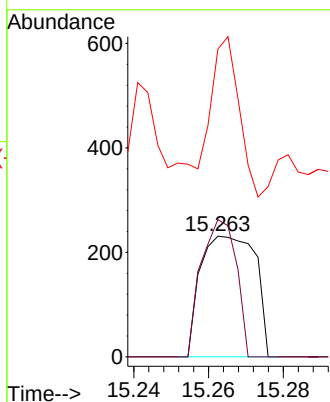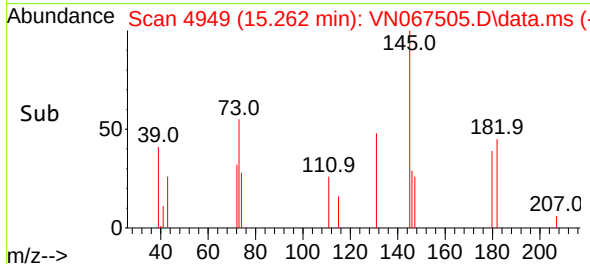


#95
Naphthalene
Concen: 4.90 ug/l
RT: 15.509 min Scan# 5041
Delta R.T. 0.002 min
Lab File: VN067505.D
Acq: 25 Jun 2021 15:31

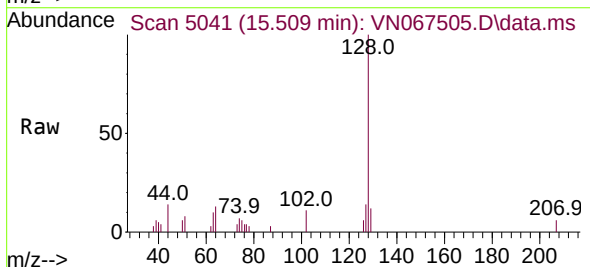


Tgt Ion:128 Resp: 11611
Ion Ratio Lower Upper
128 100
127 13.6 10.6 15.8
129 10.0 8.6 12.8

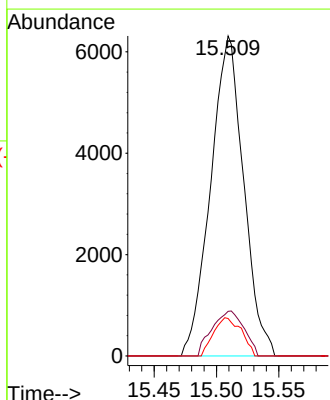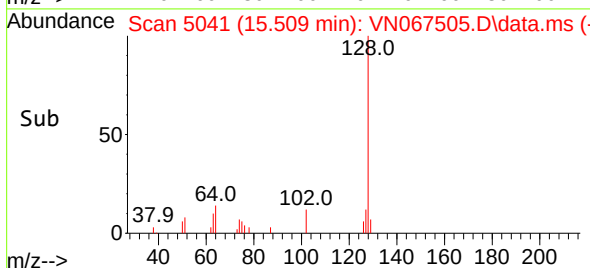

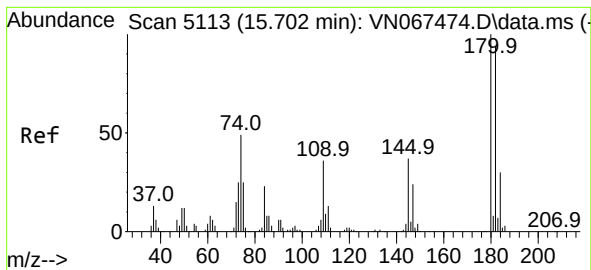

#96
 1,2,3-Trichlorobenzene
 Concen: 2.78 ug/l
 RT: 15.708 min Scan# 5115
 Delta R.T. 0.006 min
 Lab File: VN067505.D
 Acq: 25 Jun 2021 15:31

Instrument :
 MSVOA_N
 ClientSampleId :

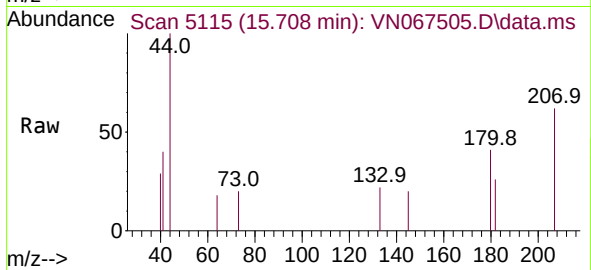

Tgt Ion:180 Resp: 540
 Ion Ratio Lower Upper
 180 100
 182 0.0 47.8 143.3#
 145 10.0 18.2 54.6#

