

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN062521\
 Data File : VN067507.D
 Acq On : 25 Jun 2021 16:20
 Operator : JC/MD
 Sample : M2806-04 20X
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :

Quant Time: Jun 26 00:39:06 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N062421W.M
 Quant Title : SW846 8260
 QLast Update : Thu Jun 24 12:18:45 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.088	168	192135	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.971	114	430024	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.746	117	384855	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.678	152	132398	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.440	65	216524	55.06	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	=	110.12%
35) Dibromofluoromethane	8.024	113	130962	49.43	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	=	98.86%
50) Toluene-d8	10.443	98	597027	52.84	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	=	105.68%
62) 4-Bromofluorobenzene	12.733	95	203788	50.62	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	=	101.24%


Target Compounds						Qvalue
3) Chloromethane	2.301	50	781	0.22	ug/l #	85
5) Bromomethane	2.869	94	434	0.24	ug/l	90
11) Tert butyl alcohol	5.401	59	3307	5.15	ug/l #	85
13) Acrolein	4.041	56	156	0.29	ug/l #	24
16) Acetone	4.288	43	922	0.61	ug/l #	48
27) cis-1,2-Dichloroethene	7.335	96	1568	0.47	ug/l #	1
31) Cyclohexane	8.088	56	8559	1.36	ug/l #	18
36) 1,1-Dichloropropene	8.086	75	27357	5.65	ug/l #	47
38) Carbon Tetrachloride	8.091	117	26349	6.39	ug/l #	15
59) 2-Hexanone	11.087	43	746	0.21	ug/l #	45
67) Ethyl Benzene	11.848	91	98932	6.07	ug/l	95
68) m/p-Xylenes	11.958	106	14279	2.59	ug/l	98
69) o-Xylene	12.283	106	3399	0.62	ug/l	99
71) Bromoform	12.739	173	1268	3.23	ug/l #	1
73) Isopropylbenzene	12.583	105	87573	6.50	ug/l	97
74) N-amyl acetate	12.371	43	1513	0.23	ug/l #	61
76) 1,2,3-Trichloropropane	12.733	75	122366	31.40	ug/l #	100
78) n-propylbenzene	12.924	91	188330	11.33	ug/l	95
79) 2-Chlorotoluene	12.924	91	188330	18.87	ug/l #	46
80) 1,3,5-Trimethylbenzene	13.063	105	15427	1.40	ug/l	98
81) trans-1,4-Dichloro-2-b...	12.733	75	122366	85.93	ug/l #	6
82) 4-Chlorotoluene	13.224	91	7892	0.81	ug/l #	45
83) tert-Butylbenzene	13.326	119	9247	1.06	ug/l	88
84) 1,2,4-Trimethylbenzene	13.372	105	1016041	94.09	ug/l	100
85) sec-Butylbenzene	13.503	105	47134	3.62	ug/l	87
86) p-Isopropyltoluene	13.774	119	17759	1.84	ug/l	96
89) n-Butylbenzene	13.946	91	24696	2.55	ug/l #	82
90) Hexachloroethane	14.222	117	7808	4.23	ug/l #	16
92) 1,2-Dibromo-3-Chloropr...	14.584	75	335	0.43	ug/l #	16
93) 1,2,4-Trichlorobenzene	15.257	180	59	2.35	ug/l #	1
95) Naphthalene	15.509	128	38075	8.15	ug/l	99
96) 1,2,3-Trichlorobenzene	15.710	180	50	2.55	ug/l #	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN062521\
Data File : VN067507.D
Acq On : 25 Jun 2021 16:20
Operator : JC/MD
Sample : M2806-04 20X
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampled :

Quant Time: Jun 26 00:39:06 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N062421W.M
Quant Title : SW846 8260
QLast Update : Thu Jun 24 12:18:45 2021
Response via : Initial Calibration

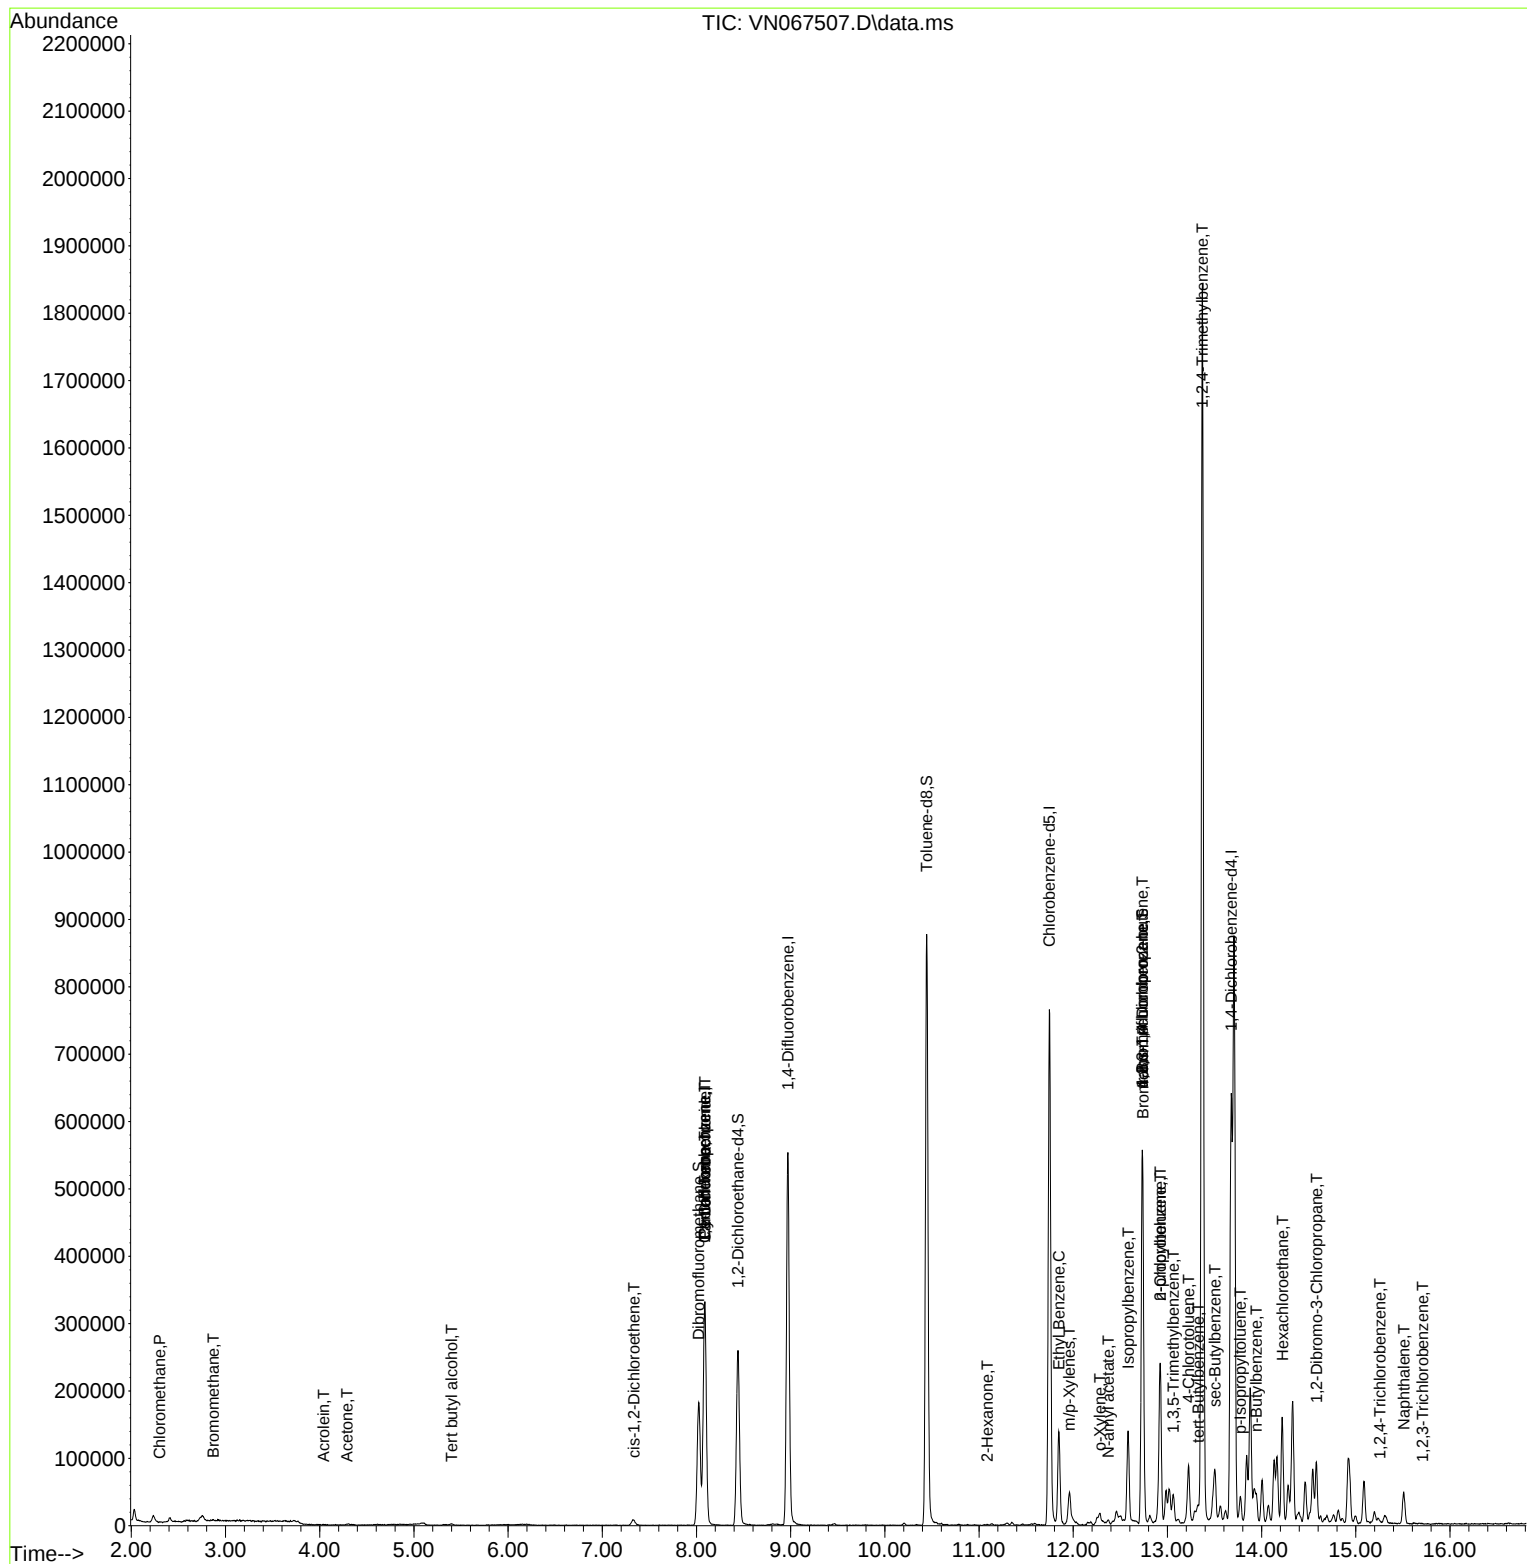




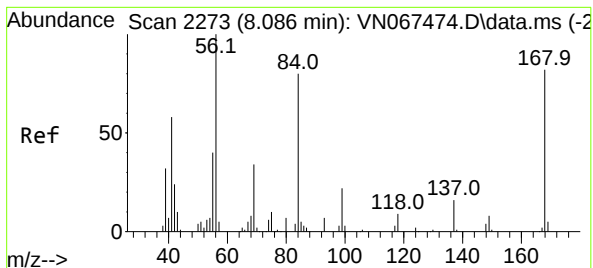


#1

Pentafluorobenzene
Concen: 50.00 ug/l
RT: 8.088 min Scan# 2274
Delta R.T. 0.002 min
Lab File: VN067507.D
Acq: 25 Jun 2021 16:20

Instrument :
MSVOA_N
ClientSampleId :




Tgt Ion:168 Resp: 192135
Ion Ratio Lower Upper
168 100
99 91.4 62.9 94.3

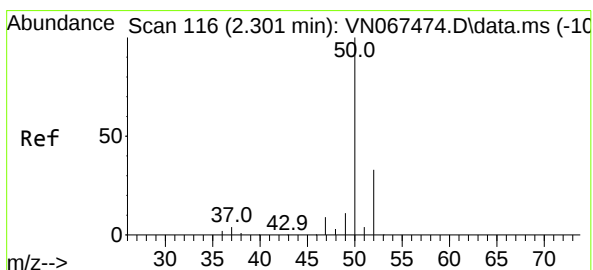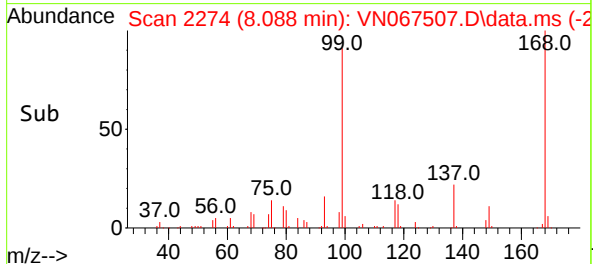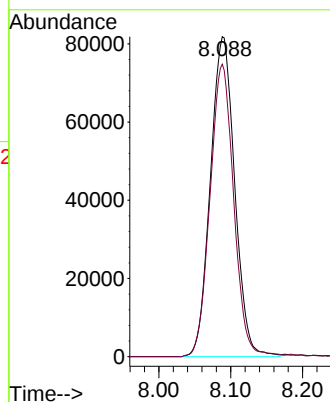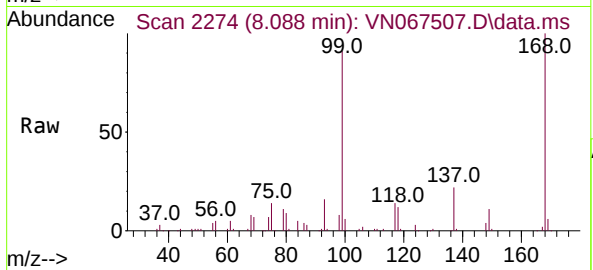


#3

Chloromethane
Concen: 0.22 ug/l
RT: 2.301 min Scan# 116
Delta R.T. -0.000 min
Lab File: VN067507.D
Acq: 25 Jun 2021 16:20

Tgt Ion: 50 Resp: 781
Ion Ratio Lower Upper
50 100
52 40.5 25.6 38.4#


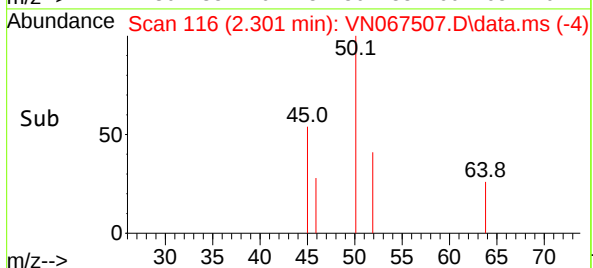
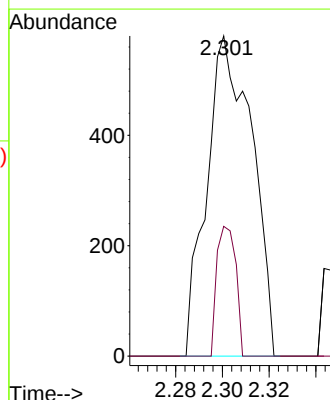
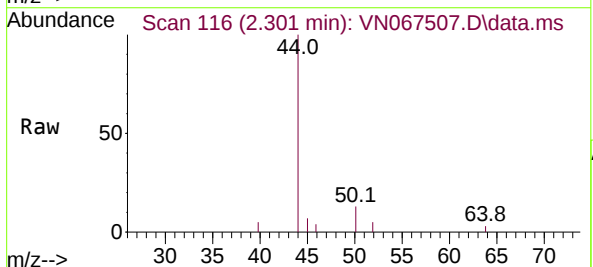




#5
Bromomethane
Concen: 0.24 ug/l
RT: 2.869 min Scan# 328
Delta R.T. 0.037 min
Lab File: VN067507.D
Acq: 25 Jun 2021 16:20




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 94 Resp: 434
Ion Ratio Lower Upper
94 100
96 83.0 73.7 110.5

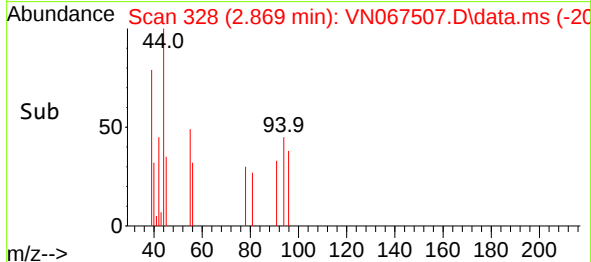

#11
Tert butyl alcohol
Concen: 5.15 ug/l
RT: 5.401 min Scan# 1272
Delta R.T. 0.013 min
Lab File: VN067507.D
Acq: 25 Jun 2021 16:20

Tgt Ion: 59 Resp: 3307
Ion Ratio Lower Upper
59 100
57 5.1 8.7 13.1#




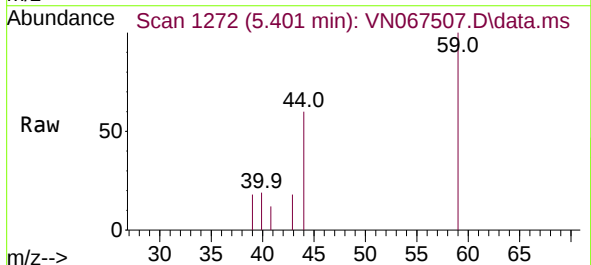




#13
Acrolein
Concen: 0.29 ug/l
RT: 4.041 min Scan# 765
Delta R.T. 0.002 min
Lab File: VN067507.D
Acq: 25 Jun 2021 16:20




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 56 Resp: 156
Ion Ratio Lower Upper
56 100
55 134.6 57.4 86.0#

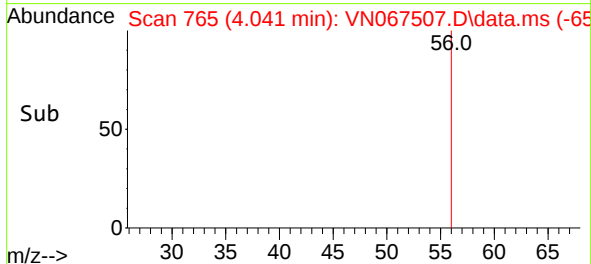

#16
Acetone
Concen: 0.61 ug/l
RT: 4.288 min Scan# 857
Delta R.T. -0.003 min
Lab File: VN067507.D
Acq: 25 Jun 2021 16:20

Tgt Ion: 43 Resp: 922
Ion Ratio Lower Upper
43 100
58 0.0 21.2 31.8#

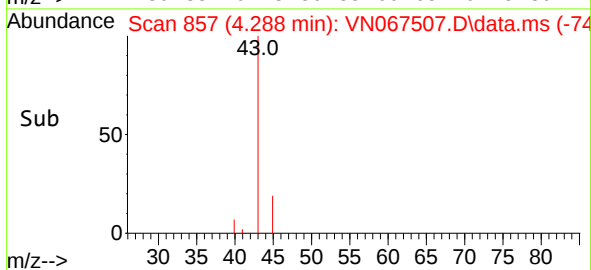




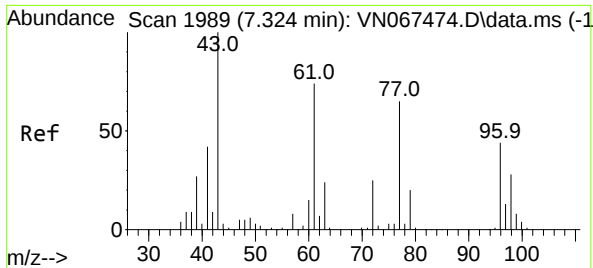


#27

cis-1,2-Dichloroethene
Concen: 0.47 ug/l
RT: 7.335 min Scan# 1993
Delta R.T. 0.011 min
Lab File: VN067507.D
Acq: 25 Jun 2021 16:20

Instrument :
MSVOA_N
ClientSampled :




Tgt Ion: 96 Resp: 1568
Ion Ratio Lower Upper
96 100
61 0.0 0.0 338.8
98 23.2 0.0 129.8

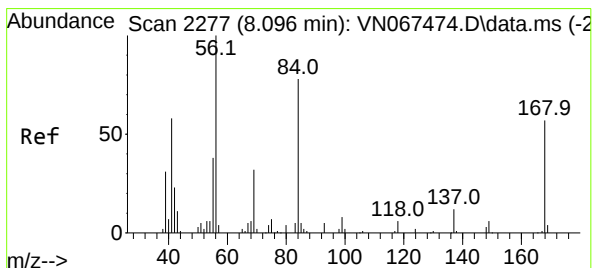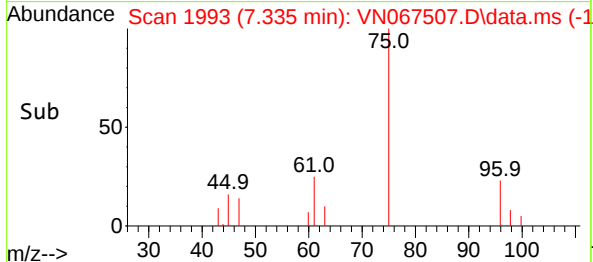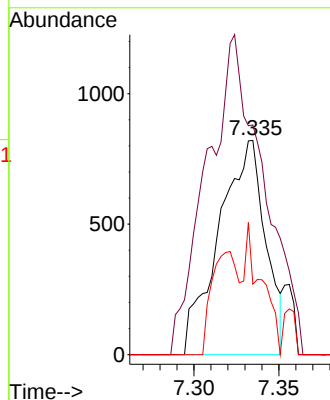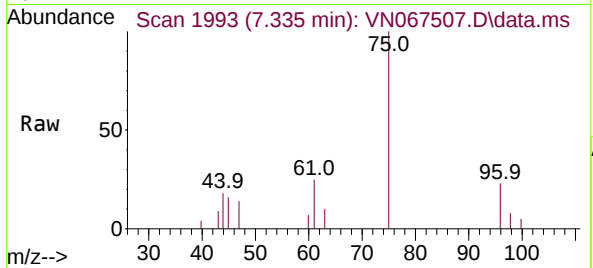


#31

Cyclohexane
Concen: 1.36 ug/l
RT: 8.088 min Scan# 2274
Delta R.T. -0.008 min
Lab File: VN067507.D
Acq: 25 Jun 2021 16:20

Tgt Ion: 56 Resp: 8559
Ion Ratio Lower Upper
56 100
69 153.4 27.3 40.9#
84 107.0 64.9 97.3#


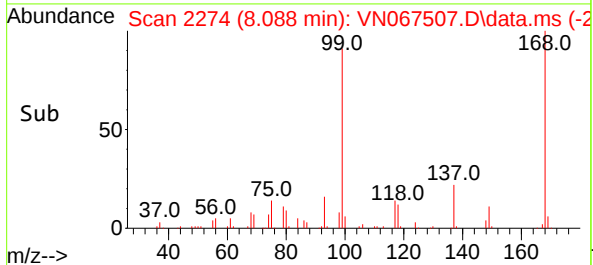
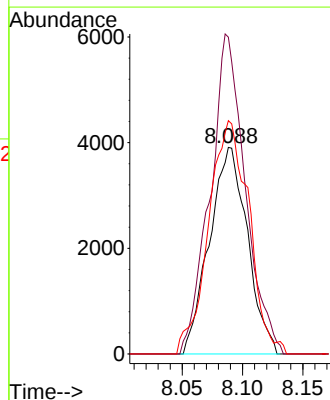
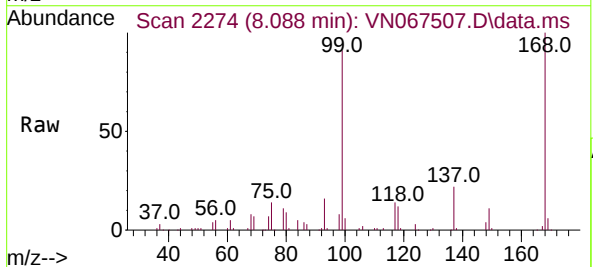


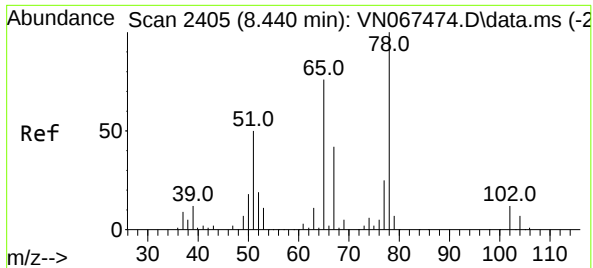

#33
 1,2-Dichloroethane-d4
 Concen: 55.06 ug/l
 RT: 8.440 min Scan# 2405
 Delta R.T. -0.000 min
 Lab File: VN067507.D
 Acq: 25 Jun 2021 16:20




Instrument :
 MSVOA_N
 ClientSampleId :


Tgt Ion: 65 Resp: 216524
 Ion Ratio Lower Upper
 65 100
 67 52.2 0.0 98.6

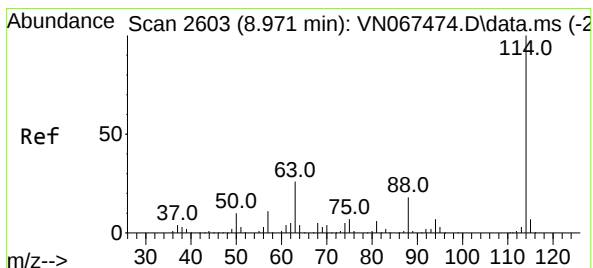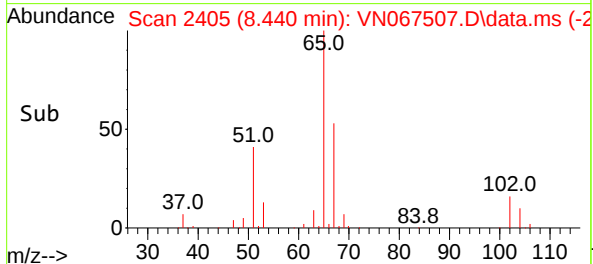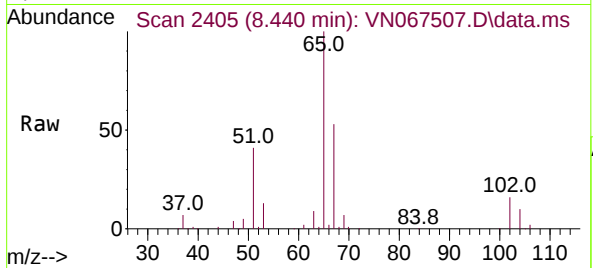

#34
 1,4-Difluorobenzene
 Concen: 50.00 ug/l
 RT: 8.971 min Scan# 2603
 Delta R.T. -0.000 min
 Lab File: VN067507.D
 Acq: 25 Jun 2021 16:20

Tgt Ion: 114 Resp: 430024
 Ion Ratio Lower Upper
 114 100
 63 26.9 0.0 49.0
 88 19.1 0.0 36.6


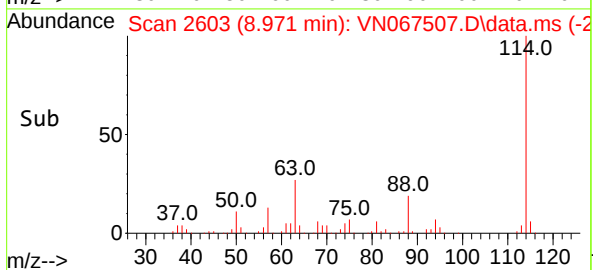

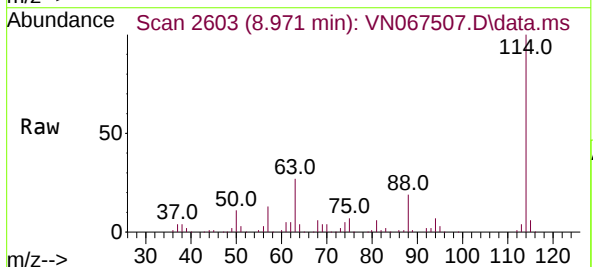




#35
Dibromofluoromethane
Concen: 49.43 ug/l
RT: 8.024 min Scan# 2250
Delta R.T. -0.000 min
Lab File: VN067507.D
Acq: 25 Jun 2021 16:20




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:113 Resp: 130962
Ion Ratio Lower Upper
113 100
111 104.5 83.8 125.8
192 12.7 13.4 20.0#

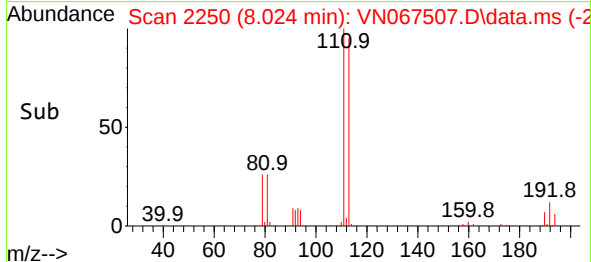

#36
1,1-Dichloropropene
Concen: 5.65 ug/l
RT: 8.086 min Scan# 2273
Delta R.T. -0.136 min
Lab File: VN067507.D
Acq: 25 Jun 2021 16:20


Tgt Ion: 75 Resp: 27357
Ion Ratio Lower Upper
75 100
110 3.6 15.7 47.0#
77 0.0 24.6 37.0#

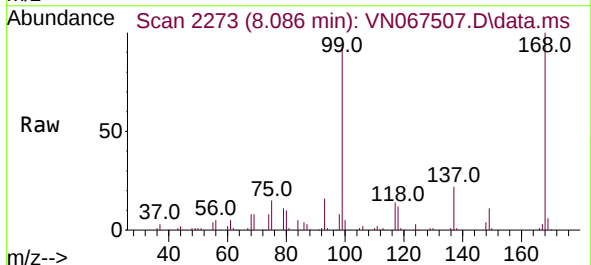






#38
Carbon Tetrachloride
Concen: 6.39 ug/l
RT: 8.091 min Scan# 2275
Delta R.T. -0.115 min
Lab File: VN067507.D
Acq: 25 Jun 2021 16:20


Instrument :
MSVOA_N
ClientSampleId :





Tgt Ion:117 Resp: 26349
Ion Ratio Lower Upper
117 100
119 3.6 75.4 113.2#
121 0.0 23.5 35.3#

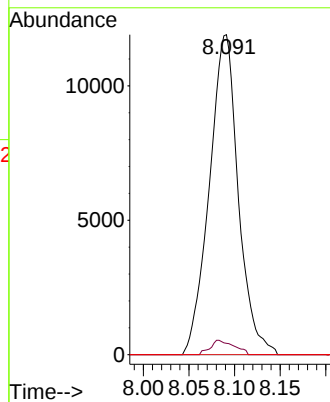


#50
Toluene-d8
Concen: 52.84 ug/l
RT: 10.443 min Scan# 3152
Delta R.T. 0.000 min
Lab File: VN067507.D
Acq: 25 Jun 2021 16:20



Tgt Ion: 98 Resp: 597027
Ion Ratio Lower Upper
98 100
100 62.7 51.7 77.5



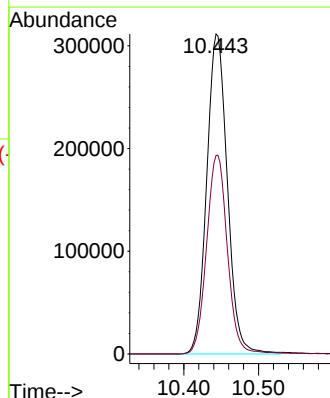





#59
2-Hexanone
Concen: 0.21 ug/l
RT: 11.087 min Scan# 3392
Delta R.T. -0.000 min
Lab File: VN067507.D
Acq: 25 Jun 2021 16:20




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 43 Resp: 746
Ion Ratio Lower Upper
43 100
58 11.5 24.7 74.1#

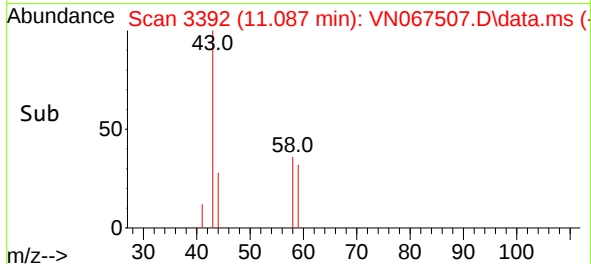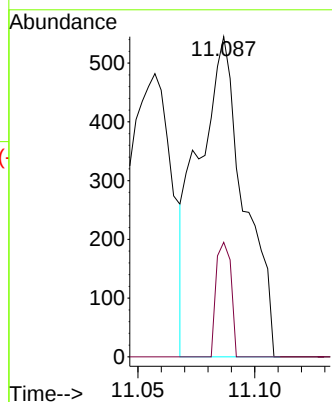

#62
4-Bromofluorobenzene
Concen: 50.62 ug/l
RT: 12.733 min Scan# 4006
Delta R.T. 0.000 min
Lab File: VN067507.D
Acq: 25 Jun 2021 16:20

Tgt Ion: 95 Resp: 203788
Ion Ratio Lower Upper
95 100
174 51.2 0.0 122.0
176 48.2 0.0 117.6









#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 11.746 min Scan# 3638
Delta R.T. 0.000 min
Lab File: VN067507.D
Acq: 25 Jun 2021 16:20




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:117 Resp: 384855
Ion Ratio Lower Upper
117 100
82 72.3 53.1 79.7
119 30.9 25.5 38.3

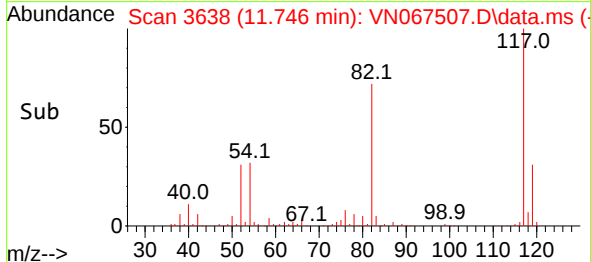

#67
Ethyl Benzene
Concen: 6.07 ug/l
RT: 11.848 min Scan# 3676
Delta R.T. 0.000 min
Lab File: VN067507.D
Acq: 25 Jun 2021 16:20

Tgt Ion: 91 Resp: 98932
Ion Ratio Lower Upper
91 100
106 26.7 23.4 35.0




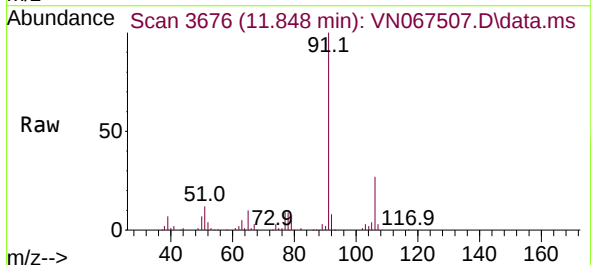




#68
m/p-Xylenes
Concen: 2.59 ug/l
RT: 11.958 min Scan# 3717
Delta R.T. 0.002 min
Lab File: VN067507.D
Acq: 25 Jun 2021 16:20




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion:106 Resp: 14279
Ion Ratio Lower Upper
106 100
91 222.6 180.6 270.8

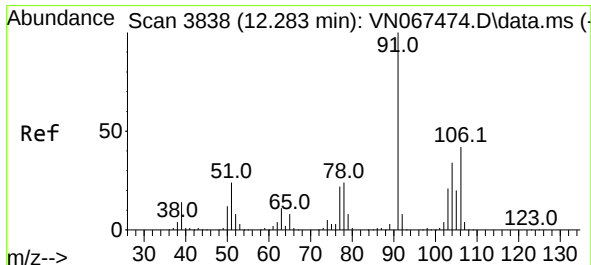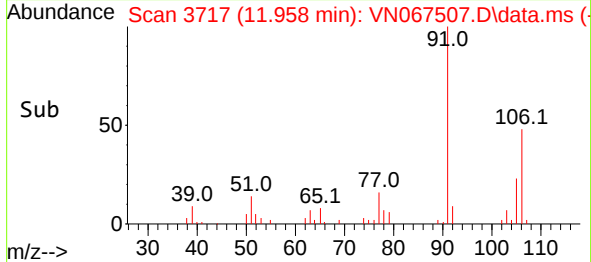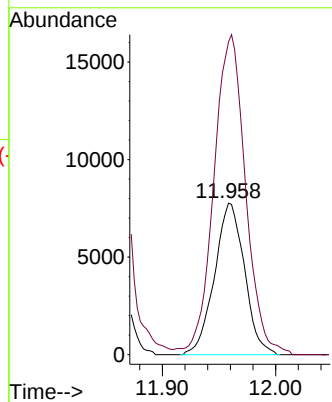

#69
o-Xylene
Concen: 0.62 ug/l
RT: 12.283 min Scan# 3838
Delta R.T. -0.000 min
Lab File: VN067507.D
Acq: 25 Jun 2021 16:20

Tgt Ion:106 Resp: 3399
Ion Ratio Lower Upper
106 100
91 237.8 118.3 354.9




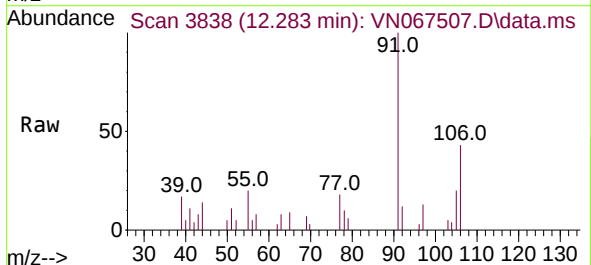


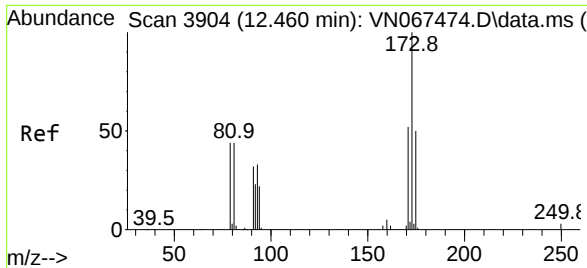

#71
Bromoform
Concen: 3.23 ug/l
RT: 12.739 min Scan# 4008
Delta R.T. 0.279 min
Lab File: VN067507.D
Acq: 25 Jun 2021 16:20




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion:173 Resp: 1268
Ion Ratio Lower Upper
173 100
175 607.8 23.9 71.8#
254 0.0 0.0 0.0

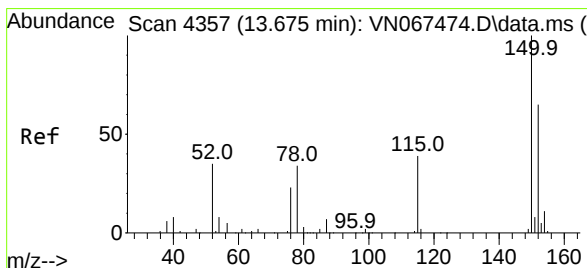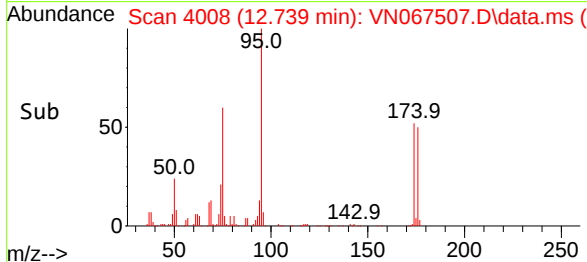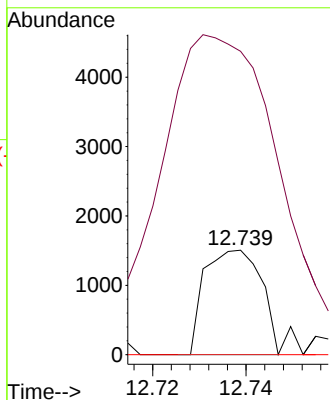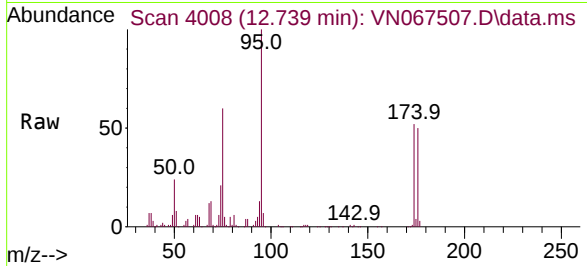

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 13.678 min Scan# 4358
Delta R.T. 0.002 min
Lab File: VN067507.D
Acq: 25 Jun 2021 16:20

Tgt Ion:152 Resp: 132398
Ion Ratio Lower Upper
152 100
115 90.9 36.1 108.5
150 159.7 0.0 351.8


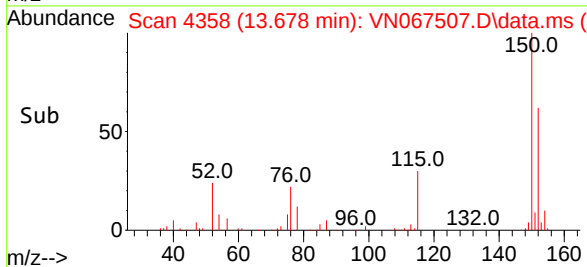
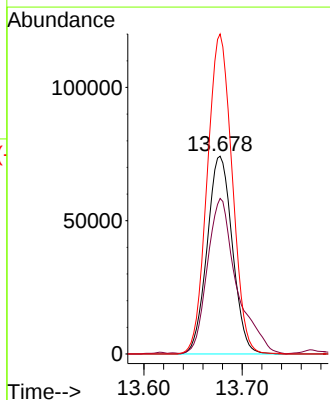
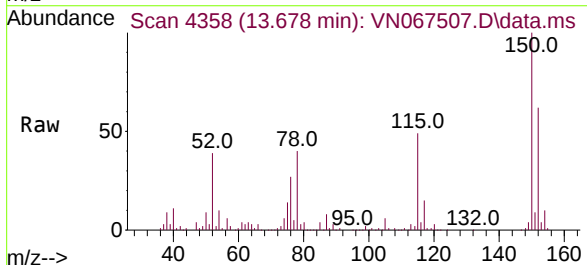




#73
Isopropylbenzene
Concen: 6.50 ug/l
RT: 12.583 min Scan# 3950
Delta R.T. 0.002 min
Lab File: VN067507.D
Acq: 25 Jun 2021 16:20




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion:105 Resp: 87573
Ion Ratio Lower Upper
105 100
120 23.6 12.5 37.5

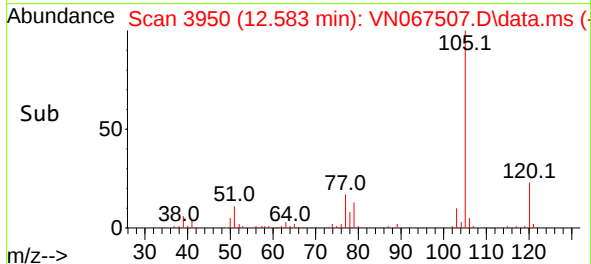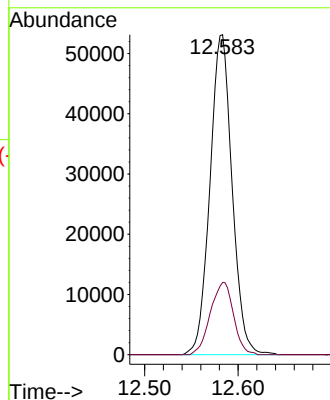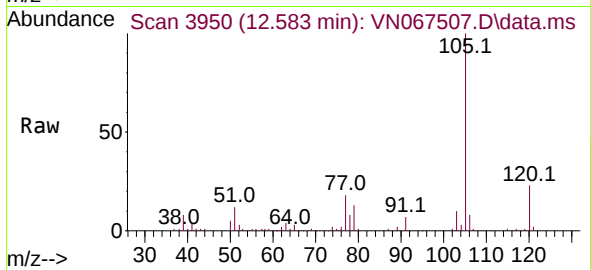

#74
N-ethyl acetate
Concen: 0.23 ug/l
RT: 12.371 min Scan# 3871
Delta R.T. -0.019 min
Lab File: VN067507.D
Acq: 25 Jun 2021 16:20

Tgt Ion: 43 Resp: 1513
Ion Ratio Lower Upper
43 100
70 17.8 29.4 44.2#
55 0.0 17.0 25.4#
61 0.0 17.6 26.4#



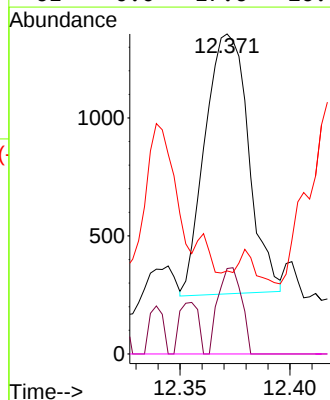





#76
1,2,3-Trichloropropane
Concen: 31.40 ug/l
RT: 12.733 min Scan# 4006
Delta R.T. -0.151 min
Lab File: VN067507.D
Acq: 25 Jun 2021 16:20




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 75 Resp: 122366
Ion Ratio Lower Upper
75 100
77 1.1 0.0 0.0#

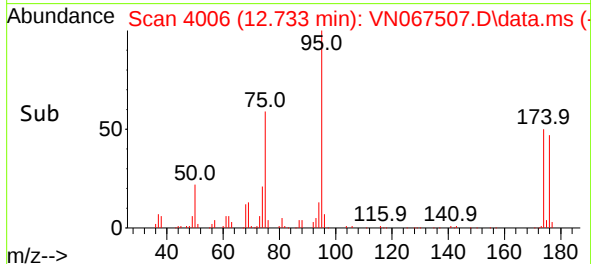

#78
n-propylbenzene
Concen: 11.33 ug/l
RT: 12.924 min Scan# 4077
Delta R.T. 0.003 min
Lab File: VN067507.D
Acq: 25 Jun 2021 16:20

Tgt Ion: 91 Resp: 188330
Ion Ratio Lower Upper
91 100
120 18.7 10.4 31.4



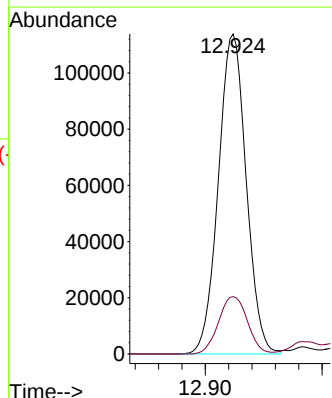
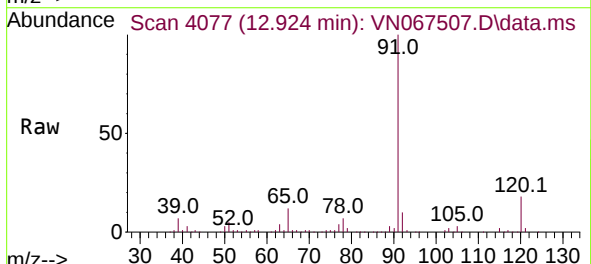




#79
2-Chlorotoluene
Concen: 18.87 ug/l
RT: 12.924 min Scan# 4077
Delta R.T. -0.086 min
Lab File: VN067507.D
Acq: 25 Jun 2021 16:20




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 91 Resp: 188330
Ion Ratio Lower Upper
91 100
126 0.0 14.5 43.5#

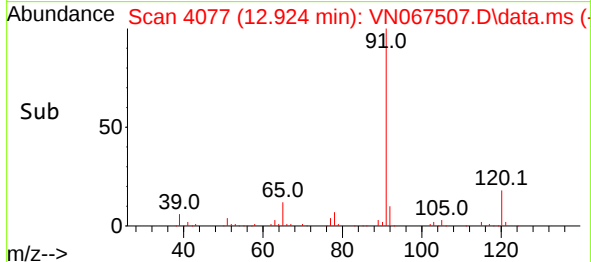

#80
1,3,5-Trimethylbenzene
Concen: 1.40 ug/l
RT: 13.063 min Scan# 4129
Delta R.T. 0.002 min
Lab File: VN067507.D
Acq: 25 Jun 2021 16:20

Tgt Ion: 105 Resp: 15427
Ion Ratio Lower Upper
105 100
120 43.4 22.2 66.6




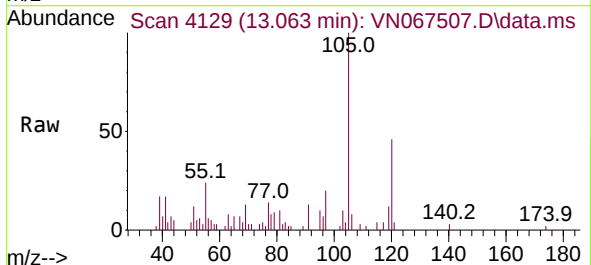




#81
trans-1,4-Dichloro-2-butene
Concen: 85.93 ug/l
RT: 12.733 min Scan# 4006
Delta R.T. 0.104 min
Lab File: VN067507.D
Acq: 25 Jun 2021 16:20




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 75 Resp: 122366
Ion Ratio Lower Upper
75 100
53 0.0 87.6 131.4#
89 0.0 37.8 56.8#

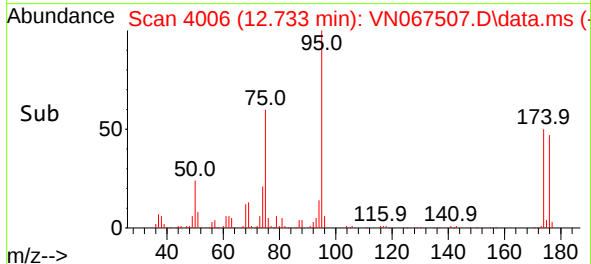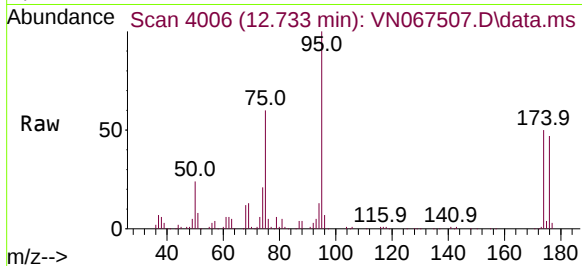

#82
4-Chlorotoluene
Concen: 0.81 ug/l
RT: 13.224 min Scan# 4189
Delta R.T. 0.118 min
Lab File: VN067507.D
Acq: 25 Jun 2021 16:20

Tgt Ion: 91 Resp: 7892
Ion Ratio Lower Upper
91 100
126 0.0 14.8 44.4#




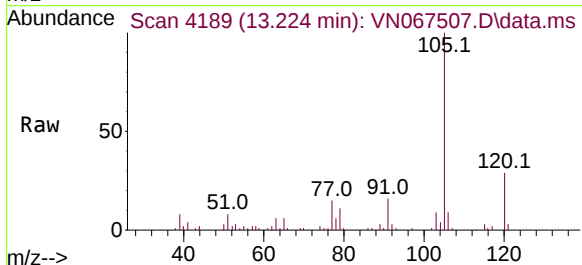




#83
tert-Butylbenzene
Concen: 1.06 ug/l
RT: 13.326 min Scan# 4227
Delta R.T. 0.000 min
Lab File: VN067507.D
Acq: 25 Jun 2021 16:20




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:119 Resp: 9247
Ion Ratio Lower Upper
119 100
91 92.6 39.5 118.5
134 24.3 12.0 36.0

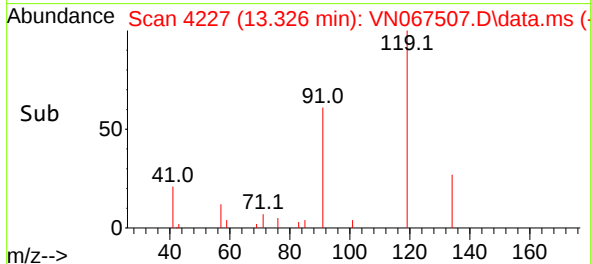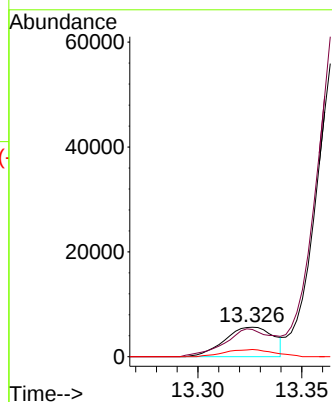

#84
1,2,4-Trimethylbenzene
Concen: 94.09 ug/l
RT: 13.372 min Scan# 4244
Delta R.T. 0.003 min
Lab File: VN067507.D
Acq: 25 Jun 2021 16:20

Tgt Ion:105 Resp: 1016041
Ion Ratio Lower Upper
105 100
120 41.1 20.6 61.8



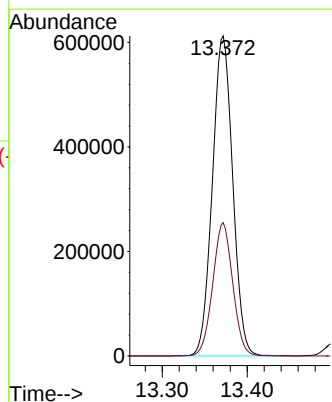





#85
sec-Butylbenzene
Concen: 3.62 ug/l
RT: 13.503 min Scan# 4293
Delta R.T. 0.000 min
Lab File: VN067507.D
Acq: 25 Jun 2021 16:20




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:105 Resp: 47134
Ion Ratio Lower Upper
105 100
134 24.0 9.0 27.1

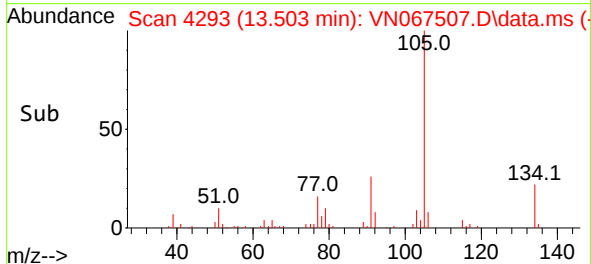

#86
p-Isopropyltoluene
Concen: 1.84 ug/l
RT: 13.774 min Scan# 4394
Delta R.T. 0.156 min
Lab File: VN067507.D
Acq: 25 Jun 2021 16:20

Tgt Ion:119 Resp: 17759
Ion Ratio Lower Upper
119 100
134 28.4 12.4 37.4
91 30.7 14.8 44.3


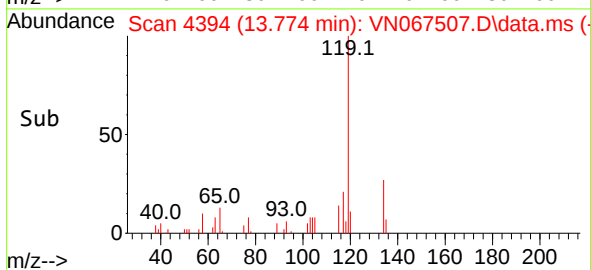




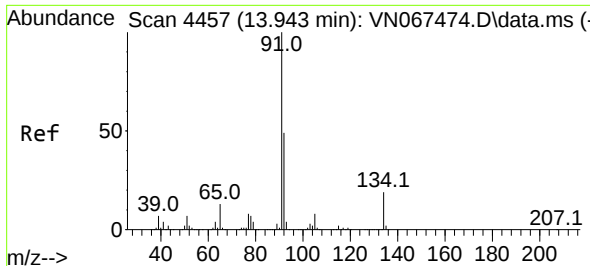

#89
n-Butylbenzene
Concen: 2.55 ug/l
RT: 13.946 min Scan# 4458
Delta R.T. 0.003 min
Lab File: VN067507.D
Acq: 25 Jun 2021 16:20




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 91 Resp: 24696
Ion Ratio Lower Upper
91 100
92 47.5 25.7 77.1
134 0.0 11.2 33.6#

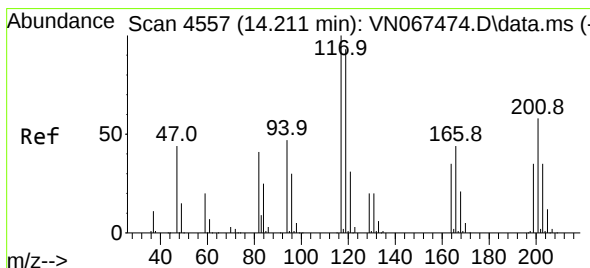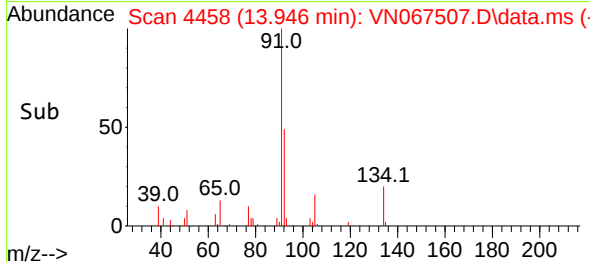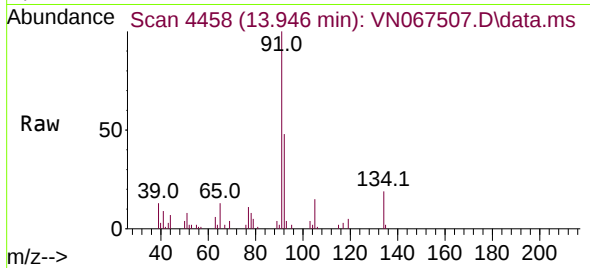

#90
Hexachloroethane
Concen: 4.23 ug/l
RT: 14.222 min Scan# 4561
Delta R.T. 0.011 min
Lab File: VN067507.D
Acq: 25 Jun 2021 16:20


Tgt Ion: 117 Resp: 7808
Ion Ratio Lower Upper
117 100
201 0.0 33.5 100.5#

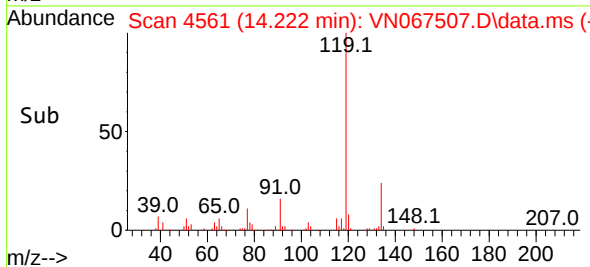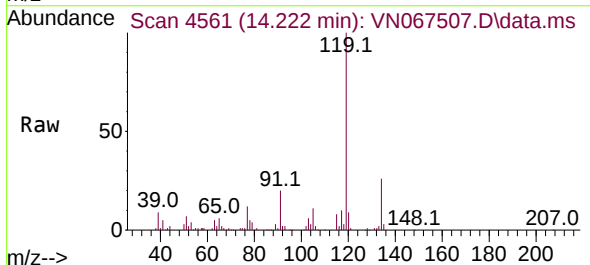



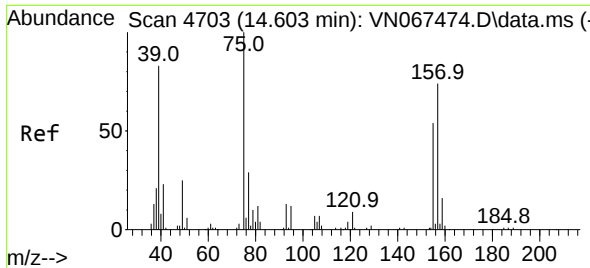


#92
 1,2-Dibromo-3-Chloropropane
 Concen: 0.43 ug/l
 RT: 14.584 min Scan# 4696
 Delta R.T. -0.019 min
 Lab File: VN067507.D
 Acq: 25 Jun 2021 16:20

Instrument :
 MSVOA_N
 ClientSampleId :



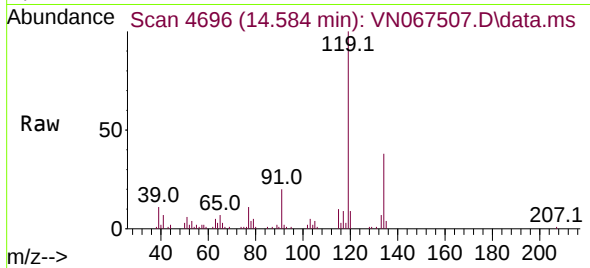



Tgt Ion: 75 Resp: 335
 Ion Ratio Lower Upper
 75 100
 155 0.0 29.8 89.5#
 157 0.0 37.6 112.8#

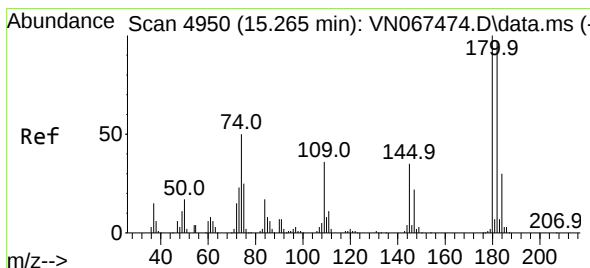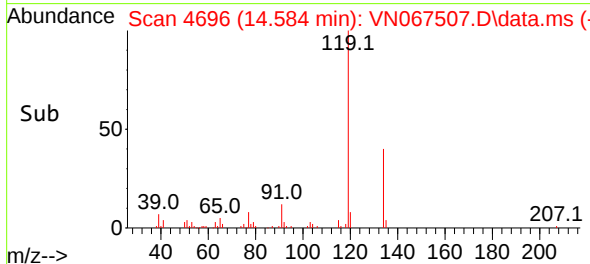

#93
 1,2,4-Trichlorobenzene
 Concen: 2.35 ug/l
 RT: 15.257 min Scan# 4947
 Delta R.T. -0.008 min
 Lab File: VN067507.D
 Acq: 25 Jun 2021 16:20

Tgt Ion: 180 Resp: 59
 Ion Ratio Lower Upper
 180 100
 182 89.8 47.5 142.5
 145 1108.5 17.2 51.6#


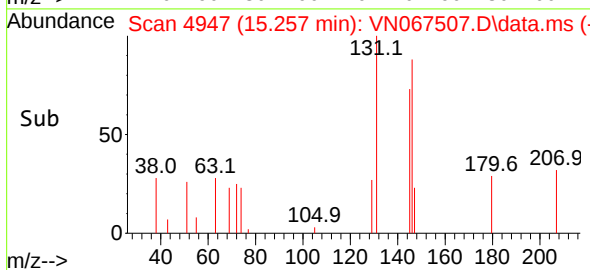
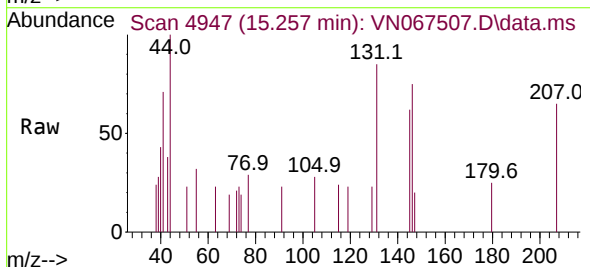



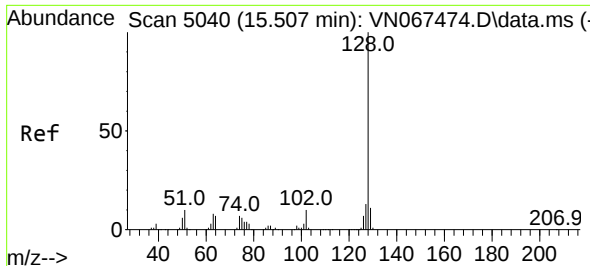

#95
Naphthalene
Concen: 8.15 ug/l
RT: 15.509 min Scan# 5041
Delta R.T. 0.002 min
Lab File: VN067507.D
Acq: 25 Jun 2021 16:20

Instrument :
MSVOA_N
ClientSampleId :

Tgt Ion:128	Resp:	38075
Ion Ratio	Lower	Upper
128	100	
127	13.6	10.6 15.8
129	10.3	8.6 12.8

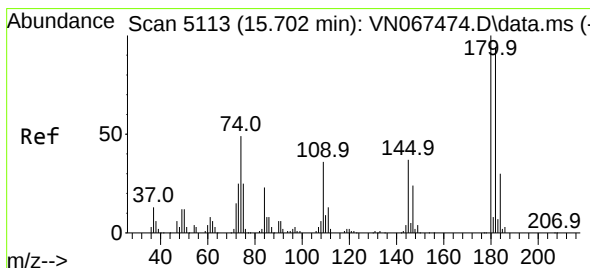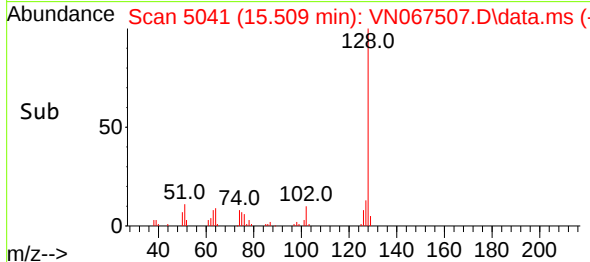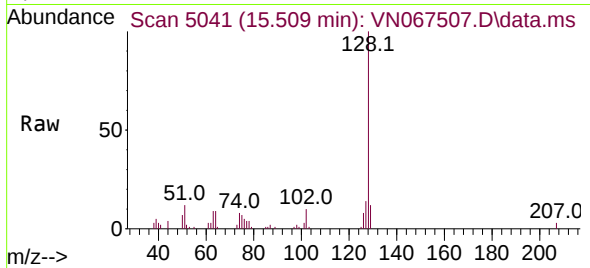

#96
1,2,3-Trichlorobenzene
Concen: 2.55 ug/l
RT: 15.710 min Scan# 5116
Delta R.T. 0.008 min
Lab File: VN067507.D
Acq: 25 Jun 2021 16:20

Tgt Ion:180	Resp:	50
Ion Ratio	Lower	Upper
180	100	
182	432.0	47.8 143.3#
145	54.0	18.2 54.6

