
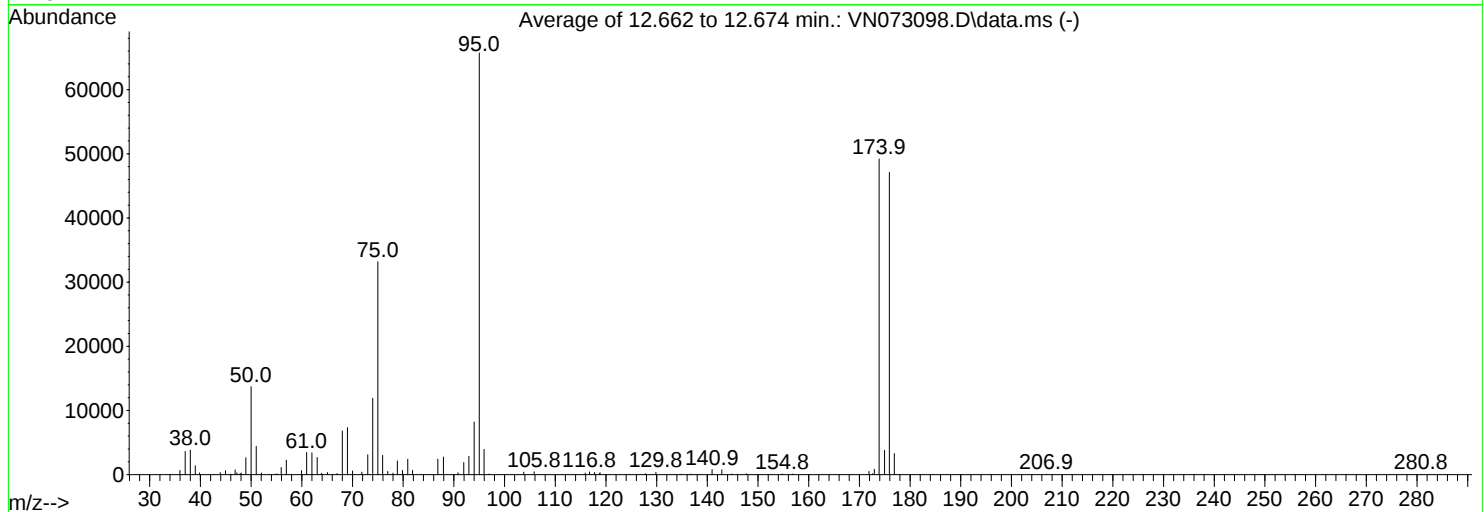


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN062522\  
Data File : VN073098.D  
Acq On : 25 Jun 2022 09:34  
Operator : JC\MD  
Sample : BFB  
Misc : 5.0mL/MSVOA\_N/WATER  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N061722W.M  
Title : SW846 8260  
Last Update : Sat Jun 18 06:22:45 2022

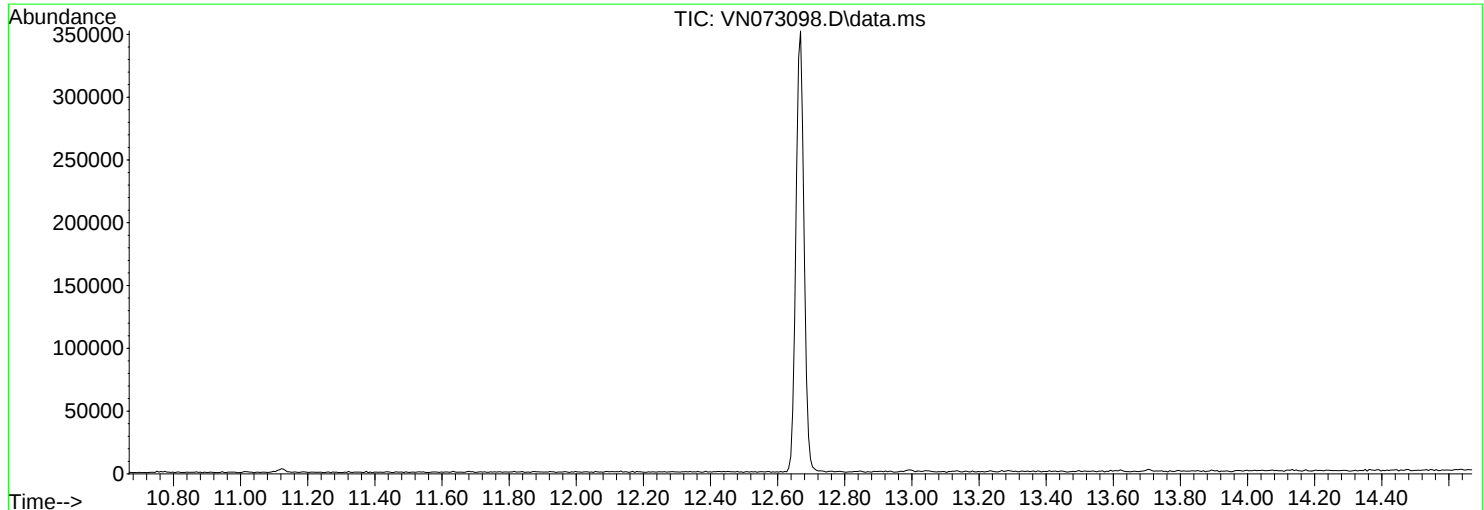

AutoFind: Scans 1832, 1833, 1834; Background Corrected with Scan 1823

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 50             | 95              | 15              | 40              | 20.9         | 13720      | PASS                |
| 75             | 95              | 30              | 60              | 50.5         | 33195      | PASS                |
| 95             | 95              | 100             | 100             | 100.0        | 65731      | PASS                |
| 96             | 95              | 5               | 9               | 6.0          | 3940       | PASS                |
| 173            | 174             | 0.00            | 2               | 1.7          | 858        | PASS                |
| 174            | 95              | 50              | 100             | 74.9         | 49200      | PASS                |
| 175            | 174             | 5               | 9               | 7.7          | 3797       | PASS                |
| 176            | 174             | 95              | 101             | 95.8         | 47120      | PASS                |
| 177            | 176             | 5               | 9               | 7.0          | 3293       | PASS                |