
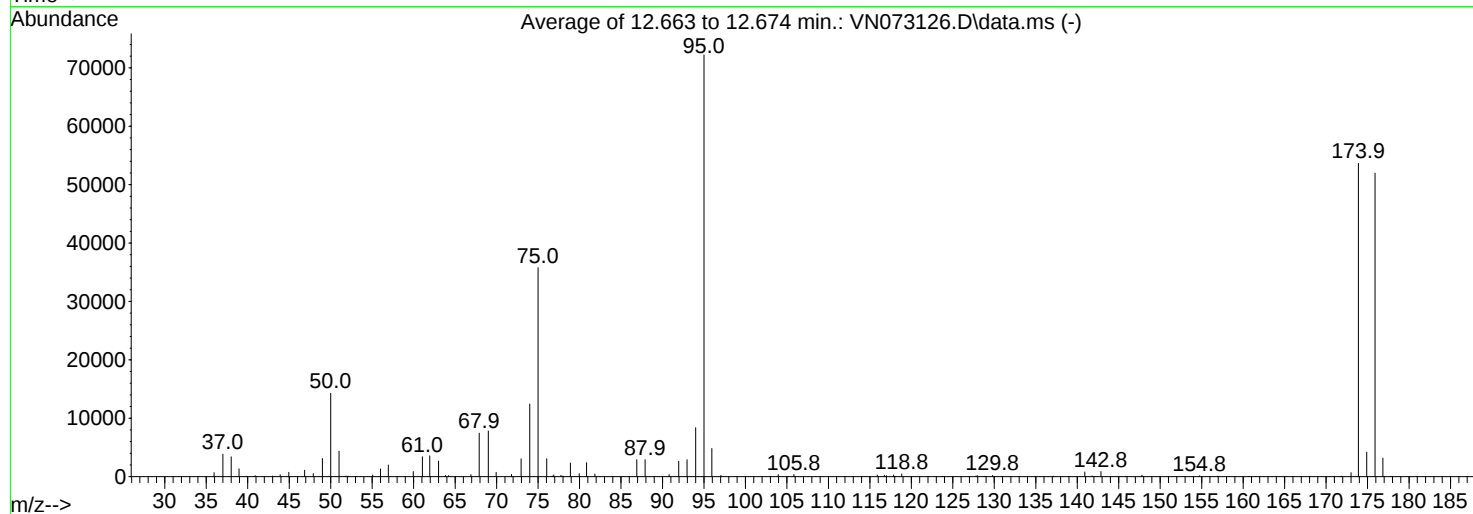


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN062522\
Data File : VN073126.D
Acq On : 25 Jun 2022 22:50
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N061722W.M
Title : SW846 8260
Last Update : Sat Jun 18 06:22:45 2022

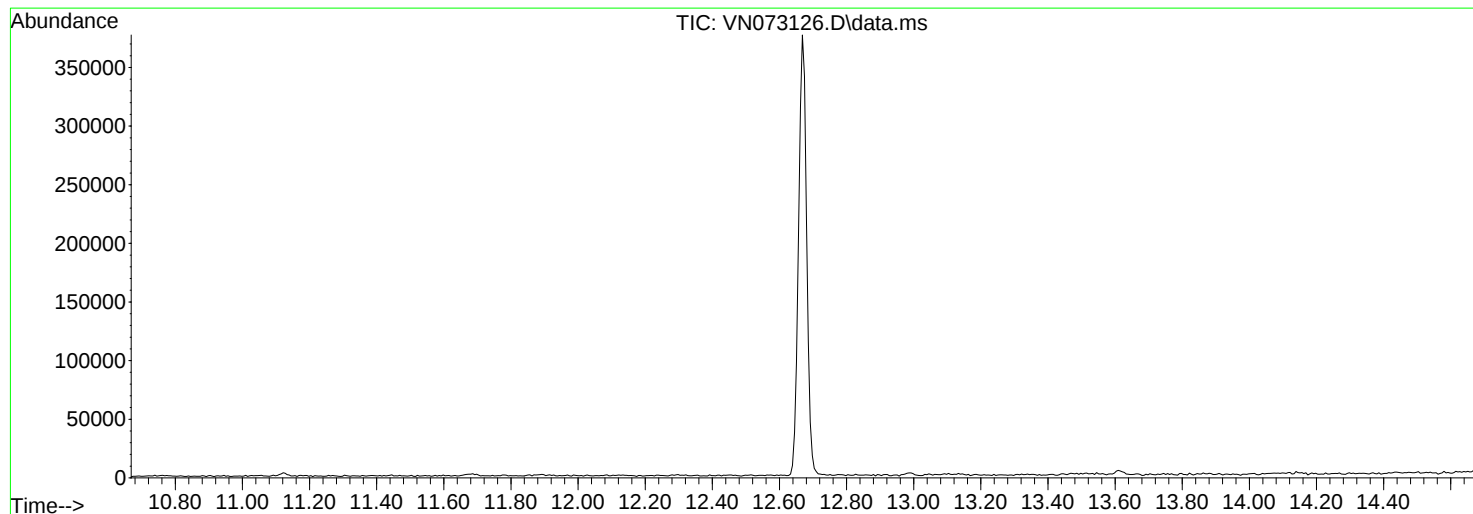

AutoFind: Scans 1832, 1833, 1834; Background Corrected with Scan 1824

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.8	14287	PASS
75	95	30	60	49.5	35792	PASS
95	95	100	100	100.0	72235	PASS
96	95	5	9	6.7	4814	PASS
173	174	0.00	2	1.3	677	PASS
174	95	50	100	74.3	53656	PASS
175	174	5	9	7.8	4193	PASS
176	174	95	101	96.9	51987	PASS
177	176	5	9	6.1	3195	PASS