
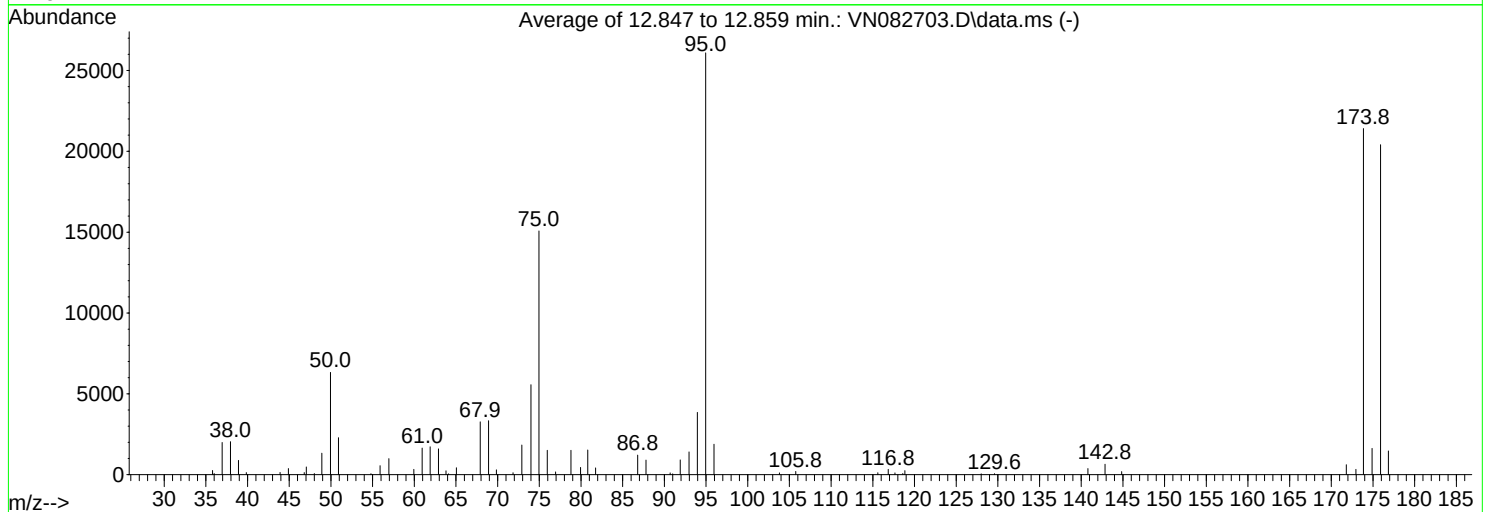


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN062524\
Data File : VN082703.D
Acq On : 25 Jun 2024 08:29
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N061724W.M
Title : SW846 8260
Last Update : Tue Jun 18 04:52:44 2024

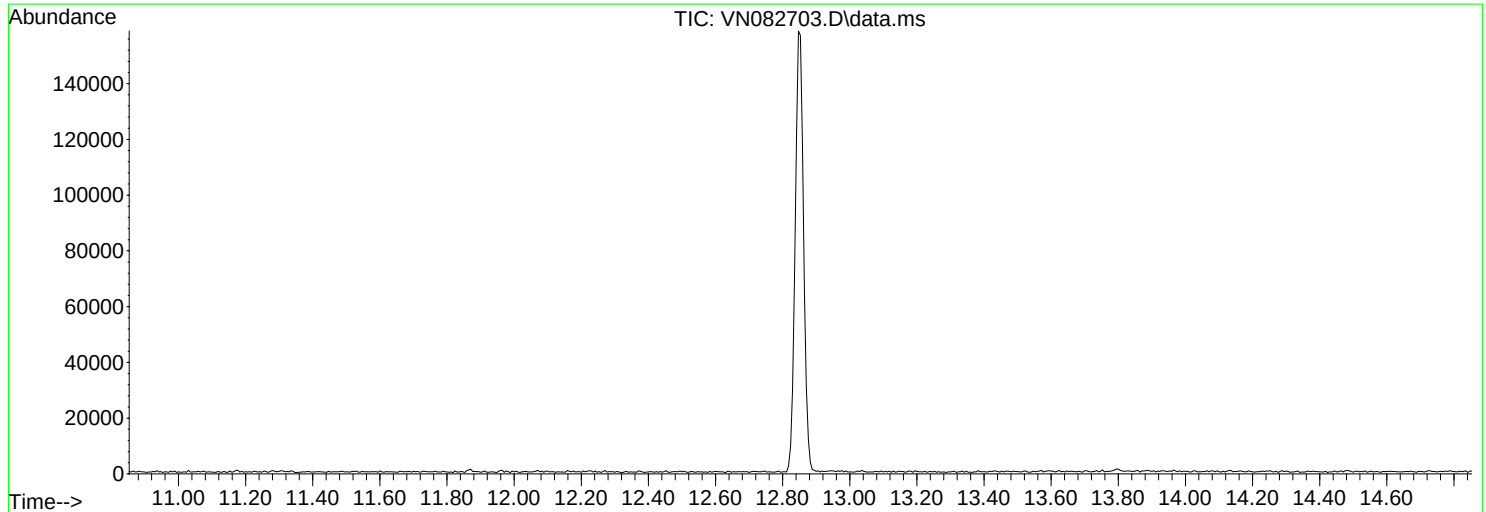

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1844

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	24.3	6329	PASS
75	95	30	60	57.8	15075	PASS
95	95	100	100	100.0	26093	PASS
96	95	5	9	7.2	1879	PASS
173	174	0.00	2	1.5	328	PASS
174	95	50	100	82.0	21408	PASS
175	174	5	9	7.6	1622	PASS
176	174	95	101	95.3	20408	PASS
177	176	5	9	7.2	1463	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.80	261	48.90	1330	64.10	53	78.80	150
36.00	71	49.95	6329	65.05	426	79.95	44
36.95	1993	50.90	2285	67.90	3262	80.80	152
37.95	2035	54.80	58	68.90	3337	81.75	41
38.90	885	55.90	555	69.85	302	86.80	1205
39.85	132	56.95	990	71.85	118	87.80	899
43.90	139	59.95	324	72.90	1833	90.70	112
44.90	381	60.95	1648	74.00	5568	91.00	52
46.80	131	61.90	1725	74.95	15075	91.90	908
47.05	480	62.90	1590	75.95	1507	92.95	1403
48.00	70	63.80	235	76.95	164	93.95	3847

Average of 12.847 to 12.859 min.: VN082703.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
94.95	26093	140.80	373				
95.95	1879	142.85	642				
103.80	113	144.85	187				
105.75	196	171.80	612				
115.60	116	172.95	328				
116.85	325	173.85	21408				
117.65	114	174.90	1622				
118.60	71	175.90	20408				
118.85	244	176.85	1463				
128.00	50						
129.60	56						

Instrument :

MSVOA_N

ClientSampleId :

BFB