


Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN062618\
Data File : VN049544.D
Acq On : 26 Jun 2018 10:12
Operator : MD\SY
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N061618W.M
Title : SW846 8260
Last Update : Sat Jun 16 01:02:01 2018

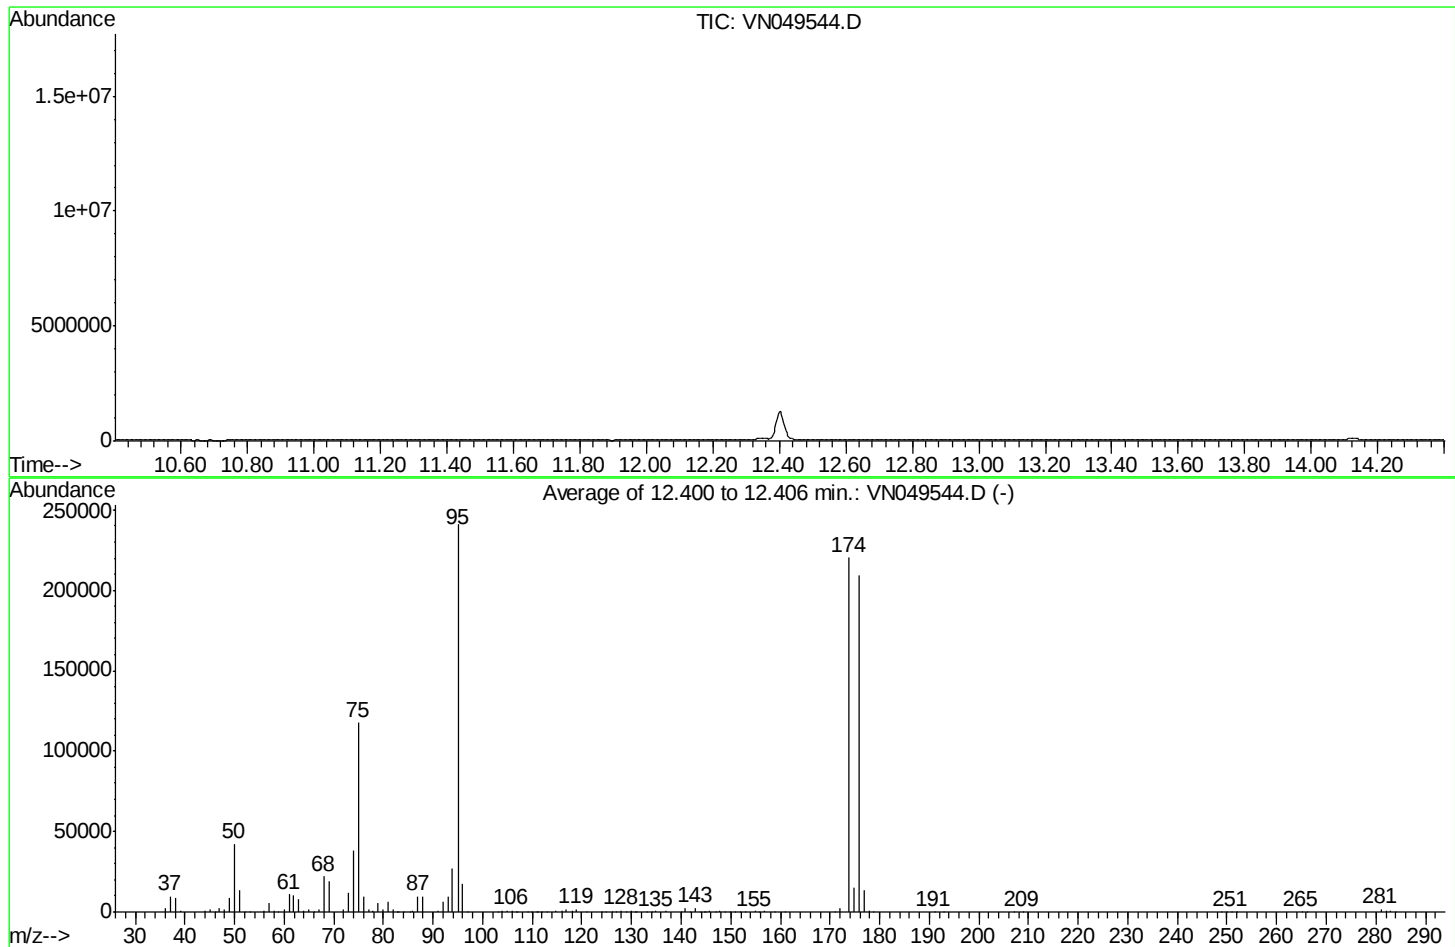

AutoFind: Scans 3362, 3363, 3364; Background Corrected with Scan 3342

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.5	42284	PASS
75	95	30	60	48.8	117666	PASS
95	95	100	100	100.0	240981	PASS
96	95	5	9	7.1	17151	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	91.3	220074	PASS
175	174	5	9	6.9	15113	PASS
176	174	95	101	95.1	209322	PASS
177	176	5	9	6.5	13707	PASS