

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN062620\
 Data File : VN062165.D
 Acq On : 27 Jun 2020 2:16
 Operator : JC/MD
 Sample : L3115-02
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 TP

Quant Time: Jun 27 03:50:48 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N062420W.M
 Quant Title : SW846 8260
 QLast Update : Wed Jun 24 15:33:00 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.63	168	220069	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.55	114	413221	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.38	117	406705	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.32	152	153131	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	7.99	65	152169	49.27	ug/l	0.00
Spiked Amount			Recovery	=	98.54%	
35) Dibromofluoromethane	7.55	113	129323	48.78	ug/l	0.00
Spiked Amount			Recovery	=	97.56%	
50) Toluene-d8	10.06	98	535640	50.55	ug/l	0.00
Spiked Amount			Recovery	=	101.10%	
62) 4-Bromofluorobenzene	12.38	95	176466	49.29	ug/l	0.00
Spiked Amount			Recovery	=	98.58%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
3) Chloromethane	2.04	50	317	Below Cal	#	41
11) Tert butyl alcohol	4.71	59	116	0.262	ug/l #	72
16) Acetone	3.78	43	16898	13.601	ug/l	95
18) Methyl Acetate	4.29	43	4416	1.799	ug/l #	52
20) Methylene Chloride	4.51	84	9697	3.218	ug/l	97
25) 2-Butanone	6.80	43	2513	1.665	ug/l #	81
29) Tetrahydrofuran	7.16	42	256	0.259	ug/l #	50
31) Cyclohexane	7.63	56	4841	1.135	ug/l #	14
36) 1,1-Dichloropropene	7.63	75	17658	4.251	ug/l #	50
37) Ethyl Acetate	6.80	43	2513	0.731	ug/l #	66
38) Carbon Tetrachloride	7.63	117	21776	5.561	ug/l #	16
41) Methacrylonitrile	7.17	41	473	0.297	ug/l #	17
43) Isopropyl Acetate	8.13	43	56426	10.064	ug/l	99
44) Trichloroethene	8.81	130	939	0.294	ug/l	89
45) 1,2-Dichloropropane	9.24	63	1366	0.437	ug/l #	43
48) Methyl methacrylate	9.14	41	3266	1.299	ug/l #	6
51) 4-Methyl-2-Pentanone	9.95	43	6321	1.930	ug/l	96
54) cis-1,3-Dichloropropene	9.88	75	28658	5.722	ug/l #	66
56) Ethyl methacrylate	10.52	69	1079	0.266	ug/l #	1
57) 1,3-Dichloropropane	10.74	76	5351	1.024	ug/l #	42
59) 2-Hexanone	10.74	43	60528	25.589	ug/l #	50
71) Bromoform	12.38	173	1210	0.551	ug/l #	1
74) N-ethyl acetate	12.01	43	2378	3.852	ug/l #	38
76) 1,2,3-Trichloropropane	12.37	75	90190	25.019	ug/l #	100
81) trans-1,4-Dichloro-2-buten	12.37	75	90190	73.066	ug/l #	13
95) Naphthalene	15.11	128	402	4.046	ug/l #	69

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN062620\
Data File : VN062165.D
Acq On : 27 Jun 2020 2:16
Operator : JC/MD
Sample : L3115-02
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampled :
TP

Quant Time: Jun 27 03:50:48 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N062420W.M
Quant Title : SW846 8260
QLast Update : Wed Jun 24 15:33:00 2020
Response via : Initial Calibration

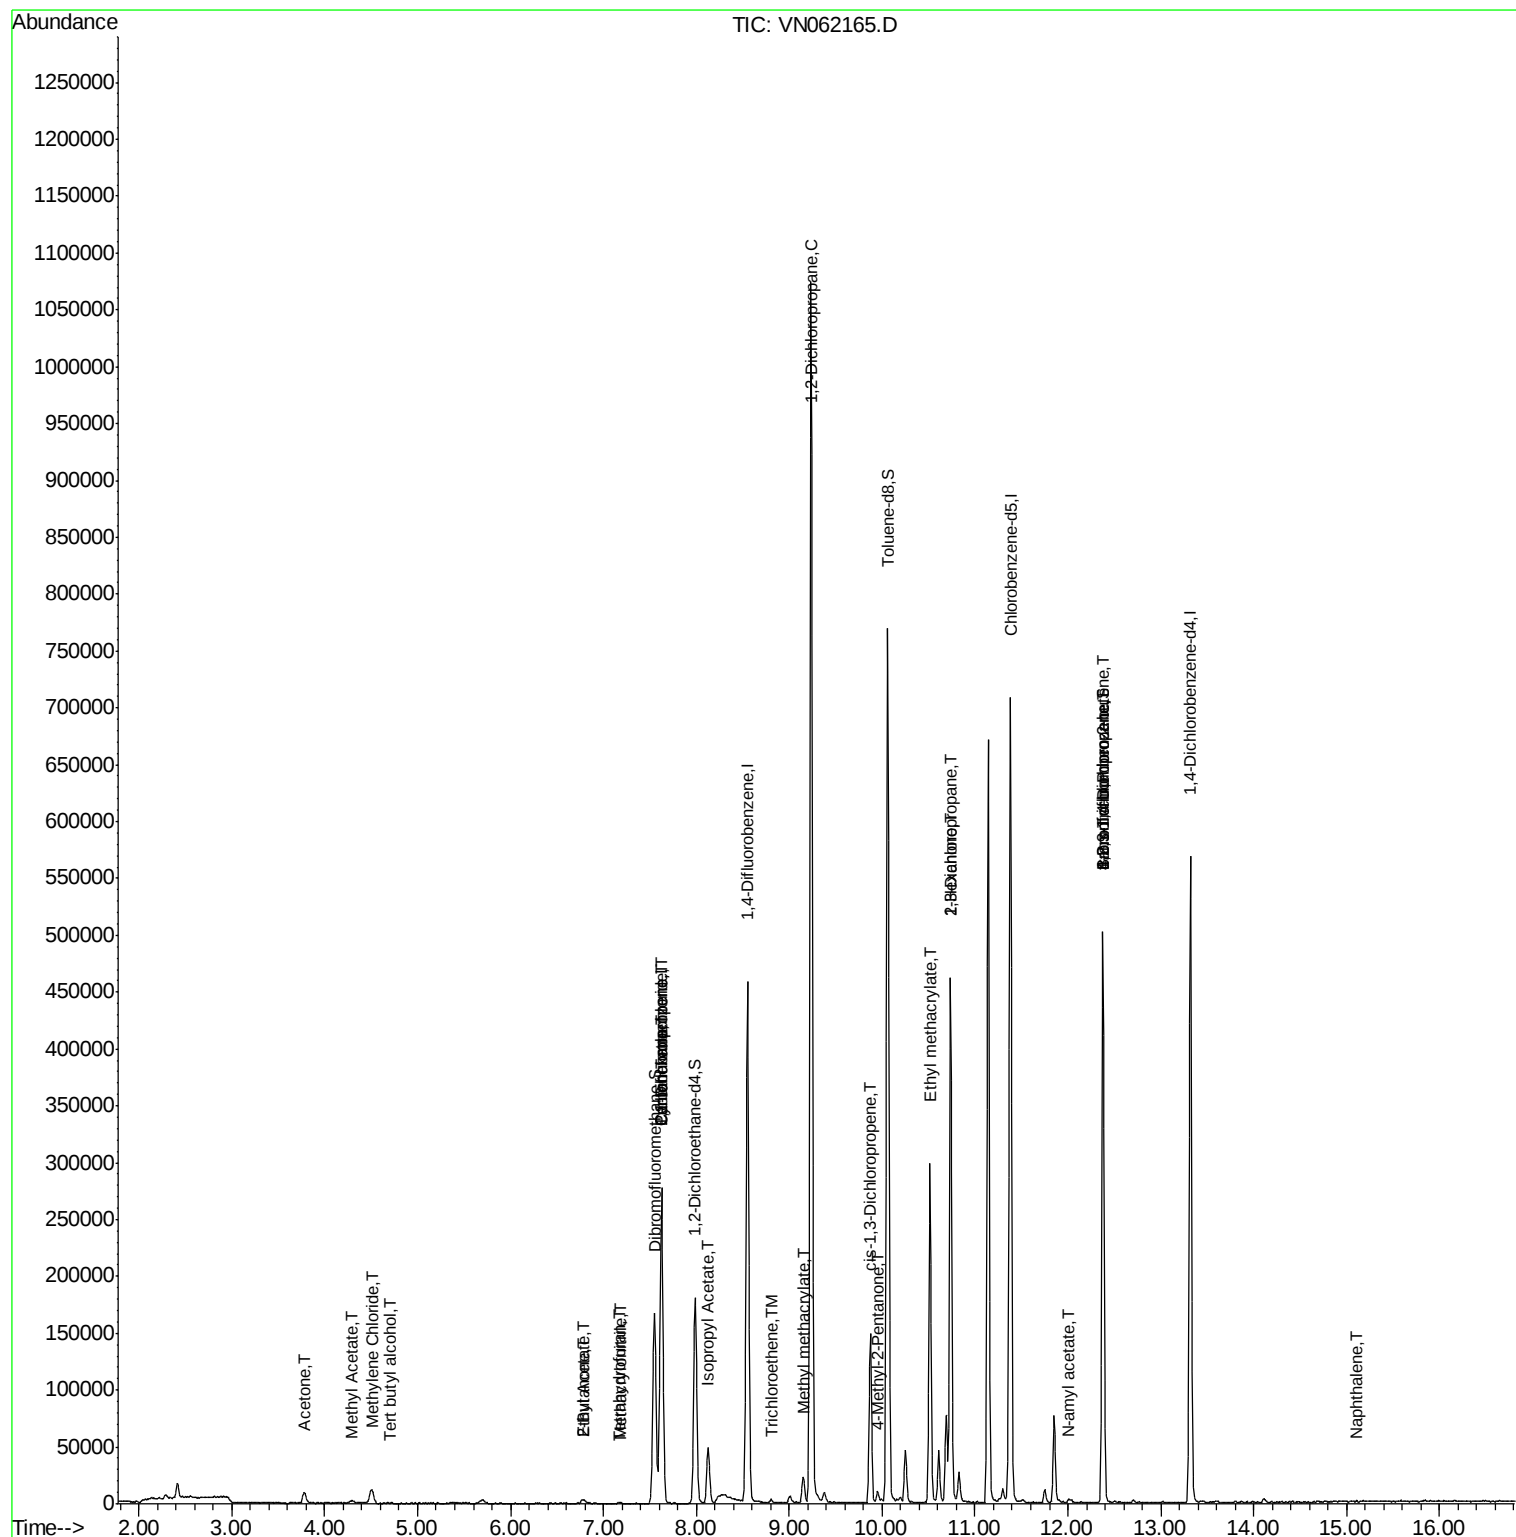



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.63 min Scan# 1820

Delta R.T. -0.00 min

Lab File: VN062165.D

Acq: 27 Jun 2020 2:16


Instrument :
MSVOA_N
ClientSampled :
TP

Tot Ion:168 Resp: 220069

Ion Ratio Lower Upper

168 100

99 57.3 45.8 68.8

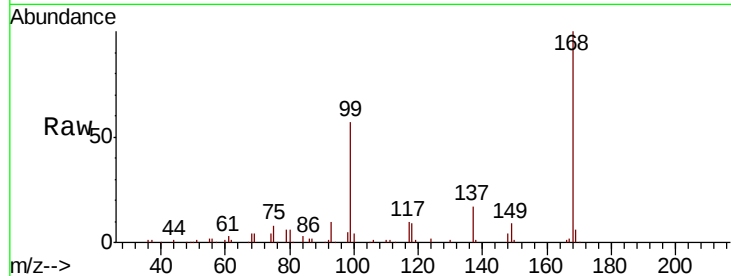

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VN

7.63

100000

80000



60000

40000

20000

0

Time--> 7.50 7.60 7.70



#3

Chloromethane

Concen: Below Cal

RT: 2.04 min Scan# 82

Delta R.T. 0.00 min

Lab File: VN062165.D


Acq: 27 Jun 2020 2:16

Tgt Ion: 50 Resp: 317

Ion Ratio Lower Upper

50 100

52 0.0 27.0 40.6#



Abundance Ion 49.90 (49.60 to 50.60): VN

Ion 51.90 (51.60 to 52.60): VN

2.04

400


300


200

100

0

Time--> 2.02 2.04 2.06






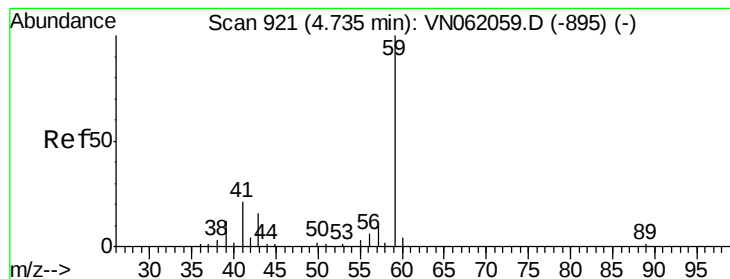


#11

Tert butyl alcohol
 Concen: 0.262 ug/l
 RT: 4.71 min Scan# 912
 Delta R.T. -0.03 min
 Lab File: VN062165.D
 Acq: 27 Jun 2020 2:16

Instrument :
 MSVOA_N
 ClientSampleId :
 TP




Tot Ion: 59 Resp: 116
 Ion Ratio Lower Upper
 59 100
 57 0.0 8.3 12.5#

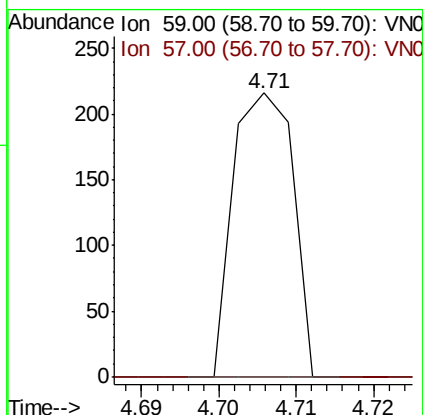

#16

Acetone
 Concen: 13.601 ug/l
 RT: 3.78 min Scan# 623
 Delta R.T. 0.00 min
 Lab File: VN062165.D
 Acq: 27 Jun 2020 2:16

Tgt Ion: 43 Resp: 16898
 Ion Ratio Lower Upper
 43 100
 58 31.6 27.5 41.3



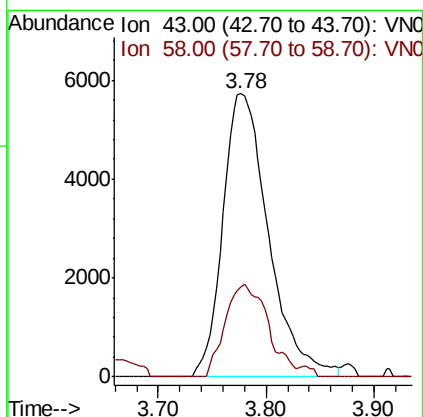





#18
Methyl Acetate
Concen: 1.799 ug/l
RT: 4.29 min Scan# 783
Delta R.T. 0.02 min
Lab File: VN062165.D
Acq: 27 Jun 2020 2:16




Instrument :
MSVOA_N
ClientSampled :
TP


Tot Ion: 43 Resp: 4416
Ion Ratio Lower Upper
43 100
74 3.1 22.9 34.3#

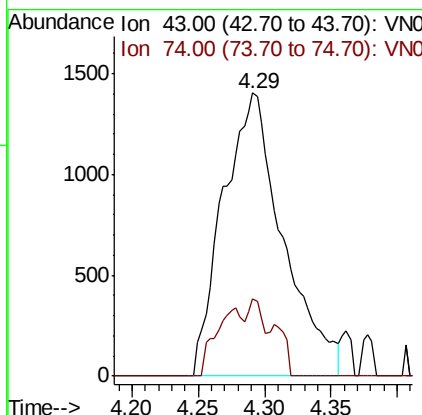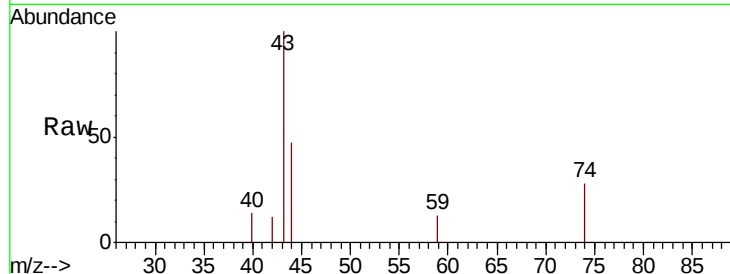

#20
Methylene Chloride
Concen: 3.218 ug/l
RT: 4.51 min Scan# 850
Delta R.T. 0.01 min
Lab File: VN062165.D
Acq: 27 Jun 2020 2:16

Tgt Ion: 84 Resp: 9697
Ion Ratio Lower Upper
84 100
49 110.9 90.6 136.0
51 31.5 27.8 41.8
86 64.8 50.1 75.1



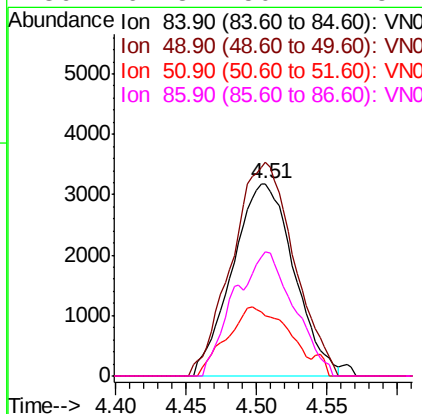
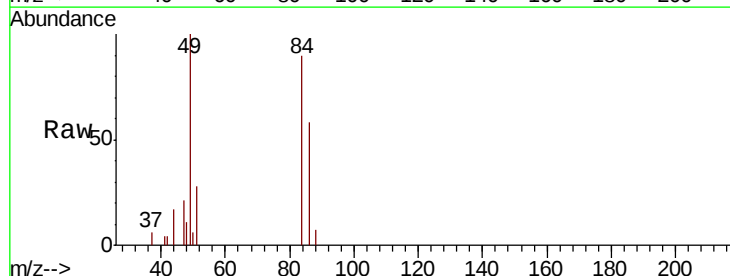


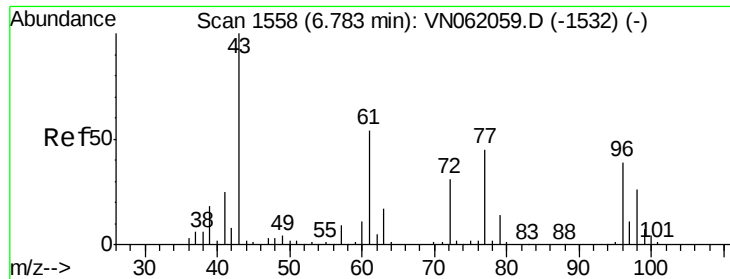

#25
2-Butanone
Concen: 1.665 ug/l
RT: 6.80 min Scan# 1563
Delta R.T. 0.02 min
Lab File: VN062165.D
Acq: 27 Jun 2020 2:16




Instrument :
MSVOA_N
ClientSampleId :
TP


Tot Ion: 43 Resp: 2513
Ion Ratio Lower Upper
43 100
72 20.8 24.8 37.2#

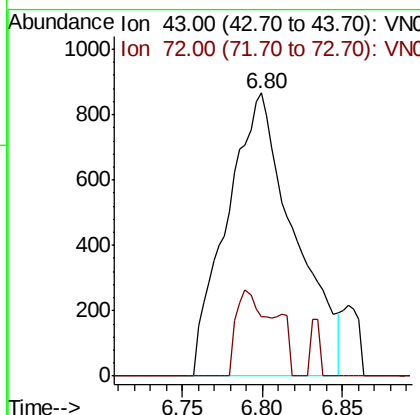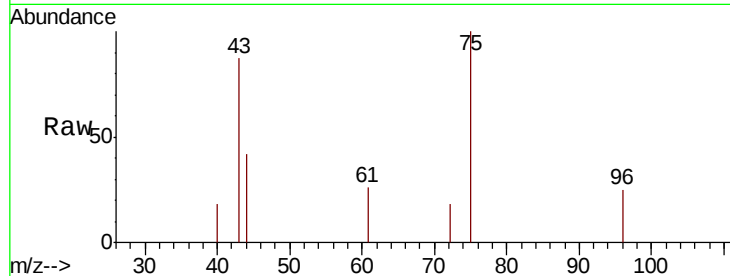

#29
Tetrahydrofuran
Concen: 0.259 ug/l
RT: 7.16 min Scan# 1675
Delta R.T. -0.01 min
Lab File: VN062165.D
Acq: 27 Jun 2020 2:16

Tgt Ion: 42 Resp: 256
Ion Ratio Lower Upper
42 100
72 110.9 41.1 61.7#
71 56.6 38.2 57.4

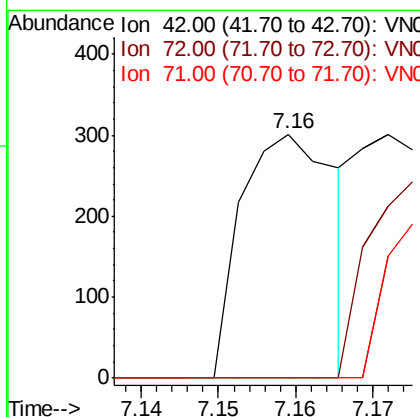

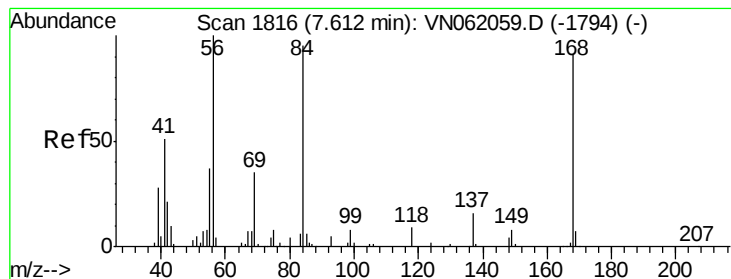

#31

Cyclohexane

Concen: 1.135 ug/l

RT: 7.63 min Scan# 1820

Delta R.T. 0.01 min

Lab File: VN062165.D

Acq: 27 Jun 2020 2:16

Instrument :

MSVOA_N

ClientSampled :

TP


Tot Ion: 56 Resp: 4841

Ion Ratio Lower Upper

56 100

69 155.1 28.0 42.0#




84 135.7 76.1 114.1#



Abundance Ion 56.00 (55.70 to 56.70): VN0

Ion 69.00 (68.70 to 69.70): VN0

Ion 84.00 (83.70 to 84.70): VN0

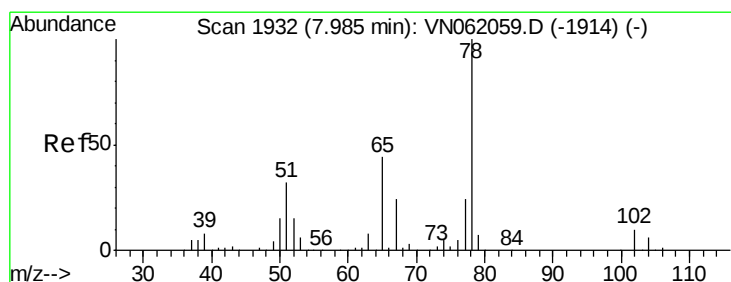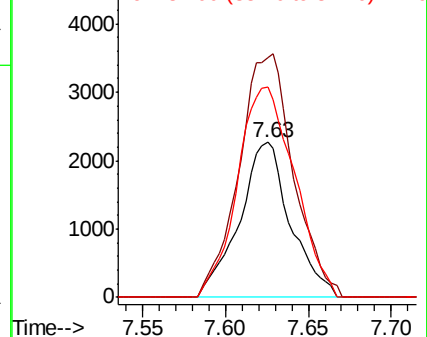

#33

1,2-Dichloroethane-d4

Concen: 49.273 ug/l

RT: 7.99 min Scan# 1933

Delta R.T. 0.00 min

Lab File: VN062165.D


Acq: 27 Jun 2020 2:16

Tgt Ion: 65 Resp: 152169

Ion Ratio Lower Upper



65 100


67 52.8 0.0 106.2



Abundance Ion 64.90 (64.60 to 65.60): VN0

Ion 66.90 (66.60 to 67.60): VN0



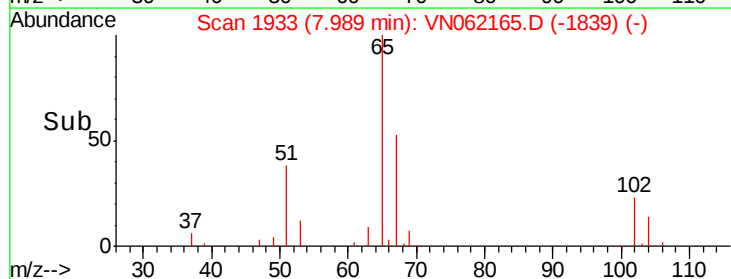
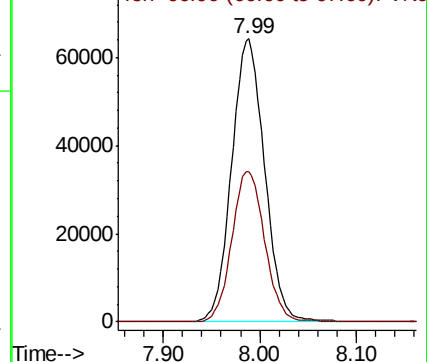


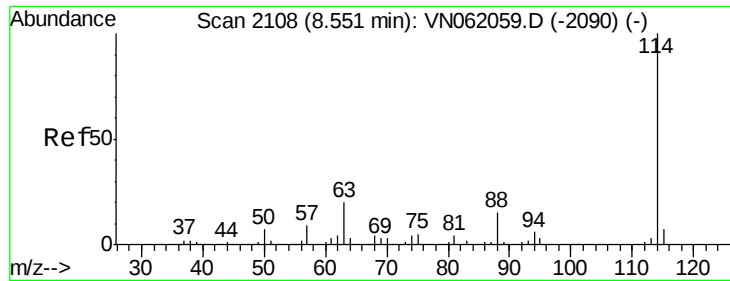

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.55 min Scan# 2108
 Delta R.T. -0.00 min
 Lab File: VN062165.D
 Acq: 27 Jun 2020 2:16




Instrument :
 MSVOA_N
 ClientSampleId :
 TP


Tot Ion:114 Resp: 413221
 Ion Ratio Lower Upper
 114 100
 63 19.4 0.0 39.2
 88 15.8 0.0 30.8

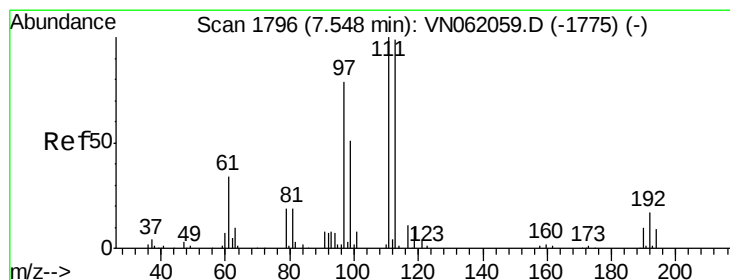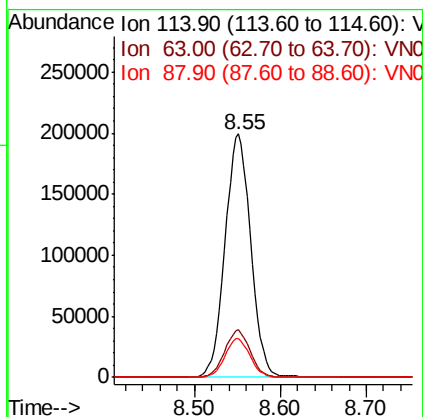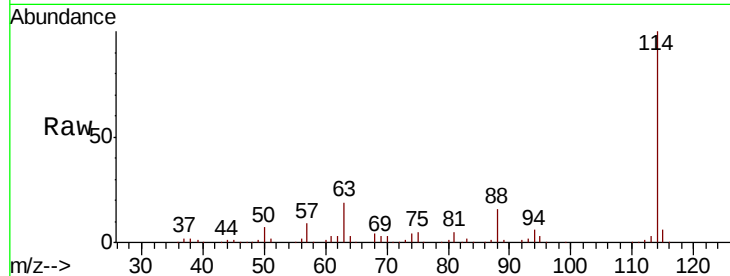

#35
 Dibromofluoromethane
 Concen: 48.783 ug/l
 RT: 7.55 min Scan# 1797
 Delta R.T. 0.00 min
 Lab File: VN062165.D
 Acq: 27 Jun 2020 2:16

Tgt Ion:113 Resp: 129323
 Ion Ratio Lower Upper
 113 100
 111 101.9 82.2 123.4
 192 17.8 14.0 21.0

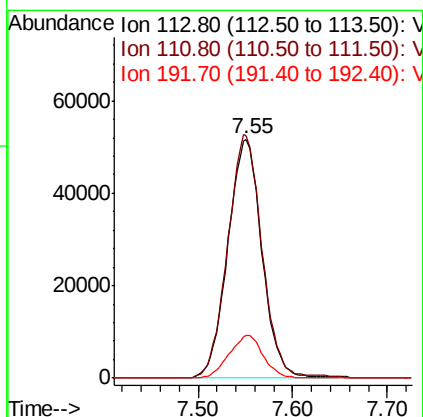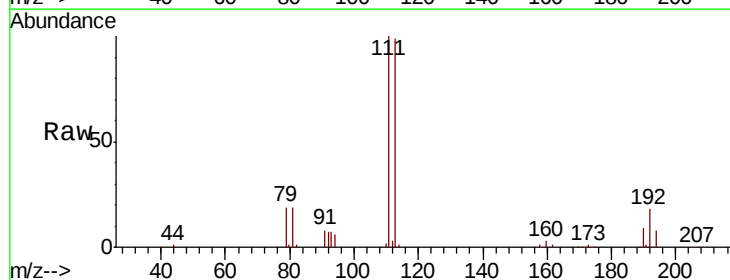



#36

1,1-Dichloropropene

Concen: 4.251 ug/l

RT: 7.63 min Scan# 1820

Delta R.T. -0.13 min

Lab File: VN062165.D

Acq: 27 Jun 2020 2:16

Instrument :

MSVOA_N

ClientSampleId :

TP


Tot Ion: 75 Resp: 17658

Ion Ratio Lower Upper

75 100

110 9.4 17.9 53.8#




77 0.0 24.9 37.3#



Abundance Ion 74.90 (74.60 to 75.60): VN0

Ion 109.90 (109.60 to 110.60): VN0

Ion 76.90 (76.60 to 77.60): VN0

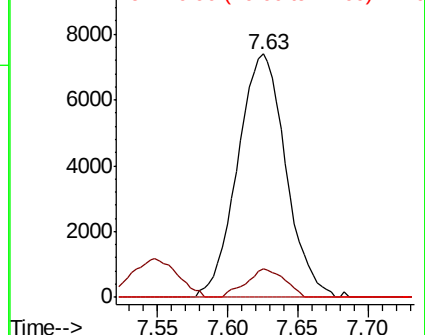

#37

Ethyl Acetate

Concen: 0.731 ug/l

RT: 6.80 min Scan# 1563

Delta R.T. -0.08 min

Lab File: VN062165.D

Acq: 27 Jun 2020 2:16


Tgt Ion: 43 Resp: 2513

Ion Ratio Lower Upper

43 100

61 0.0 12.0 18.0#



70 0.0 9.6 14.4#




Abundance Ion 43.00 (42.70 to 43.70): VN0

Ion 60.90 (60.60 to 61.60): VN0

Ion 70.00 (69.70 to 70.70): VN0

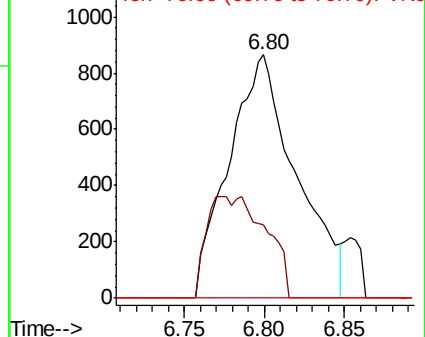



#38

Carbon Tetrachloride

Concen: 5.561 ug/l

RT: 7.63 min Scan# 1820

Delta R.T. -0.11 min

Lab File: VN062165.D

Acq: 27 Jun 2020 2:16

Instrument :

MSVOA_N

ClientSampled :

TP


Tot Ion: 117 Resp: 21776

Ion Ratio Lower Upper

117 100

119 5.9 78.2 117.2#




121 0.0 25.8 38.6#



Abundance Ion 116.80 (116.50 to 117.50): V

Ion 118.80 (118.50 to 119.50): V

Ion 120.80 (120.50 to 121.50): V

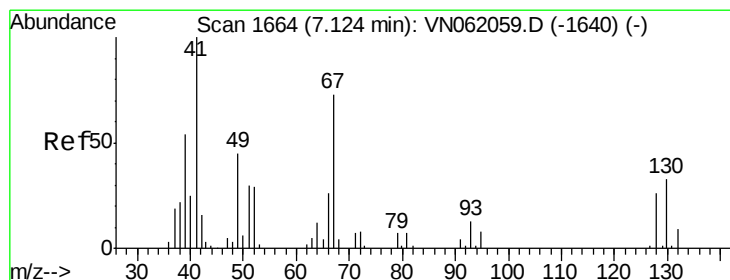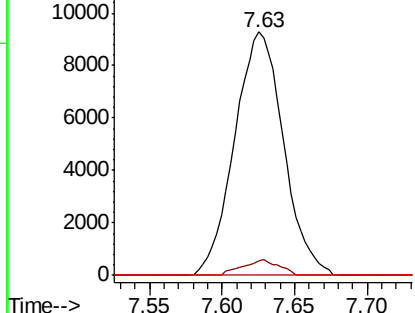

#41

Methacrylonitrile

Concen: 0.297 ug/l

RT: 7.17 min Scan# 1679

Delta R.T. 0.05 min

Lab File: VN062165.D

Acq: 27 Jun 2020 2:16

Tgt Ion: 41 Resp: 473


Ion Ratio Lower Upper

41 100

39 6.8 44.2 66.2#

67 0.0 79.5 119.3#

52 0.0 32.3 48.5#






Abundance Ion 41.00 (40.70 to 41.70): V

Ion 39.00 (38.70 to 39.70): V

Ion 67.00 (66.70 to 67.70): V

Ion 52.00 (51.70 to 52.70): V

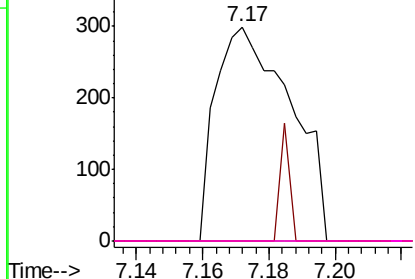

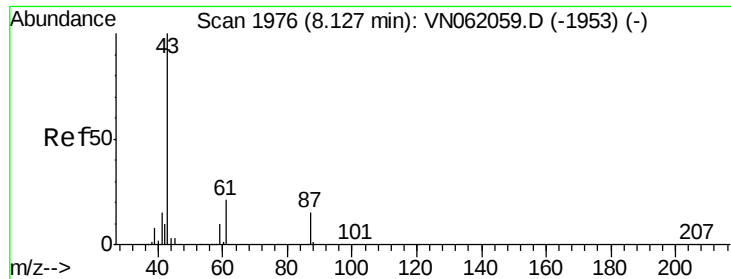

#43

Isopropyl Acetate

Concen: 10.064 ug/l

RT: 8.13 min Scan# 1976

Delta R.T. -0.00 min

Lab File: VN062165.D

Acq: 27 Jun 2020 2:16

Instrument :

MSVOA_N

ClientSampled :

TP





Tot Ion: 43 Resp: 56426

Ion Ratio Lower Upper

43 100

61 20.9 17.2 25.8

87 14.7 12.1 18.1

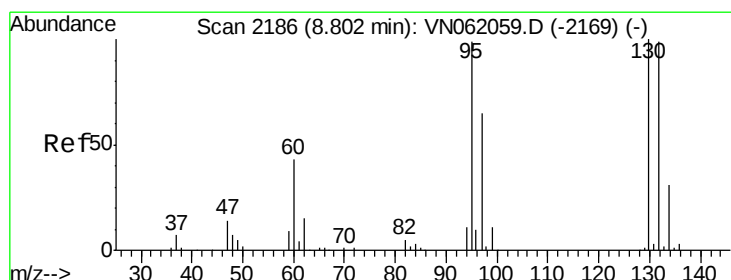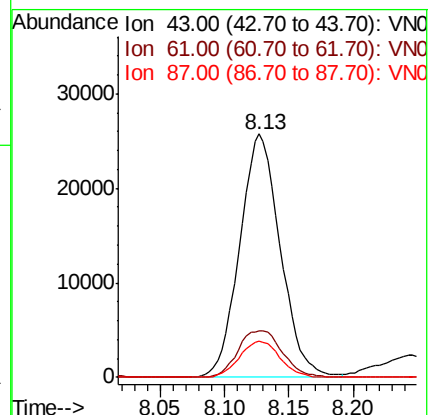

#44

Trichloroethene

Concen: 0.294 ug/l

RT: 8.81 min Scan# 2187

Delta R.T. 0.00 min

Lab File: VN062165.D




Acq: 27 Jun 2020 2:16


Tgt Ion: 130 Resp: 939

Ion Ratio Lower Upper

130 100

95 88.3 0.0 197.8


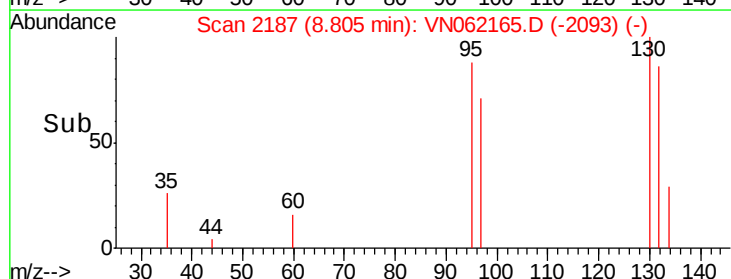
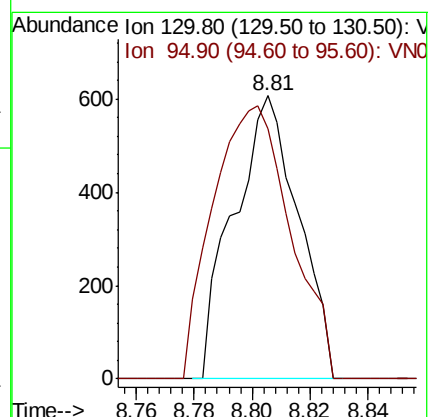
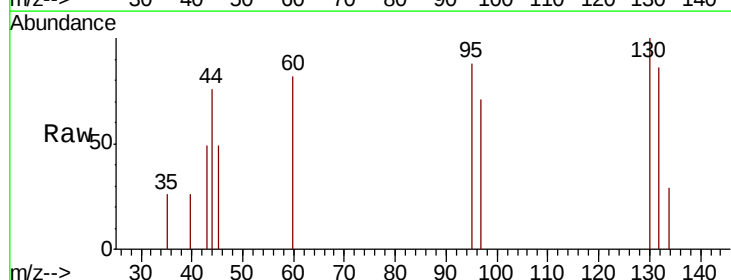




#45
 1,2-Dichloropropane
 Concen: 0.437 ug/l
 RT: 9.24 min Scan# 2322
 Delta R.T. 0.15 min
 Lab File: VN062165.D
 Acq: 27 Jun 2020 2:16




Instrument :
 MSVOA_N
 ClientSampleId :
 TP


Tot Ion: 63 Resp: 1366
 Ion Ratio Lower Upper
 63 100
 65 0.0 25.0 37.4#

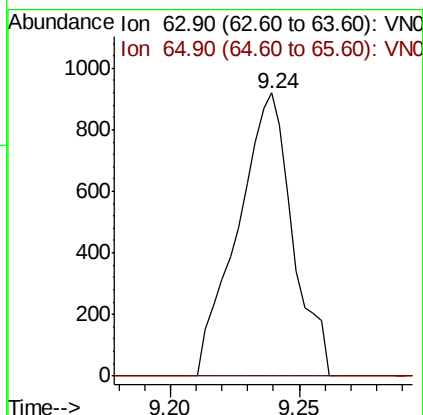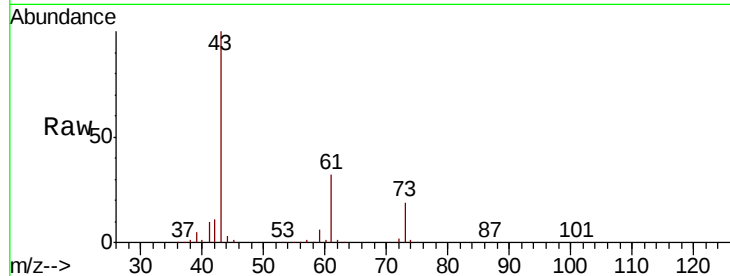

#48
 Methyl methacrylate
 Concen: 1.299 ug/l
 RT: 9.14 min Scan# 2292
 Delta R.T. -0.02 min
 Lab File: VN062165.D
 Acq: 27 Jun 2020 2:16

Tgt Ion: 41 Resp: 3266
 Ion Ratio Lower Upper
 41 100
 69 0.0 80.7 121.1#
 39 0.0 54.5 81.7#

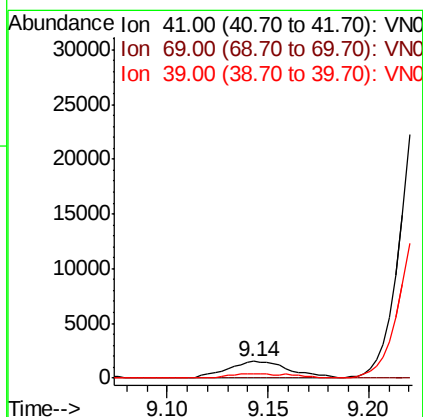

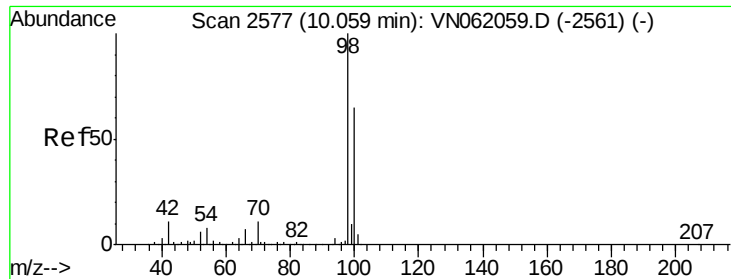

#50

Toluene-d8

Concen: 50.546 ug/l

RT: 10.06 min Scan# 2577

Delta R.T. -0.00 min

Lab File: VN062165.D

Acq: 27 Jun 2020 2:16

Instrument :

MSVOA_N

ClientSampleId :


TP

Tot Ion: 98 Resp: 535640

Ion Ratio Lower Upper

98 100

100 65.1 51.2 76.8

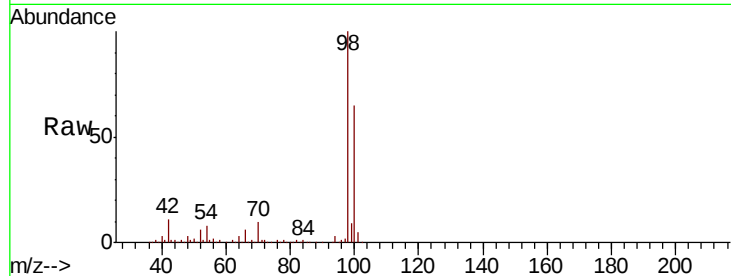

Abundance Ion 98.00 (97.70 to 98.70): VN062059.D (-2561) (-)

Ion 100.00 (99.70 to 100.70): VN062059.D (-2561) (-)

10.06

300000



200000

100000

0

10.00 10.10

Time-->



#51

4-Methyl-2-Pentanone

Concen: 1.930 ug/l

RT: 9.95 min Scan# 2544

Delta R.T. -0.00 min

Lab File: VN062165.D


Acq: 27 Jun 2020 2:16

Tgt Ion: 43 Resp: 6321

Ion Ratio Lower Upper

43 100

58 40.2 34.2 51.2



Abundance Ion 43.00 (42.70 to 43.70): VN062059.D (-2522) (-)

Ion 58.00 (57.70 to 58.70): VN062059.D (-2522) (-)

15000


10000


5000

0

9.90 9.95 10.00

Time-->






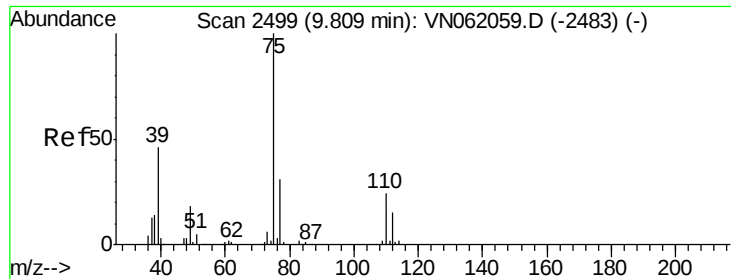


#54

cis-1,3-Dichloropropene
 Concen: 5.722 ug/l
 RT: 9.88 min Scan# 2520
 Delta R.T. 0.07 min
 Lab File: VN062165.D
 Acq: 27 Jun 2020 2:16

Instrument :
 MSVOA_N
 ClientSampled :
 TP




Tot Ion	Ratio	Lower	Upper
75	100		
77	0.0	25.0	37.6#
39	33.9	36.9	55.3#

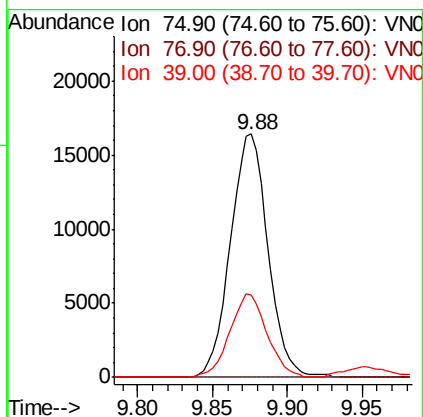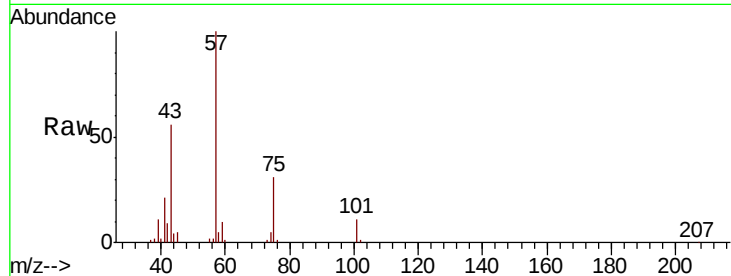


#56

Ethyl methacrylate
 Concen: 0.266 ug/l
 RT: 10.52 min Scan# 2719
 Delta R.T. 0.12 min
 Lab File: VN062165.D
 Acq: 27 Jun 2020 2:16

Tgt Ion	Ratio	Lower	Upper
69	100		
41	5206.5	46.6	70.0#
39	2327.1	31.0	46.4#



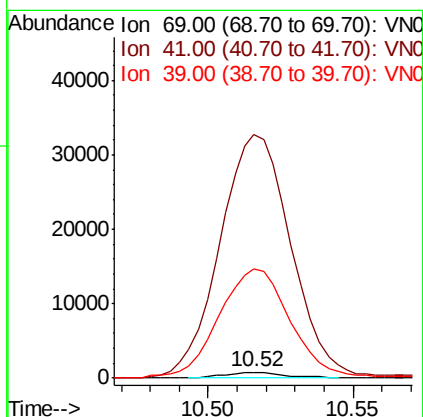



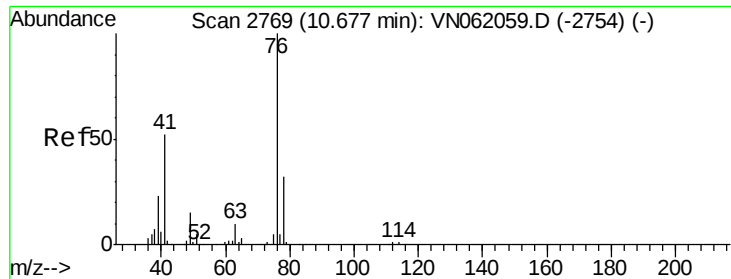

#57
 1,3-Dichloropropane
 Concen: 1.024 ug/l
 RT: 10.74 min Scan# 2788
 Delta R.T. 0.06 min
 Lab File: VN062165.D
 Acq: 27 Jun 2020 2:16




Instrument :
 MSVOA_N
 ClientSampled :
 TP


Tot Ion: 76 Resp: 5351
 Ion Ratio Lower Upper
 76 100
 78 0.0 25.8 38.8#

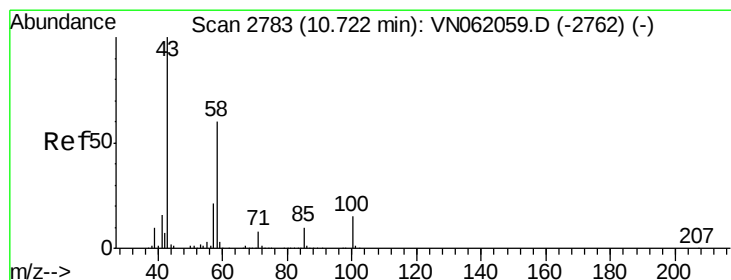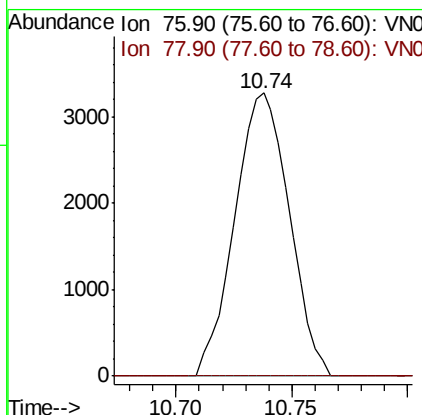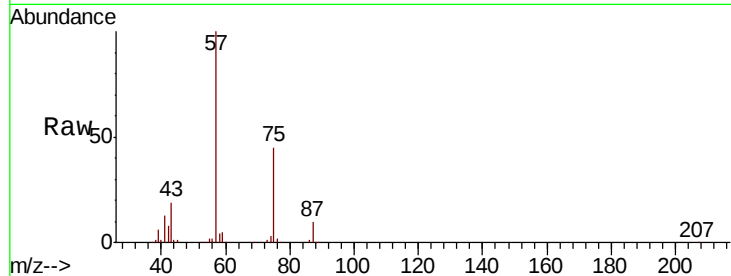

#59
 2-Hexanone
 Concen: 25.589 ug/l
 RT: 10.74 min Scan# 2788
 Delta R.T. 0.02 min
 Lab File: VN062165.D
 Acq: 27 Jun 2020 2:16

Tgt Ion: 43 Resp: 60528
 Ion Ratio Lower Upper
 43 100
 58 21.5 29.5 88.5#

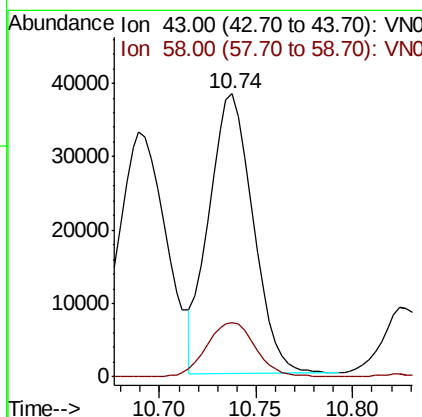







#62
4-Bromofluorobenzene
Concen: 49.288 ug/l
RT: 12.38 min Scan# 3298
Delta R.T. -0.00 min
Lab File: VN062165.D
Acq: 27 Jun 2020 2:16

Instrument :
MSVOA_N
ClientSampleId :
TP

Tot Ion: 95 Resp: 176466
Ion Ratio Lower Upper
95 100
174 78.5 0.0 154.8
176 74.1 0.0 147.4

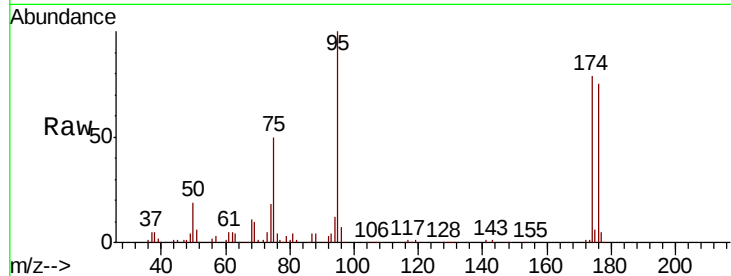


Abundance Ion 94.90 (94.60 to 95.60): VN062165.D (-3205) (-)
Ion 173.80 (173.50 to 174.50): VN062165.D (-3205) (-)
Ion 175.80 (175.50 to 176.50): VN062165.D (-3205) (-)


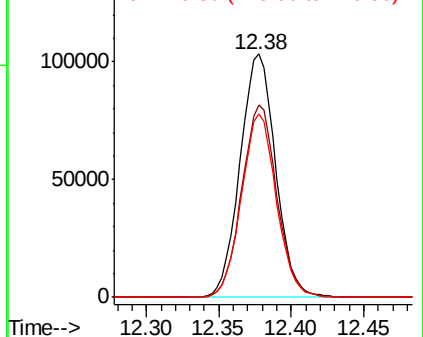



#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.38 min Scan# 2988
Delta R.T. -0.00 min
Lab File: VN062165.D
Acq: 27 Jun 2020 2:16

Tgt Ion: 117 Resp: 406705
Ion Ratio Lower Upper
117 100
82 55.6 43.8 65.8
119 31.6 25.2 37.8



Abundance Ion 116.90 (116.60 to 117.60): VN062165.D (-2895) (-)
Ion 82.00 (81.70 to 82.70): VN062165.D (-2895) (-)
Ion 118.90 (118.60 to 119.60): VN062165.D (-2895) (-)

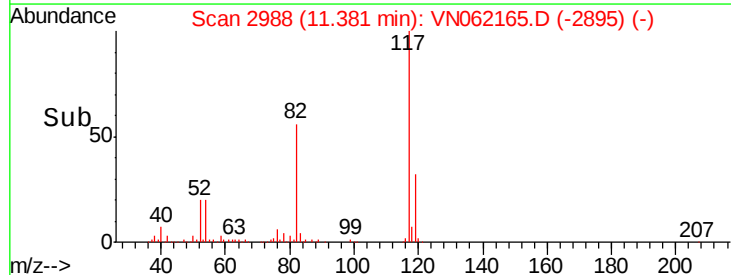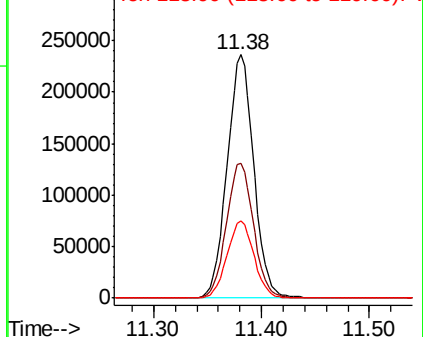



#71

Bromoform

Concen: 0.551 ug/l

RT: 12.38 min Scan# 3298

Delta R.T. 0.28 min

Lab File: VN062165.D

Acq: 27 Jun 2020 2:16

Instrument :

MSVOA_N

ClientSampled :

TP


Tot Ion:173 Resp: 1210

Ion Ratio Lower Upper

173 100

175 695.4 24.7 74.1#




254 0.0 0.0 0.0



Abundance Ion 172.70 (172.40 to 173.40): V

Ion 174.70 (174.40 to 175.40): V

Ion 254.40 (254.10 to 255.10): V

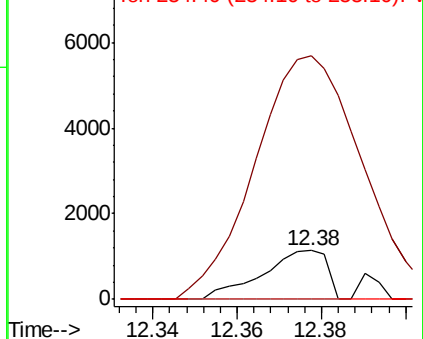

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.32 min Scan# 3591

Delta R.T. 0.00 min

Lab File: VN062165.D

Acq: 27 Jun 2020 2:16


Tgt Ion:152 Resp: 153131

Ion Ratio Lower Upper

152 100

115 59.5 29.5 88.5



150 159.0 0.0 351.4




Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

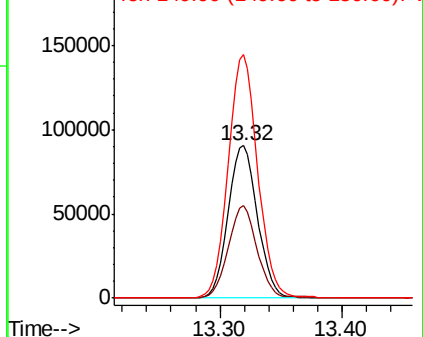



#74

N-amvl acetate

Concen: 3.852 ug/l

RT: 12.01 min Scan# 3183

Delta R.T. -0.04 min

Lab File: VN062165.D

Acq: 27 Jun 2020 2:16

Instrument :

MSVOA_N

ClientSampleId :

TP

Tot Ion: 43 Resp: 2378





Ion Ratio Lower Upper

43 100

70 0.0 39.4 59.2#

55 0.0 21.7 32.5#

61 0.0 21.3 31.9#

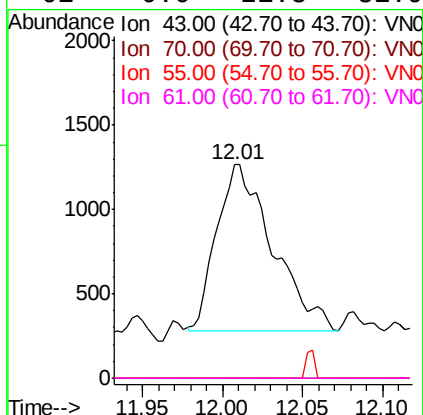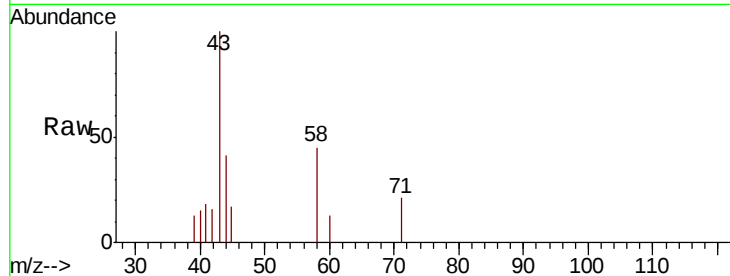

#76

1,2,3-Trichloropropane

Concen: 25.019 ug/l

RT: 12.37 min Scan# 3297

Delta R.T. -0.15 min

Lab File: VN062165.D




Acq: 27 Jun 2020 2:16


Tgt Ion: 75 Resp: 90190

Ion Ratio Lower Upper

75 100

77 1.1 0.0 0.0#

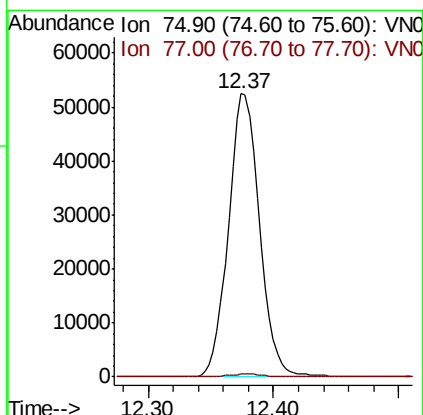

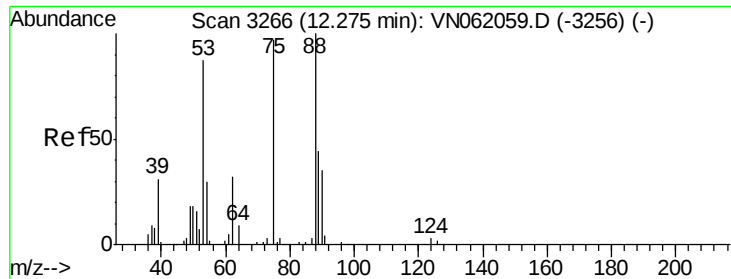

#81

trans-1,4-Dichloro-2-butene

Concen: 73.066 ug/l

RT: 12.37 min Scan# 3297

Delta R.T. 0.10 min

Lab File: VN062165.D

Acq: 27 Jun 2020 2:16

Instrument :

MSVOA_N

ClientSampleId :

TP


Tot Ion: 75 Resp: 90190

Ion Ratio Lower Upper

75 100

53 0.0 72.0 108.0#




89 0.0 36.9 55.3#

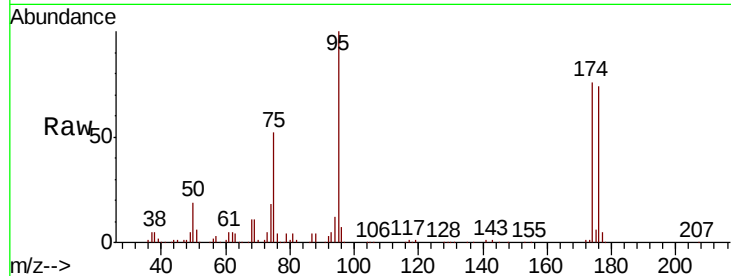

Abundance Ion 74.90 (74.60 to 75.60): VN062165.D (-3173) (-)

Ion 53.00 (52.70 to 53.70): VN062165.D (-3173) (-)

Ion 88.90 (88.60 to 89.60): VN062165.D (-3173) (-)

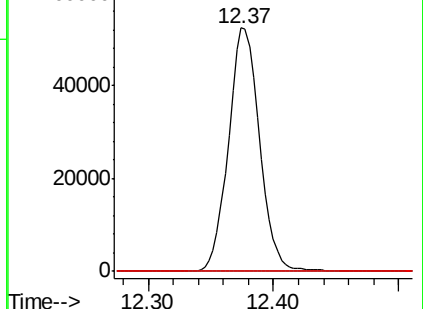

#95

Naphthalene

Concen: 4.046 ug/l

RT: 15.11 min Scan# 4148

Delta R.T. 0.01 min

Lab File: VN062165.D

Acq: 27 Jun 2020 2:16


Tgt Ion: 128 Resp: 402

Ion Ratio Lower Upper

128 100

127 0.0 10.5 15.7#

129 0.0 8.6 13.0#



Abundance Ion 128.00 (127.70 to 128.70): VN062165.D (-4053) (-)

Ion 127.00 (126.70 to 127.70): VN062165.D (-4053) (-)

Ion 129.00 (128.70 to 129.70): VN062165.D (-4053) (-)

