


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN062620\  
 Data File : VN062154.D  
 Acq On : 26 Jun 2020 21:27  
 Operator : JC/MD  
 Sample : BFB  
 Misc : 5.00mL/MSVOA N/WATER  
 ALS Vial : 29 Sample Multiplier: 1

Instrument :  
 MSVOA\_N  
 ClientSampleId :  
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA\_N\METHODS\82N062420W.M  
 Title : SW846 8260  
 Last Update : Wed Jun 24 15:33:00 2020

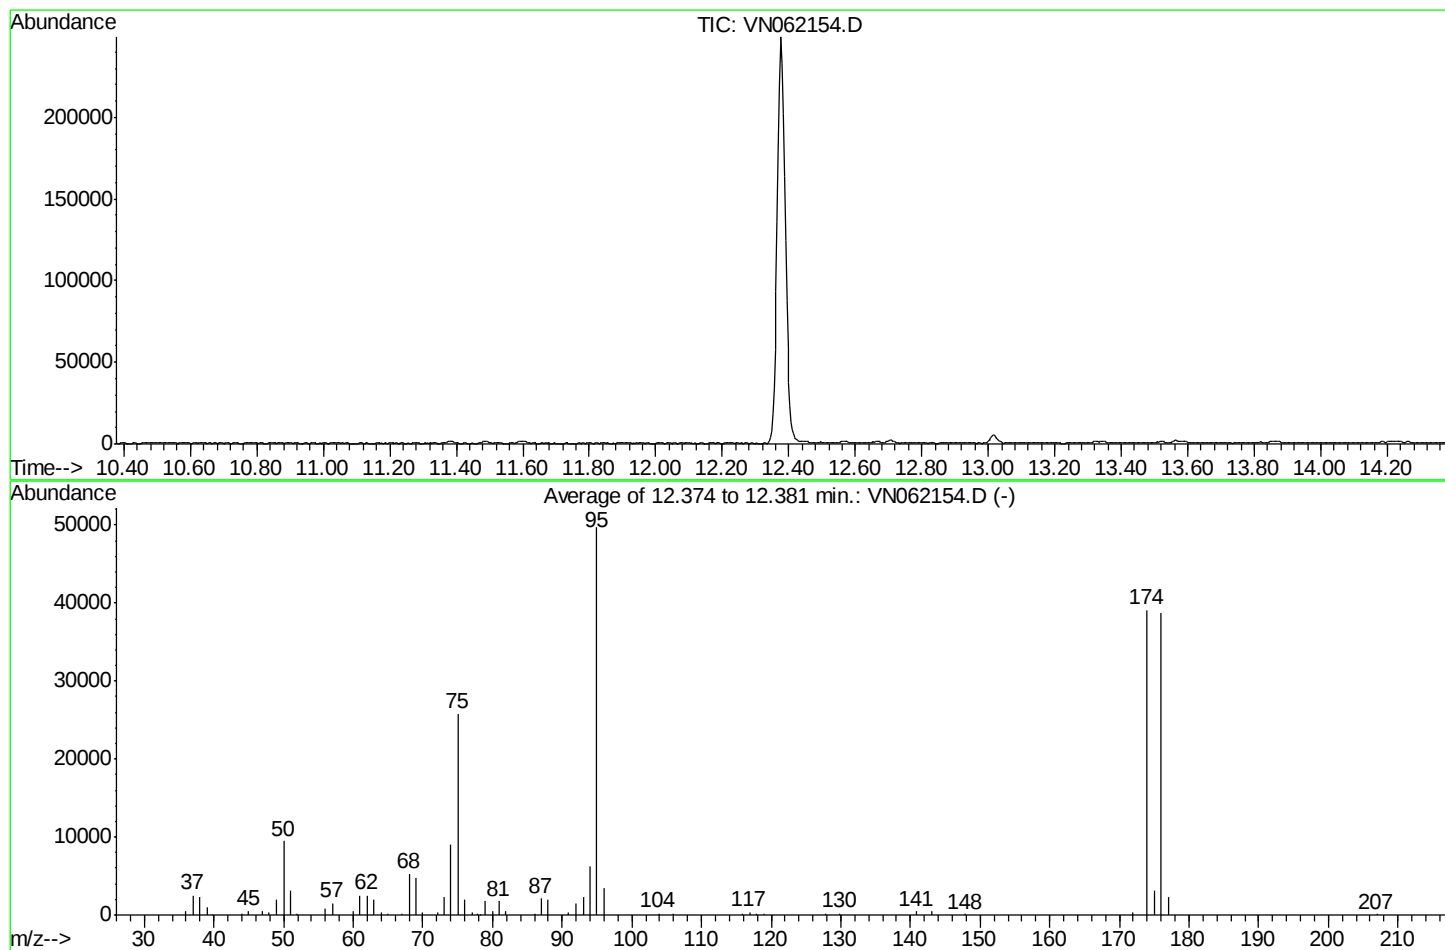

AutoFind: Scans 3297, 3298, 3299; Background Corrected with Scan 3283

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 50          | 95           | 15           | 40           | 19.1      | 9508    | PASS             |
| 75          | 95           | 30           | 60           | 51.9      | 25781   | PASS             |
| 95          | 95           | 100          | 100          | 100.0     | 49720   | PASS             |
| 96          | 95           | 5            | 9            | 7.0       | 3488    | PASS             |
| 173         | 174          | 0.00         | 2            | 0.0       | 0       | PASS             |
| 174         | 95           | 50           | 100          | 78.7      | 39136   | PASS             |
| 175         | 174          | 5            | 9            | 7.8       | 3051    | PASS             |
| 176         | 174          | 95           | 101          | 98.8      | 38685   | PASS             |
| 177         | 176          | 5            | 9            | 6.1       | 2356    | PASS             |