
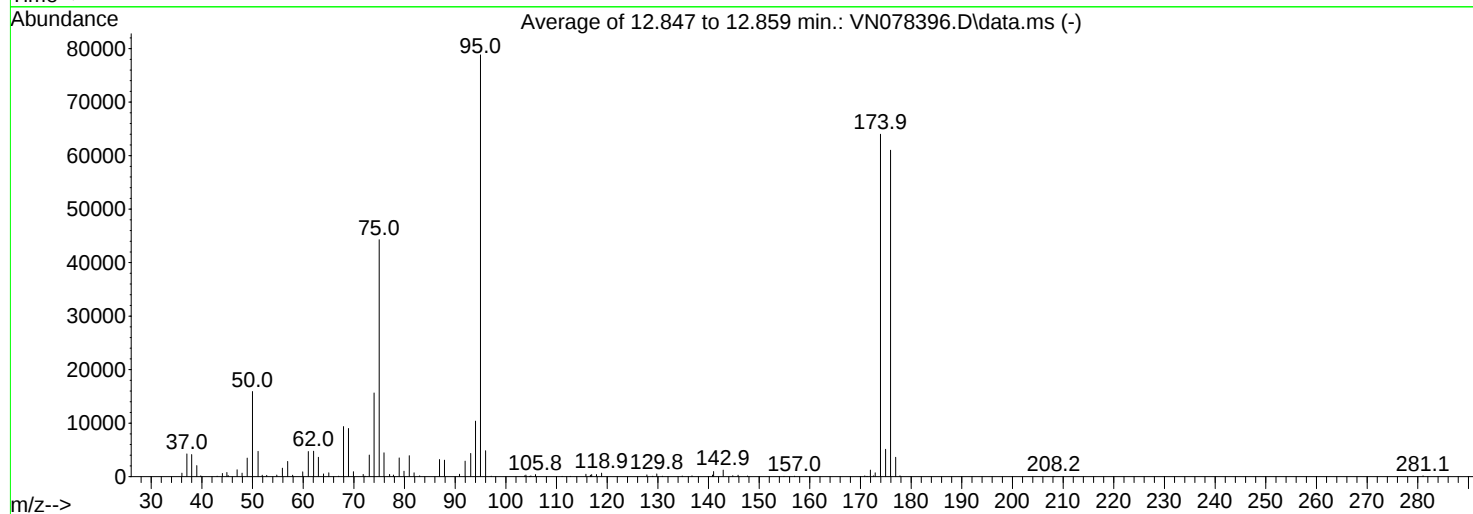


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN062623\
Data File : VN078396.D
Acq On : 26 Jun 2023 10:39
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N060623W.M
Title : SW846 8260
Last Update : Wed Jun 07 05:05:00 2023

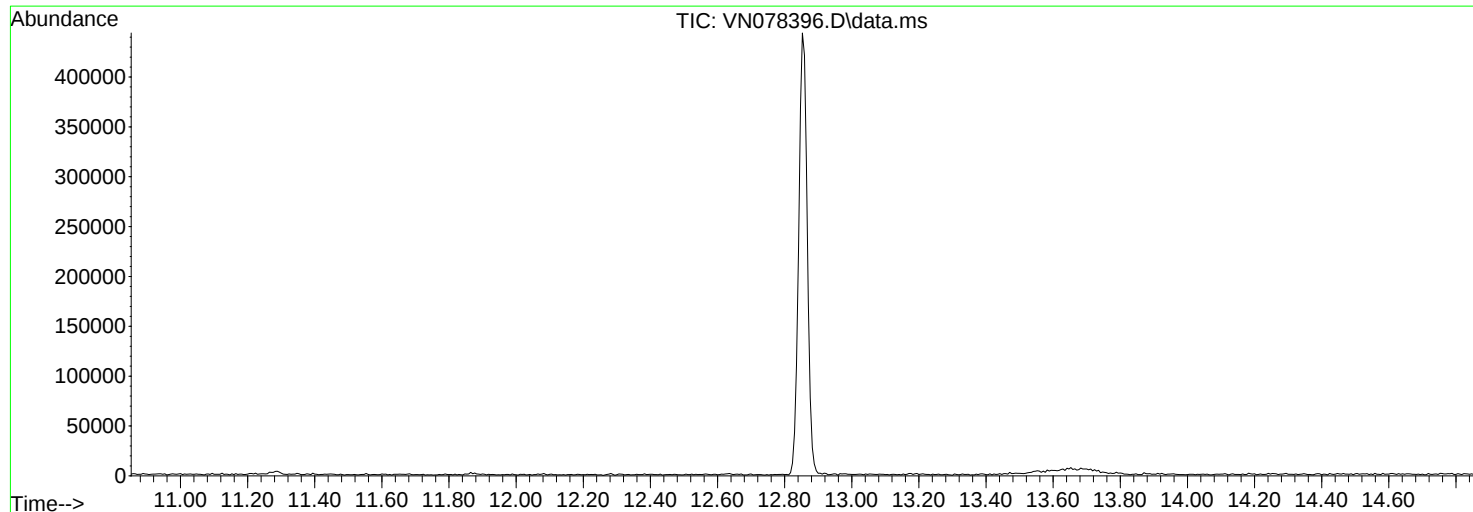

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1844

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.2	15906	PASS
75	95	30	60	56.2	44296	PASS
95	95	100	100	100.0	78835	PASS
96	95	5	9	6.2	4854	PASS
173	174	0.00	2	1.1	716	PASS
174	95	50	100	81.2	64005	PASS
175	174	5	9	8.0	5108	PASS
176	174	95	101	95.3	60997	PASS
177	176	5	9	5.9	3628	PASS

Average of 12.847 to 12.859 min.: VN078396.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	655	48.95	3463	62.05	4747	74.00	1565
37.05	4236	50.00	15906	63.00	3631	75.00	4429
38.00	4138	51.10	4733	64.00	517	75.95	446
39.00	2053	51.90	260	65.05	719	77.05	42
39.80	152	52.80	228	67.00	99	77.80	309
43.00	84	54.80	298	67.95	9351	78.95	3507
44.05	609	55.90	1592	68.95	8994	79.90	1022
44.95	790	56.95	2829	69.90	941	80.95	3932
45.20	219	57.90	272	71.85	417	81.90	709
46.95	1281	59.90	904	72.20	94	83.00	136
47.95	670	61.00	4694	73.05	4046	86.90	3190

Average of 12.847 to 12.859 min.: VN078396.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
87.90	3091	104.95	165	129.80	520	157.00	97
90.85	460	105.85	405	130.90	82	170.85	137
91.95	2894	111.10	66	134.80	112	171.30	62
93.05	4334	112.70	66	136.75	167	171.95	1243
94.00	10381	115.80	454	140.80	298	172.60	166
95.00	78835	116.70	274	141.00	964	172.90	716
96.00	4854	116.95	394	142.90	1237	173.95	64005
97.10	93	117.90	393	144.80	194	174.95	5108
103.70	137	118.90	662	145.85	262	175.95	60997
103.95	301	127.85	333	147.70	134	176.95	3628
104.70	71	129.00	106	154.90	51	177.80	159

Average of 12.847 to 12.859 min.: VN078396.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
208.20	61						
281.05	144						

Instrument :

MSVOA_N

ClientSampleId :

BFB